

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
 Data File : PL061899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 14:47
 Operator : DD\AJ
 Sample : L4198-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 16:09:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	29481545	45253002	17.281	16.587
28)	SA Decachlor...	8.209	9.094	28990082	38877143	17.821	17.660
Target Compounds							
2)	A alpha-BHC	0.000	4.422f	0	2529105	N.D.	0.633 #
10)	B gamma-Chl...	5.419f	6.122	2658394	6408502	1.531	2.182 #
11)	B alpha-Chl...	0.000	6.196	0	6207999	N.D.	2.067 #
12)	B 4,4'-DDE	5.619	6.349	5765935	9251048	3.669	3.389
17)	MA 4,4'-DDT	6.374	7.143	3717978	6684800	2.947	3.053
23)	Chlordane-1	4.331	0.000	2662249	0	53.766	N.D. #
25)	Chlordane-3	5.419f	6.122	2658394	6408502	16.913	17.489
26)	Chlordane-4	0.000	6.196	0	6207999	N.D.	13.829 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
Data File : PL061899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 14:47
Operator : DD\AJ
Sample : L4198-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 16:09:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

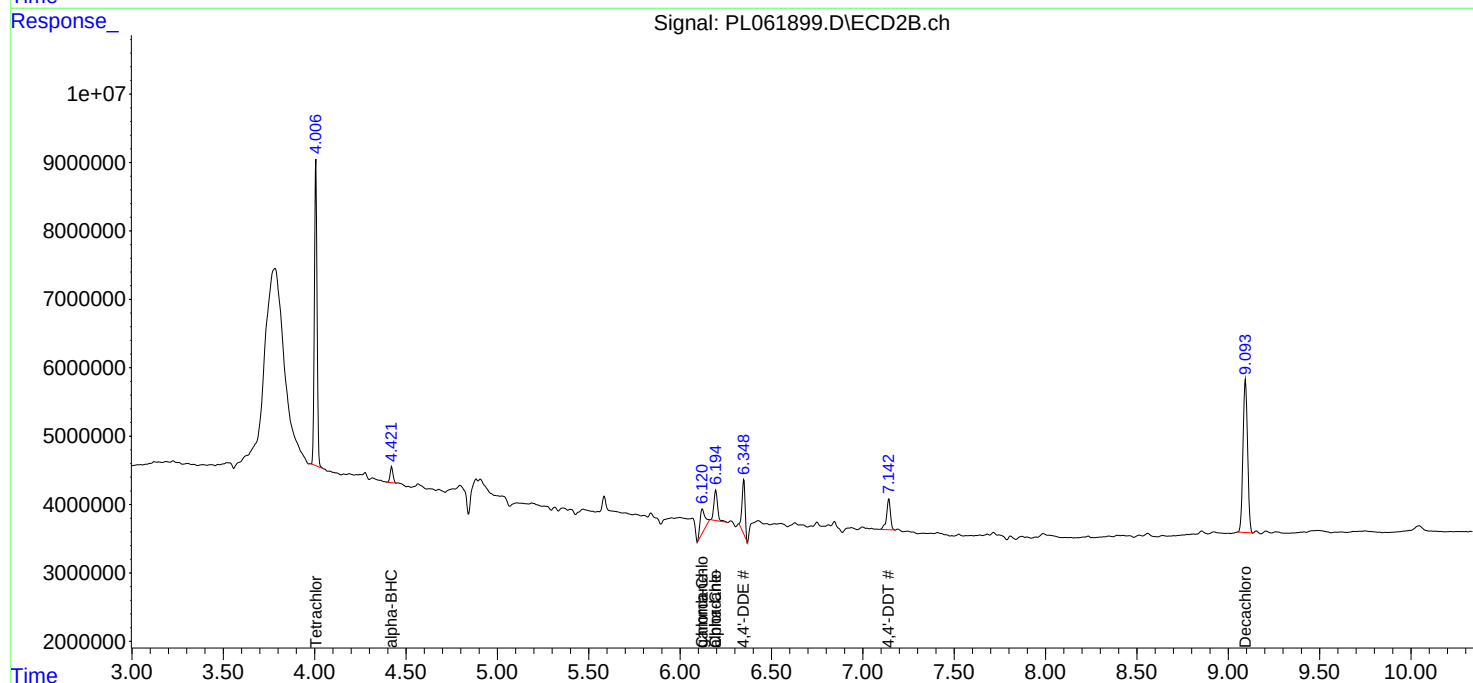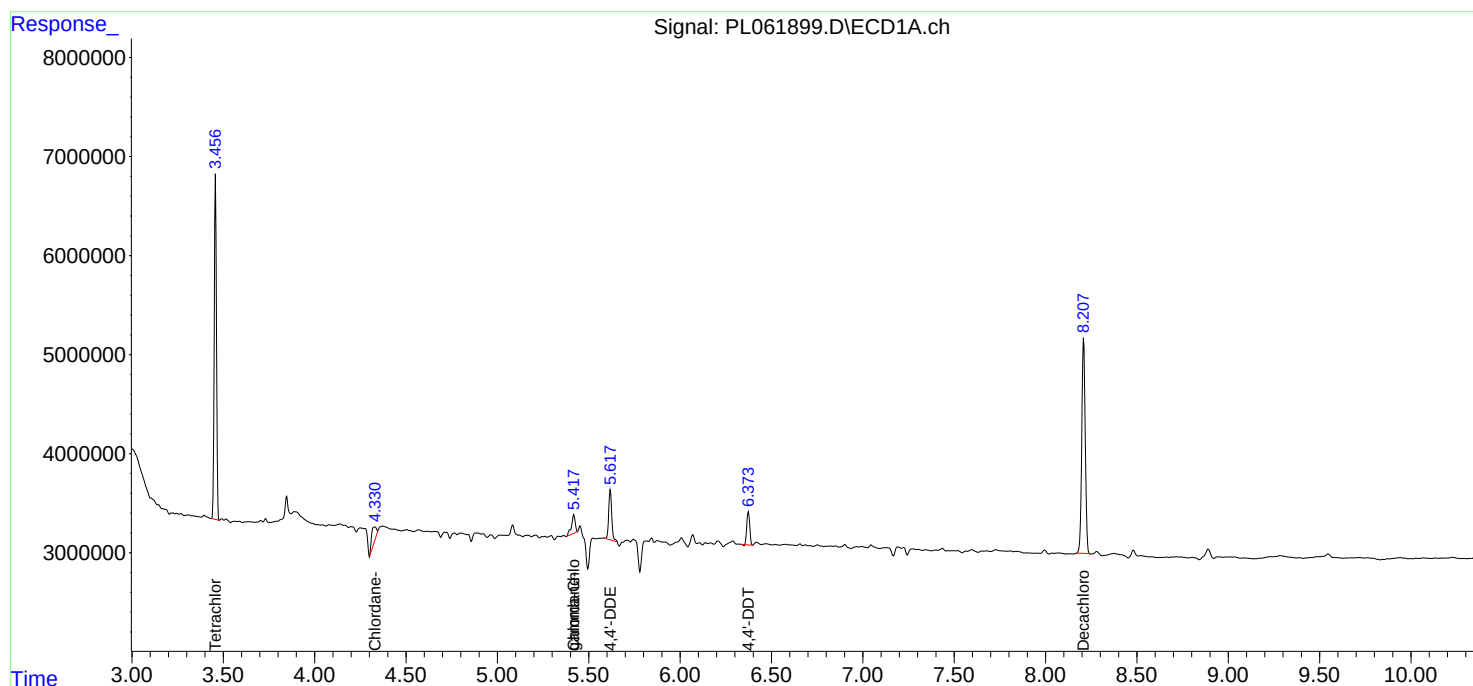


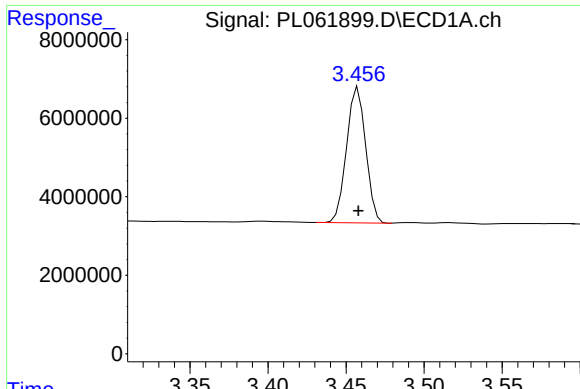

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 29481545
Conc: 17.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

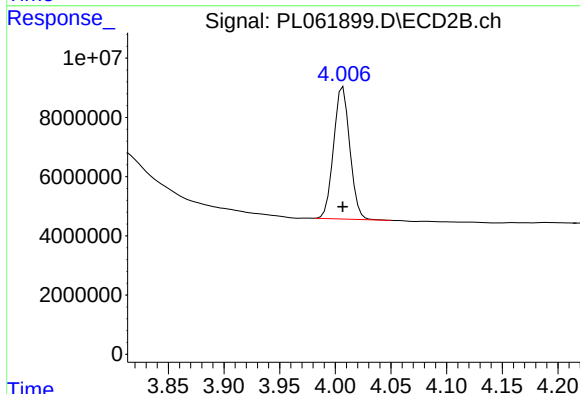


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 45253002
Conc: 16.59 ng/ml

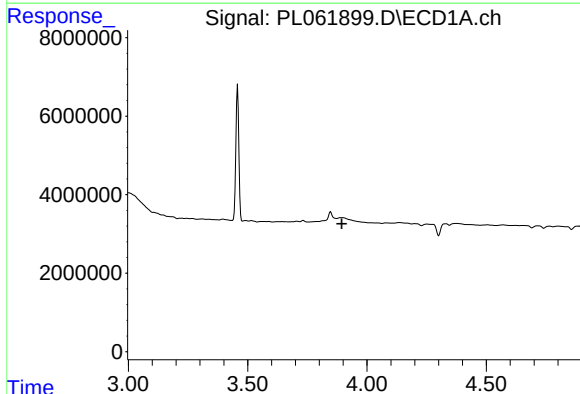


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.894 min
Response: 0
Conc: N.D.

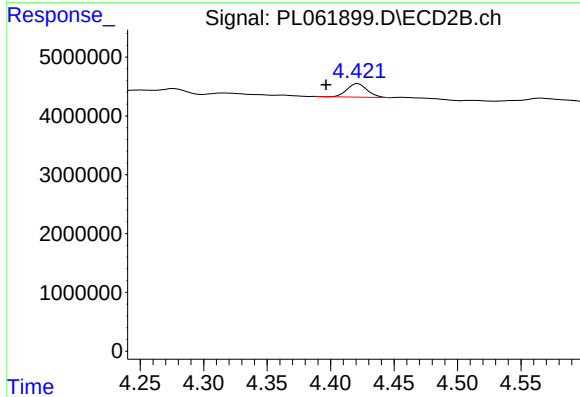

#2 alpha-BHC


R.T.: 4.422 min
Delta R.T.: 0.026 min
Response: 2529105
Conc: 0.63 ng/ml

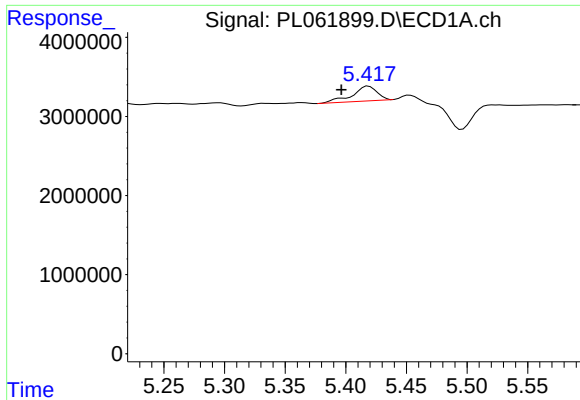

#10 gamma-Chlordane


R.T.: 5.419 min
Delta R.T.: 0.022 min
Response: 2658394
Conc: 1.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

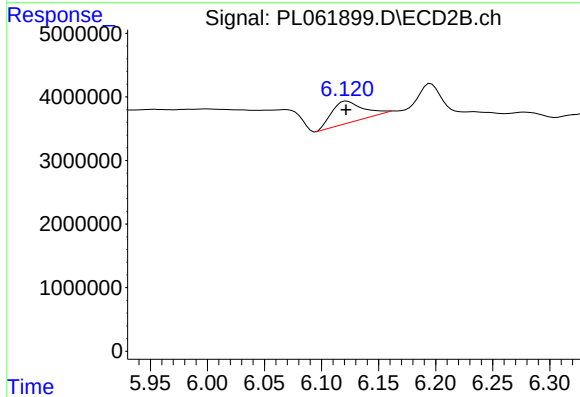


#10 gamma-Chlordane

R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 6408502
Conc: 2.18 ng/ml

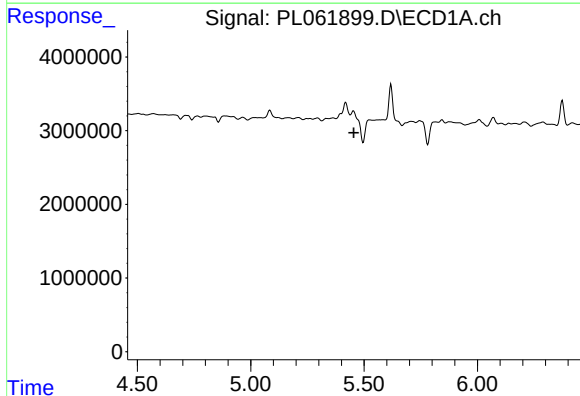


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

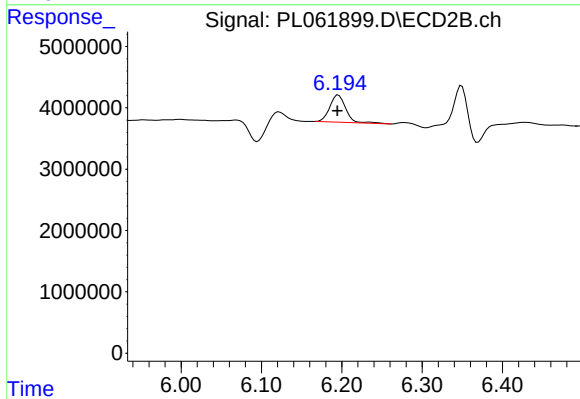

#11 alpha-Chlordane


R.T.: 6.196 min
Delta R.T.: 0.001 min
Response: 6207999
Conc: 2.07 ng/ml

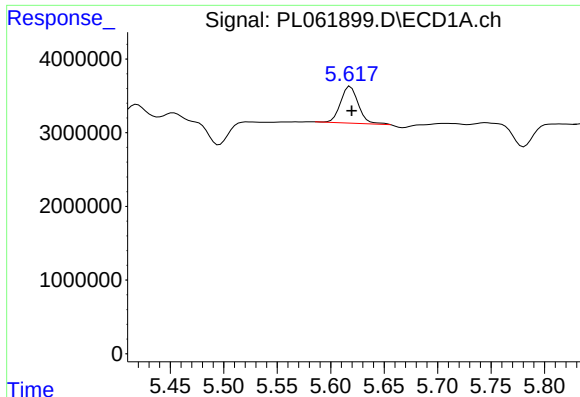

#12 4,4'-DDE


R.T.: 5.619 min
Delta R.T.: -0.001 min
Response: 5765935
Conc: 3.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

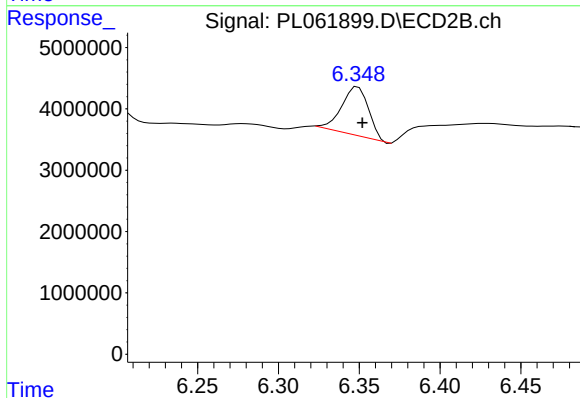


#12 4,4'-DDE

R.T.: 6.349 min
Delta R.T.: -0.003 min
Response: 9251048
Conc: 3.39 ng/ml

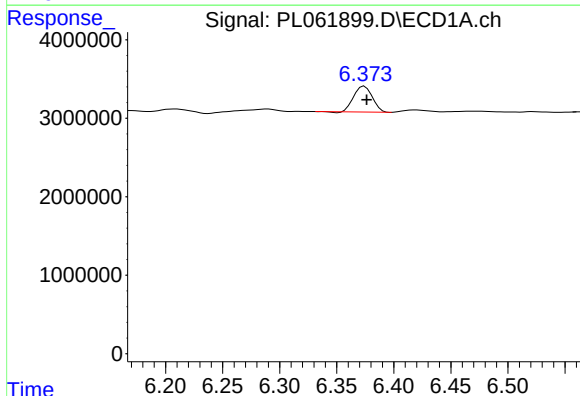


#17 4,4'-DDT

R.T.: 6.374 min
Delta R.T.: -0.002 min
Response: 3717978
Conc: 2.95 ng/ml

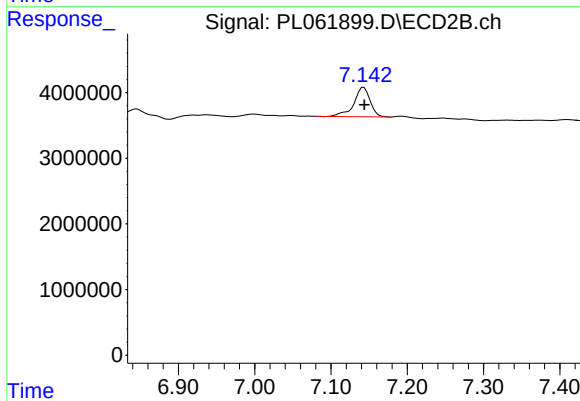

#17 4,4'-DDT


R.T.: 7.143 min
Delta R.T.: 0.000 min
Response: 6684800
Conc: 3.05 ng/ml

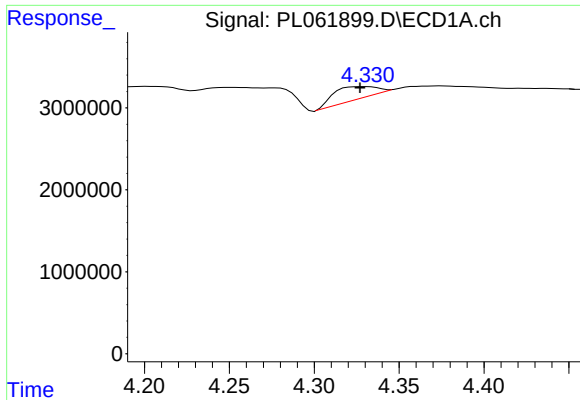

#23 Chlordane-1


R.T.: 4.331 min
Delta R.T.: 0.004 min
Response: 2662249
Conc: 53.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

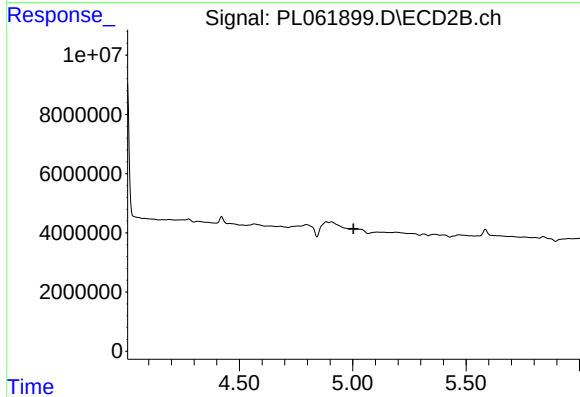


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

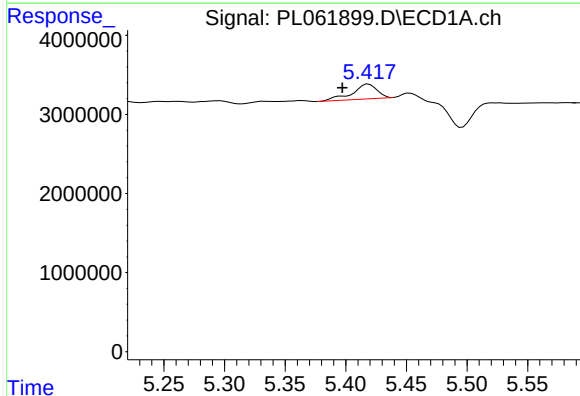


#25 Chlordane-3

R.T.: 5.419 min
Delta R.T.: 0.021 min
Response: 2658394
Conc: 16.91 ng/ml

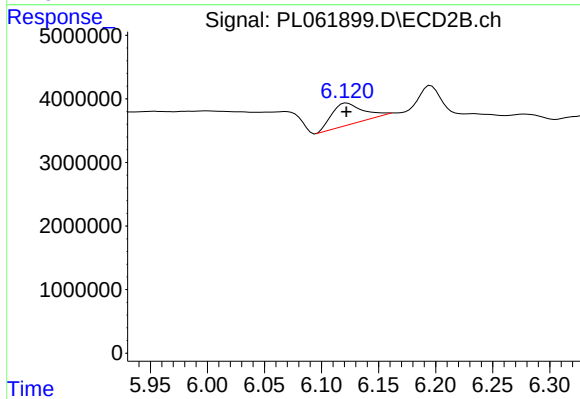

#25 Chlordane-3


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 6408502
Conc: 17.49 ng/ml

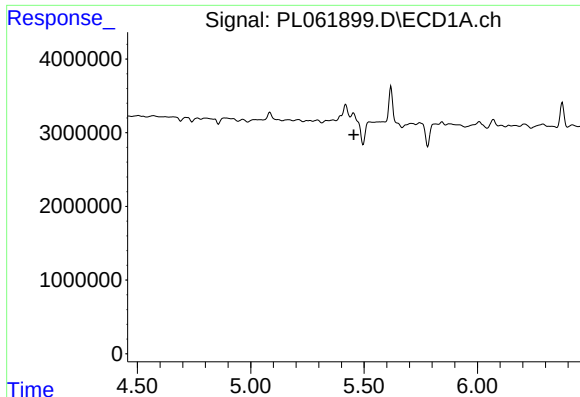

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

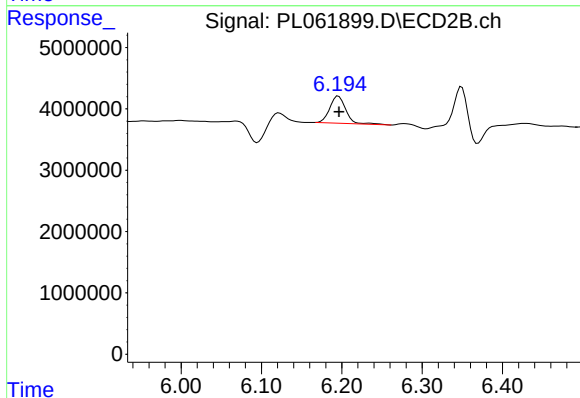


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 6207999
Conc: 13.83 ng/ml

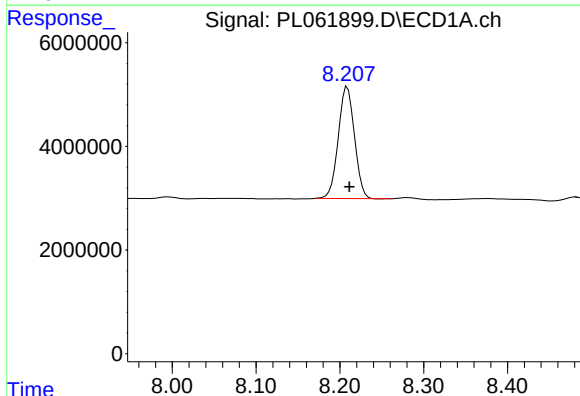

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.003 min
Response: 28990082
Conc: 17.82 ng/ml

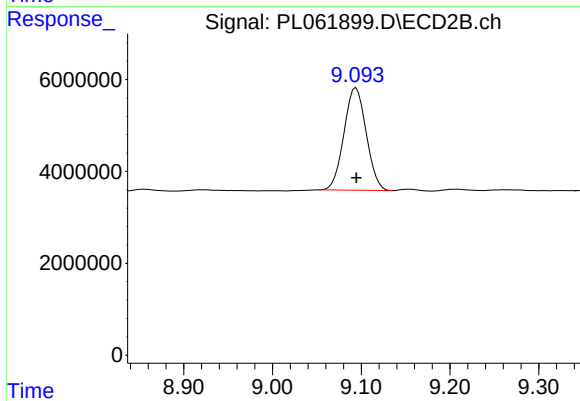

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 38877143
Conc: 17.66 ng/ml