

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
 Data File : PL061900.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 15:01
 Operator : DD\AJ
 Sample : L4198-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 16:09:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.007	25502460	38631551	14.949	14.160
28)	SA Decachlor...	8.209	9.094	24620957	33138914	15.135	15.054
Target Compounds							
10)	B gamma-Chl...	0.000	6.122	0	4702219	N.D.	1.601 #
11)	B alpha-Chl...	0.000	6.196	0	6772753	N.D.	2.255 #
16)	A 4,4'-DDD	0.000	6.846	0	4818250	N.D.	2.167 #
17)	MA 4,4'-DDT	6.375	7.144	22905347	37255060	18.157	17.013
25)	Chlordane-3	0.000	6.122	0	4702219	N.D.	12.832 #
26)	Chlordane-4	0.000	6.196	0	6772753	N.D.	15.087 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
Data File : PL061900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 15:01
Operator : DD\AJ
Sample : L4198-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 16:09:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

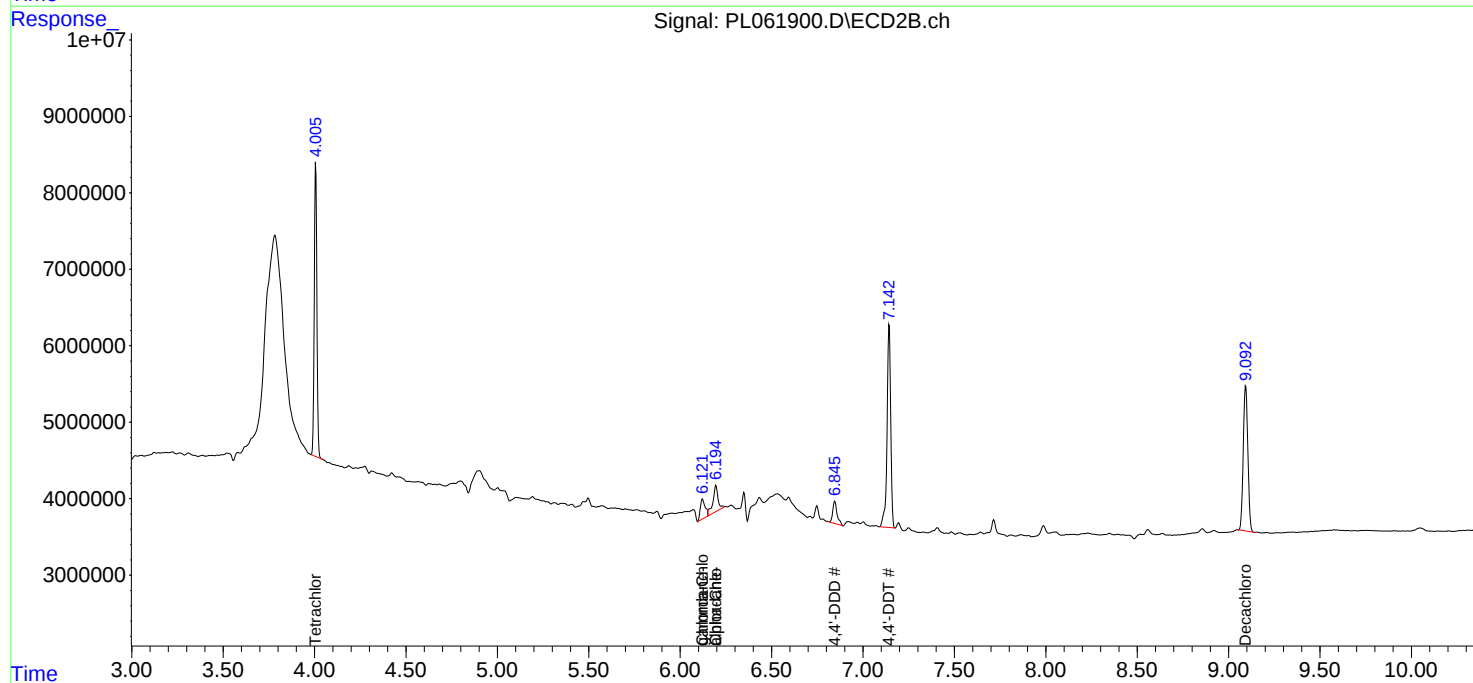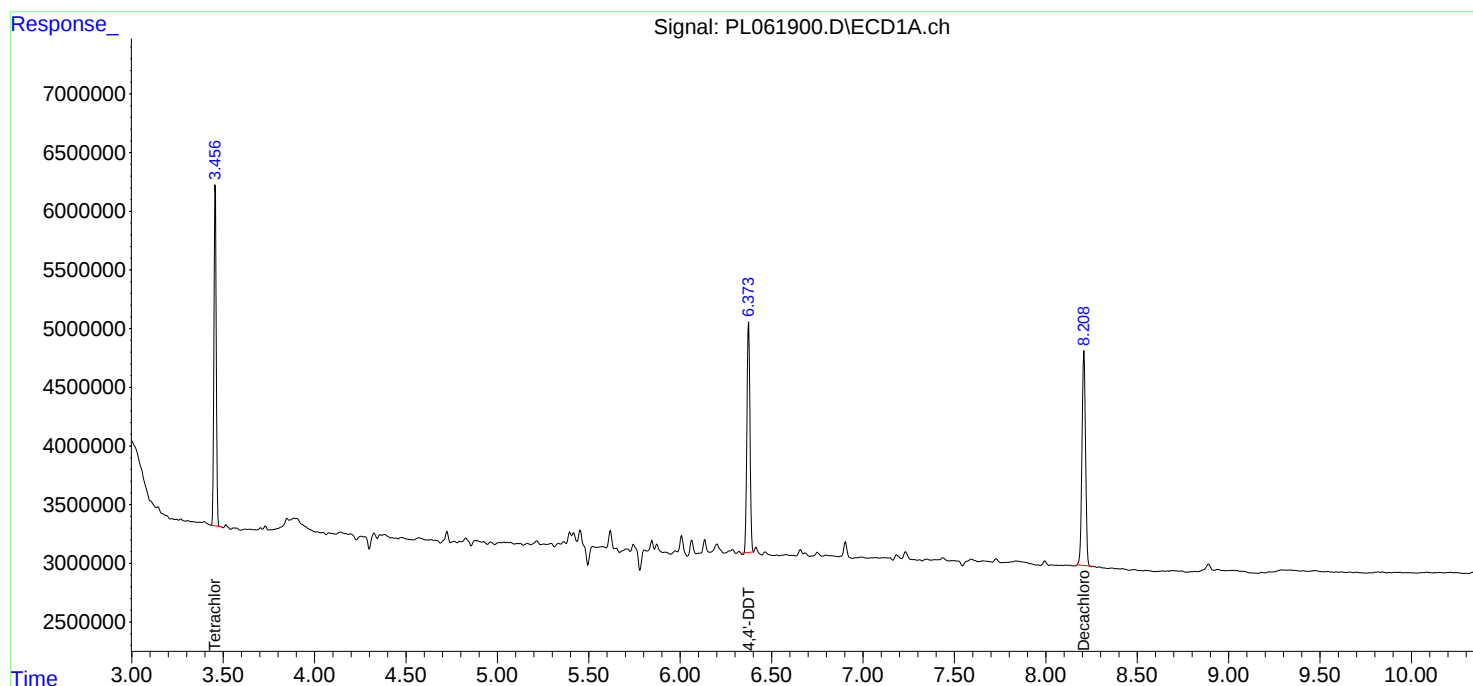


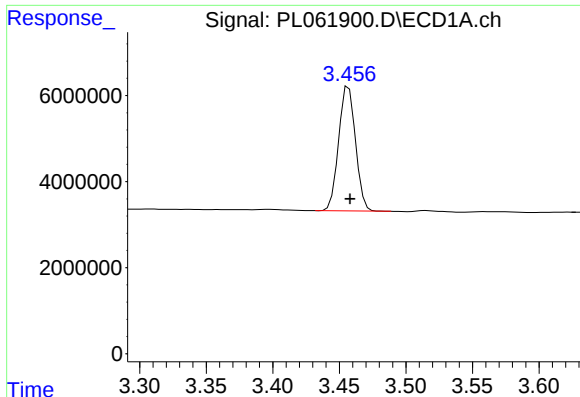

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 25502460
Conc: 14.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

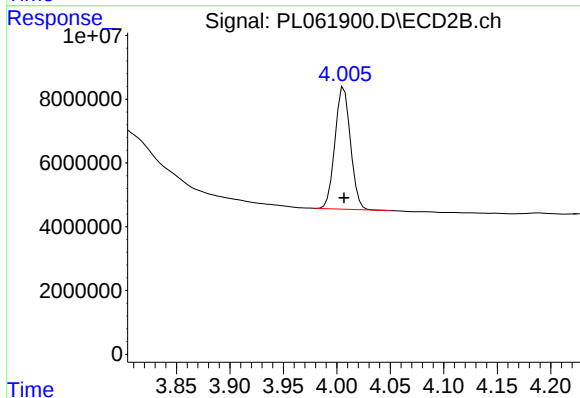


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 38631551
Conc: 14.16 ng/ml

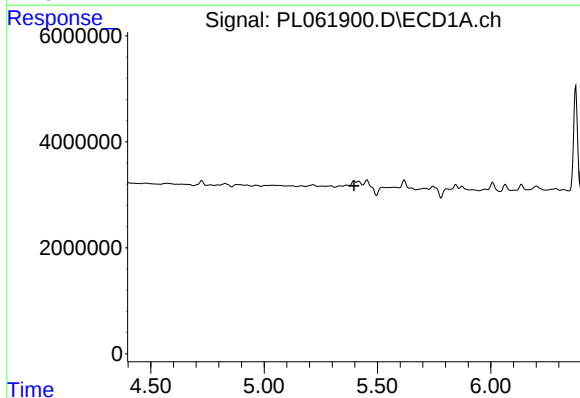


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

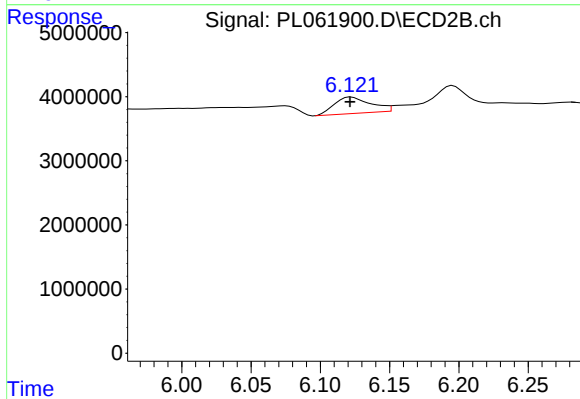

#10 gamma-Chlordane


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 4702219
Conc: 1.60 ng/ml

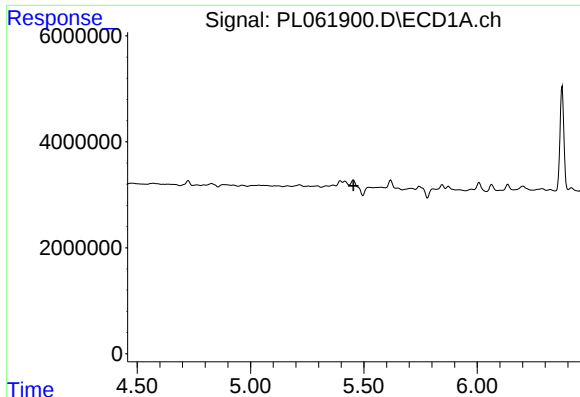

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

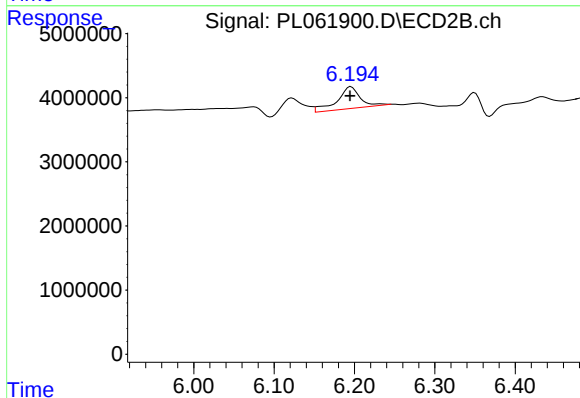


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: 0.001 min
Response: 6772753
Conc: 2.25 ng/ml

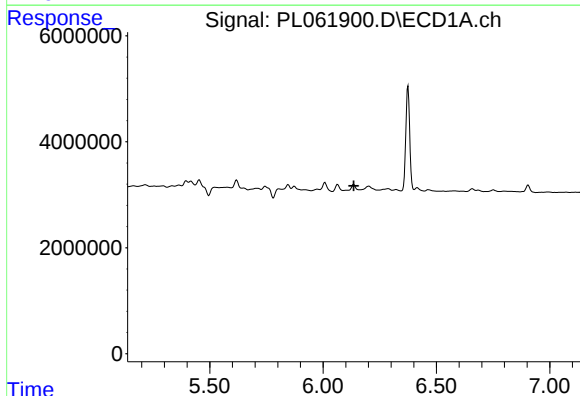


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.135 min
Response: 0
Conc: N.D.

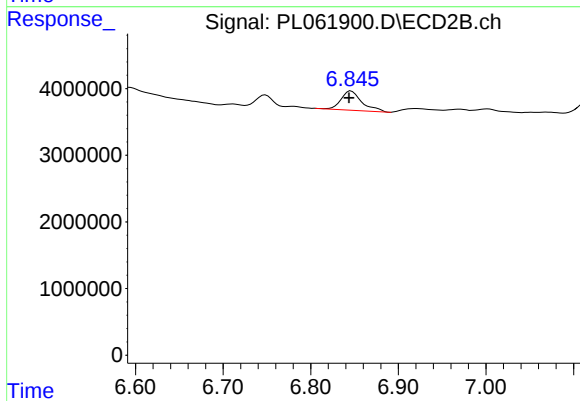

#16 4,4'-DDD


R.T.: 6.846 min
Delta R.T.: 0.002 min
Response: 4818250
Conc: 2.17 ng/ml

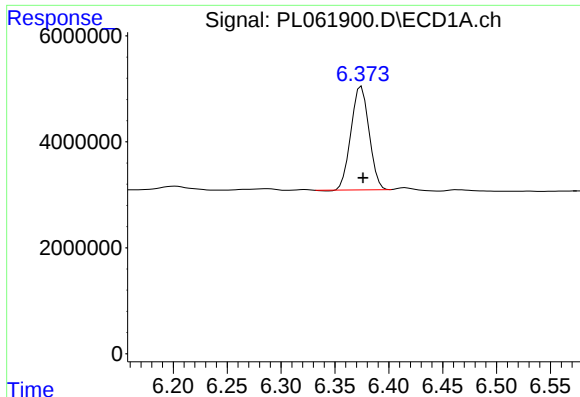

#17 4,4'-DDT


R.T.: 6.375 min
Delta R.T.: -0.002 min
Response: 22905347
Conc: 18.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

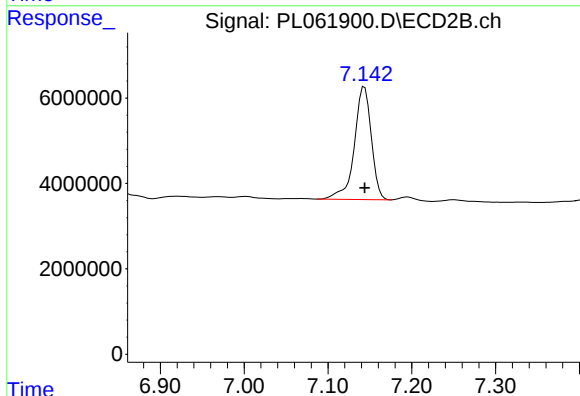


#17 4,4'-DDT

R.T.: 7.144 min
Delta R.T.: 0.000 min
Response: 37255060
Conc: 17.01 ng/ml

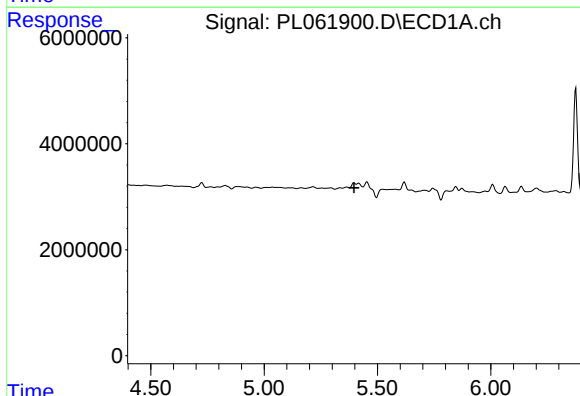


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

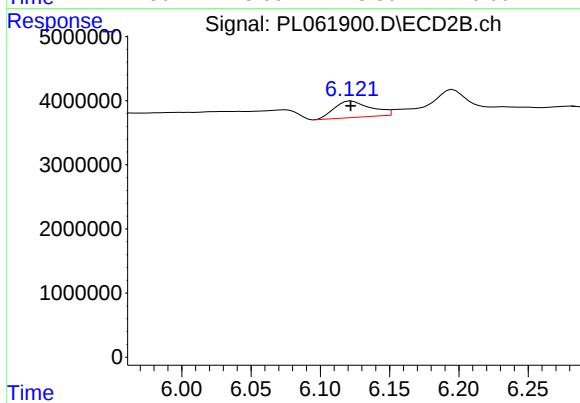

#25 Chlordane-3


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 4702219
Conc: 12.83 ng/ml

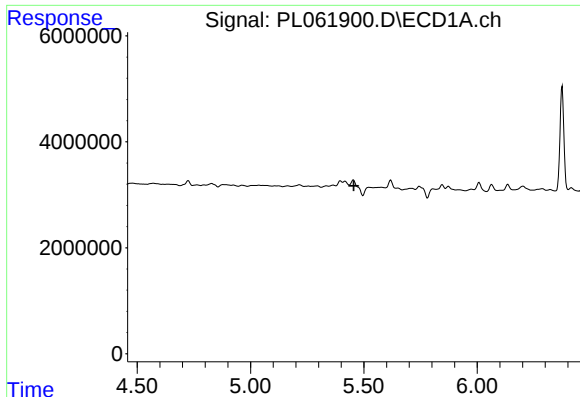

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

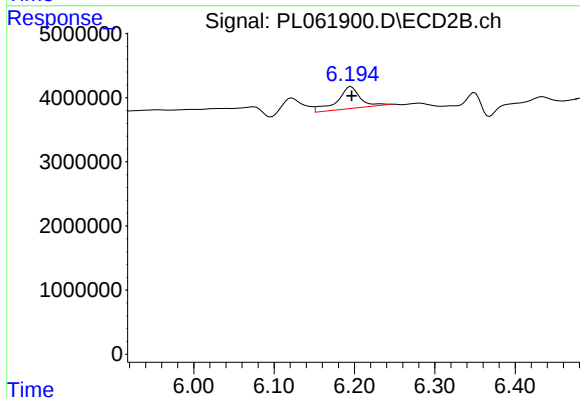


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 6772753
Conc: 15.09 ng/ml

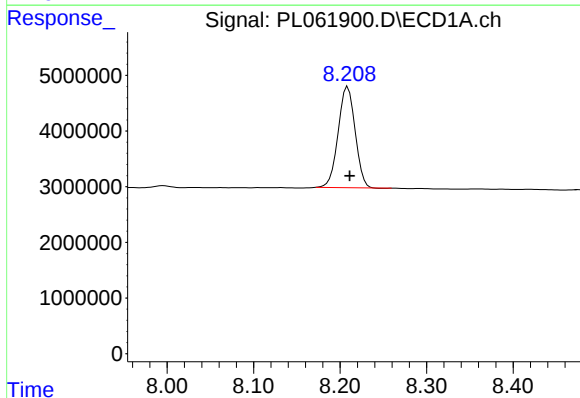

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.003 min
Response: 24620957
Conc: 15.13 ng/ml

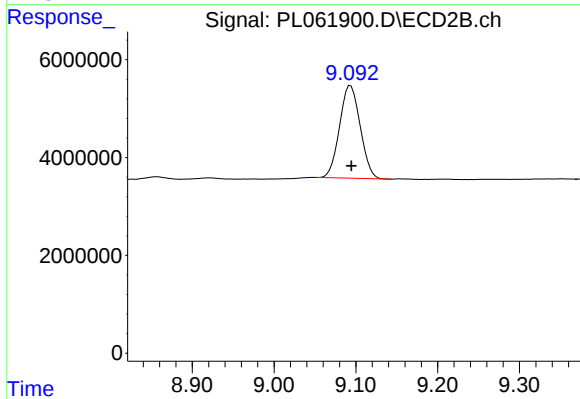

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 33138914
Conc: 15.05 ng/ml