

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
 Data File : PL061901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 15:15
 Operator : DD\AJ
 Sample : L4198-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 16:09:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.007	26607808	40736163	15.597	14.931
28)	SA Decachlor...	8.209	9.093	24052251	32959576	14.785	14.972
Target Compounds							
5)	MB Aldrin	0.000	5.469f	0	4125503	N.D.	1.274 #
10)	B gamma-Chl...	5.396	6.121	8566289	17504909	4.933	5.961
11)	B alpha-Chl...	5.454	6.196	13709201	32259535	7.892	10.741 #
15)	B Endosulfa...	6.288	0.000	3353291	0	2.074	N.D. #
23)	Chlordane-1	4.326	0.000	1874452	0	37.856	N.D. #
24)	Chlordane-2	0.000	5.469	0	4125503	N.D.	40.090 #
25)	Chlordane-3	5.396	6.121	8566289	17504909	54.499	47.771
26)	Chlordane-4	5.454	6.196	13709201	32259535	105.074	71.861 #
27)	Chlordane-5	6.288	7.003	3353291	5511059	61.499	75.826



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
Data File : PL061901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 15:15
Operator : DD\AJ
Sample : L4198-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 16:09:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

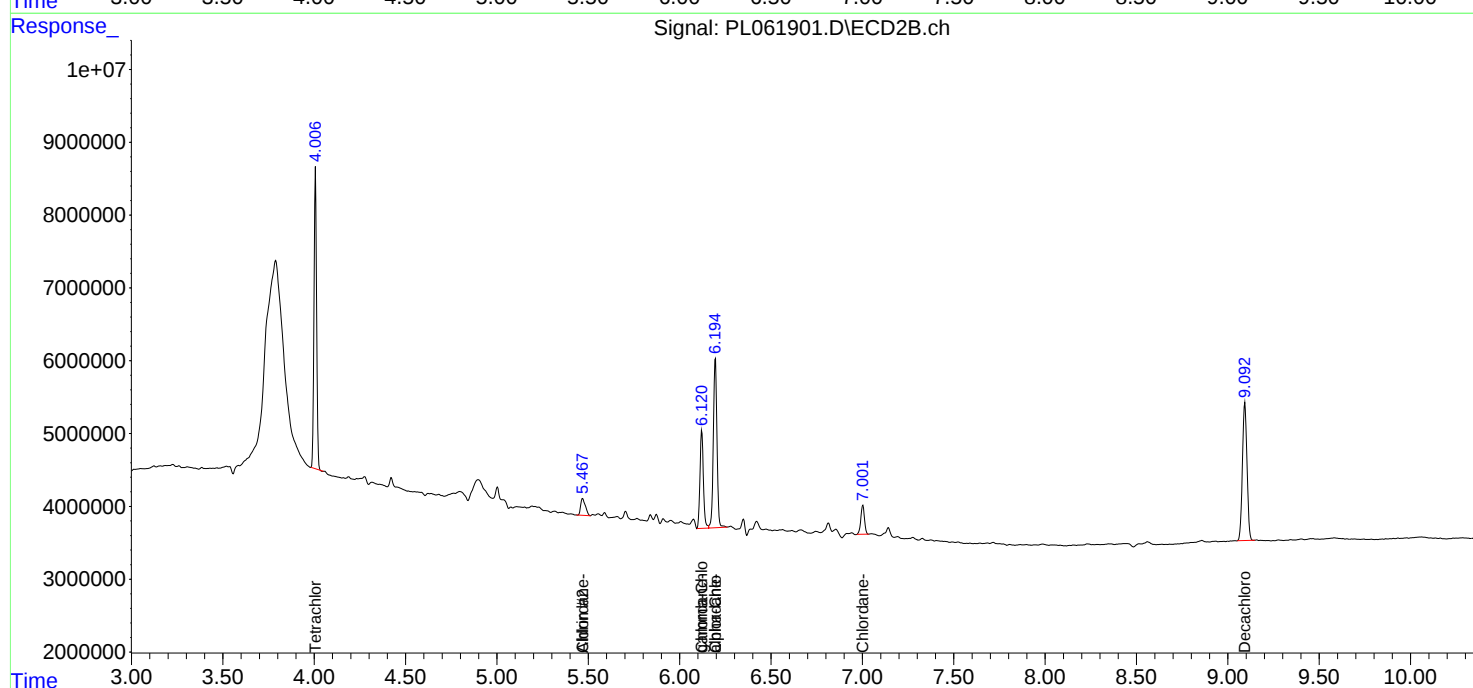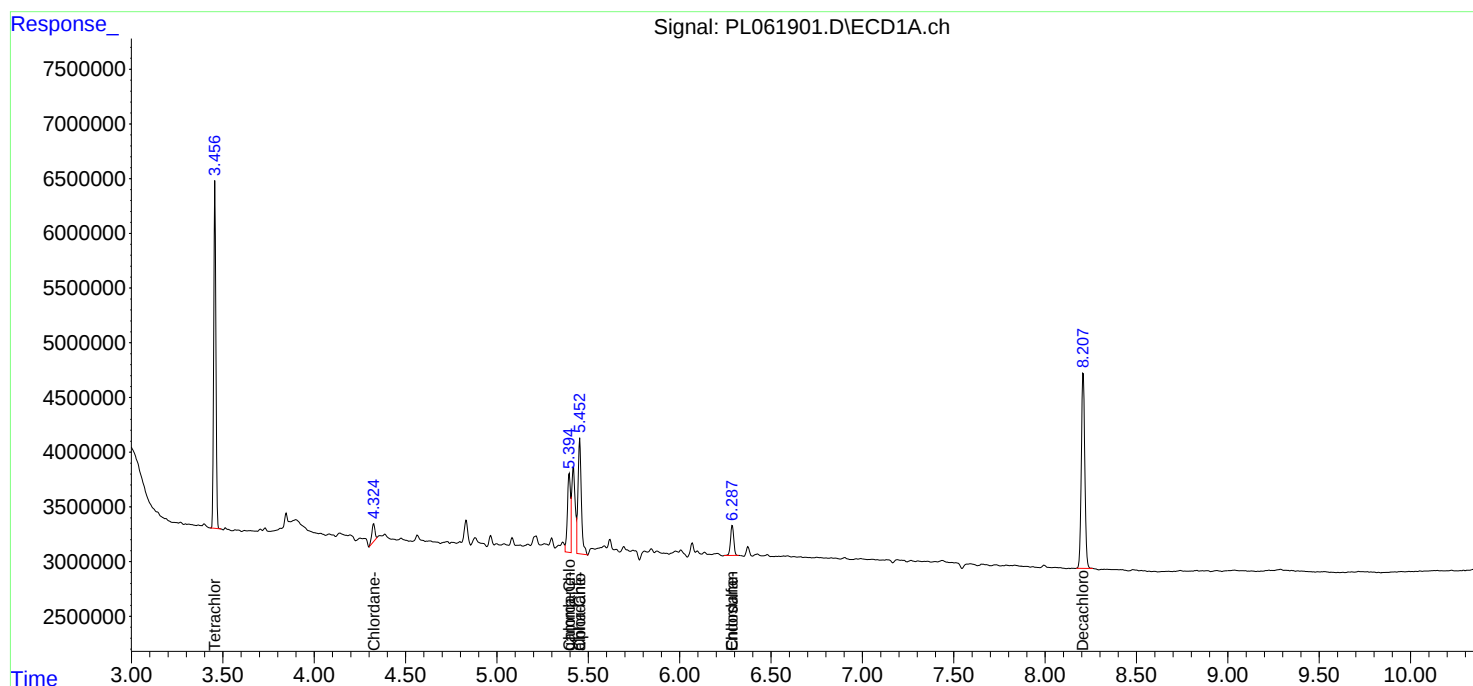


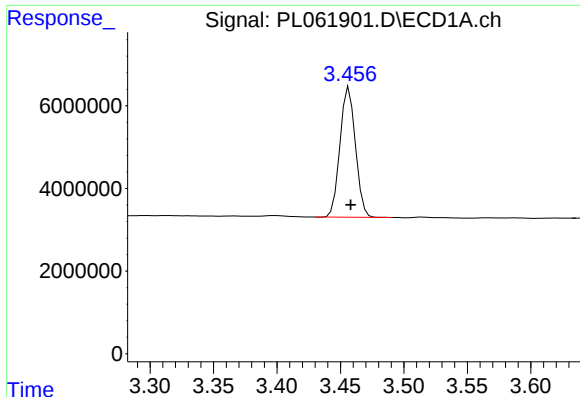

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 26607808
Conc: 15.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

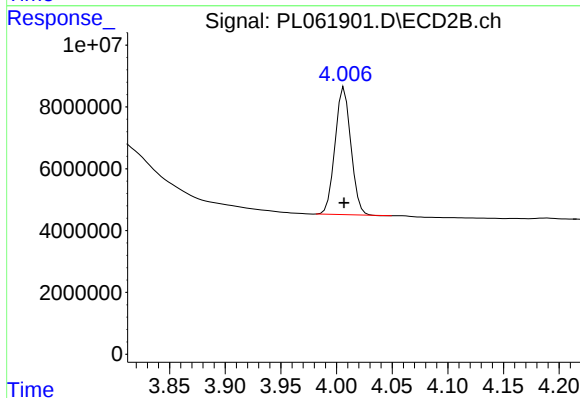


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 40736163
Conc: 14.93 ng/ml

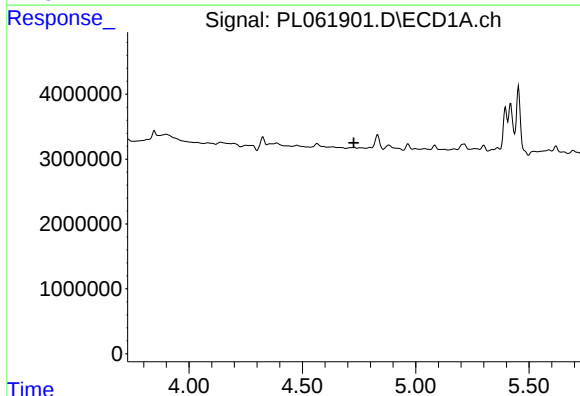


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

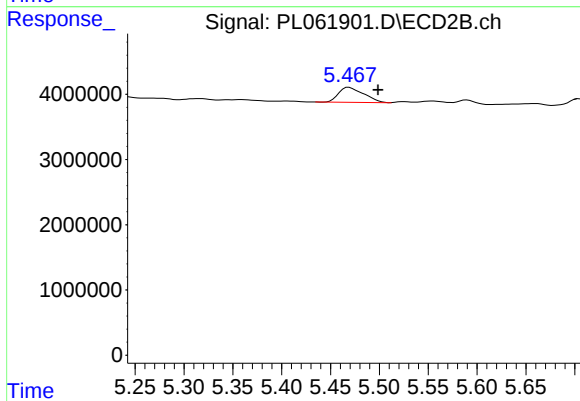

#5 Aldrin


R.T.: 5.469 min
Delta R.T.: -0.030 min
Response: 4125503
Conc: 1.27 ng/ml

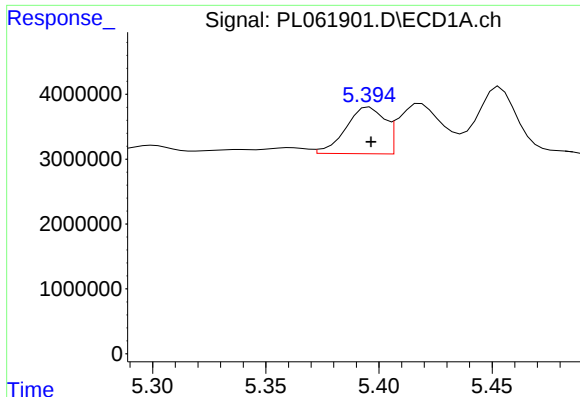

#10 gamma-Chlordane


R.T.: 5.396 min
Delta R.T.: 0.000 min
Response: 8566289
Conc: 4.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

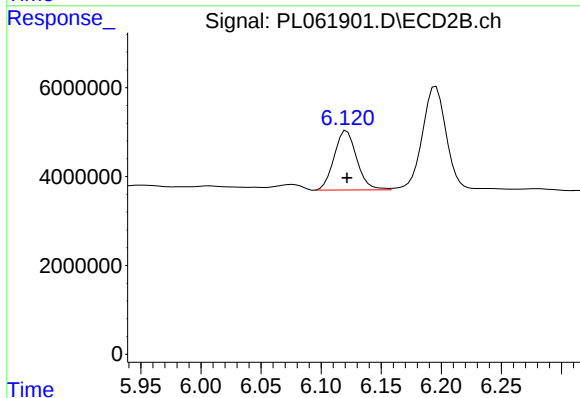


#10 gamma-Chlordane

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 17504909
Conc: 5.96 ng/ml

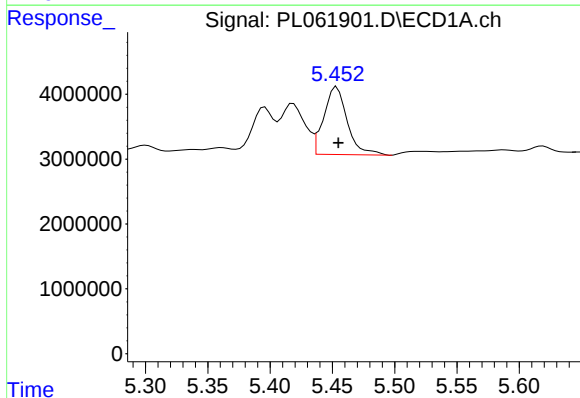


#11 alpha-Chlordane

R.T.: 5.454 min
Delta R.T.: -0.001 min
Response: 13709201
Conc: 7.89 ng/ml

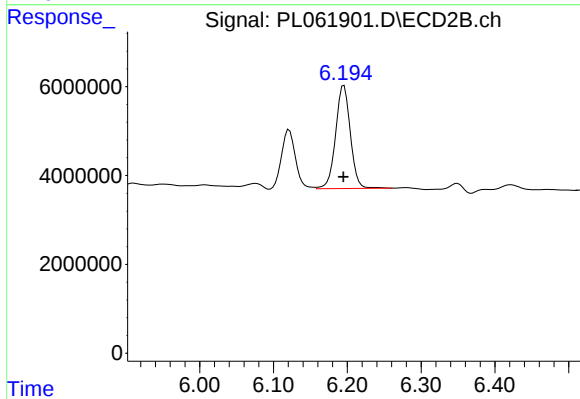

#11 alpha-Chlordane


R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 32259535
Conc: 10.74 ng/ml

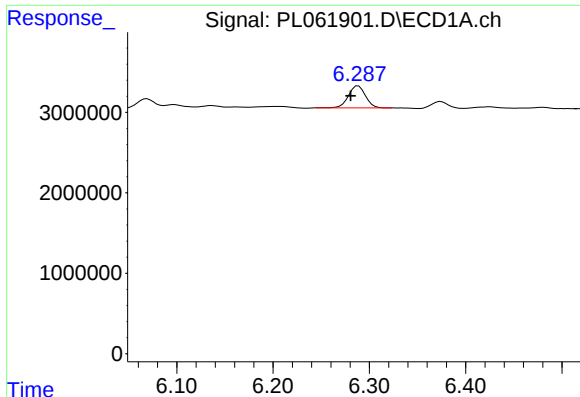

#15 Endosulfan II


R.T.: 6.288 min
Delta R.T.: 0.008 min
Response: 3353291
Conc: 2.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

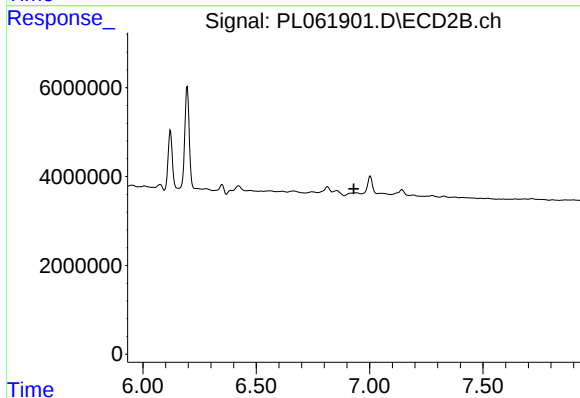


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.931 min
Response: 0
Conc: N.D.

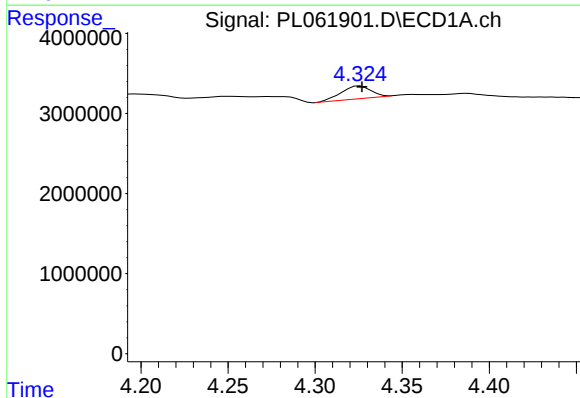


#23 Chlordane-1

R.T.: 4.326 min
Delta R.T.: -0.001 min
Response: 1874452
Conc: 37.86 ng/ml

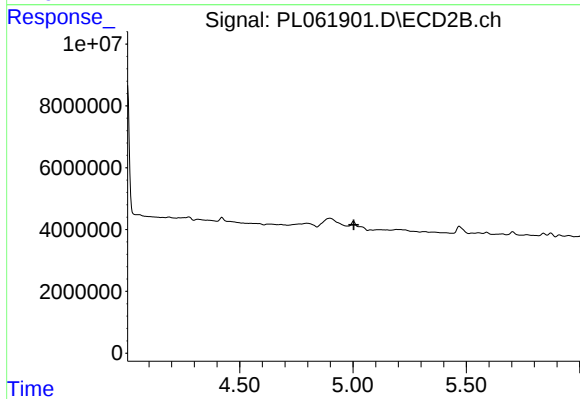

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

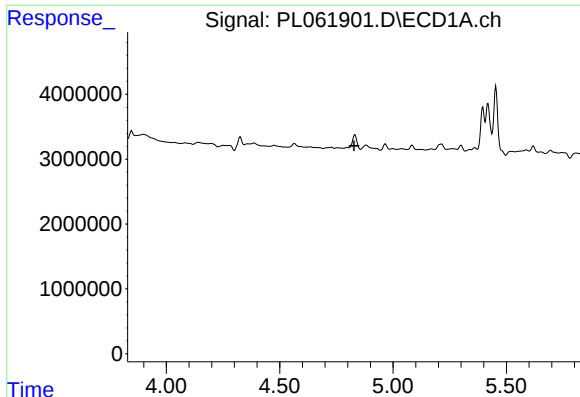

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.829 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

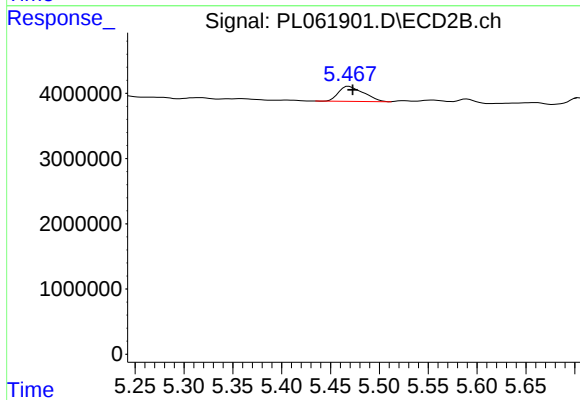


#24 Chlordane-2

R.T.: 5.469 min
Delta R.T.: -0.004 min
Response: 4125503
Conc: 40.09 ng/ml

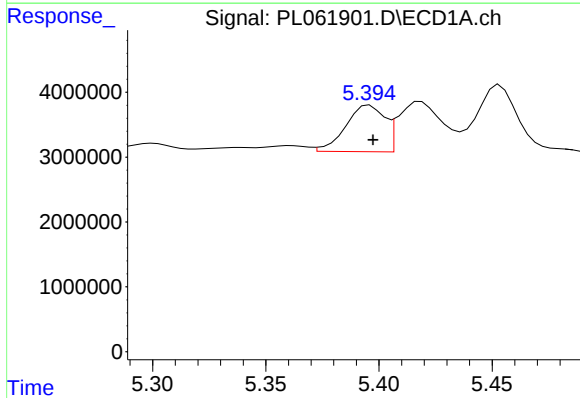


#25 Chlordane-3

R.T.: 5.396 min
Delta R.T.: -0.001 min
Response: 8566289
Conc: 54.50 ng/ml

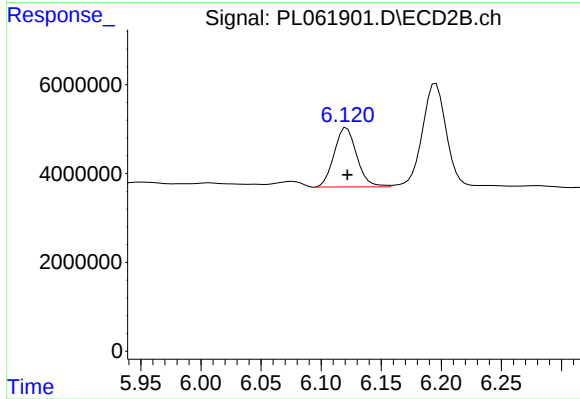

#25 Chlordane-3


R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 17504909
Conc: 47.77 ng/ml

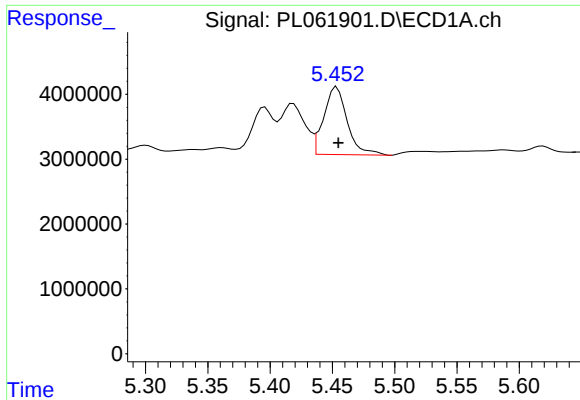

#26 Chlordane-4


R.T.: 5.454 min
Delta R.T.: -0.001 min
Response: 13709201
Conc: 105.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

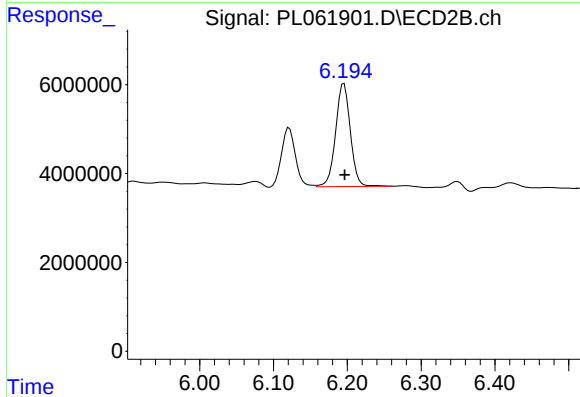


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: -0.001 min
Response: 32259535
Conc: 71.86 ng/ml

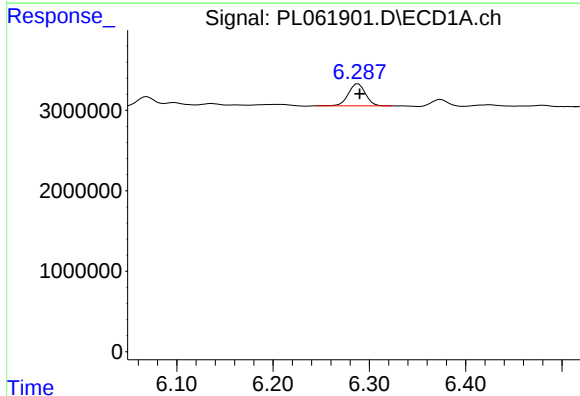


#27 Chlordane-5

R.T.: 6.288 min
Delta R.T.: -0.002 min
Response: 3353291
Conc: 61.50 ng/ml

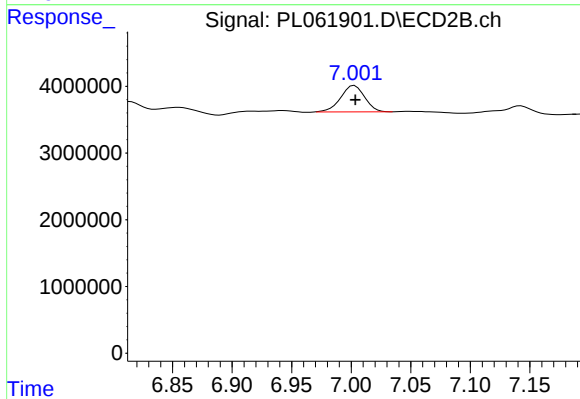

#27 Chlordane-5


R.T.: 7.003 min
Delta R.T.: 0.000 min
Response: 5511059
Conc: 75.83 ng/ml

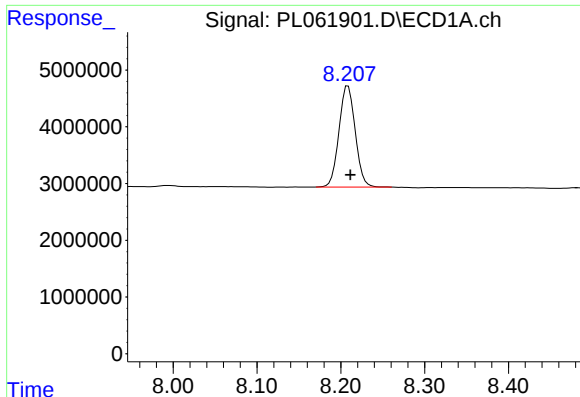

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.003 min
Response: 24052251
Conc: 14.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

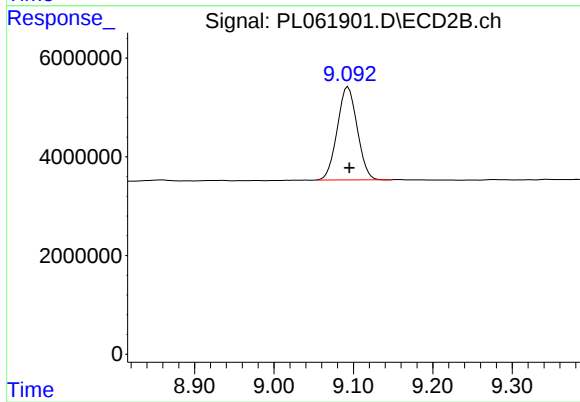

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.001 min
Response: 32959576
Conc: 14.97 ng/ml