

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
 Data File : PL061905.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 16:12
 Operator : DD\AJ
 Sample : L4198-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 03:38:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.006	26749669	40015649	15.680	14.667
28)	SA Decachlor...	8.211	9.095	27410283	37226661	16.850	16.911
Target Compounds							
2)	A alpha-BHC	0.000	4.422f	0	2783748	N.D.	0.697 #
9)	A Endosulfan I	5.522	0.000	4121676	0	2.544	N.D. #
10)	B gamma-Chl...	5.419f	6.124	17028161	3294716	9.805	1.122 #
11)	B alpha-Chl...	0.000	6.197	0	6287695	N.D.	2.093 #
12)	B 4,4'-DDE	5.620	6.351	20355577	31366176	12.952	11.490
17)	MA 4,4'-DDT	6.375	7.144	10715242	18435953	8.494	8.419
23)	Chlordane-1	4.323	0.000	5568639	0	112.462	N.D. #
25)	Chlordane-3	5.419f	6.124	17028161	3294716	108.334	8.991 #
26)	Chlordane-4	0.000	6.197	0	6287695	N.D.	14.006 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
Data File : PL061905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 16:12
Operator : DD\AJ
Sample : L4198-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 03:38:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

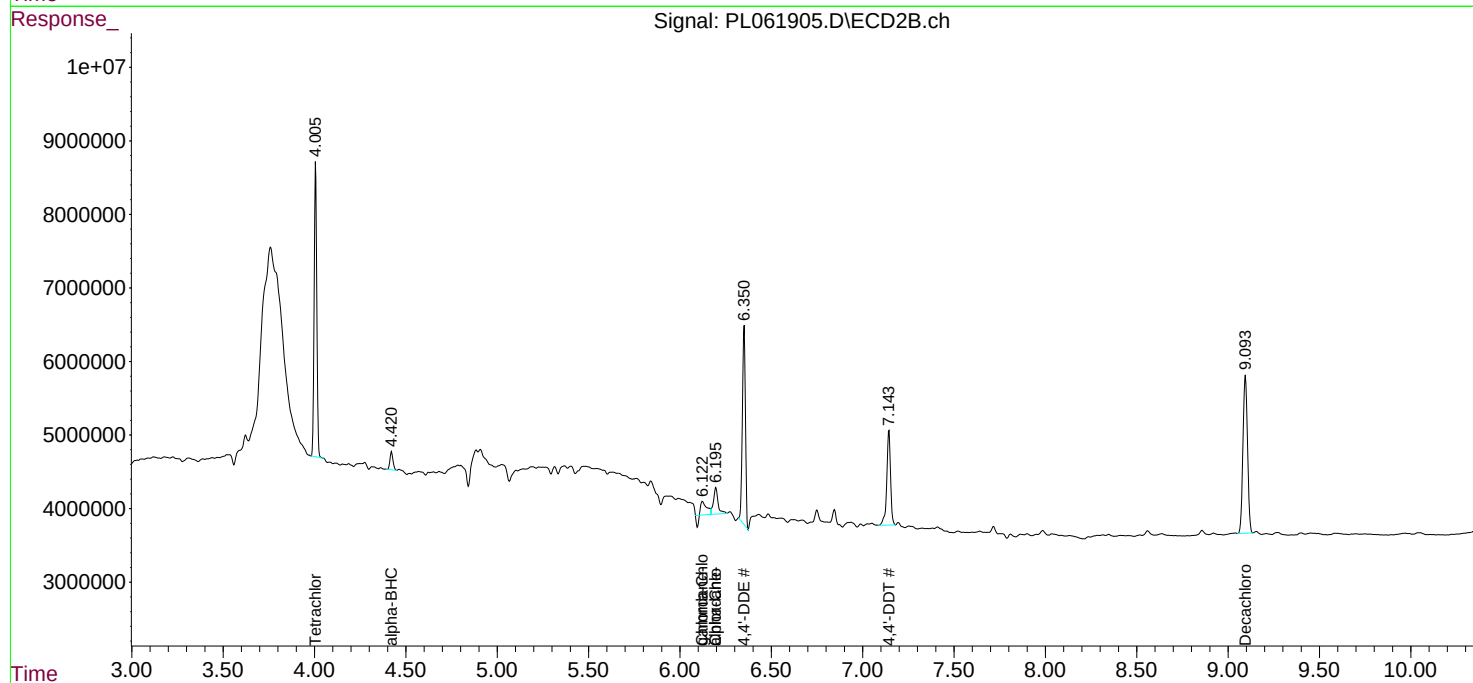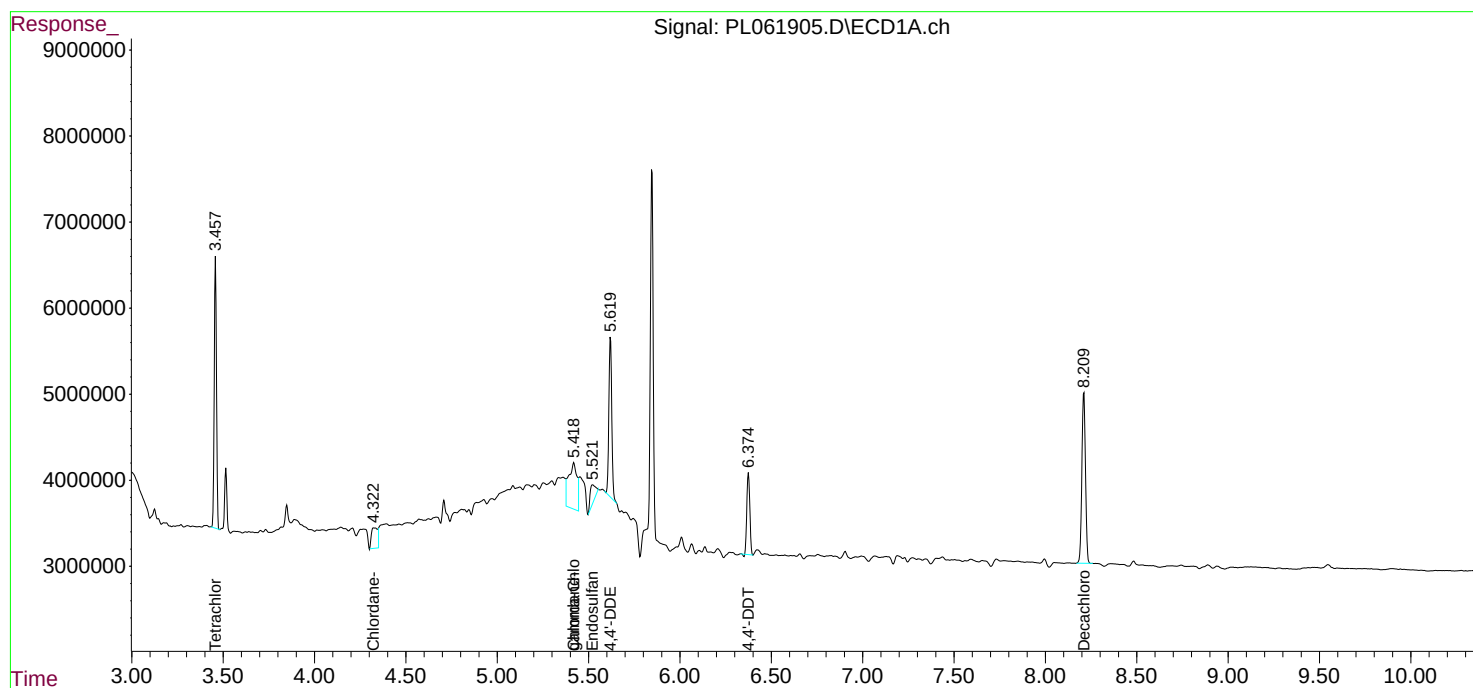


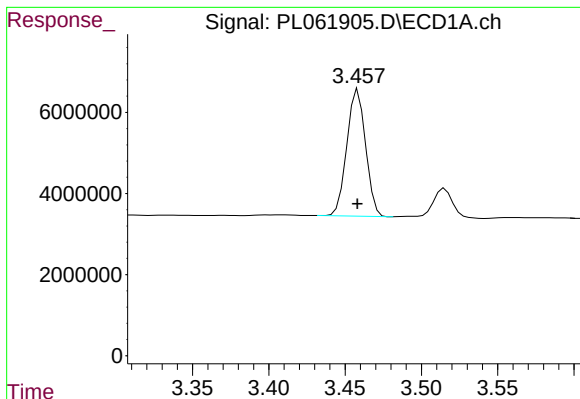

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 26749669
Conc: 15.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

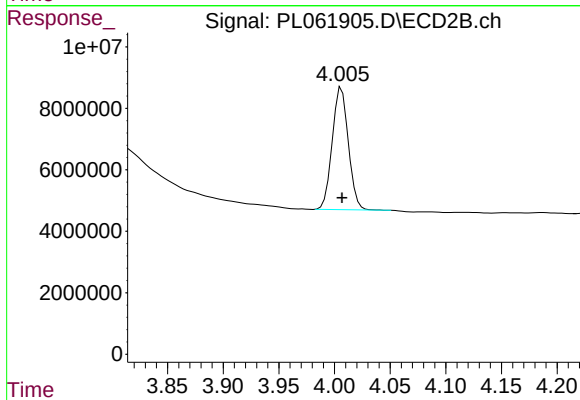


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 40015649
Conc: 14.67 ng/ml

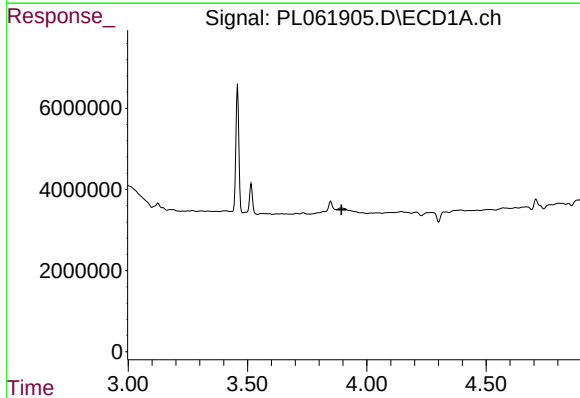


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.894 min
Response: 0
Conc: N.D.

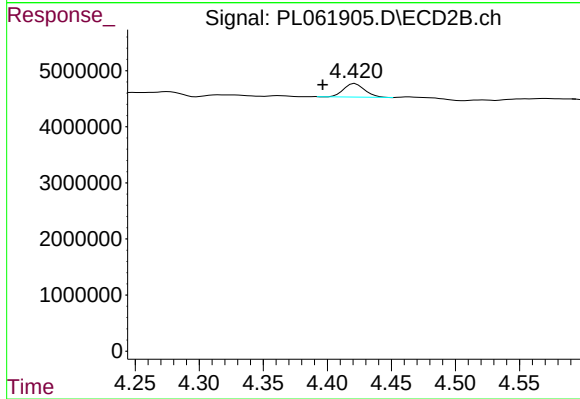

#2 alpha-BHC


R.T.: 4.422 min
Delta R.T.: 0.025 min
Response: 2783748
Conc: 0.70 ng/ml

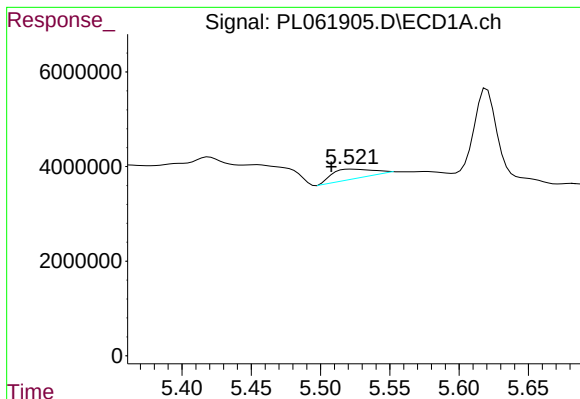

#9 Endosulfan I


R.T.: 5.522 min
Delta R.T.: 0.014 min
Response: 4121676
Conc: 2.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

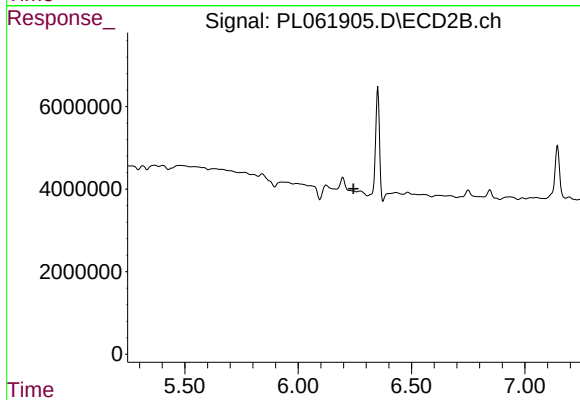


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

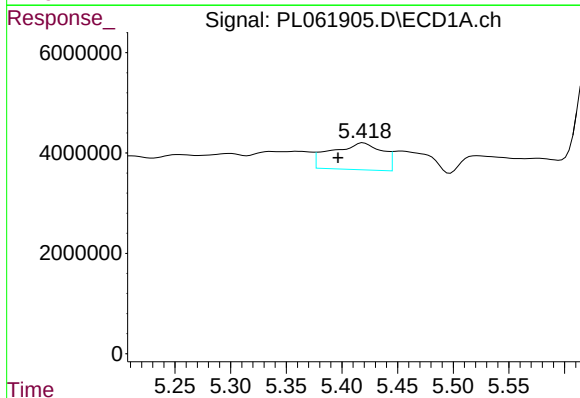


#10 gamma-Chlordane

R.T.: 5.419 min
Delta R.T.: 0.023 min
Response: 17028161
Conc: 9.81 ng/ml

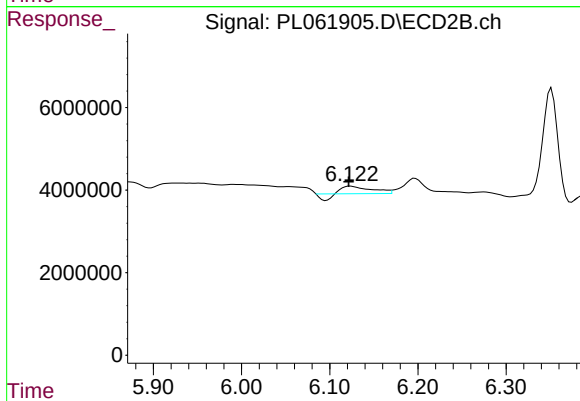

#10 gamma-Chlordane


R.T.: 6.124 min
Delta R.T.: 0.002 min
Response: 3294716
Conc: 1.12 ng/ml

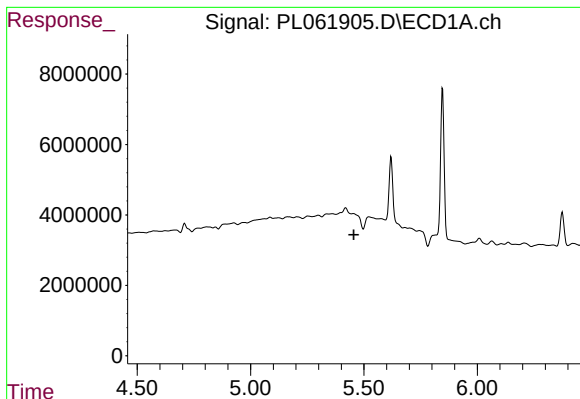

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

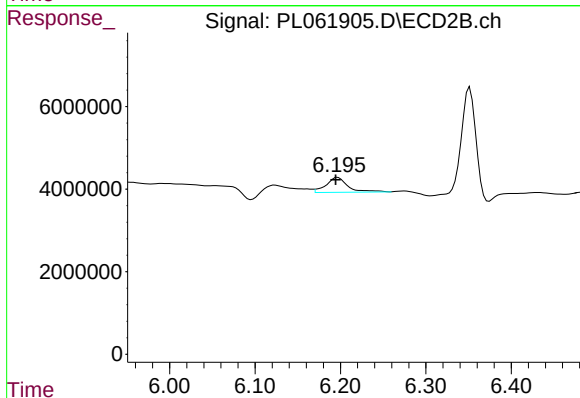


#11 alpha-Chlordane

R.T.: 6.197 min
Delta R.T.: 0.002 min
Response: 6287695
Conc: 2.09 ng/ml

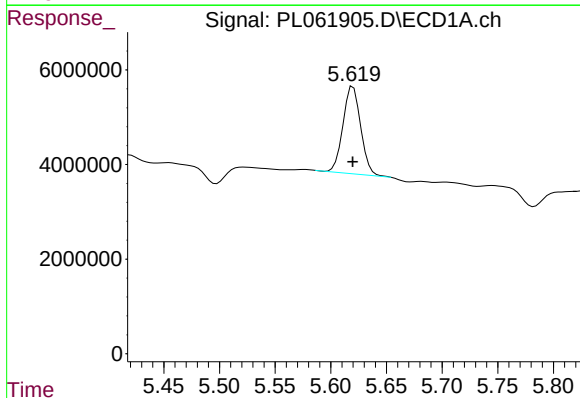


#12 4,4'-DDE

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 20355577
Conc: 12.95 ng/ml

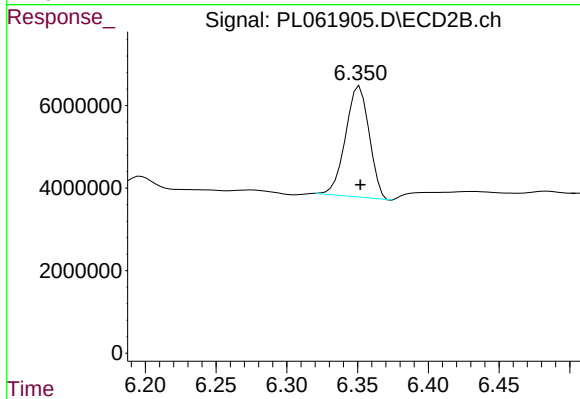

#12 4,4'-DDE


R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 31366176
Conc: 11.49 ng/ml

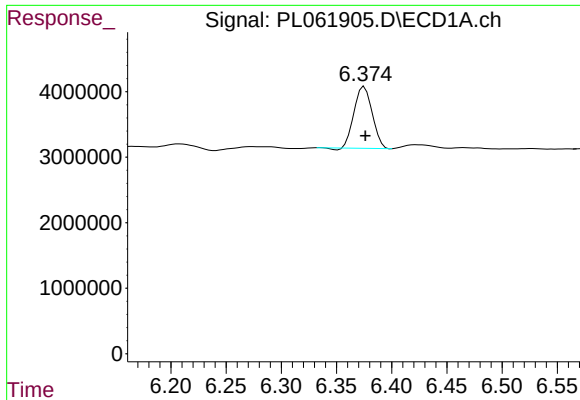

#17 4,4'-DDT


R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 10715242
Conc: 8.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

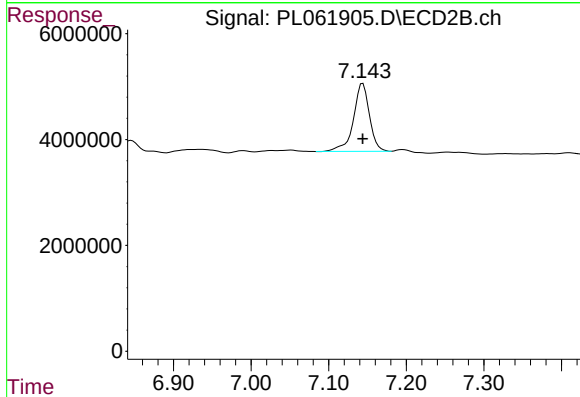


#17 4,4'-DDT

R.T.: 7.144 min
Delta R.T.: 0.000 min
Response: 18435953
Conc: 8.42 ng/ml

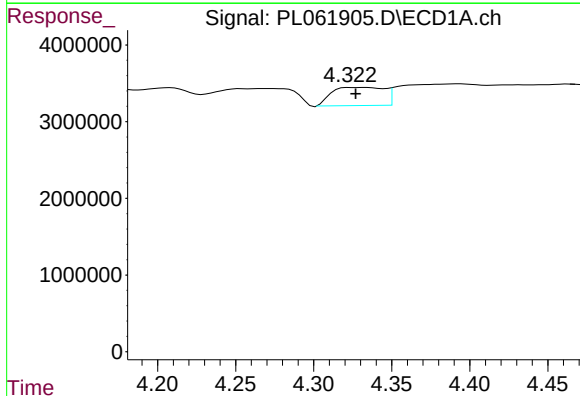


#23 Chlordane-1

R.T.: 4.323 min
Delta R.T.: -0.004 min
Response: 5568639
Conc: 112.46 ng/ml

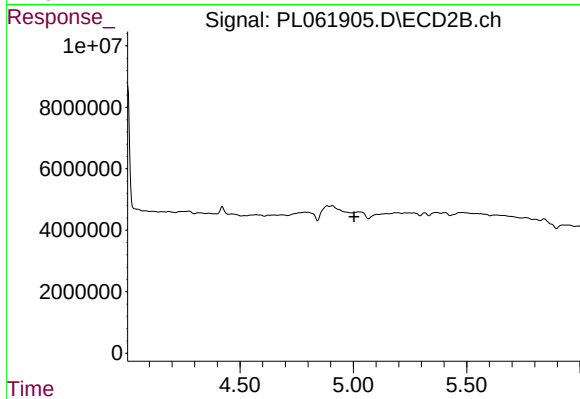

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

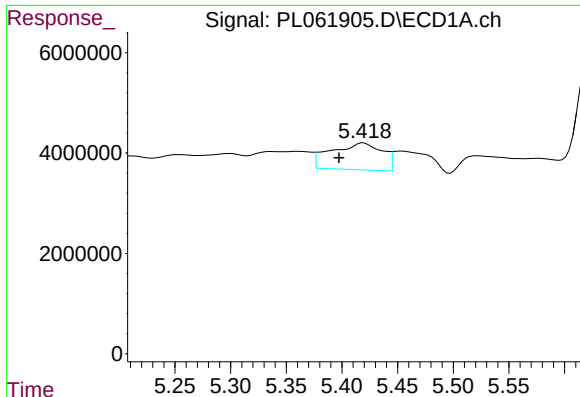

#25 Chlordane-3


R.T.: 5.419 min
Delta R.T.: 0.022 min
Response: 17028161
Conc: 108.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

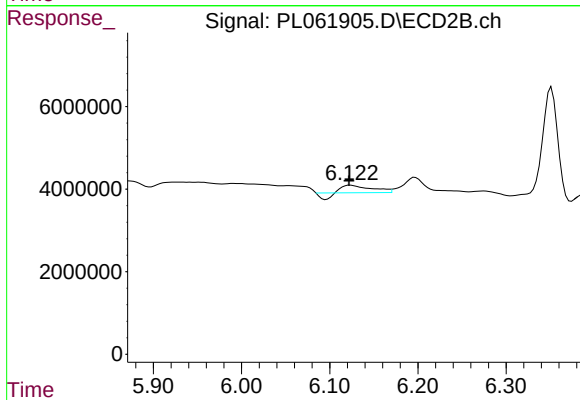


#25 Chlordane-3

R.T.: 6.124 min
Delta R.T.: 0.002 min
Response: 3294716
Conc: 8.99 ng/ml

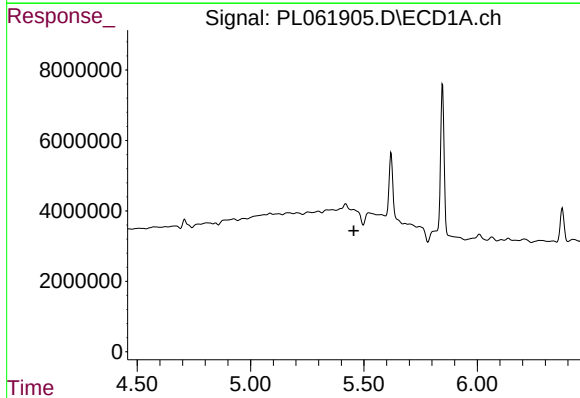


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

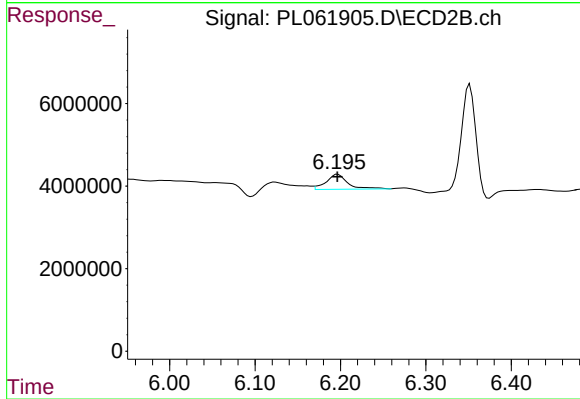

#26 Chlordane-4


R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 6287695
Conc: 14.01 ng/ml

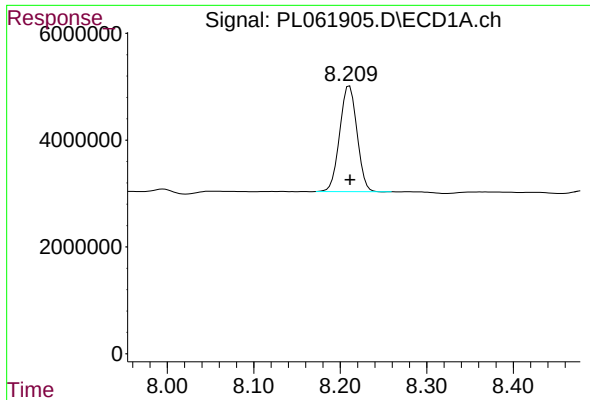

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 27410283
Conc: 16.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

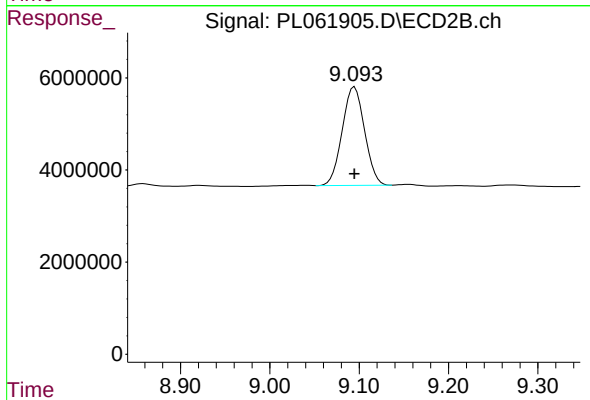

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 37226661
Conc: 16.91 ng/ml