

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
 Data File : PL061907.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 16:40
 Operator : DD\AJ
 Sample : L4198-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 03:39:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	26912616	40914246	15.776	14.997
28)	SA Decachlor...	8.208	9.095	31416256	25215621	19.312	11.455 #
Target Compounds							
2)	A alpha-BHC	0.000	4.422f	0	7980863	N.D.	1.998 #
10)	B gamma-Chl...	5.419f	6.123	2409718	15959813	1.388	5.435 #
11)	B alpha-Chl...	0.000	6.196	0	27871754	N.D.	9.280 #
12)	B 4,4'-DDE	5.619	6.348	3019061	6750171	1.921	2.473 #
17)	MA 4,4'-DDT	6.374	7.144	3183859	5208620	2.524	2.379
23)	Chlordane-1	4.326	0.000	2036734	0	41.133	N.D. #
25)	Chlordane-3	5.419f	6.123	2409718	15959813	15.331	43.554 #
26)	Chlordane-4	0.000	6.196	0	27871754	N.D.	62.087 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
Data File : PL061907.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 16:40
Operator : DD\AJ
Sample : L4198-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 03:39:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

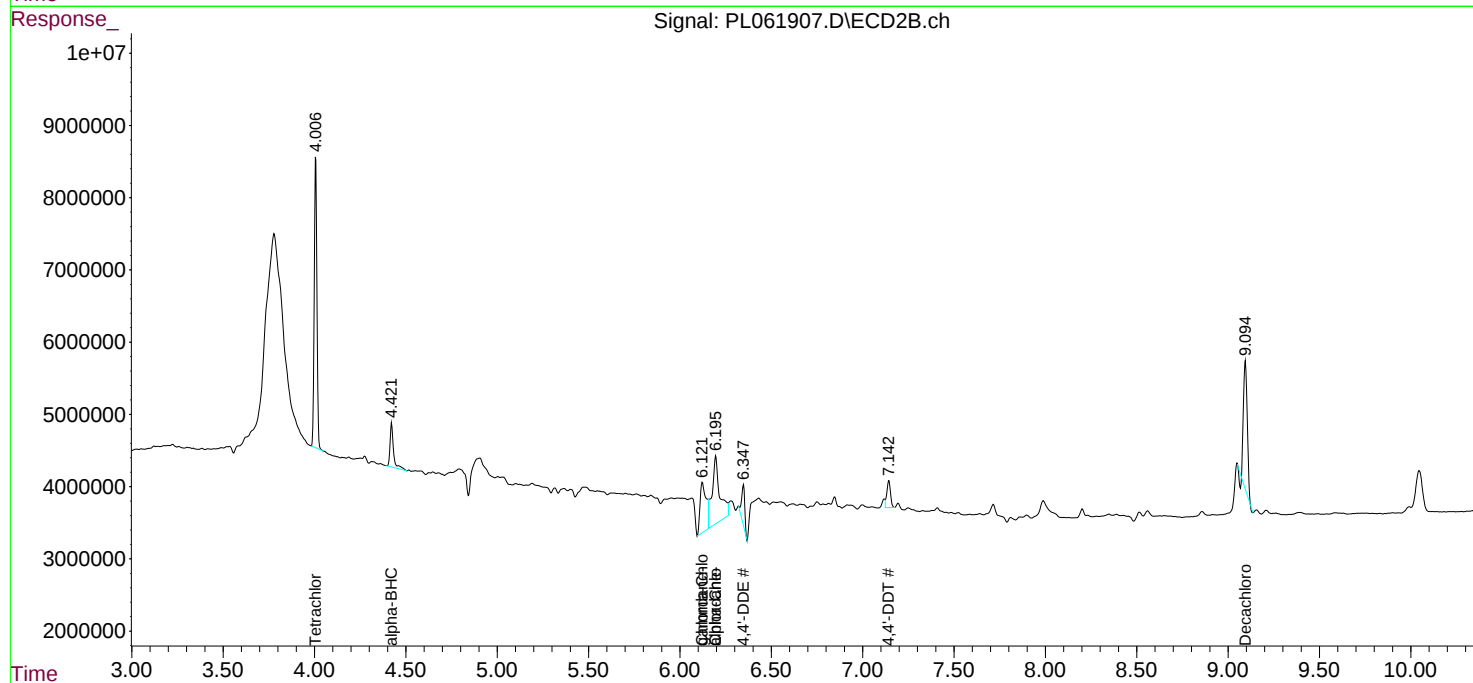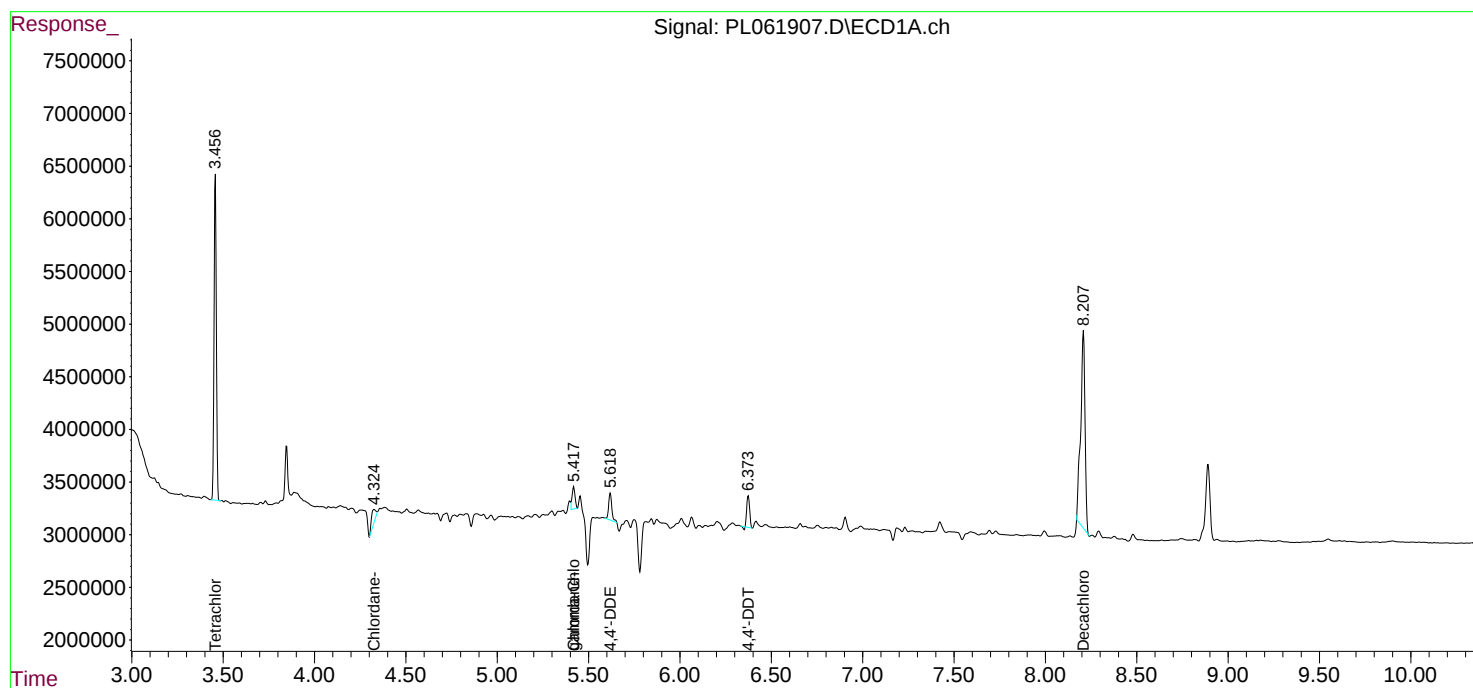


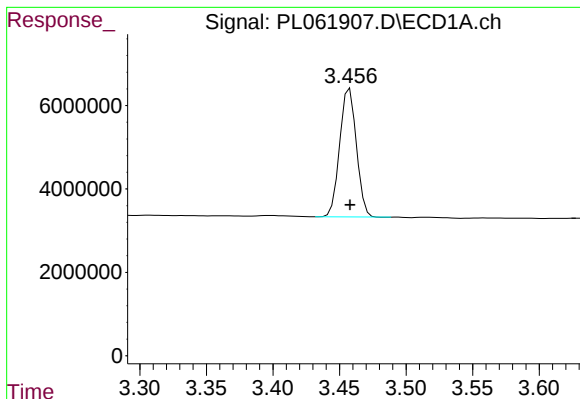

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 26912616
Conc: 15.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

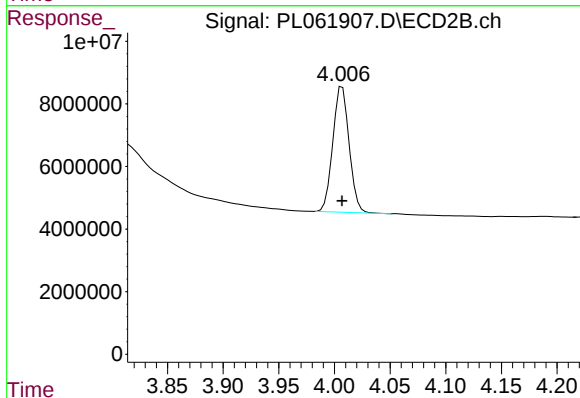


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 40914246
Conc: 15.00 ng/ml

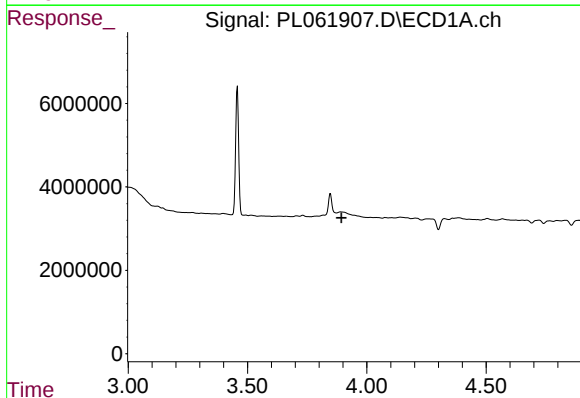


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.894 min
Response: 0
Conc: N.D.

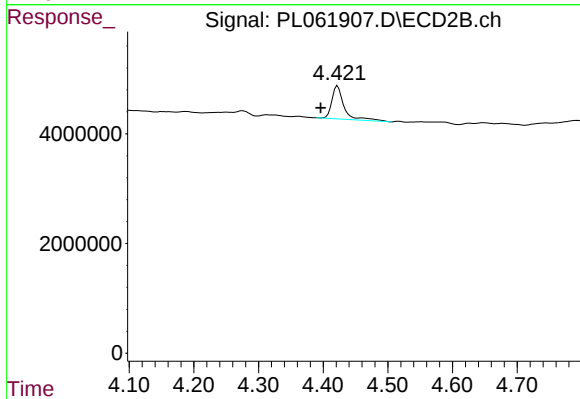

#2 alpha-BHC


R.T.: 4.422 min
Delta R.T.: 0.026 min
Response: 7980863
Conc: 2.00 ng/ml

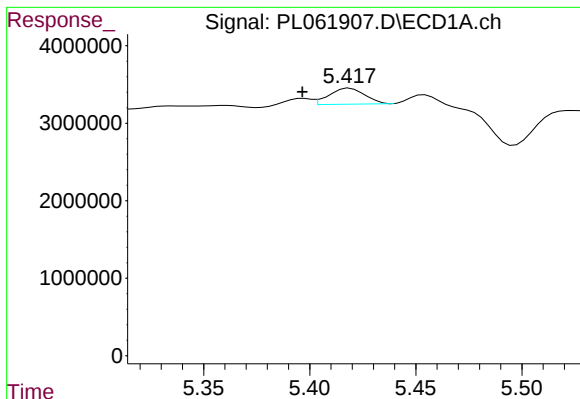

#10 gamma-Chlordane


R.T.: 5.419 min
Delta R.T.: 0.022 min
Response: 2409718
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

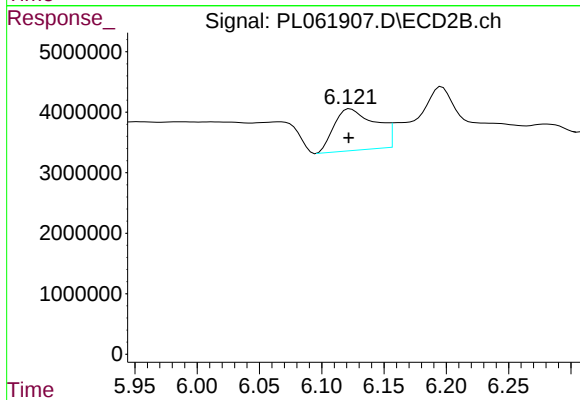


#10 gamma-Chlordane

R.T.: 6.123 min
Delta R.T.: 0.001 min
Response: 15959813
Conc: 5.43 ng/ml

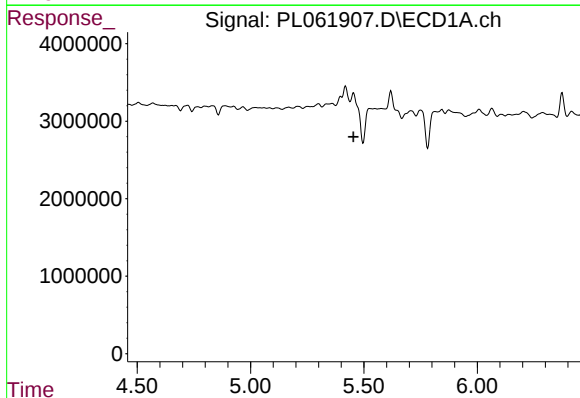


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

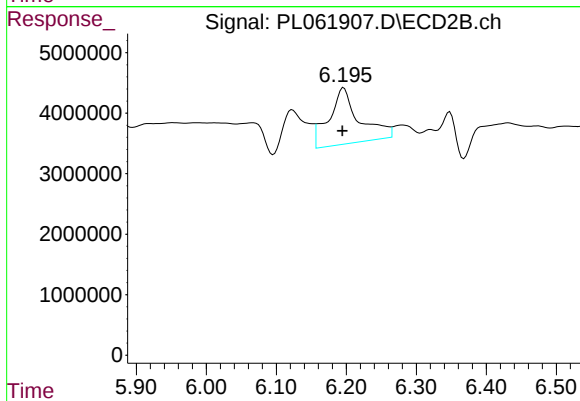

#11 alpha-Chlordane


R.T.: 6.196 min
Delta R.T.: 0.002 min
Response: 27871754
Conc: 9.28 ng/ml

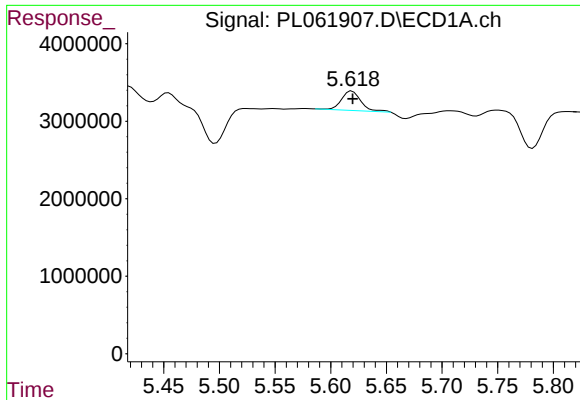

#12 4,4'-DDE


R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 3019061
Conc: 1.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

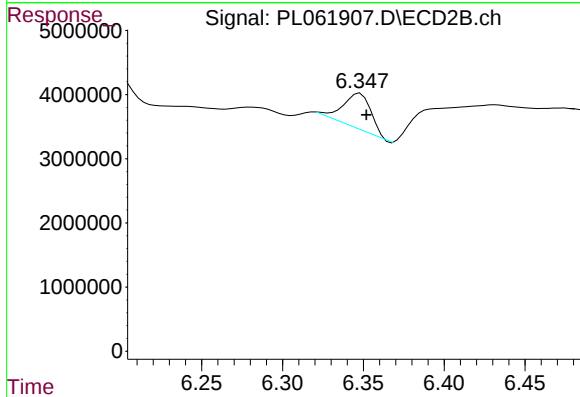


#12 4,4'-DDE

R.T.: 6.348 min
Delta R.T.: -0.004 min
Response: 6750171
Conc: 2.47 ng/ml

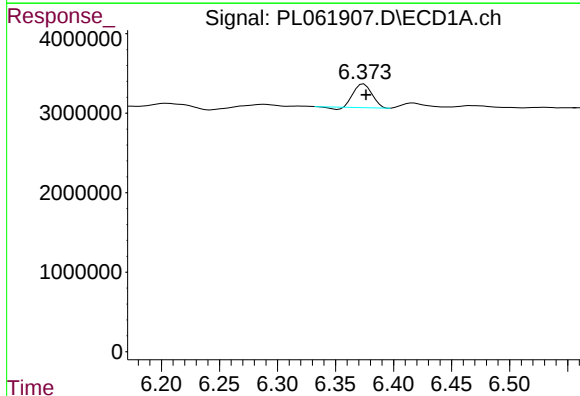


#17 4,4'-DDT

R.T.: 6.374 min
Delta R.T.: -0.002 min
Response: 3183859
Conc: 2.52 ng/ml

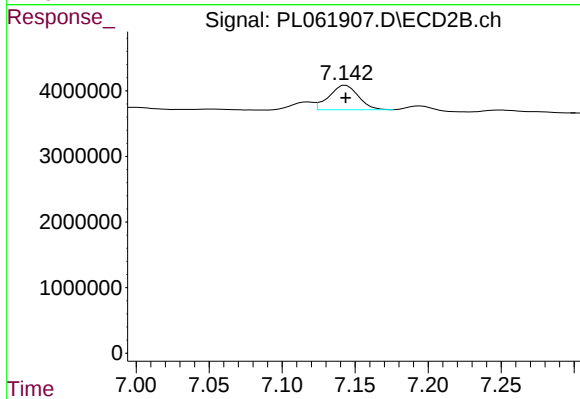

#17 4,4'-DDT


R.T.: 7.144 min
Delta R.T.: 0.000 min
Response: 5208620
Conc: 2.38 ng/ml

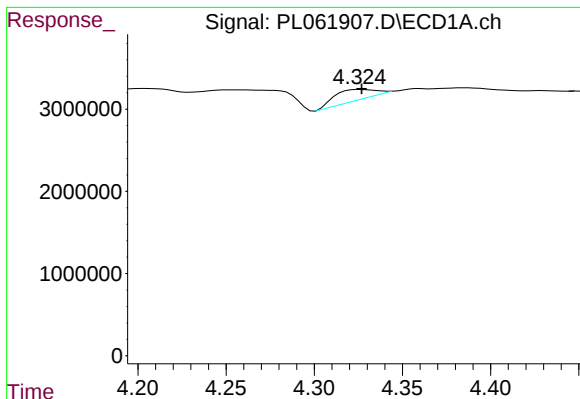

#23 Chlordane-1


R.T.: 4.326 min
Delta R.T.: 0.000 min
Response: 2036734
Conc: 41.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

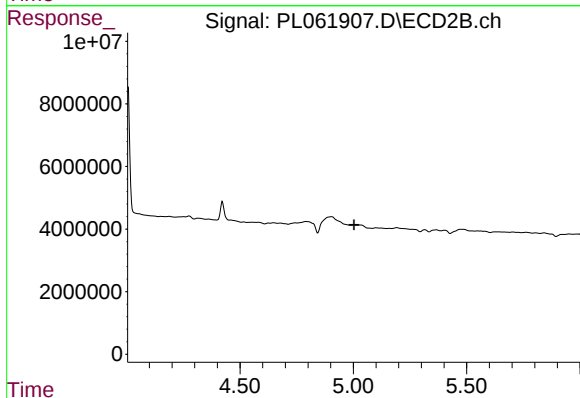


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

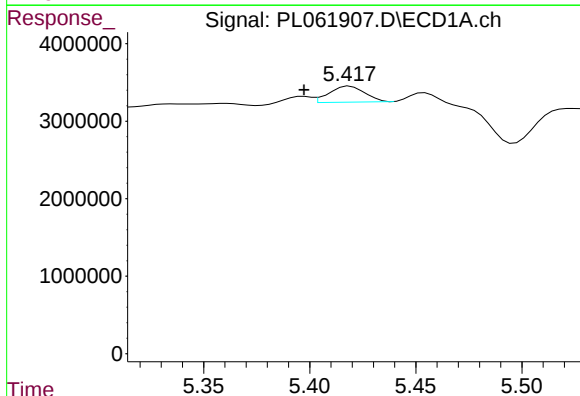


#25 Chlordane-3

R.T.: 5.419 min
Delta R.T.: 0.022 min
Response: 2409718
Conc: 15.33 ng/ml

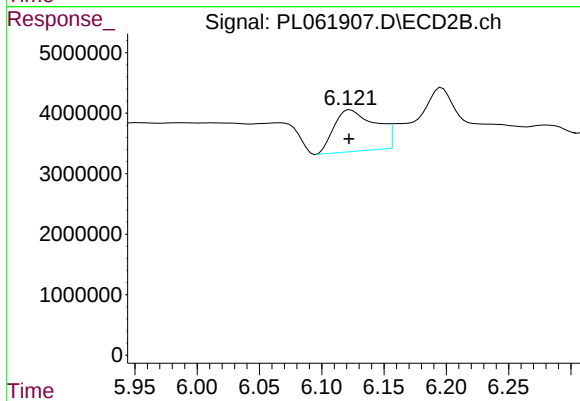

#25 Chlordane-3


R.T.: 6.123 min
Delta R.T.: 0.001 min
Response: 15959813
Conc: 43.55 ng/ml

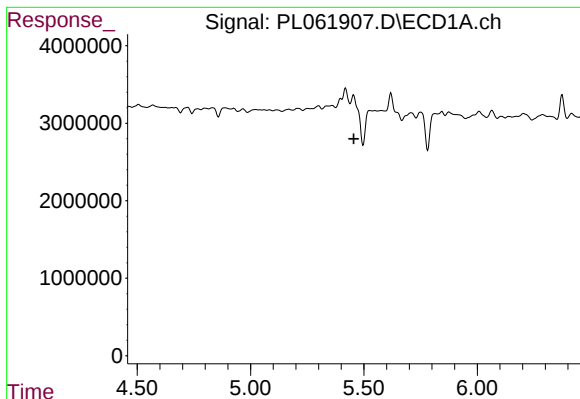

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

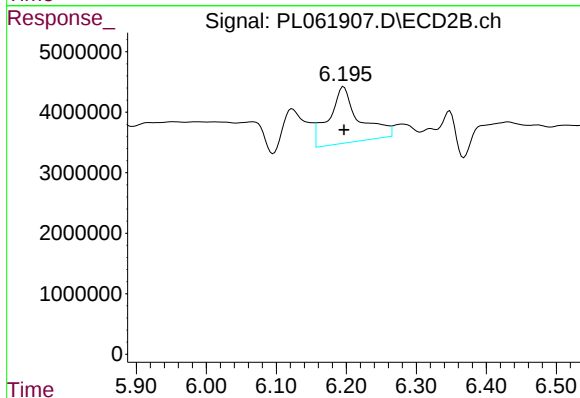


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 27871754
Conc: 62.09 ng/ml

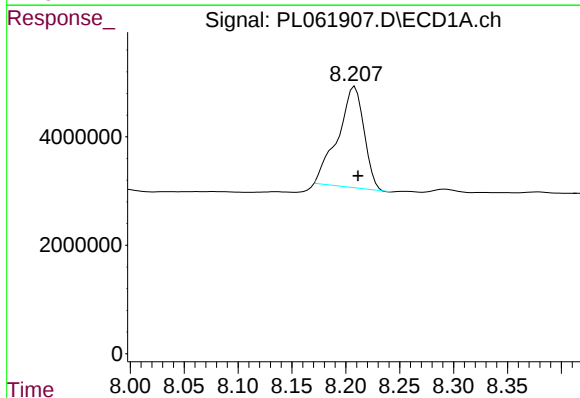

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.003 min
Response: 31416256
Conc: 19.31 ng/ml

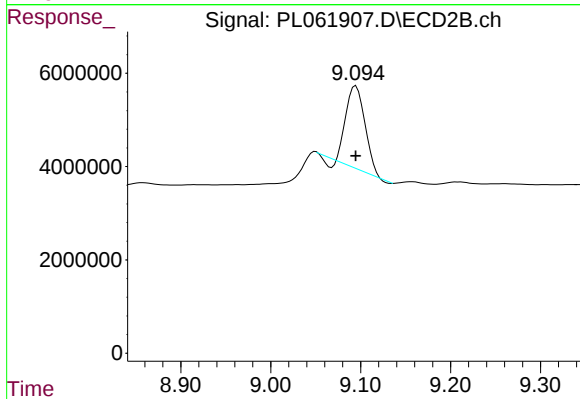

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 25215621
Conc: 11.45 ng/ml