

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
 Data File : PL061908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 16:55
 Operator : DD\AJ
 Sample : L4198-28
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 03:39:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	37167382	57572925	21.787	21.103
28)	SA Decachlor...	8.209	9.095	36733951	48005290	22.581	21.807
Target Compounds							
2)	A alpha-BHC	0.000	4.422f	0	3578229	N.D.	0.896 #
9)	A Endosulfan I	5.529f	0.000	11699024	0	7.220	N.D. #
10)	B gamma-Chl...	0.000	6.123	0	10742376	N.D.	3.658 #
11)	B alpha-Chl...	0.000	6.196	0	9624066	N.D.	3.204 #
12)	B 4,4'-DDE	5.619	6.348	2696186	5969182	1.715	2.187 #
17)	MA 4,4'-DDT	6.375	7.143	2822650	3674139	2.238	1.678 #
23)	Chlordane-1	4.327	0.000	2451134	0	49.502	N.D. #
25)	Chlordane-3	0.000	6.123	0	10742376	N.D.	29.316 #
26)	Chlordane-4	0.000	6.196	0	9624066	N.D.	21.438 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
Data File : PL061908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 16:55
Operator : DD\AJ
Sample : L4198-28
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 03:39:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

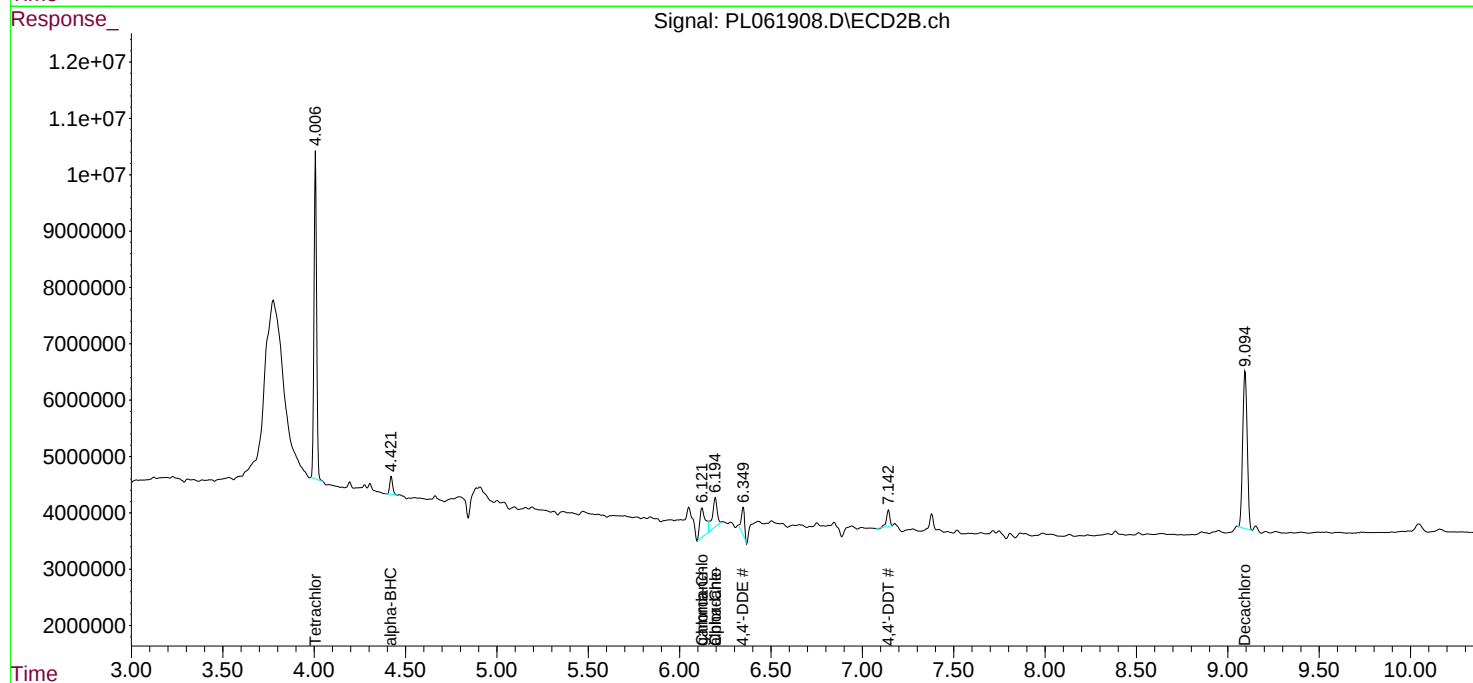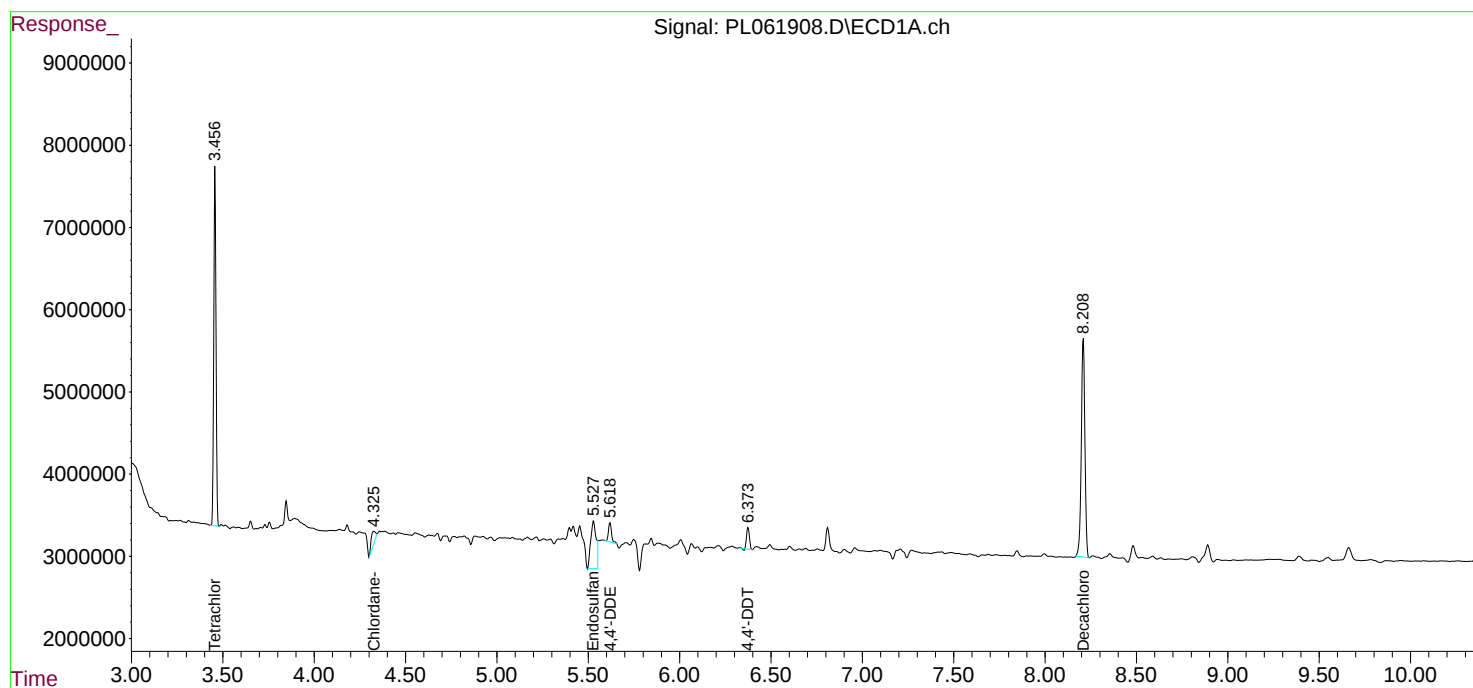


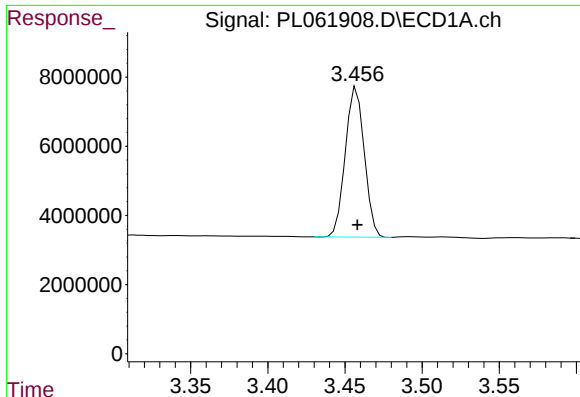

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 37167382
Conc: 21.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

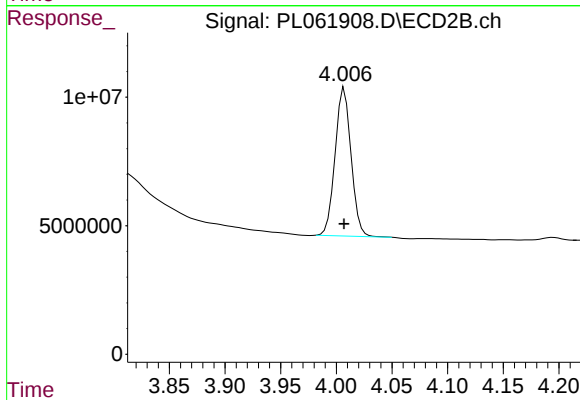


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 57572925
Conc: 21.10 ng/ml

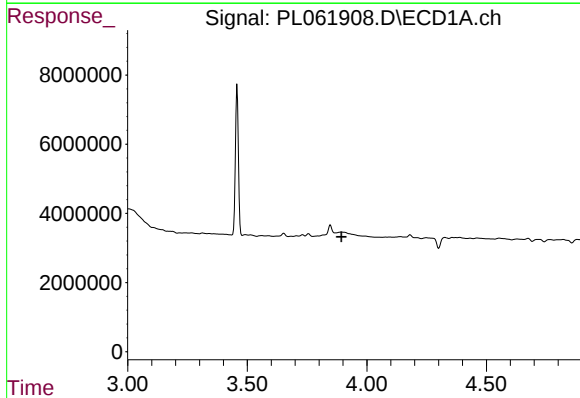


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.894 min
Response: 0
Conc: N.D.

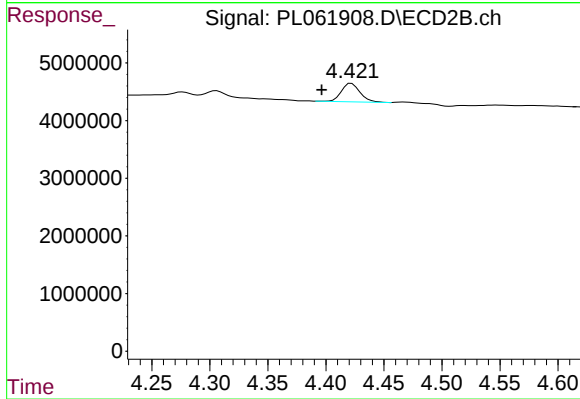

#2 alpha-BHC


R.T.: 4.422 min
Delta R.T.: 0.026 min
Response: 3578229
Conc: 0.90 ng/ml

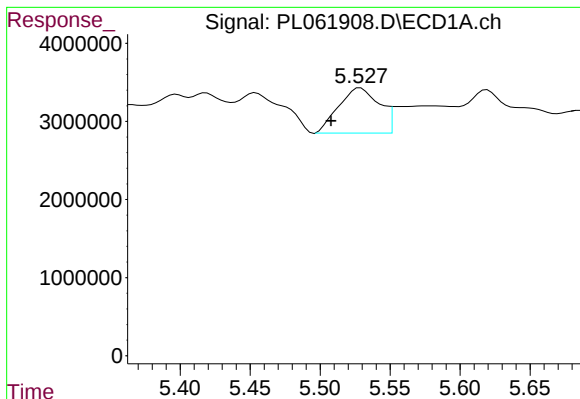

#9 Endosulfan I


R.T.: 5.529 min
Delta R.T.: 0.021 min
Response: 11699024
Conc: 7.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

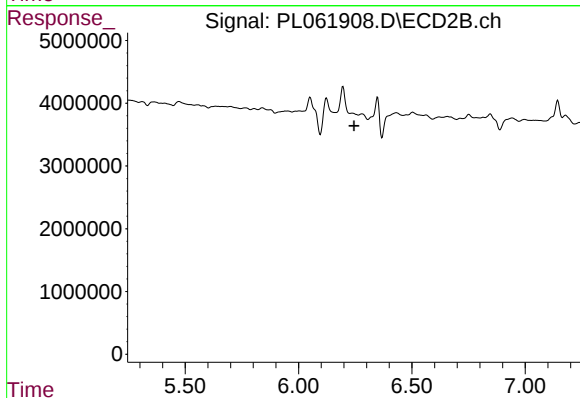


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

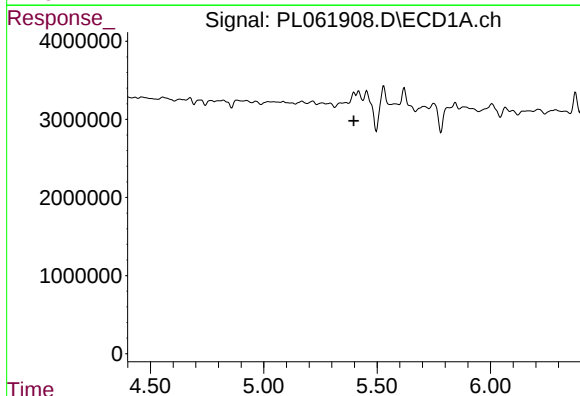


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

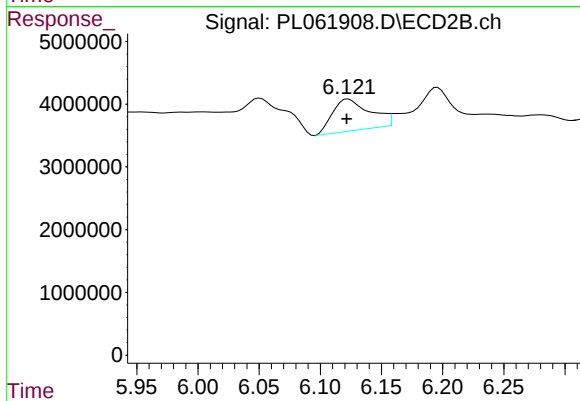

#10 gamma-Chlordane


R.T.: 6.123 min
Delta R.T.: 0.001 min
Response: 10742376
Conc: 3.66 ng/ml

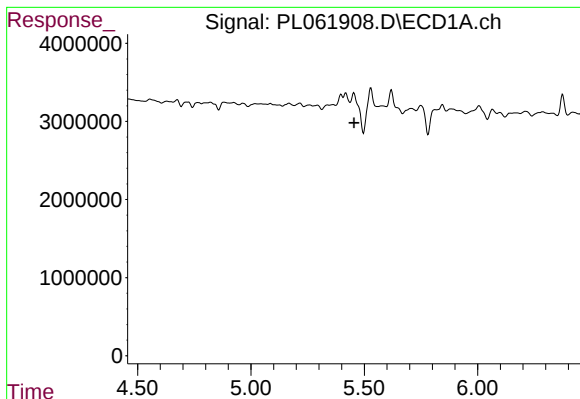

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

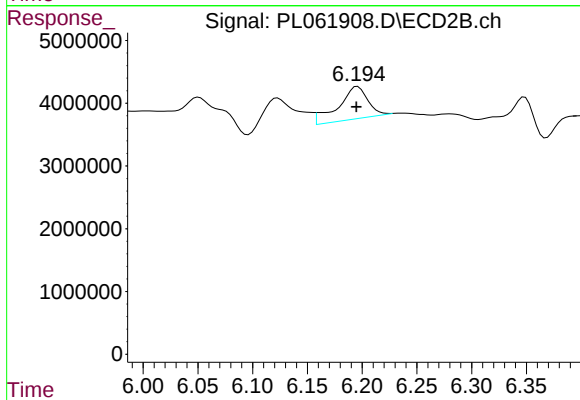


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: 0.001 min
Response: 9624066
Conc: 3.20 ng/ml

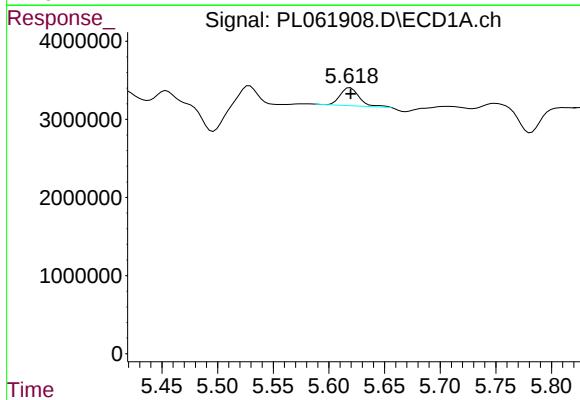


#12 4,4'-DDE

R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 2696186
Conc: 1.72 ng/ml

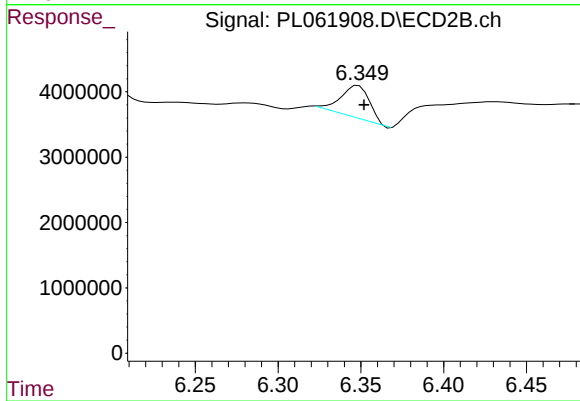

#12 4,4'-DDE


R.T.: 6.348 min
Delta R.T.: -0.004 min
Response: 5969182
Conc: 2.19 ng/ml

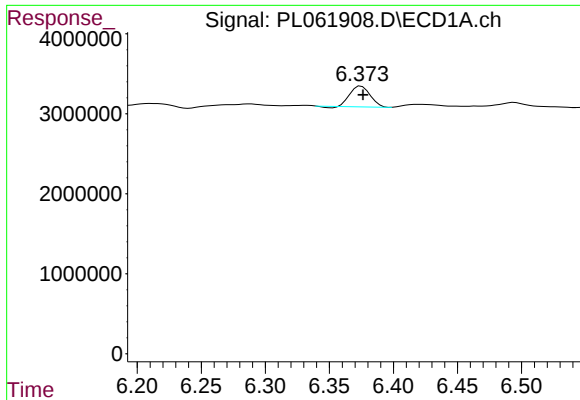

#17 4,4'-DDT


R.T.: 6.375 min
Delta R.T.: -0.001 min
Response: 2822650
Conc: 2.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

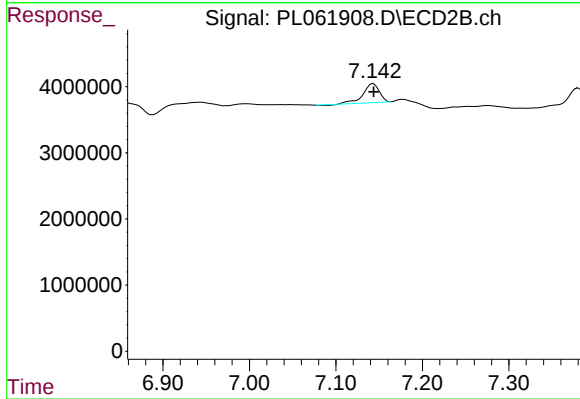


#17 4,4'-DDT

R.T.: 7.143 min
Delta R.T.: 0.000 min
Response: 3674139
Conc: 1.68 ng/ml

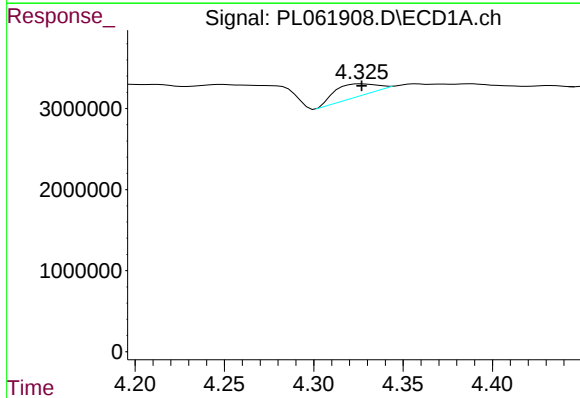


#23 Chlordane-1

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 2451134
Conc: 49.50 ng/ml

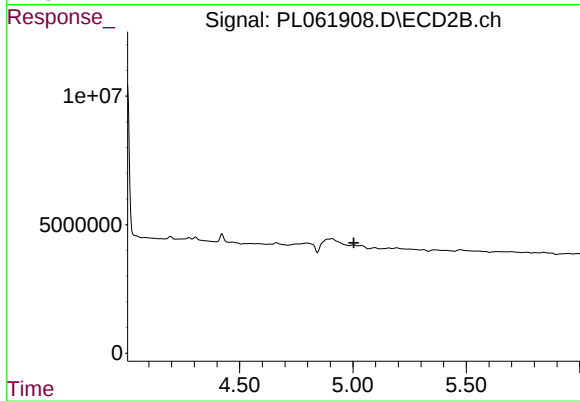

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.004 min
Response: 0
Conc: N.D.

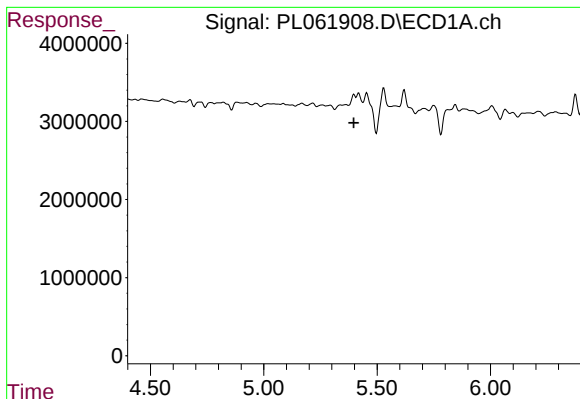

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

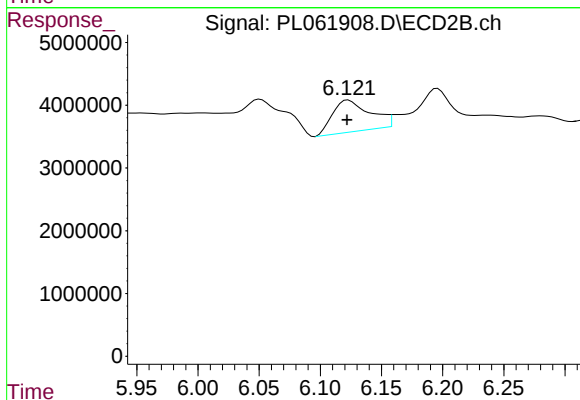


#25 Chlordane-3

R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 10742376
Conc: 29.32 ng/ml

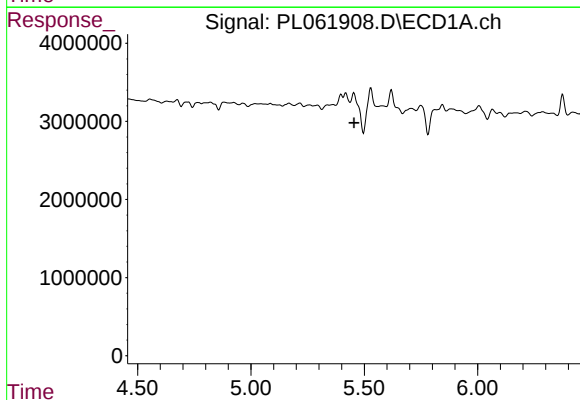


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

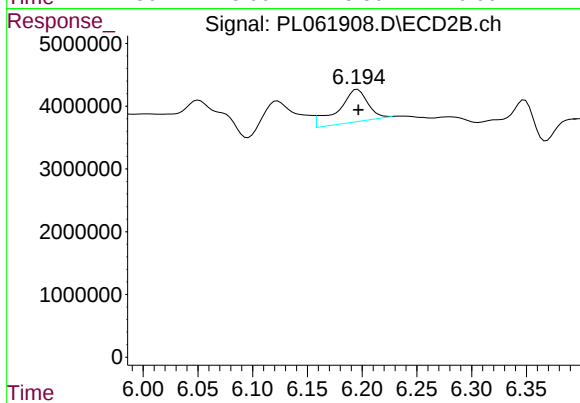

#26 Chlordane-4


R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 9624066
Conc: 21.44 ng/ml

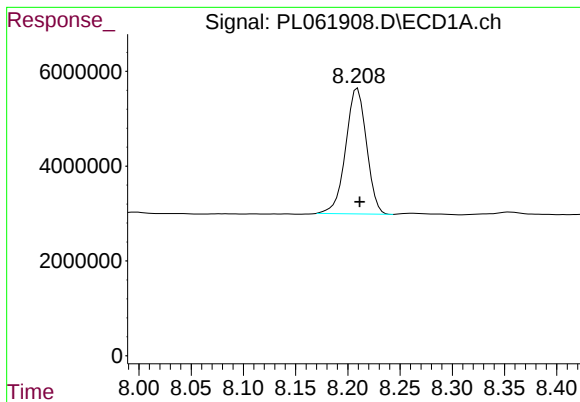

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 36733951
Conc: 22.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

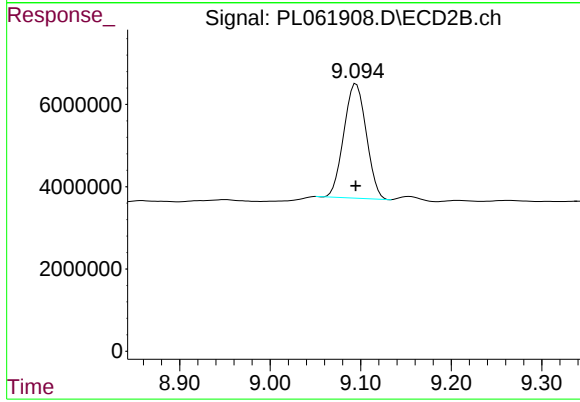

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 48005290
Conc: 21.81 ng/ml