

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
 Data File : PL061910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 17:23
 Operator : DD\AJ
 Sample : L4199-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 03:40:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	37495750	58000750	21.979	21.259
28)	SA Decachlor...	8.209	9.094	33695639	44044525	20.713	20.008
Target Compounds							
2)	A alpha-BHC	0.000	4.423f	0	5056638	N.D.	1.266 #
9)	A Endosulfan I	5.529f	0.000	10504345	0	6.482	N.D. #
10)	B gamma-Chl...	5.419f	6.122	9833179	13710415	5.662	4.669
11)	B alpha-Chl...	0.000	6.196	0	18396237	N.D.	6.125 #
13)	MA Dieldrin	5.750	0.000	6304420	0	3.748	N.D. #
15)	B Endosulfa...	0.000	6.948f	0	6296103	N.D.	2.436 #
17)	MA 4,4'-DDT	6.374	0.000	2286785	0	1.813	N.D. #
23)	Chlordane-1	4.326	0.000	2257537	0	45.592	N.D. #
25)	Chlordane-3	5.419f	6.122	9833179	13710415	62.559	37.415 #
26)	Chlordane-4	0.000	6.196	0	18396237	N.D.	40.979 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
Data File : PL061910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 17:23
Operator : DD\AJ
Sample : L4199-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 03:40:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

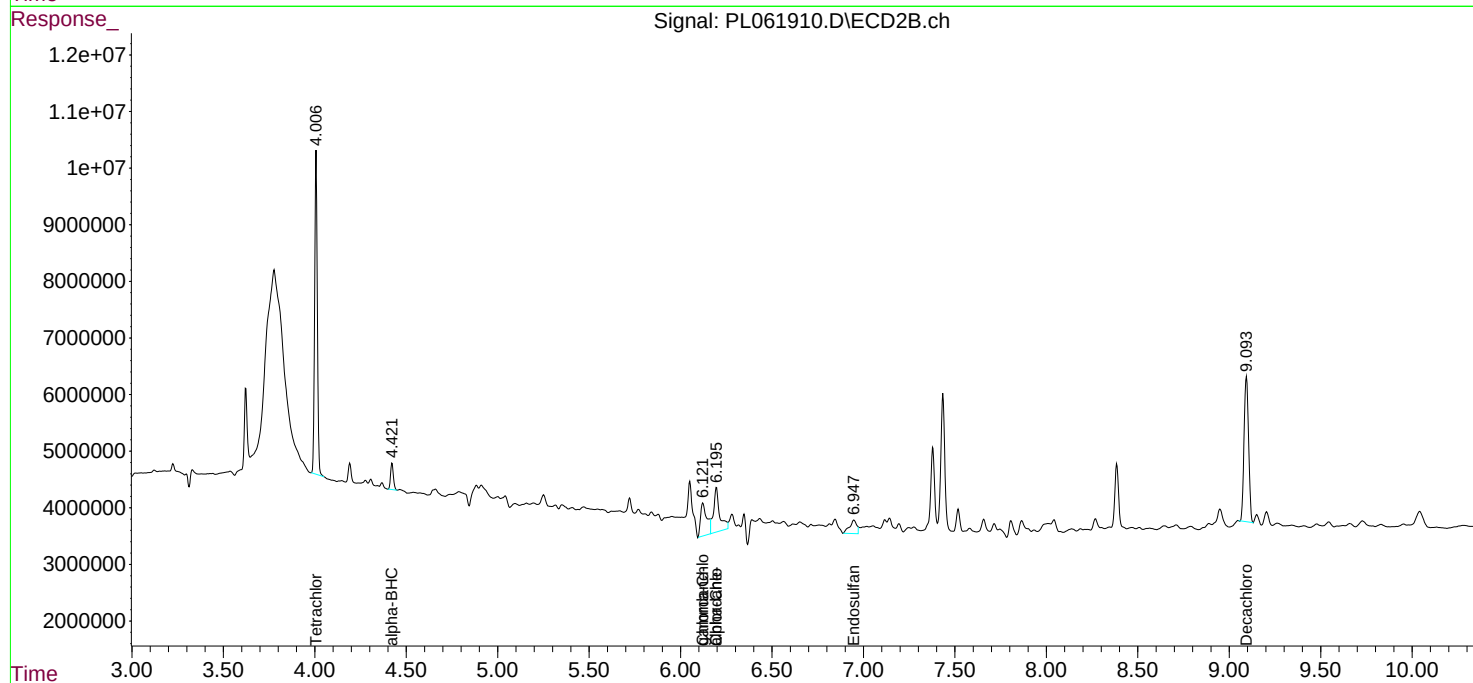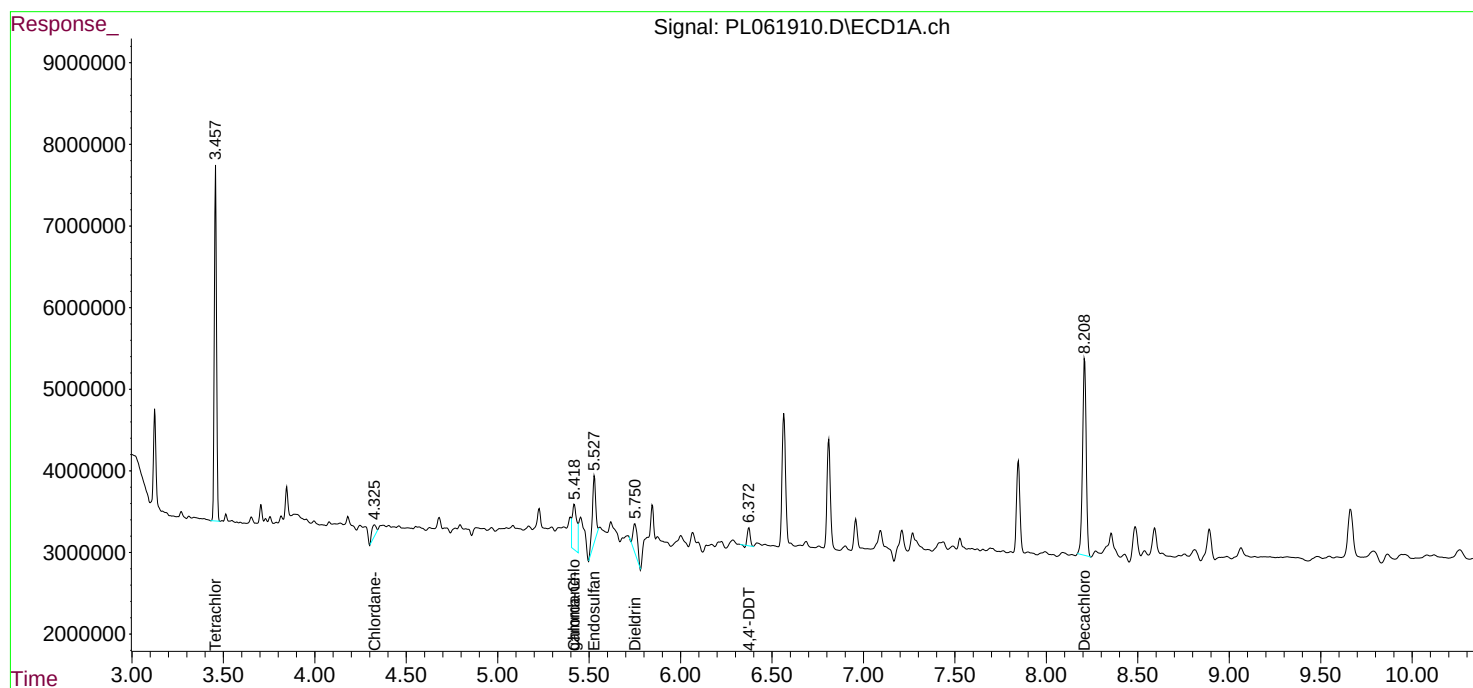


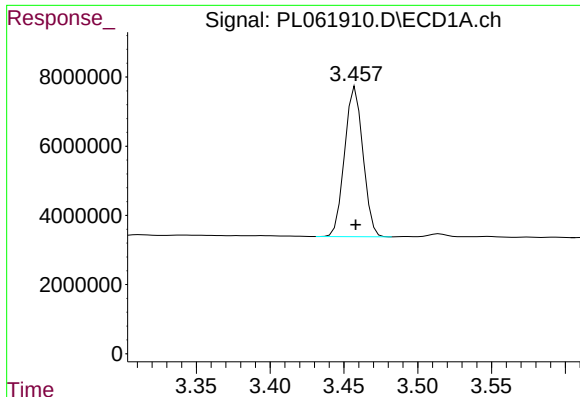

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 37495750
Conc: 21.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

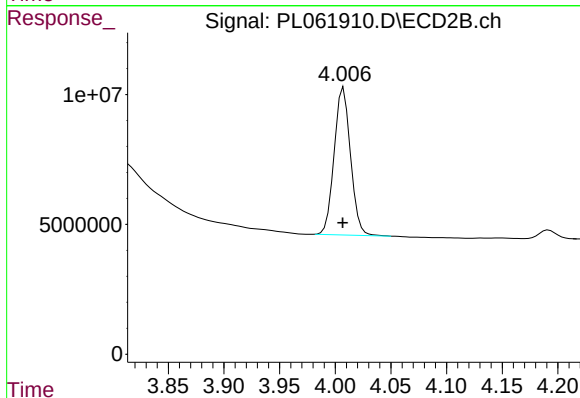


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 58000750
Conc: 21.26 ng/ml

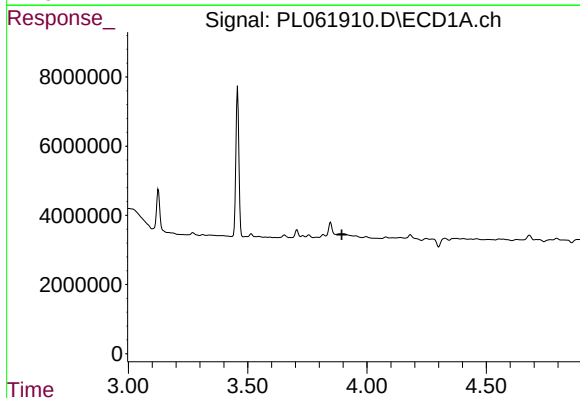


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.894 min
Response: 0
Conc: N.D.

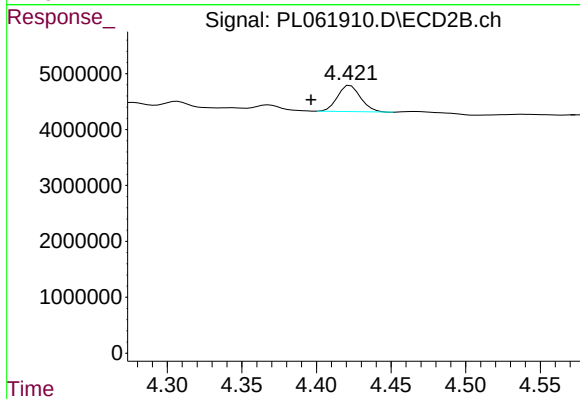

#2 alpha-BHC


R.T.: 4.423 min
Delta R.T.: 0.026 min
Response: 5056638
Conc: 1.27 ng/ml

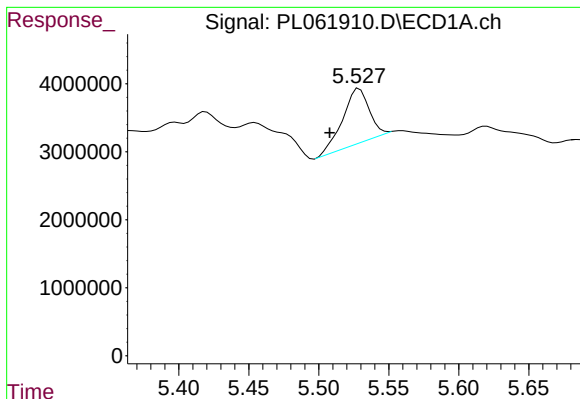

#9 Endosulfan I


R.T.: 5.529 min
Delta R.T.: 0.021 min
Response: 10504345
Conc: 6.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

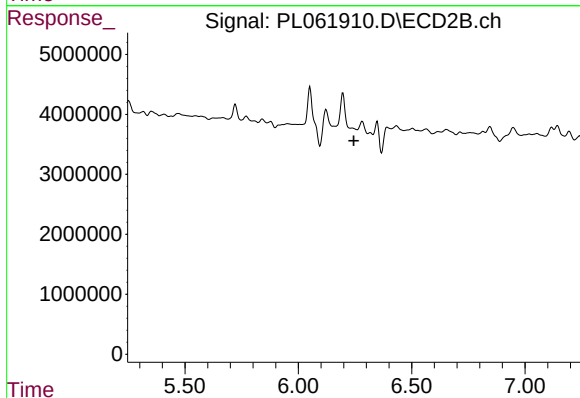


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

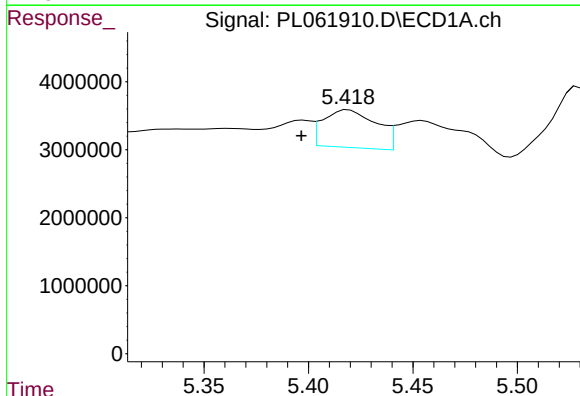


#10 gamma-Chlordane

R.T.: 5.419 min
Delta R.T.: 0.023 min
Response: 9833179
Conc: 5.66 ng/ml

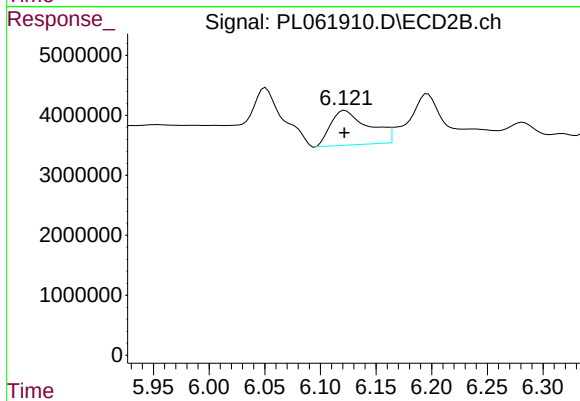

#10 gamma-Chlordane


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 13710415
Conc: 4.67 ng/ml

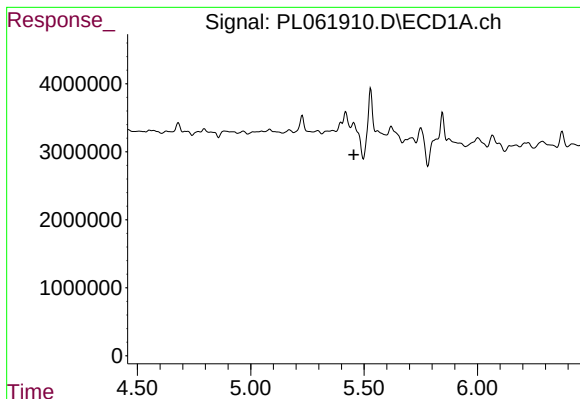

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

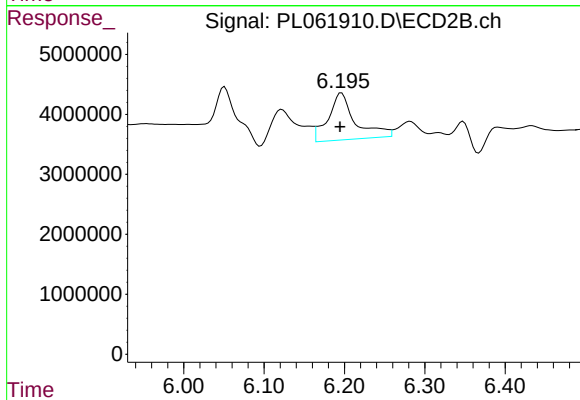


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: 0.002 min
Response: 18396237
Conc: 6.12 ng/ml

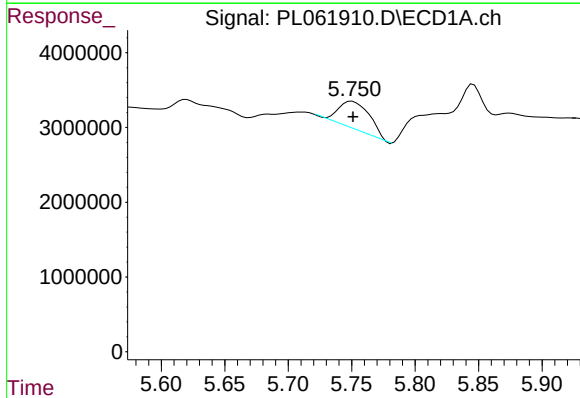


#13 Dieldrin

R.T.: 5.750 min
Delta R.T.: 0.000 min
Response: 6304420
Conc: 3.75 ng/ml

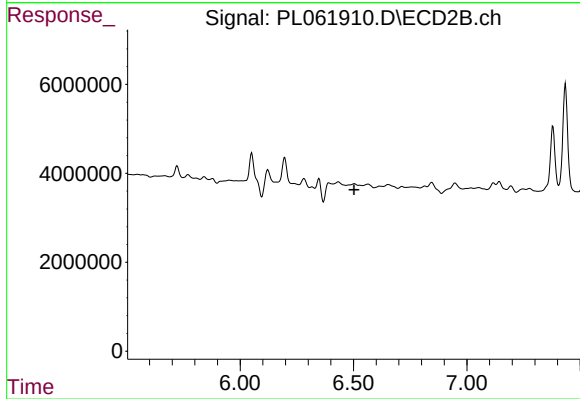

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.502 min
Response: 0
Conc: N.D.

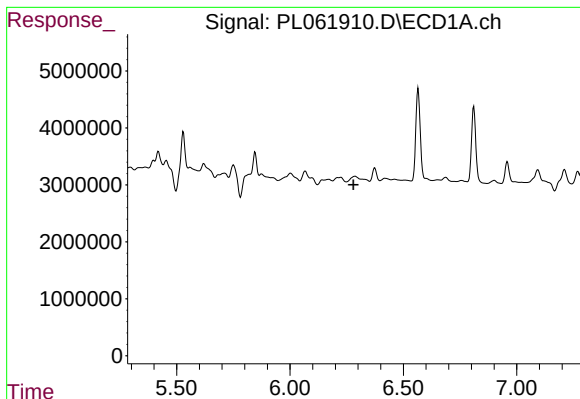

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

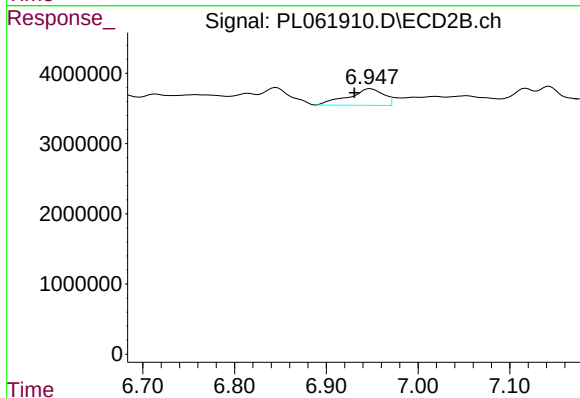


#15 Endosulfan II

R.T.: 6.948 min
Delta R.T.: 0.017 min
Response: 6296103
Conc: 2.44 ng/ml

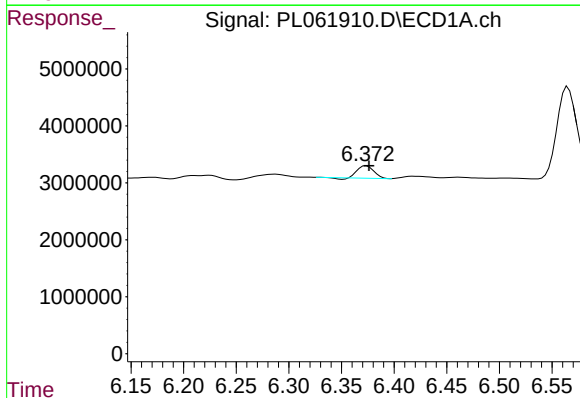


#17 4,4'-DDT

R.T.: 6.374 min
Delta R.T.: -0.003 min
Response: 2286785
Conc: 1.81 ng/ml

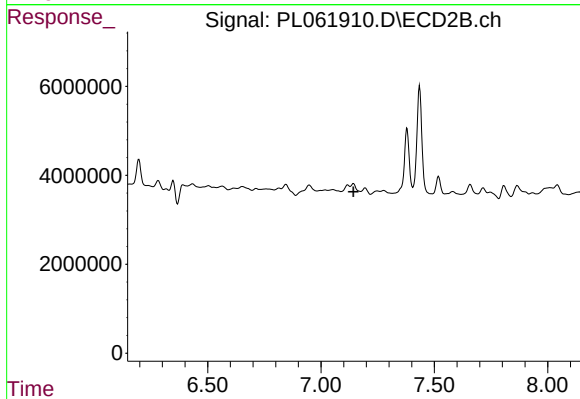

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.144 min
Response: 0
Conc: N.D.

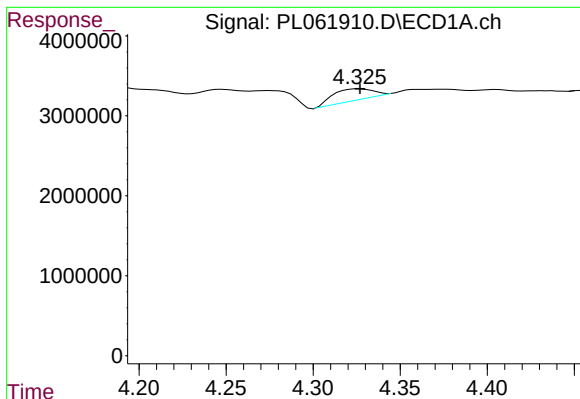

#23 Chlordane-1


R.T.: 4.326 min
Delta R.T.: 0.000 min
Response: 2257537
Conc: 45.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

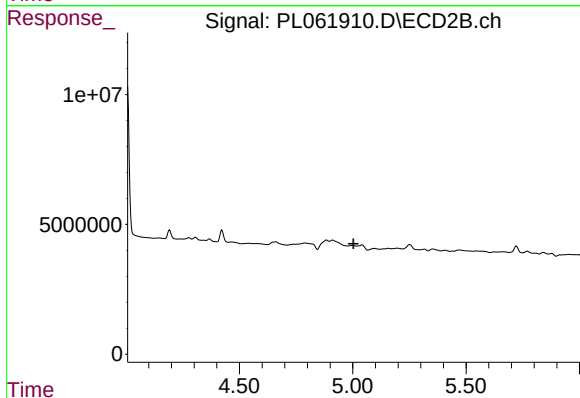


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

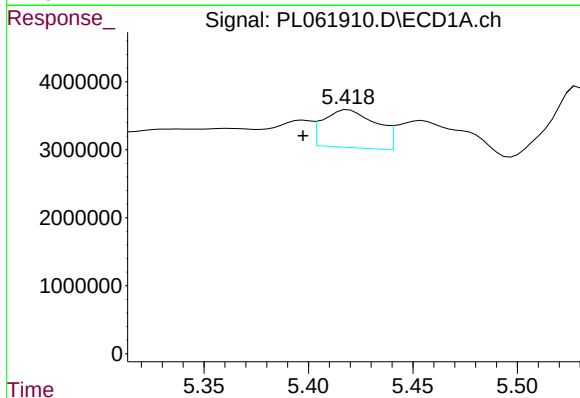


#25 Chlordane-3

R.T.: 5.419 min
Delta R.T.: 0.022 min
Response: 9833179
Conc: 62.56 ng/ml

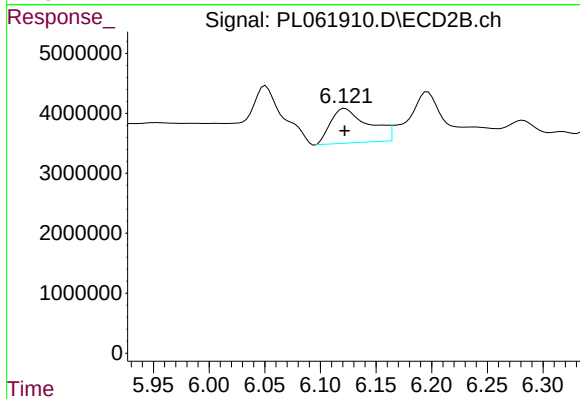

#25 Chlordane-3


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 13710415
Conc: 37.42 ng/ml

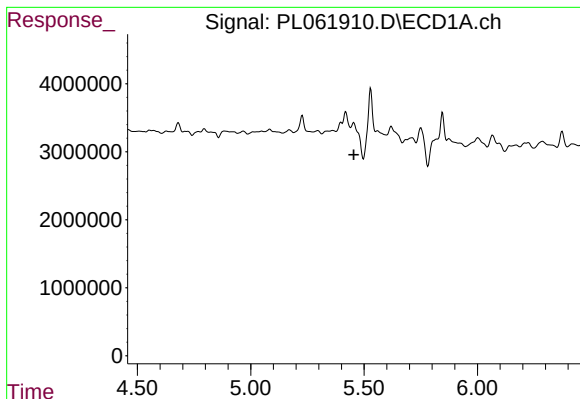

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

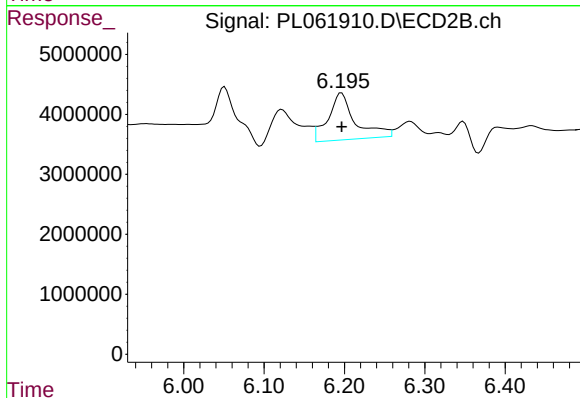


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 18396237
Conc: 40.98 ng/ml

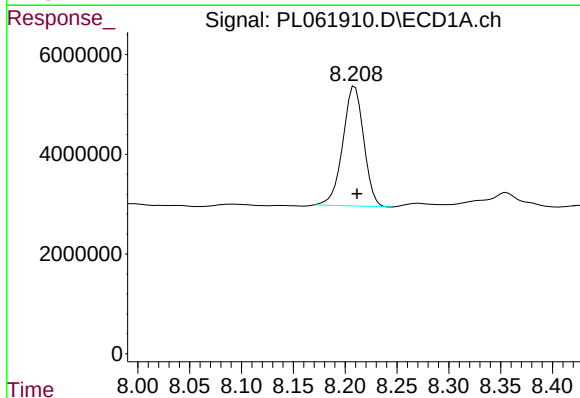

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 33695639
Conc: 20.71 ng/ml

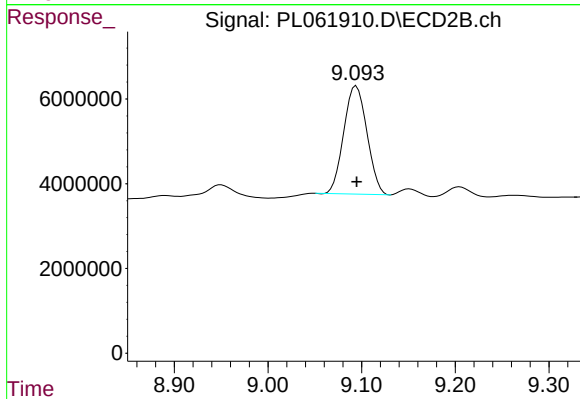

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 44044525
Conc: 20.01 ng/ml