

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
 Data File : PL061894.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 13:37
 Operator : DD\AJ
 Sample : L4176-01MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AC-4MS

Manual Integrations
 APPROVED

Ankita
 10/2/2020 2:59:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 16:08:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	42706442	63695674	25.033	23.347
28)	SA Decachlor...	8.209	9.094	38693305	51038171	23.786	23.185
Target Compounds							
2)	A alpha-BHC	3.894	4.396	145.3E6	227.6E6	59.612	56.987
3)	MA gamma-BHC...	4.177	4.682	131.7E6	207.6E6	60.215	56.066
4)	MA Heptachlor	4.478	5.192	120.8E6	198.0E6	59.199	57.178
5)	MB Aldrin	4.726	5.499	108.7E6	183.3E6	60.221	56.573
6)	B beta-BHC	4.428	4.853	53942526	84975868	59.062	56.277
7)	B delta-BHC	4.631	5.071	120.2E6	147.2E6	58.642	57.754
8)	B Heptachlo...	5.168	5.886	103.7E6	151.8E6	59.420	61.252
9)	A Endosulfan I	5.507	6.245	94675605	152.5E6	58.426	55.214
10)	B gamma-Chl...	5.396	6.121	117.6E6	175.7E6	67.702	59.838
11)	B alpha-Chl...	5.453	6.195	107.4E6	192.7E6	61.818	64.160
12)	B 4,4'-DDE	5.619	6.353	367.4E6	586.0E6	233.764	214.654
13)	MA Dieldrin	5.749	6.502	150.8E6	239.2E6	89.650	84.308
14)	MA Endrin	6.007	6.719	103.5E6	135.8E6	65.017	55.657m
15)	B Endosulfa...	6.280	6.930	93486926	134.6E6	57.821	52.064
16)	A 4,4'-DDD	6.134	6.843	83190442	135.1E6	62.831	60.765
17)	MA 4,4'-DDT	6.375	7.143	203.7E6	300.0E6	161.483	136.980
18)	B Endrin al...	6.447	7.054	87040562	117.2E6	61.898	54.755
19)	B Endosulfa...	6.661	7.279	85134441	119.9E6	55.030	51.190
20)	A Methoxychlor	6.921	7.603	46801283	63135133	57.885	50.108
21)	B Endrin ke...	7.150	7.751	101.5E6	131.6E6	59.371	56.061
22)	Mirex	7.340	8.206	73959250	87605753	52.756	49.721

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
Data File : PL061894.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 13:37
Operator : DD\AJ
Sample : L4176-01MS
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 16:08:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

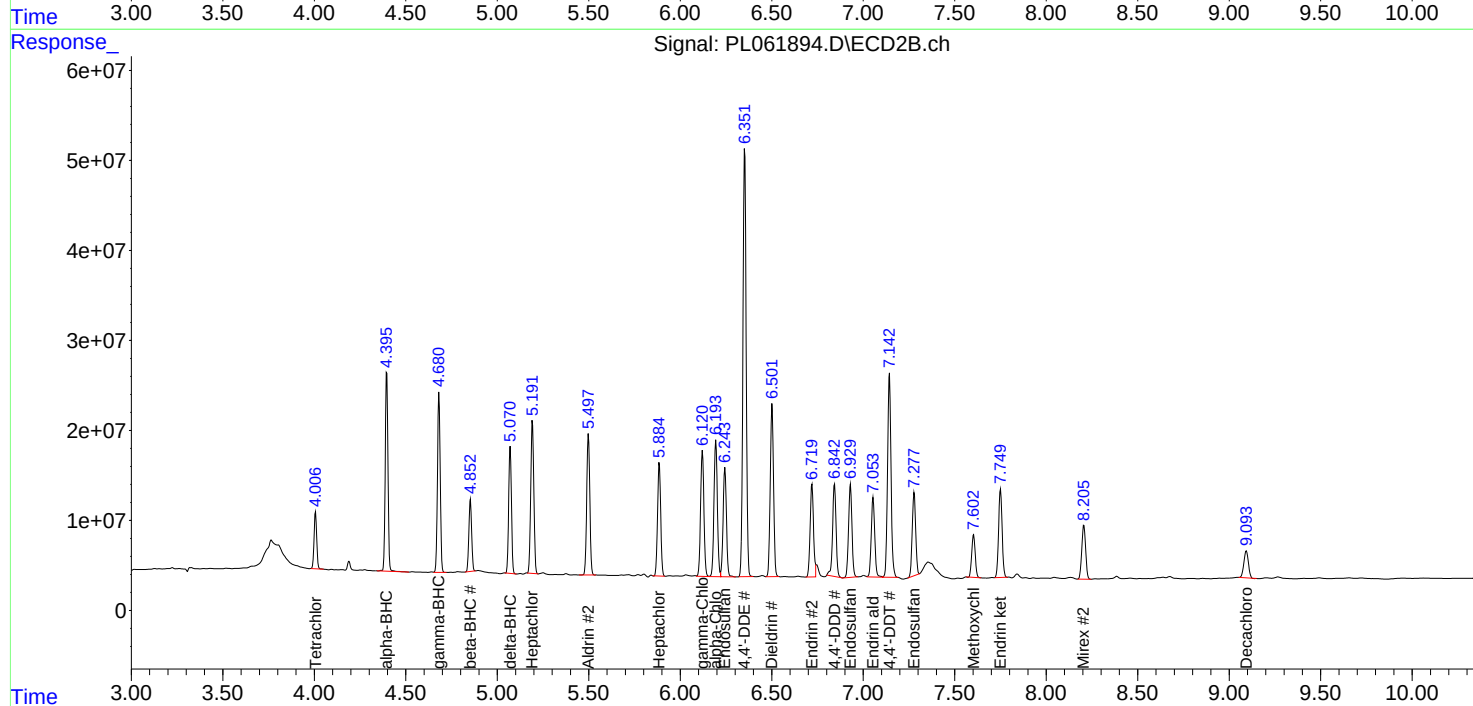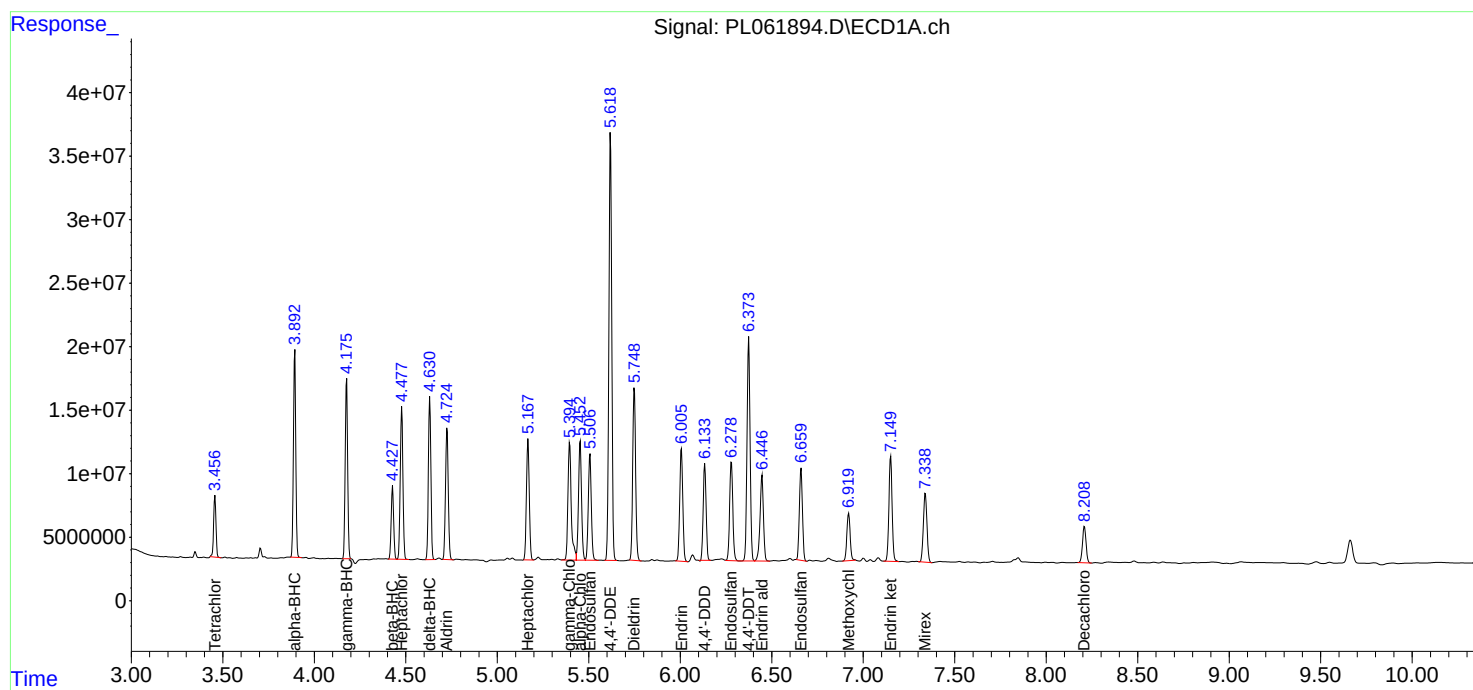

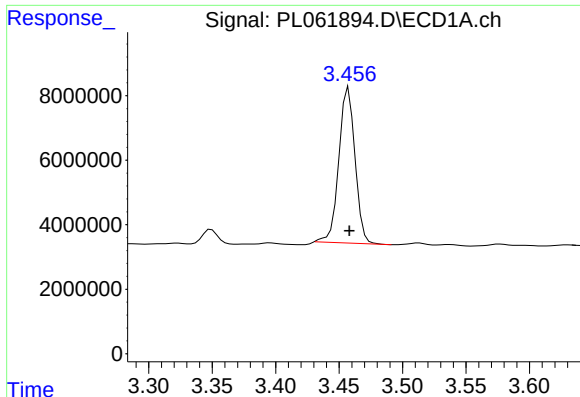


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 42706442
Conc: 25.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

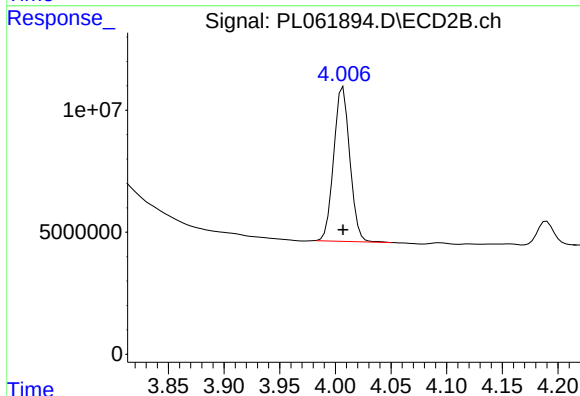


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 63695674
Conc: 23.35 ng/ml

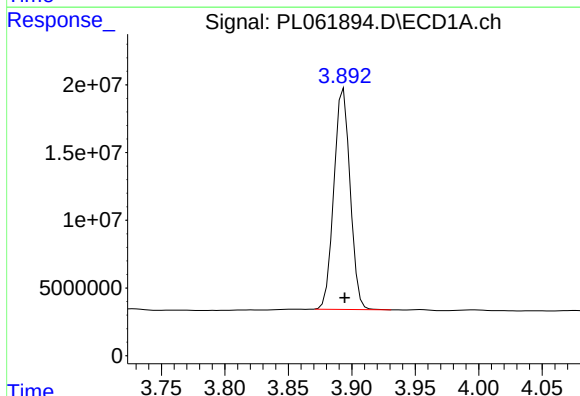


#2 alpha-BHC

R.T.: 3.894 min
Delta R.T.: 0.000 min
Response: 145299557
Conc: 59.61 ng/ml

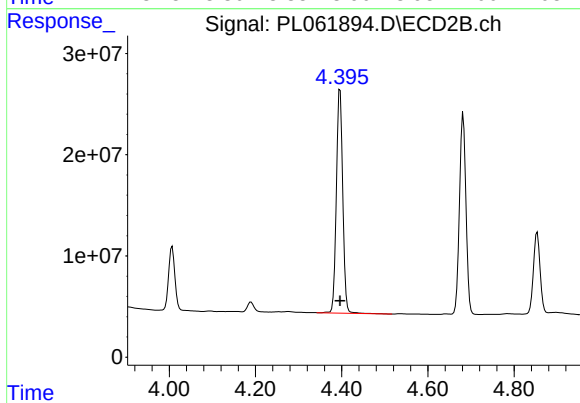

#2 alpha-BHC

R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 227621855
Conc: 56.99 ng/ml

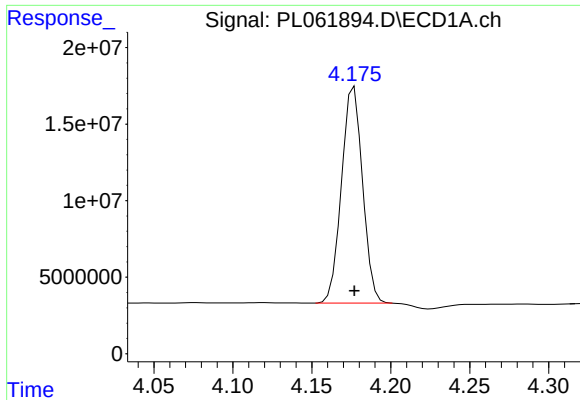


#3 gamma-BHC (Lindane)

R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 131703709
Conc: 60.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

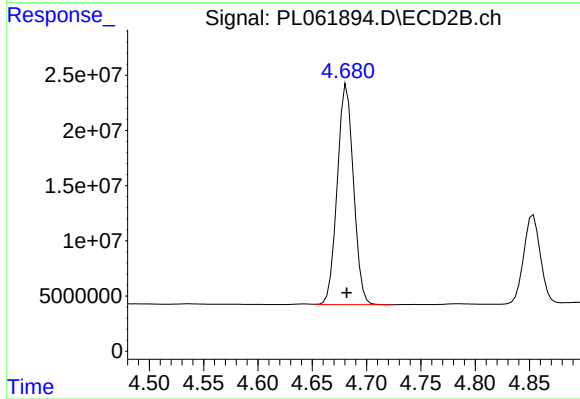


#3 gamma-BHC (Lindane)

R.T.: 4.682 min
Delta R.T.: 0.000 min
Response: 207550956
Conc: 56.07 ng/ml

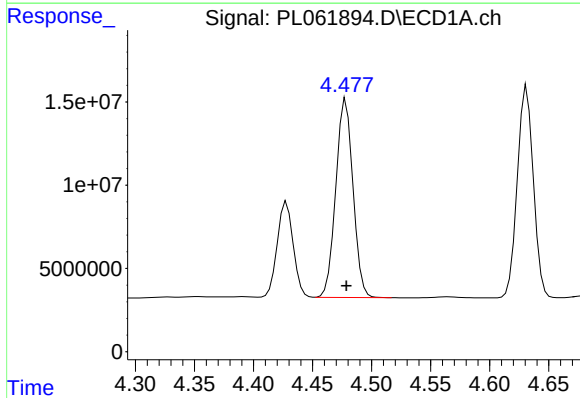


#4 Heptachlor

R.T.: 4.478 min
Delta R.T.: 0.000 min
Response: 120805483
Conc: 59.20 ng/ml

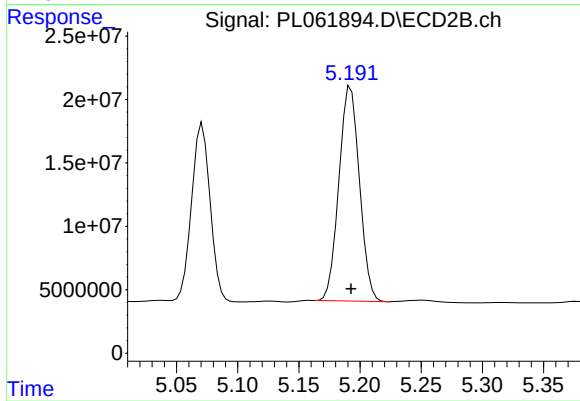

#4 Heptachlor

R.T.: 5.192 min
Delta R.T.: 0.000 min
Response: 198001608
Conc: 57.18 ng/ml

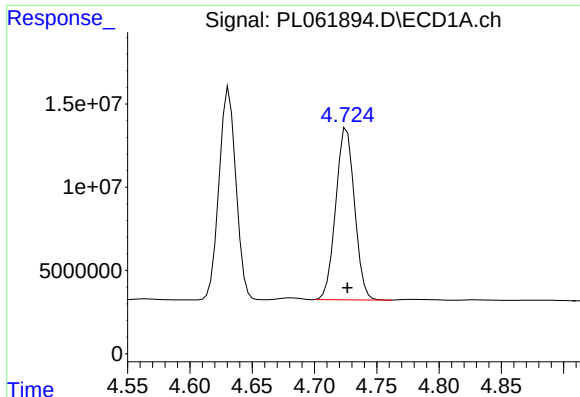


#5 Aldrin

R.T.: 4.726 min
Delta R.T.: 0.000 min
Response: 108658027
Conc: 60.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

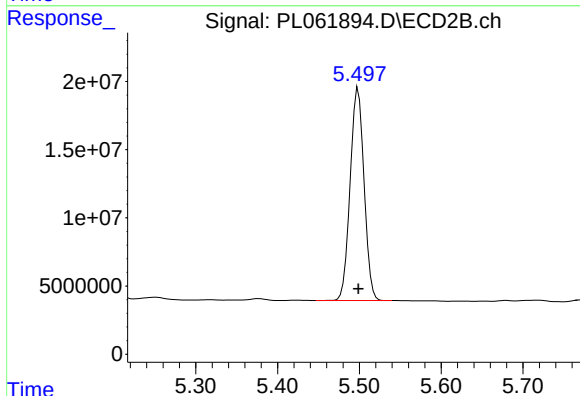


#5 Aldrin

R.T.: 5.499 min
Delta R.T.: 0.000 min
Response: 183266544
Conc: 56.57 ng/ml

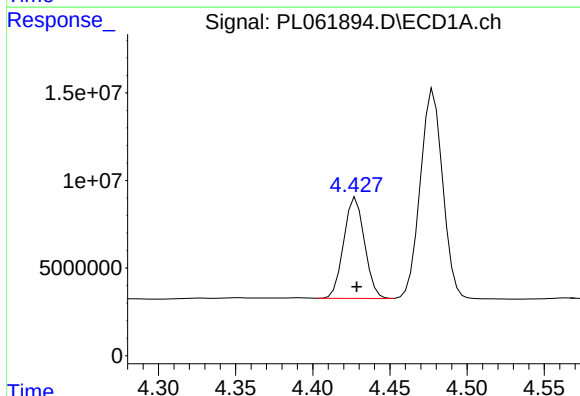


#6 beta-BHC

R.T.: 4.428 min
Delta R.T.: 0.000 min
Response: 53942526
Conc: 59.06 ng/ml

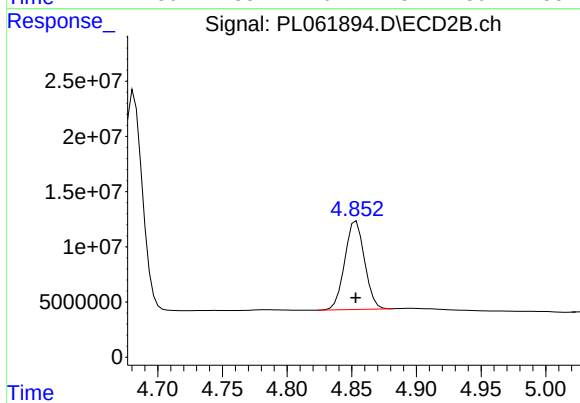

#6 beta-BHC

R.T.: 4.853 min
Delta R.T.: 0.000 min
Response: 84975868
Conc: 56.28 ng/ml

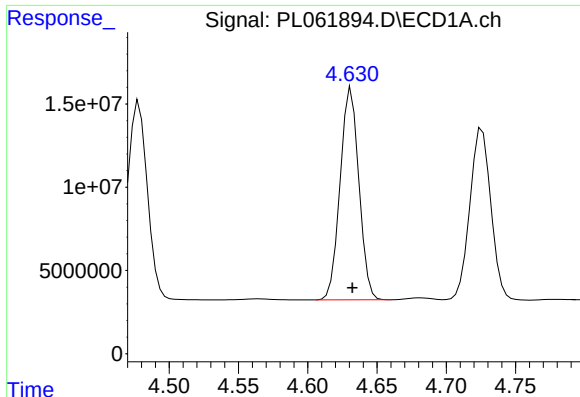


#7 delta-BHC

R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 120230062
Conc: 58.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

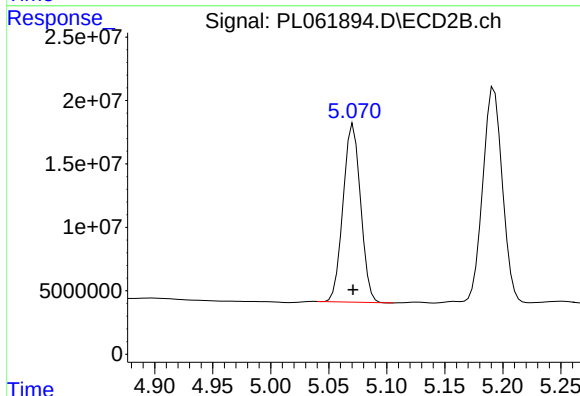


#7 delta-BHC

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 147162552
Conc: 57.75 ng/ml

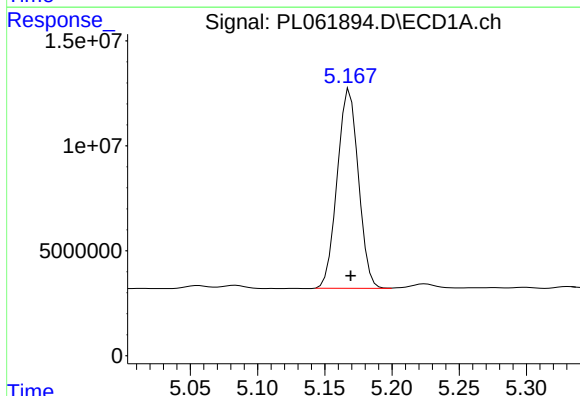


#8 Heptachlor epoxide

R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 103739702
Conc: 59.42 ng/ml

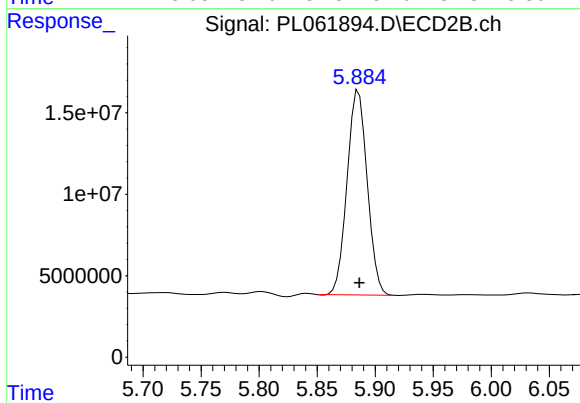

#8 Heptachlor epoxide

R.T.: 5.886 min
Delta R.T.: 0.000 min
Response: 151804613
Conc: 61.25 ng/ml

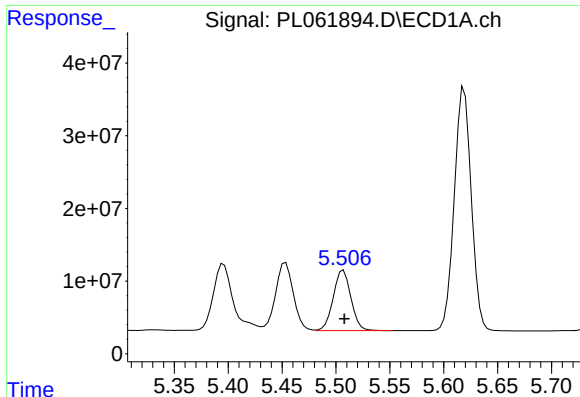


#9 Endosulfan I

R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 94675605
Conc: 58.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

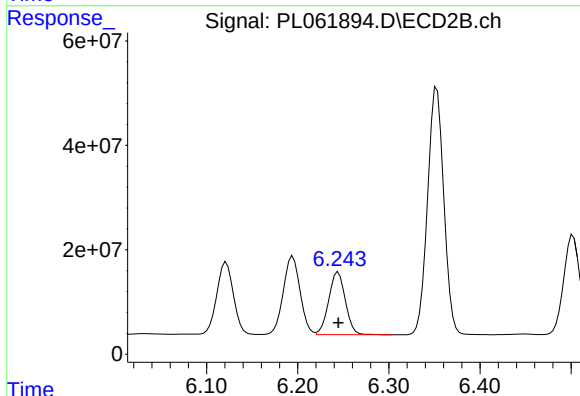


#9 Endosulfan I

R.T.: 6.245 min
Delta R.T.: 0.000 min
Response: 152528916
Conc: 55.21 ng/ml

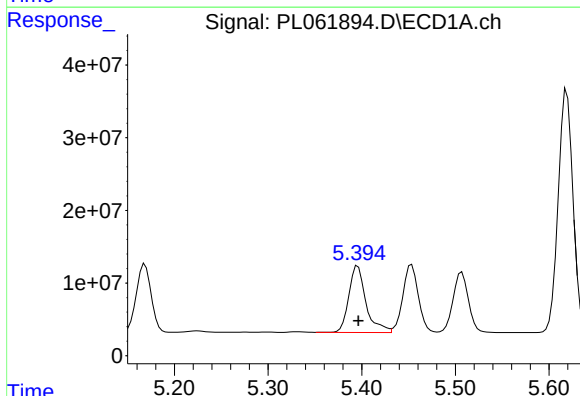


#10 gamma-Chlordane

R.T.: 5.396 min
Delta R.T.: 0.000 min
Response: 117575474
Conc: 67.70 ng/ml

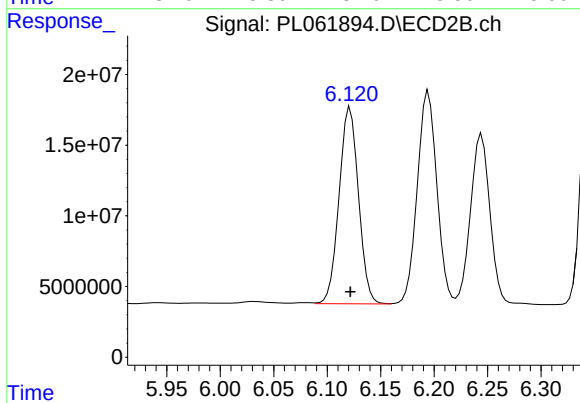

#10 gamma-Chlordane

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 175721884
Conc: 59.84 ng/ml

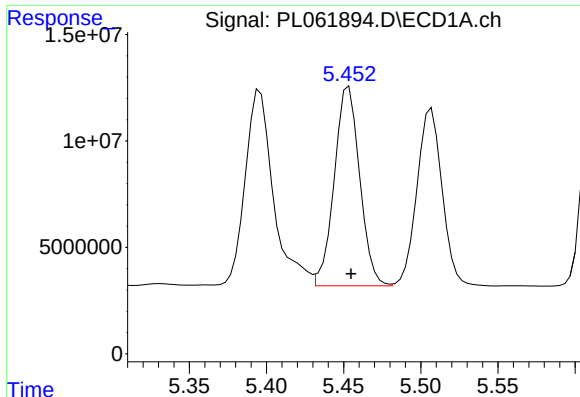


#11 alpha-Chlordane

R.T.: 5.453 min
Delta R.T.: -0.001 min
Response: 107381548
Conc: 61.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

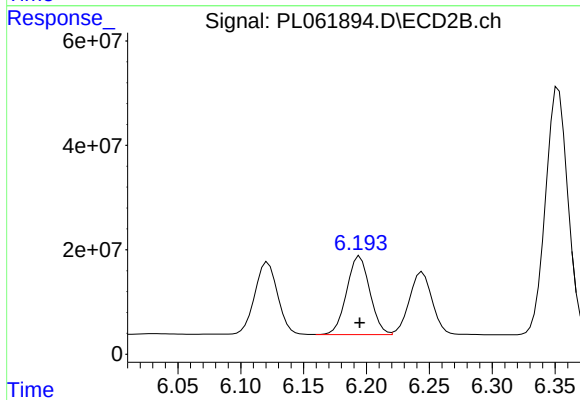


#11 alpha-Chlordane

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 192708081
Conc: 64.16 ng/ml

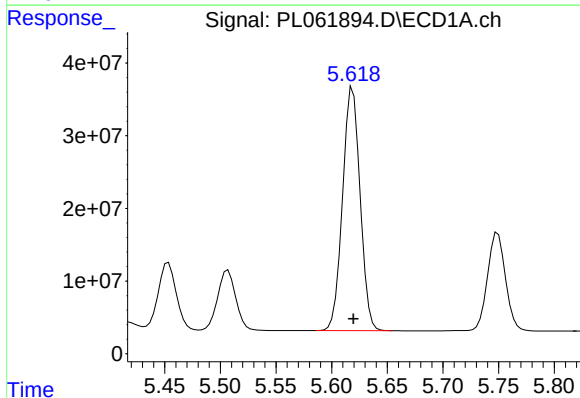


#12 4,4'-DDE

R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 367399234
Conc: 233.76 ng/ml

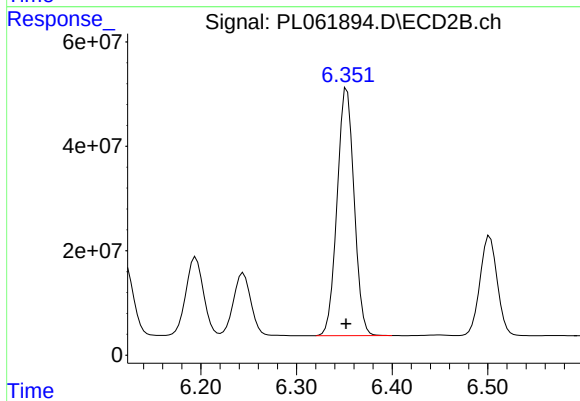

#12 4,4'-DDE

R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 585962820
Conc: 214.65 ng/ml

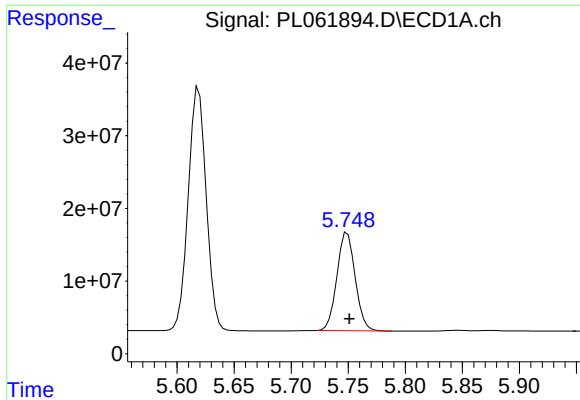


#13 Dieldrin

R.T.: 5.749 min
Delta R.T.: -0.002 min
Response: 150782292
Conc: 89.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

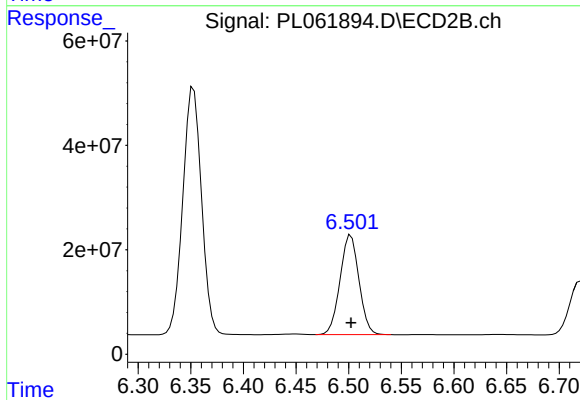


#13 Dieldrin

R.T.: 6.502 min
Delta R.T.: 0.000 min
Response: 239176637
Conc: 84.31 ng/ml

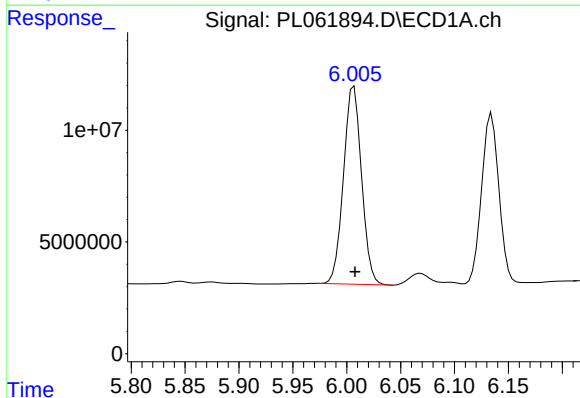


#14 Endrin

R.T.: 6.007 min
Delta R.T.: -0.001 min
Response: 103455339
Conc: 65.02 ng/ml

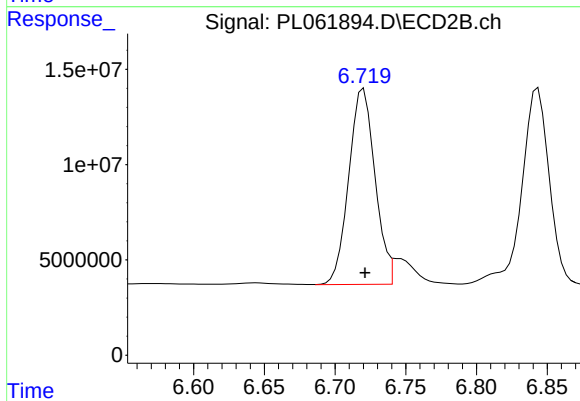

#14 Endrin

R.T.: 6.719 min
Delta R.T.: -0.002 min
Response: 135779810
Conc: 55.66 ng/ml m

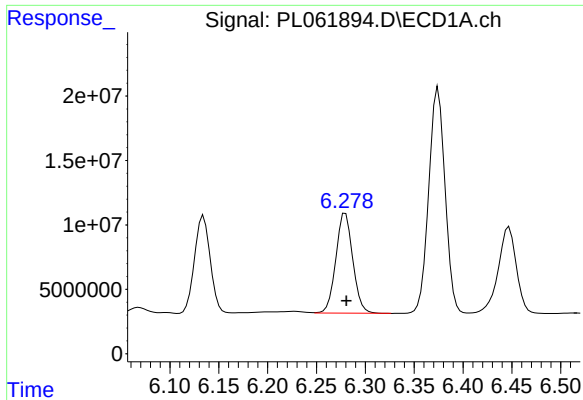


#15 Endosulfan II

R.T.: 6.280 min
Delta R.T.: -0.001 min
Response: 93486926
Conc: 57.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

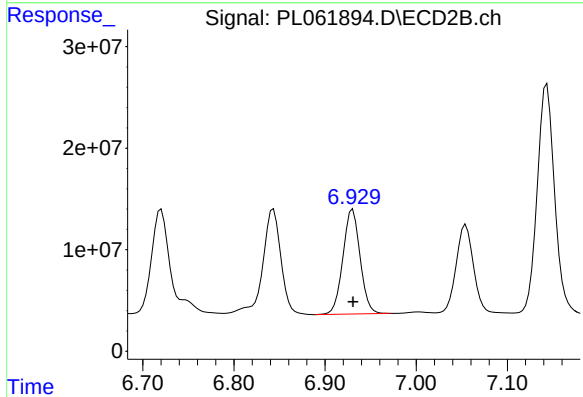


#15 Endosulfan II

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 134569471
Conc: 52.06 ng/ml

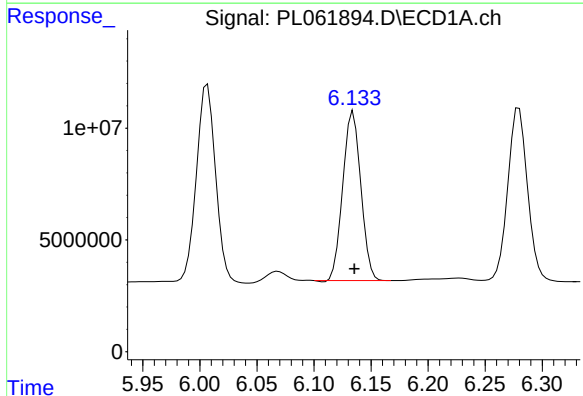


#16 4,4'-DDD

R.T.: 6.134 min
Delta R.T.: 0.000 min
Response: 83190442
Conc: 62.83 ng/ml

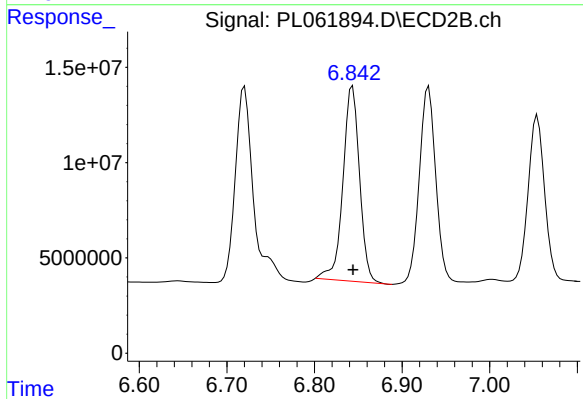

#16 4,4'-DDD

R.T.: 6.843 min
Delta R.T.: 0.000 min
Response: 135085175
Conc: 60.76 ng/ml

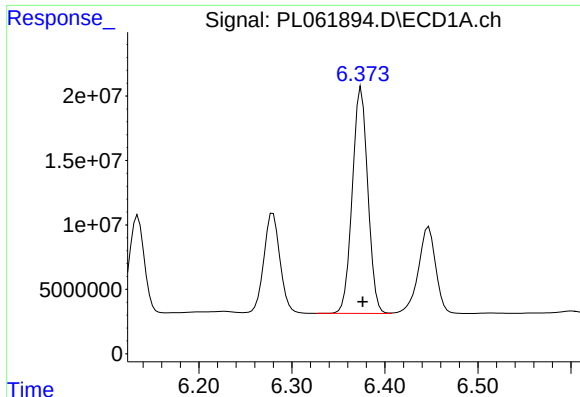


#17 4,4'-DDT

R.T.: 6.375 min
Delta R.T.: -0.002 min
Response: 203707881
Conc: 161.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

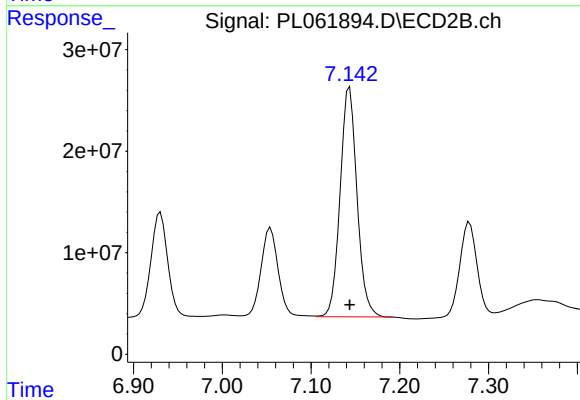


#17 4,4'-DDT

R.T.: 7.143 min
Delta R.T.: 0.000 min
Response: 299958596
Conc: 136.98 ng/ml

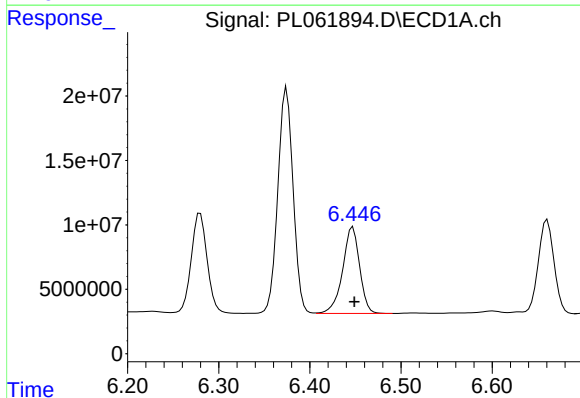


#18 Endrin aldehyde

R.T.: 6.447 min
Delta R.T.: -0.002 min
Response: 87040562
Conc: 61.90 ng/ml

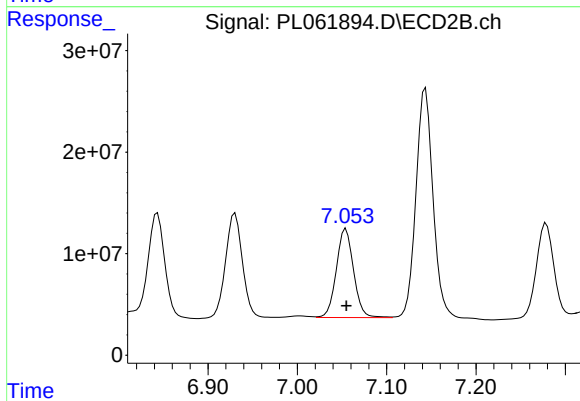

#18 Endrin aldehyde

R.T.: 7.054 min
Delta R.T.: 0.000 min
Response: 117200868
Conc: 54.76 ng/ml

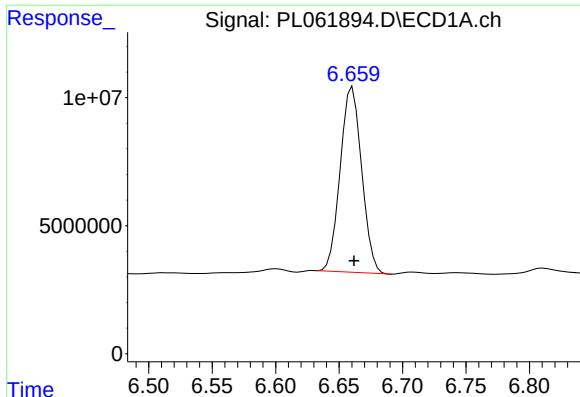


#19 Endosulfan Sulfate

R.T.: 6.661 min
Delta R.T.: -0.001 min
Response: 85134441
Conc: 55.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

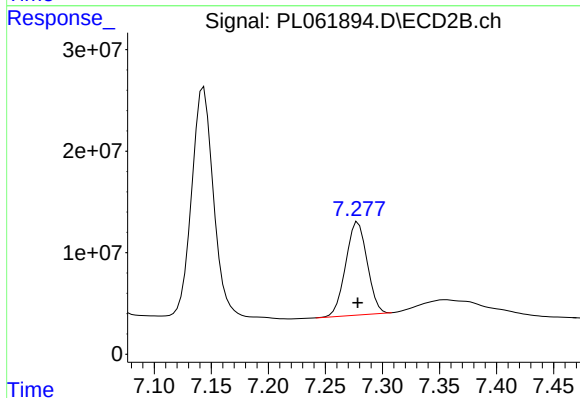


#19 Endosulfan Sulfate

R.T.: 7.279 min
Delta R.T.: 0.000 min
Response: 119865520
Conc: 51.19 ng/ml

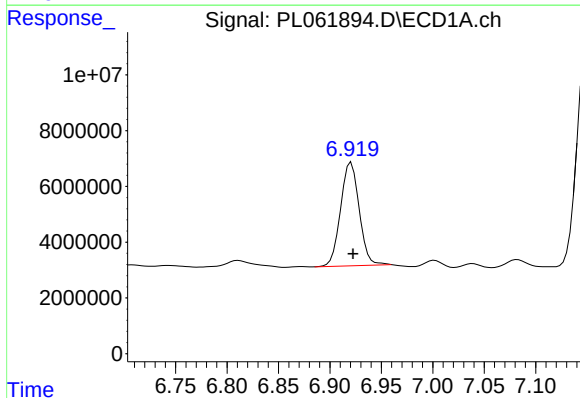


#20 Methoxychlor

R.T.: 6.921 min
Delta R.T.: -0.002 min
Response: 46801283
Conc: 57.89 ng/ml

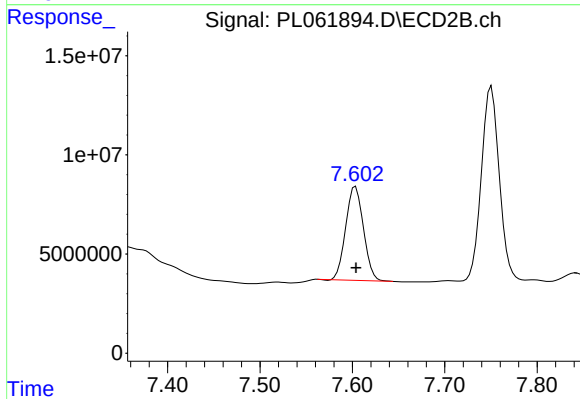

#20 Methoxychlor

R.T.: 7.603 min
Delta R.T.: 0.000 min
Response: 63135133
Conc: 50.11 ng/ml

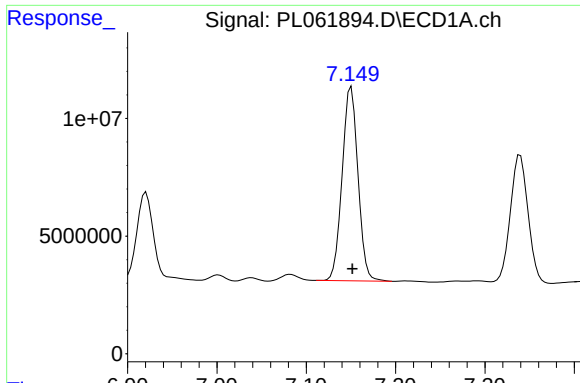


#21 Endrin ketone

R.T.: 7.150 min
Delta R.T.: -0.001 min
Response: 101466205
Conc: 59.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

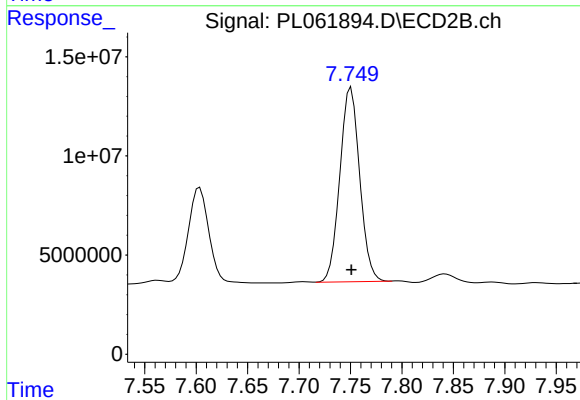


#21 Endrin ketone

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 131576870
Conc: 56.06 ng/ml

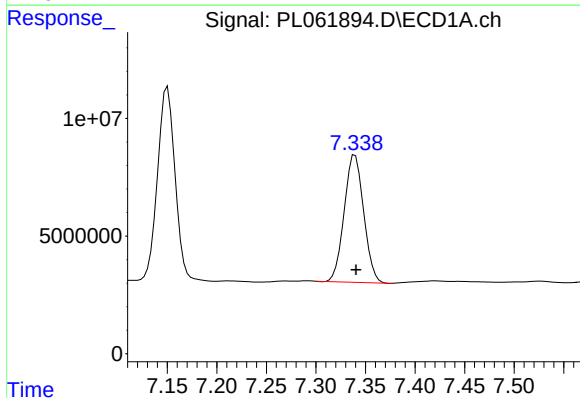


#22 Mirex

R.T.: 7.340 min
Delta R.T.: -0.001 min
Response: 73959250
Conc: 52.76 ng/ml

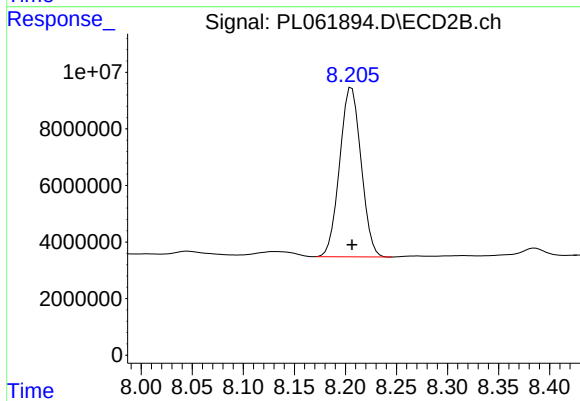

#22 Mirex

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 87605753
Conc: 49.72 ng/ml

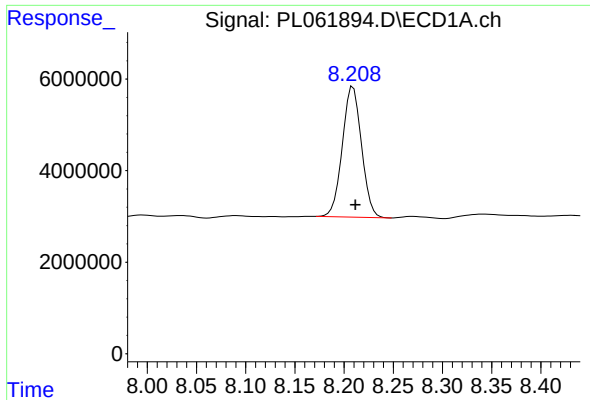


#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 38693305
Conc: 23.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
AC-4MS

Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:12 PM

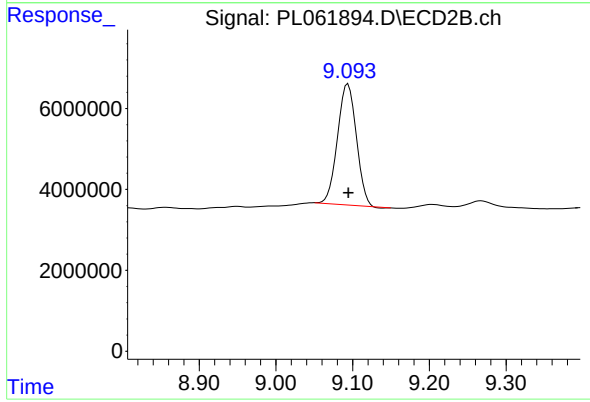

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 51038171
Conc: 23.18 ng/ml