

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
 Data File : PL061911.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 17:37
 Operator : DD\AJ
 Sample : L4175-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RR-3

Manual Integrations
 APPROVED

Ankita
 10/2/2020 2:59:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 03:40:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.458	4.007	32892689	48051518	19.281	17.613
28) SA Decachlor...	8.209	9.095	31421968	43161913	19.316	19.607
Target Compounds						
13) MA Dieldrin	5.750	6.499	2759674	1764524	1.641m	0.622m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
Data File : PL061911.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 17:37
Operator : DD\AJ
Sample : L4175-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RR-3


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 03:40:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

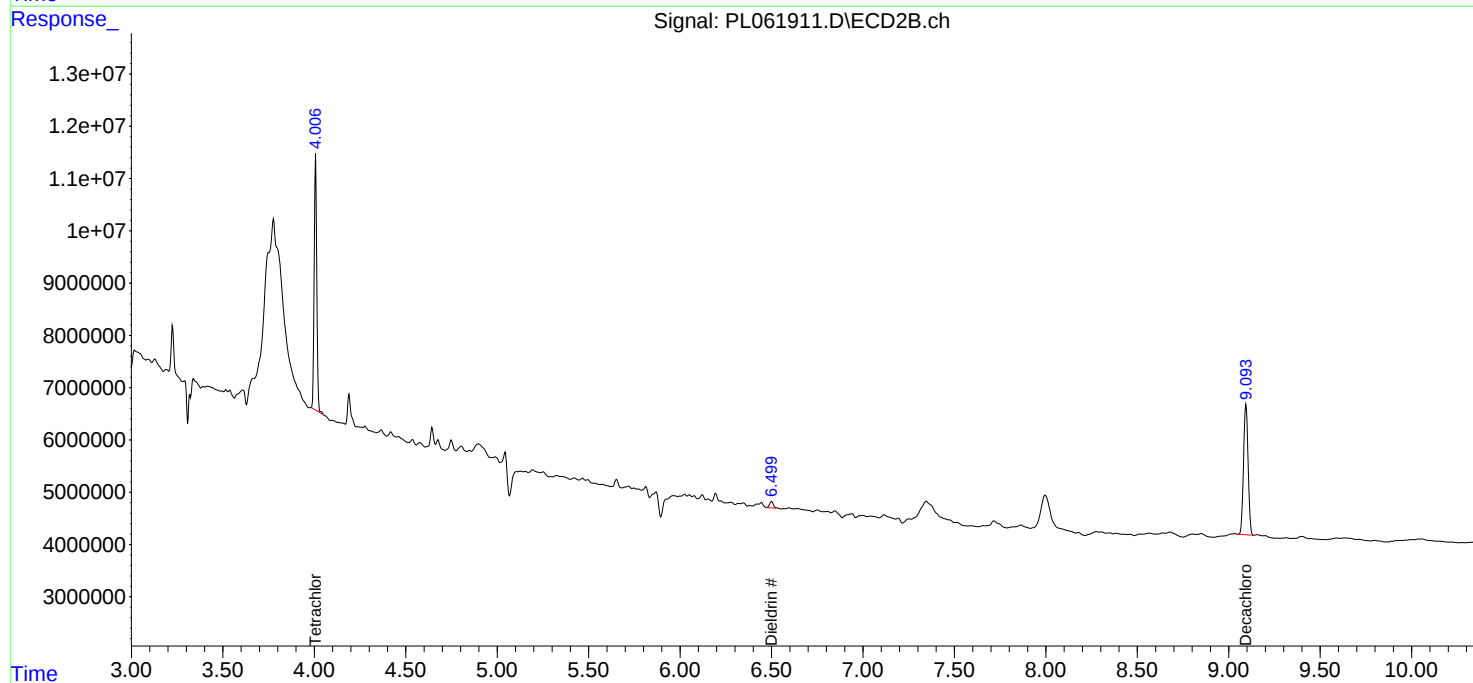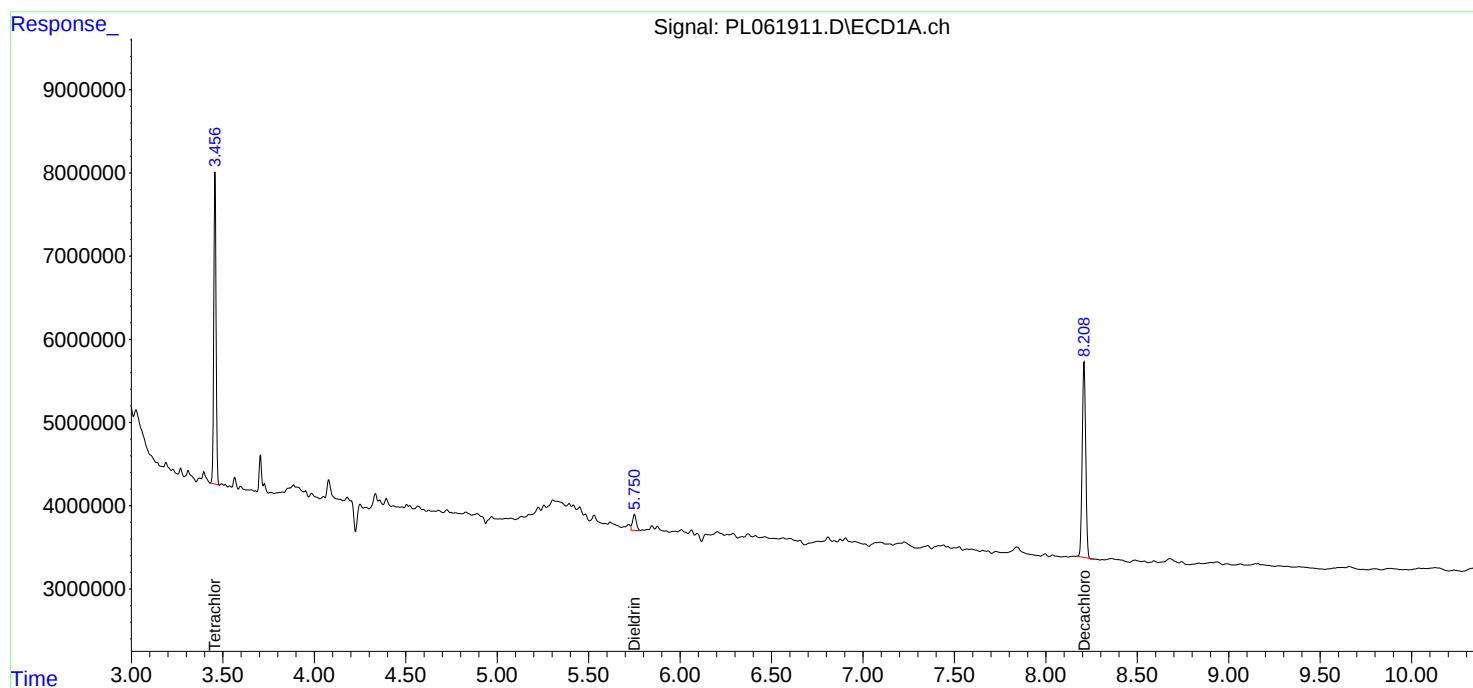

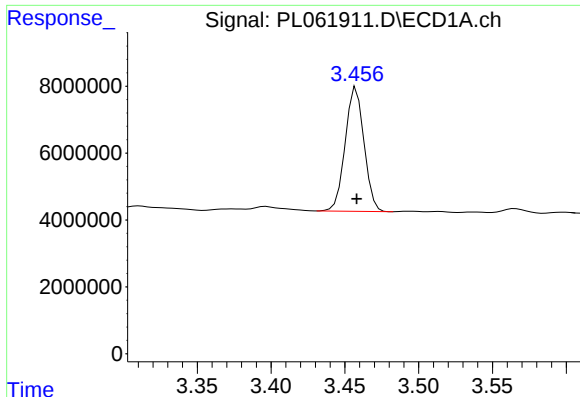


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 32892689
Conc: 19.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
RR-3


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:34 PM

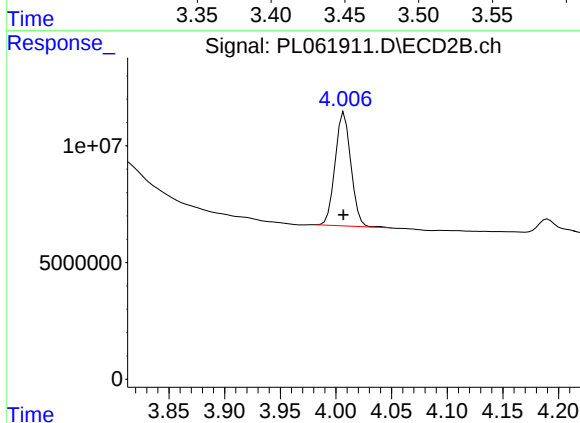


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 48051518
Conc: 17.61 ng/ml

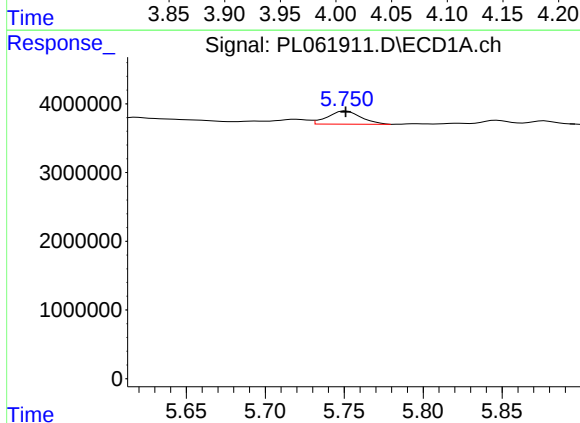


#13 Dieldrin

R.T.: 5.750 min
Delta R.T.: -0.001 min
Response: 2759674
Conc: 1.64 ng/ml m

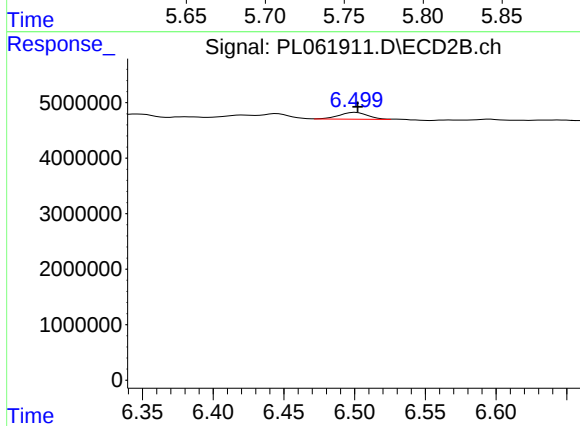

#13 Dieldrin

R.T.: 6.499 min
Delta R.T.: -0.003 min
Response: 1764524
Conc: 0.62 ng/ml m

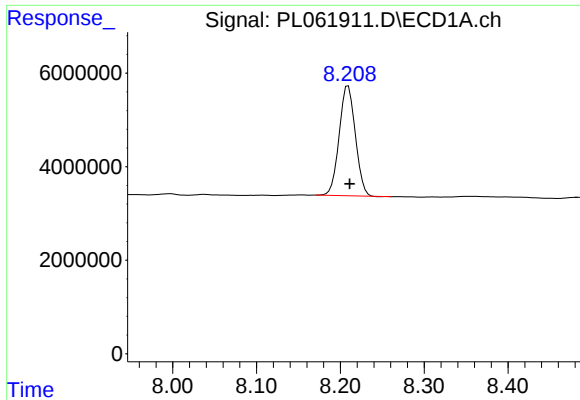


#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 31421968
Conc: 19.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
RR-3

Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:34 PM

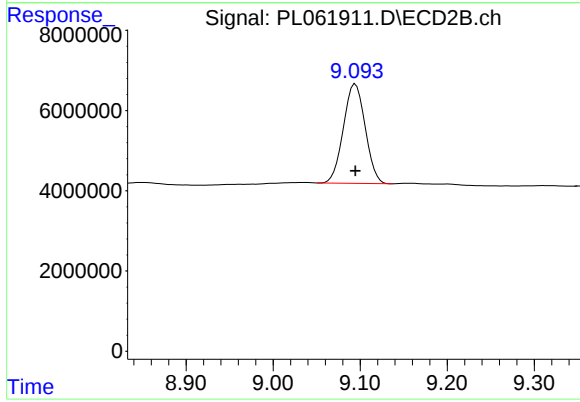

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 43161913
Conc: 19.61 ng/ml