

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
 Data File : PL061915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 18:33
 Operator : DD\AJ
 Sample : L4175-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RR-1

Manual Integrations
 APPROVED

Ankita
 10/2/2020 2:59:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 03:41:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.457	4.007	30839112	46786982	18.077	17.149
28) SA Decachlor...	8.210	9.095	35021745	50045855	21.529	22.734
Target Compounds						
13) MA Dieldrin	5.749	6.501	2394903	3090973	1.424m	1.090

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100120\
Data File : PL061915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 18:33
Operator : DD\AJ
Sample : L4175-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RR-1


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 03:41:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

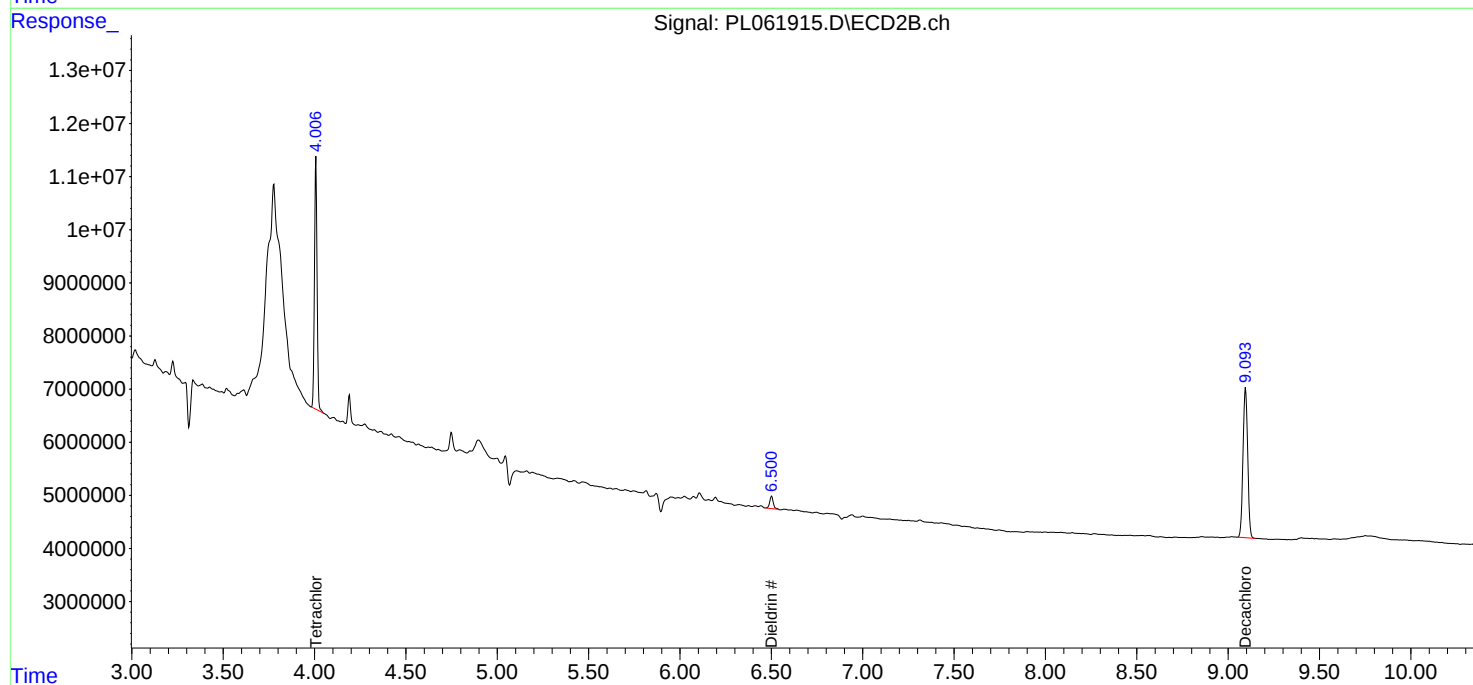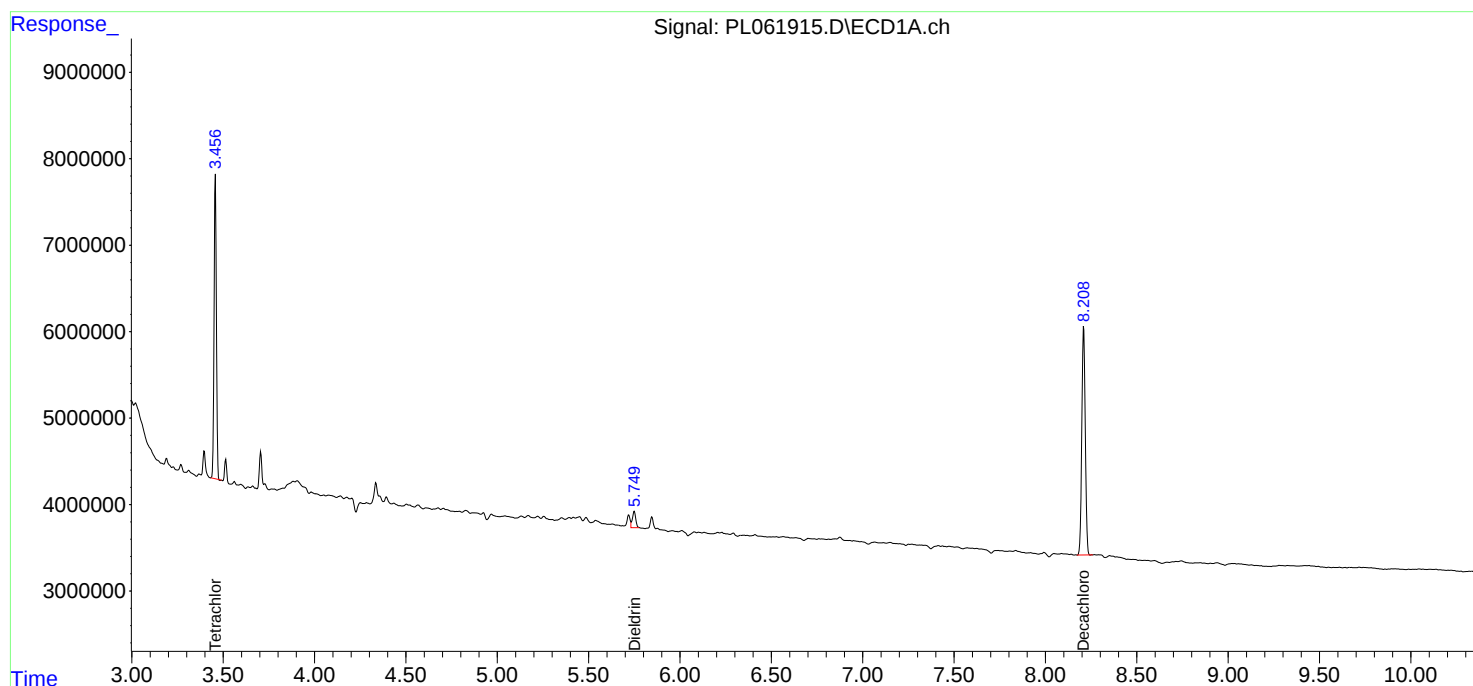

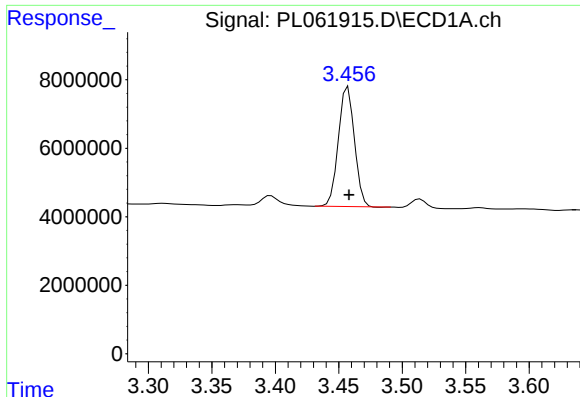


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 30839112
Conc: 18.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
RR-1


Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:38 PM

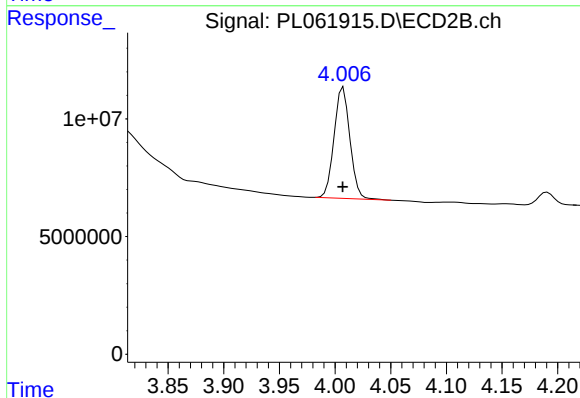


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 46786982
Conc: 17.15 ng/ml

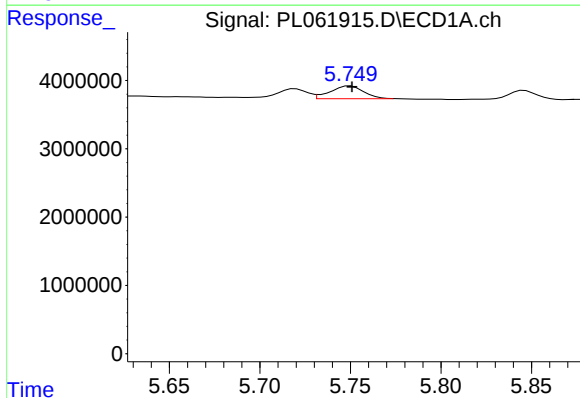


#13 Dieldrin

R.T.: 5.749 min
Delta R.T.: -0.002 min
Response: 2394903
Conc: 1.42 ng/ml m

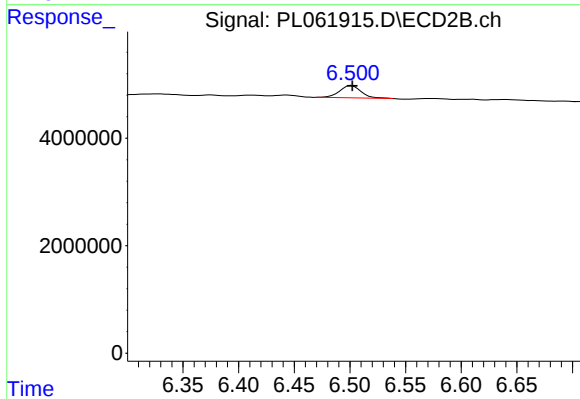

#13 Dieldrin

R.T.: 6.501 min
Delta R.T.: 0.000 min
Response: 3090973
Conc: 1.09 ng/ml

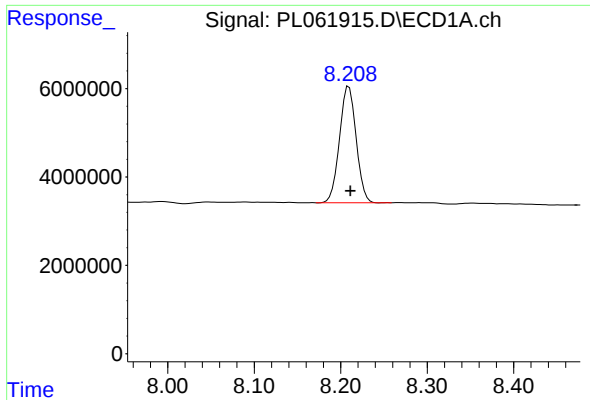


#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: -0.002 min
Response: 35021745
Conc: 21.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
RR-1

Manual Integrations
APPROVED

Ankita
10/2/2020 2:59:38 PM

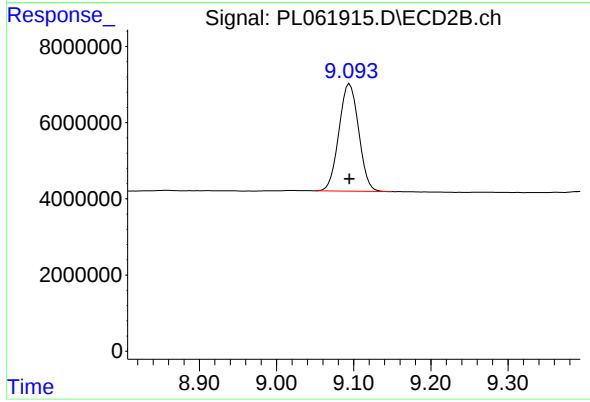

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 50045855
Conc: 22.73 ng/ml