

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100121\
 Data File : PL070091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2021 14:57
 Operator : AR\AJ
 Sample : M3988-01 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-092921

Manual Integrations
 APPROVED

mohammad
 10/4/2021 11:14:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 01:14:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.626	5.562	1374031	3082640	2.746	2.331
28)	SA Decachlor...	10.391	11.481	1997453	3317620	2.887	2.741
Target Compounds							
10)	B gamma-Chl...	7.341	8.295	285536	1428981	0.394m	0.893 #
11)	B alpha-Chl...	7.410	8.378	408495	1841722	0.561m	1.168 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100121\
Data File : PL070091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2021 14:57
Operator : AR\AJ
Sample : M3988-01 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
OR-03-092921


Manual Integrations
APPROVED

mohammad
10/4/2021 11:14:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 01:14:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

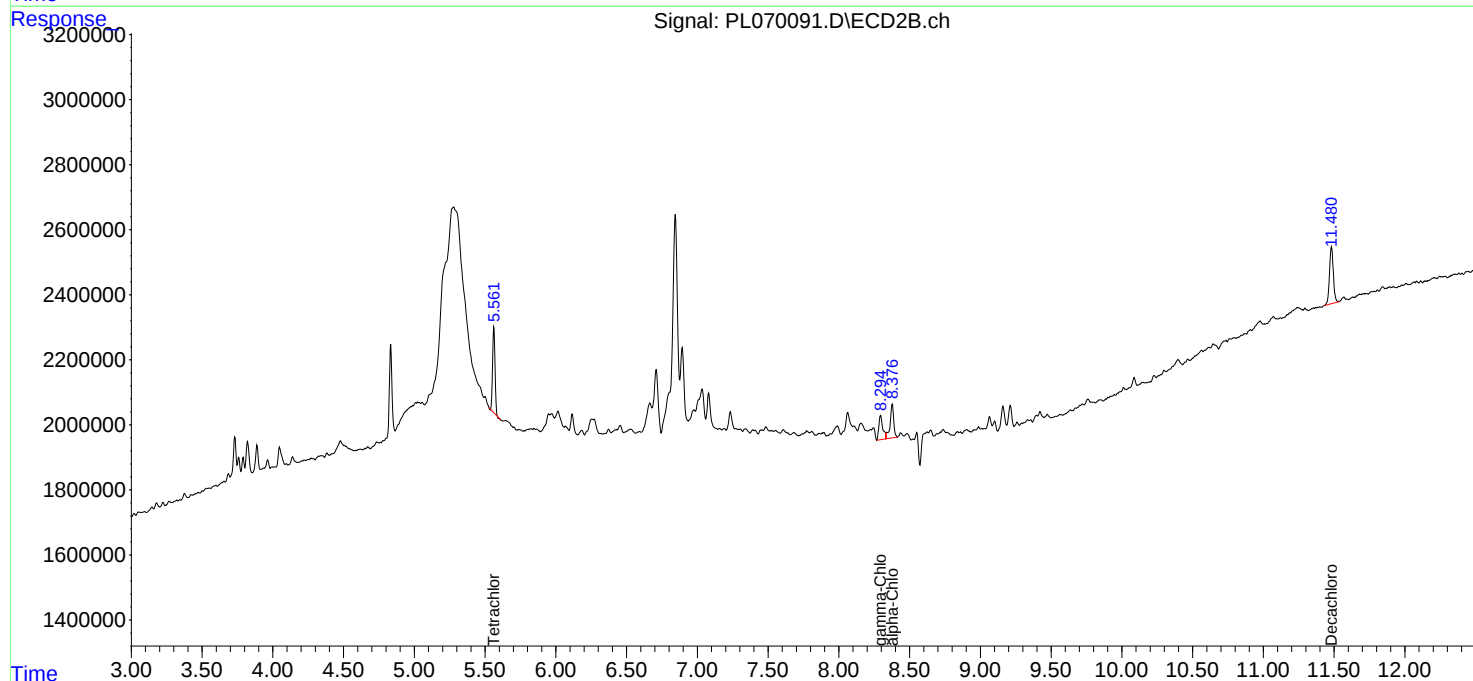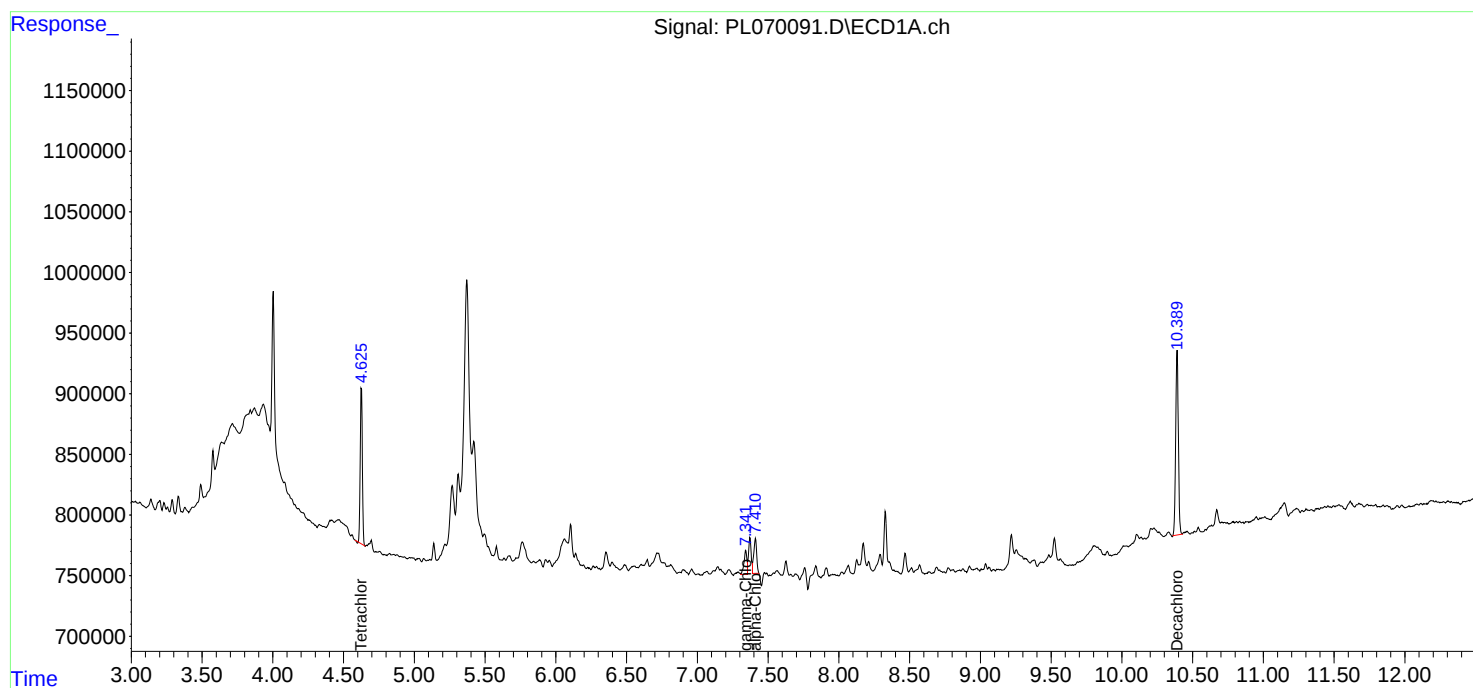

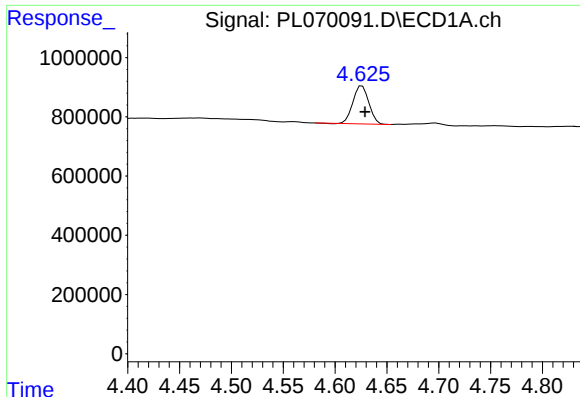


#1 Tetrachloro-m-xylene

R.T.: 4.626 min
Delta R.T.: -0.003 min
Response: 1374031
Conc: 2.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-092921


Manual Integrations
APPROVED

mohammad
10/4/2021 11:14:56 AM

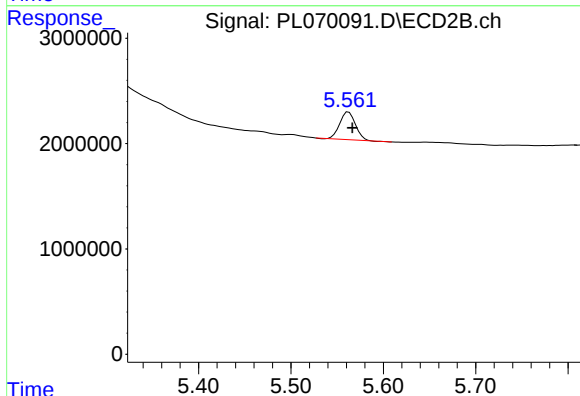


#1 Tetrachloro-m-xylene

R.T.: 5.562 min
Delta R.T.: -0.004 min
Response: 3082640
Conc: 2.33 ng/ml

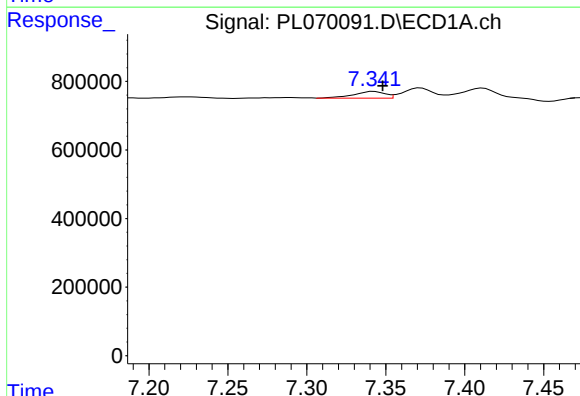


#10 gamma-Chlordane

R.T.: 7.341 min
Delta R.T.: -0.007 min
Response: 285536
Conc: 0.39 ng/ml m

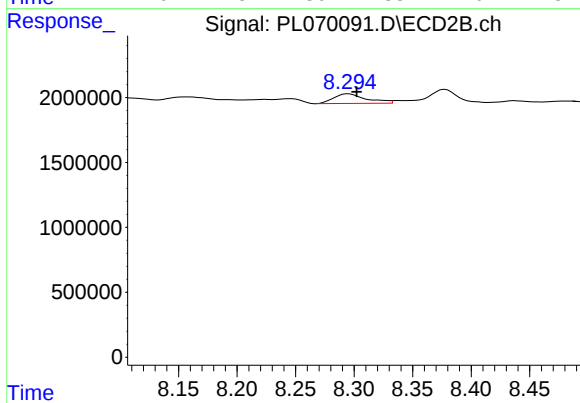

#10 gamma-Chlordane

R.T.: 8.295 min
Delta R.T.: -0.007 min
Response: 1428981
Conc: 0.89 ng/ml

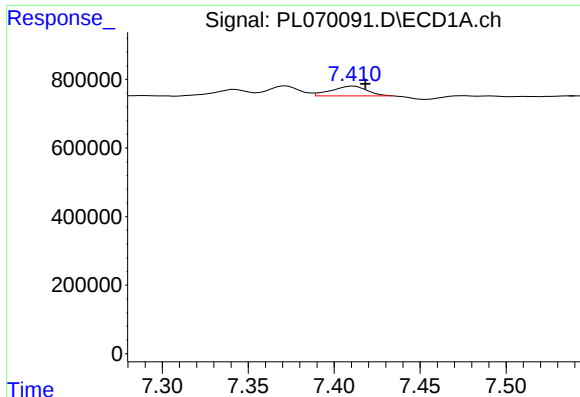


#11 alpha-Chlordane

R.T.: 7.410 min
Delta R.T.: -0.008 min
Response: 408495
Conc: 0.56 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OR-03-092921


Manual Integrations
APPROVED

mohammad
10/4/2021 11:14:56 AM

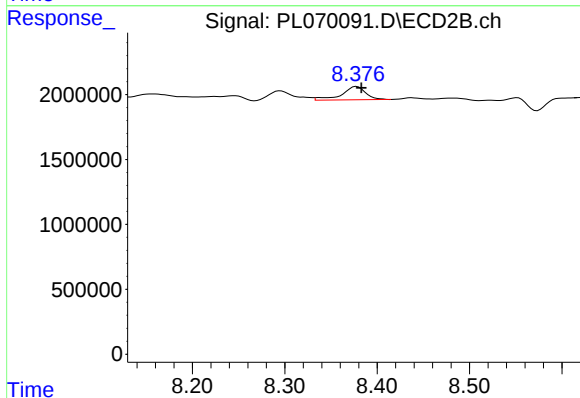


#11 alpha-Chlordane

R.T.: 8.378 min
Delta R.T.: -0.005 min
Response: 1841722
Conc: 1.17 ng/ml

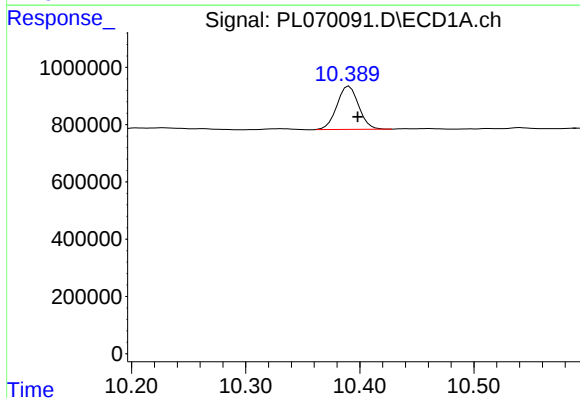

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.007 min
Response: 1997453
Conc: 2.89 ng/ml

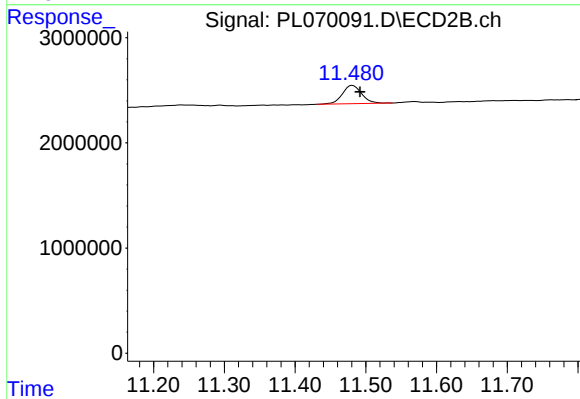

#28 Decachlorobiphenyl

R.T.: 11.481 min
Delta R.T.: -0.010 min
Response: 3317620
Conc: 2.74 ng/ml