

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100125\
 Data File : PL097466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2025 09:18
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:02:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.644	0.000	70995095	0	12.354	N.D. #
10) B	gamma-Chl...	5.876f	0.000	39168678	0	6.928	N.D. #
11) B	alpha-Chl...	5.959f	0.000	28728977	0	5.058	N.D. #
13) MA	Dieldrin	0.000	5.424	0	41938838	N.D.	5.129 #
14) MA	Endrin	0.000	5.708	0	102.7E6	N.D.	13.673 #
24)	Chlordane-2	0.000	4.400	0	11783742	N.D.	40.120 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100125\
Data File : PL097466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2025 09:18
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:02:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

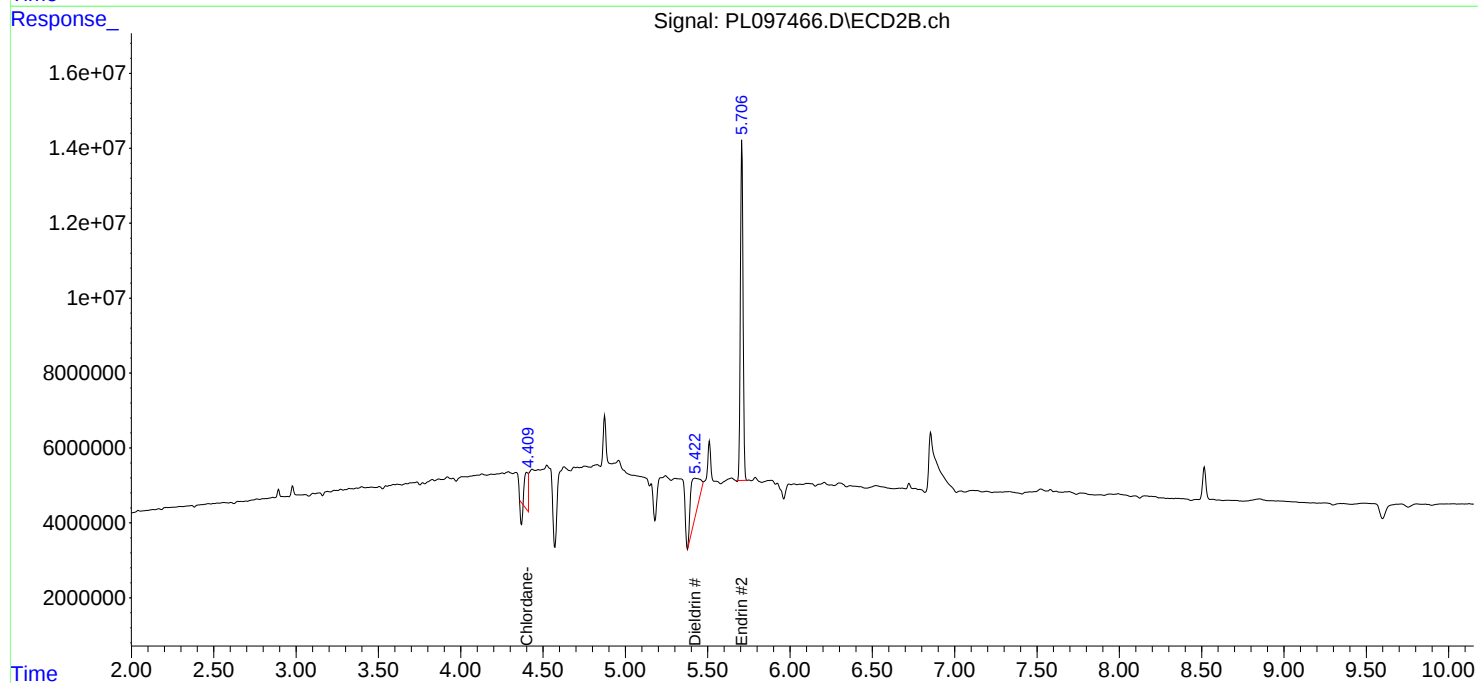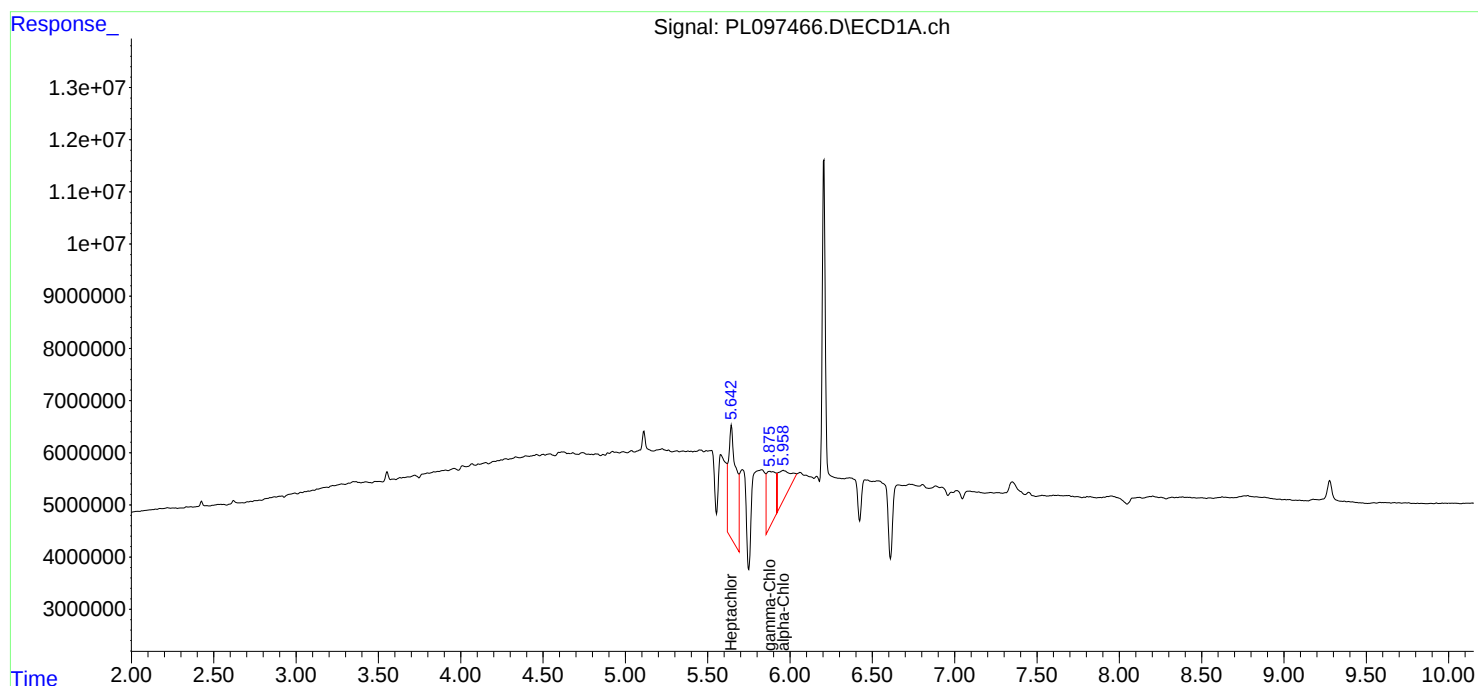


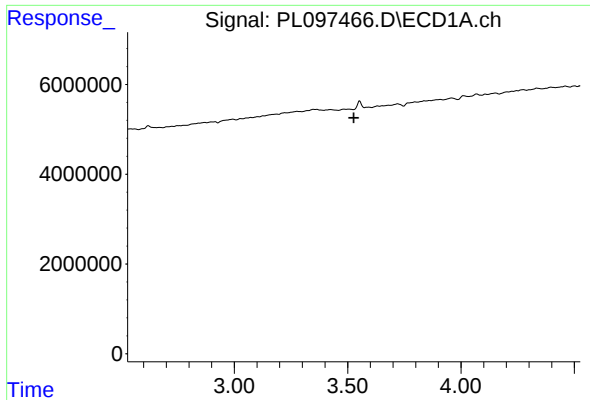

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

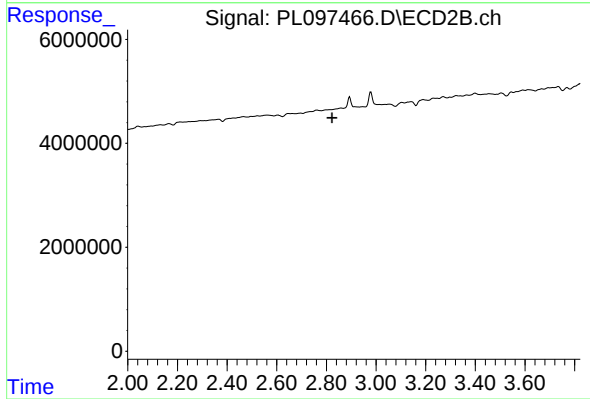


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.823 min
Response: 0
Conc: N.D.

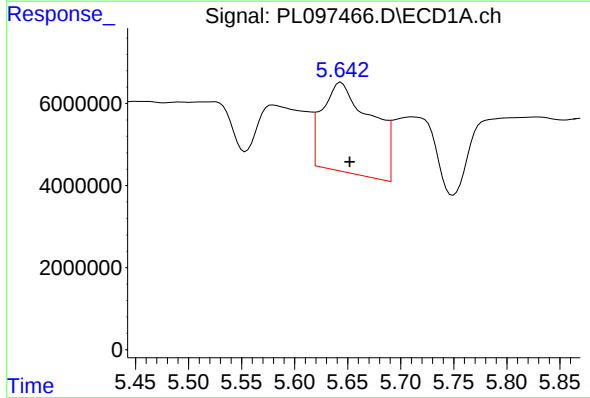


#8 Heptachlor epoxide

R.T.: 5.644 min
Delta R.T.: -0.008 min
Response: 70995095
Conc: 12.35 ng/ml

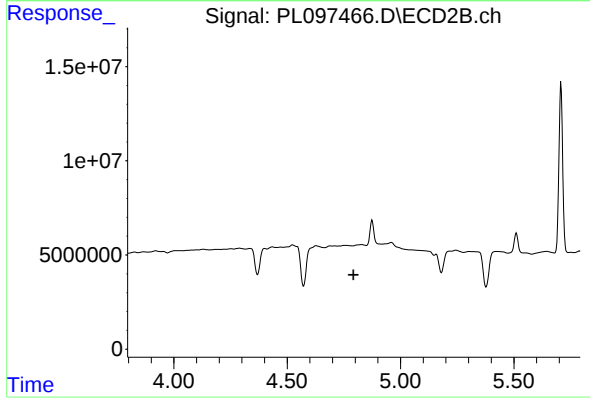

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.793 min
Response: 0
Conc: N.D.

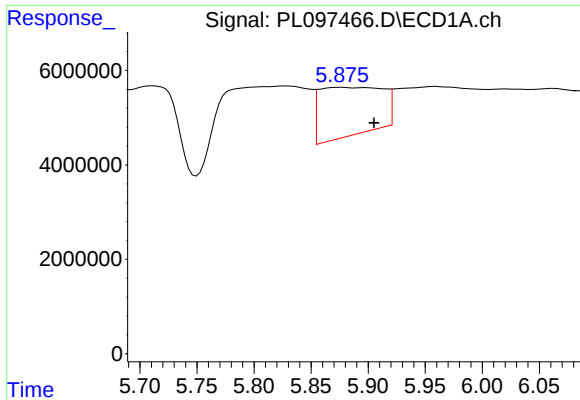

#10 gamma-Chlordane


R.T.: 5.876 min
Delta R.T.: -0.029 min
Response: 39168678
Conc: 6.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

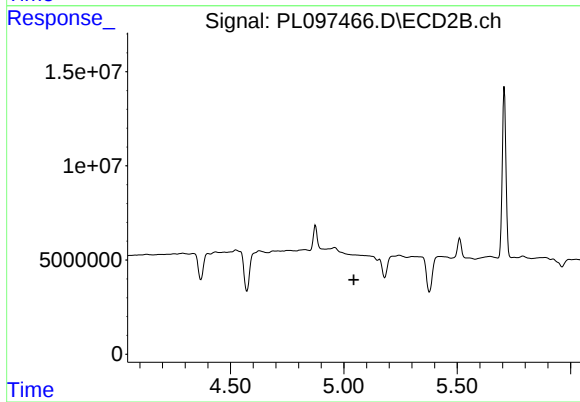


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.044 min
Response: 0
Conc: N.D.

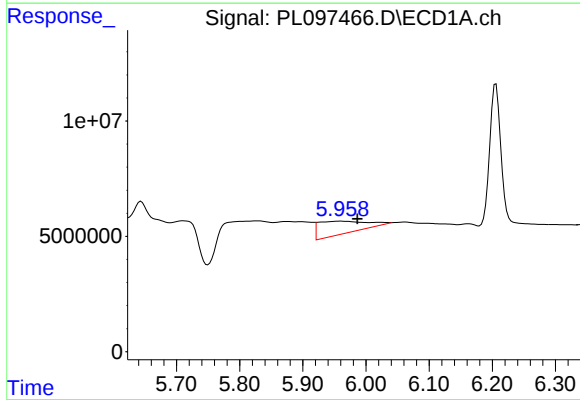


#11 alpha-Chlordane

R.T.: 5.959 min
Delta R.T.: -0.027 min
Response: 28728977
Conc: 5.06 ng/ml

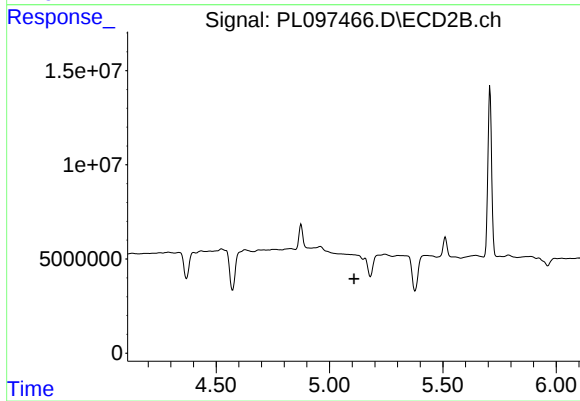

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

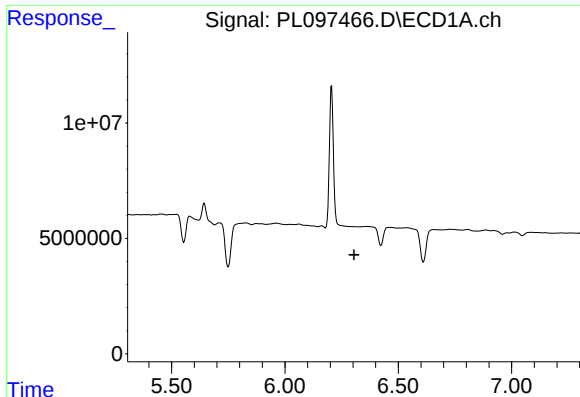

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

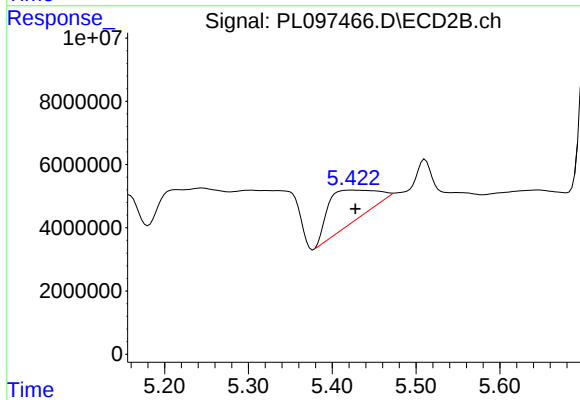


#13 Dieldrin

R.T.: 5.424 min
Delta R.T.: -0.004 min
Response: 41938838
Conc: 5.13 ng/ml

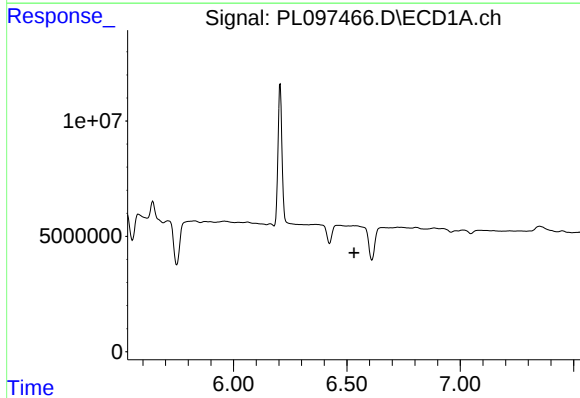


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

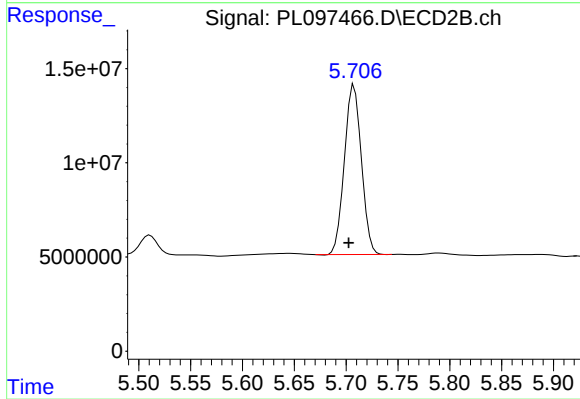

#14 Endrin


R.T.: 5.708 min
Delta R.T.: 0.005 min
Response: 102694035
Conc: 13.67 ng/ml

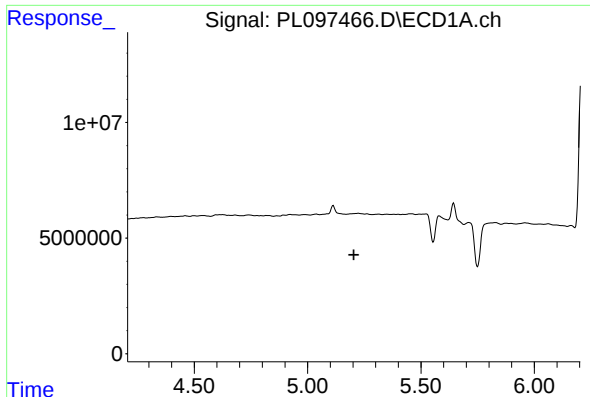

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

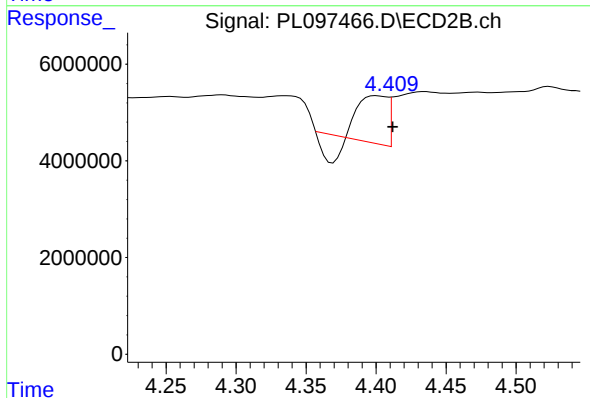


#24 Chlordane-2

R.T.: 4.400 min
Delta R.T.: -0.012 min
Response: 11783742
Conc: 40.12 ng/ml

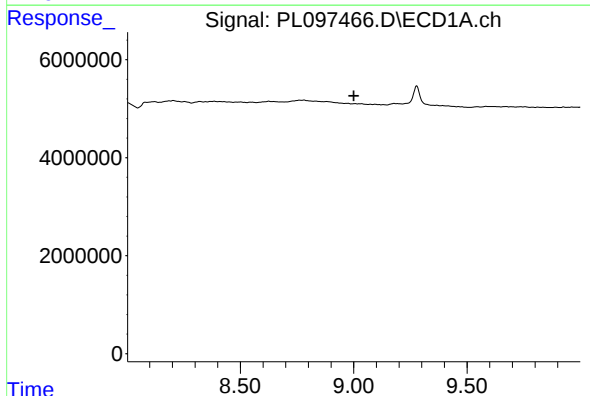

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.001 min
Response: 0
Conc: N.D.

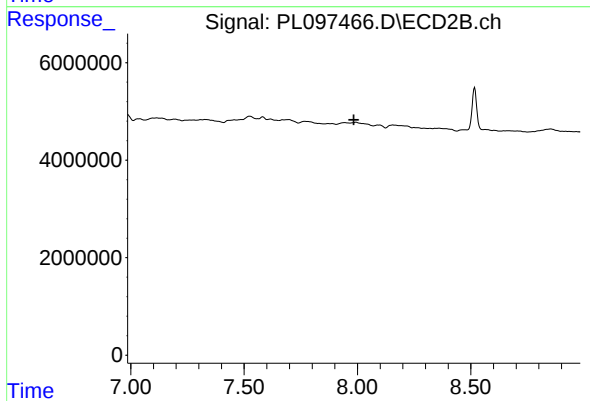

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.984 min
Response: 0
Conc: N.D.