

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100125\
 Data File : PL097479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2025 13:20
 Operator : AR\AJ
 Sample : Q3253-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ARS20-0009

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/02/2025
 Supervised By : mohammad ahmed 10/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 13:43:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.820	56395672	74599363	12.457	11.345m
28)	SA Decachlor...	9.000	7.980	55787499	79583055	17.049	13.983m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100125\
Data File : PL097479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2025 13:20
Operator : AR\AJ
Sample : Q3253-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ARS20-0009


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/02/2025
Supervised By : mohammad ahmed 10/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 13:43:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

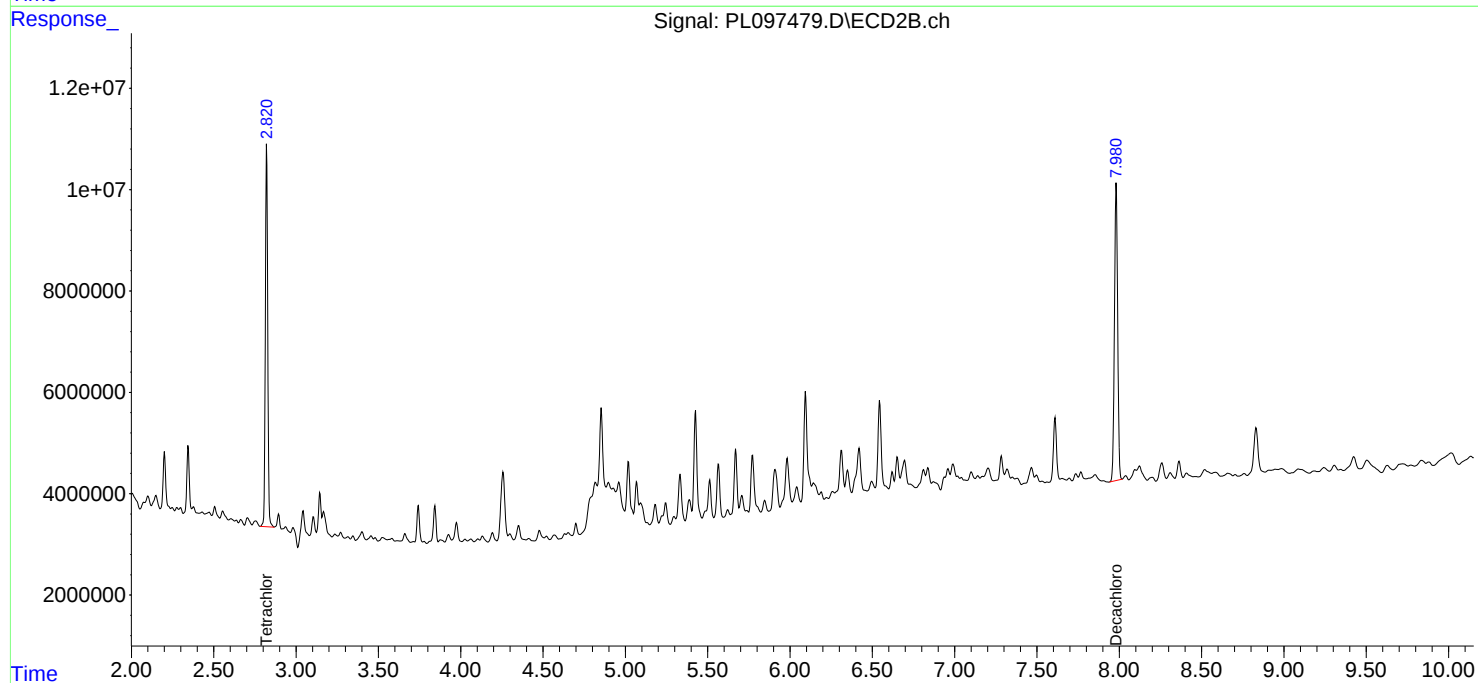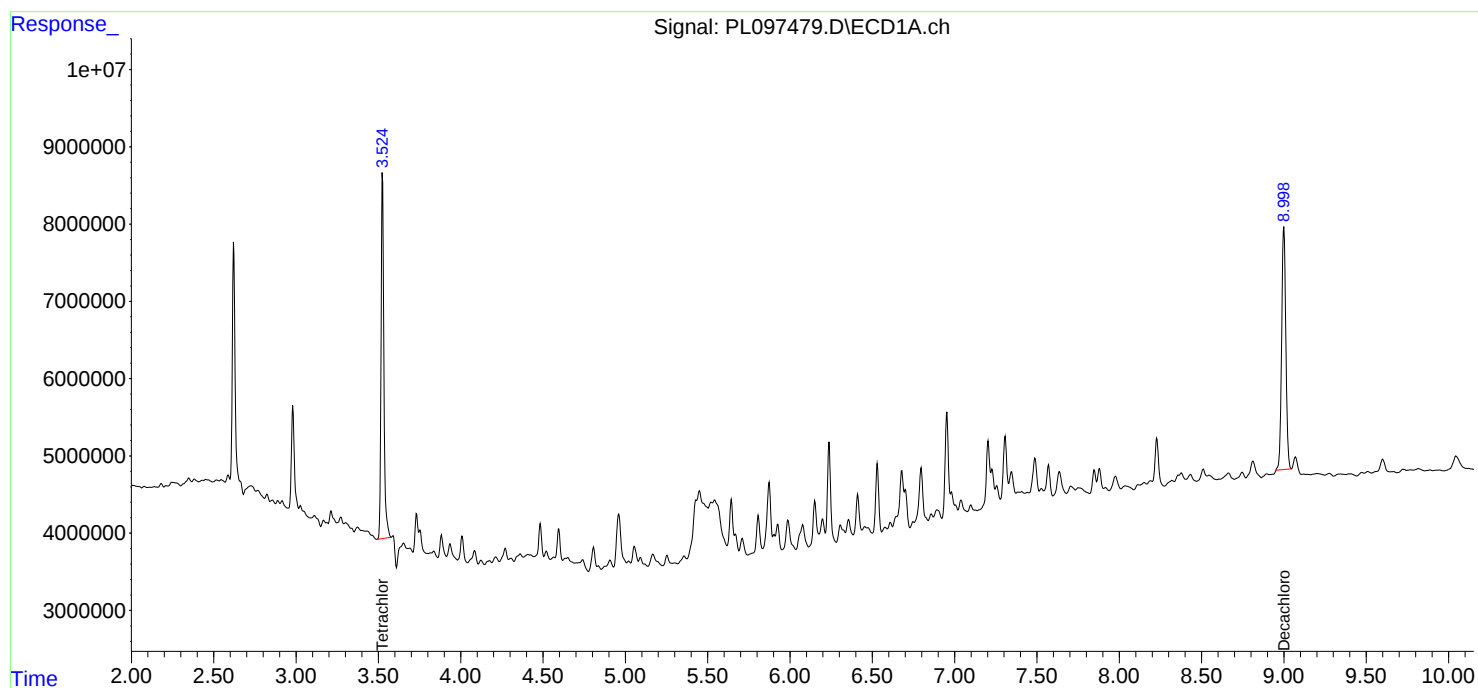

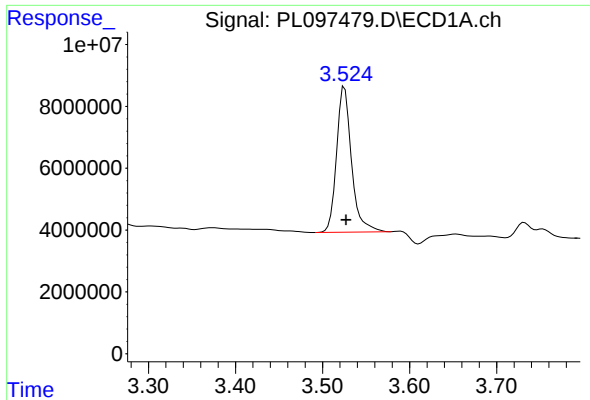


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.002 min
Response: 56395672
Conc: 12.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
ARS20-0009


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/02/2025
Supervised By :mohammad ahmed 10/06/2025

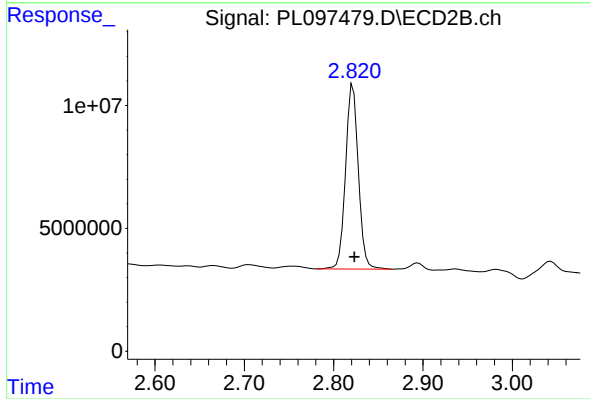


#1 Tetrachloro-m-xylene

R.T.: 2.820 min
Delta R.T.: -0.003 min
Response: 74599363
Conc: 11.34 ng/ml m

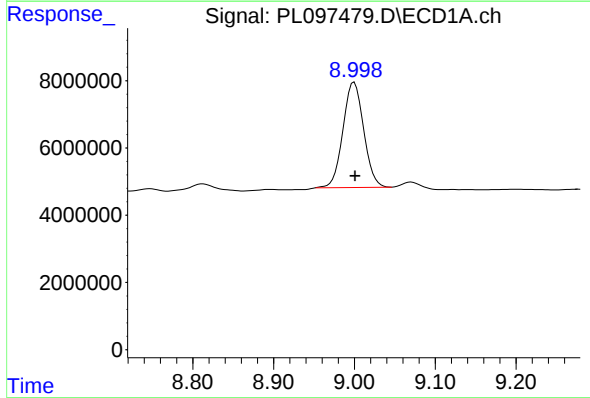

#28 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: -0.001 min
Response: 55787499
Conc: 17.05 ng/ml

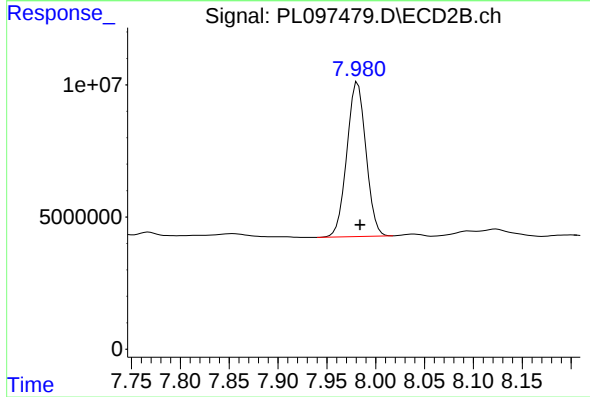

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.004 min
Response: 79583055
Conc: 13.98 ng/ml m