

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100125\
 Data File : PL097487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2025 15:20
 Operator : AR\AJ
 Sample : Q3257-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ENV2-6FT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/03/2025
 Supervised By :mohammad ahmed 10/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:03:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.524	2.823	62966974	89906479	13.909m	13.673
28) SA Decachlor...	8.996	7.980	46532970	70218052	14.221	12.337

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100125\
Data File : PL097487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2025 15:20
Operator : AR\AJ
Sample : Q3257-02
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ENV2-6FT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2025
Supervised By :mohammad ahmed 10/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:03:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

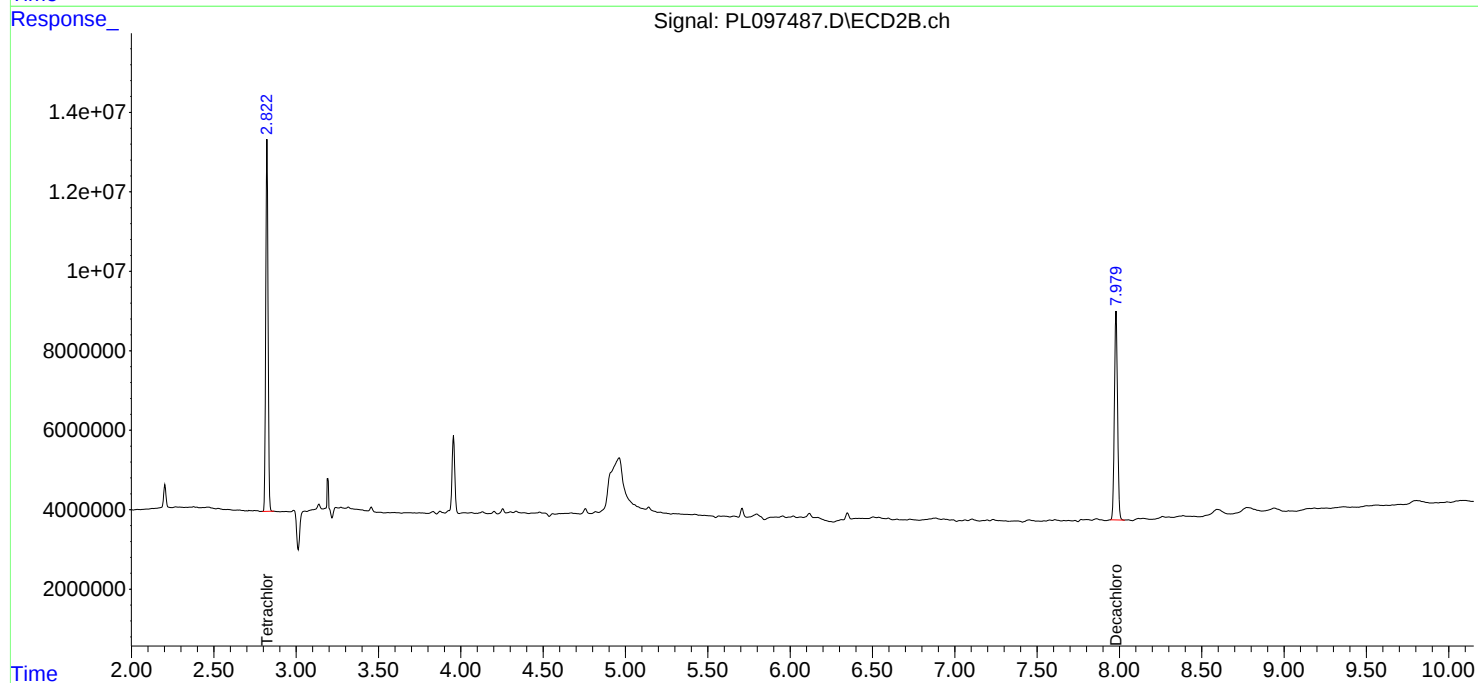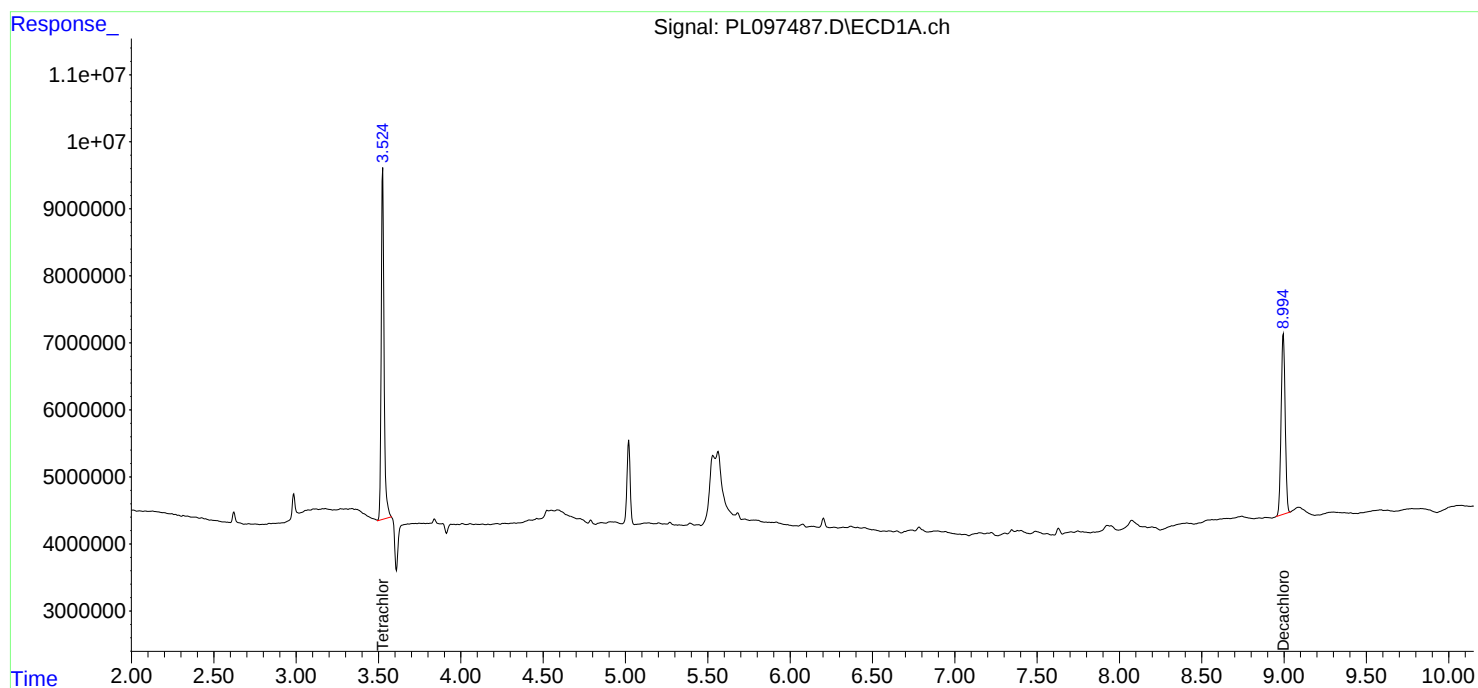

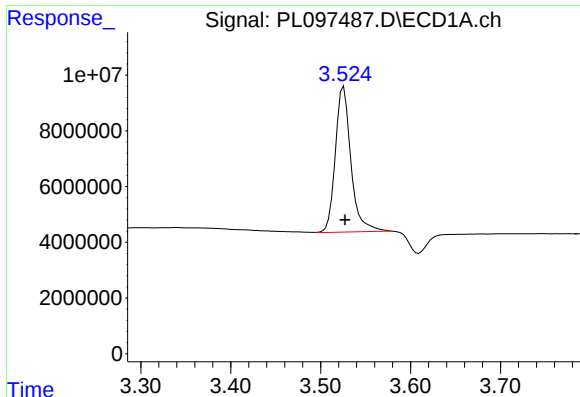


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: -0.003 min
Response: 62966974
Conc: 13.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
ENV2-6FT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2025
Supervised By :mohammad ahmed 10/06/2025

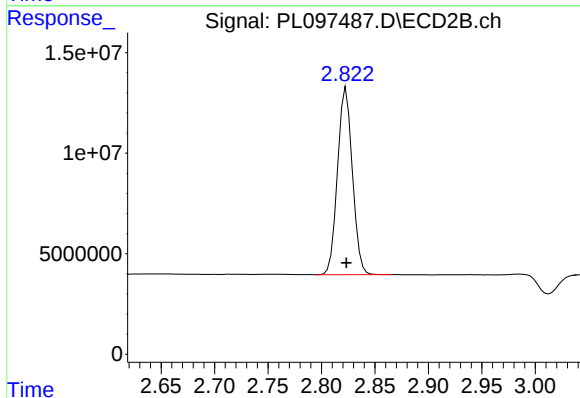


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 89906479
Conc: 13.67 ng/ml

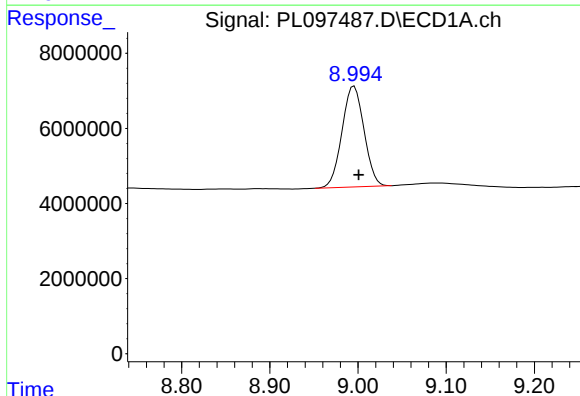

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: -0.005 min
Response: 46532970
Conc: 14.22 ng/ml

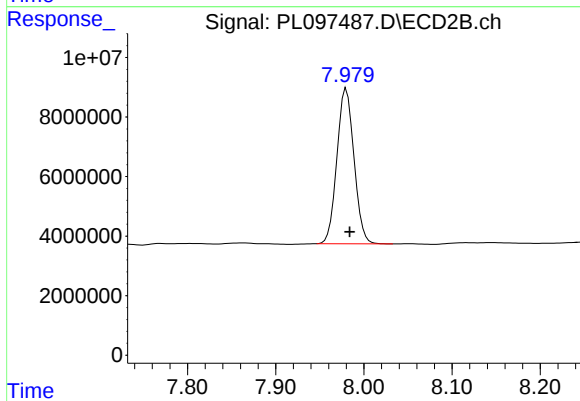

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.004 min
Response: 70218052
Conc: 12.34 ng/ml