

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
 Data File : PL040578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 17:08
 Operator : AJ\SJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Manual Integrations
 APPROVED

Sohil
 10/3/2018 8:42:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 02:44:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.806	361.5E6	136.5E6	49.380	43.225
2)	SA Decachlor...	7.809	8.728	433.7E6	127.1E6	45.624	40.136m
Target Compounds							
2)	A alpha-BHC	3.630	4.177	582.4E6	205.2E6	49.775	43.290
3)	MA gamma-BHC...	3.900	4.451	542.5E6	191.9E6	49.896	42.284
4)	MA Heptachlor	4.174	4.949	590.8E6	191.5E6	50.207	45.073
5)	MB Aldrin	4.406	5.245	540.0E6	179.3E6	51.102	42.487
6)	B beta-BHC	4.154	4.614	200.8E6	84878183	47.570	42.479
7)	B delta-BHC	4.340	4.823	555.3E6	190.4E6	49.753	41.253
8)	B Heptachlo...	4.836	5.622	498.2E6	160.3E6	48.134	41.761
9)	A Endosulfan I	5.159	5.969	488.3E6	158.1E6	48.440	42.487
10)	B gamma-Chl...	5.054	5.852	539.9E6	169.4E6	49.712	42.856
11)	B alpha-Chl...	5.110	5.924	519.3E6	167.4E6	49.570	42.645
12)	B 4,4'-DDE	5.277	6.082	557.6E6	168.6E6	50.448m	41.873
13)	MA Dieldrin	5.395	6.220	529.6E6	167.2E6	48.343	43.779
14)	MA Endrin	5.643	6.433	469.6E6	146.5E6	47.269m	44.857
15)	B Endosulfa...	5.918	6.636	494.7E6	146.0E6	49.656	41.771
16)	A 4,4'-DDD	5.784	6.560	437.6E6	129.6E6	47.403	40.780m
17)	MA 4,4'-DDT	6.014	6.857	379.4E6	131.1E6	46.914m	43.036
18)	B Endrin al...	6.083	6.758	390.1E6	122.6E6	46.463m	40.956
19)	B Endosulfa...	6.294	6.979	454.5E6	132.8E6	47.488	41.280
20)	A Methoxychlor	6.560	7.313	231.5E6	62143343	47.928	40.778
21)	B Endrin ke...	6.768	7.437	530.9E6	137.3E6	48.936m	44.664

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
Data File : PL040578.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 17:08
Operator : AJ\SJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 02:44:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

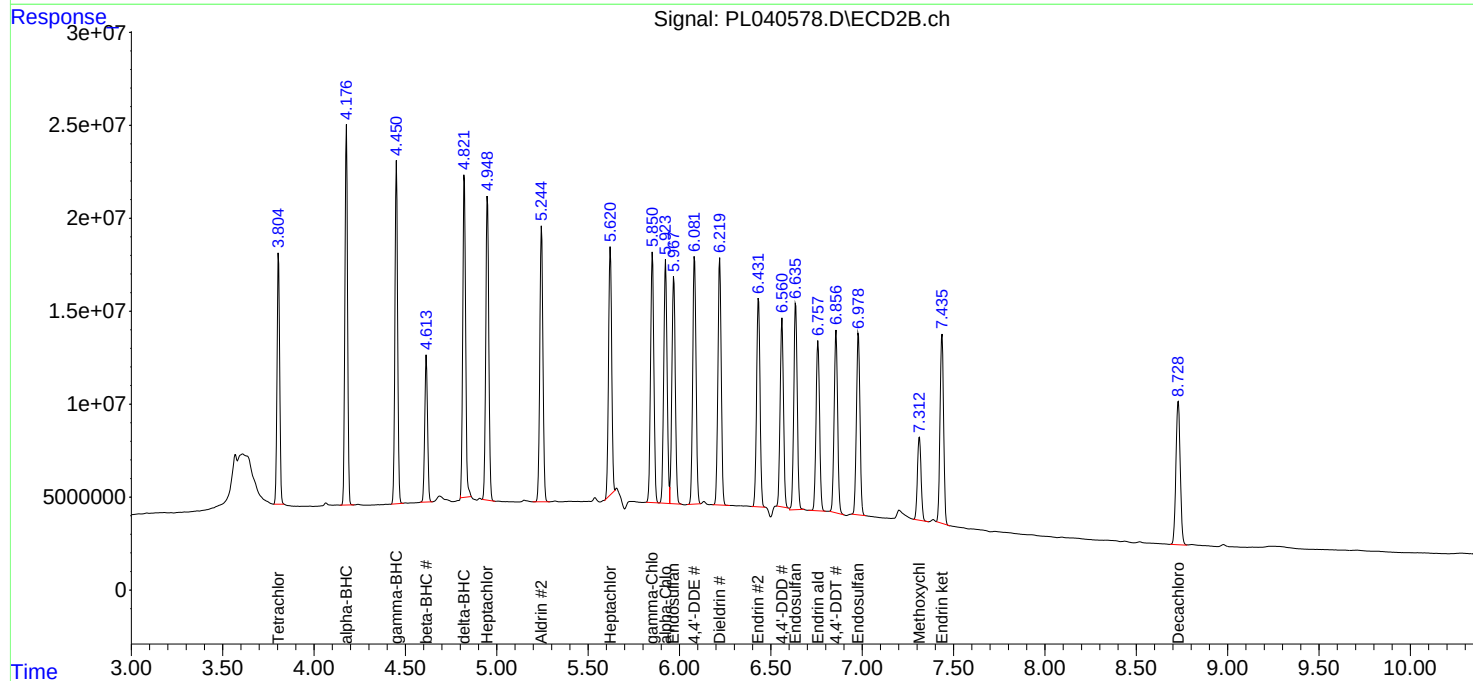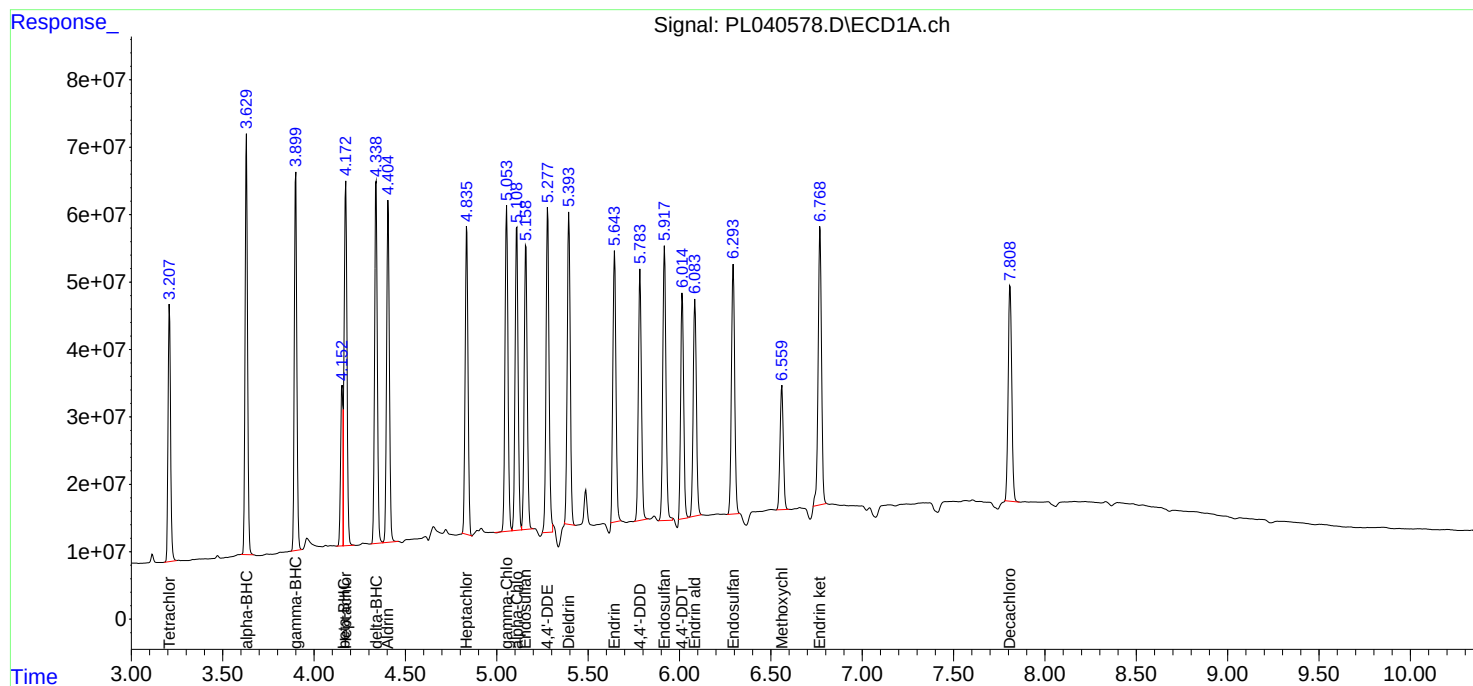

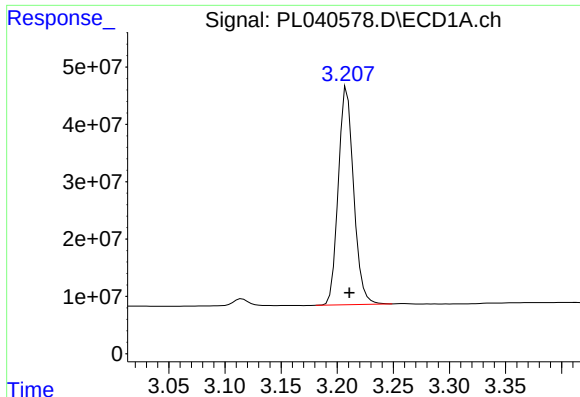


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 361465302
Conc: 49.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

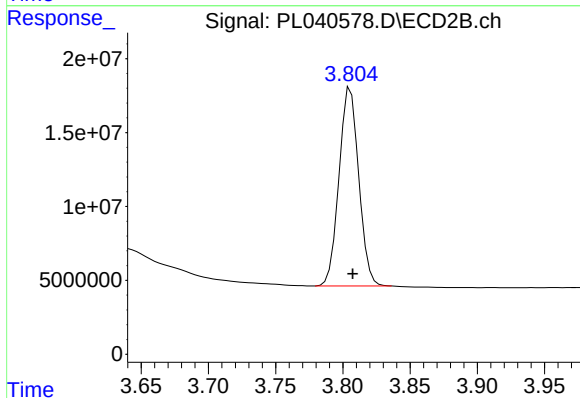


#1 Tetrachloro-m-xylene

R.T.: 3.806 min
Delta R.T.: -0.002 min
Response: 136497072
Conc: 43.23 ng/ml

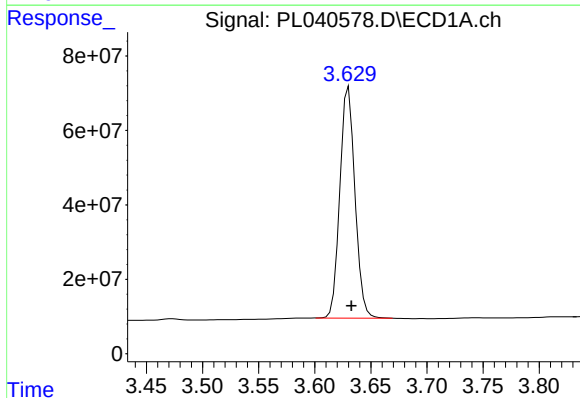


#2 alpha-BHC

R.T.: 3.630 min
Delta R.T.: -0.002 min
Response: 582392367
Conc: 49.78 ng/ml

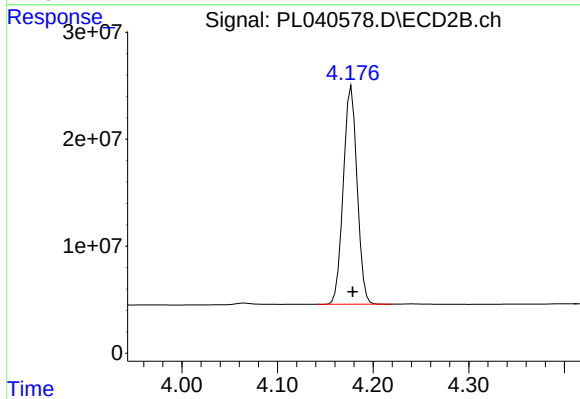

#2 alpha-BHC

R.T.: 4.177 min
Delta R.T.: -0.001 min
Response: 205246824
Conc: 43.29 ng/ml

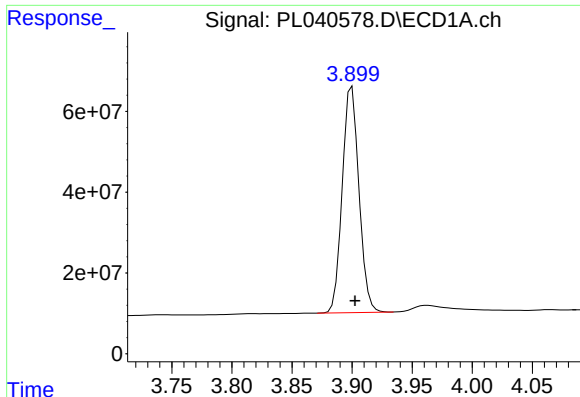


#3 gamma-BHC (Lindane)

R.T.: 3.900 min
Delta R.T.: -0.003 min
Response: 542498433
Conc: 49.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

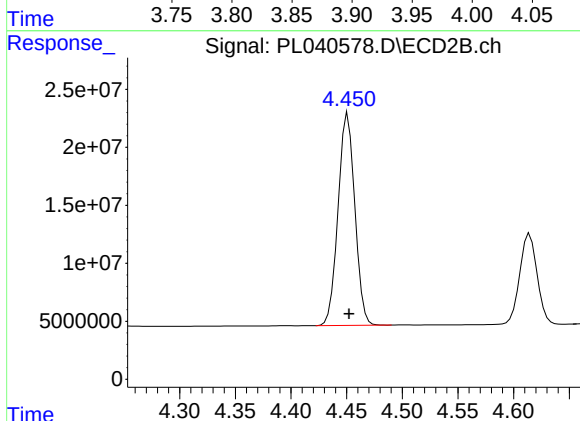


#3 gamma-BHC (Lindane)

R.T.: 4.451 min
Delta R.T.: -0.001 min
Response: 191892914
Conc: 42.28 ng/ml

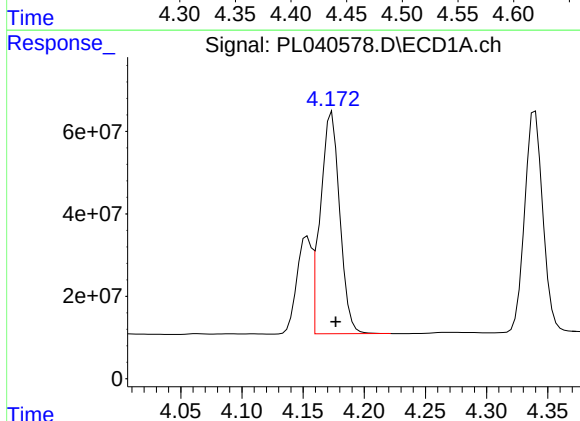


#4 Heptachlor

R.T.: 4.174 min
Delta R.T.: -0.003 min
Response: 590775329
Conc: 50.21 ng/ml

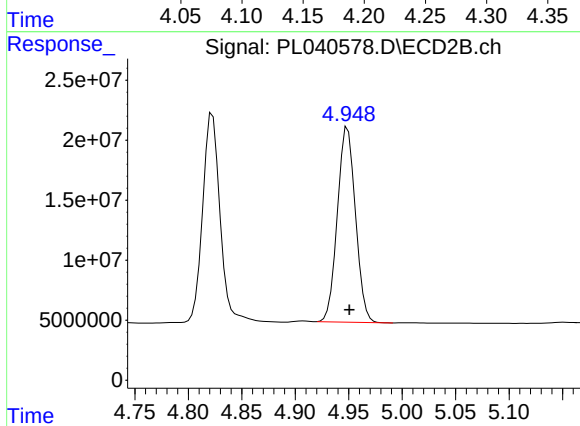

#4 Heptachlor

R.T.: 4.949 min
Delta R.T.: -0.002 min
Response: 191464704
Conc: 45.07 ng/ml

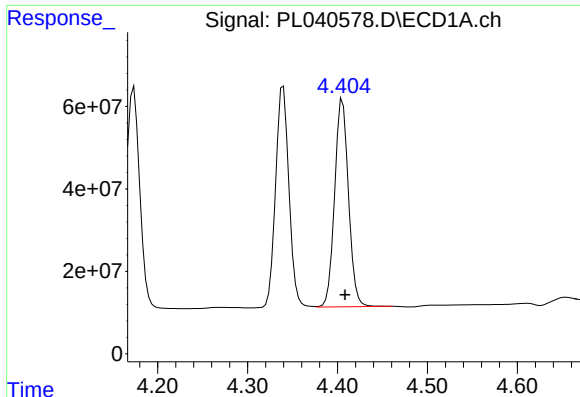


#5 Aldrin

R.T.: 4.406 min
Delta R.T.: -0.003 min
Response: 539965478
Conc: 51.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

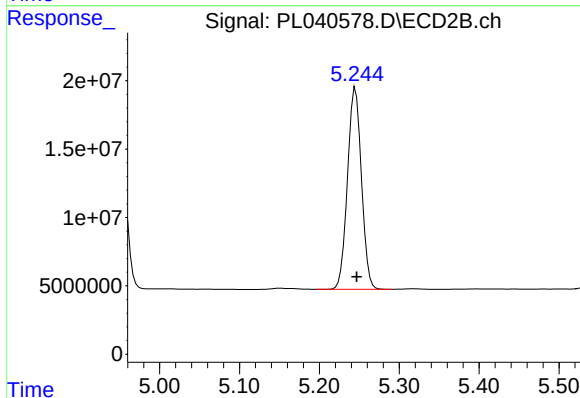


#5 Aldrin

R.T.: 5.245 min
Delta R.T.: -0.002 min
Response: 179306915
Conc: 42.49 ng/ml

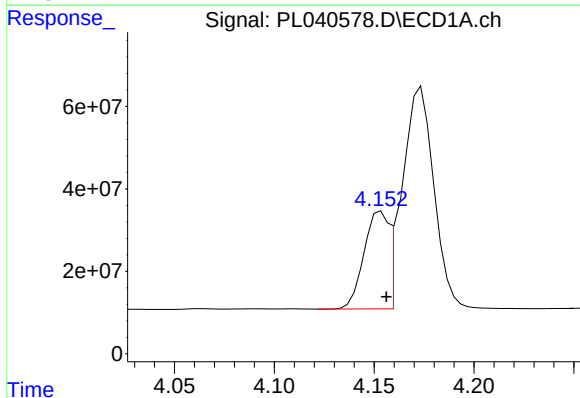


#6 beta-BHC

R.T.: 4.154 min
Delta R.T.: -0.003 min
Response: 200789732
Conc: 47.57 ng/ml

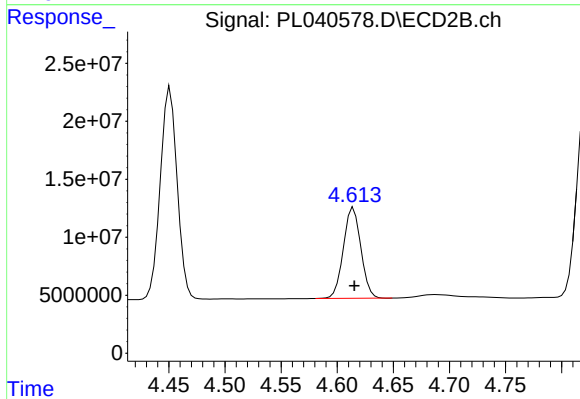

#6 beta-BHC

R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 84878183
Conc: 42.48 ng/ml

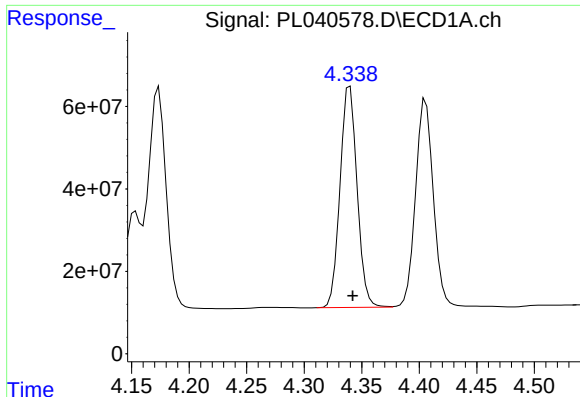


#7 delta-BHC

R.T.: 4.340 min
Delta R.T.: -0.002 min
Response: 555280978
Conc: 49.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

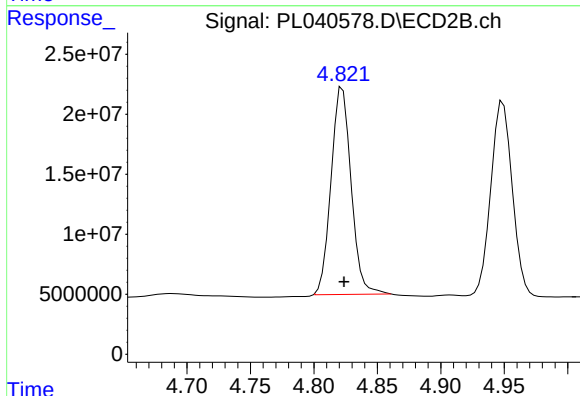


#7 delta-BHC

R.T.: 4.823 min
Delta R.T.: -0.001 min
Response: 190413155
Conc: 41.25 ng/ml

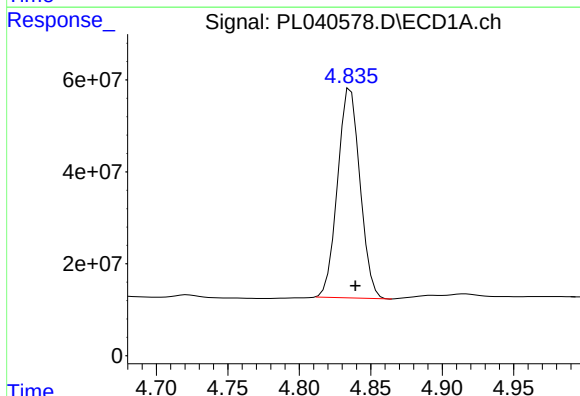


#8 Heptachlor epoxide

R.T.: 4.836 min
Delta R.T.: -0.003 min
Response: 498239638
Conc: 48.13 ng/ml

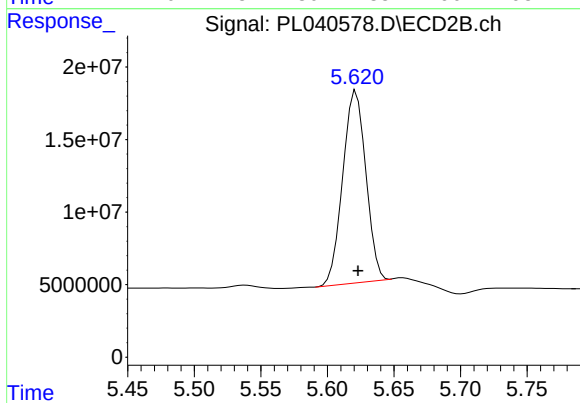

#8 Heptachlor epoxide

R.T.: 5.622 min
Delta R.T.: -0.001 min
Response: 160306225
Conc: 41.76 ng/ml

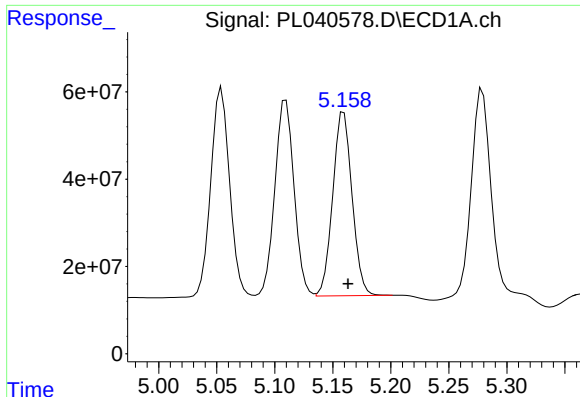


#9 Endosulfan I

R.T.: 5.159 min
Delta R.T.: -0.004 min
Response: 488257750
Conc: 48.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

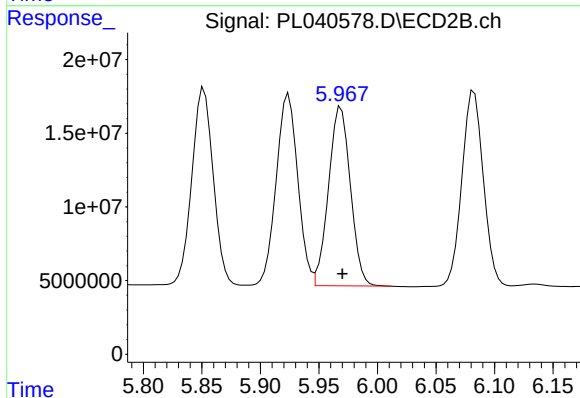


#9 Endosulfan I

R.T.: 5.969 min
Delta R.T.: -0.001 min
Response: 158077135
Conc: 42.49 ng/ml

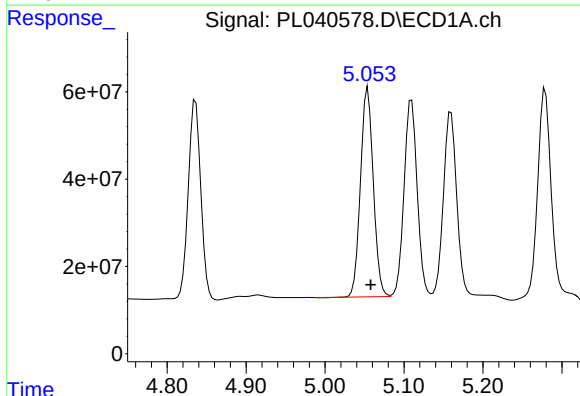


#10 gamma-Chlordane

R.T.: 5.054 min
Delta R.T.: -0.004 min
Response: 539862922
Conc: 49.71 ng/ml

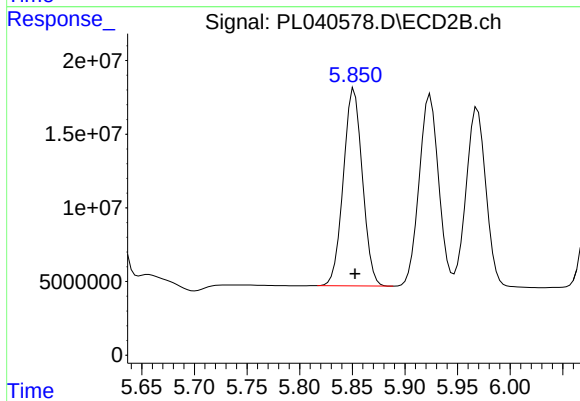

#10 gamma-Chlordane

R.T.: 5.852 min
Delta R.T.: 0.000 min
Response: 169356712
Conc: 42.86 ng/ml

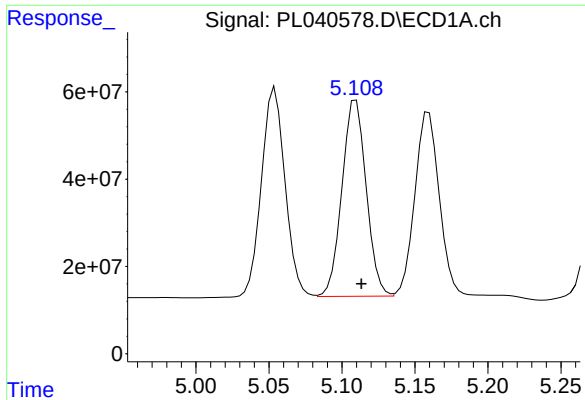


#11 alpha-Chlordane

R.T.: 5.110 min
Delta R.T.: -0.004 min
Response: 519328210
Conc: 49.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

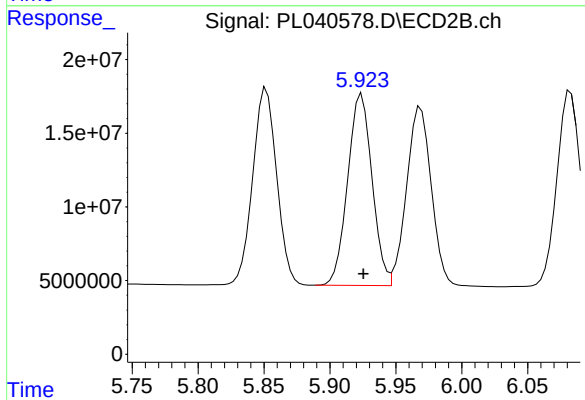


#11 alpha-Chlordane

R.T.: 5.924 min
Delta R.T.: -0.001 min
Response: 167357169
Conc: 42.64 ng/ml

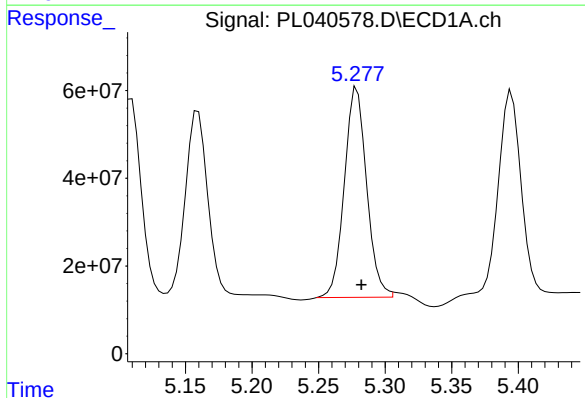


#12 4,4'-DDE

R.T.: 5.277 min
Delta R.T.: -0.005 min
Response: 557596904
Conc: 50.45 ng/ml m

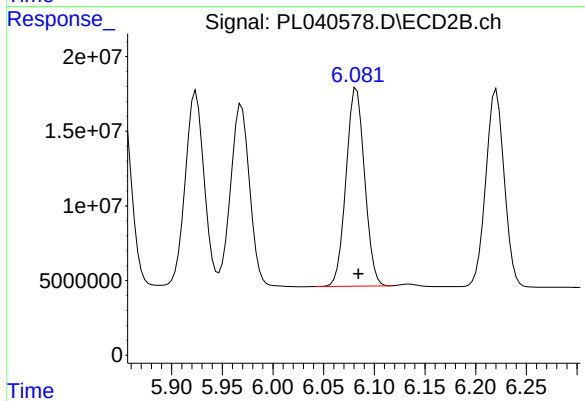

#12 4,4'-DDE

R.T.: 6.082 min
Delta R.T.: -0.002 min
Response: 168595022
Conc: 41.87 ng/ml

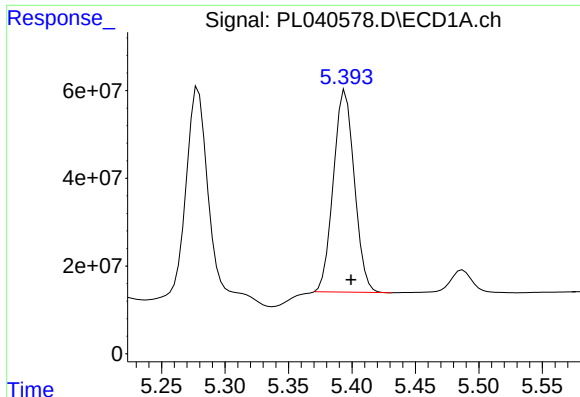


#13 Dieldrin

R.T.: 5.395 min
Delta R.T.: -0.004 min
Response: 529554719
Conc: 48.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

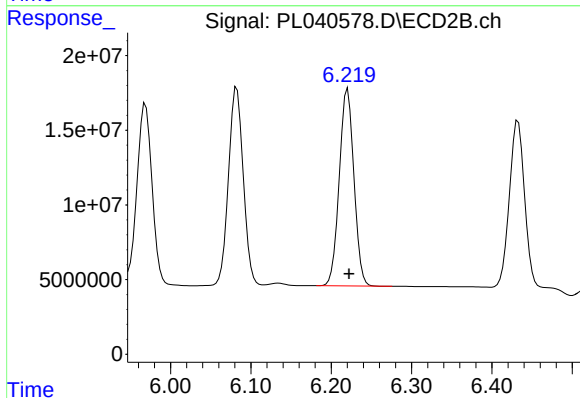


#13 Dieldrin

R.T.: 6.220 min
Delta R.T.: -0.002 min
Response: 167247658
Conc: 43.78 ng/ml

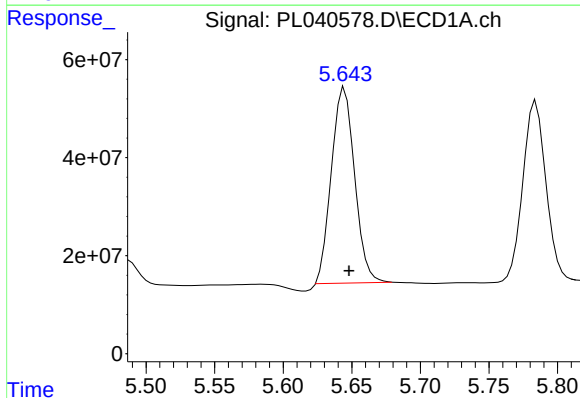


#14 Endrin

R.T.: 5.643 min
Delta R.T.: -0.005 min
Response: 469569602
Conc: 47.27 ng/ml m

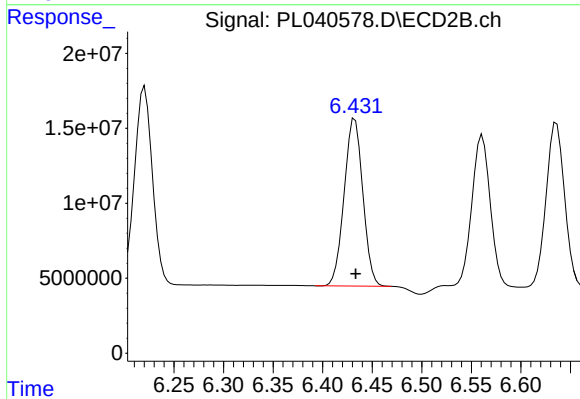

#14 Endrin

R.T.: 6.433 min
Delta R.T.: 0.000 min
Response: 146538408
Conc: 44.86 ng/ml

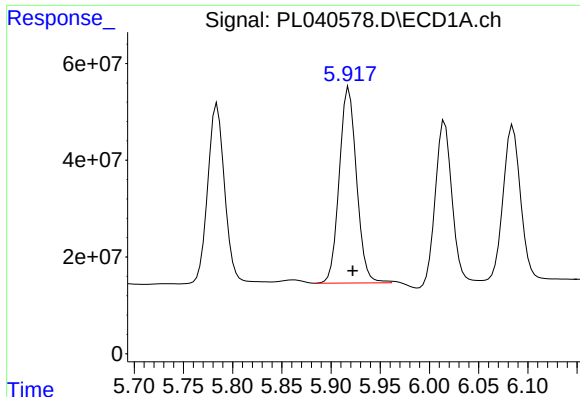


#15 Endosulfan II

R.T.: 5.918 min
Delta R.T.: -0.004 min
Response: 494699067
Conc: 49.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

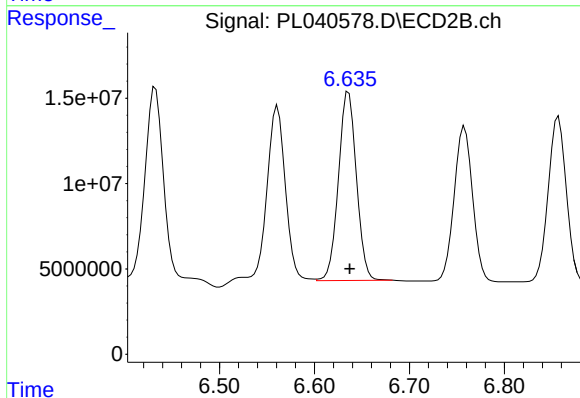


#15 Endosulfan II

R.T.: 6.636 min
Delta R.T.: -0.001 min
Response: 146019771
Conc: 41.77 ng/ml

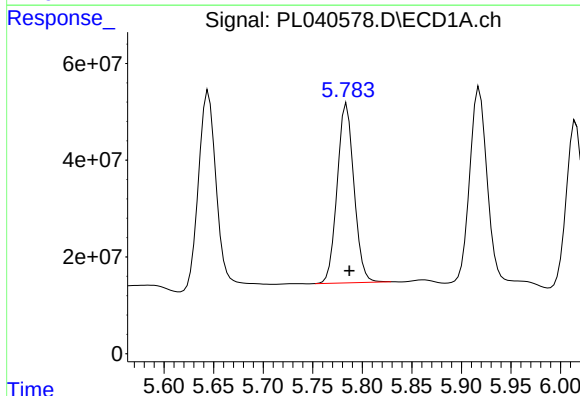


#16 4,4'-DDD

R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 437602390
Conc: 47.40 ng/ml

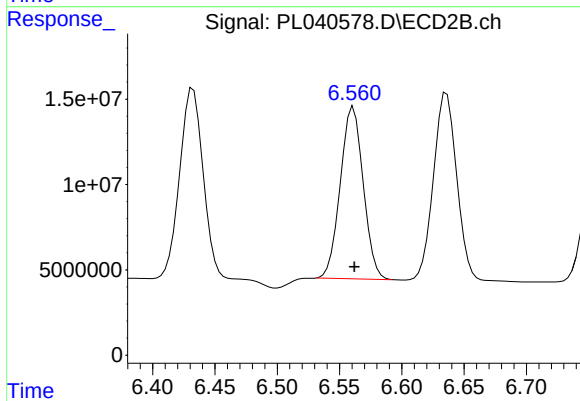

#16 4,4'-DDD

R.T.: 6.560 min
Delta R.T.: -0.002 min
Response: 129558486
Conc: 40.78 ng/ml m

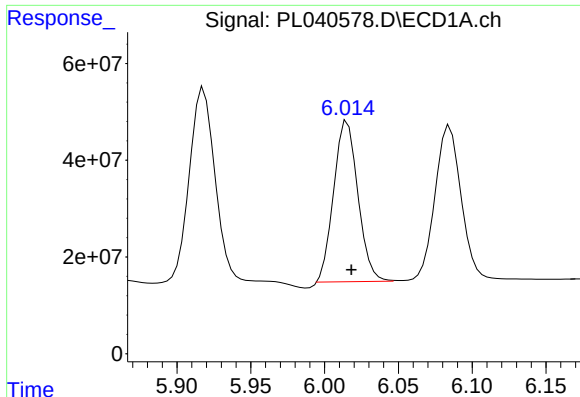


#17 4,4'-DDT

R.T.: 6.014 min
Delta R.T.: -0.004 min
Response: 379383101
Conc: 46.91 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

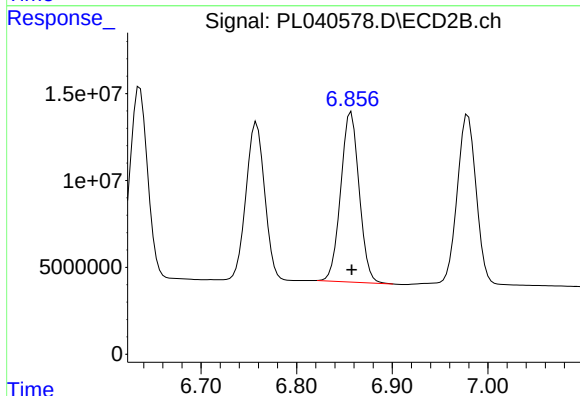


#17 4,4'-DDT

R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 131141782
Conc: 43.04 ng/ml

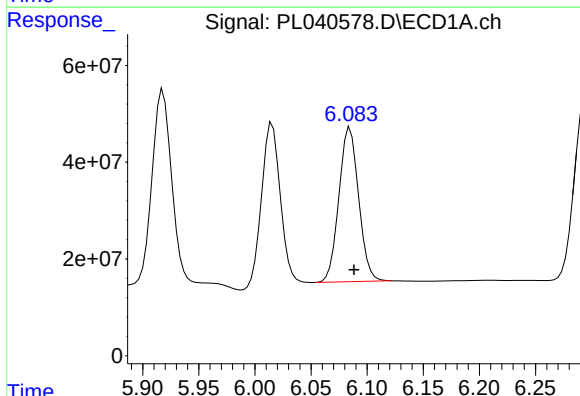


#18 Endrin aldehyde

R.T.: 6.083 min
Delta R.T.: -0.005 min
Response: 390145760
Conc: 46.46 ng/ml m

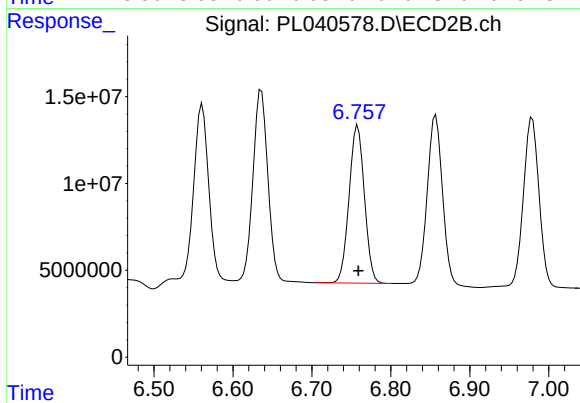

#18 Endrin aldehyde

R.T.: 6.758 min
Delta R.T.: -0.001 min
Response: 122591805
Conc: 40.96 ng/ml

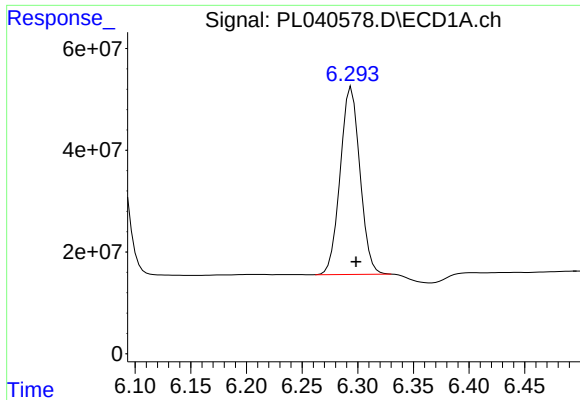


#19 Endosulfan Sulfate

R.T.: 6.294 min
Delta R.T.: -0.004 min
Response: 454520060
Conc: 47.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

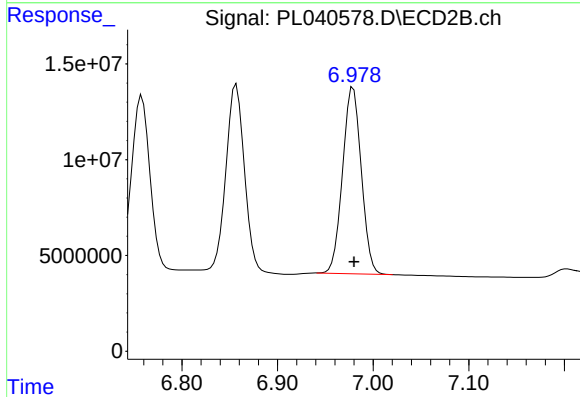


#19 Endosulfan Sulfate

R.T.: 6.979 min
Delta R.T.: 0.000 min
Response: 132775604
Conc: 41.28 ng/ml

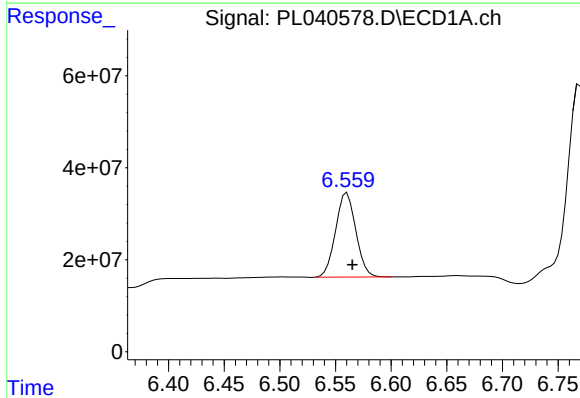


#20 Methoxychlor

R.T.: 6.560 min
Delta R.T.: -0.005 min
Response: 231507859
Conc: 47.93 ng/ml

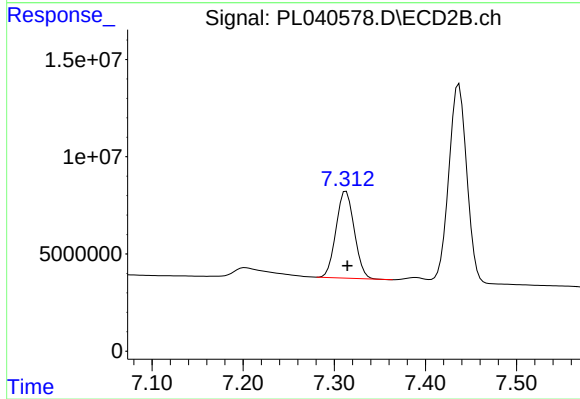

#20 Methoxychlor

R.T.: 7.313 min
Delta R.T.: -0.001 min
Response: 62143343
Conc: 40.78 ng/ml

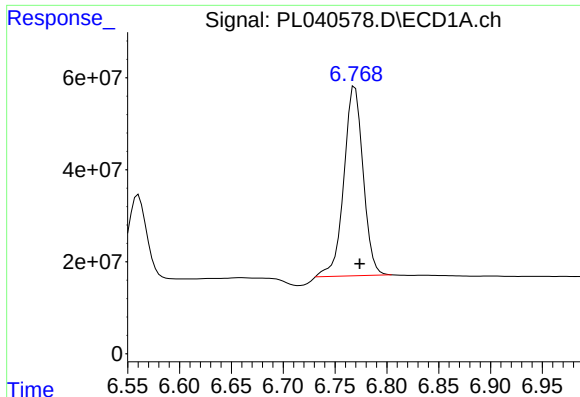


#21 Endrin ketone

R.T.: 6.768 min
Delta R.T.: -0.006 min
Response: 530939271
Conc: 48.94 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/3/2018 8:42:29 AM

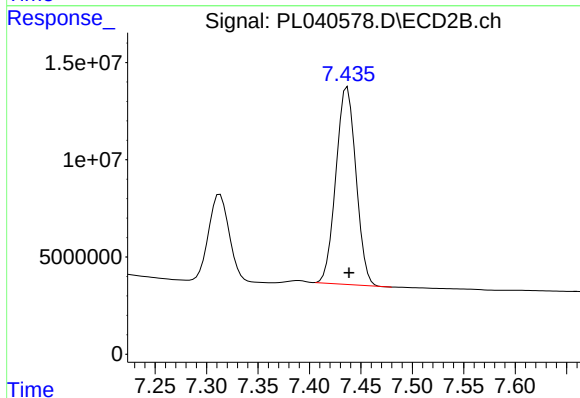


#21 Endrin ketone

R.T.: 7.437 min
Delta R.T.: -0.002 min
Response: 137302480
Conc: 44.66 ng/ml

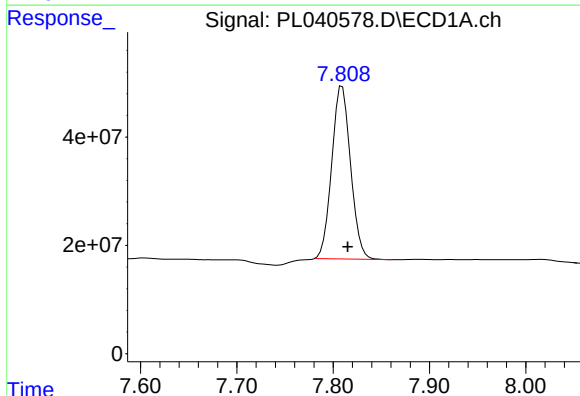

#28 Decachlorobiphenyl

R.T.: 7.809 min
Delta R.T.: -0.006 min
Response: 433690213
Conc: 45.62 ng/ml

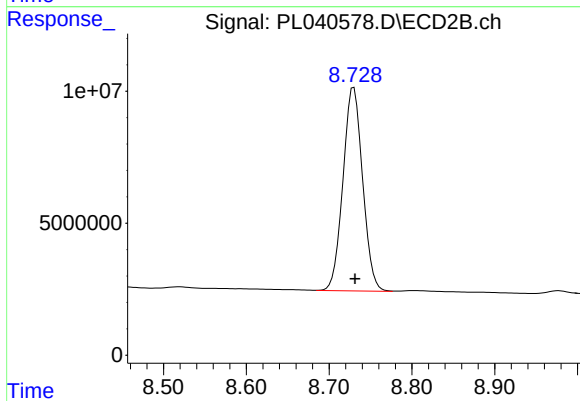

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: -0.003 min
Response: 127102108
Conc: 40.14 ng/ml m