

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
 Data File : PL052978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2019 09:19
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:08:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	4.047	254.0E6	66010001	25.536	24.583
28)	SA Decachlor...	8.346	9.127	209.7E6	68929951	20.936	23.496
Target Compounds							
8)	B Heptachlo...	0.000	5.919	0	13105652	N.D.	3.910 #
9)	A Endosulfan I	0.000	6.279	0	37834676	N.D.	12.104 #
12)	B 4,4'-DDE	0.000	6.381	0	3266978	N.D.	1.000 #
14)	MA Endrin	0.000	6.754	0	8685290	N.D.	3.128 #
15)	B Endosulfa...	0.000	6.979f	0	9329650	N.D.	3.144 #
16)	A 4,4'-DDD	0.000	6.899f	0	6229381	N.D.	2.540 #
17)	MA 4,4'-DDT	0.000	7.150f	0	310998	N.D.	0.119 #
18)	B Endrin al...	0.000	7.072f	0	7045072	N.D.	2.872 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
Data File : PL052978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2019 09:19
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:08:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

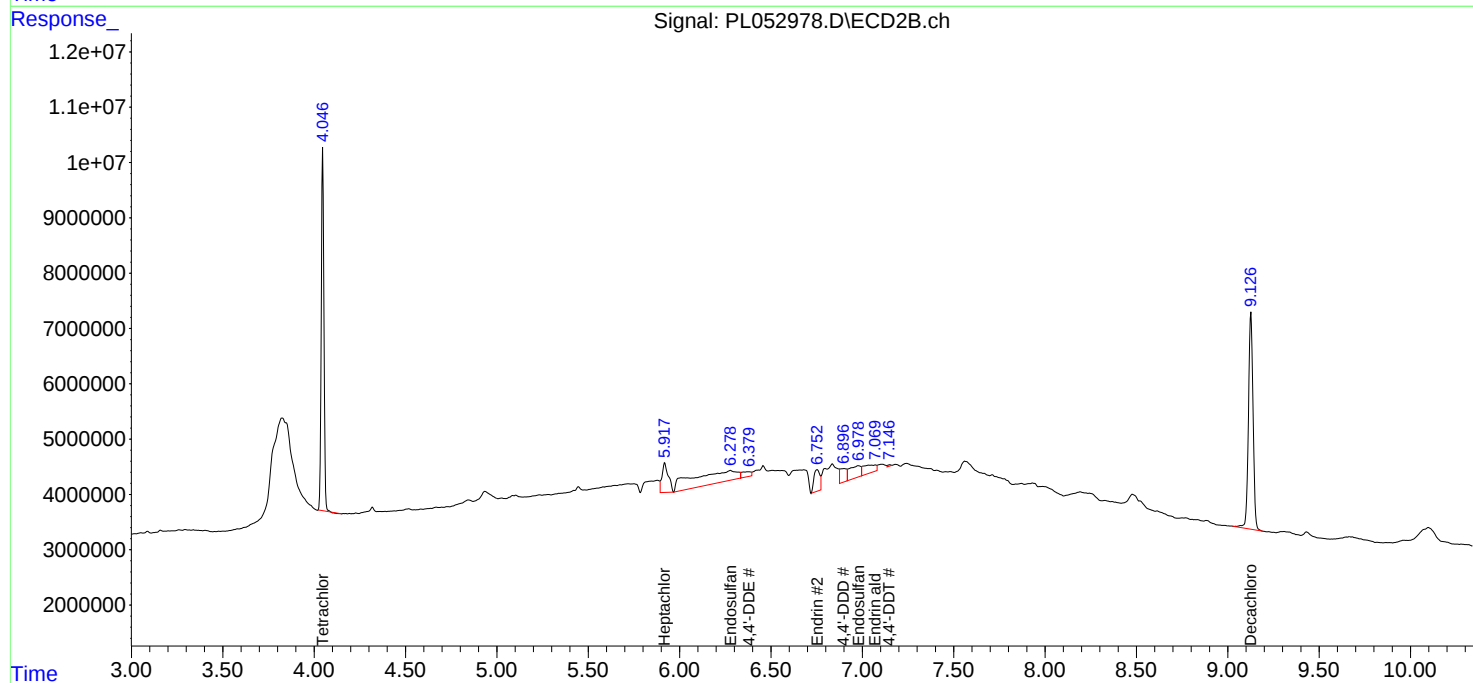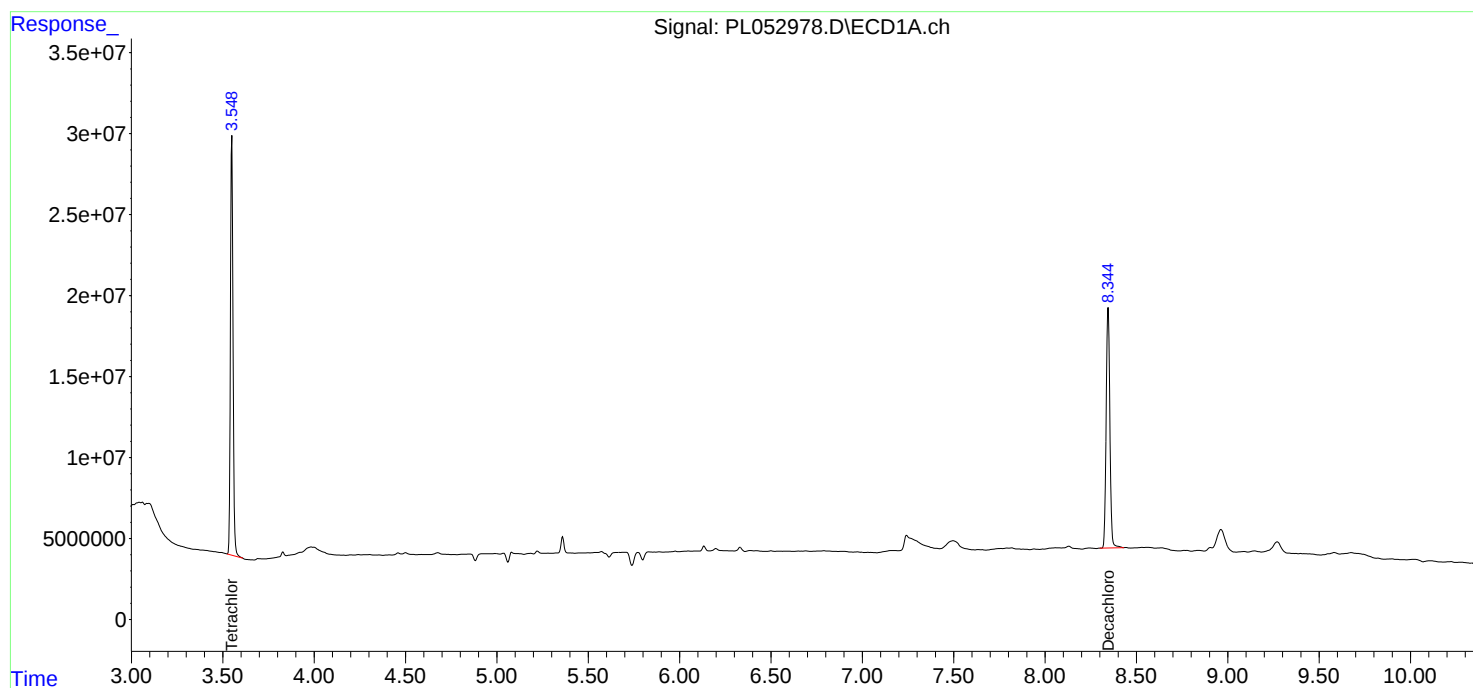


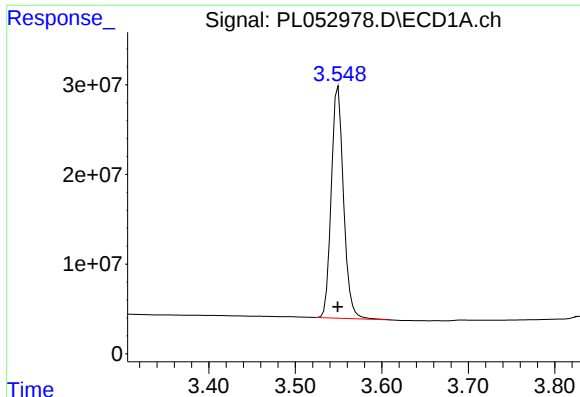

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 253996298
Conc: 25.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

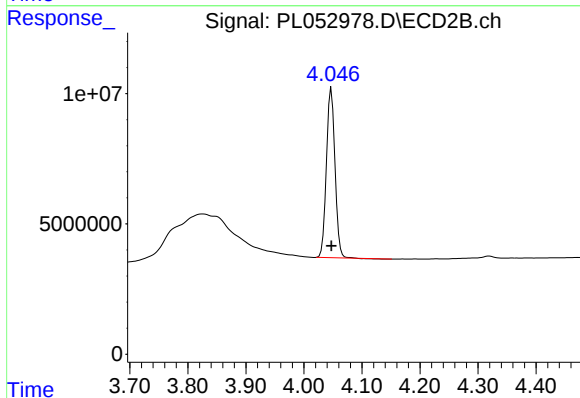


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 66010001
Conc: 24.58 ng/ml

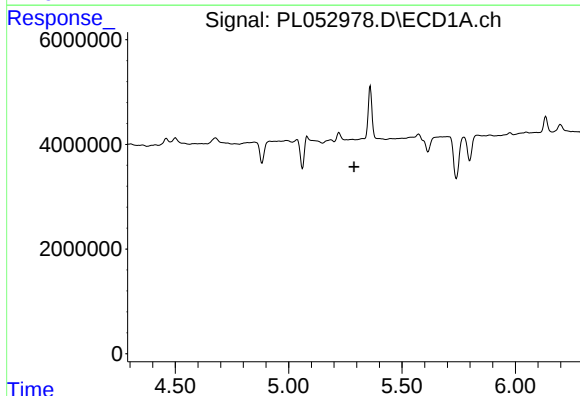


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.289 min
Response: 0
Conc: N.D.

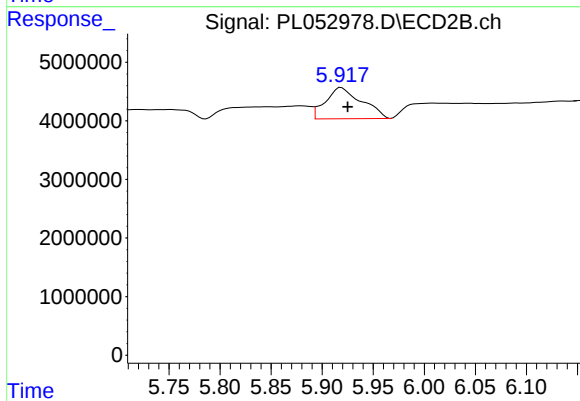

#8 Heptachlor epoxide


R.T.: 5.919 min
Delta R.T.: -0.006 min
Response: 13105652
Conc: 3.91 ng/ml

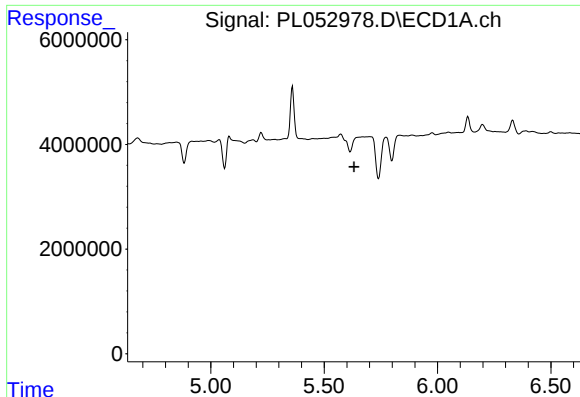

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.632 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

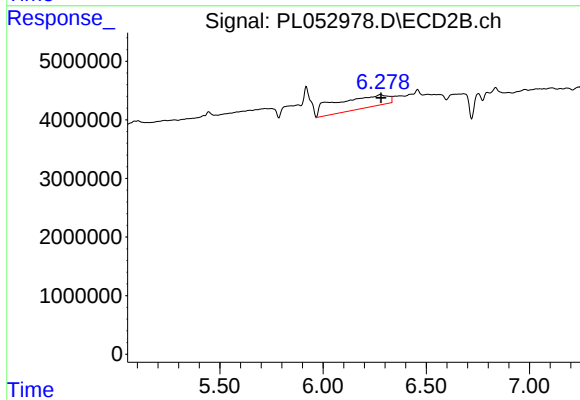


#9 Endosulfan I

R.T.: 6.279 min
Delta R.T.: -0.002 min
Response: 37834676
Conc: 12.10 ng/ml

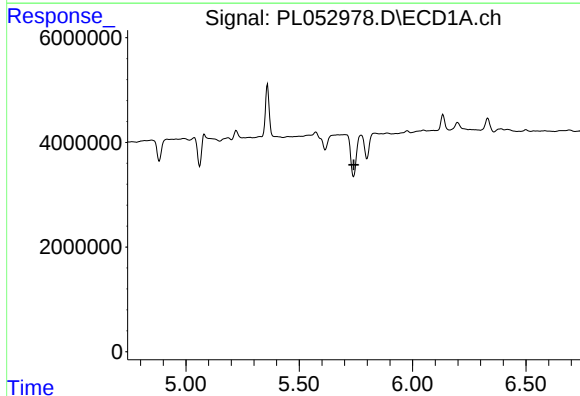


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

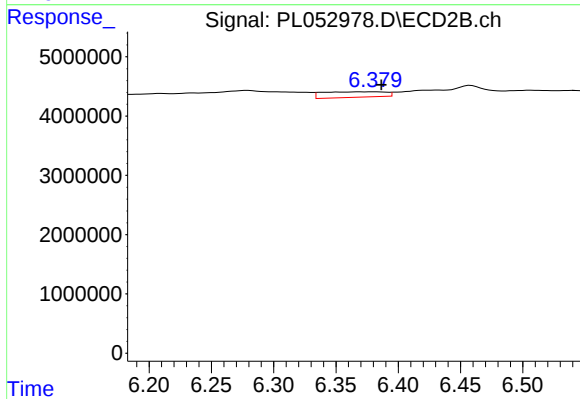

#12 4,4'-DDE


R.T.: 6.381 min
Delta R.T.: -0.005 min
Response: 3266978
Conc: 1.00 ng/ml

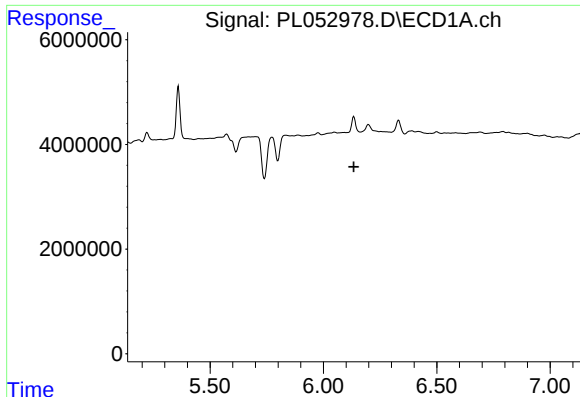

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

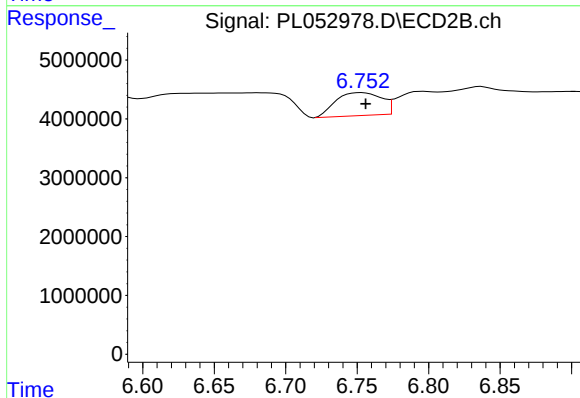


#14 Endrin

R.T.: 6.754 min
Delta R.T.: -0.002 min
Response: 8685290
Conc: 3.13 ng/ml

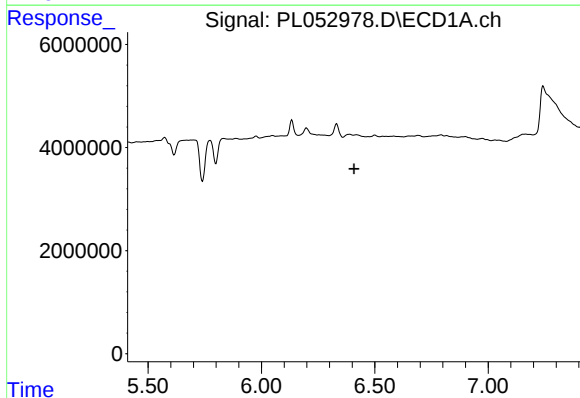


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

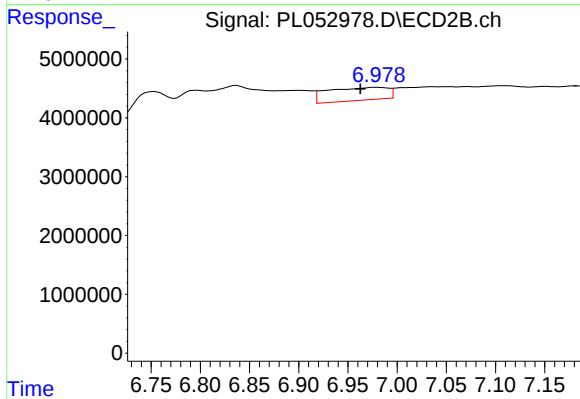

#15 Endosulfan II


R.T.: 6.979 min
Delta R.T.: 0.017 min
Response: 9329650
Conc: 3.14 ng/ml

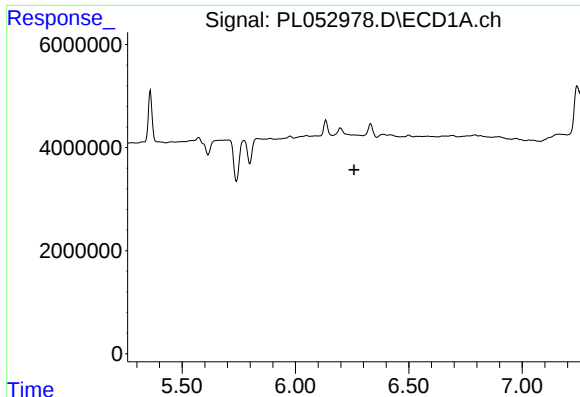

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

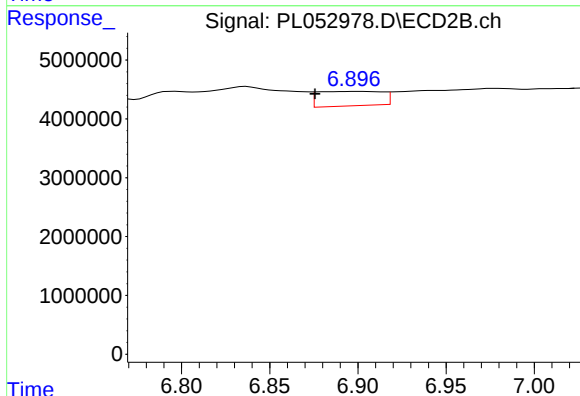


#16 4,4'-DDD

R.T.: 6.899 min
Delta R.T.: 0.023 min
Response: 6229381
Conc: 2.54 ng/ml

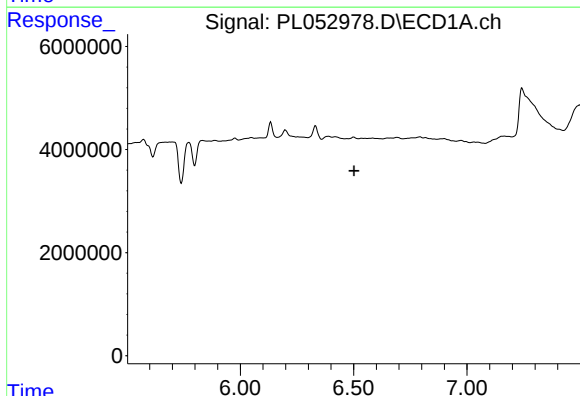


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.502 min
Response: 0
Conc: N.D.

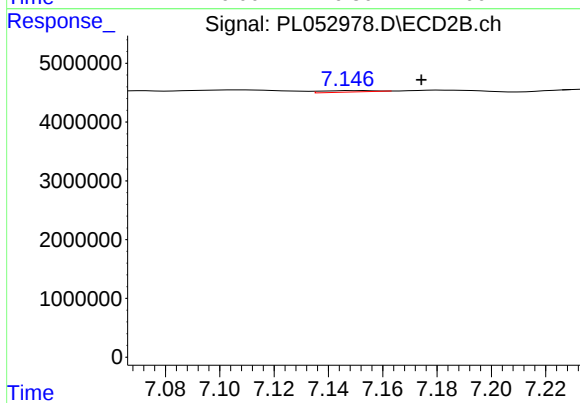

#17 4,4'-DDT


R.T.: 7.150 min
Delta R.T.: -0.024 min
Response: 310998
Conc: 0.12 ng/ml

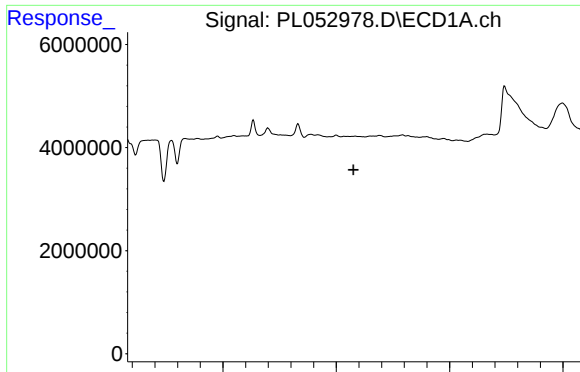

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

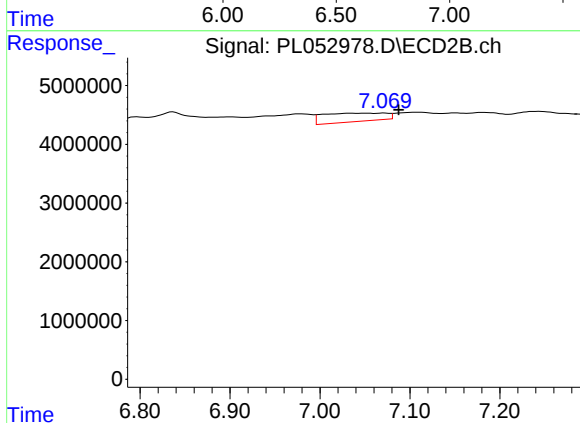


#18 Endrin aldehyde

R.T.: 7.072 min
Delta R.T.: -0.016 min
Response: 7045072
Conc: 2.87 ng/ml

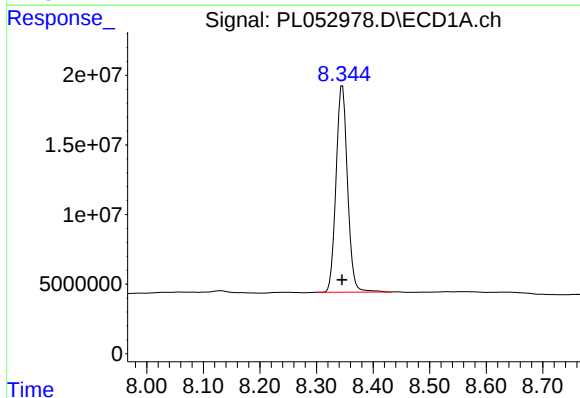

#28 Decachlorobiphenyl

R.T.: 8.346 min
Delta R.T.: 0.000 min
Response: 209700332
Conc: 20.94 ng/ml

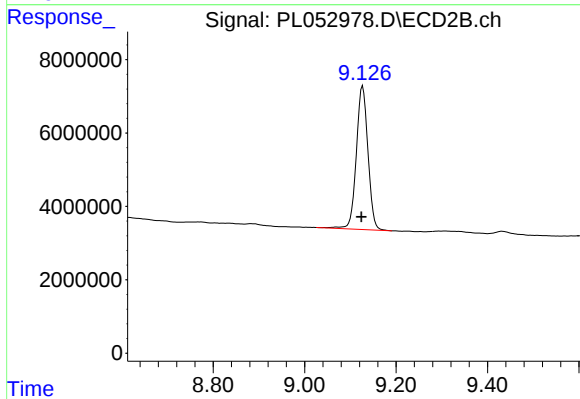

#28 Decachlorobiphenyl

R.T.: 9.127 min
Delta R.T.: 0.003 min
Response: 68929951
Conc: 23.50 ng/ml