

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
 Data File : PL052989.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2019 14:48
 Operator : SG\AJ
 Sample : K5127-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:10:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	4.047	177.4E6	48919889	17.834	18.218
28)	SA Decachlor...	8.345	9.126	139.1E6	45210165	13.883	15.411
Target Compounds							
3)	MA gamma-BHC...	0.000	4.721	0	972736	N.D.	0.269 #
5)	MB Aldrin	0.000	5.562f	0	77147246	N.D.	22.261 #
6)	B beta-BHC	4.504f	4.879	13740116	2650539	2.213	1.686
7)	B delta-BHC	0.000	5.120	0	20446544	N.D.	5.648 #
8)	B Heptachlo...	0.000	5.940	0	19348250	N.D.	5.773 #
15)	B Endosulfa...	0.000	6.971	0	3040136	N.D.	1.025 #
21)	B Endrin ke...	0.000	7.774	0	5807842	N.D.	2.036 #
23)	Chlordane-1	0.000	5.036	0	6936747	N.D.	68.390 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
Data File : PL052989.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2019 14:48
Operator : SG\AJ
Sample : K5127-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:10:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

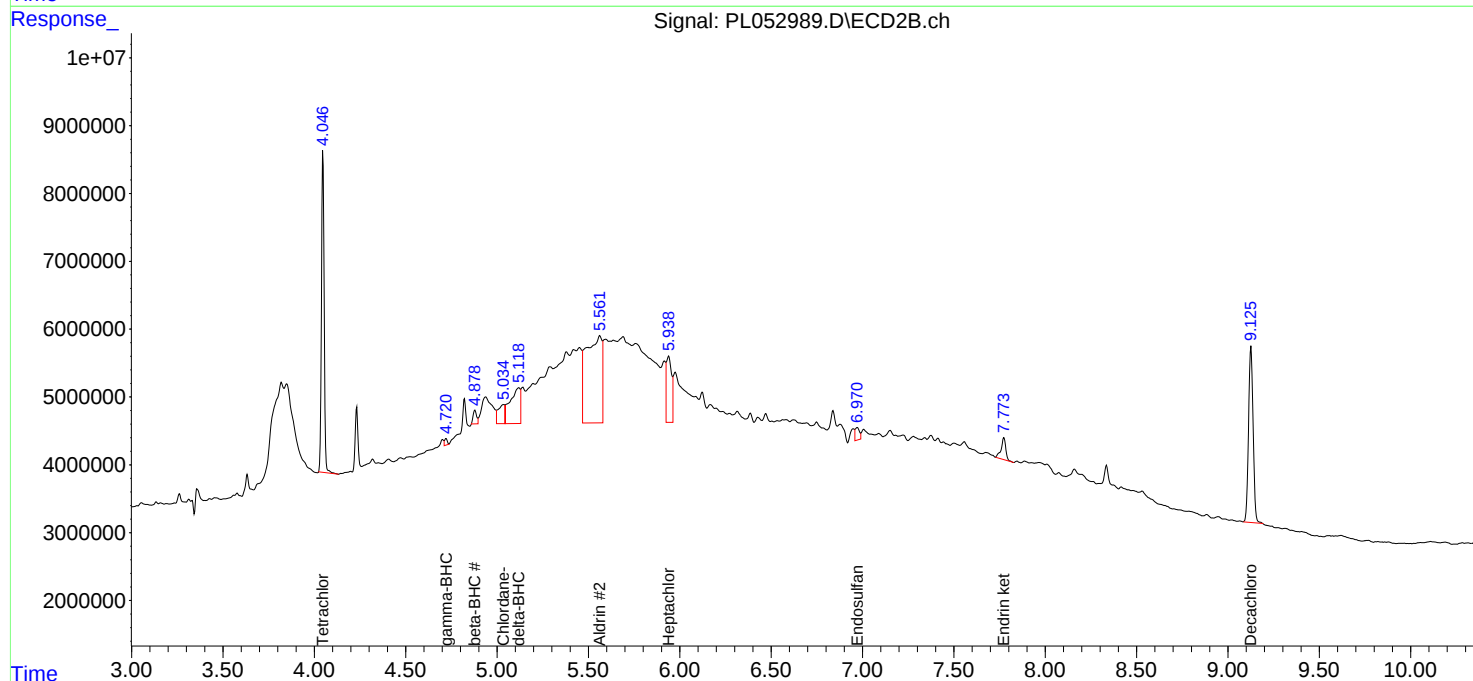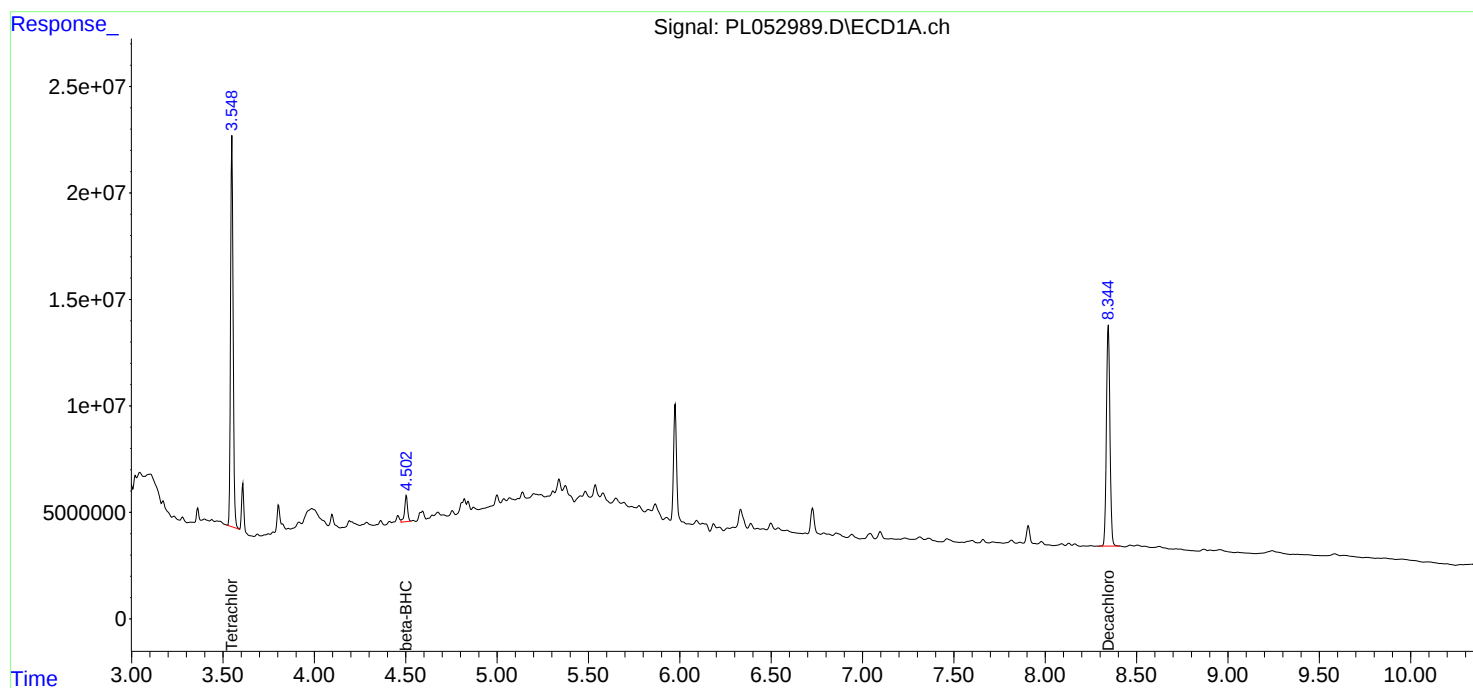


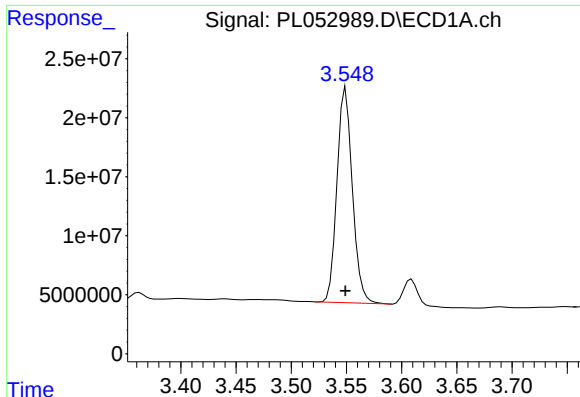

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 177393329
Conc: 17.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

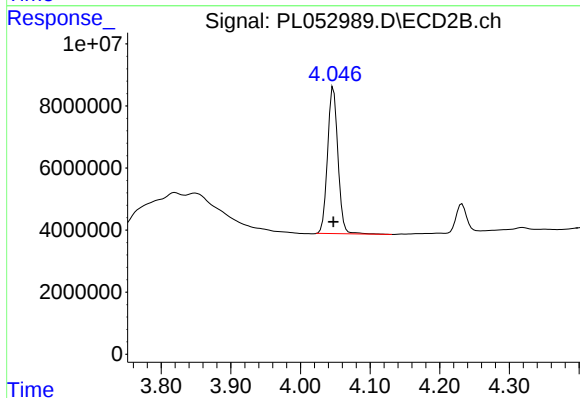


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 48919889
Conc: 18.22 ng/ml

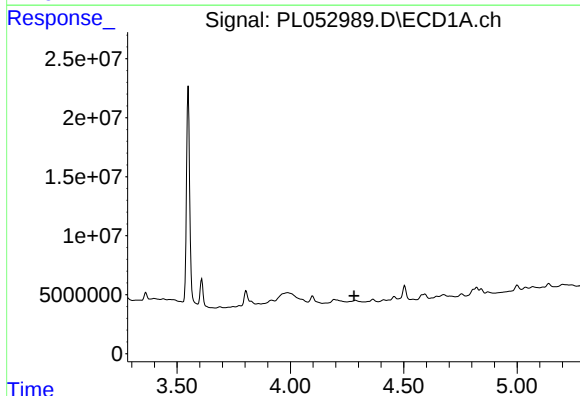


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.281 min
Response: 0
Conc: N.D.

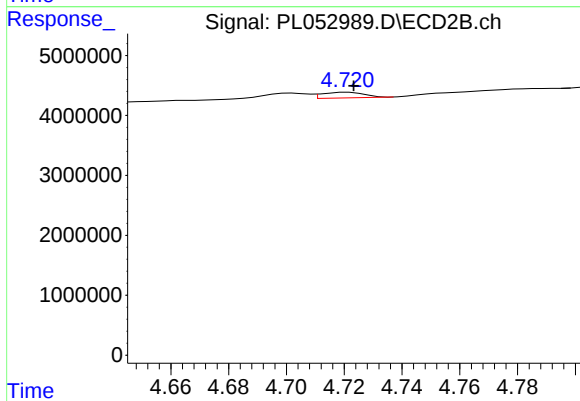

#3 gamma-BHC (Lindane)


R.T.: 4.721 min
Delta R.T.: -0.002 min
Response: 972736
Conc: 0.27 ng/ml

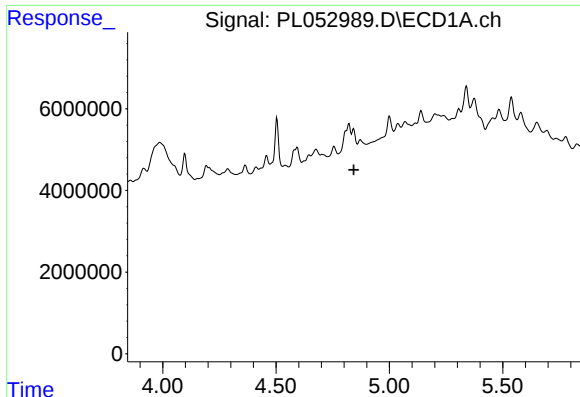

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.843 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

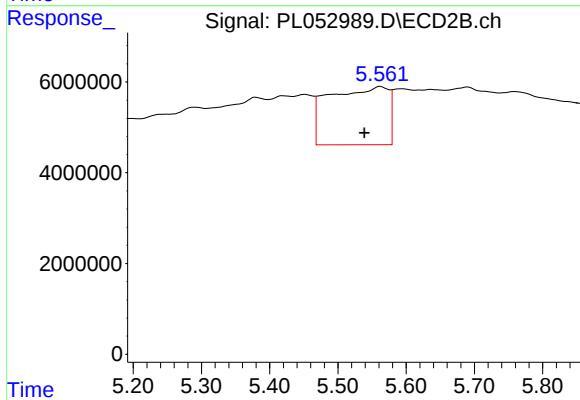


#5 Aldrin

R.T.: 5.562 min
Delta R.T.: 0.023 min
Response: 77147246
Conc: 22.26 ng/ml

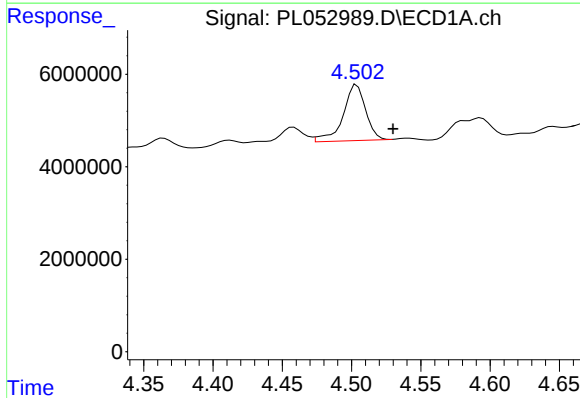


#6 beta-BHC

R.T.: 4.504 min
Delta R.T.: -0.026 min
Response: 13740116
Conc: 2.21 ng/ml

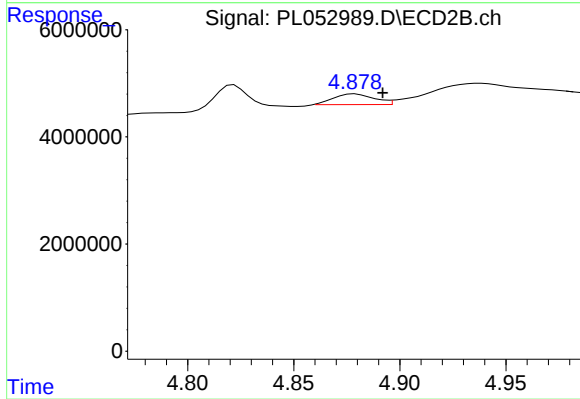

#6 beta-BHC


R.T.: 4.879 min
Delta R.T.: -0.013 min
Response: 2650539
Conc: 1.69 ng/ml

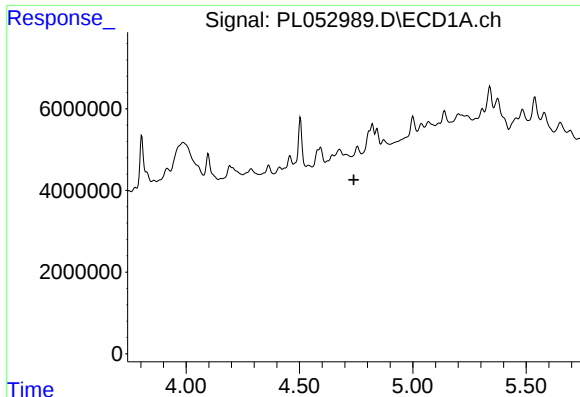

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

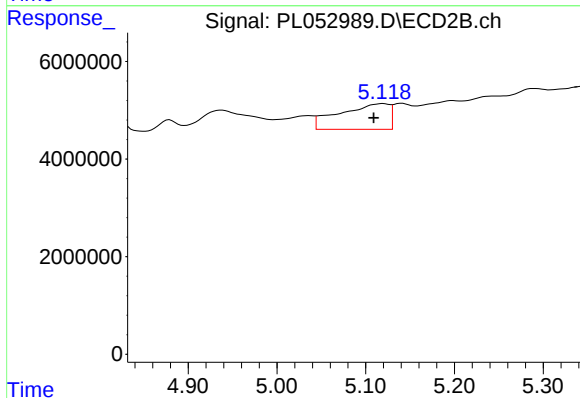


#7 delta-BHC

R.T.: 5.120 min
Delta R.T.: 0.010 min
Response: 20446544
Conc: 5.65 ng/ml

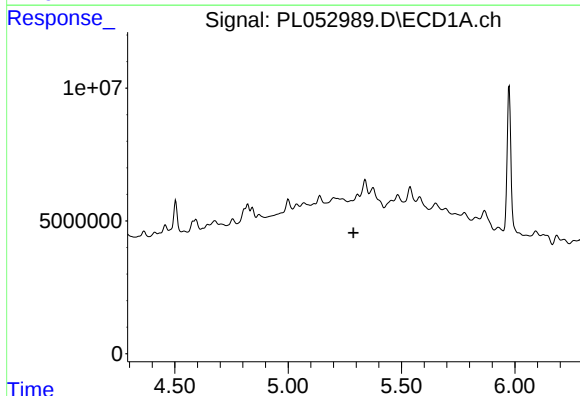


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

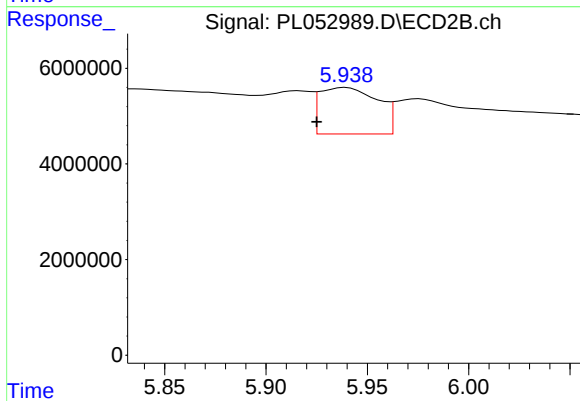

#8 Heptachlor epoxide


R.T.: 5.940 min
Delta R.T.: 0.015 min
Response: 19348250
Conc: 5.77 ng/ml

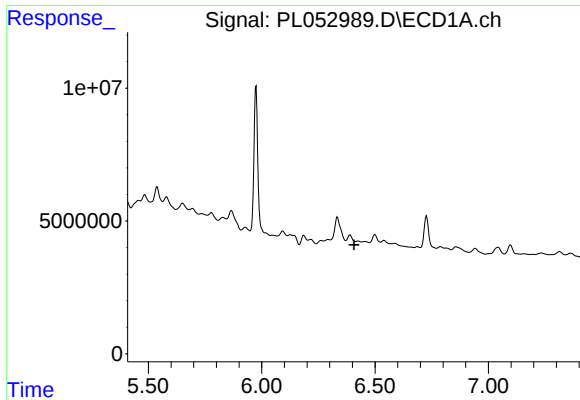

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

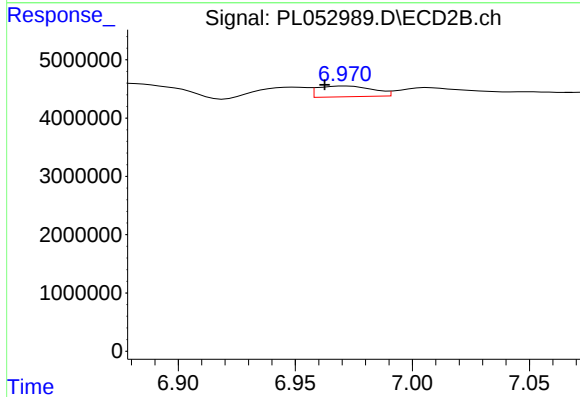


#15 Endosulfan II

R.T.: 6.971 min
Delta R.T.: 0.009 min
Response: 3040136
Conc: 1.02 ng/ml

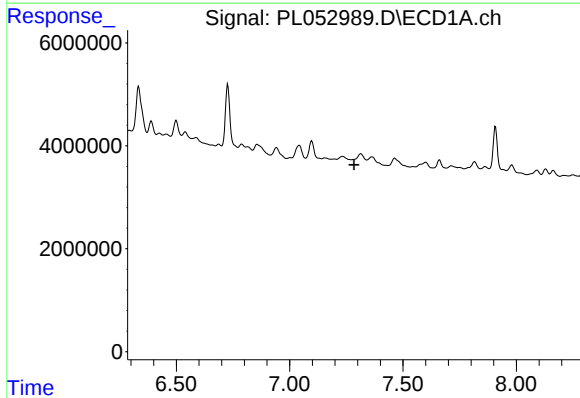


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

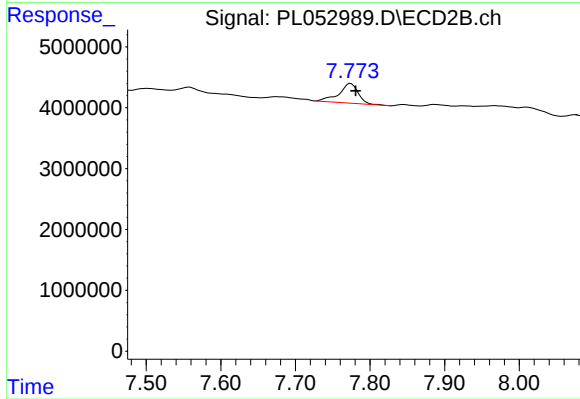

#21 Endrin ketone


R.T.: 7.774 min
Delta R.T.: -0.007 min
Response: 5807842
Conc: 2.04 ng/ml

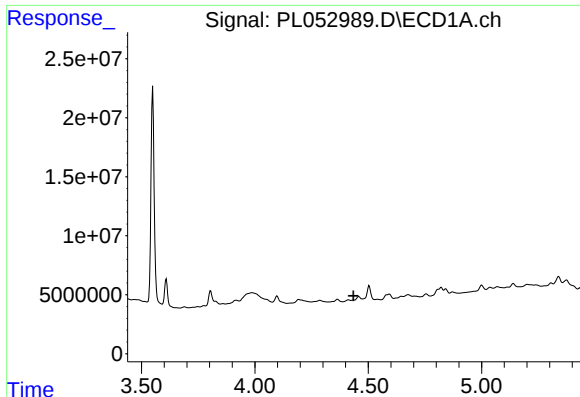

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

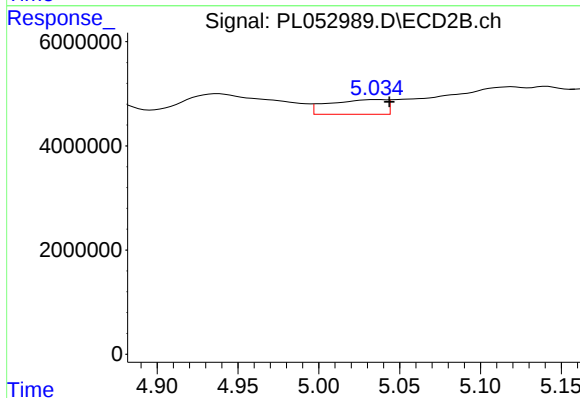


#23 Chlordane-1

R.T.: 5.036 min
Delta R.T.: -0.008 min
Response: 6936747
Conc: 68.39 ng/ml

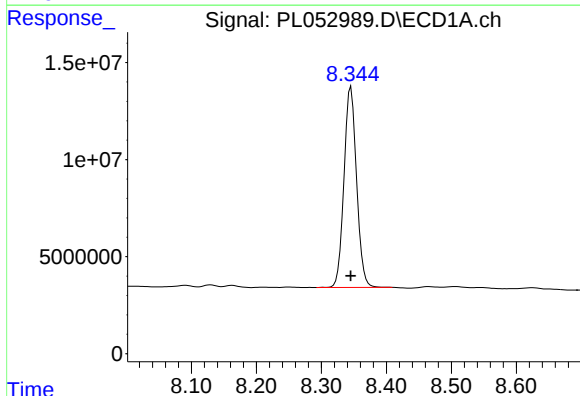

#28 Decachlorobiphenyl

R.T.: 8.345 min
Delta R.T.: 0.000 min
Response: 139053579
Conc: 13.88 ng/ml

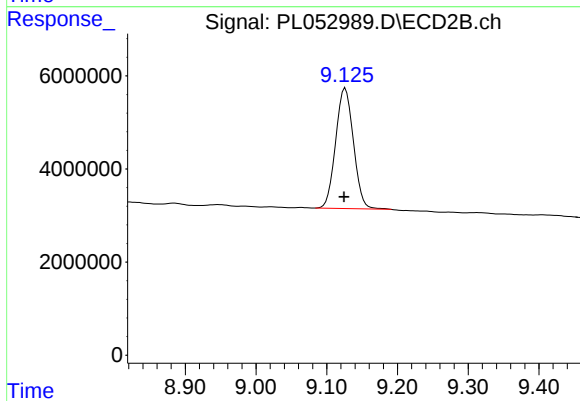

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.002 min
Response: 45210165
Conc: 15.41 ng/ml