

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
 Data File : PL052990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2019 15:03
 Operator : SG\AJ
 Sample : K5127-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20190762-SS-COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:10:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	4.048	196.3E6	54442435	19.740	20.275
28)	SA Decachlor...	8.345	9.127	153.7E6	51138530	15.344	17.431
Target Compounds							
3)	MA gamma-BHC...	0.000	4.721	0	812906	N.D.	0.224 #
4)	MA Heptachlor	0.000	5.237	0	2828424	N.D.	0.742 #
5)	MB Aldrin	0.000	5.562f	0	26549446	N.D.	7.661 #
6)	B beta-BHC	0.000	4.879	0	1519175	N.D.	0.967 #
7)	B delta-BHC	0.000	5.108	0	1962347	N.D.	0.542 #
8)	B Heptachlo...	0.000	5.938	0	15605238	N.D.	4.656 #
15)	B Endosulfa...	0.000	6.974	0	5636390	N.D.	1.900 #
21)	B Endrin ke...	0.000	7.773	0	3758649	N.D.	1.317 #
24)	Chlordane-2	0.000	5.494f	0	9327329	N.D.	83.338 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
Data File : PL052990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2019 15:03
Operator : SG\AJ
Sample : K5127-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20190762-SS-COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:10:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

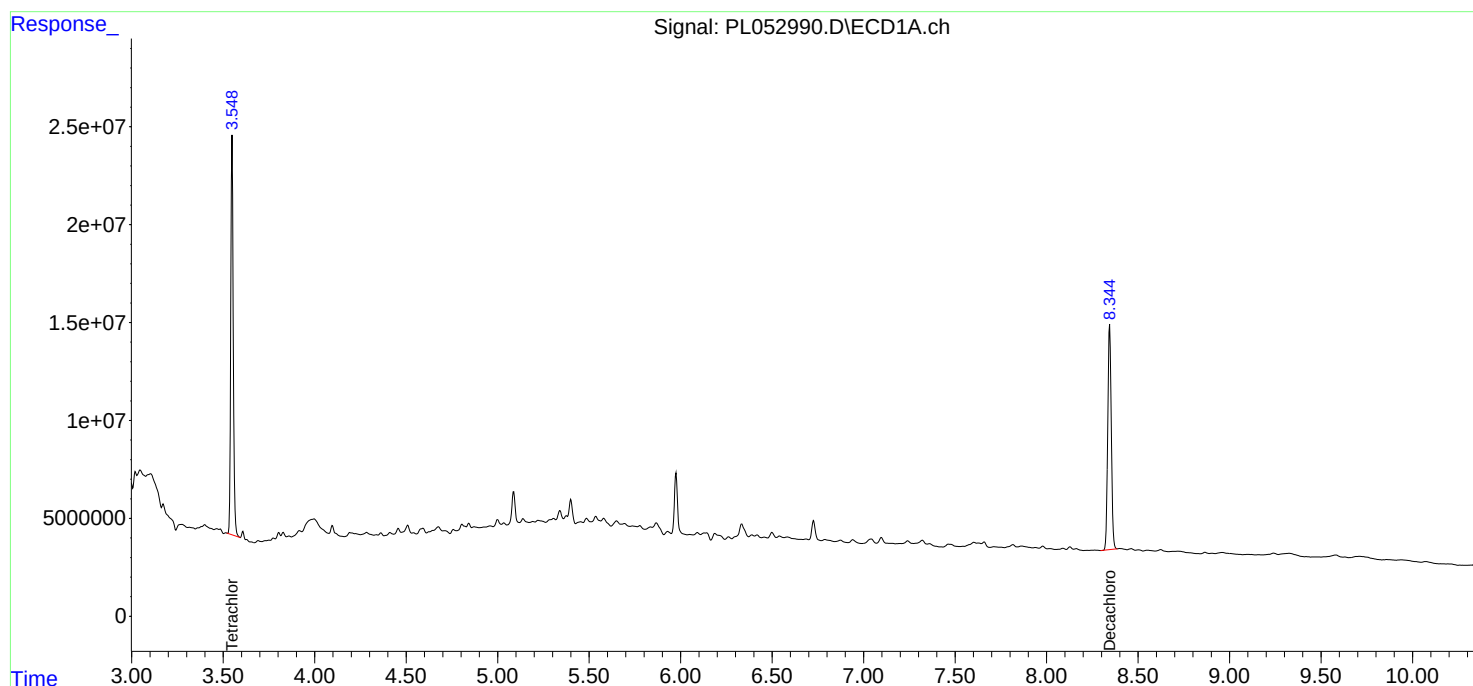


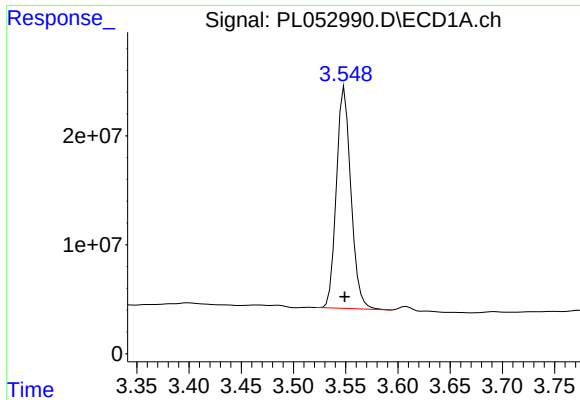

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 196349226
Conc: 19.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190762-SS-COMP-2

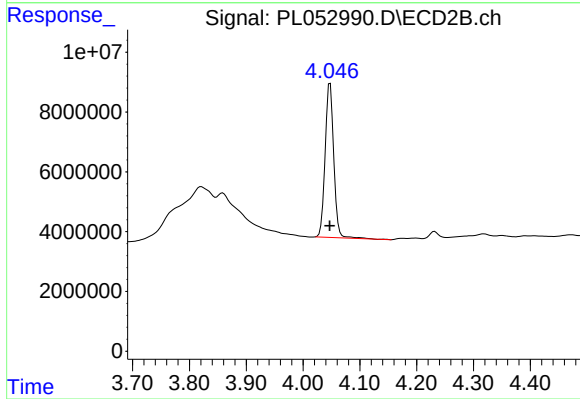


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 54442435
Conc: 20.27 ng/ml

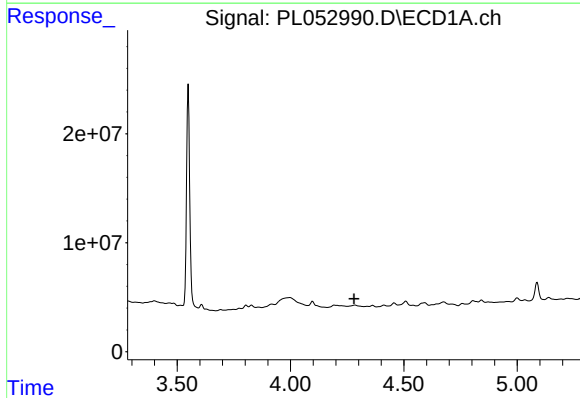


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.281 min
Response: 0
Conc: N.D.

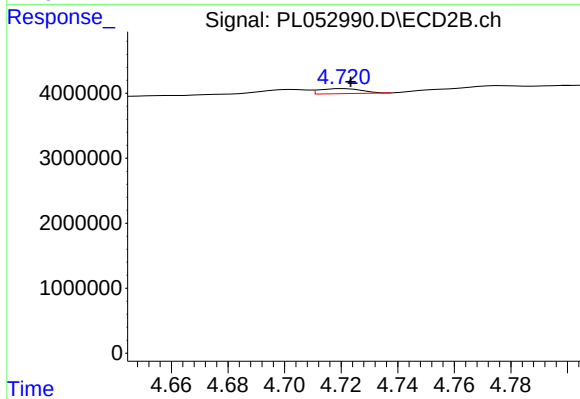

#3 gamma-BHC (Lindane)


R.T.: 4.721 min
Delta R.T.: -0.002 min
Response: 812906
Conc: 0.22 ng/ml

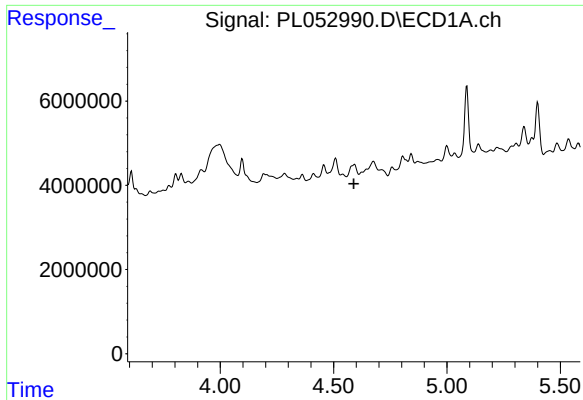

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.590 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20190762-SS-COMP-2

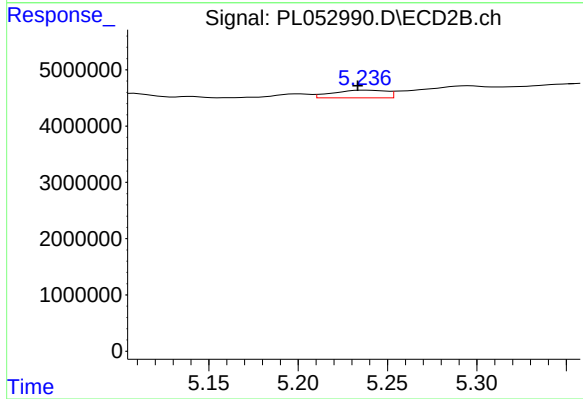


#4 Heptachlor

R.T.: 5.237 min
Delta R.T.: 0.004 min
Response: 2828424
Conc: 0.74 ng/ml

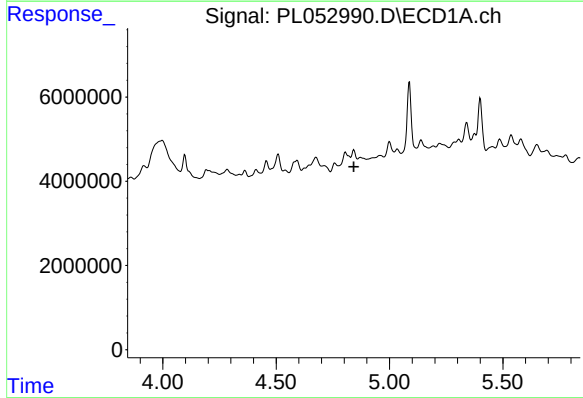


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 4.843 min
Response: 0
Conc: N.D.

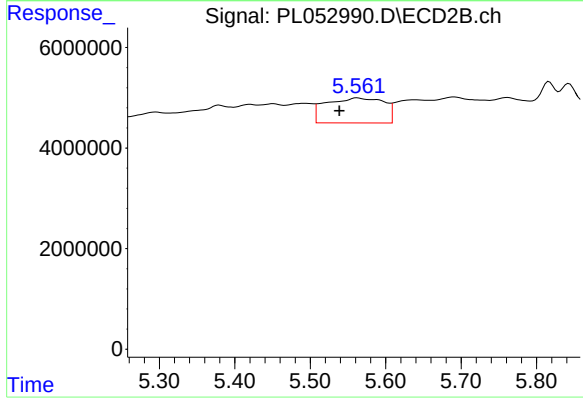

#5 Aldrin


R.T.: 5.562 min
Delta R.T.: 0.023 min
Response: 26549446
Conc: 7.66 ng/ml

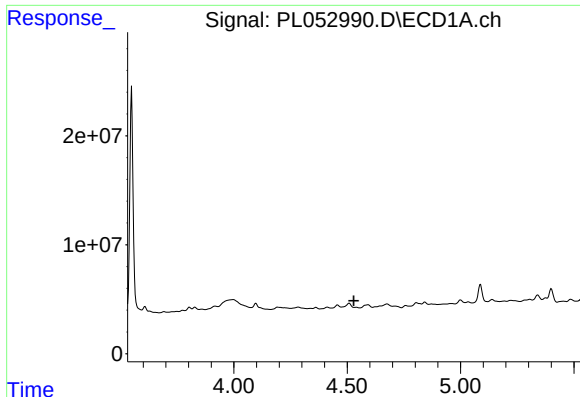

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20190762-SS-COMP-2

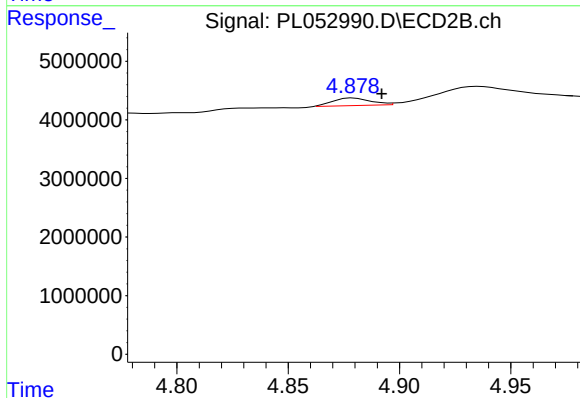


#6 beta-BHC

R.T.: 4.879 min
Delta R.T.: -0.013 min
Response: 1519175
Conc: 0.97 ng/ml

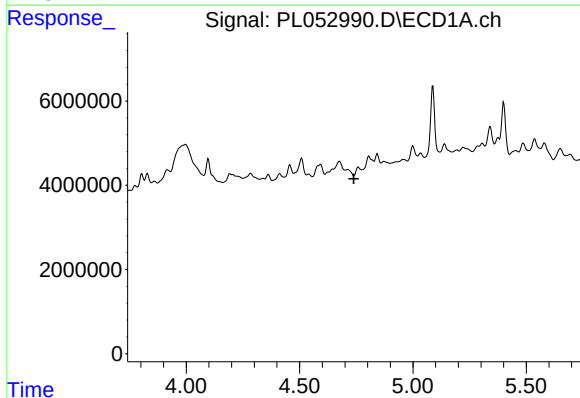


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.740 min
Response: 0
Conc: N.D.

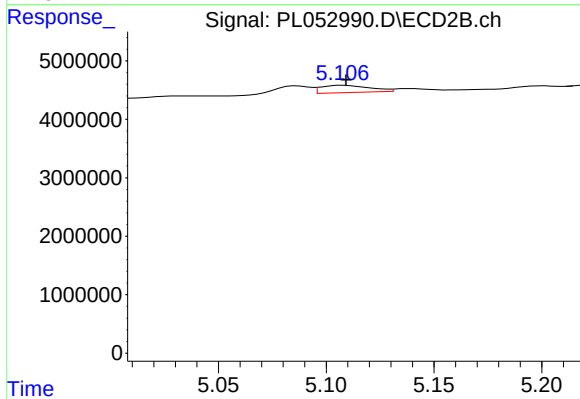

#7 delta-BHC


R.T.: 5.108 min
Delta R.T.: -0.001 min
Response: 1962347
Conc: 0.54 ng/ml

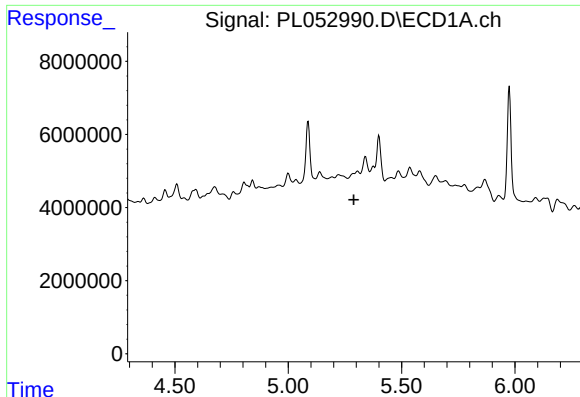

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20190762-SS-COMP-2

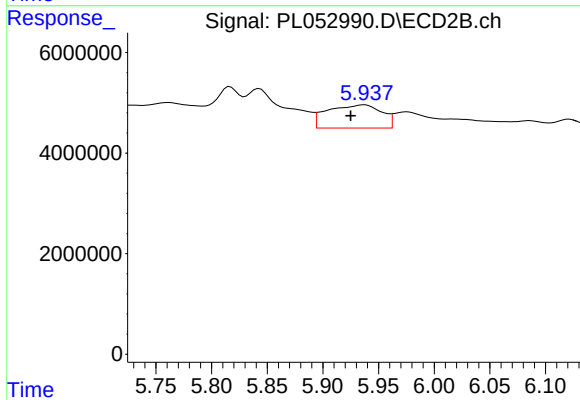


#8 Heptachlor epoxide

R.T.: 5.938 min
Delta R.T.: 0.013 min
Response: 15605238
Conc: 4.66 ng/ml

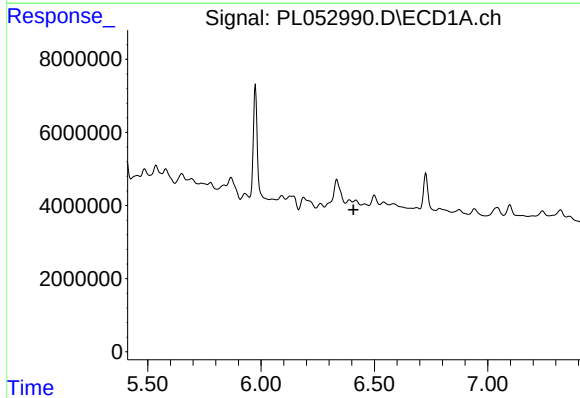


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

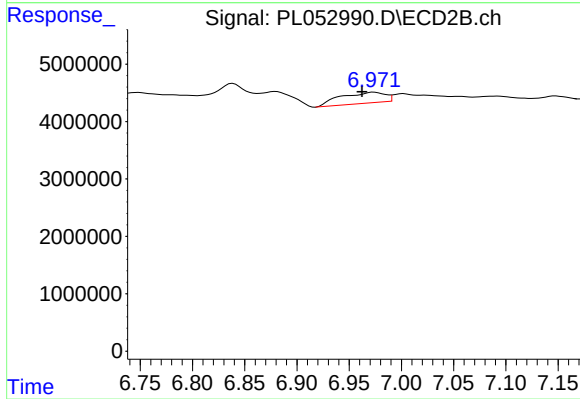

#15 Endosulfan II


R.T.: 6.974 min
Delta R.T.: 0.011 min
Response: 5636390
Conc: 1.90 ng/ml

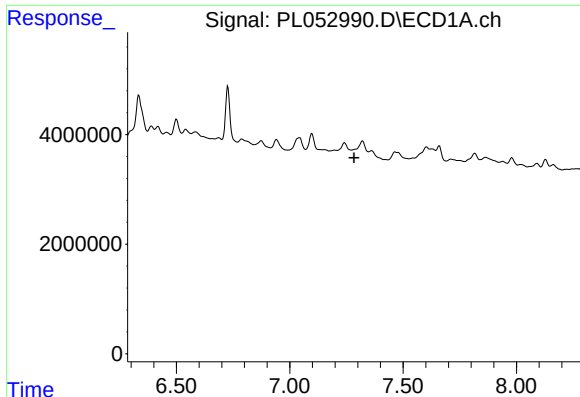

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20190762-SS-COMP-2

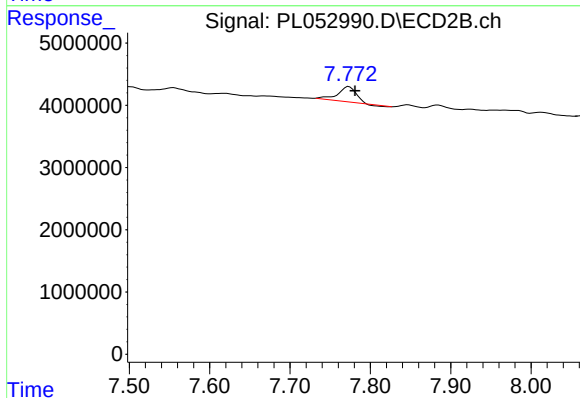


#21 Endrin ketone

R.T.: 7.773 min
Delta R.T.: -0.008 min
Response: 3758649
Conc: 1.32 ng/ml

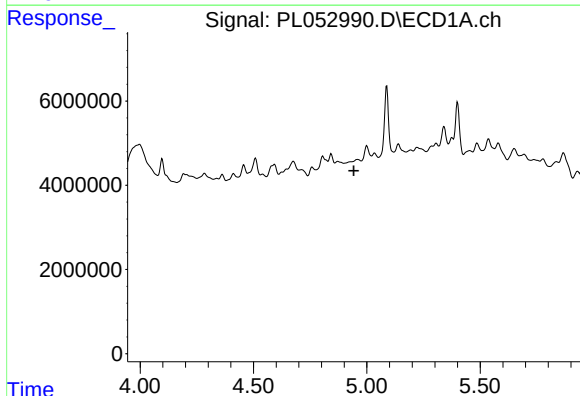


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

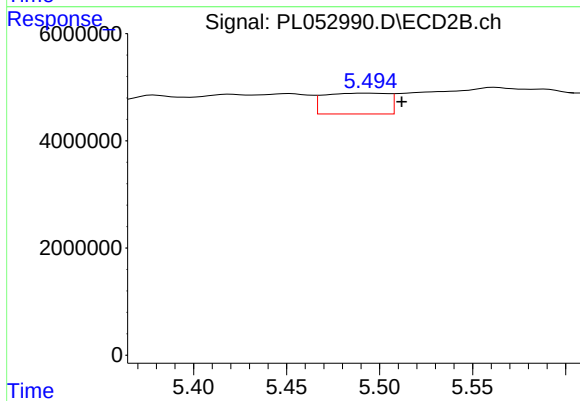

#24 Chlordane-2


R.T.: 5.494 min
Delta R.T.: -0.018 min
Response: 9327329
Conc: 83.34 ng/ml

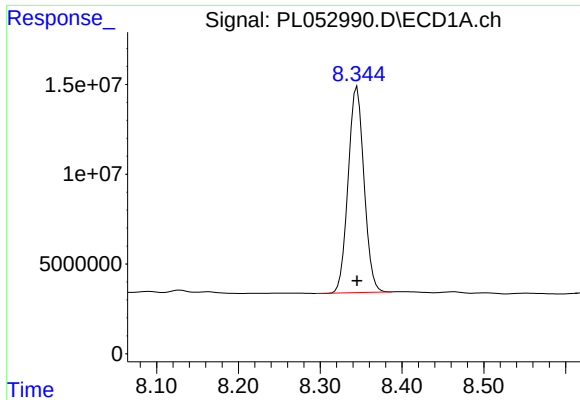

#28 Decachlorobiphenyl

R.T.: 8.345 min
Delta R.T.: 0.000 min
Response: 153683604
Conc: 15.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190762-SS-COMP-2

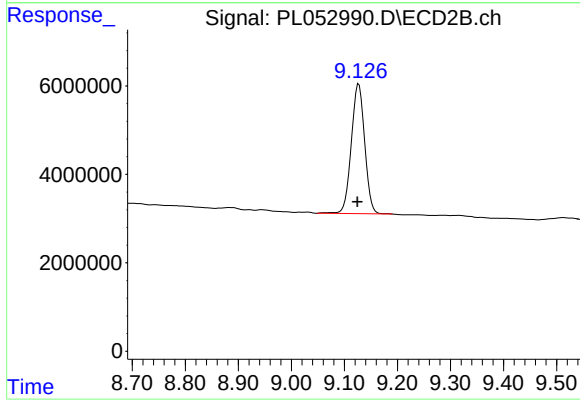

#28 Decachlorobiphenyl

R.T.: 9.127 min
Delta R.T.: 0.003 min
Response: 51138530
Conc: 17.43 ng/ml