

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
 Data File : PL052999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2019 17:22
 Operator : SG\AJ
 Sample : K5148-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-100119

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:12:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	4.047	187.8E6	51950033	18.878	19.347
28)	SA Decachlor...	8.344	9.126	157.0E6	52691056	15.670	17.960
Target Compounds							
7)	B delta-BHC	0.000	5.087f	0	8065842	N.D.	2.228 #
8)	B Heptachlo...	0.000	5.928	0	4018563	N.D.	1.199 #
10)	B gamma-Chl...	0.000	6.143	0	1871567	N.D.	0.553 #
13)	MA Dieldrin	0.000	6.567f	0	1661598	N.D.	0.509 #
15)	B Endosulfa...	0.000	6.964	0	5339137	N.D.	1.800 #
23)	Chlordane-1	0.000	5.014f	0	3034426	N.D.	29.917 #
25)	Chlordane-3	0.000	6.143	0	1871567	N.D.	4.297 #
27)	Chlordane-5	0.000	7.028	0	3331358	N.D.	37.766 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
Data File : PL052999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2019 17:22
Operator : SG\AJ
Sample : K5148-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-02-100119

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:12:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

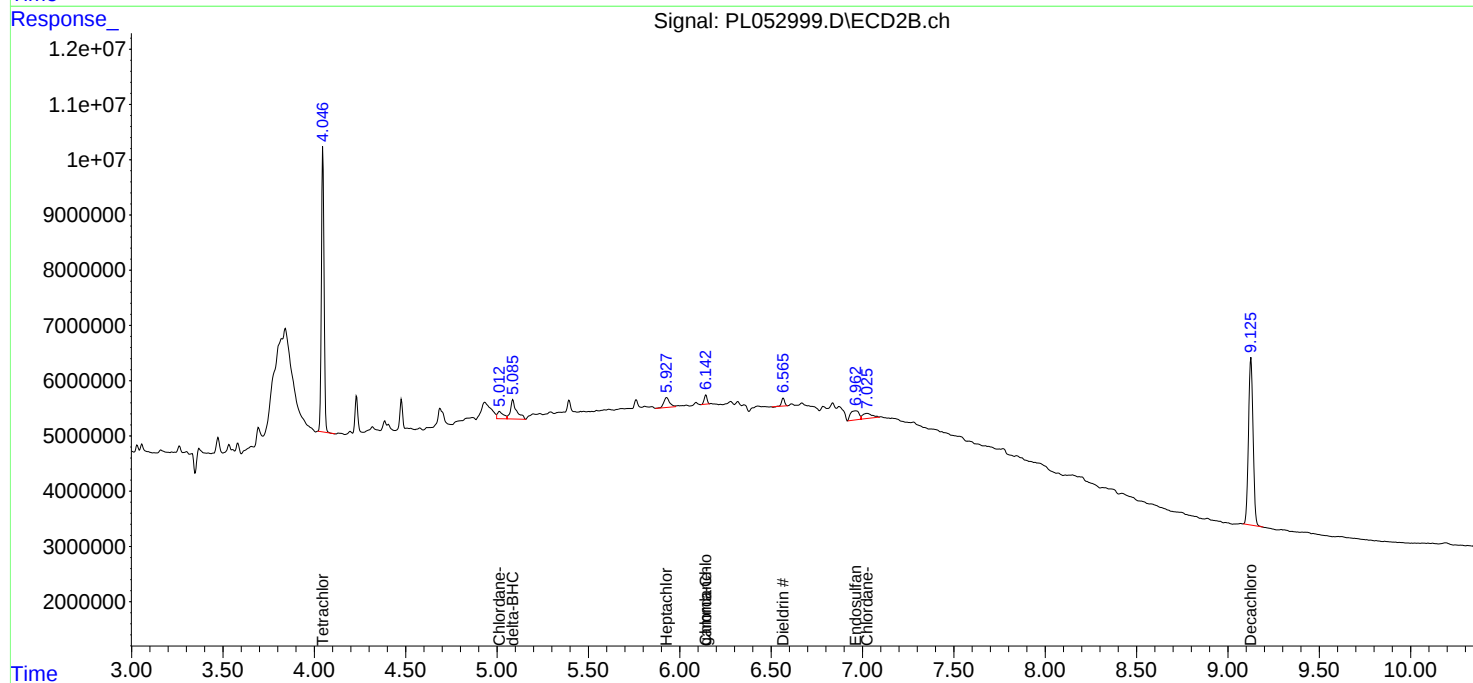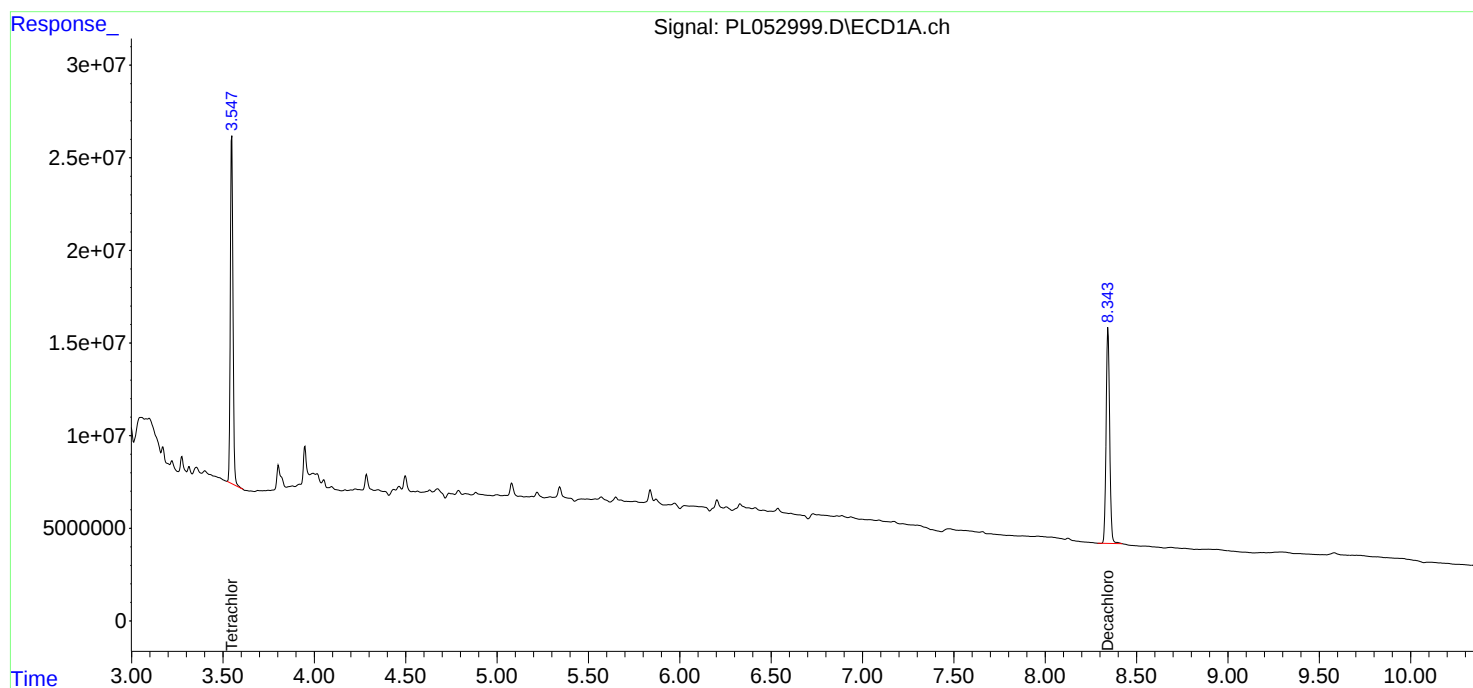


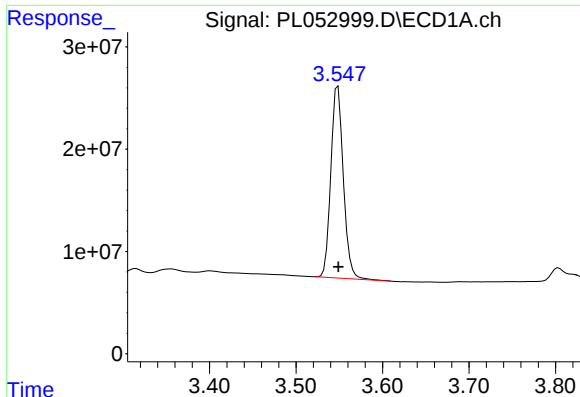

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 187778669
Conc: 18.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-100119

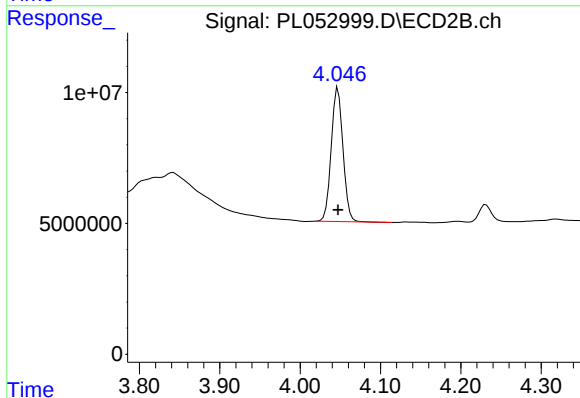


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 51950033
Conc: 19.35 ng/ml

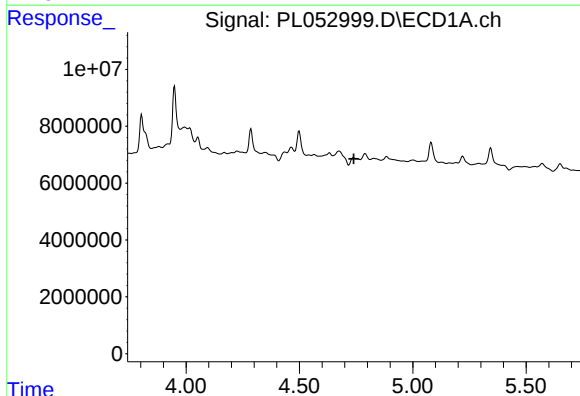


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.740 min
Response: 0
Conc: N.D.

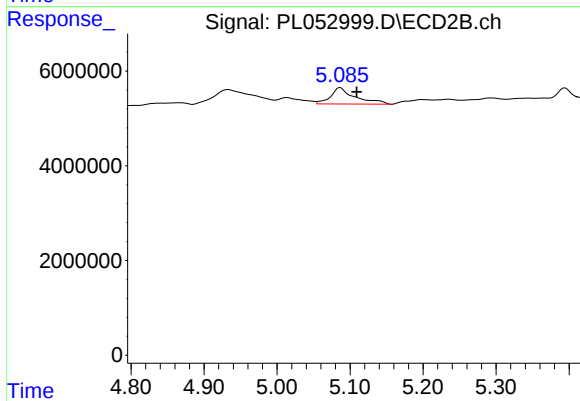

#7 delta-BHC


R.T.: 5.087 min
Delta R.T.: -0.022 min
Response: 8065842
Conc: 2.23 ng/ml

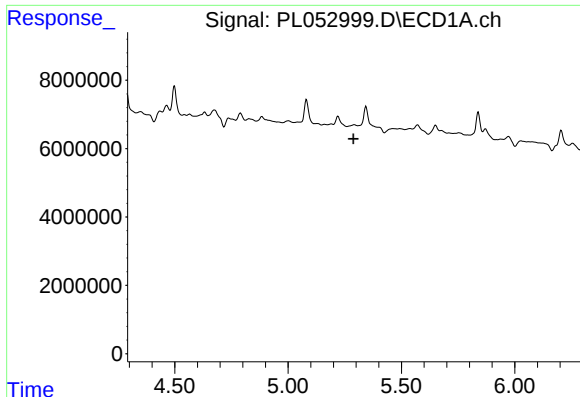

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-100119

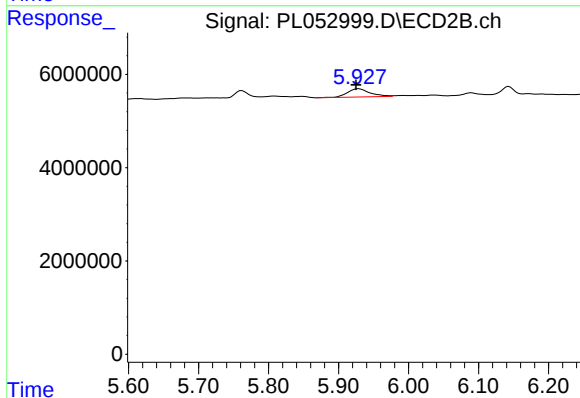


#8 Heptachlor epoxide

R.T.: 5.928 min
Delta R.T.: 0.003 min
Response: 4018563
Conc: 1.20 ng/ml

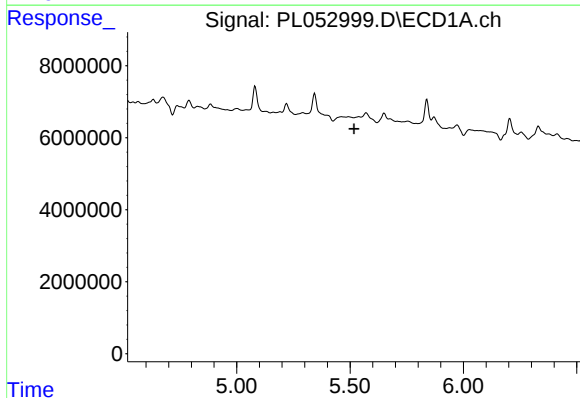


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

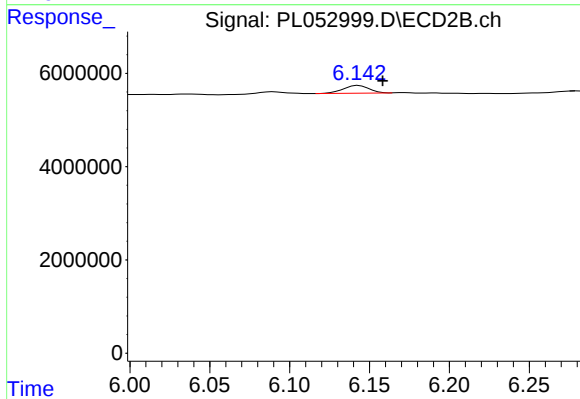

#10 gamma-Chlordane


R.T.: 6.143 min
Delta R.T.: -0.015 min
Response: 1871567
Conc: 0.55 ng/ml

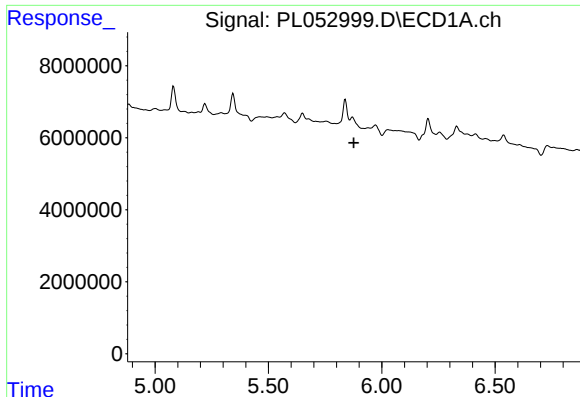

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.876 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-100119

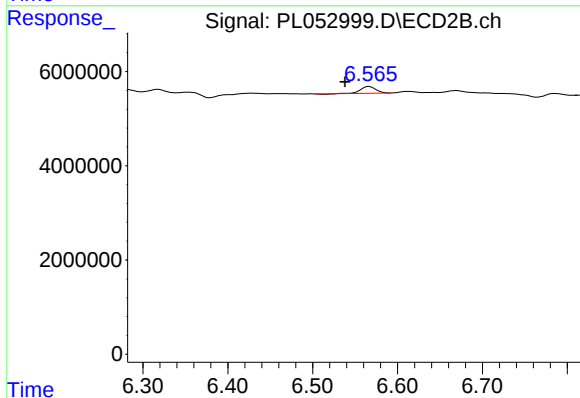


#13 Dieldrin

R.T.: 6.567 min
Delta R.T.: 0.029 min
Response: 1661598
Conc: 0.51 ng/ml

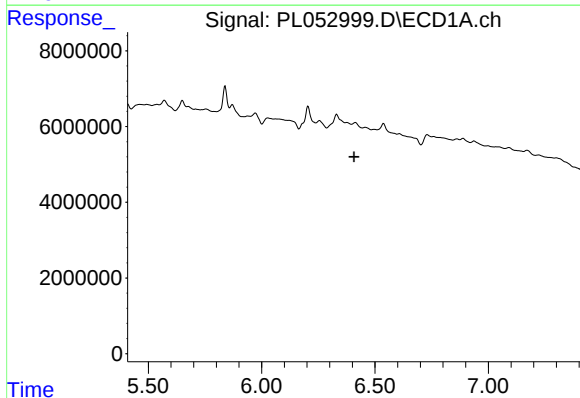


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

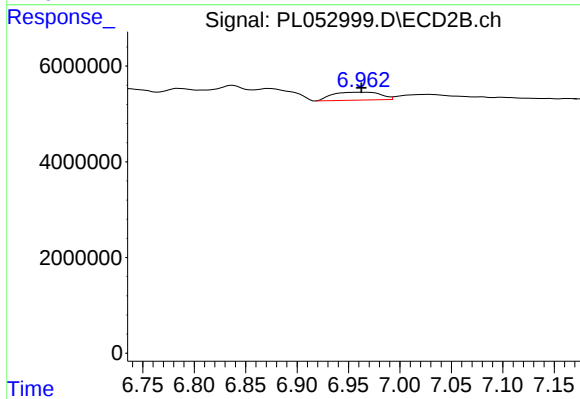

#15 Endosulfan II


R.T.: 6.964 min
Delta R.T.: 0.001 min
Response: 5339137
Conc: 1.80 ng/ml

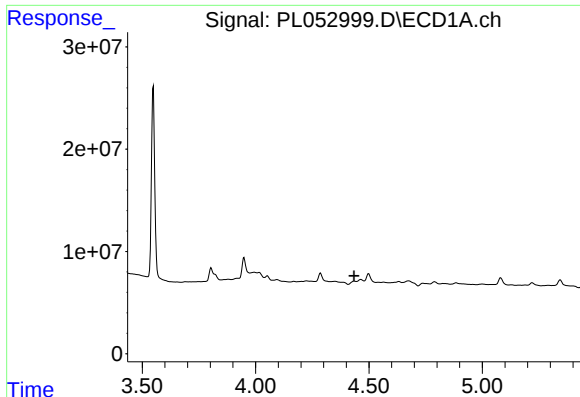

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-100119

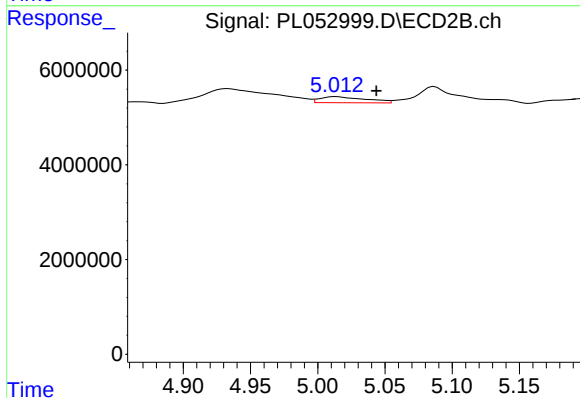


#23 Chlordane-1

R.T.: 5.014 min
Delta R.T.: -0.030 min
Response: 3034426
Conc: 29.92 ng/ml

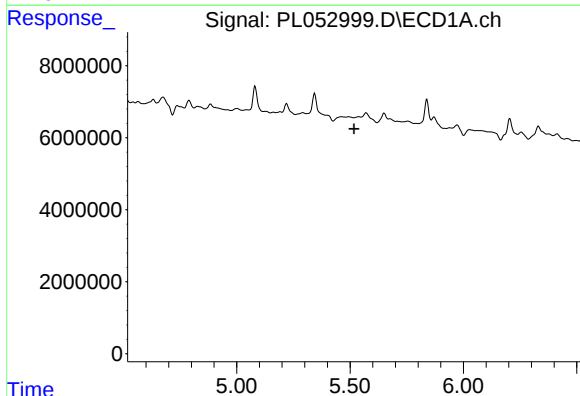


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.518 min
Response: 0
Conc: N.D.

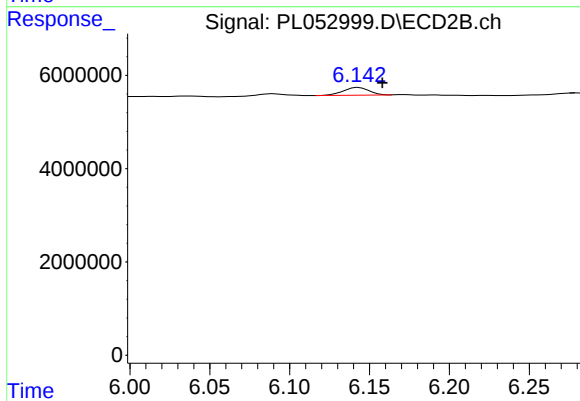

#25 Chlordane-3


R.T.: 6.143 min
Delta R.T.: -0.015 min
Response: 1871567
Conc: 4.30 ng/ml

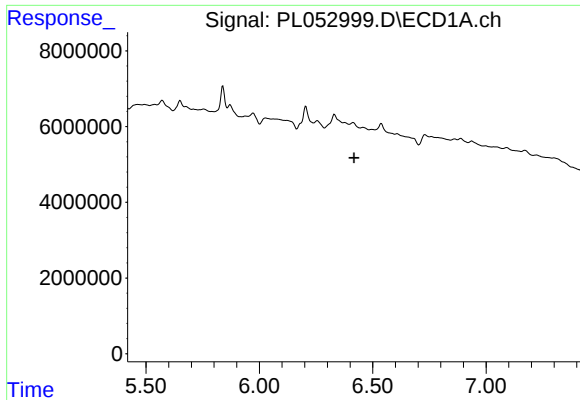

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-100119

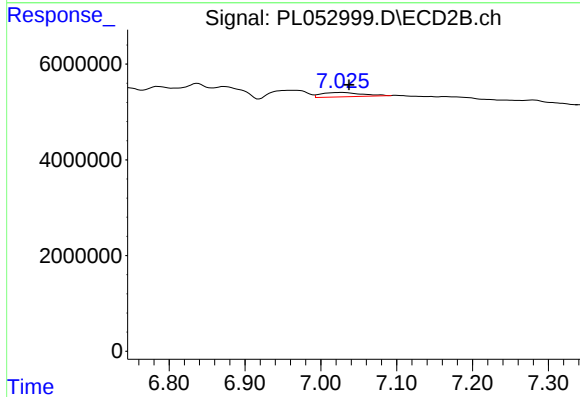


#27 Chlordane-5

R.T.: 7.028 min
Delta R.T.: -0.010 min
Response: 3331358
Conc: 37.77 ng/ml

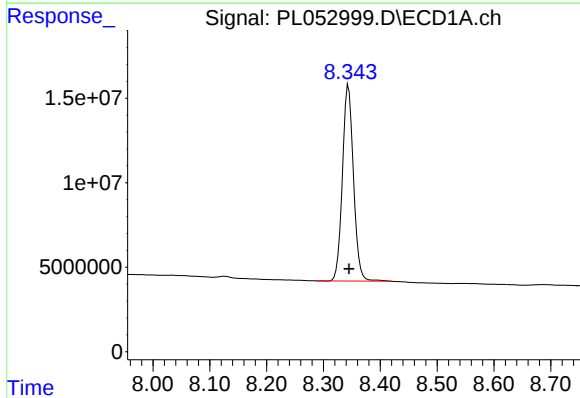

#28 Decachlorobiphenyl

R.T.: 8.344 min
Delta R.T.: -0.001 min
Response: 156951278
Conc: 15.67 ng/ml

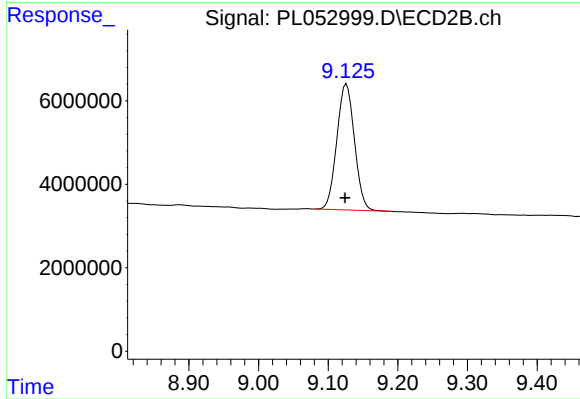

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.002 min
Response: 52691056
Conc: 17.96 ng/ml