

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
 Data File : PL053006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2019 19:01
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:13:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	4.047	244.4E6	66202271	24.575	24.654
28)	SA Decachlor...	8.343	9.127	218.7E6	70143951	21.836	23.910
Target Compounds							
5)	MB Aldrin	0.000	5.559f	0	7479517	N.D.	2.158 #
8)	B Heptachlo...	0.000	5.920	0	15427261	N.D.	4.603 #
9)	A Endosulfan I	0.000	6.279	0	35402797	N.D.	11.326 #
14)	MA Endrin	0.000	6.753	0	10714083	N.D.	3.858 #
15)	B Endosulfa...	0.000	6.975	0	9774553	N.D.	3.294 #
27)	Chlordane-5	0.000	7.034	0	5465772	N.D.	61.964 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
Data File : PL053006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2019 19:01
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:13:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

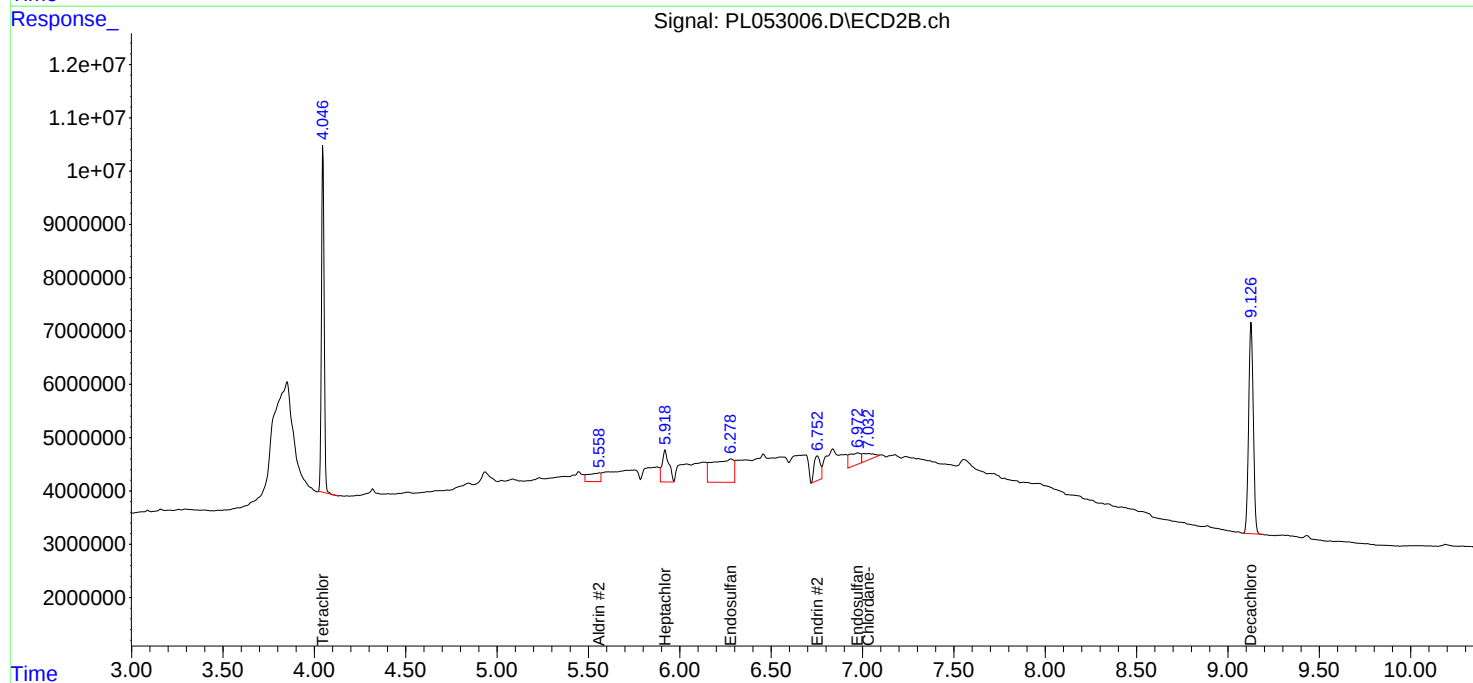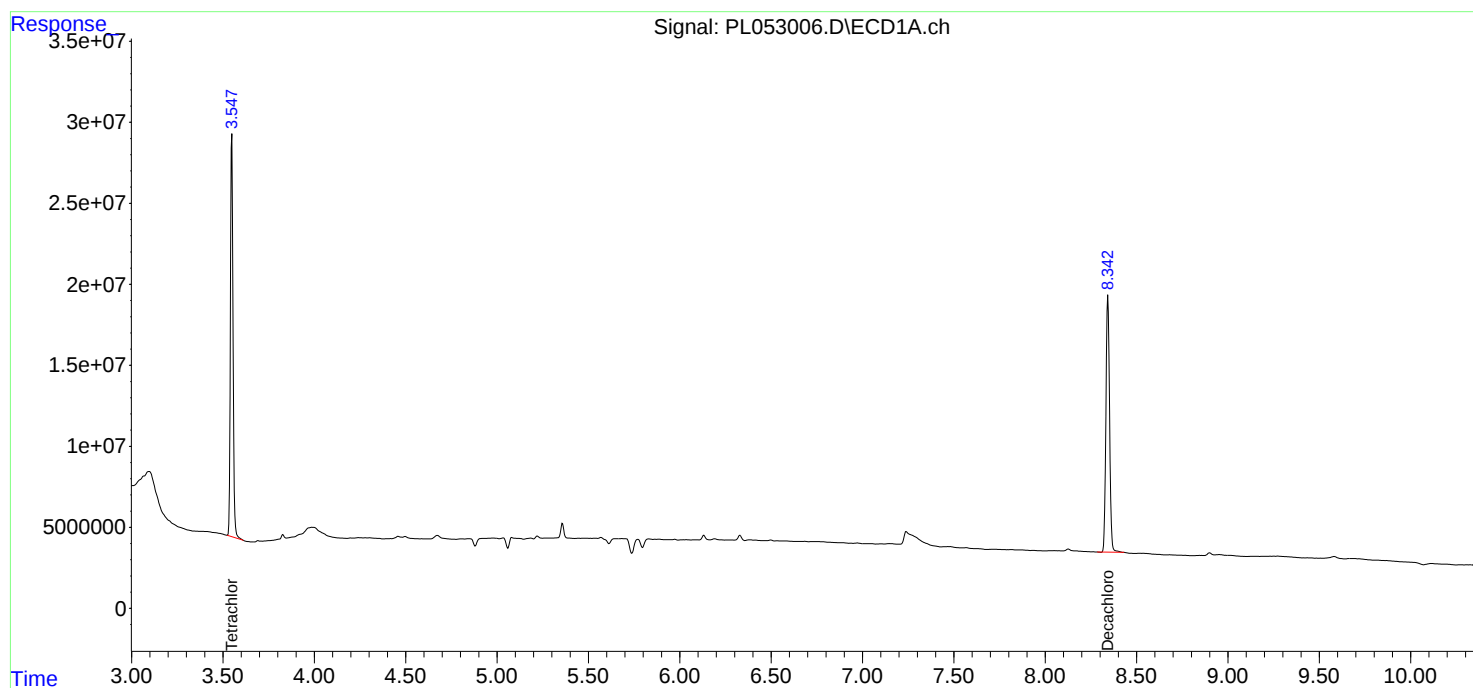


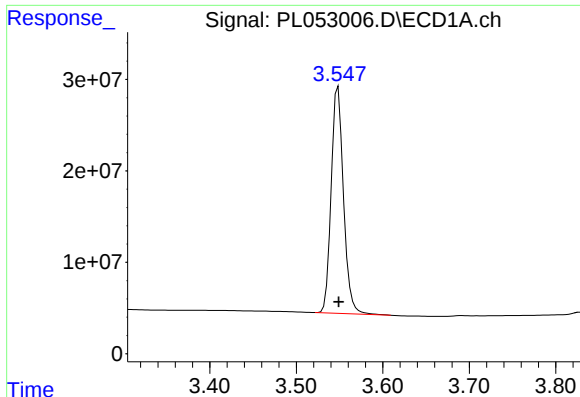

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 244440389
Conc: 24.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

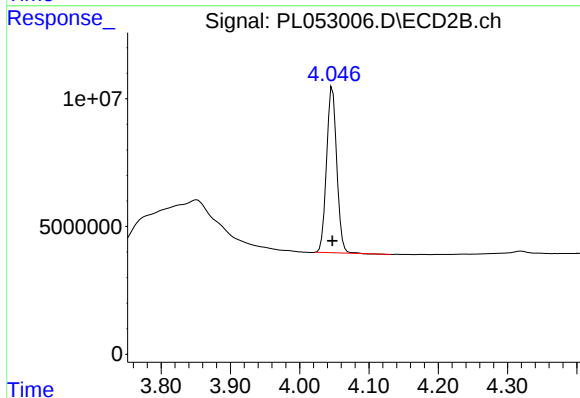


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 66202271
Conc: 24.65 ng/ml

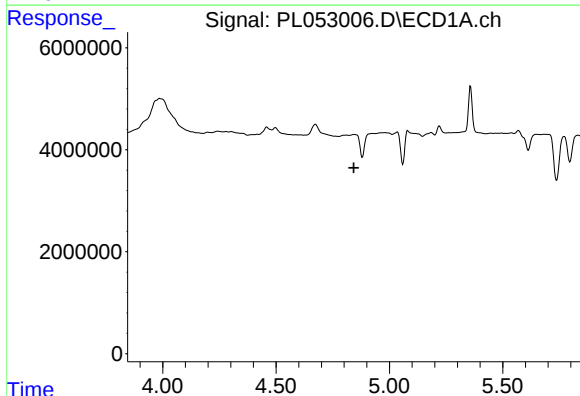


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.843 min
Response: 0
Conc: N.D.

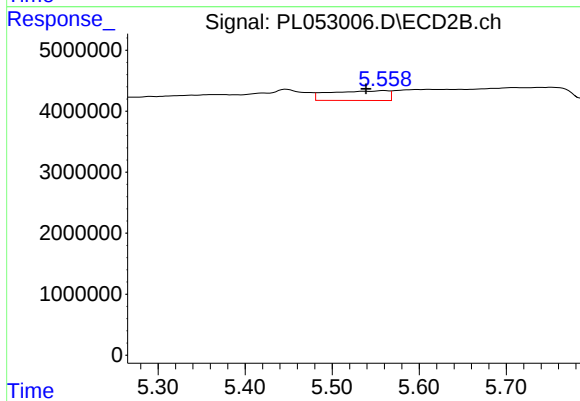

#5 Aldrin


R.T.: 5.559 min
Delta R.T.: 0.020 min
Response: 7479517
Conc: 2.16 ng/ml

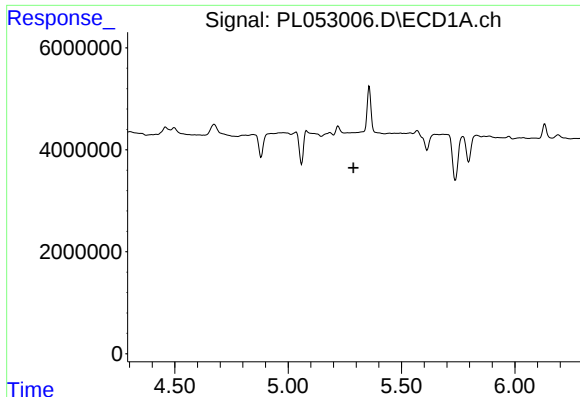

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

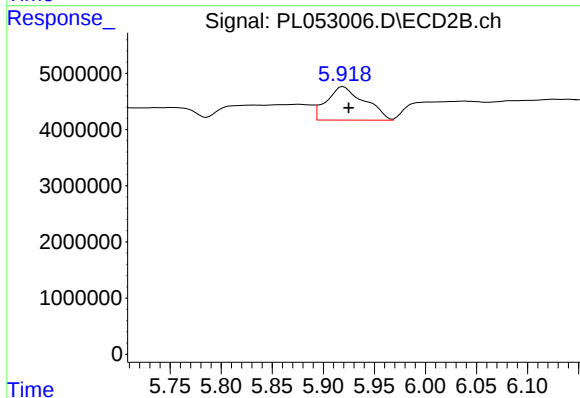


#8 Heptachlor epoxide

R.T.: 5.920 min
Delta R.T.: -0.005 min
Response: 15427261
Conc: 4.60 ng/ml

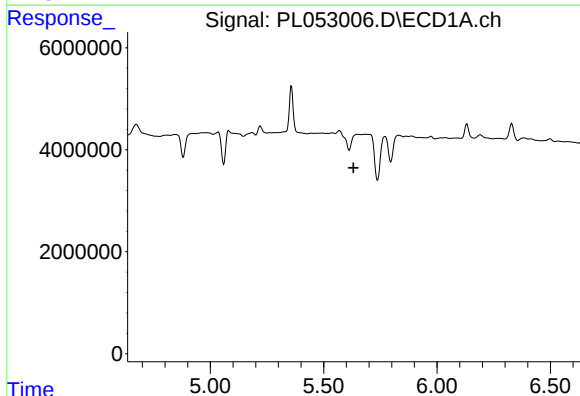


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.632 min
Response: 0
Conc: N.D.

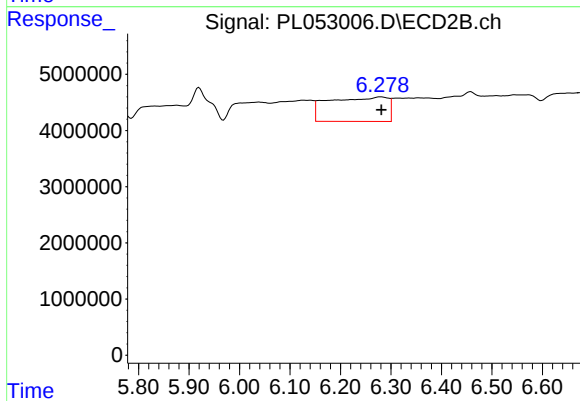

#9 Endosulfan I


R.T.: 6.279 min
Delta R.T.: -0.002 min
Response: 35402797
Conc: 11.33 ng/ml

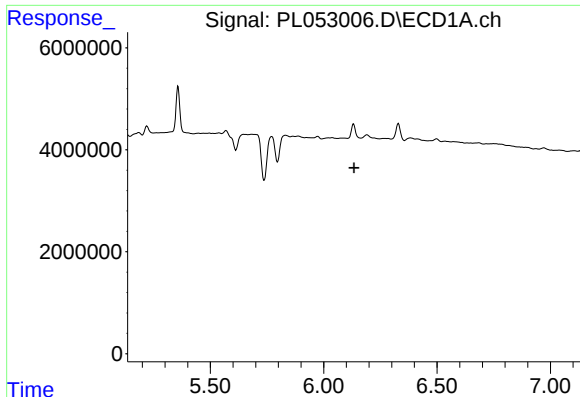

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

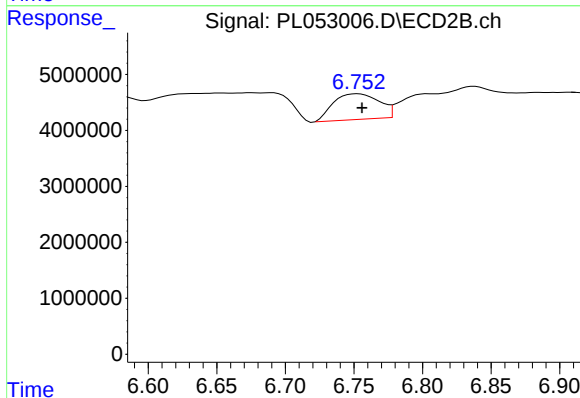


#14 Endrin

R.T.: 6.753 min
Delta R.T.: -0.003 min
Response: 10714083
Conc: 3.86 ng/ml

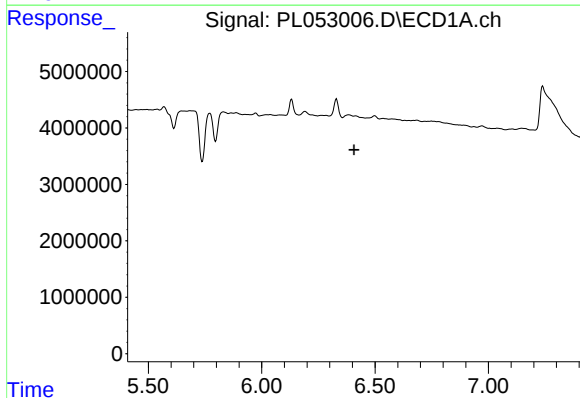


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

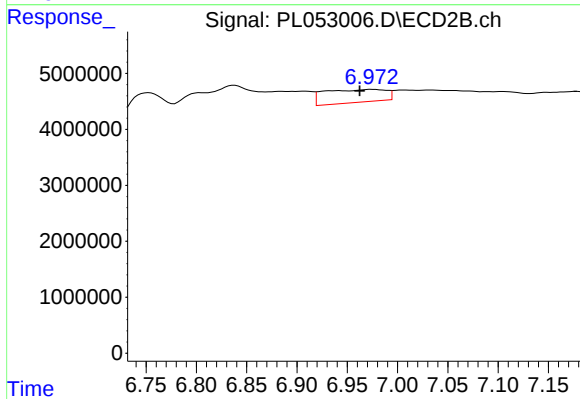

#15 Endosulfan II


R.T.: 6.975 min
Delta R.T.: 0.012 min
Response: 9774553
Conc: 3.29 ng/ml

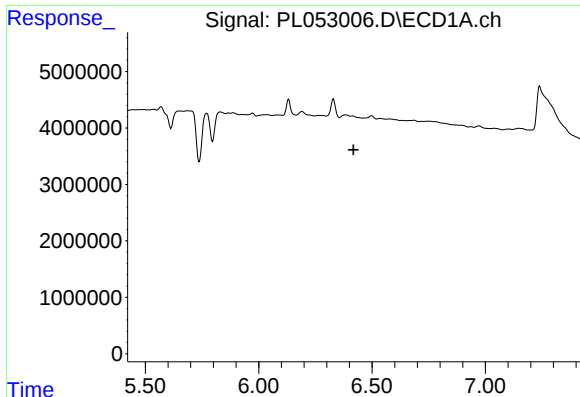

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

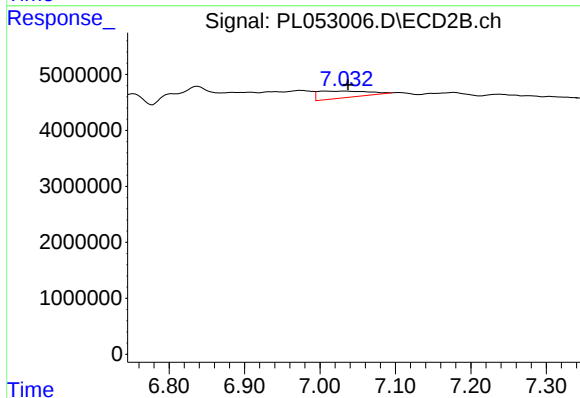


#27 Chlordane-5

R.T.: 7.034 min
Delta R.T.: -0.004 min
Response: 5465772
Conc: 61.96 ng/ml

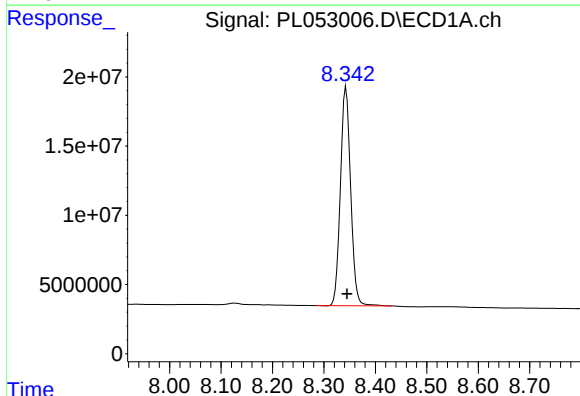

#28 Decachlorobiphenyl

R.T.: 8.343 min
Delta R.T.: -0.002 min
Response: 218710546
Conc: 21.84 ng/ml

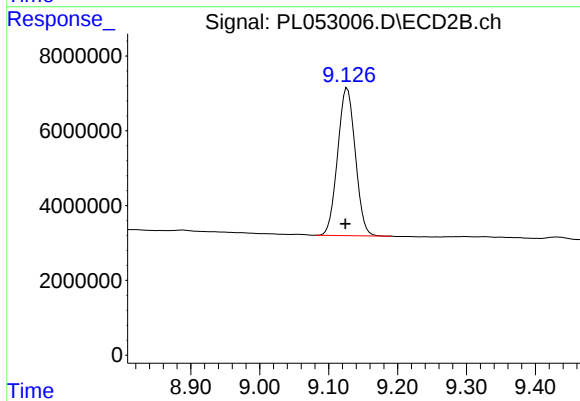

#28 Decachlorobiphenyl

R.T.: 9.127 min
Delta R.T.: 0.003 min
Response: 70143951
Conc: 23.91 ng/ml