

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
 Data File : PL053022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2019 22:46
 Operator : SG\AJ
 Sample : K4659-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-02-093019-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:16:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	4.048	170.3E6	51373243	17.122	19.132
28)	SA Decachlor...	8.342	9.126	170.4E6	58762897	17.014	20.030
Target Compounds							
2)	A alpha-BHC	0.000	4.435	0	1670102	N.D.	0.435 #
4)	MA Heptachlor	0.000	5.237	0	494355	N.D.	0.130 #
7)	B delta-BHC	0.000	5.086f	0	4091750	N.D.	1.130 #
10)	B gamma-Chl...	0.000	6.159	0	3357794	N.D.	0.993 #
11)	B alpha-Chl...	0.000	6.233	0	4056419	N.D.	1.205 #
23)	Chlordane-1	0.000	5.034	0	4359326	N.D.	42.979 #
25)	Chlordane-3	0.000	6.159	0	3357794	N.D.	7.710 #
26)	Chlordane-4	0.000	6.233	0	4056419	N.D.	7.639 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
Data File : PL053022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2019 22:46
Operator : SG\AJ
Sample : K4659-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JC-02-093019-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:16:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

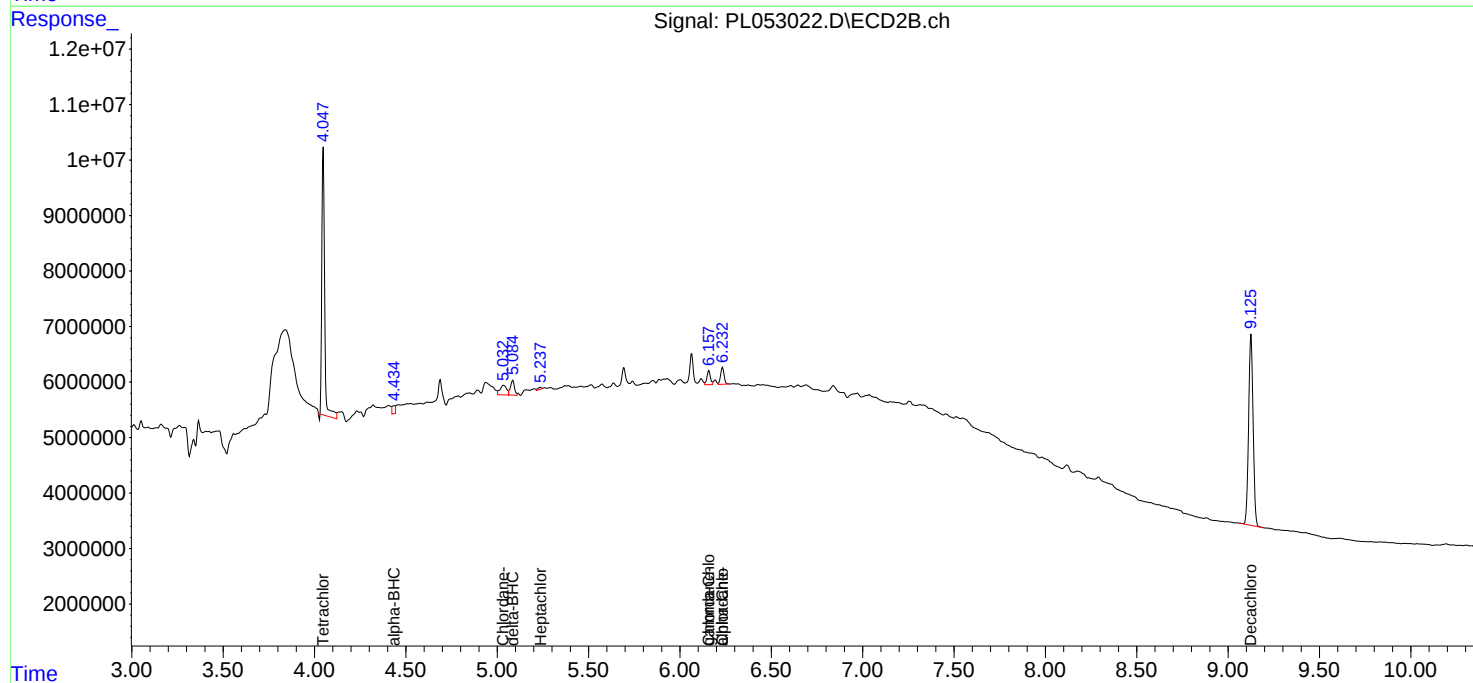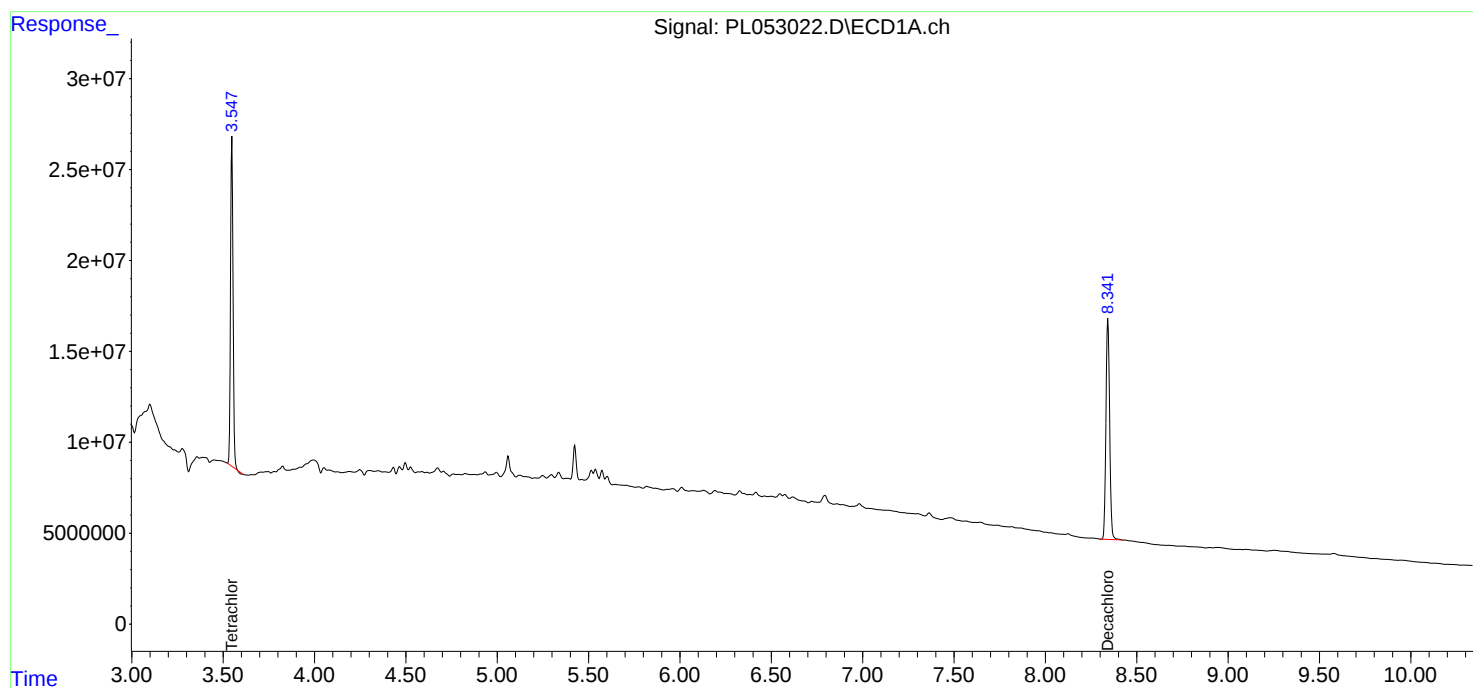


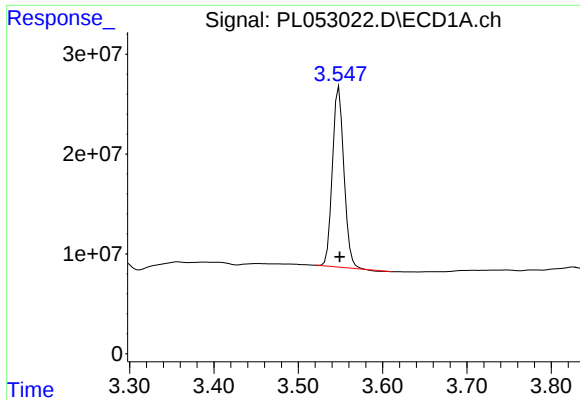

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 170305144
Conc: 17.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-02-093019-B

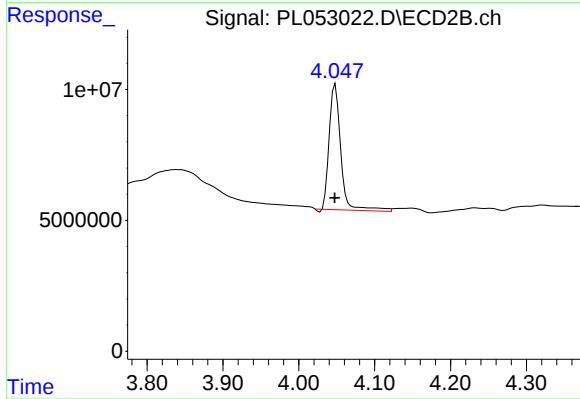


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 51373243
Conc: 19.13 ng/ml

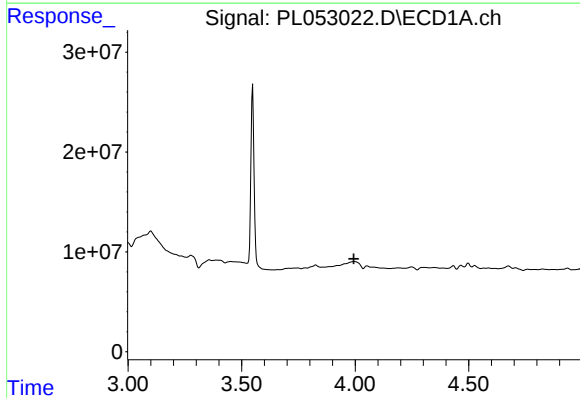


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.994 min
Response: 0
Conc: N.D.

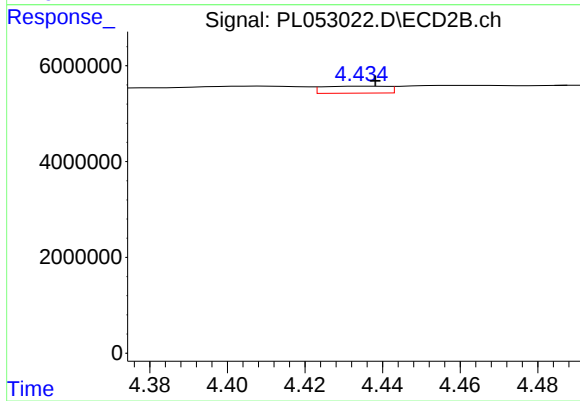

#2 alpha-BHC


R.T.: 4.435 min
Delta R.T.: -0.003 min
Response: 1670102
Conc: 0.43 ng/ml

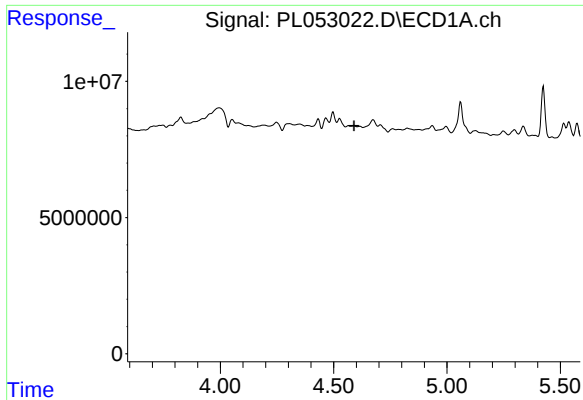

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.590 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-02-093019-B

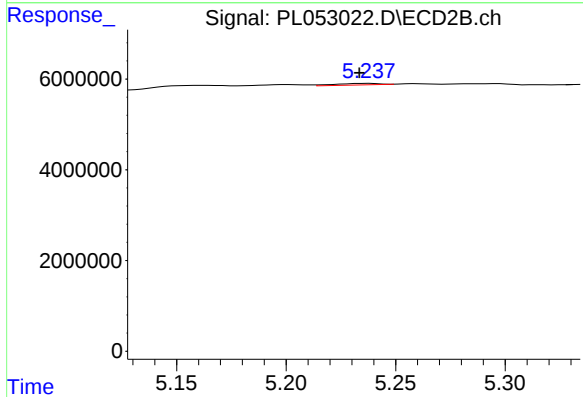


#4 Heptachlor

R.T.: 5.237 min
Delta R.T.: 0.004 min
Response: 494355
Conc: 0.13 ng/ml

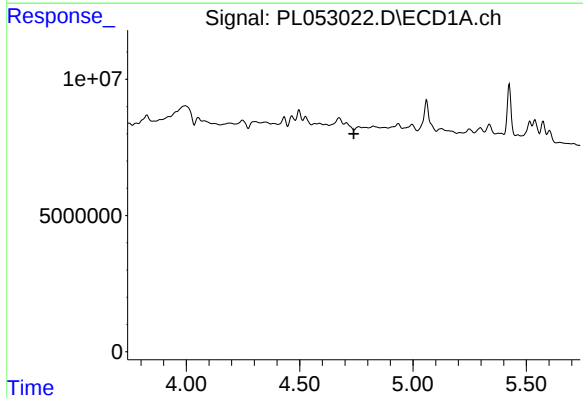


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.740 min
Response: 0
Conc: N.D.

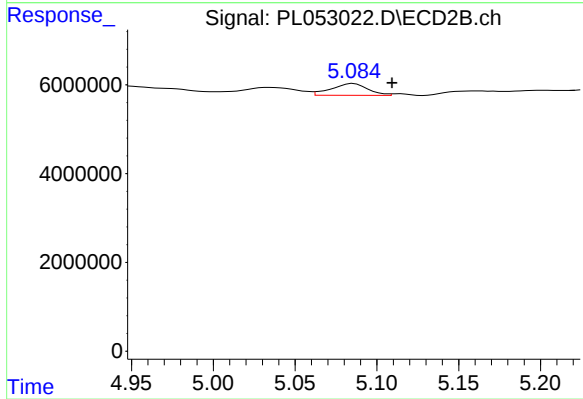

#7 delta-BHC


R.T.: 5.086 min
Delta R.T.: -0.024 min
Response: 4091750
Conc: 1.13 ng/ml

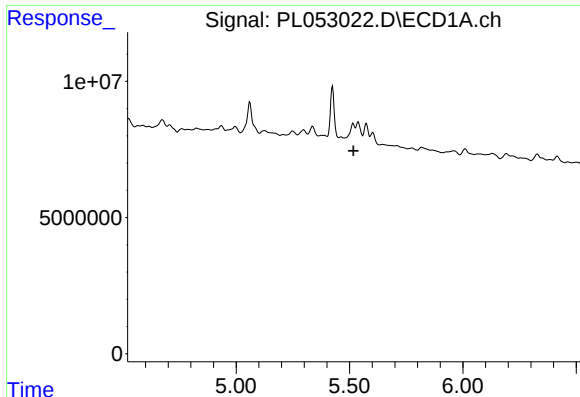

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-02-093019-B

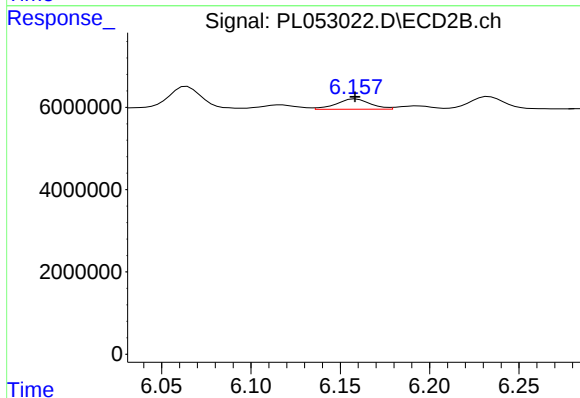


#10 gamma-Chlordane

R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 3357794
Conc: 0.99 ng/ml

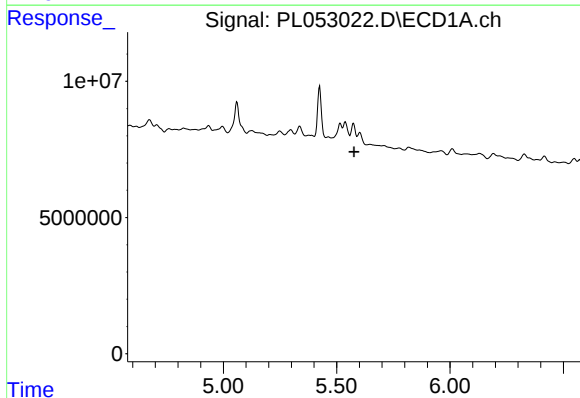


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

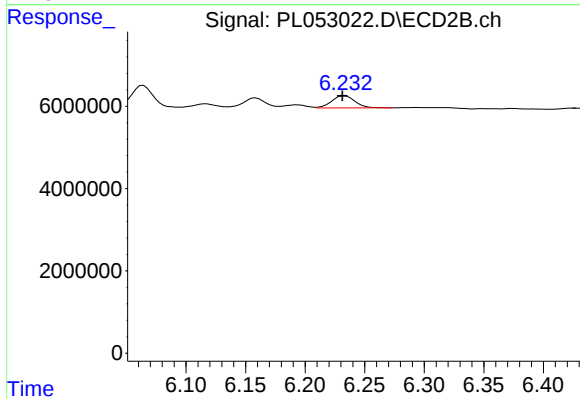

#11 alpha-Chlordane


R.T.: 6.233 min
Delta R.T.: 0.002 min
Response: 4056419
Conc: 1.21 ng/ml

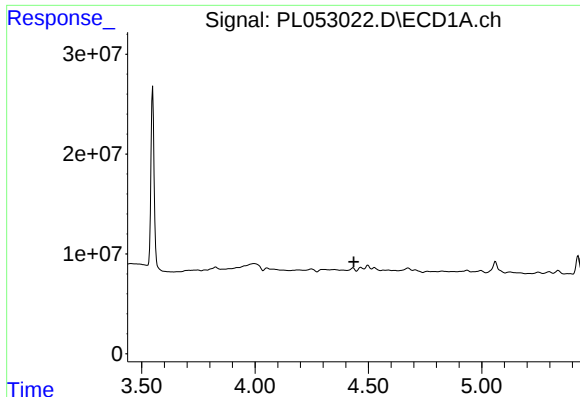

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-02-093019-B

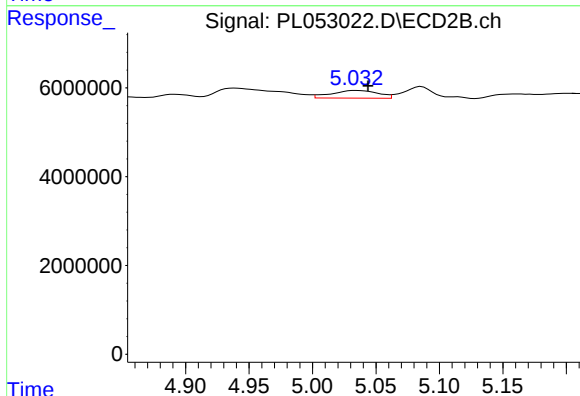


#23 Chlordane-1

R.T.: 5.034 min
Delta R.T.: -0.009 min
Response: 4359326
Conc: 42.98 ng/ml

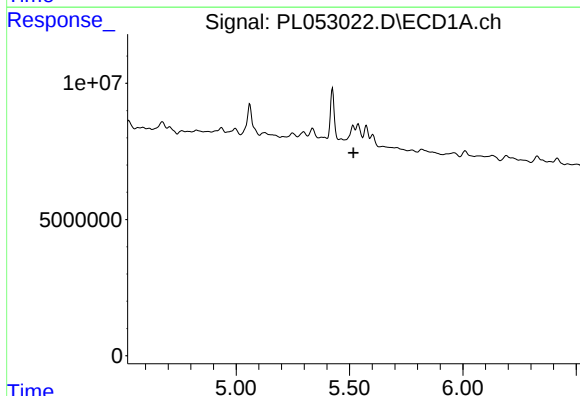


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

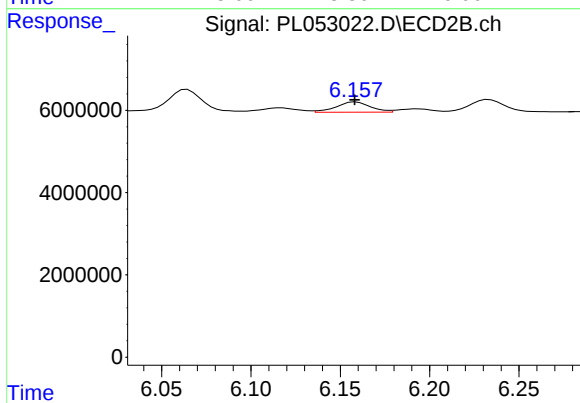

#25 Chlordane-3


R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 3357794
Conc: 7.71 ng/ml

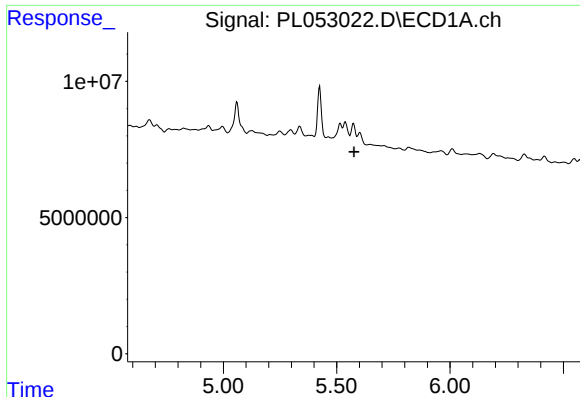

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-02-093019-B

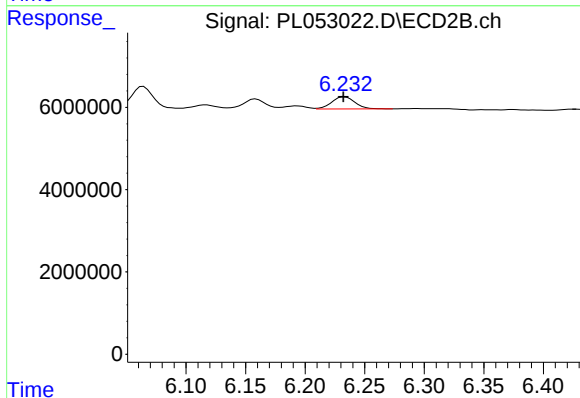


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 4056419
Conc: 7.64 ng/ml

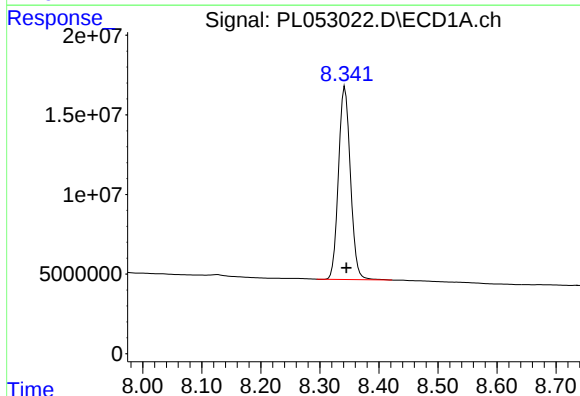

#28 Decachlorobiphenyl

R.T.: 8.342 min
Delta R.T.: -0.003 min
Response: 170413790
Conc: 17.01 ng/ml

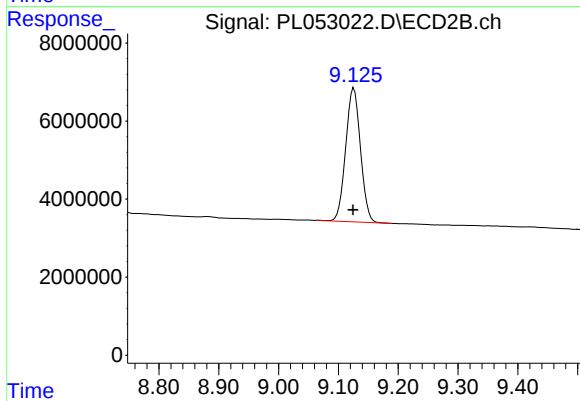

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.002 min
Response: 58762897
Conc: 20.03 ng/ml