

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
 Data File : PL053026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2019 23:42
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:17:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	4.048	232.0E6	64025318	23.328	23.844
28)	SA Decachlor...	8.342	9.126	207.2E6	67777058	20.685	23.103
Target Compounds							
8)	B Heptachlo...	0.000	5.920	0	17537561	N.D.	5.233 #
9)	A Endosulfan I	0.000	6.280	0	23914840	N.D.	7.651 #
10)	B gamma-Chl...	0.000	6.139f	0	16923197	N.D.	5.002 #
12)	B 4,4'-DDE	5.769f	6.358f	3191072	7156257	0.275	2.191 #
14)	MA Endrin	0.000	6.752	0	9932302	N.D.	3.577 #
15)	B Endosulfa...	0.000	6.972	0	8925846	N.D.	3.008 #
16)	A 4,4'-DDD	0.000	6.872	0	4369667	N.D.	1.782 #
18)	B Endrin al...	0.000	7.062f	0	3872640	N.D.	1.579 #
25)	Chlordane-3	0.000	6.139f	0	16923197	N.D.	38.858 #
27)	Chlordane-5	0.000	7.062f	0	3872640	N.D.	43.903 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
Data File : PL053026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2019 23:42
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:17:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

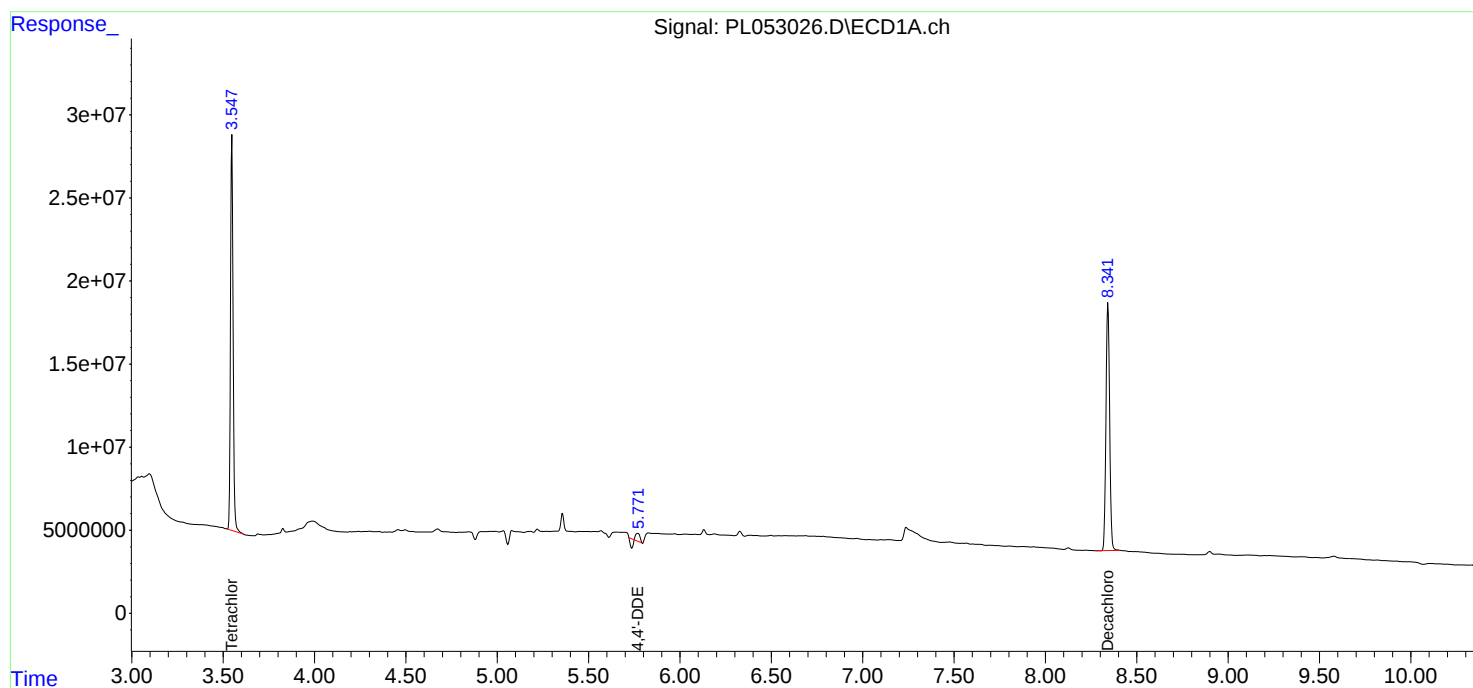


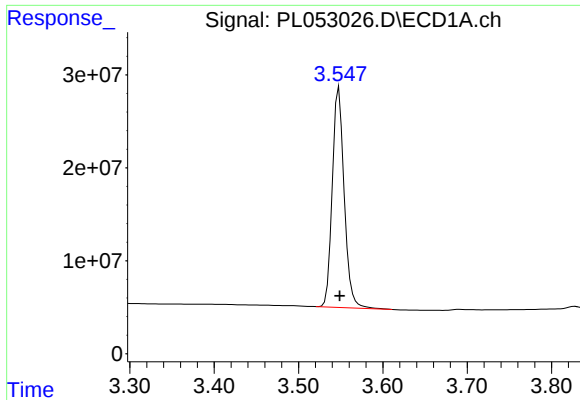

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: -0.001 min
Response: 232039813
Conc: 23.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

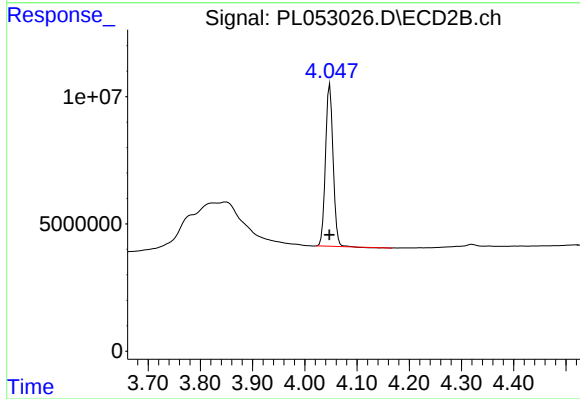


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 64025318
Conc: 23.84 ng/ml

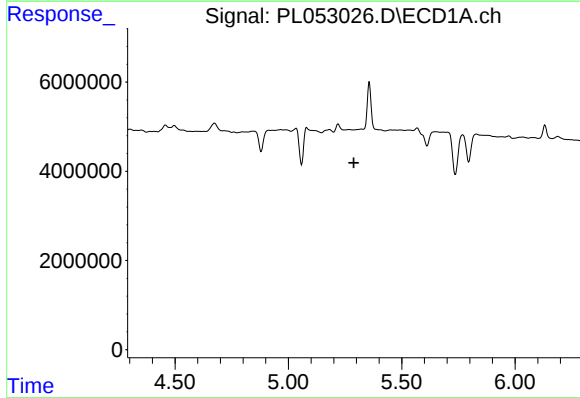


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.289 min
Response: 0
Conc: N.D.

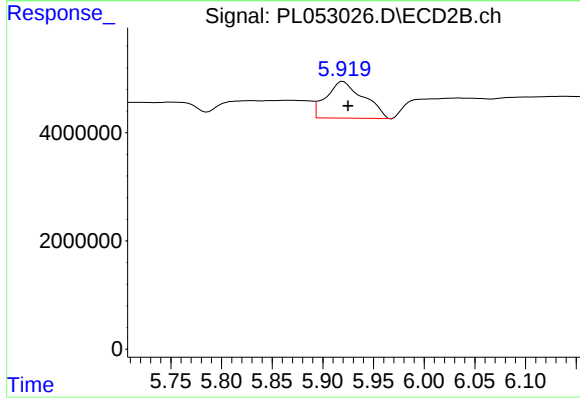

#8 Heptachlor epoxide


R.T.: 5.920 min
Delta R.T.: -0.005 min
Response: 17537561
Conc: 5.23 ng/ml

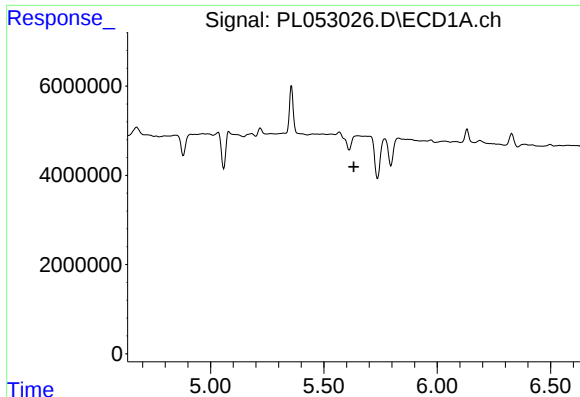

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.632 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

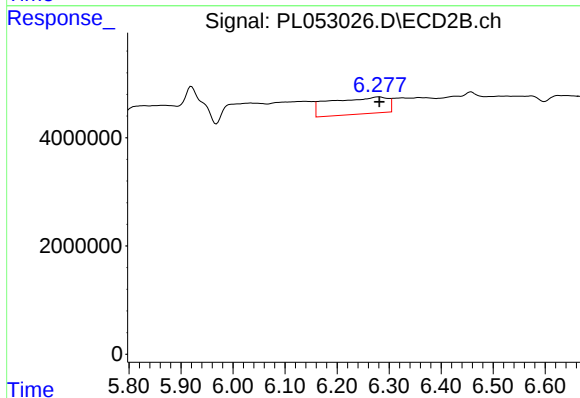


#9 Endosulfan I

R.T.: 6.280 min
Delta R.T.: -0.001 min
Response: 23914840
Conc: 7.65 ng/ml

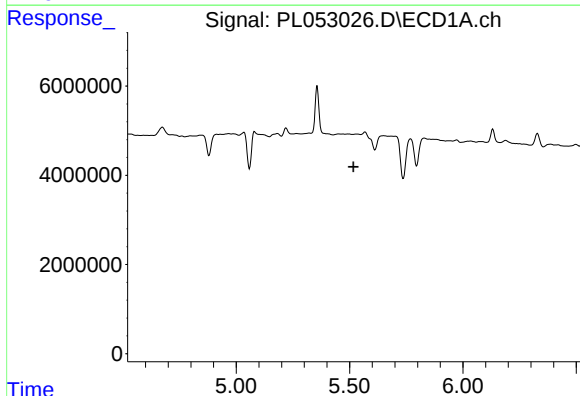


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

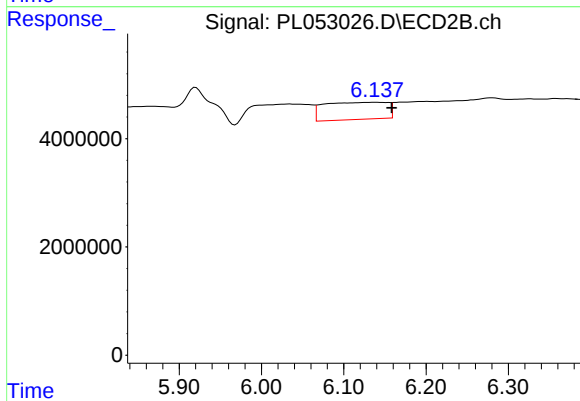

#10 gamma-Chlordane


R.T.: 6.139 min
Delta R.T.: -0.019 min
Response: 16923197
Conc: 5.00 ng/ml

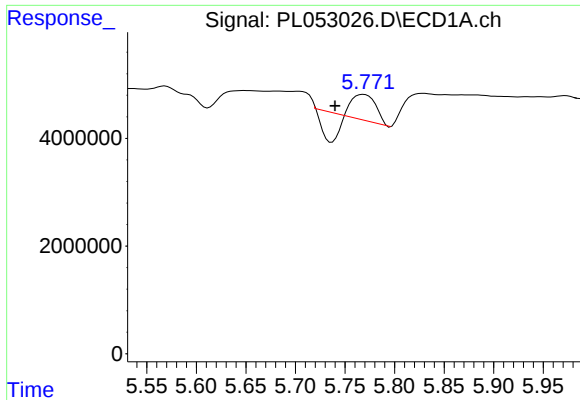

#12 4,4'-DDE


R.T.: 5.769 min
Delta R.T.: 0.029 min
Response: 3191072
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

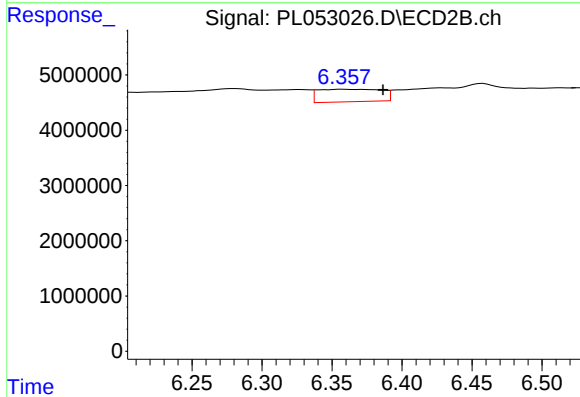


#12 4,4'-DDE

R.T.: 6.358 min
Delta R.T.: -0.028 min
Response: 7156257
Conc: 2.19 ng/ml

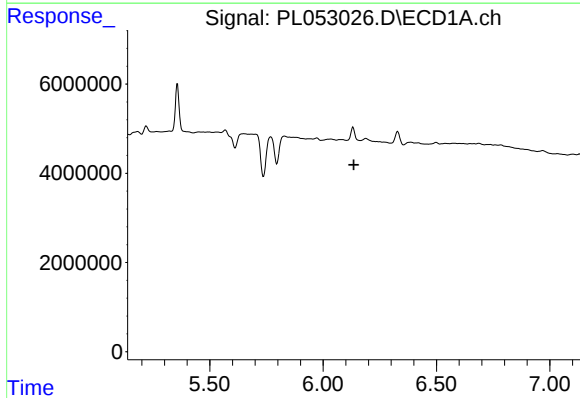


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.135 min
Response: 0
Conc: N.D.

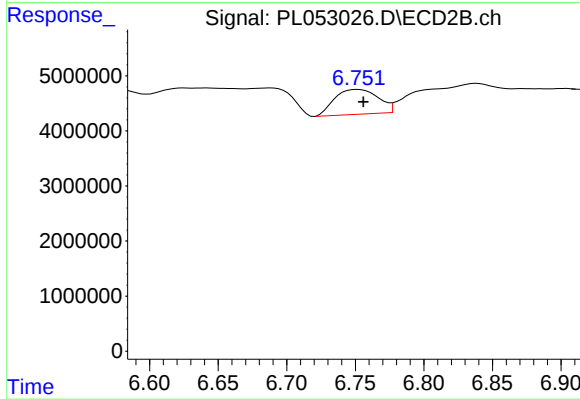

#14 Endrin


R.T.: 6.752 min
Delta R.T.: -0.004 min
Response: 9932302
Conc: 3.58 ng/ml

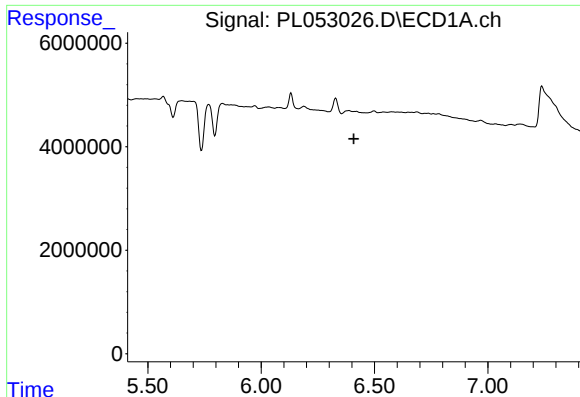

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

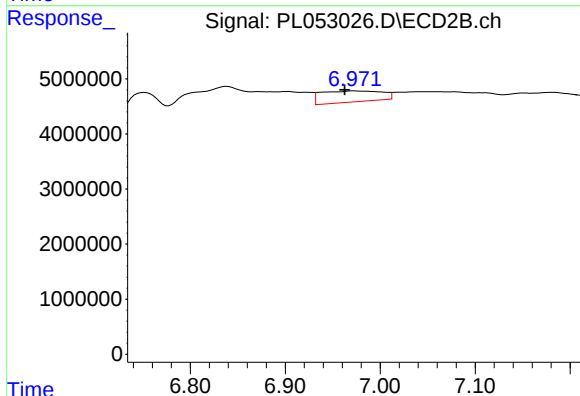


#15 Endosulfan II

R.T.: 6.972 min
Delta R.T.: 0.010 min
Response: 8925846
Conc: 3.01 ng/ml

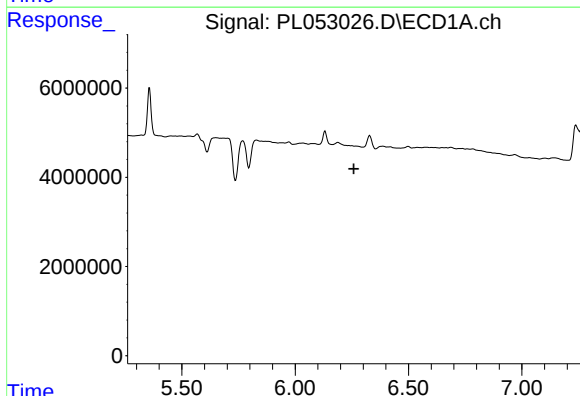


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.258 min
Response: 0
Conc: N.D.

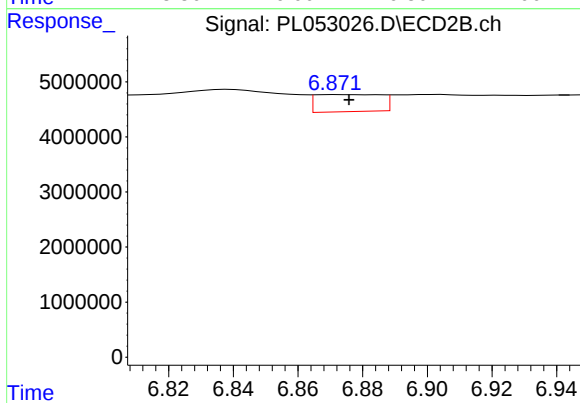

#16 4,4'-DDD


R.T.: 6.872 min
Delta R.T.: -0.004 min
Response: 4369667
Conc: 1.78 ng/ml

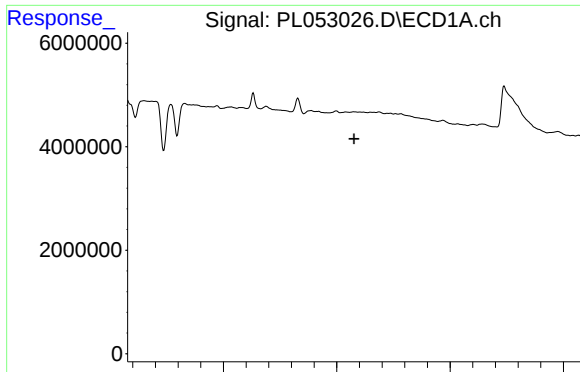

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

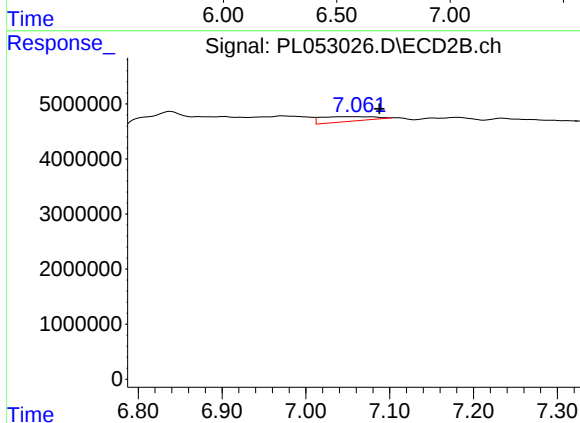


#18 Endrin aldehyde

R.T.: 7.062 min
Delta R.T.: -0.026 min
Response: 3872640
Conc: 1.58 ng/ml

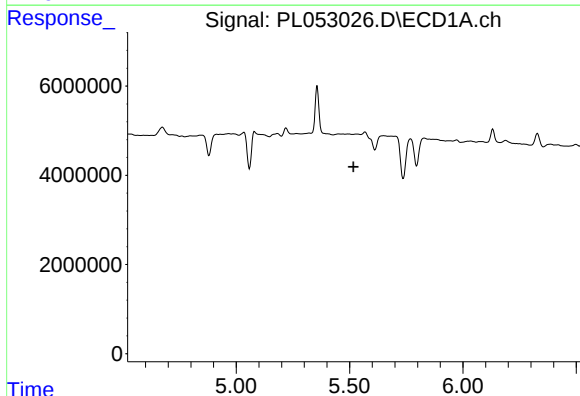


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

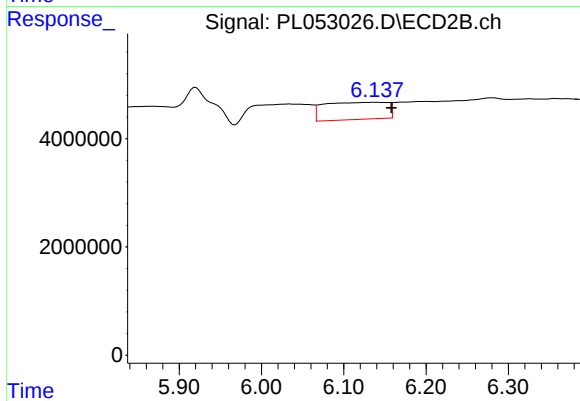

#25 Chlordane-3


R.T.: 6.139 min
Delta R.T.: -0.019 min
Response: 16923197
Conc: 38.86 ng/ml

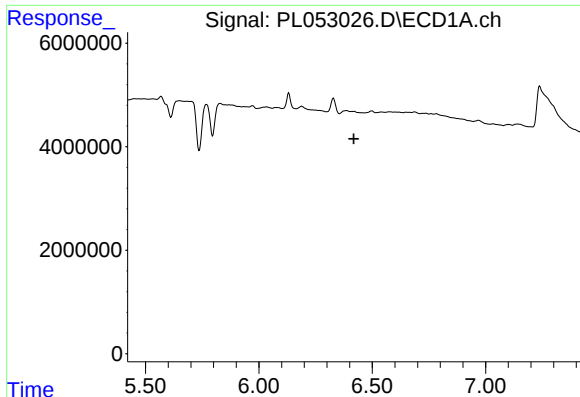

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

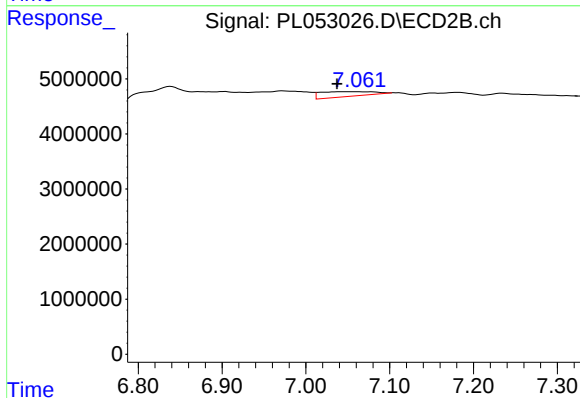


#27 Chlordane-5

R.T.: 7.062 min
Delta R.T.: 0.025 min
Response: 3872640
Conc: 43.90 ng/ml

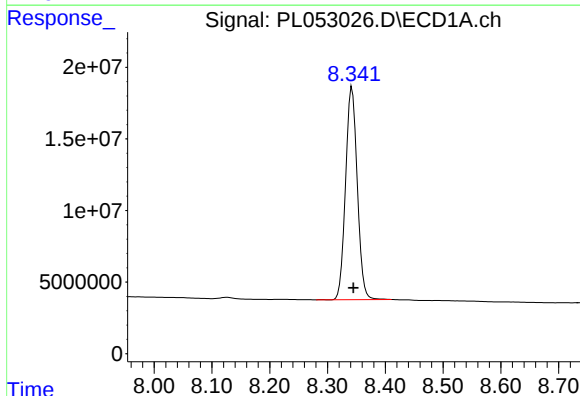

#28 Decachlorobiphenyl

R.T.: 8.342 min
Delta R.T.: -0.003 min
Response: 207178148
Conc: 20.68 ng/ml

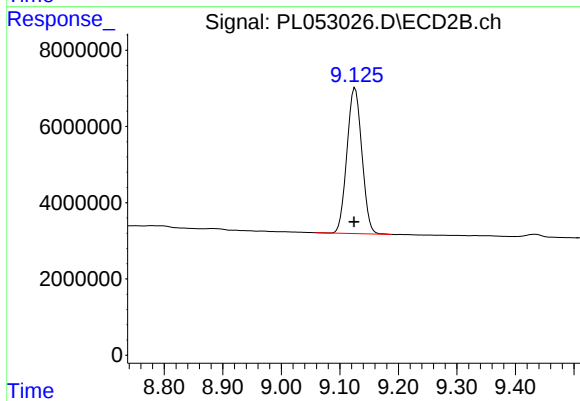

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.002 min
Response: 67777058
Conc: 23.10 ng/ml