

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
 Data File : PL053009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2019 19:43
 Operator : SG\AJ
 Sample : K5134-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-061

Manual Integrations
 APPROVED

Ankita
 10/3/2019 5:47:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:14:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	4.047	102.0E6	28632700	10.250	10.663
28)	SA Decachlor...	8.343	9.126	68431529	21383431	6.832	7.289
Target Compounds							
10)	B gamma-Chl...	5.516	6.158	4611647	2420619	0.343m	0.716m#
11)	B alpha-Chl...	5.573	6.232	10229920	6366854	0.776m	1.892m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100219\
Data File : PL053009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2019 19:43
Operator : SG\AJ
Sample : K5134-01
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
FK-PS-01-061


Manual Integrations
APPROVED

Ankita
10/3/2019 5:47:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:14:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

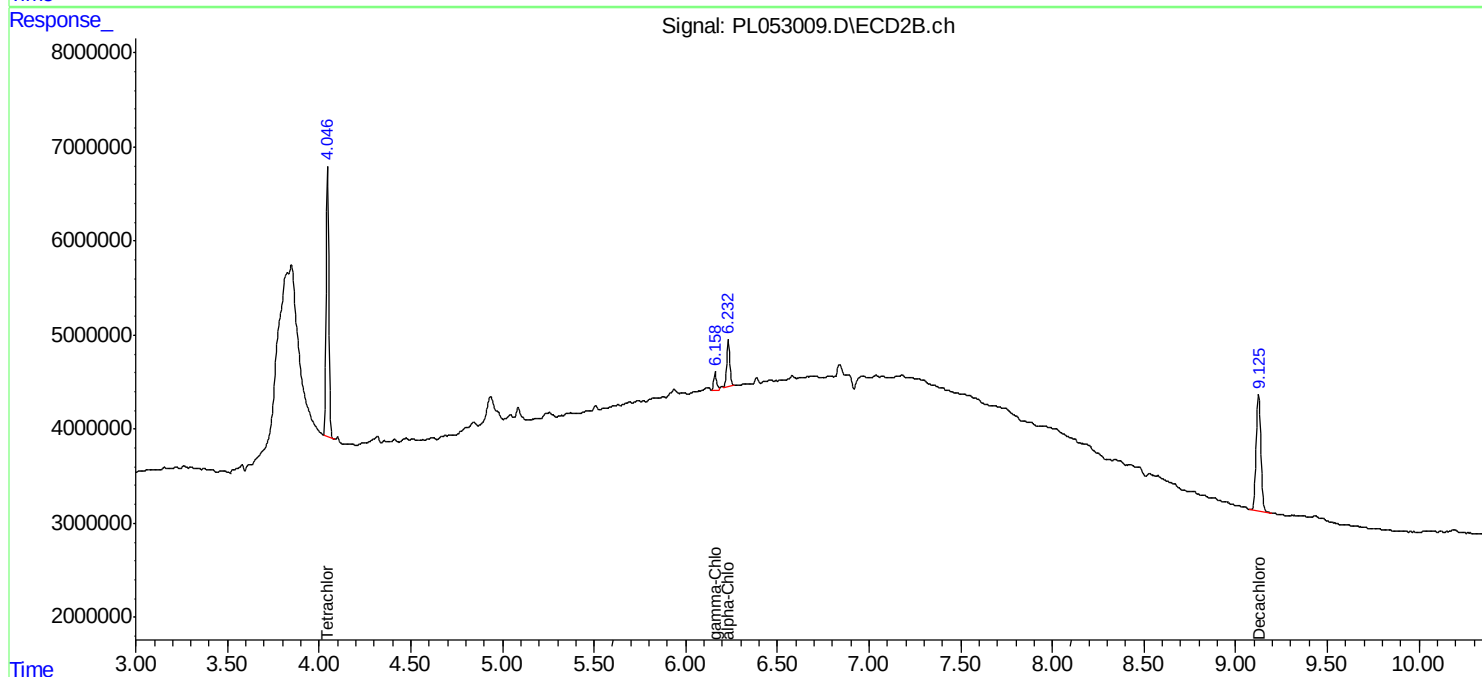

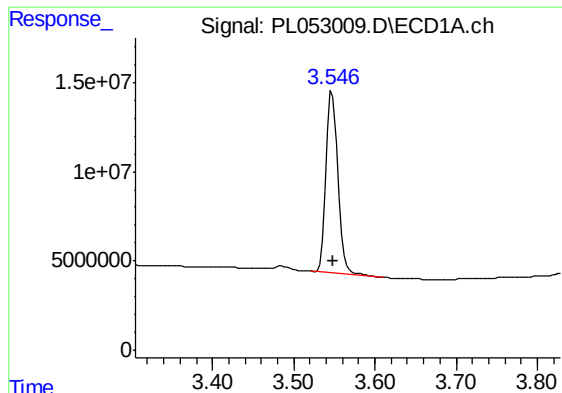


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: -0.001 min
Response: 101955309
Conc: 10.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-061


Manual Integrations
APPROVED

Ankita
10/3/2019 5:47:42 PM

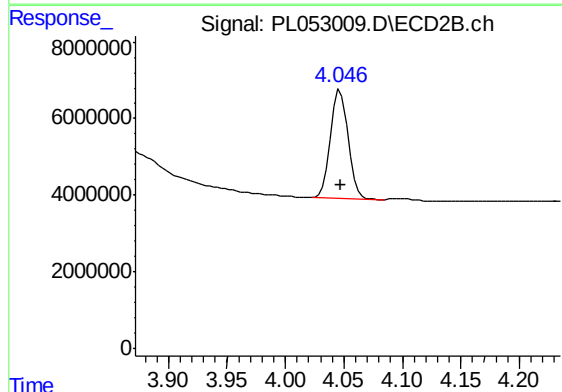


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 28632700
Conc: 10.66 ng/ml

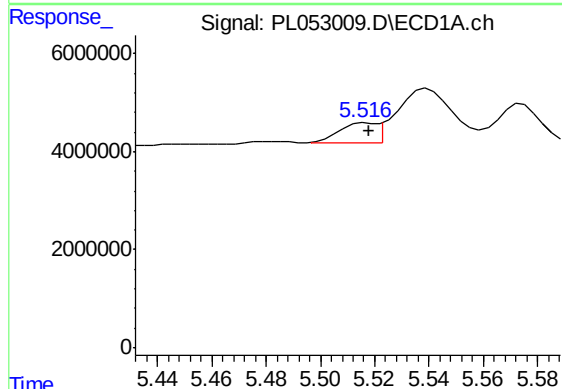


#10 gamma-Chlordane

R.T.: 5.516 min
Delta R.T.: -0.002 min
Response: 4611647
Conc: 0.34 ng/ml m

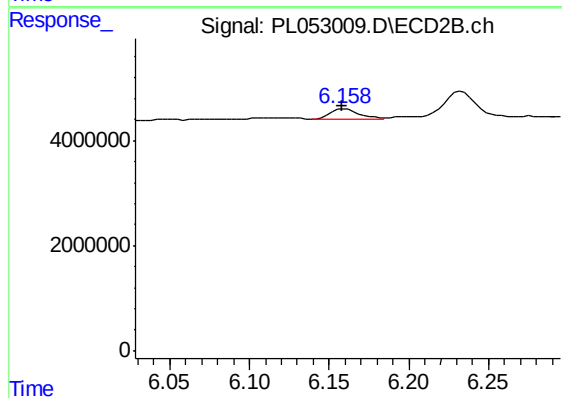

#10 gamma-Chlordane

R.T.: 6.158 min
Delta R.T.: 0.000 min
Response: 2420619
Conc: 0.72 ng/ml m

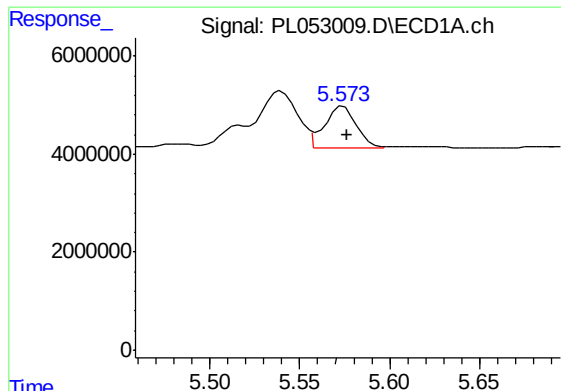


#11 alpha-Chlordane

R.T.: 5.573 min
Delta R.T.: -0.004 min
Response: 10229920
Conc: 0.78 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-061


Manual Integrations
APPROVED

Ankita
10/3/2019 5:47:42 PM

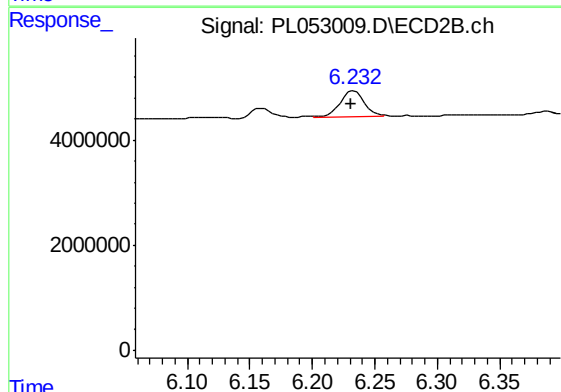


#11 alpha-Chlordane

R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 6366854
Conc: 1.89 ng/ml m

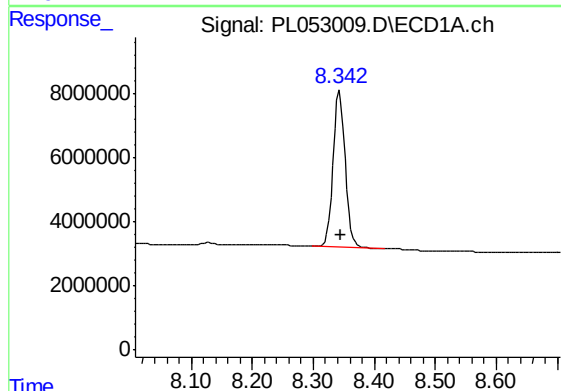

#28 Decachlorobiphenyl

R.T.: 8.343 min
Delta R.T.: -0.002 min
Response: 68431529
Conc: 6.83 ng/ml

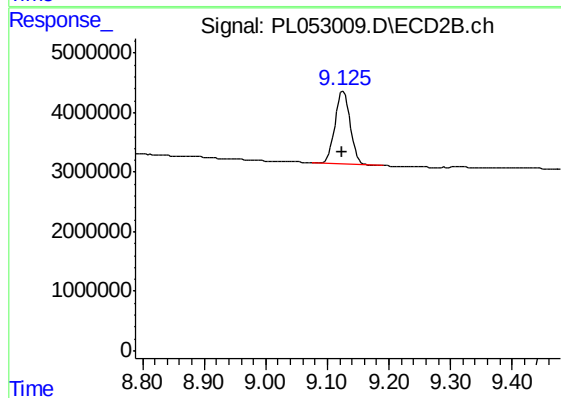

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.002 min
Response: 21383431
Conc: 7.29 ng/ml