

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
 Data File : PL061932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 12:28
 Operator : DD\AJ
 Sample : L3865-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 15:55:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.006	25363479	37293212	14.867	13.669
28)	SA Decachlor...	8.208	9.093	22905835	32072551	14.081	14.569
Target Compounds							
2)	A alpha-BHC	0.000	4.368f	0	5181708	N.D.	1.297 #
9)	A Endosulfan I	5.522	0.000	8555424	0	5.280	N.D. #
10)	B gamma-Chl...	0.000	6.123	0	8709601	N.D.	2.966 #
11)	B alpha-Chl...	0.000	6.196	0	5129553	N.D.	1.708 #
12)	B 4,4'-DDE	5.618	6.348	2418015	6112238	1.539	2.239 #
16)	A 4,4'-DDD	0.000	6.844	0	5008939	N.D.	2.253 #
17)	MA 4,4'-DDT	6.374	7.143	2932744	6230781	2.325	2.845
23)	Chlordane-1	4.322	0.000	2304161	0	46.534	N.D. #
25)	Chlordane-3	0.000	6.123	0	8709601	N.D.	23.768 #
26)	Chlordane-4	0.000	6.196	0	5129553	N.D.	11.427 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
Data File : PL061932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 12:28
Operator : DD\AJ
Sample : L3865-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 15:55:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

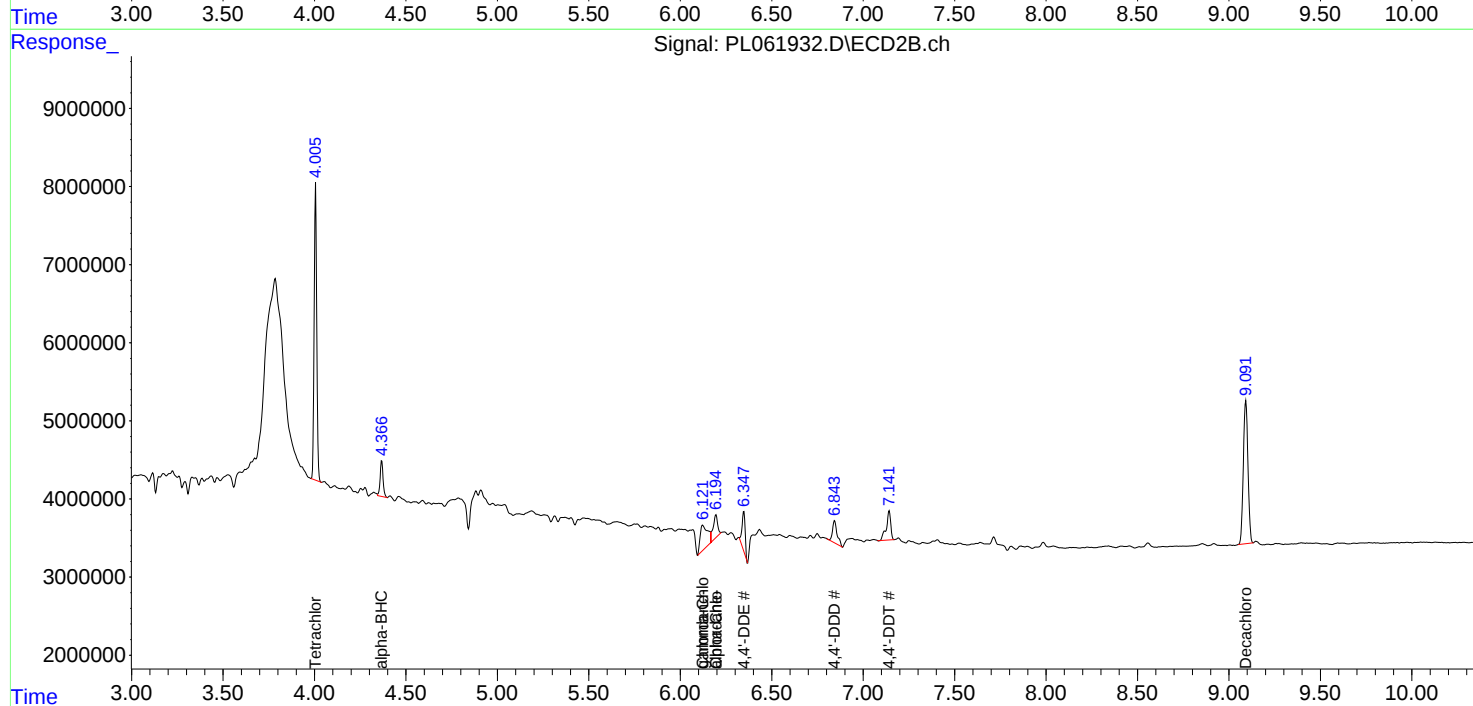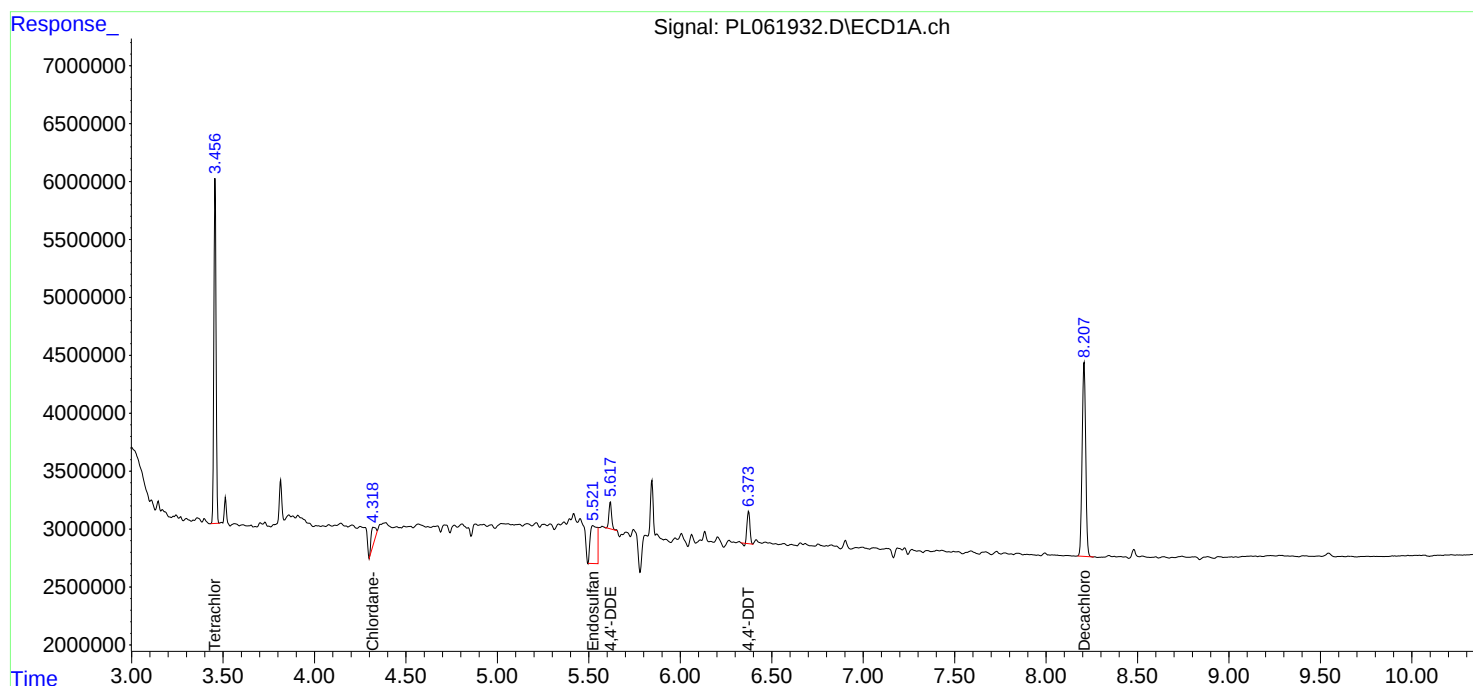


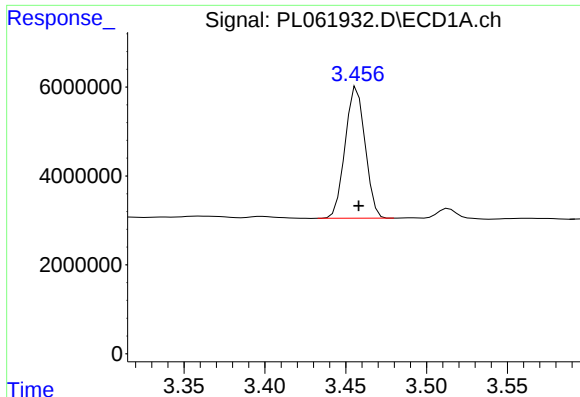

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 25363479
Conc: 14.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

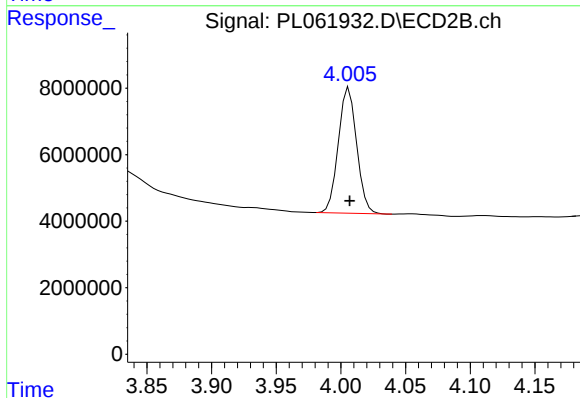


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 37293212
Conc: 13.67 ng/ml

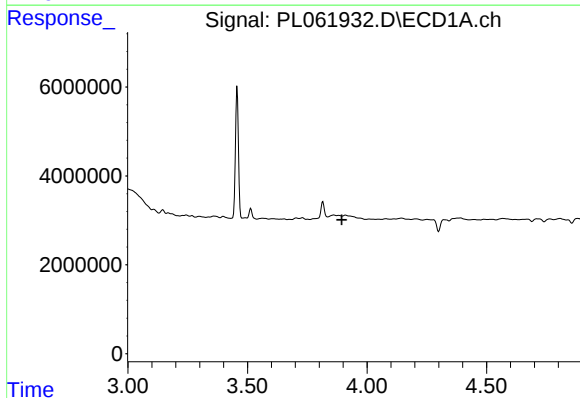


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.894 min
Response: 0
Conc: N.D.

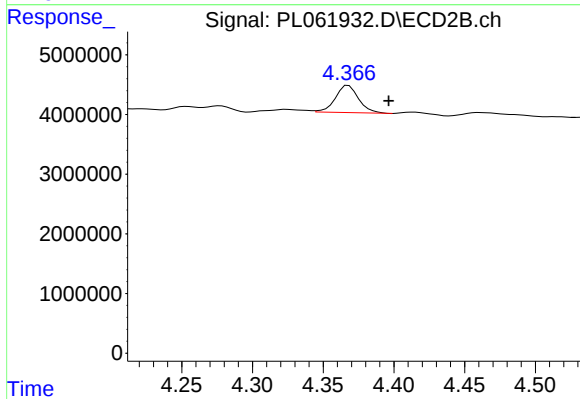

#2 alpha-BHC


R.T.: 4.368 min
Delta R.T.: -0.028 min
Response: 5181708
Conc: 1.30 ng/ml

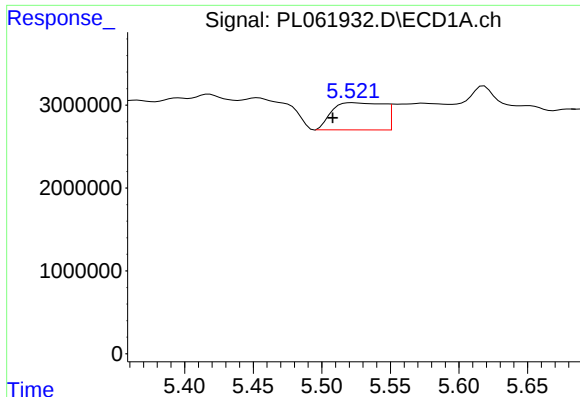

#9 Endosulfan I


R.T.: 5.522 min
Delta R.T.: 0.014 min
Response: 8555424
Conc: 5.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

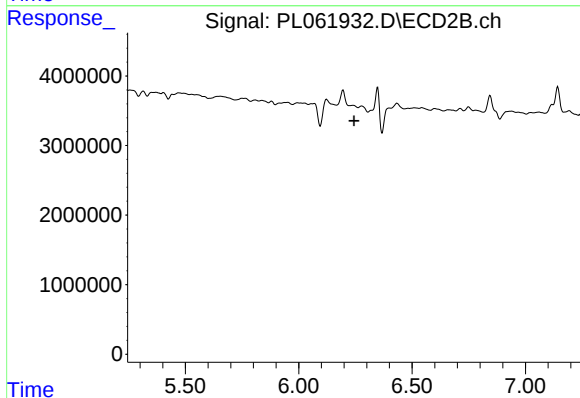


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

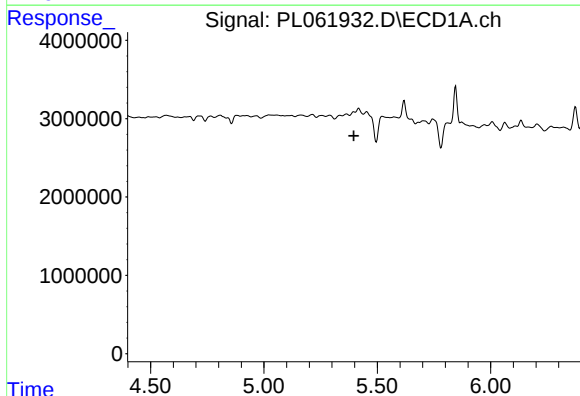


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

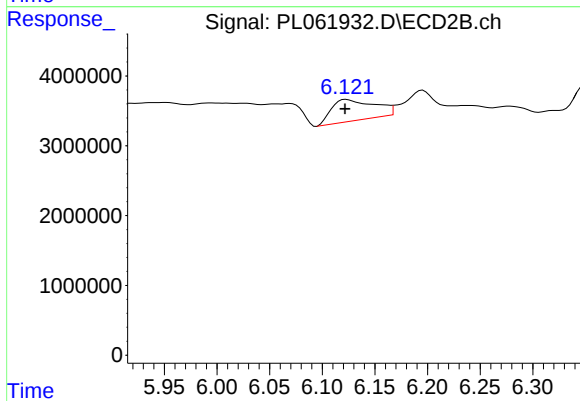

#10 gamma-Chlordane


R.T.: 6.123 min
Delta R.T.: 0.001 min
Response: 8709601
Conc: 2.97 ng/ml

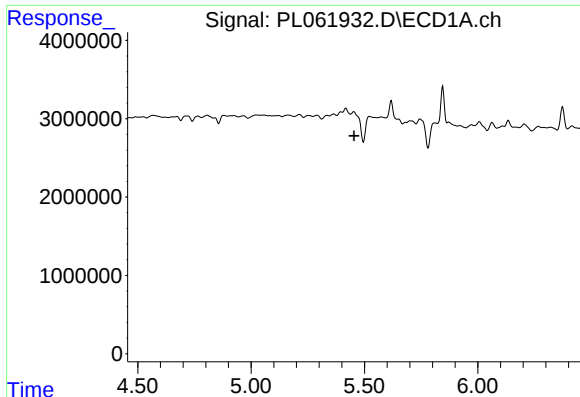

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

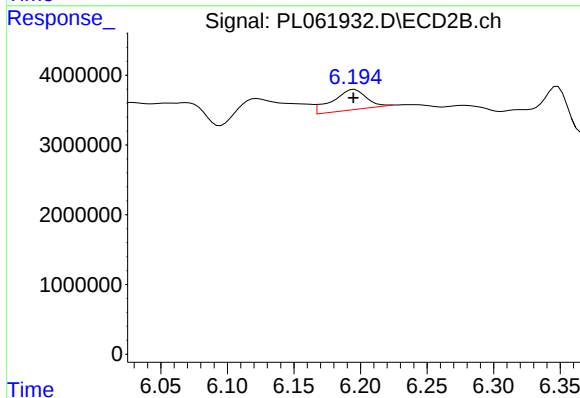


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 5129553
Conc: 1.71 ng/ml

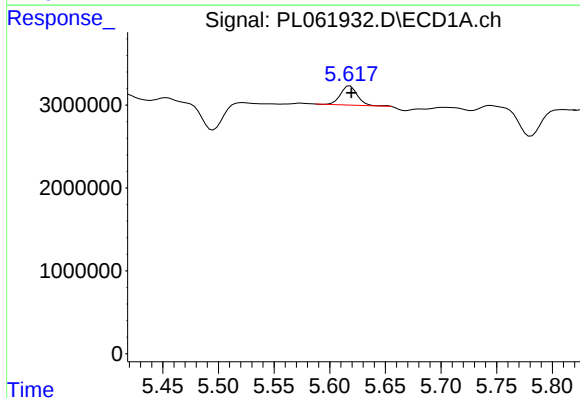


#12 4,4'-DDE

R.T.: 5.618 min
Delta R.T.: -0.001 min
Response: 2418015
Conc: 1.54 ng/ml

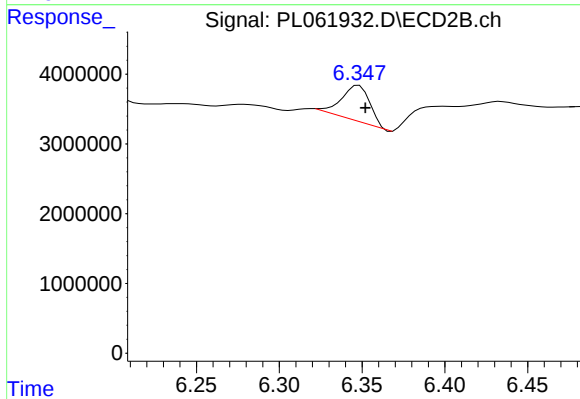

#12 4,4'-DDE


R.T.: 6.348 min
Delta R.T.: -0.004 min
Response: 6112238
Conc: 2.24 ng/ml

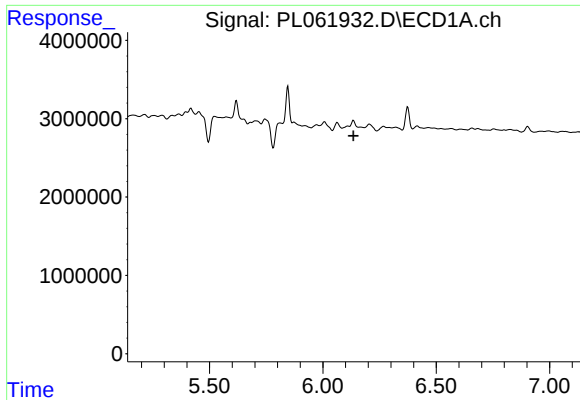

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

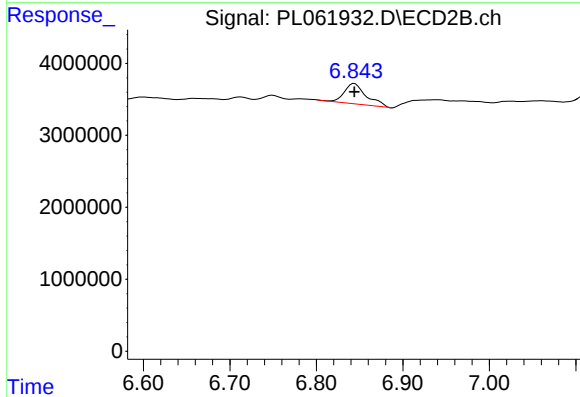


#16 4,4'-DDD

R.T.: 6.844 min
Delta R.T.: 0.000 min
Response: 5008939
Conc: 2.25 ng/ml

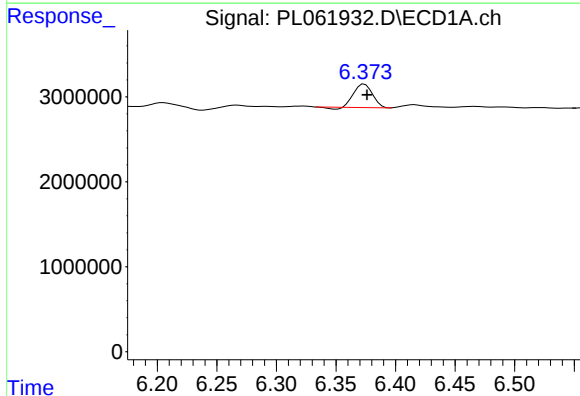


#17 4,4'-DDT

R.T.: 6.374 min
Delta R.T.: -0.002 min
Response: 2932744
Conc: 2.32 ng/ml

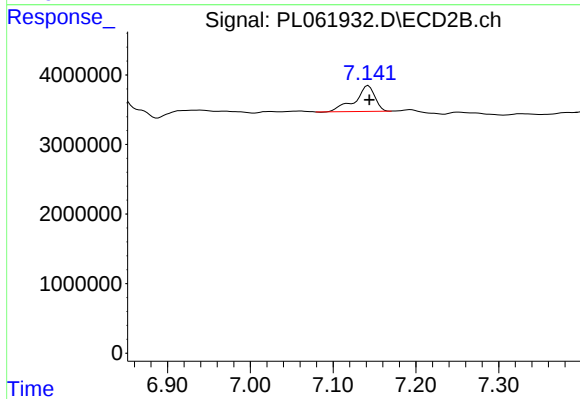

#17 4,4'-DDT


R.T.: 7.143 min
Delta R.T.: -0.001 min
Response: 6230781
Conc: 2.85 ng/ml

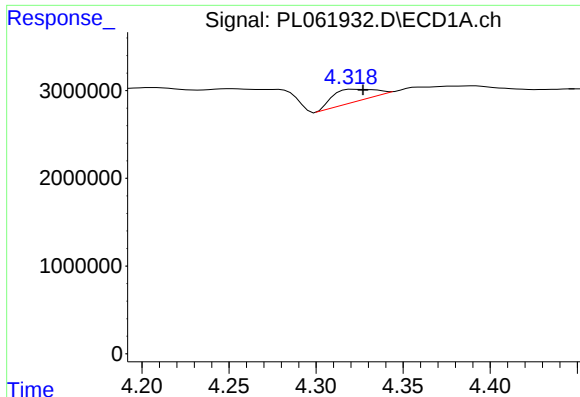

#23 Chlordane-1


R.T.: 4.322 min
Delta R.T.: -0.005 min
Response: 2304161
Conc: 46.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

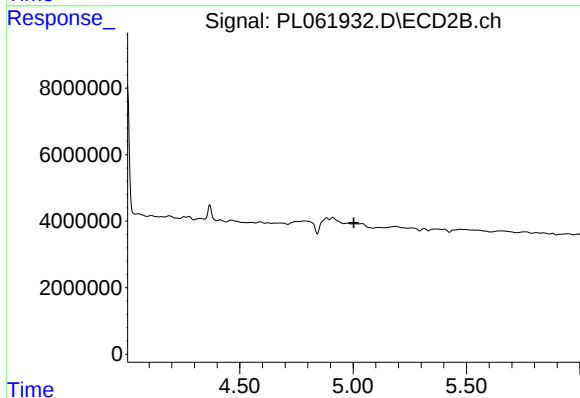


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

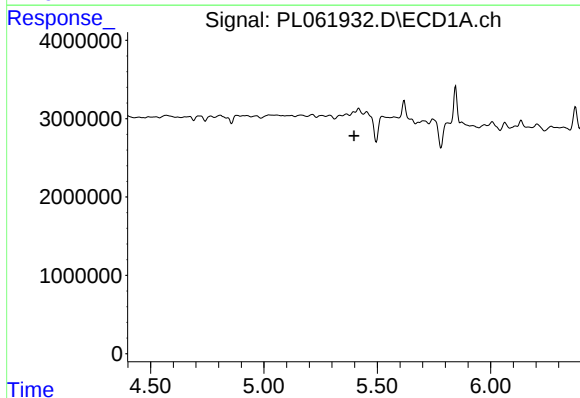


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

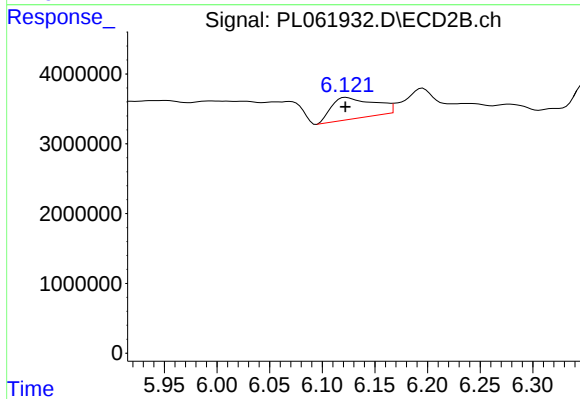

#25 Chlordane-3


R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 8709601
Conc: 23.77 ng/ml

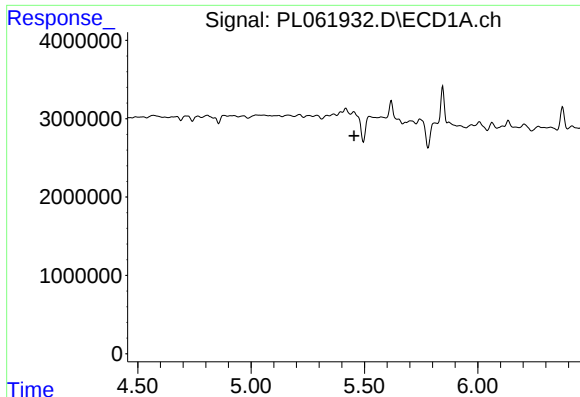

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

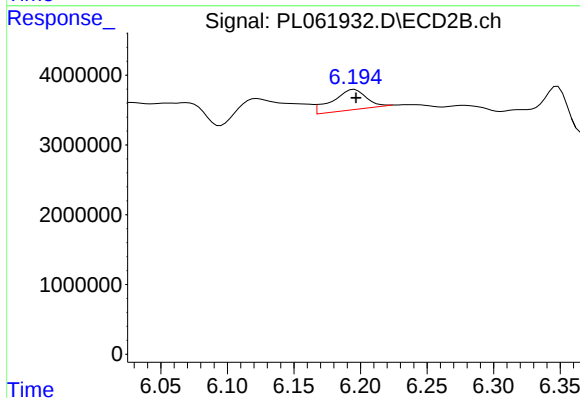


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: -0.001 min
Response: 5129553
Conc: 11.43 ng/ml

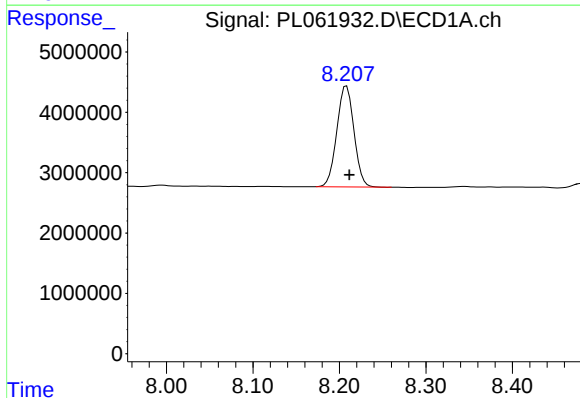

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.003 min
Response: 22905835
Conc: 14.08 ng/ml

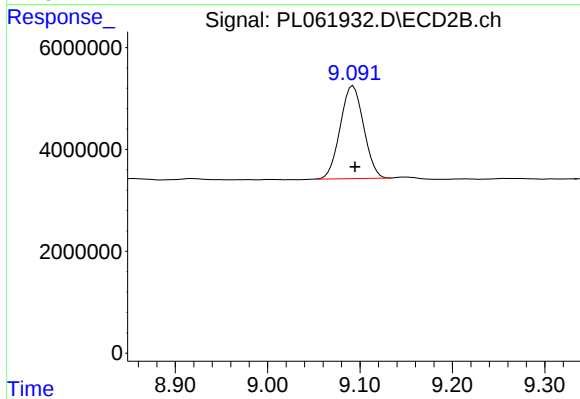

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.002 min
Response: 32072551
Conc: 14.57 ng/ml