

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
 Data File : PL061934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 12:56
 Operator : DD\AJ
 Sample : L4190-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 17:41:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.006	27566840	40313533	16.159	14.776
28)	SA Decachlor...	8.208	9.093	25561403	36258969	15.713	16.471
Target Compounds							
23)	Chlordane-1	4.323	0.000	3185350	0	64.330	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
Data File : PL061934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 12:56
Operator : DD\AJ
Sample : L4190-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 17:41:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

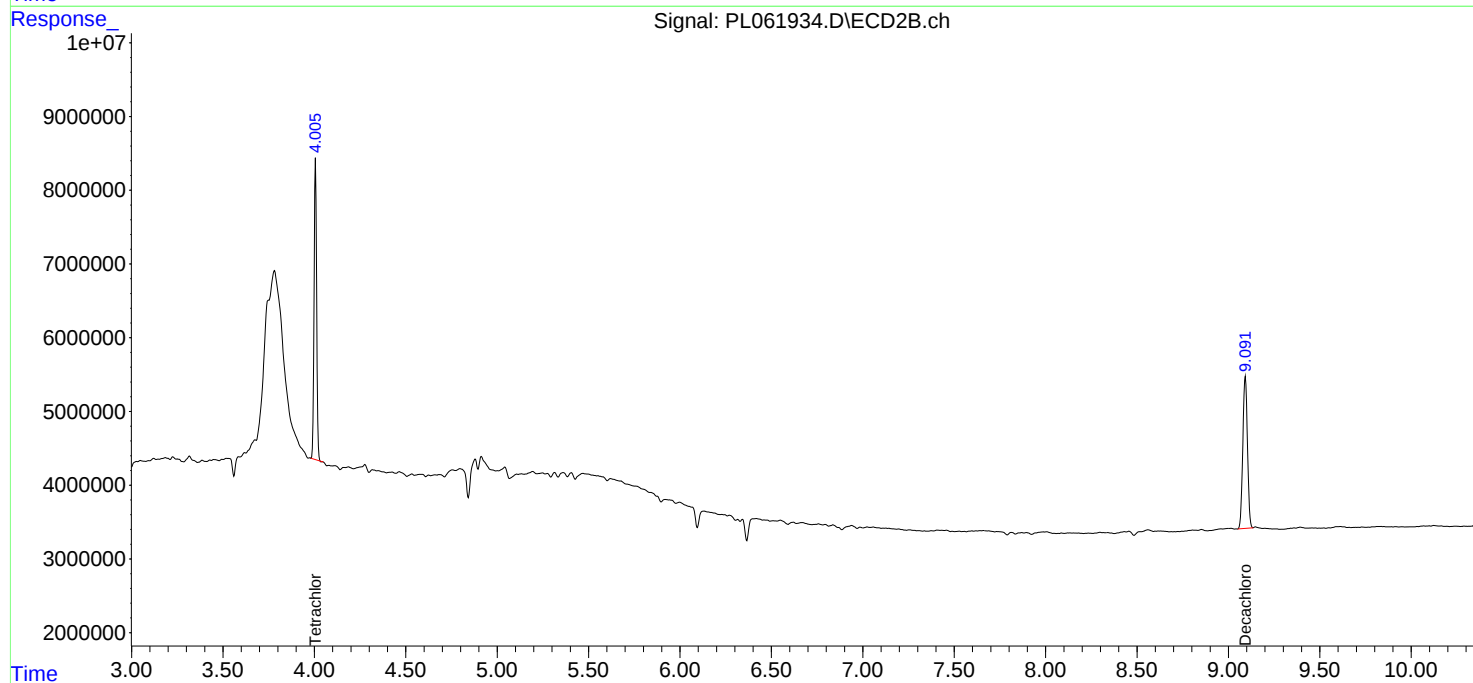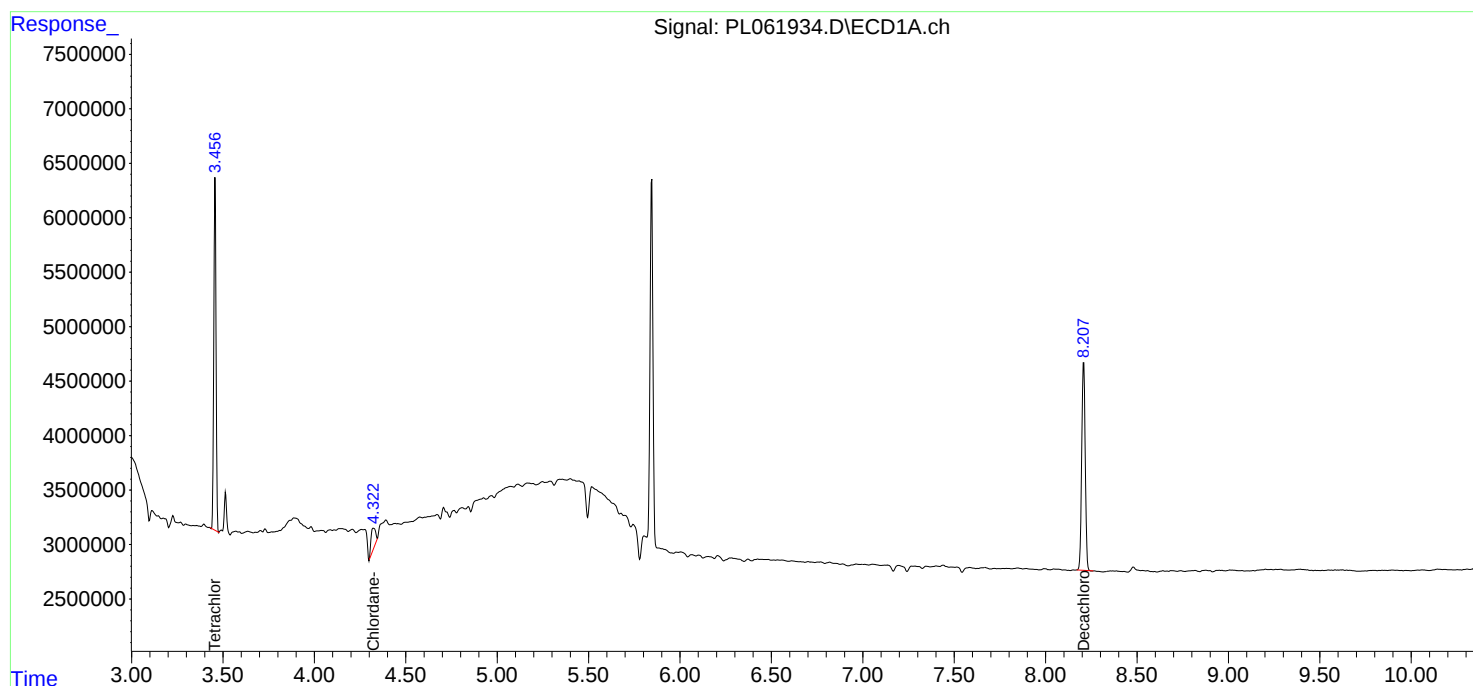


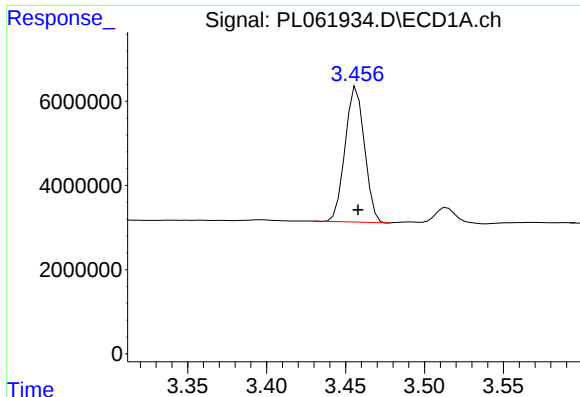

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 27566840
Conc: 16.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

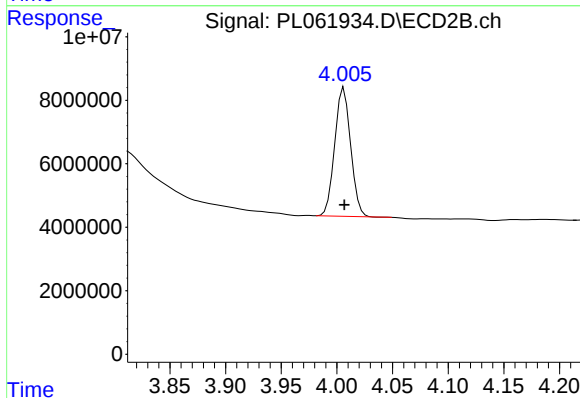


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 40313533
Conc: 14.78 ng/ml

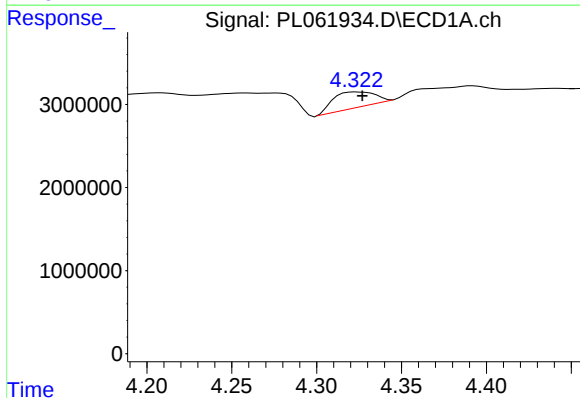


#23 Chlordane-1

R.T.: 4.323 min
Delta R.T.: -0.004 min
Response: 3185350
Conc: 64.33 ng/ml

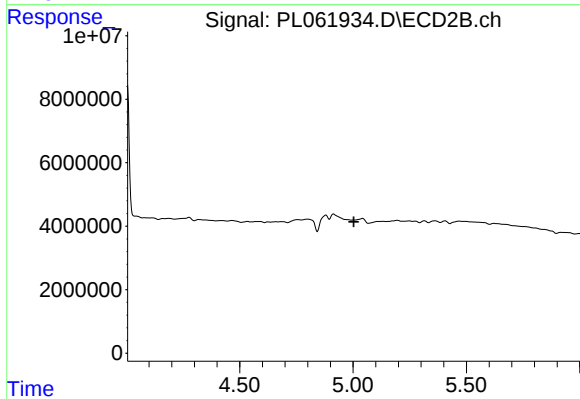

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.004 min
Response: 0
Conc: N.D.

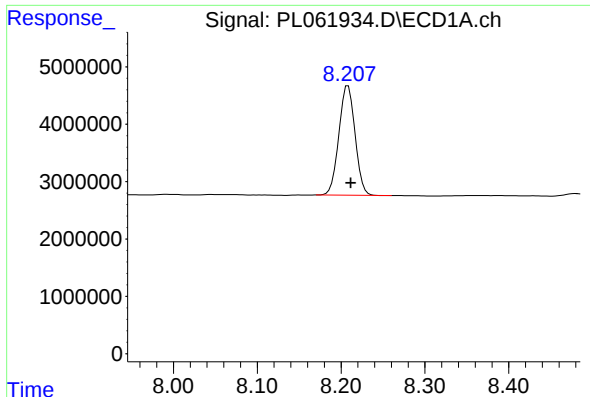

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.003 min
Response: 25561403
Conc: 15.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

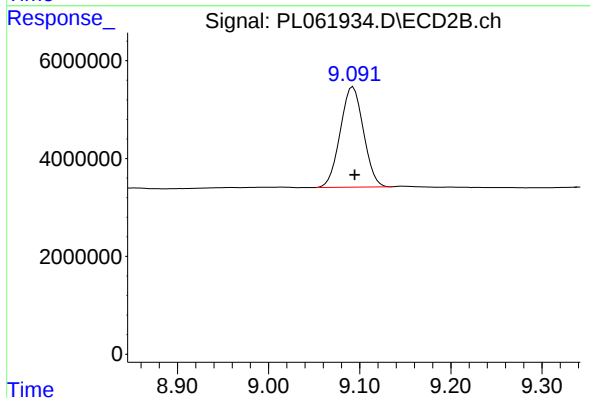

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.002 min
Response: 36258969
Conc: 16.47 ng/ml