

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
 Data File : PL061935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 13:11
 Operator : DD\AJ
 Sample : L4190-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 17:41:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.006	37874827	55518144	22.201	20.349
28)	SA Decachlor...	8.208	9.093	29813764	41941868	18.327	19.053
Target Compounds							
3)	MA gamma-BHC...	0.000	4.695	0	2522317	N.D.	0.681 #
9)	A Endosulfan I	5.524f	0.000	5614266	0	3.465	N.D. #
10)	B gamma-Chl...	5.392	0.000	58168008	0	33.494	N.D. #
15)	B Endosulfa...	0.000	6.944	0	6940442	N.D.	2.685 #
23)	Chlordane-1	4.330	0.000	1870161	0	37.769	N.D. #
25)	Chlordane-3	5.392	0.000	58168008	0	370.068	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
Data File : PL061935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 13:11
Operator : DD\AJ
Sample : L4190-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 17:41:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

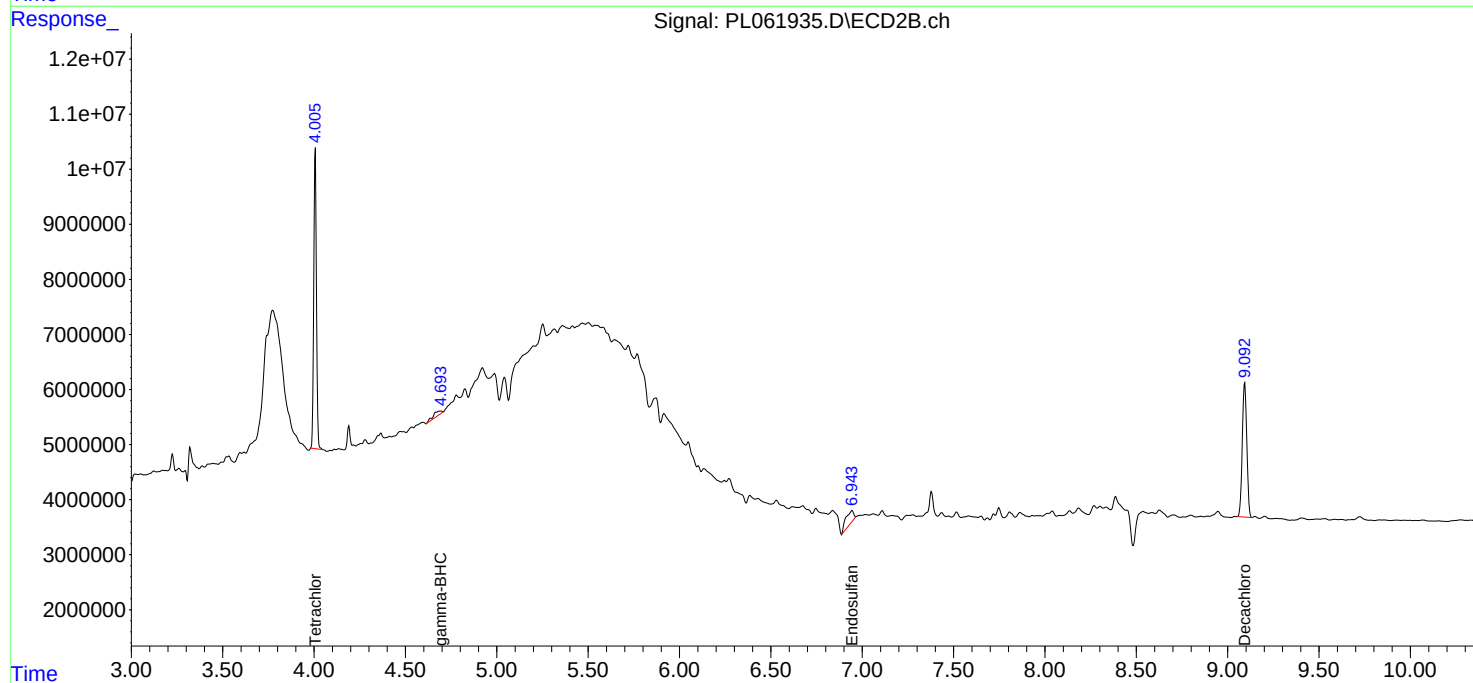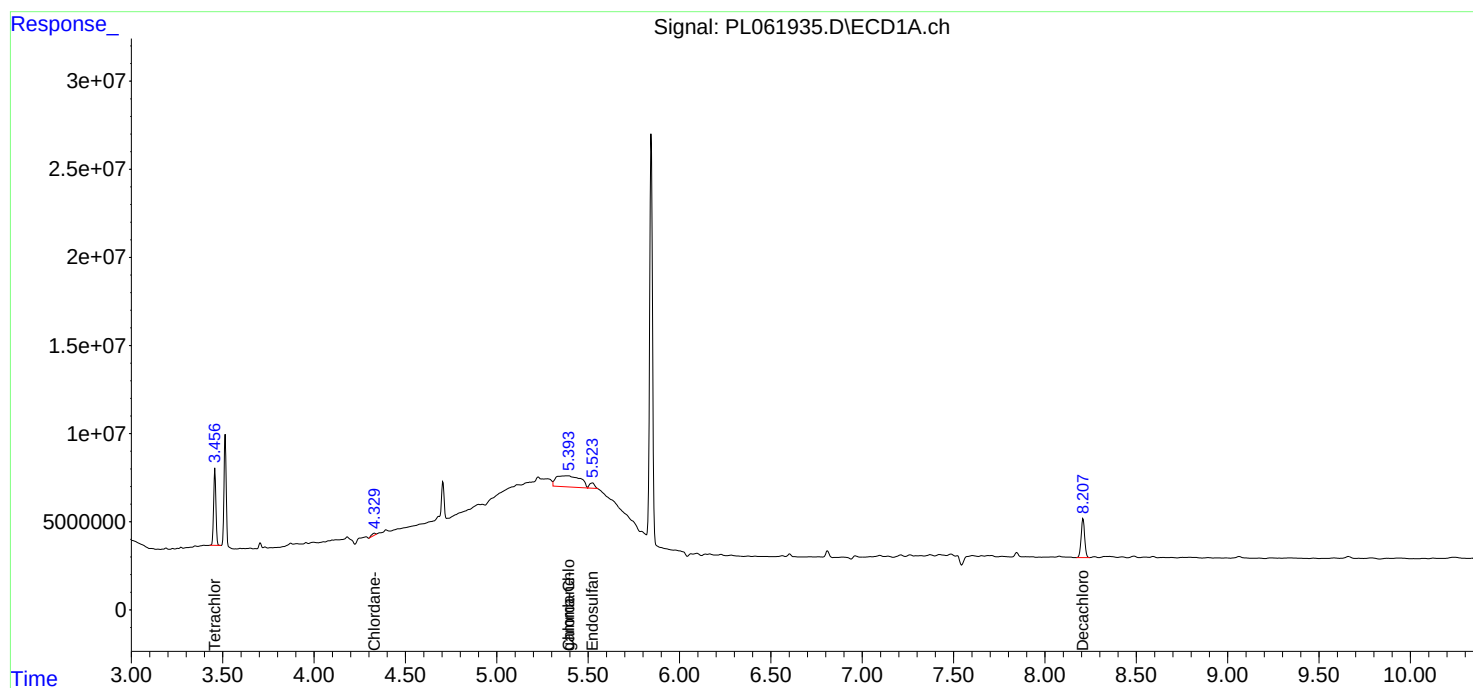


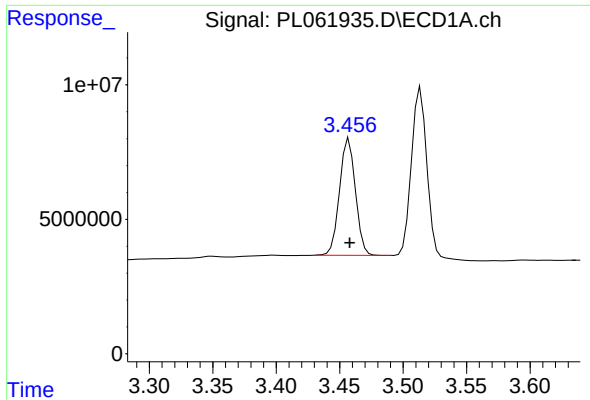

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 37874827
Conc: 22.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

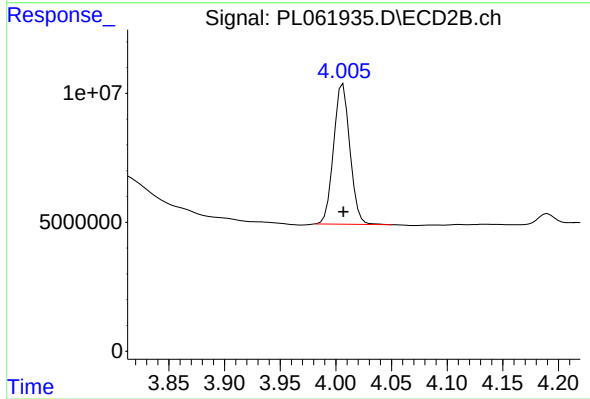


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 55518144
Conc: 20.35 ng/ml

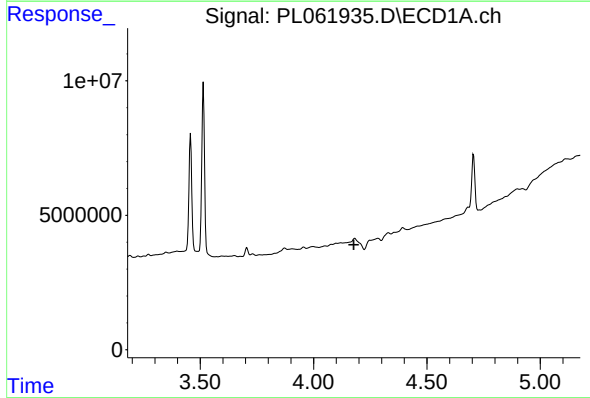


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.177 min
Response: 0
Conc: N.D.

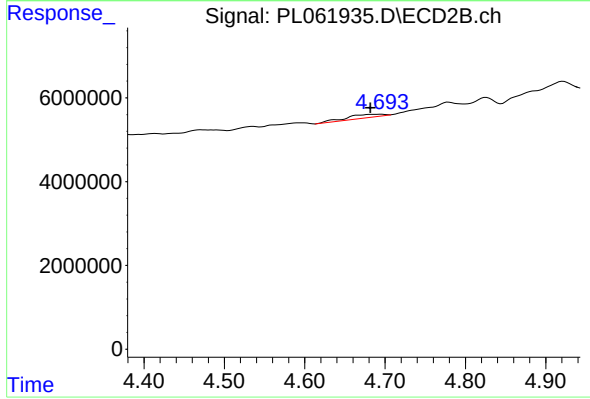

#3 gamma-BHC (Lindane)


R.T.: 4.695 min
Delta R.T.: 0.014 min
Response: 2522317
Conc: 0.68 ng/ml

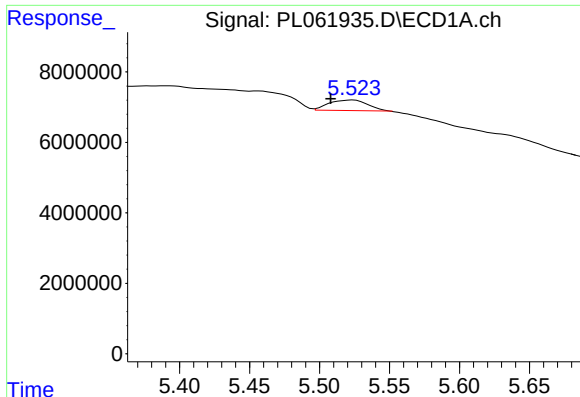

#9 Endosulfan I


R.T.: 5.524 min
Delta R.T.: 0.016 min
Response: 5614266
Conc: 3.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

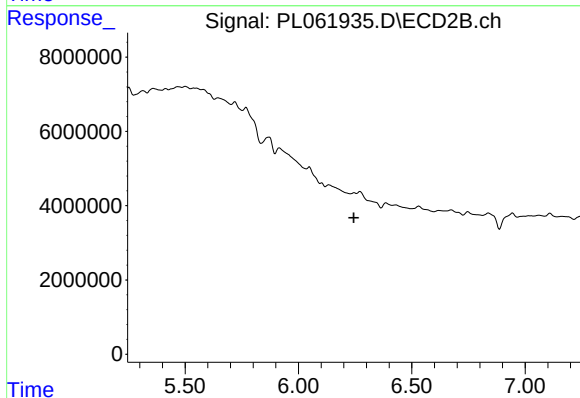


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

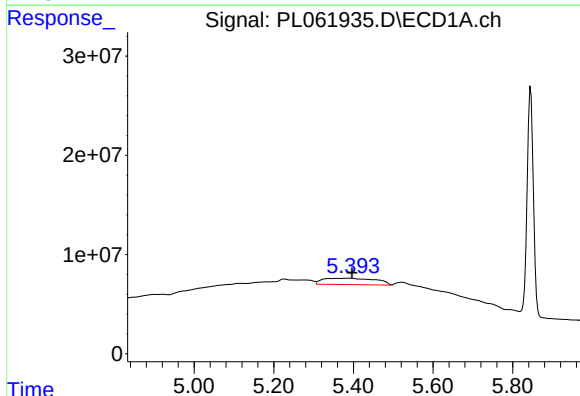


#10 gamma-Chlordane

R.T.: 5.392 min
Delta R.T.: -0.004 min
Response: 58168008
Conc: 33.49 ng/ml

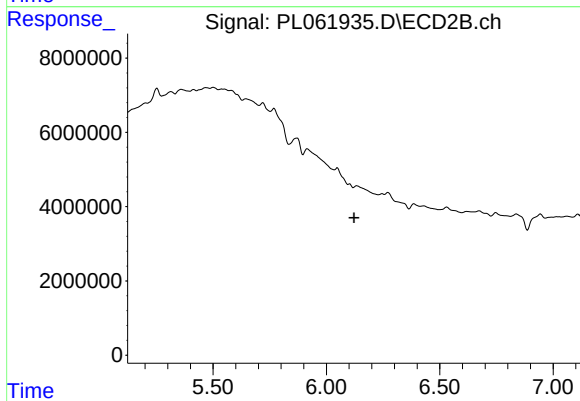

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

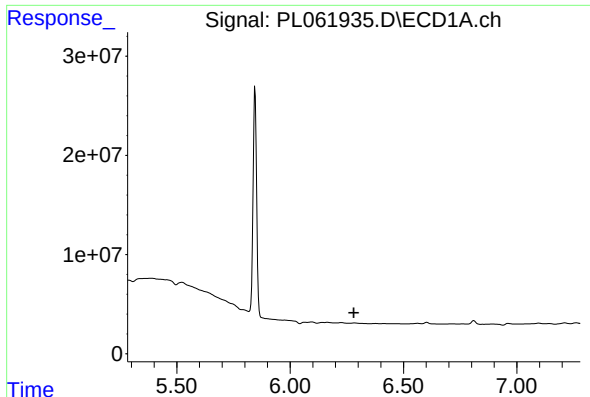

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

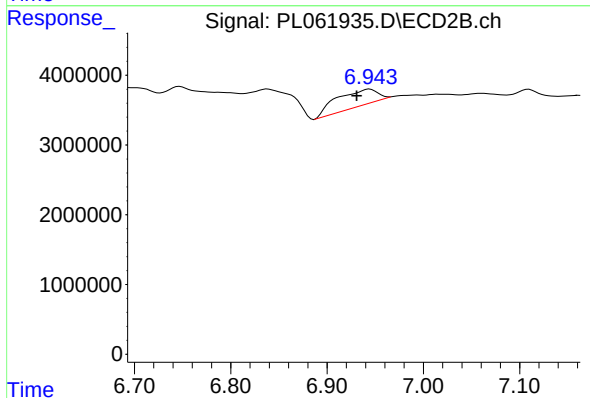


#15 Endosulfan II

R.T.: 6.944 min
Delta R.T.: 0.013 min
Response: 6940442
Conc: 2.69 ng/ml

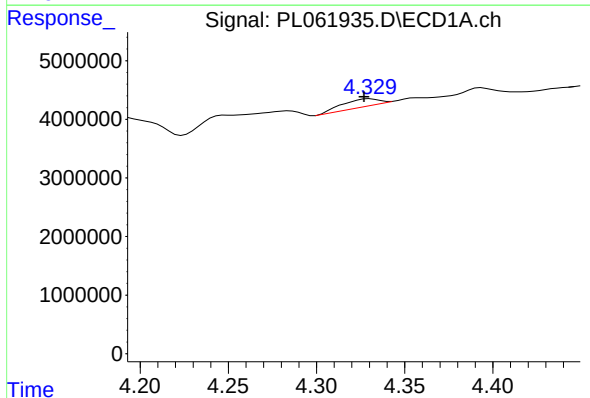


#23 Chlordane-1

R.T.: 4.330 min
Delta R.T.: 0.003 min
Response: 1870161
Conc: 37.77 ng/ml

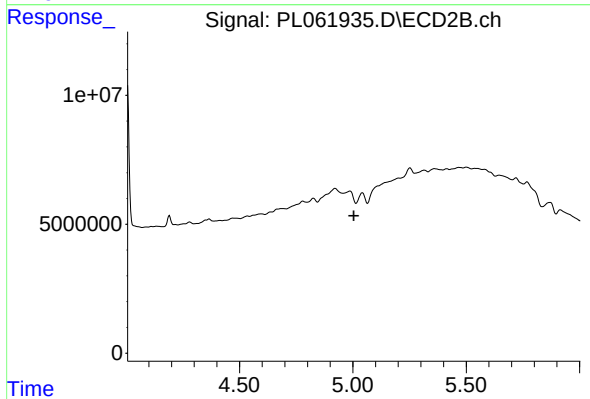

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.004 min
Response: 0
Conc: N.D.

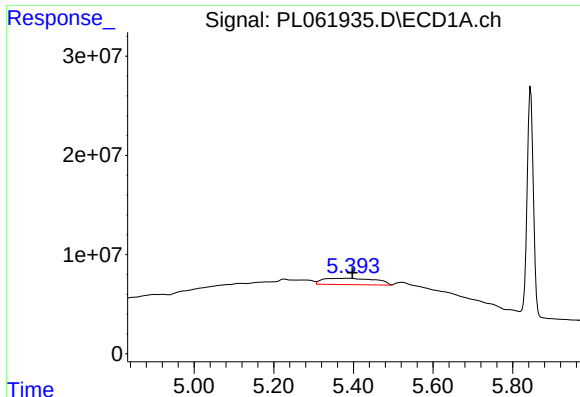

#25 Chlordane-3


R.T.: 5.392 min
Delta R.T.: -0.005 min
Response: 58168008
Conc: 370.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

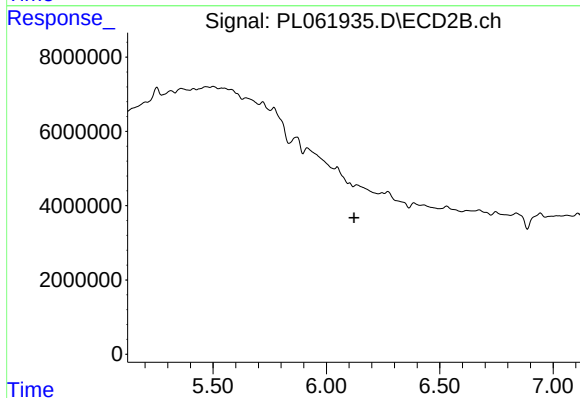


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

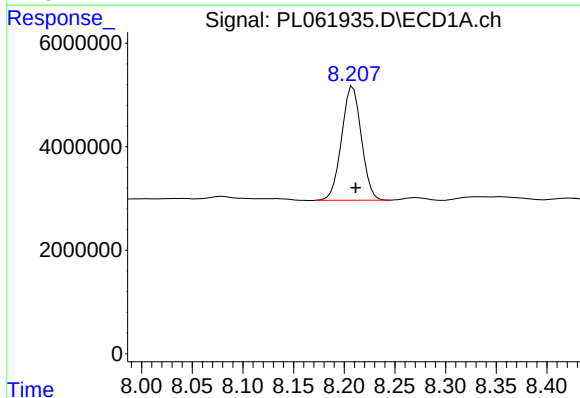

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.003 min
Response: 29813764
Conc: 18.33 ng/ml

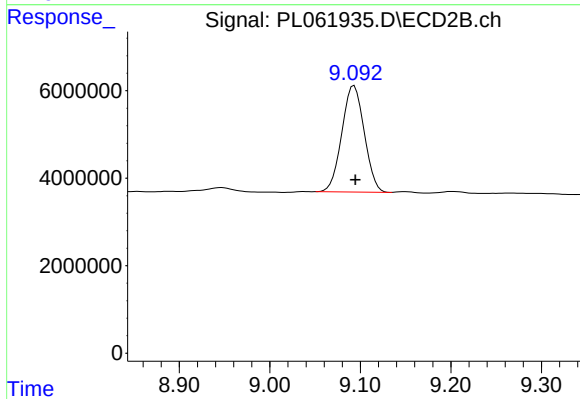

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.002 min
Response: 41941868
Conc: 19.05 ng/ml