

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
 Data File : PL061940.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 14:21
 Operator : DD\AJ
 Sample : L4190-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 17:42:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	27288917	39238153	15.996	14.382
28)	SA Decachlor...	8.209	9.094	22663669	34289096	13.932	15.576
Target Compounds							
6)	B beta-BHC	0.000	4.880f	0	1015605	N.D.	0.673 #
9)	A Endosulfan I	5.520	0.000	6595119	0	4.070	N.D. #
10)	B gamma-Chl...	0.000	6.125	0	3718896	N.D.	1.266 #
17)	MA 4,4'-DDT	6.374	7.143	2519632	4204305	1.997	1.920
23)	Chlordane-1	4.324	0.000	3965848	0	80.092	N.D. #
25)	Chlordane-3	0.000	6.125	0	3718896	N.D.	10.149 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
Data File : PL061940.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 14:21
Operator : DD\AJ
Sample : L4190-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 17:42:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

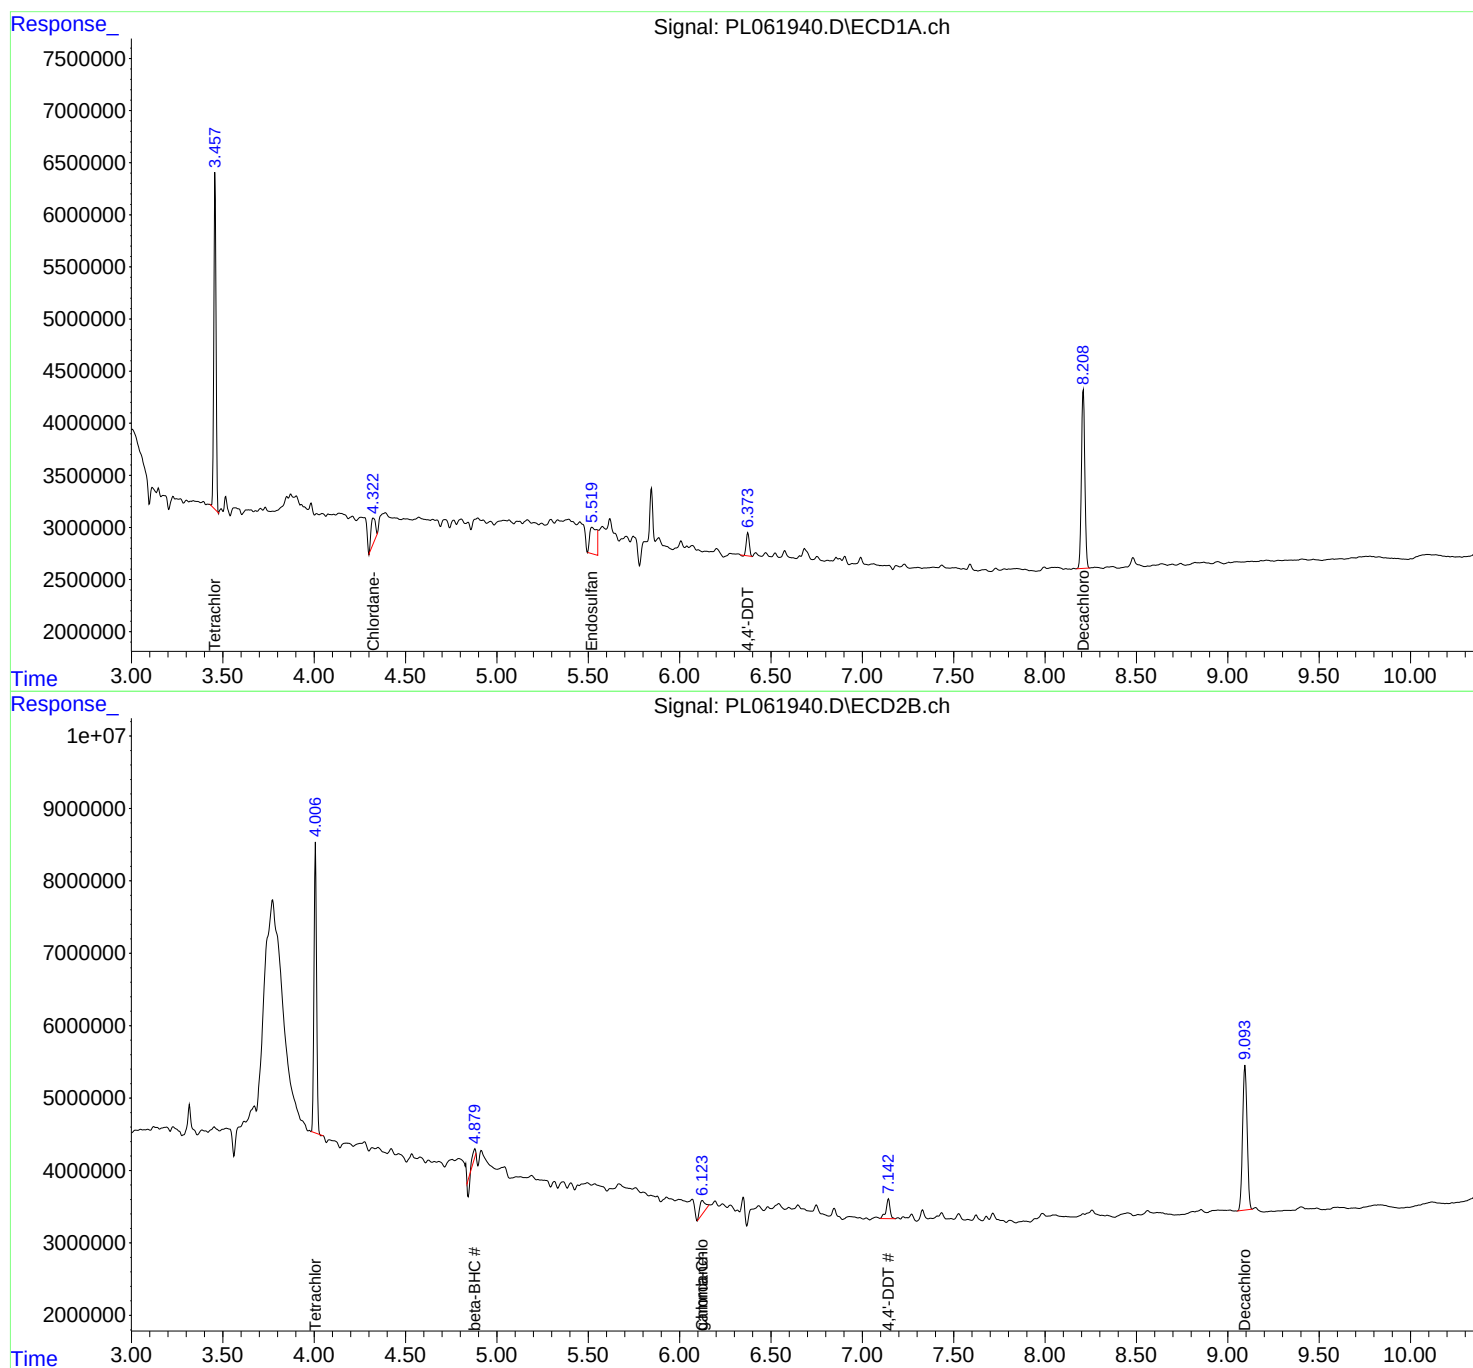


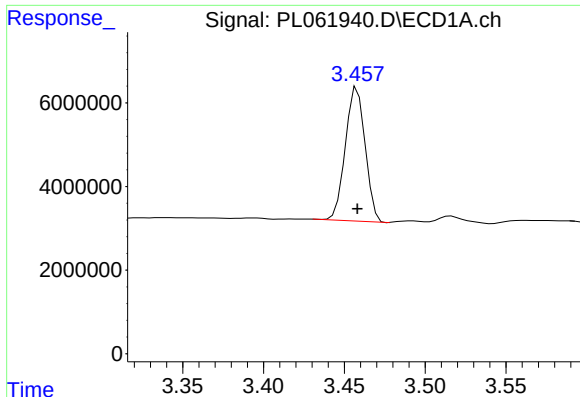

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 27288917
Conc: 16.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

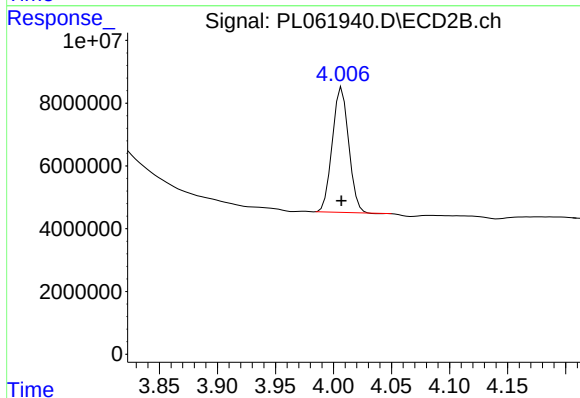


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 39238153
Conc: 14.38 ng/ml

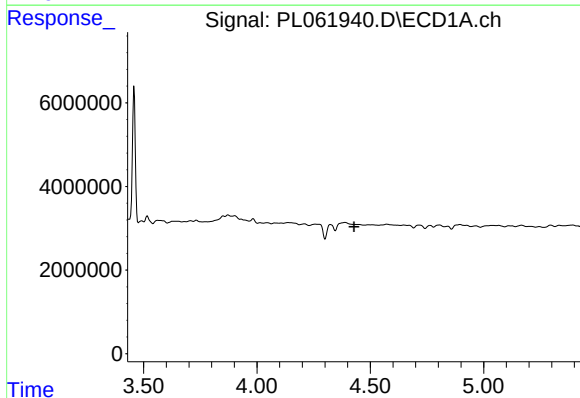


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.428 min
Response: 0
Conc: N.D.

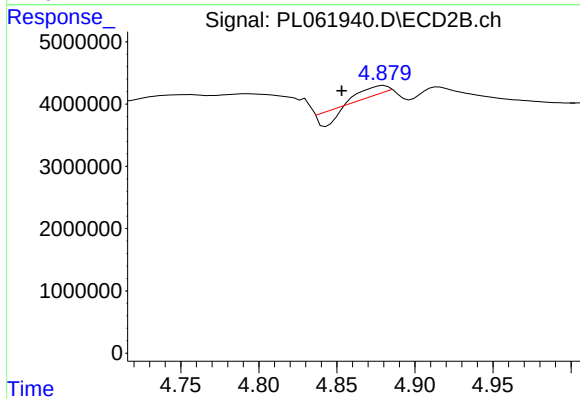

#6 beta-BHC


R.T.: 4.880 min
Delta R.T.: 0.027 min
Response: 1015605
Conc: 0.67 ng/ml

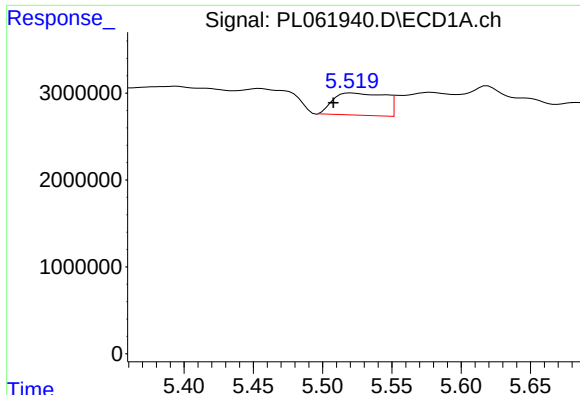

#9 Endosulfan I


R.T.: 5.520 min
Delta R.T.: 0.013 min
Response: 6595119
Conc: 4.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

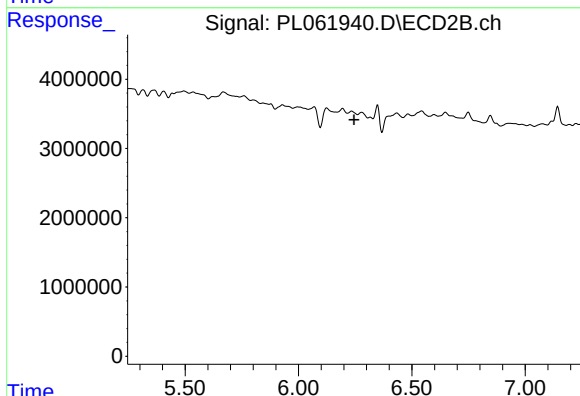


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

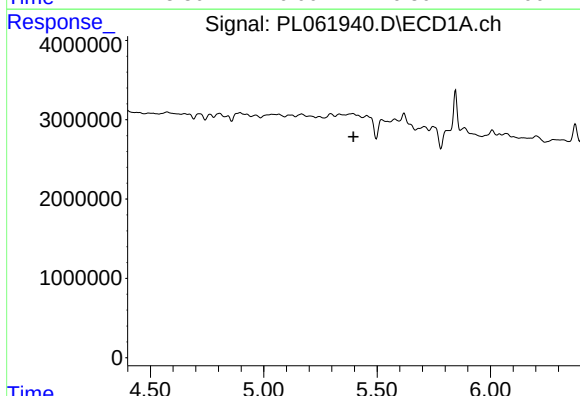


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

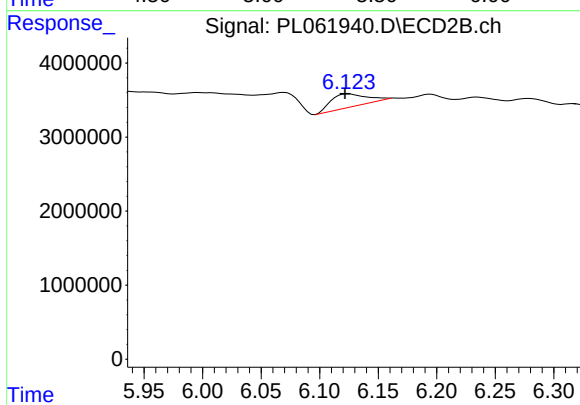

#10 gamma-Chlordane


R.T.: 6.125 min
Delta R.T.: 0.003 min
Response: 3718896
Conc: 1.27 ng/ml

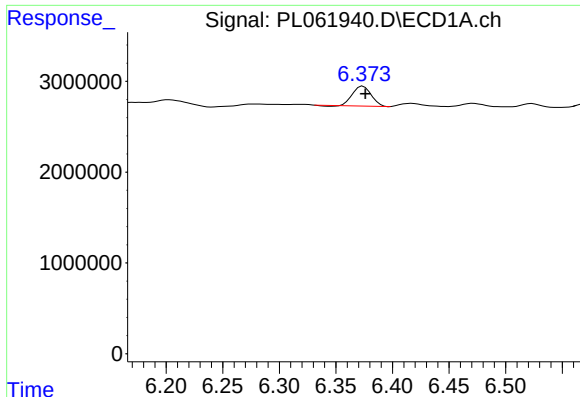

#17 4,4'-DDT


R.T.: 6.374 min
Delta R.T.: -0.002 min
Response: 2519632
Conc: 2.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

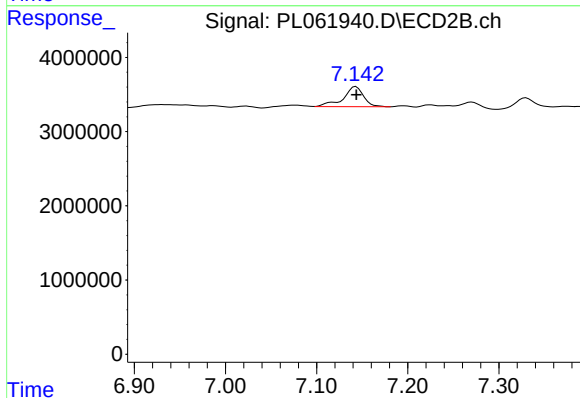


#17 4,4'-DDT

R.T.: 7.143 min
Delta R.T.: 0.000 min
Response: 4204305
Conc: 1.92 ng/ml

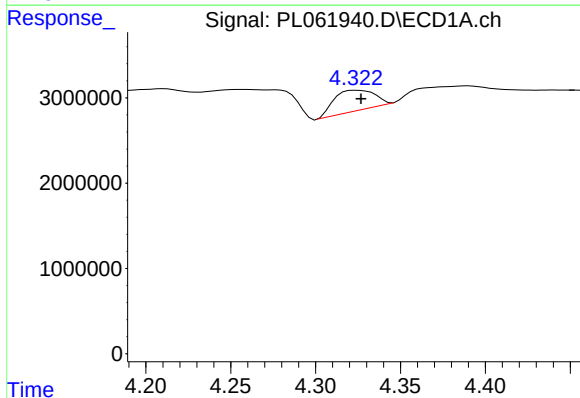


#23 Chlordane-1

R.T.: 4.324 min
Delta R.T.: -0.003 min
Response: 3965848
Conc: 80.09 ng/ml

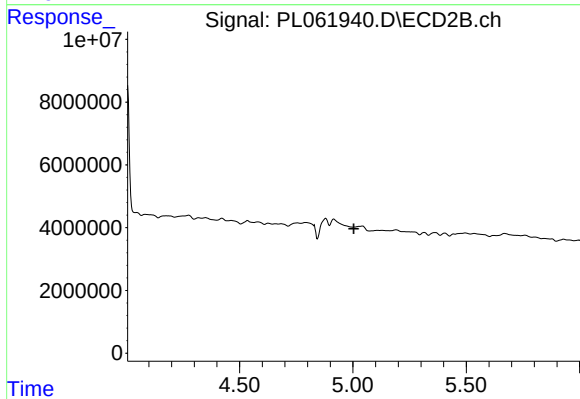

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.004 min
Response: 0
Conc: N.D.

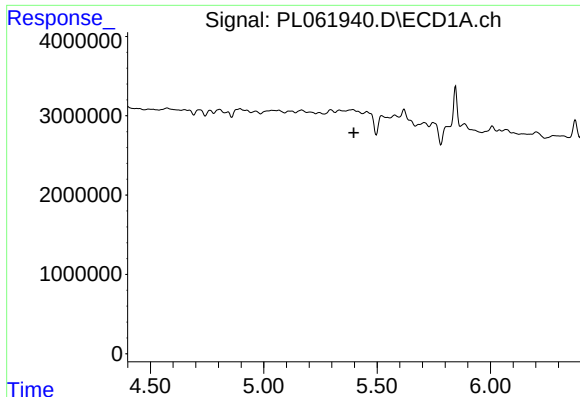

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

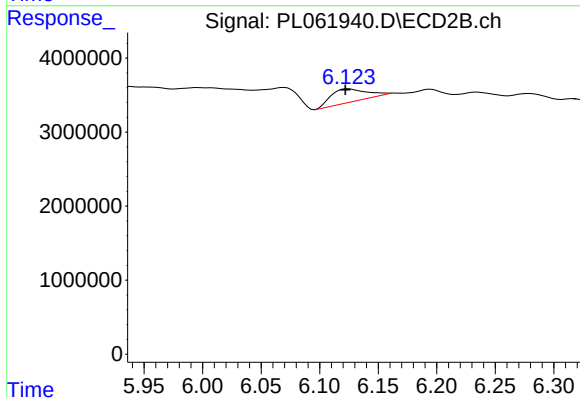


#25 Chlordane-3

R.T.: 6.125 min
Delta R.T.: 0.003 min
Response: 3718896
Conc: 10.15 ng/ml

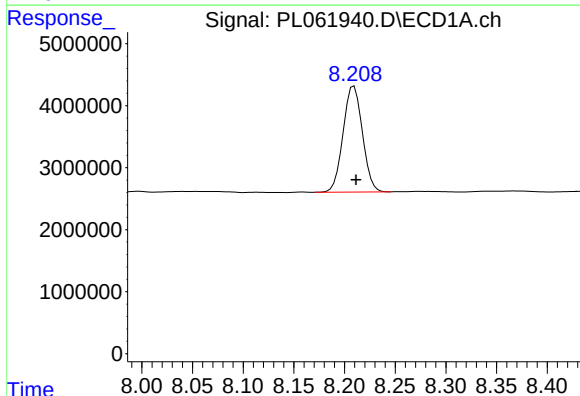

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 22663669
Conc: 13.93 ng/ml

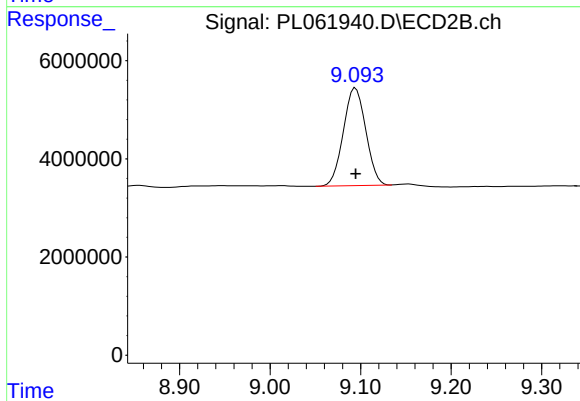

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 34289096
Conc: 15.58 ng/ml