

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
 Data File : PL061945.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 15:32
 Operator : DD\AJ
 Sample : L4221-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 17:43:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	25289802	36636715	14.824	13.429
28)	SA Decachlor...	8.209	9.095	21738056	30774681	13.363	13.980
Target Compounds							
10)	B gamma-Chl...	0.000	6.122	0	4442508	N.D.	1.513 #
11)	B alpha-Chl...	0.000	6.196	0	5309327	N.D.	1.768 #
25)	Chlordane-3	0.000	6.122	0	4442508	N.D.	12.124 #
26)	Chlordane-4	0.000	6.196	0	5309327	N.D.	11.827 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
Data File : PL061945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 15:32
Operator : DD\AJ
Sample : L4221-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 17:43:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

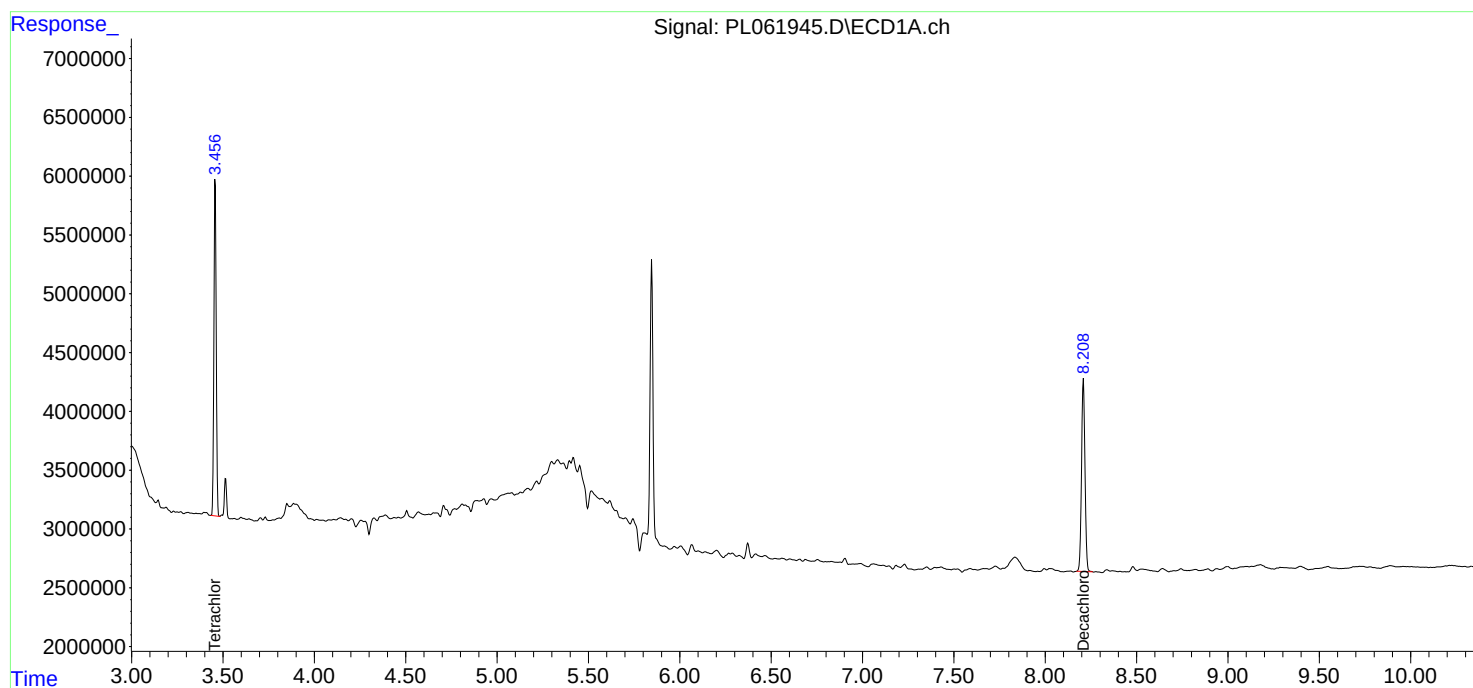


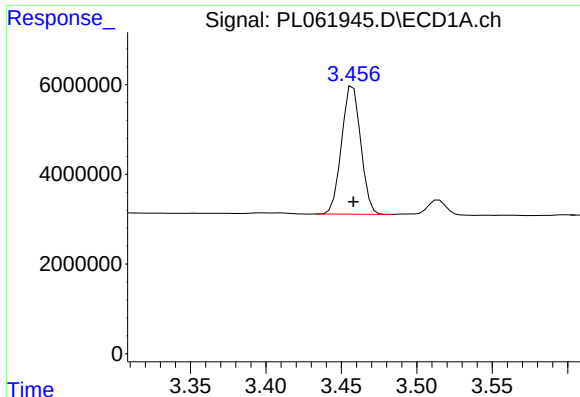

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 25289802
Conc: 14.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

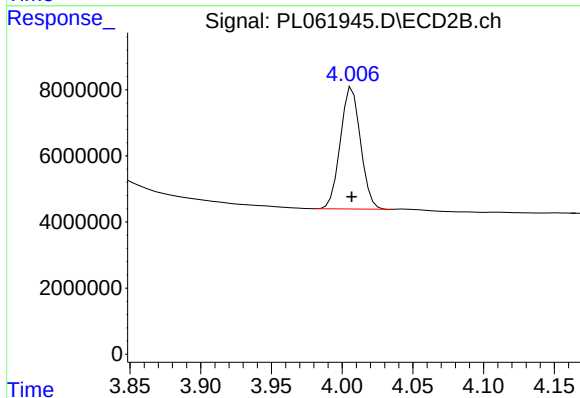


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 36636715
Conc: 13.43 ng/ml

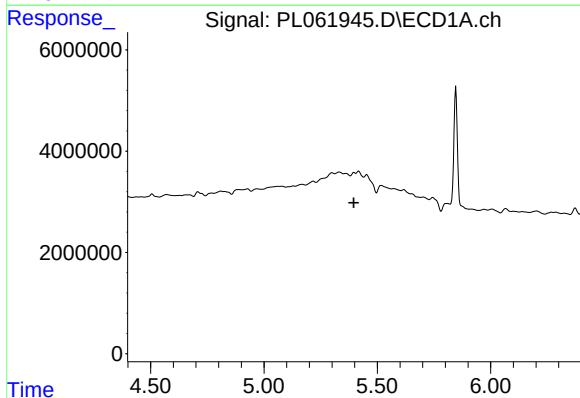


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

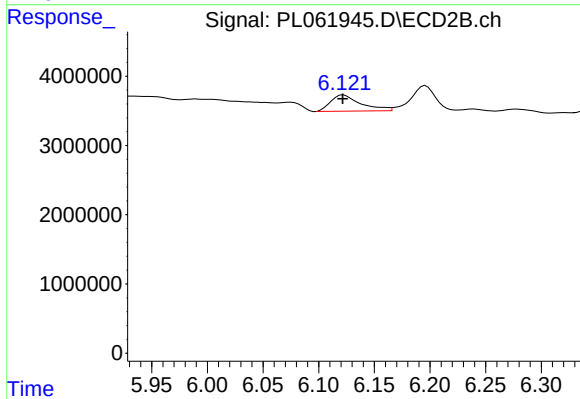

#10 gamma-Chlordane


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 4442508
Conc: 1.51 ng/ml

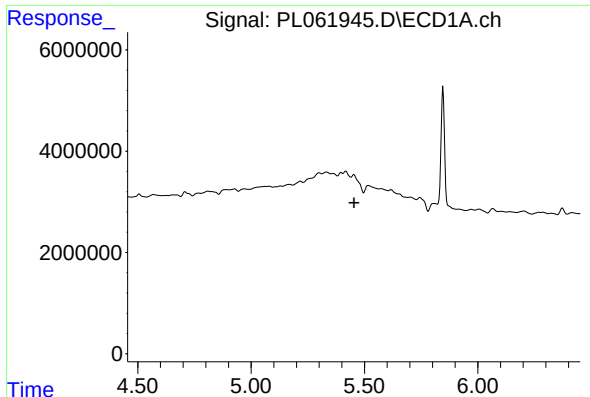

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

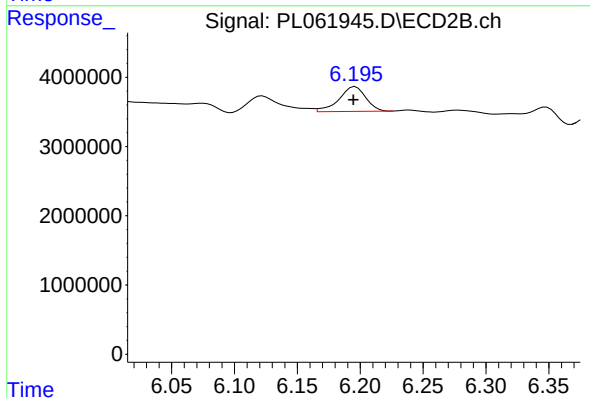


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: 0.001 min
Response: 5309327
Conc: 1.77 ng/ml

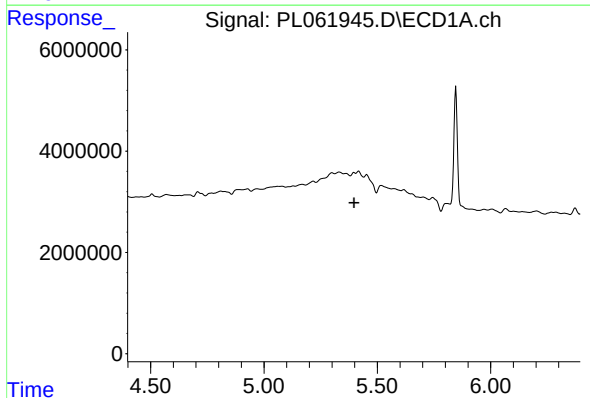


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

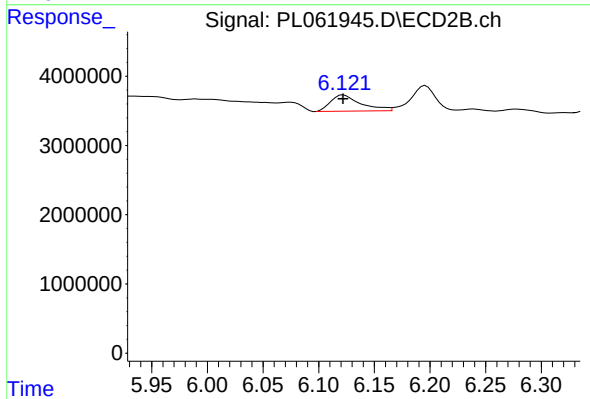

#25 Chlordane-3


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 4442508
Conc: 12.12 ng/ml

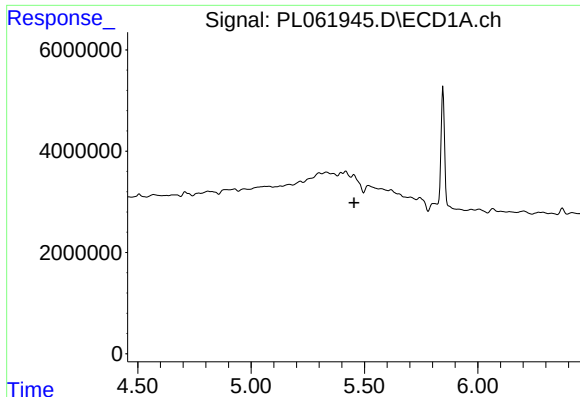

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

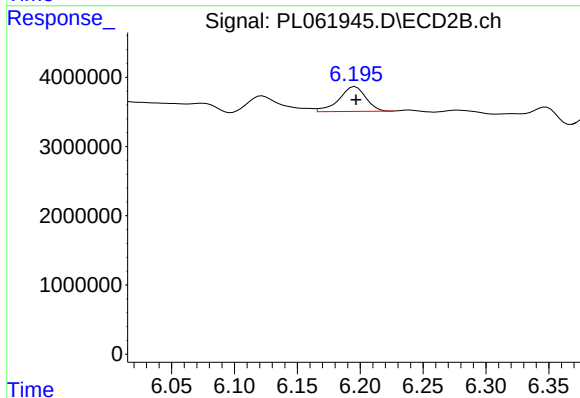


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 5309327
Conc: 11.83 ng/ml

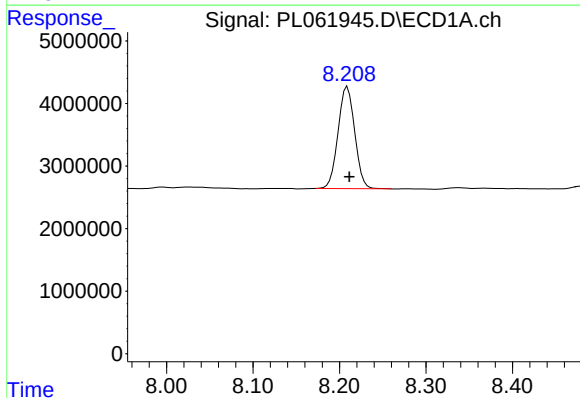

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 21738056
Conc: 13.36 ng/ml

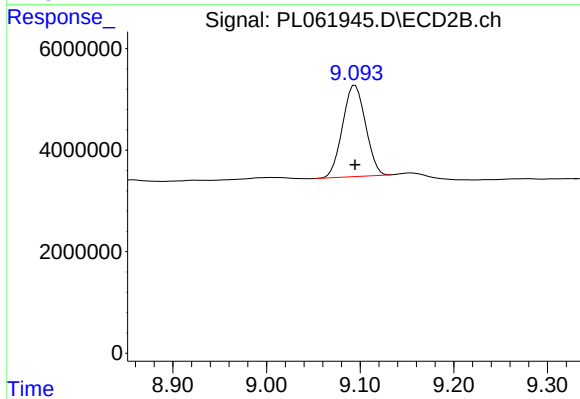

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 30774681
Conc: 13.98 ng/ml