

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
 Data File : PL061946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 15:46
 Operator : DD\AJ
 Sample : L4226-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 17:43:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	23501666	32647296	13.776	11.966
28)	SA Decachlor...	8.209	9.093	22537906	31691509	13.854	14.396
Target Compounds							
10)	B gamma-Chl...	5.418f	0.000	2772941	0	1.597	N.D. #
11)	B alpha-Chl...	0.000	6.195	0	4057183	N.D.	1.351 #
16)	A 4,4'-DDD	0.000	6.848	0	4339650	N.D.	1.952 #
17)	MA 4,4'-DDT	6.372	7.116f	2101238	5246680	1.666	2.396 #
25)	Chlordane-3	5.418f	0.000	2772941	0	17.642	N.D. #
26)	Chlordane-4	0.000	6.195	0	4057183	N.D.	9.038 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
Data File : PL061946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 15:46
Operator : DD\AJ
Sample : L4226-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 17:43:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

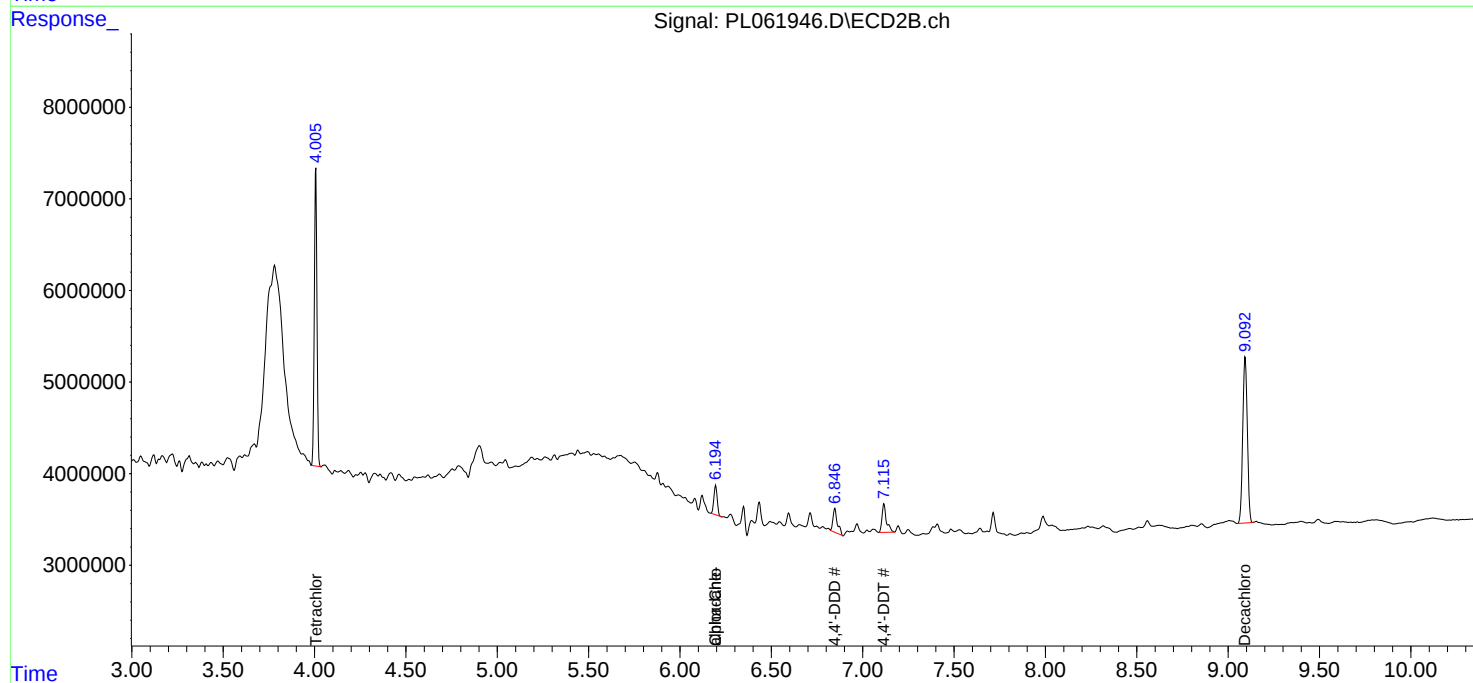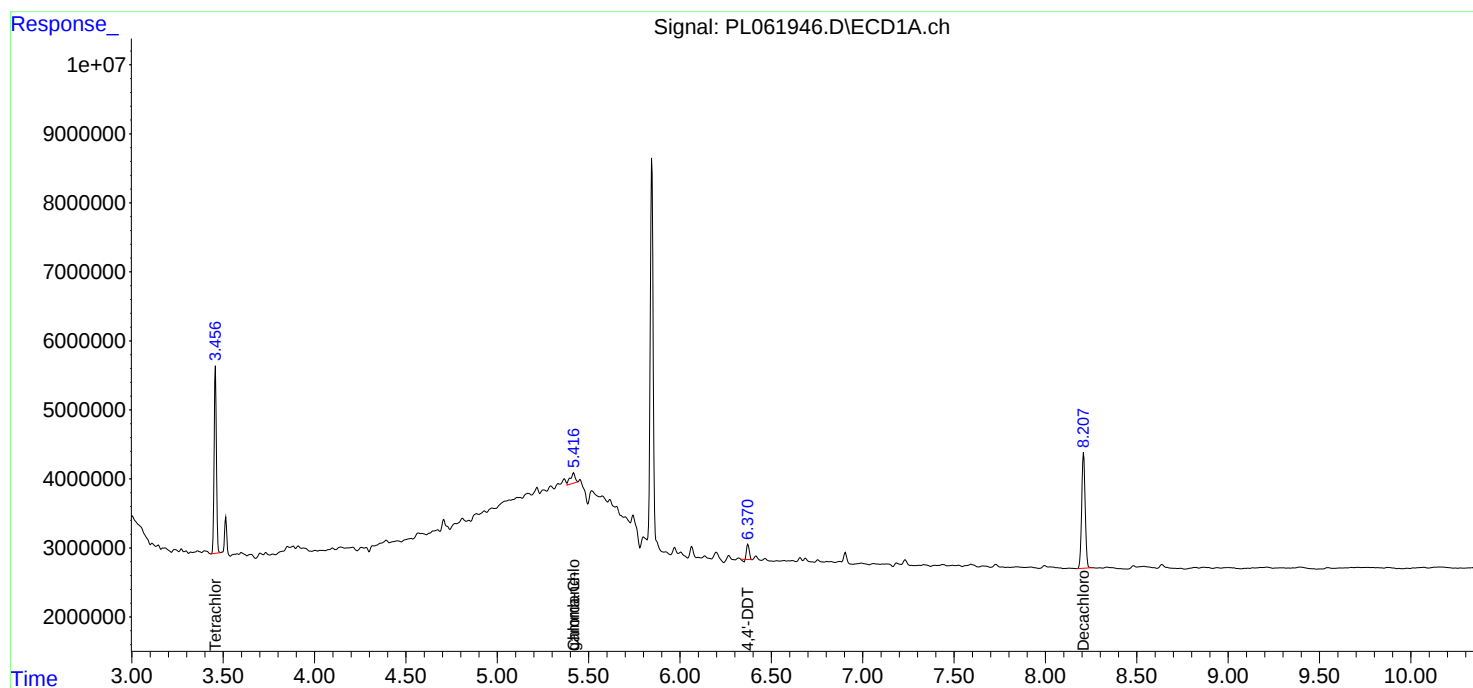


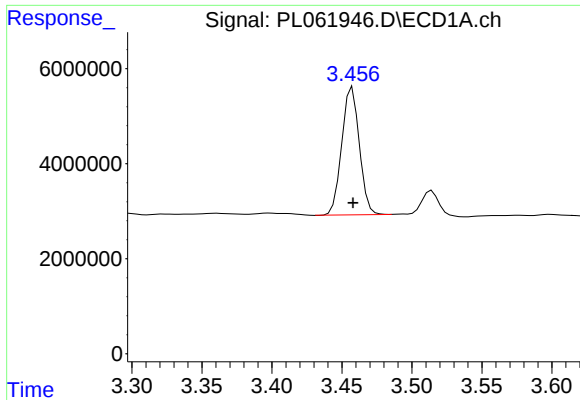

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 23501666
Conc: 13.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

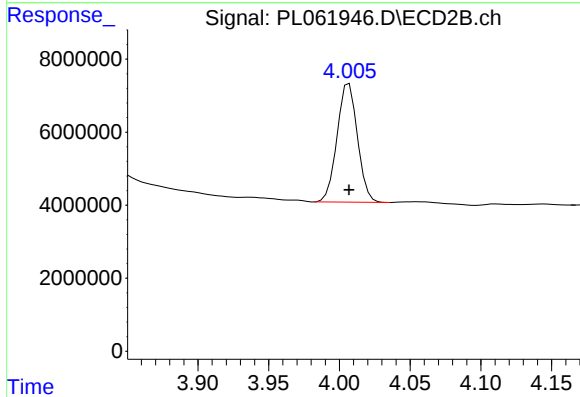


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 32647296
Conc: 11.97 ng/ml

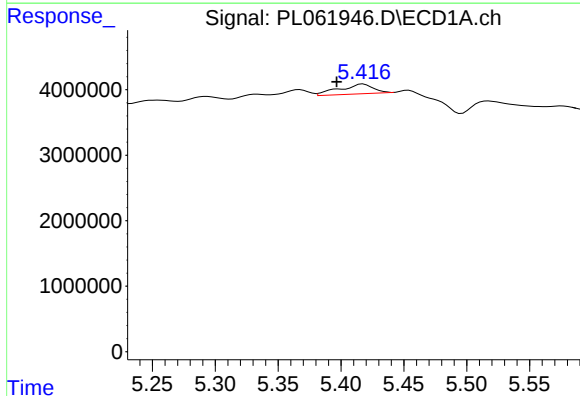


#10 gamma-Chlordane

R.T.: 5.418 min
Delta R.T.: 0.021 min
Response: 2772941
Conc: 1.60 ng/ml

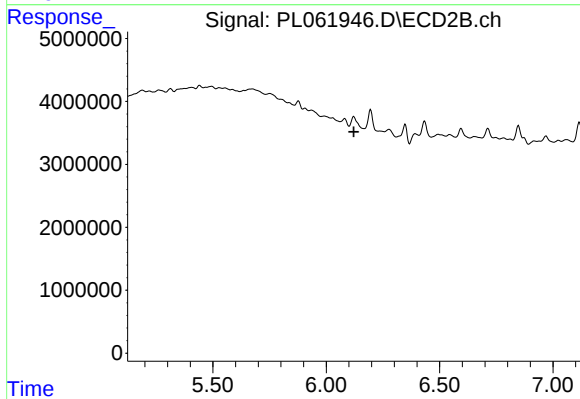

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.122 min
Response: 0
Conc: N.D.

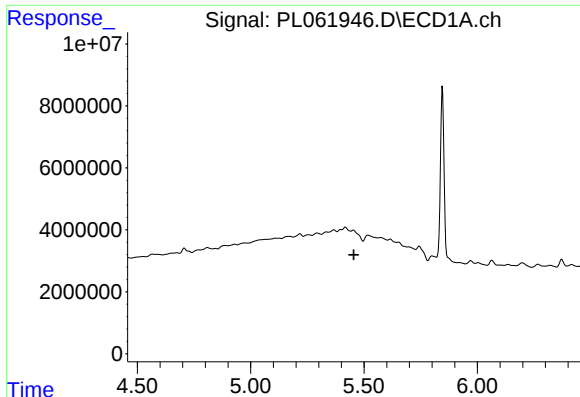

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

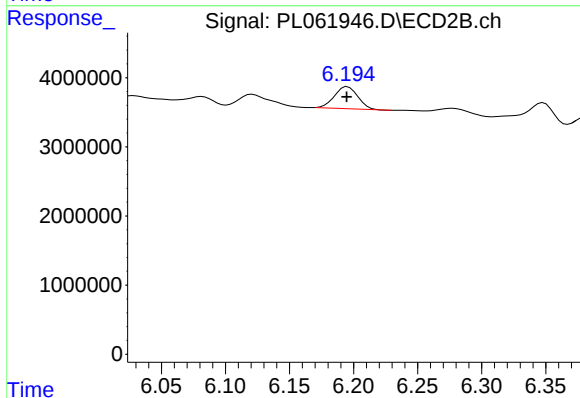


#11 alpha-Chlordane

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 4057183
Conc: 1.35 ng/ml

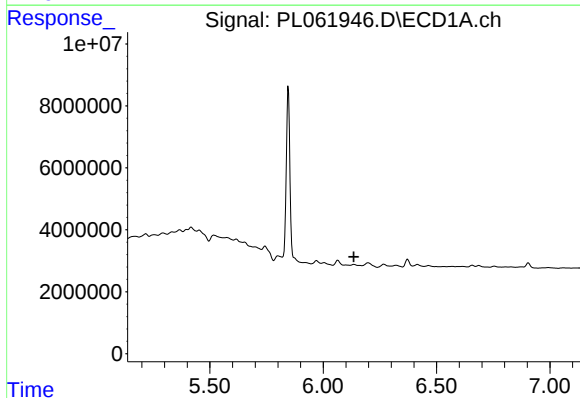


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.135 min
Response: 0
Conc: N.D.

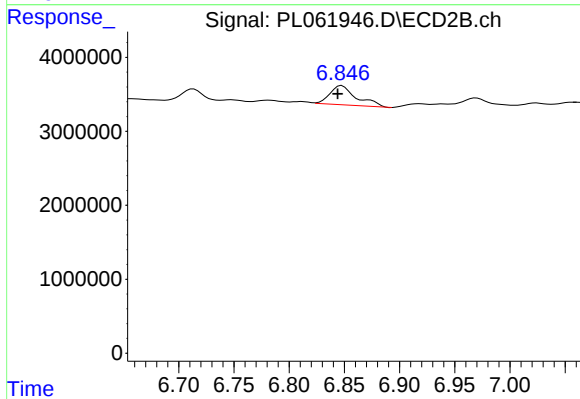

#16 4,4'-DDD


R.T.: 6.848 min
Delta R.T.: 0.004 min
Response: 4339650
Conc: 1.95 ng/ml

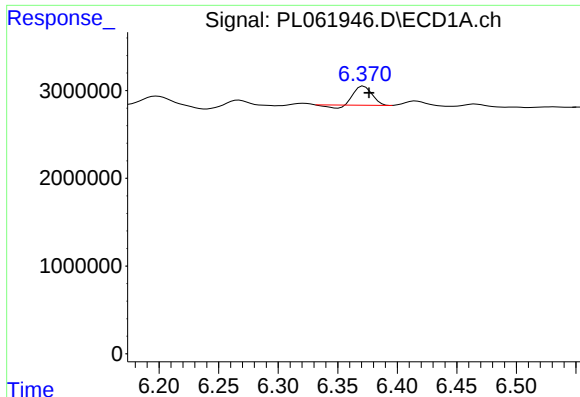

#17 4,4'-DDT


R.T.: 6.372 min
Delta R.T.: -0.004 min
Response: 2101238
Conc: 1.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

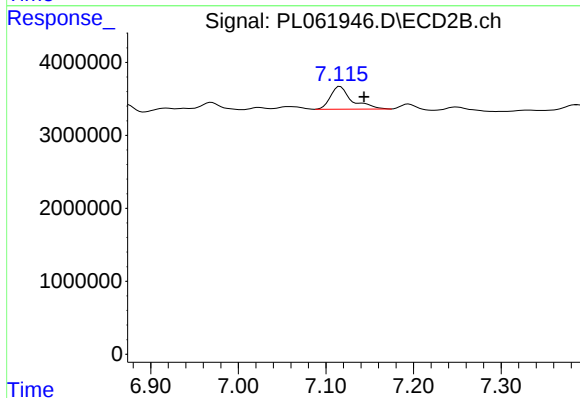


#17 4,4'-DDT

R.T.: 7.116 min
Delta R.T.: -0.027 min
Response: 5246680
Conc: 2.40 ng/ml

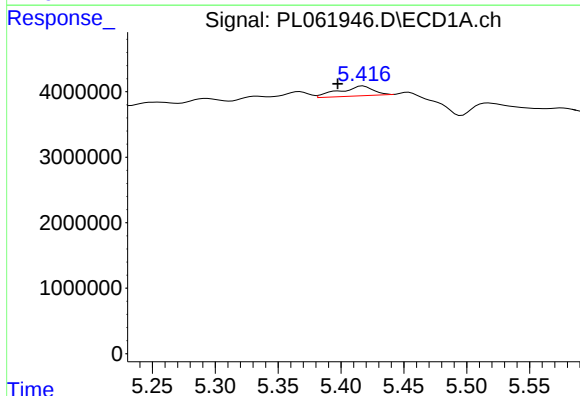


#25 Chlordane-3

R.T.: 5.418 min
Delta R.T.: 0.020 min
Response: 2772941
Conc: 17.64 ng/ml

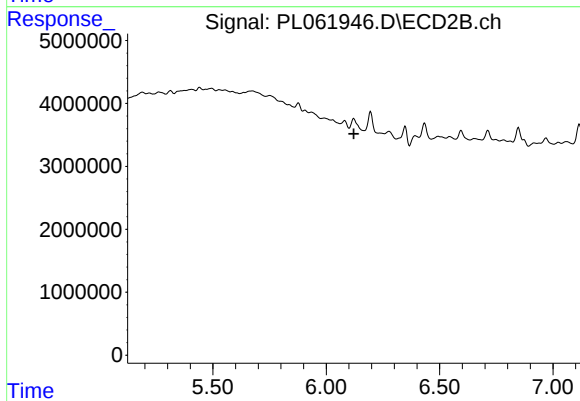

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.122 min
Response: 0
Conc: N.D.

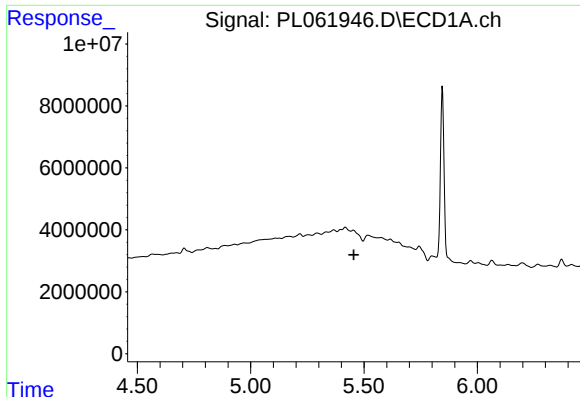

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

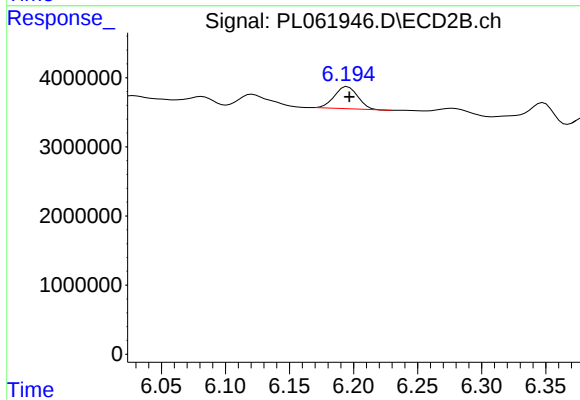


#26 Chlordane-4

R.T.: 6.195 min
Delta R.T.: -0.001 min
Response: 4057183
Conc: 9.04 ng/ml

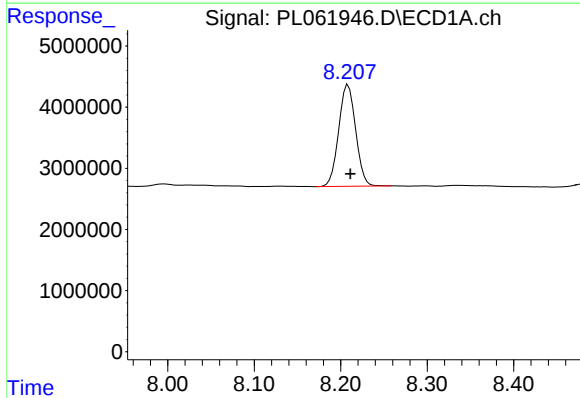

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.003 min
Response: 22537906
Conc: 13.85 ng/ml

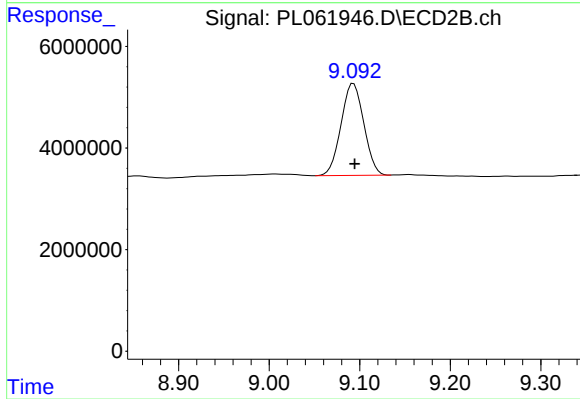

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.002 min
Response: 31691509
Conc: 14.40 ng/ml