

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
 Data File : PL061926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 10:00
 Operator : DD\AJ
 Sample : L4189-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-C-2334-C

Manual Integrations
 APPROVED

Ankita
 10/5/2020 3:33:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 15:54:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	28535036	44375730	16.727	16.265
28)	SA Decachlor...	8.210	9.093	29334553	40981641	18.033	18.616
Target Compounds							
10)	B gamma-Chl...	5.394	6.122	858975	3287240	0.495m	1.119 #
11)	B alpha-Chl...	5.452	6.194	1394866	3906613	0.803m	1.301m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
Data File : PL061926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 10:00
Operator : DD\AJ
Sample : L4189-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-C-2334-C


Manual Integrations
APPROVED

Ankita
10/5/2020 3:33:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 15:54:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

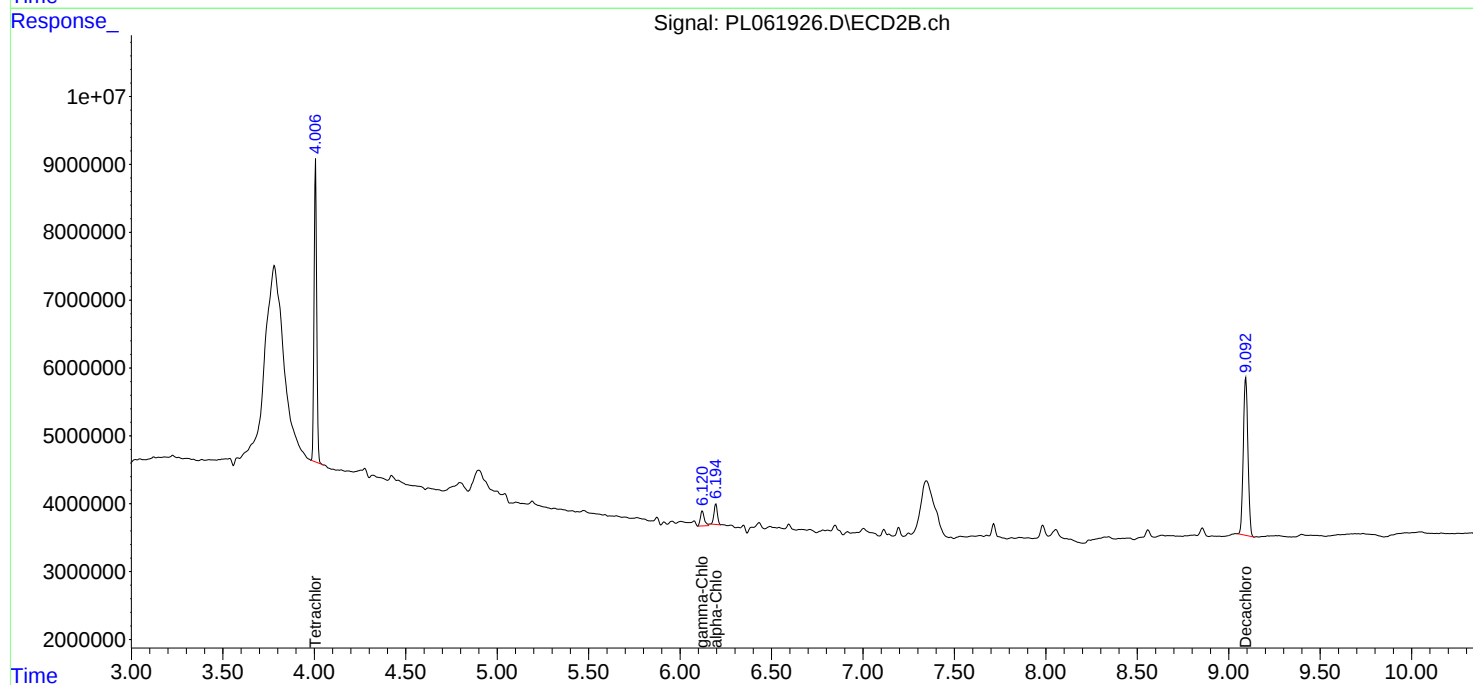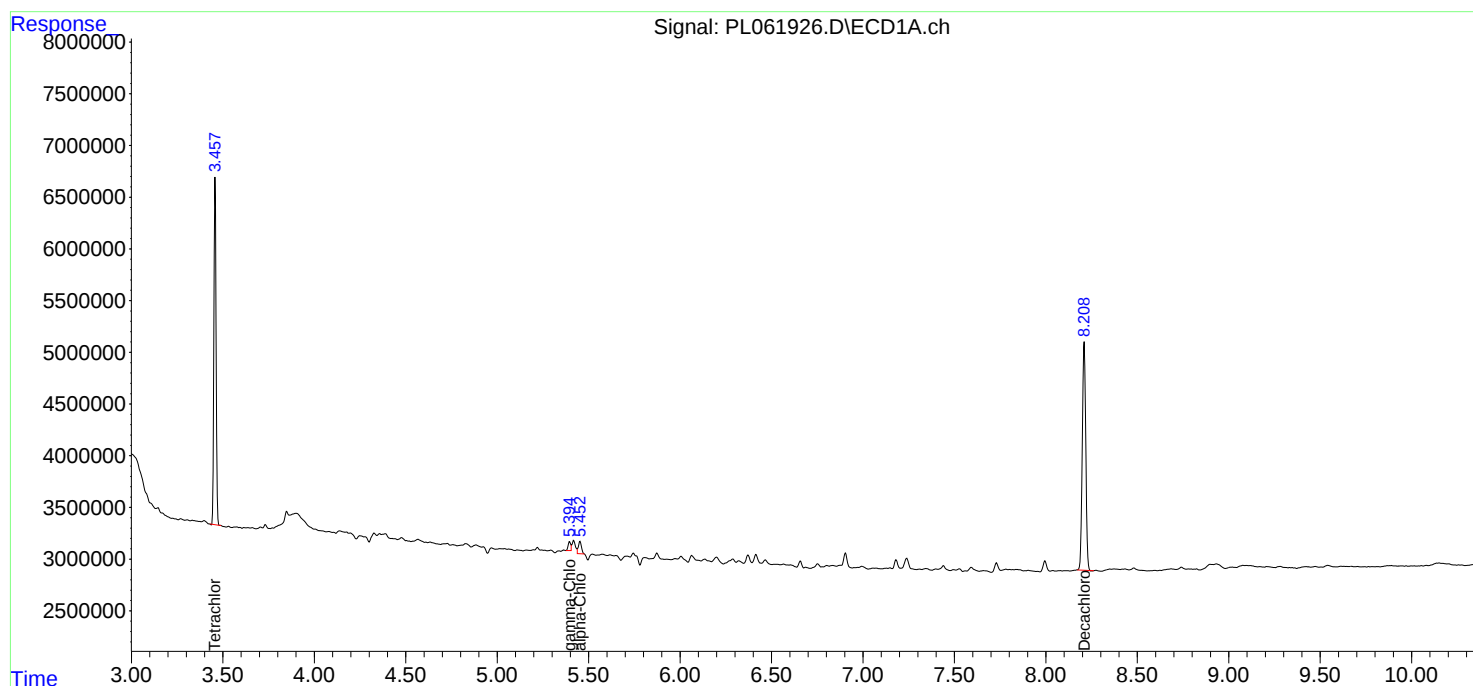

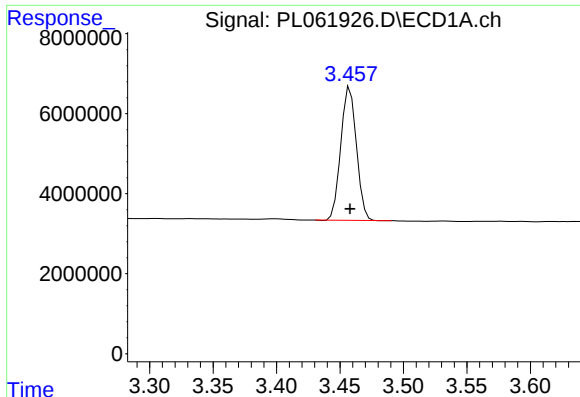


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 28535036
Conc: 16.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-C-2334-C


Manual Integrations
APPROVED

Ankita
10/5/2020 3:33:44 PM

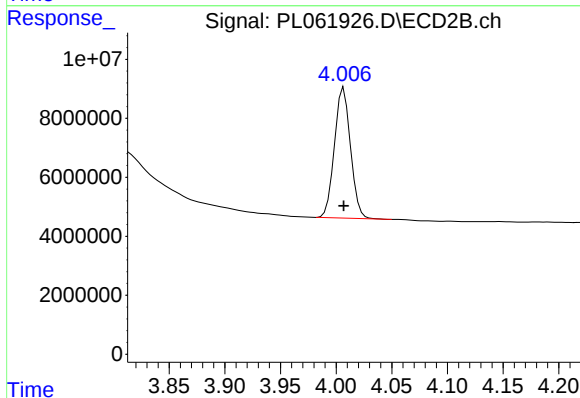


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 44375730
Conc: 16.27 ng/ml

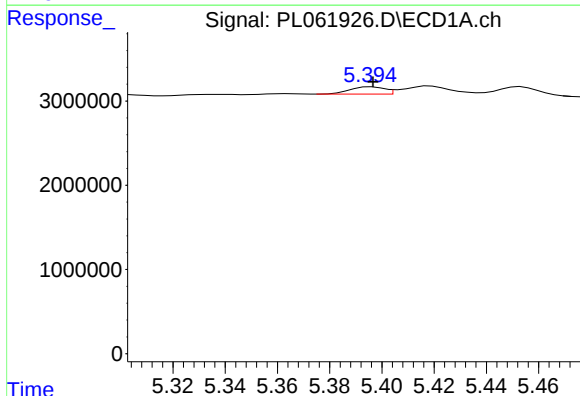


#10 gamma-Chlordane

R.T.: 5.394 min
Delta R.T.: -0.002 min
Response: 858975
Conc: 0.49 ng/ml m

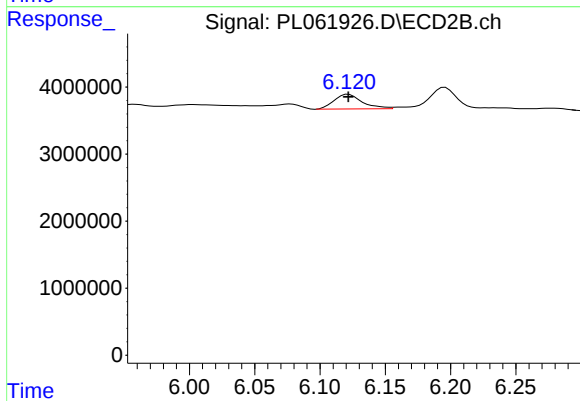

#10 gamma-Chlordane

R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 3287240
Conc: 1.12 ng/ml

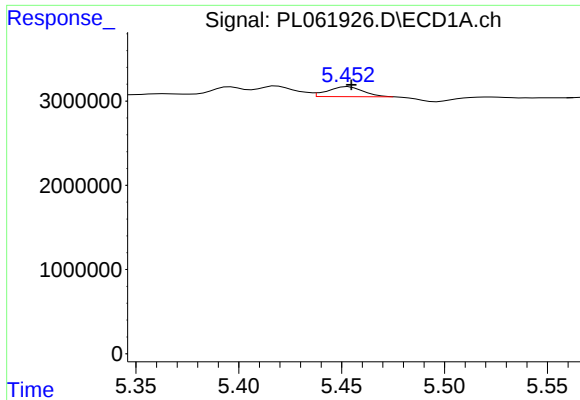


#11 alpha-Chlordane

R.T.: 5.452 min
Delta R.T.: -0.003 min
Response: 1394866
Conc: 0.80 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-C-2334-C


Manual Integrations
APPROVED

Ankita
10/5/2020 3:33:44 PM

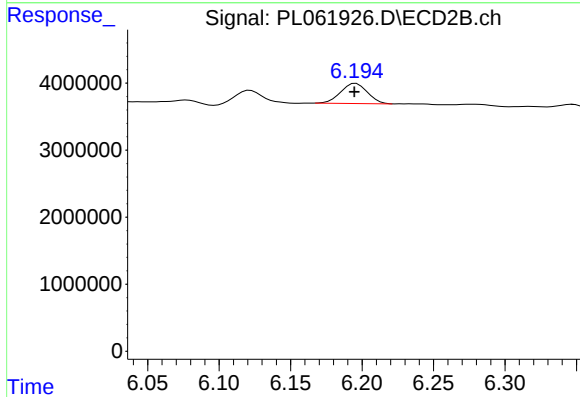


#11 alpha-Chlordane

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 3906613
Conc: 1.30 ng/ml m

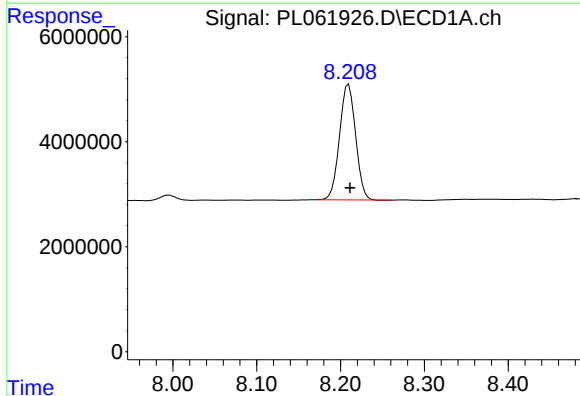

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: -0.002 min
Response: 29334553
Conc: 18.03 ng/ml

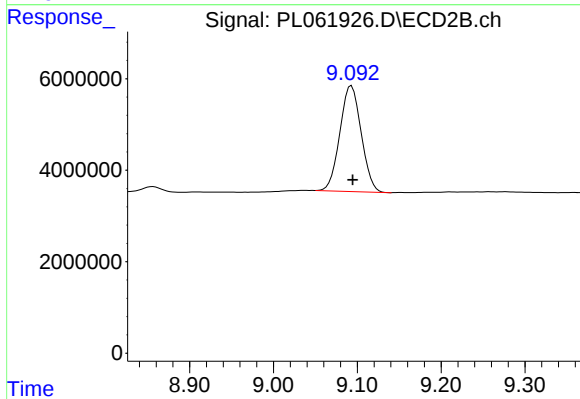

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.002 min
Response: 40981641
Conc: 18.62 ng/ml