

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
 Data File : PL061944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 15:18
 Operator : DD\AJ
 Sample : L4219-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-100120

Manual Integrations
 APPROVED

Ankita
 10/5/2020 3:34:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 17:43:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.007	25480454	28928261	14.936	10.603 #
28)	SA Decachlor...	8.208	9.093	23093074	32112879	14.196	14.588
Target Compounds							
11)	B alpha-Chl...	5.451	6.193	5150119	9533876	2.965m	3.174m
12)	B 4,4'-DDE	5.616	6.348	857611	12077670	0.546m	4.424 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
Data File : PL061944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 15:18
Operator : DD\AJ
Sample : L4219-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
CL-01-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:34:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 17:43:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

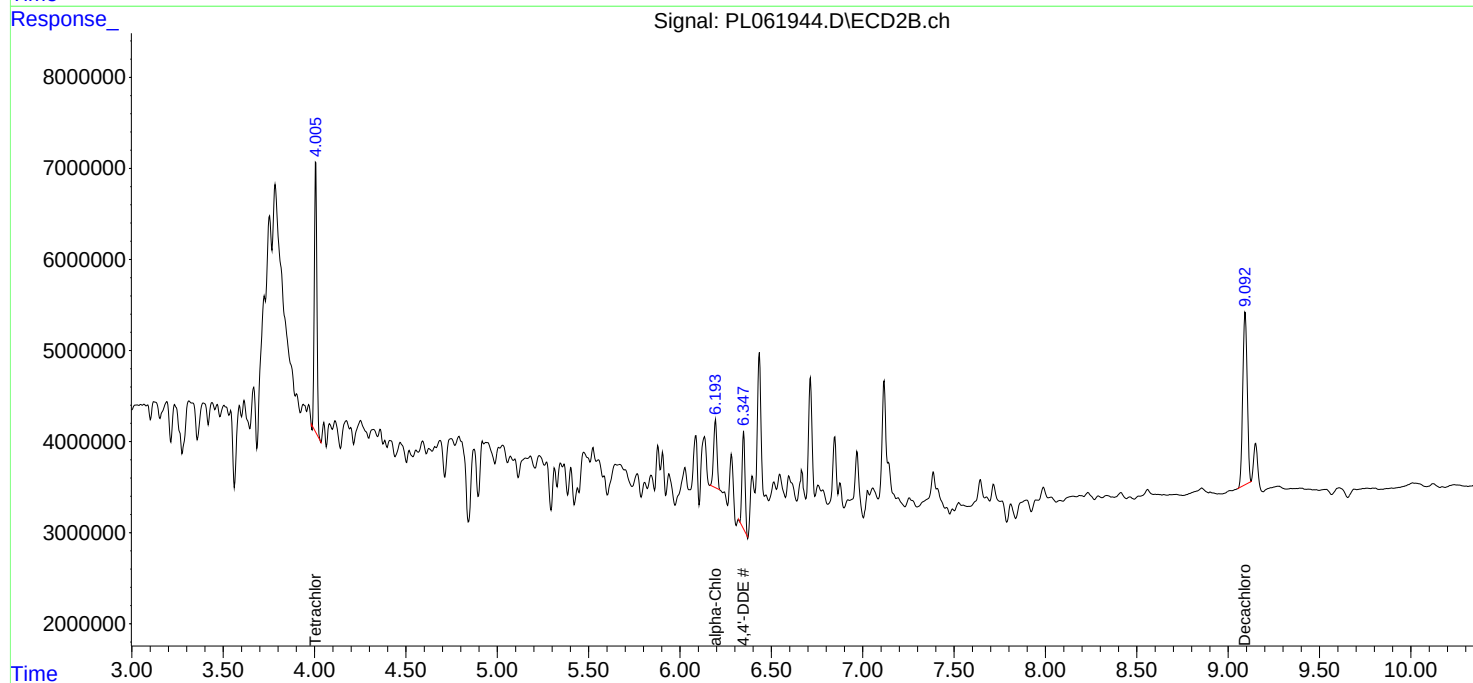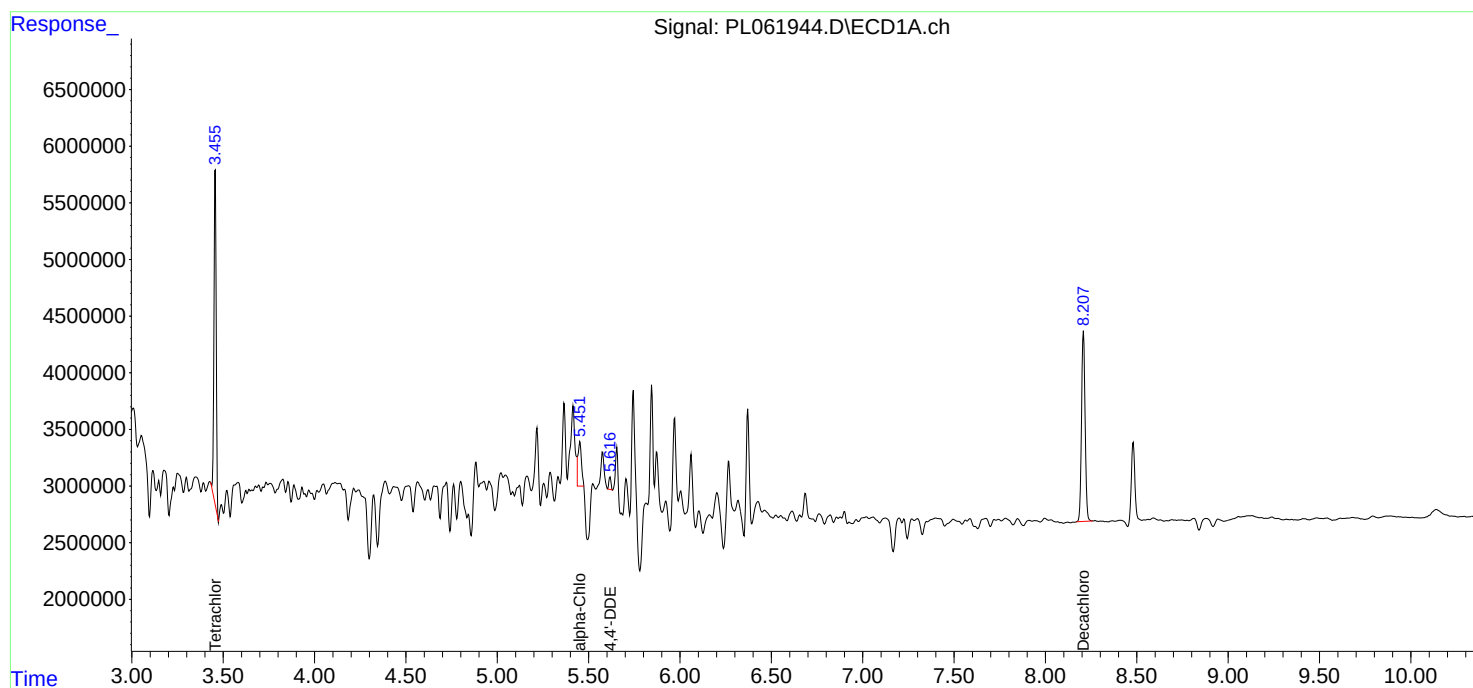

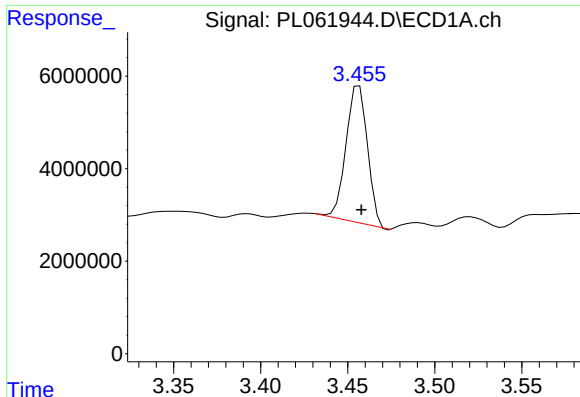


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 25480454
Conc: 14.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:34:25 PM

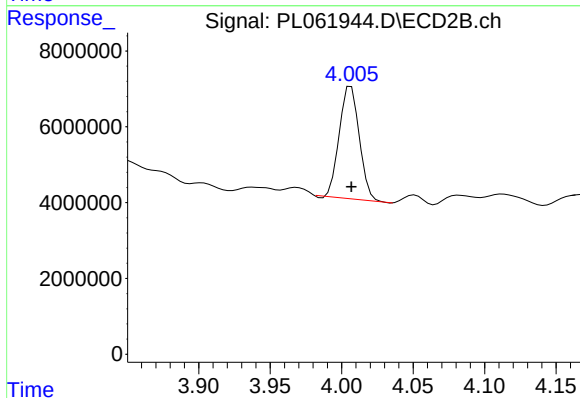


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 28928261
Conc: 10.60 ng/ml

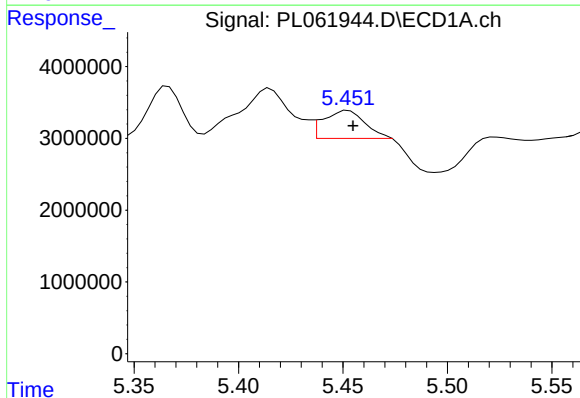


#11 alpha-Chlordane

R.T.: 5.451 min
Delta R.T.: -0.003 min
Response: 5150119
Conc: 2.96 ng/ml m

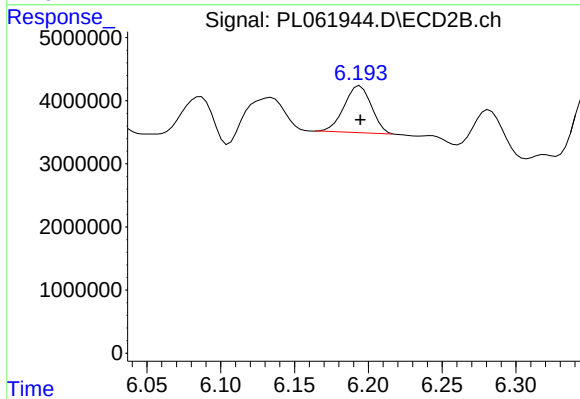

#11 alpha-Chlordane

R.T.: 6.193 min
Delta R.T.: -0.002 min
Response: 9533876
Conc: 3.17 ng/ml m

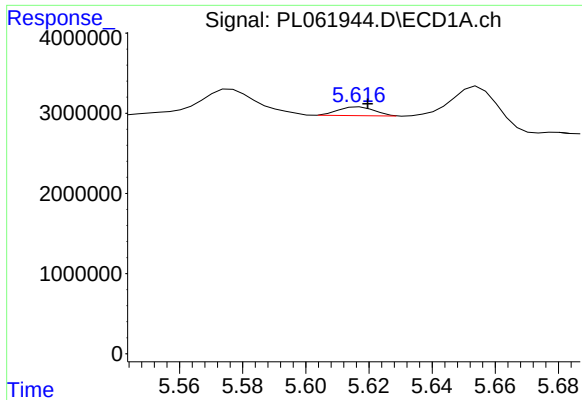


#12 4,4'-DDE

R.T.: 5.616 min
Delta R.T.: -0.004 min
Response: 857611
Conc: 0.55 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-01-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:34:25 PM

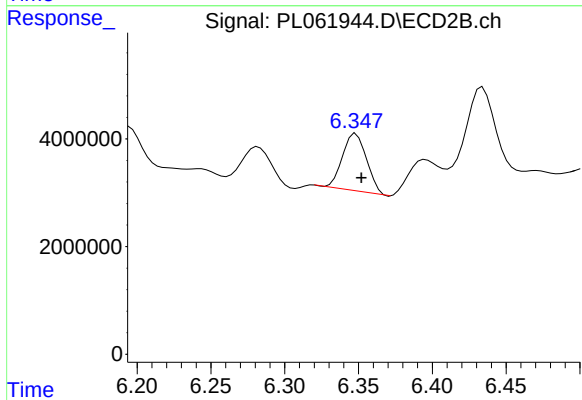


#12 4,4'-DDE

R.T.: 6.348 min
Delta R.T.: -0.004 min
Response: 12077670
Conc: 4.42 ng/ml

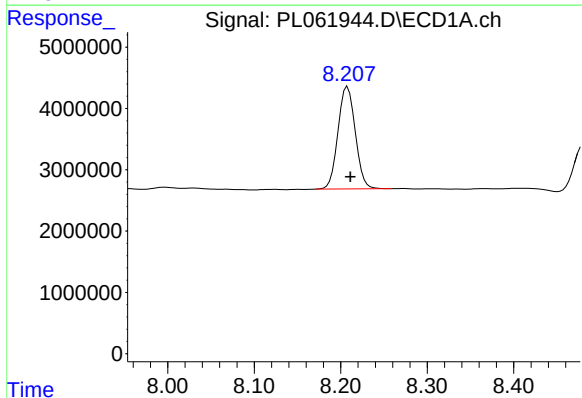

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.003 min
Response: 23093074
Conc: 14.20 ng/ml

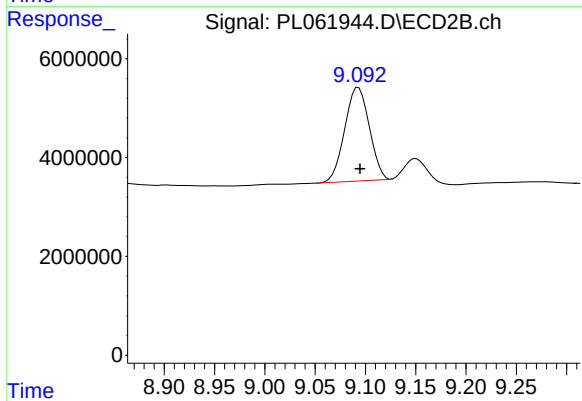

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.002 min
Response: 32112879
Conc: 14.59 ng/ml