

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
 Data File : PL061953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 17:41
 Operator : DD\AJ
 Sample : L4230-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2392

Manual Integrations
 APPROVED

Ankita
 10/5/2020 3:34:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 06:26:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	4.007	17017026	24495300	9.975	8.978
28) SA Decachlor...	8.209	9.095	23922632	32876431	14.706	14.935
Target Compounds						
11) B alpha-Chl...	5.453	6.198	3387996	24084792	1.950m	8.019 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100220\
Data File : PL061953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 17:41
Operator : DD\AJ
Sample : L4230-06
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
2392


Manual Integrations
APPROVED

Ankita
10/5/2020 3:34:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 06:26:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

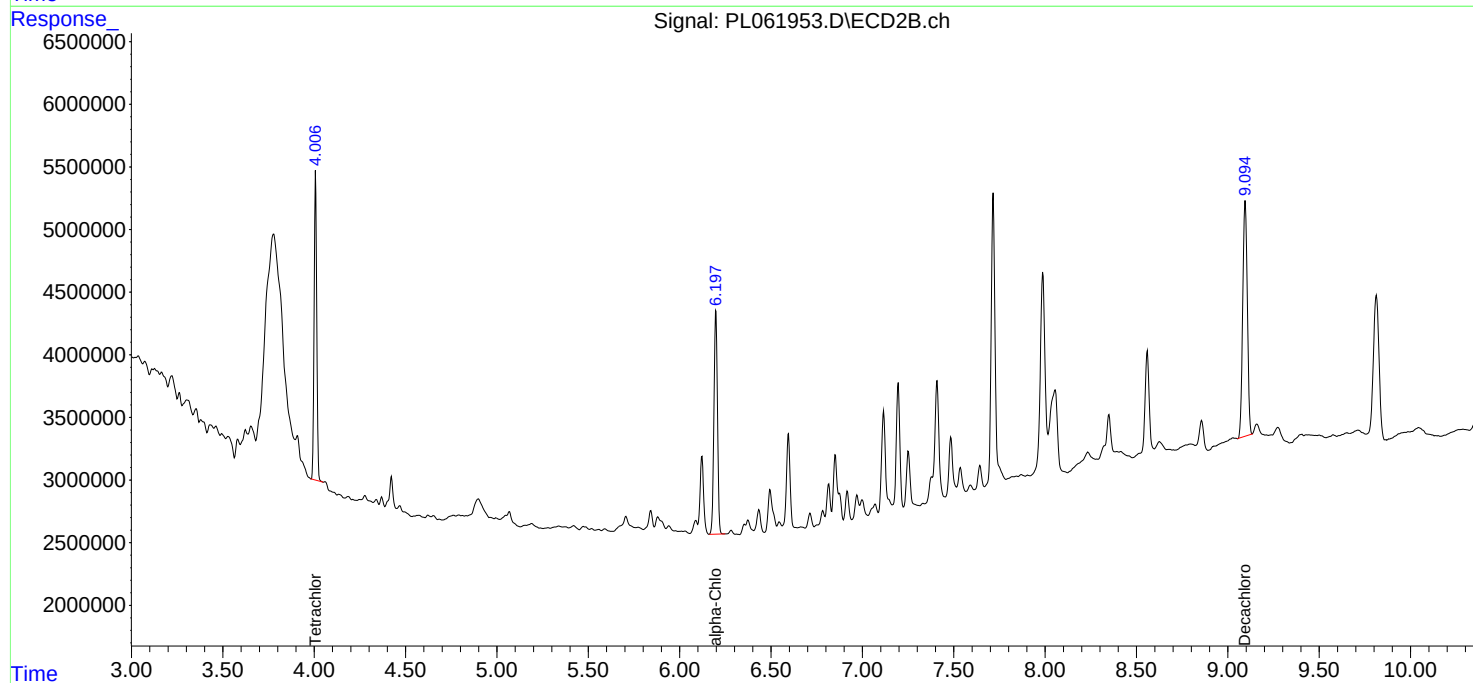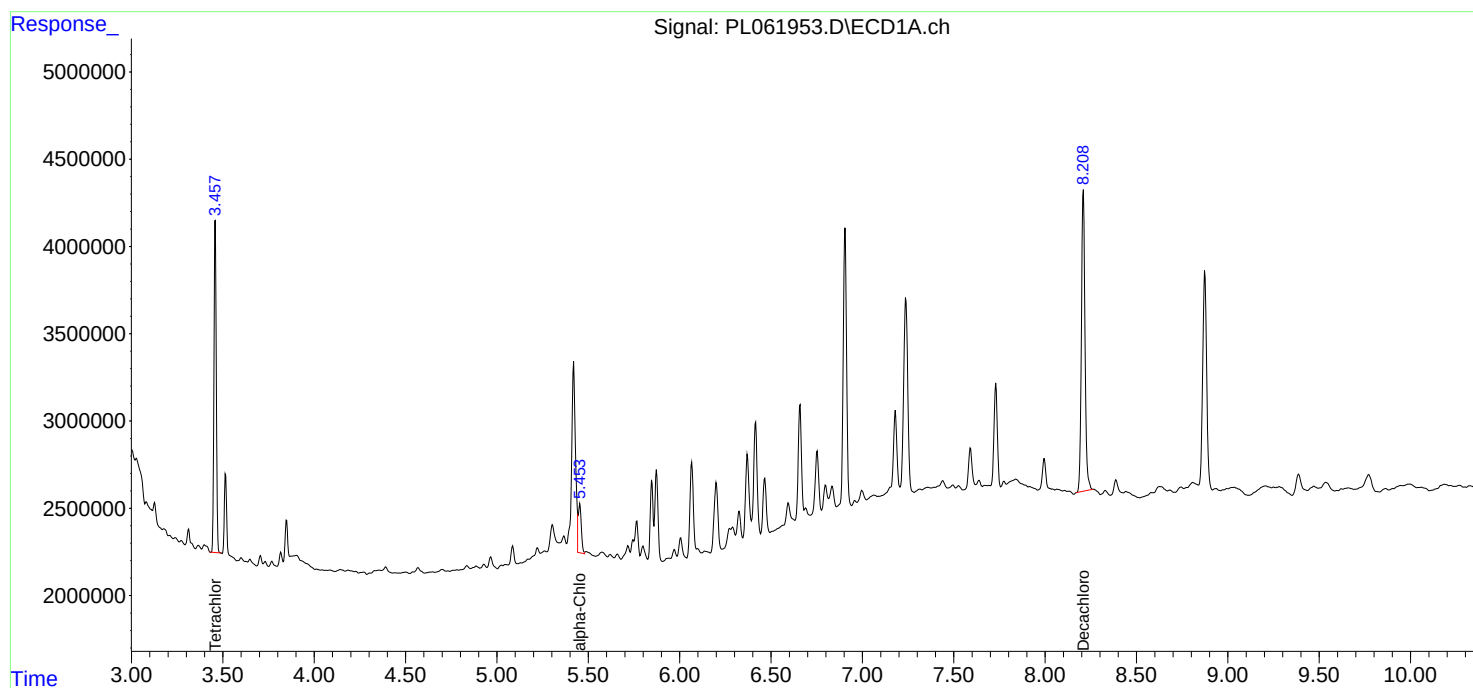

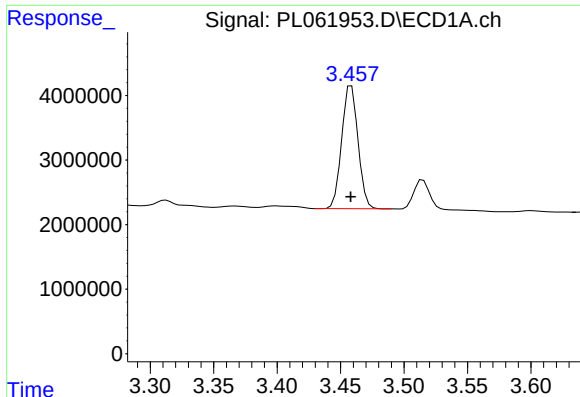


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 17017026
Conc: 9.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
2392


Manual Integrations
APPROVED

Ankita
10/5/2020 3:34:47 PM

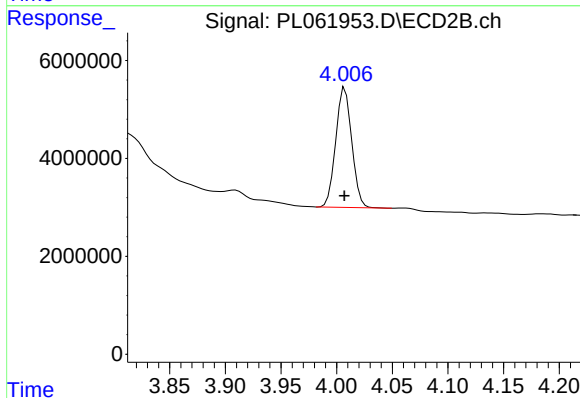


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 24495300
Conc: 8.98 ng/ml

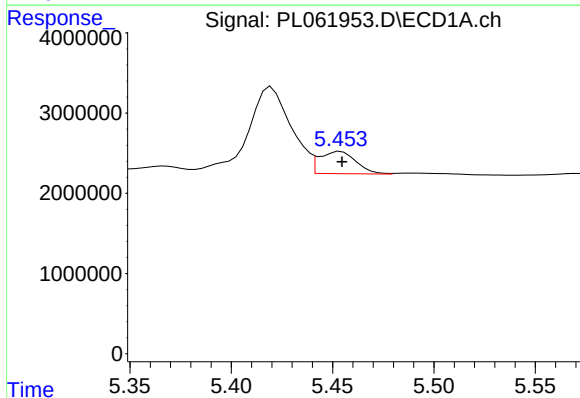


#11 alpha-Chlordane

R.T.: 5.453 min
Delta R.T.: -0.002 min
Response: 3387996
Conc: 1.95 ng/ml m

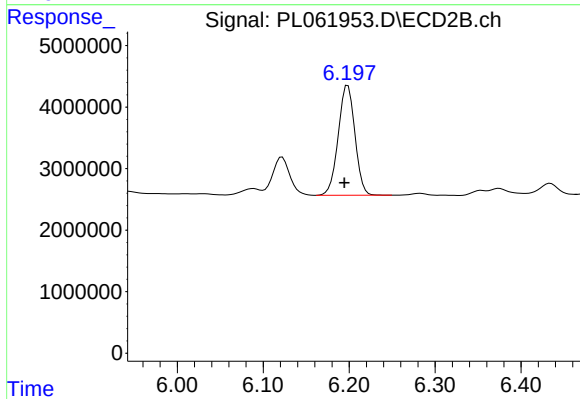

#11 alpha-Chlordane

R.T.: 6.198 min
Delta R.T.: 0.004 min
Response: 24084792
Conc: 8.02 ng/ml

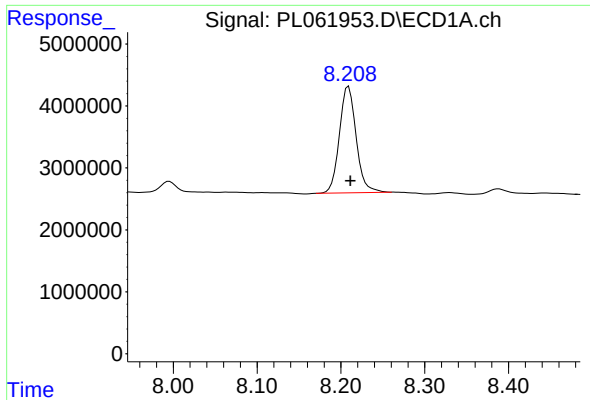


#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 23922632
Conc: 14.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
2392

Manual Integrations
APPROVED

Ankita
10/5/2020 3:34:47 PM

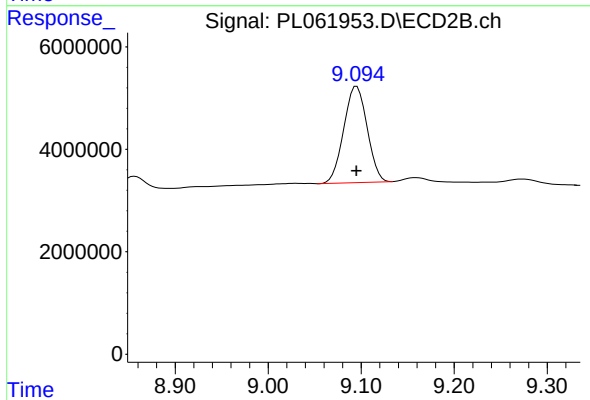

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 32876431
Conc: 14.93 ng/ml