

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
 Data File : PL085639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 20:58
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:46:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 04:44:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	2.621	211.9E6	88138242	75.013	75.621
28)	SA Decachlor...	8.855	7.772	178.0E6	64670829	73.400	72.810
Target Compounds							
23)	Chlordane-1	4.515	3.611	84244510	23477179	720.248	727.235
24)	Chlordane-2	5.047	4.189	83567475	27474357	668.835	703.161
25)	Chlordane-3	5.758	4.818	367.3E6	85865358	769.585	759.282
26)	Chlordane-4	5.840	4.879	449.0E6	91102842	765.356	774.318
27)	Chlordane-5	6.686	5.549	67777792	22716169	730.197	726.614



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
Data File : PL085639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 20:58
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:46:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 04:44:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

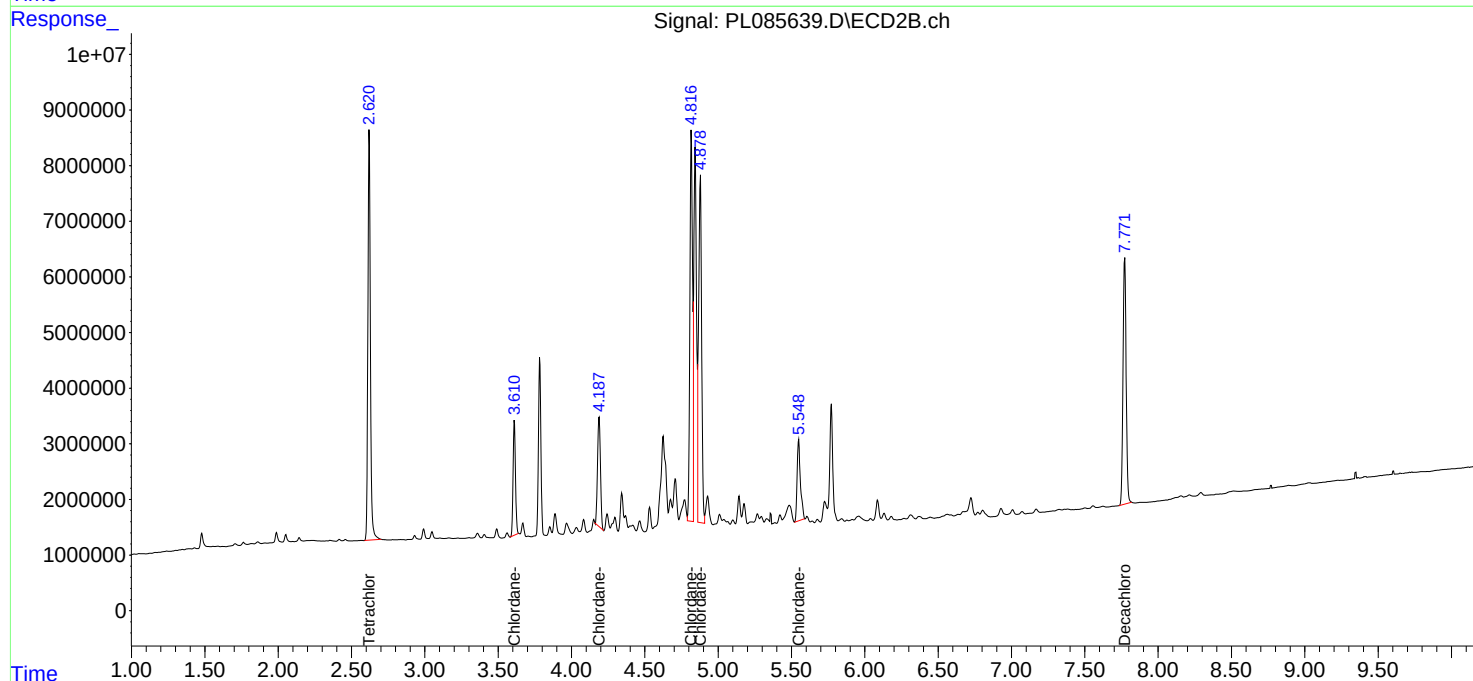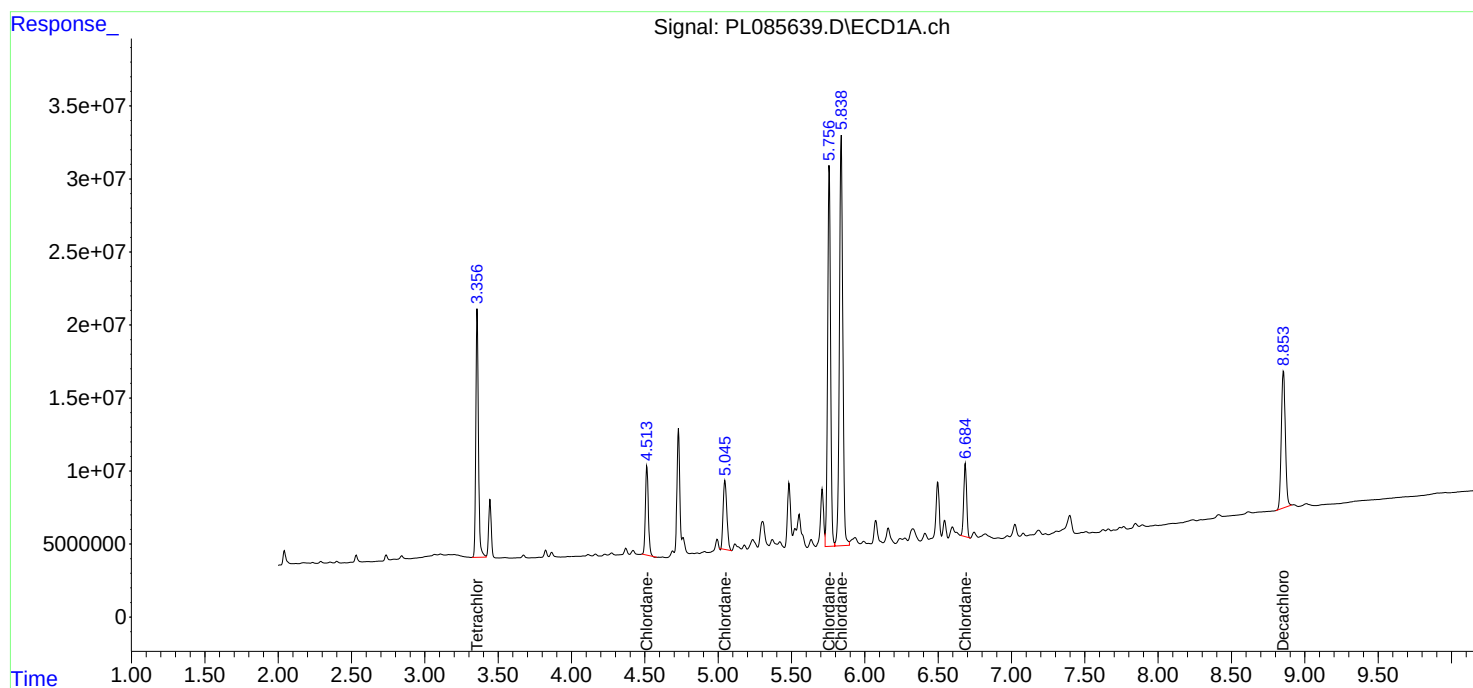


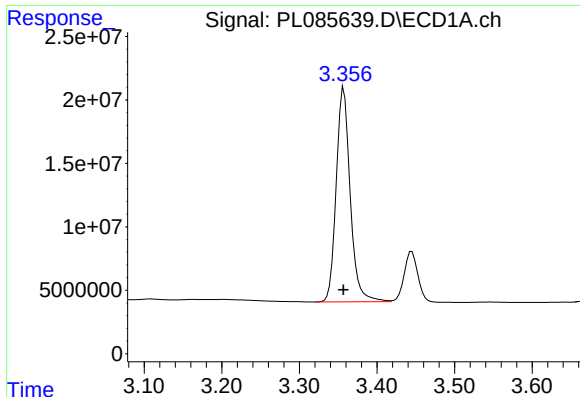

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: 0.000 min
Response: 211941626
Conc: 75.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

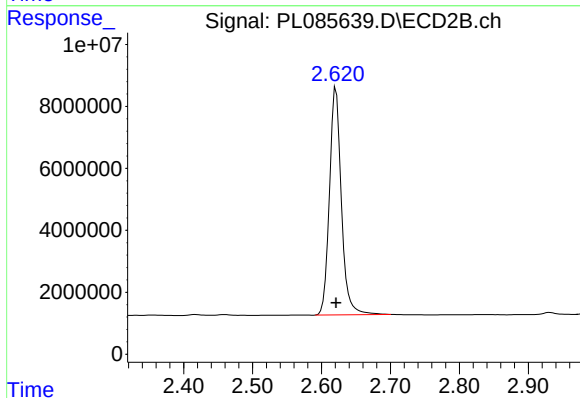


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 88138242
Conc: 75.62 ng/ml

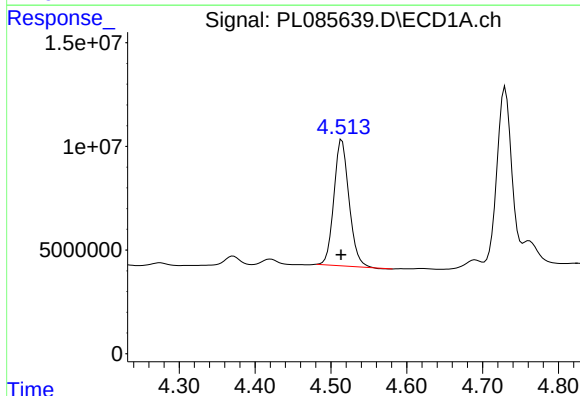


#23 Chlordane-1

R.T.: 4.515 min
Delta R.T.: 0.001 min
Response: 84244510
Conc: 720.25 ng/ml

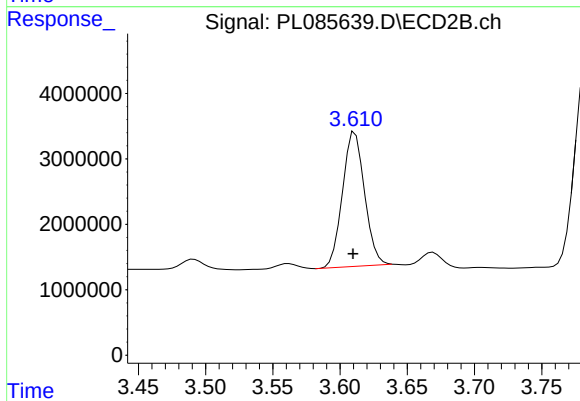

#23 Chlordane-1


R.T.: 3.611 min
Delta R.T.: 0.002 min
Response: 23477179
Conc: 727.24 ng/ml

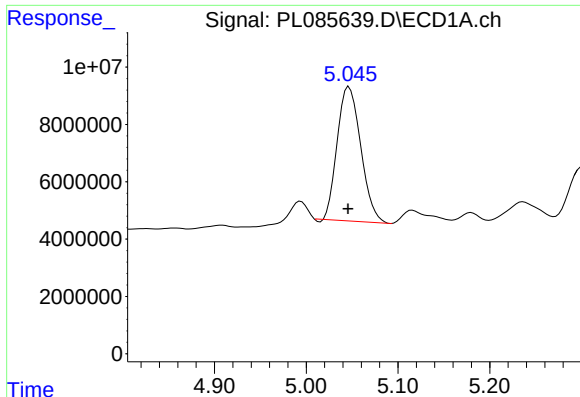

#24 Chlordane-2


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 83567475
Conc: 668.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

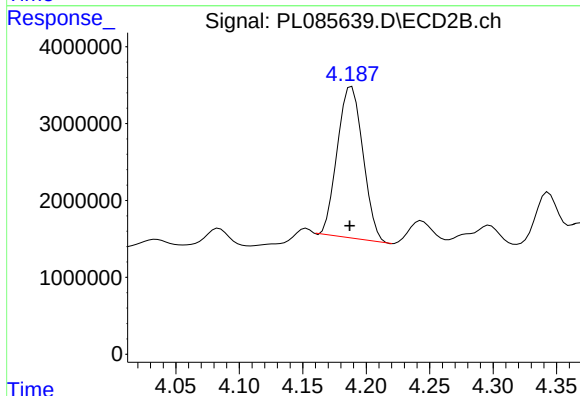


#24 Chlordane-2

R.T.: 4.189 min
Delta R.T.: 0.001 min
Response: 27474357
Conc: 703.16 ng/ml

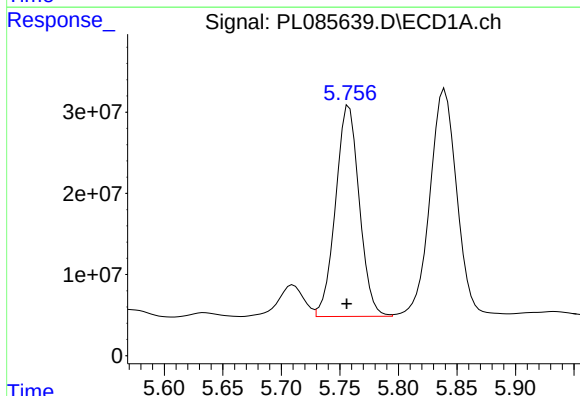


#25 Chlordane-3

R.T.: 5.758 min
Delta R.T.: 0.002 min
Response: 367254356
Conc: 769.58 ng/ml

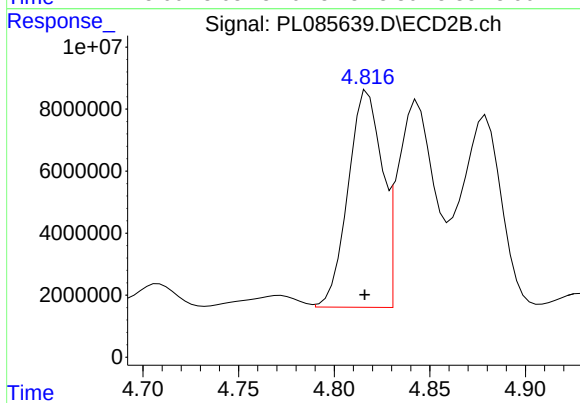

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: 0.002 min
Response: 85865358
Conc: 759.28 ng/ml

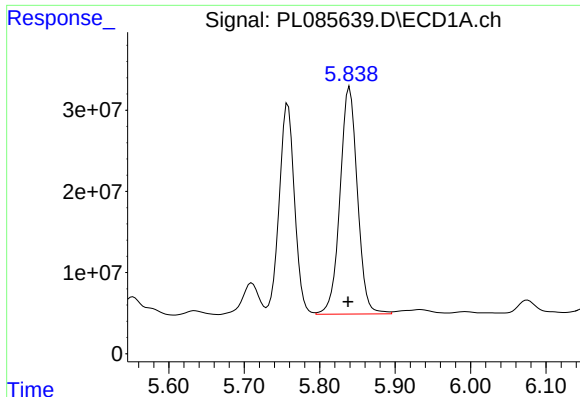

#26 Chlordane-4


R.T.: 5.840 min
Delta R.T.: 0.002 min
Response: 449044529
Conc: 765.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

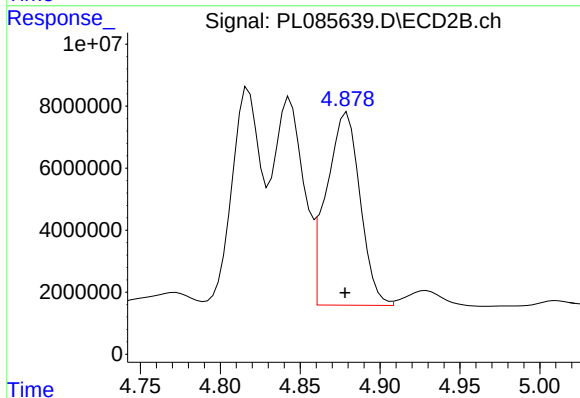


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.001 min
Response: 91102842
Conc: 774.32 ng/ml

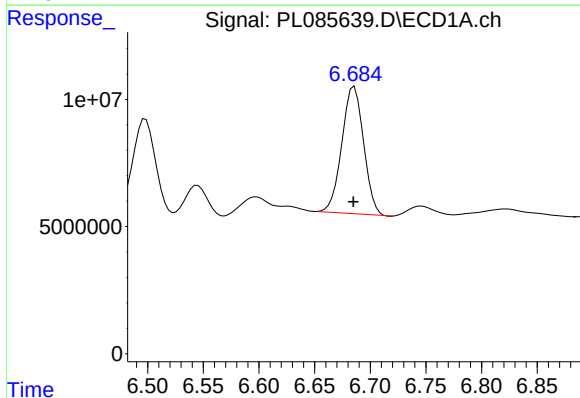


#27 Chlordane-5

R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 67777792
Conc: 730.20 ng/ml

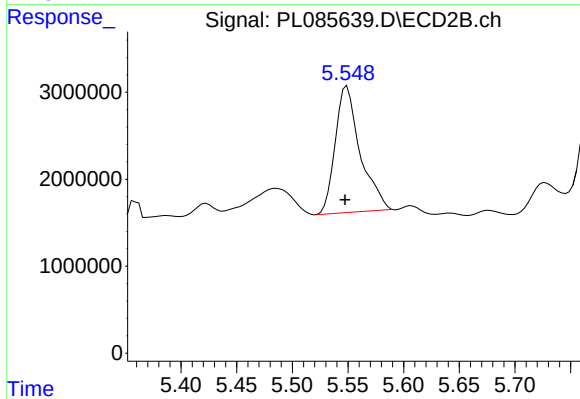

#27 Chlordane-5


R.T.: 5.549 min
Delta R.T.: 0.002 min
Response: 22716169
Conc: 726.61 ng/ml

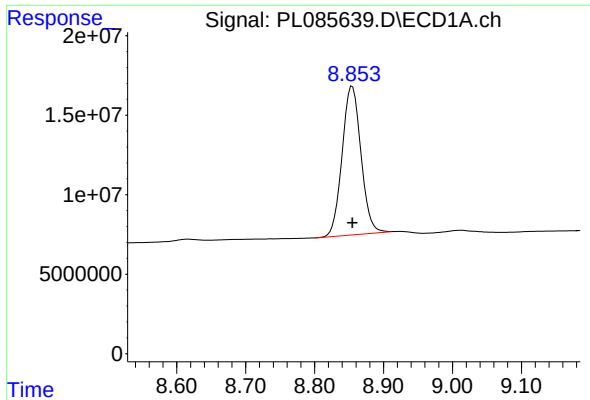

#28 Decachlorobiphenyl

R.T.: 8.855 min
Delta R.T.: 0.000 min
Response: 177977580
Conc: 73.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

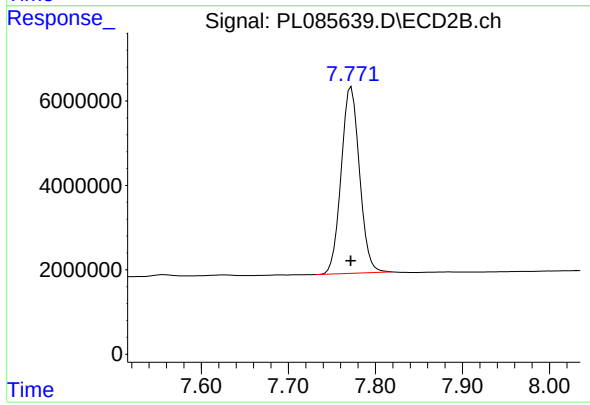

#28 Decachlorobiphenyl

R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 64670829
Conc: 72.81 ng/ml