

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
 Data File : PL085642.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 21:39
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:47:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 04:44:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	2.621	14359493	5866375	5.082	5.033
28)	SA Decachlor...	8.856	7.772	14858818	5101308	6.128	5.743
Target Compounds							
23)	Chlordane-1	4.515	3.611	7178789	1696778	61.375	52.560
24)	Chlordane-2	5.047	4.188	5835412	1916760	46.704	49.056
25)	Chlordane-3	5.758	4.817	25257164	5524392	52.927	48.851
26)	Chlordane-4	5.840	4.880	33248256	6434483	56.669	54.689
27)	Chlordane-5	6.685	5.549	4375125	1427444	47.135	45.659



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
Data File : PL085642.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 21:39
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:47:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 04:44:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

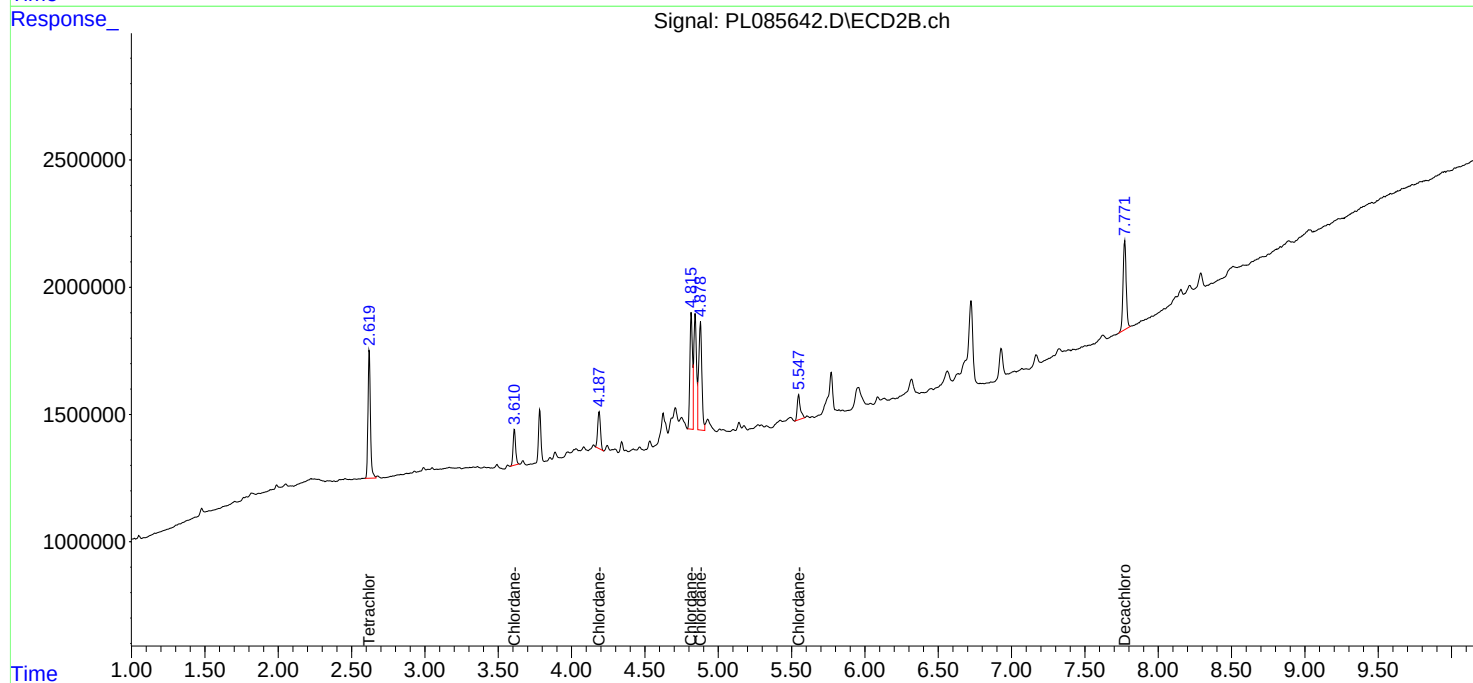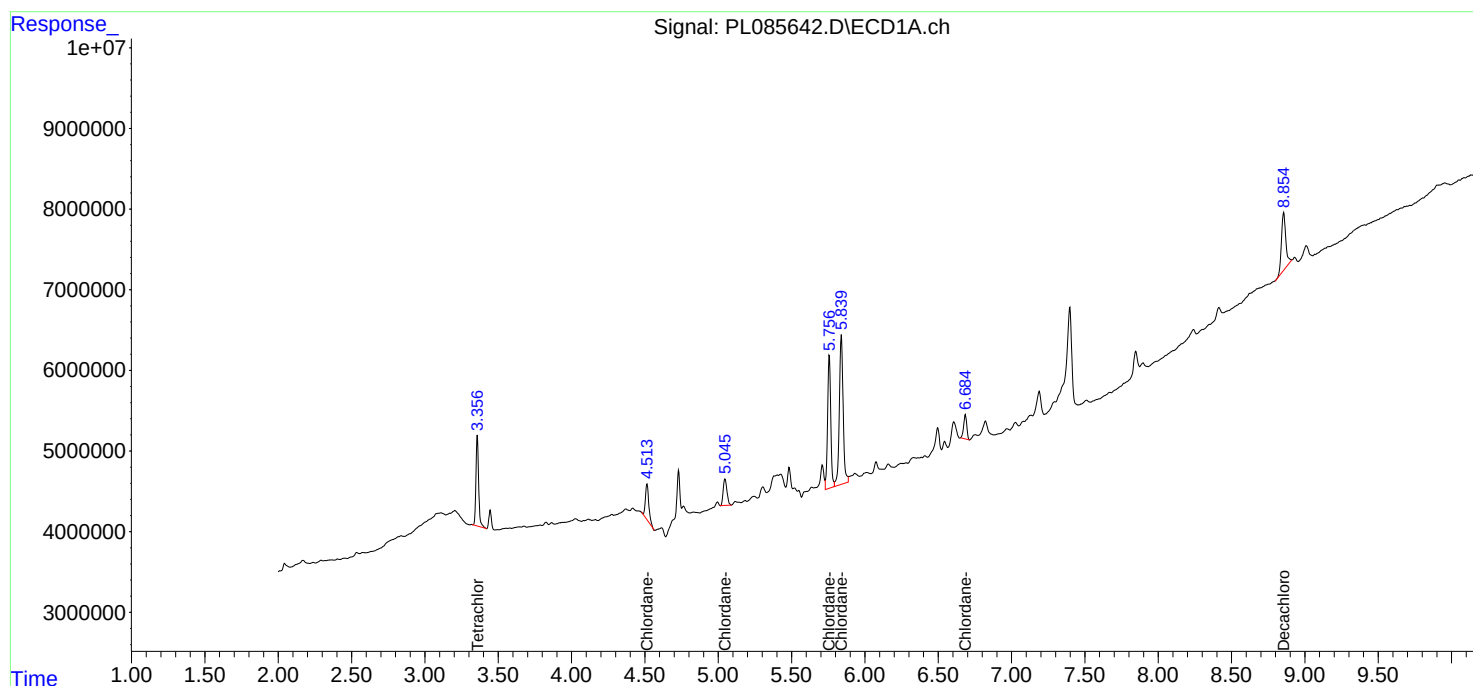


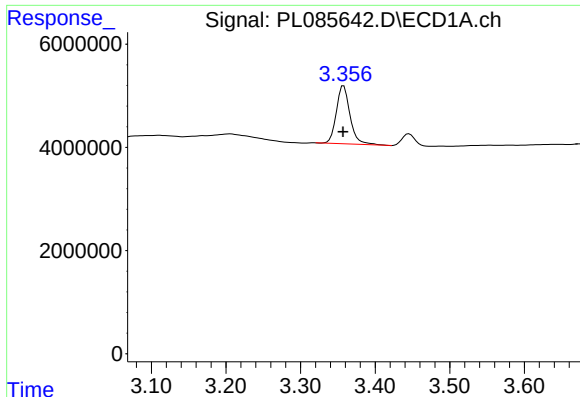

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: 0.000 min
Response: 14359493
Conc: 5.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

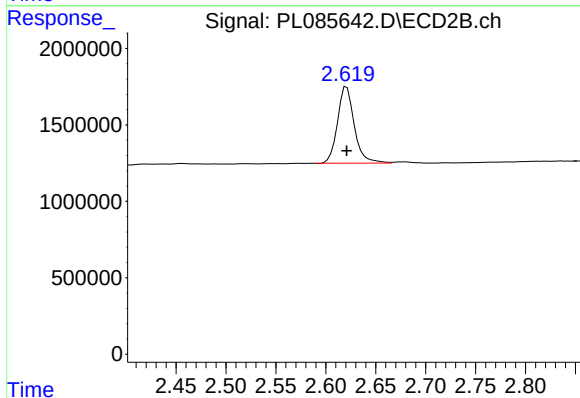


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 5866375
Conc: 5.03 ng/ml

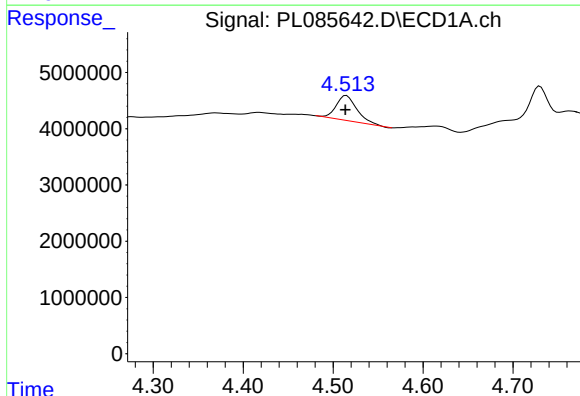


#23 Chlordane-1

R.T.: 4.515 min
Delta R.T.: 0.001 min
Response: 7178789
Conc: 61.38 ng/ml

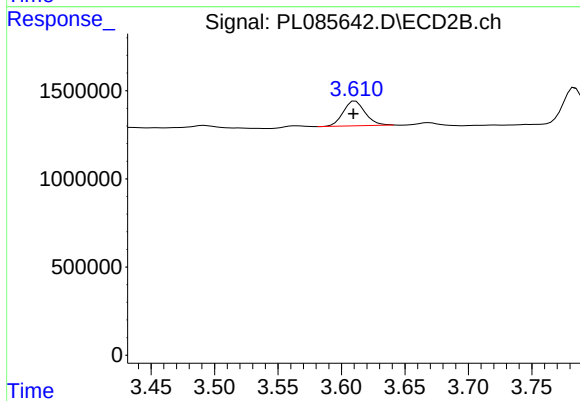

#23 Chlordane-1


R.T.: 3.611 min
Delta R.T.: 0.001 min
Response: 1696778
Conc: 52.56 ng/ml

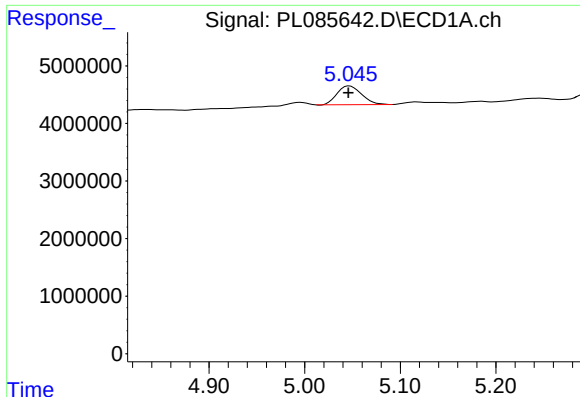

#24 Chlordane-2


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 5835412
Conc: 46.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

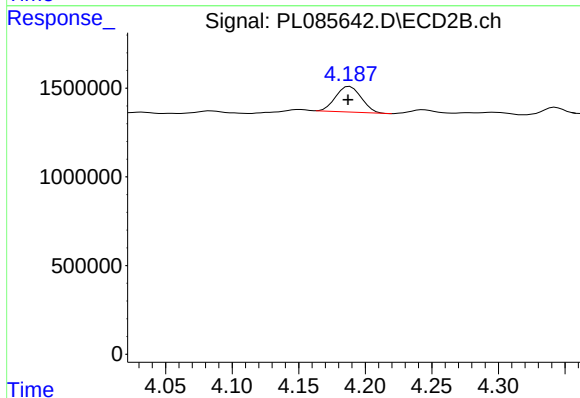


#24 Chlordane-2

R.T.: 4.188 min
Delta R.T.: 0.001 min
Response: 1916760
Conc: 49.06 ng/ml

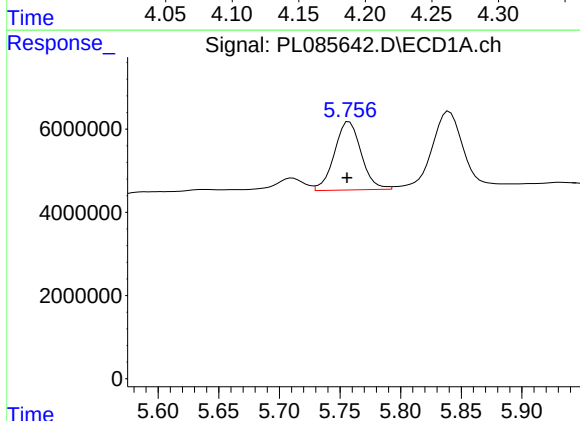


#25 Chlordane-3

R.T.: 5.758 min
Delta R.T.: 0.002 min
Response: 25257164
Conc: 52.93 ng/ml

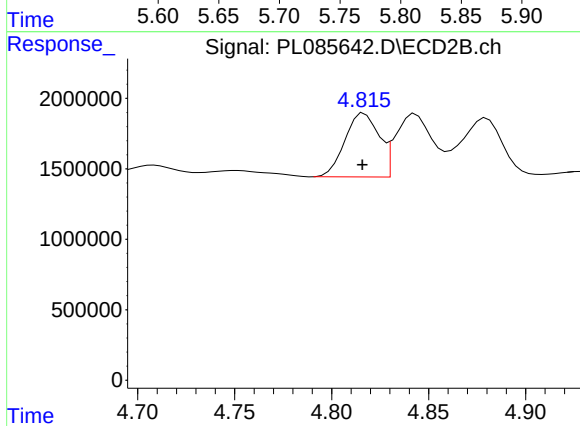

#25 Chlordane-3


R.T.: 4.817 min
Delta R.T.: 0.001 min
Response: 5524392
Conc: 48.85 ng/ml

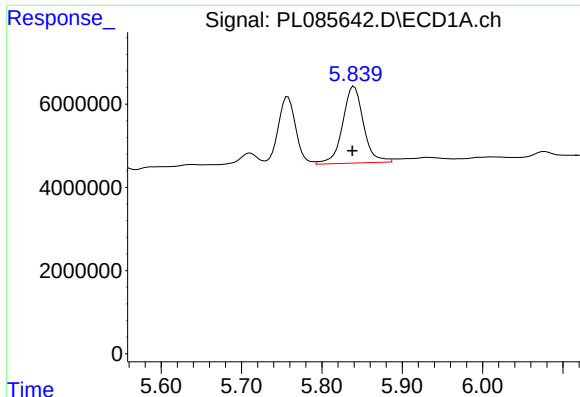

#26 Chlordane-4


R.T.: 5.840 min
Delta R.T.: 0.002 min
Response: 33248256
Conc: 56.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

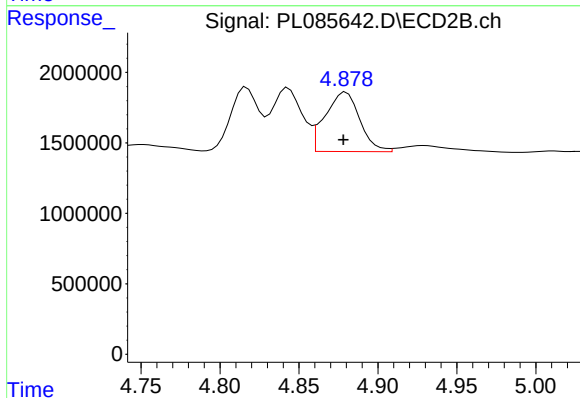


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: 0.002 min
Response: 6434483
Conc: 54.69 ng/ml

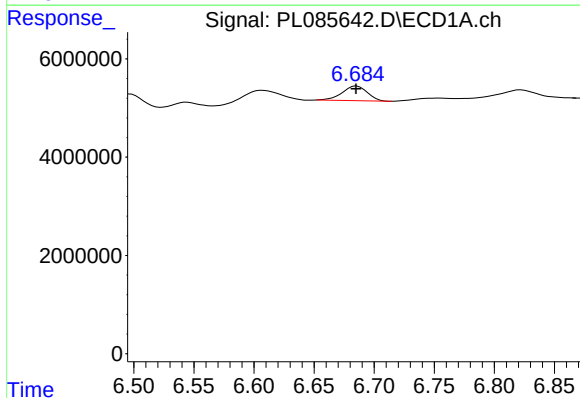


#27 Chlordane-5

R.T.: 6.685 min
Delta R.T.: 0.000 min
Response: 4375125
Conc: 47.13 ng/ml

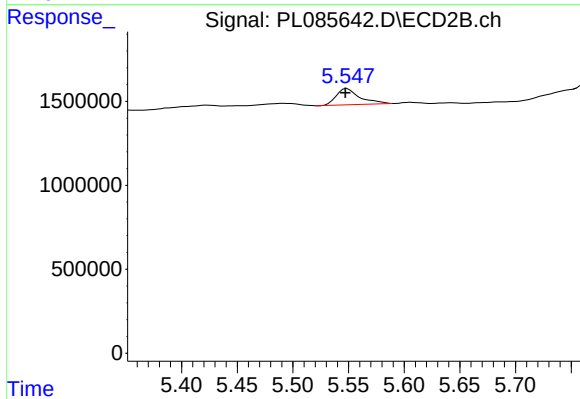

#27 Chlordane-5


R.T.: 5.549 min
Delta R.T.: 0.002 min
Response: 1427444
Conc: 45.66 ng/ml

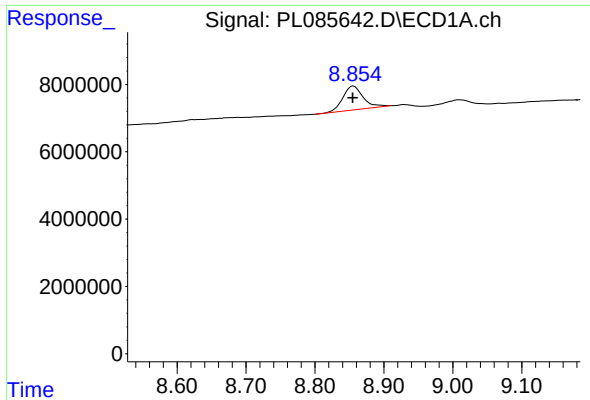

#28 Decachlorobiphenyl

R.T.: 8.856 min
Delta R.T.: 0.000 min
Response: 14858818
Conc: 6.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

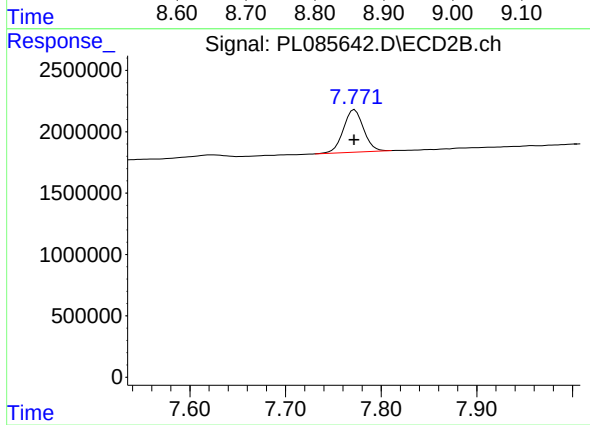

#28 Decachlorobiphenyl

R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 5101308
Conc: 5.74 ng/ml