

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
 Data File : PL085638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 20:44
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:50:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 04:49:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	2.621	284.9E6	120.0E6	100.408	101.464
28)	SA Decachlor...	8.853	7.772	238.0E6	85636708	99.076	98.174
Target Compounds							
23)	Chlordane-1	4.515	3.611	114.7E6	31497633	999.447	997.062
24)	Chlordane-2	5.047	4.189	110.9E6	35549724	978.477	966.002
25)	Chlordane-3	5.758	4.817	501.7E6	117.5E6	1017.475	1020.667
26)	Chlordane-4	5.840	4.879	607.9E6	124.3E6	1007.790	1015.812
27)	Chlordane-5	6.686	5.549	92113096	30665131	1012.500	997.706



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
Data File : PL085638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 20:44
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:50:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 04:49:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

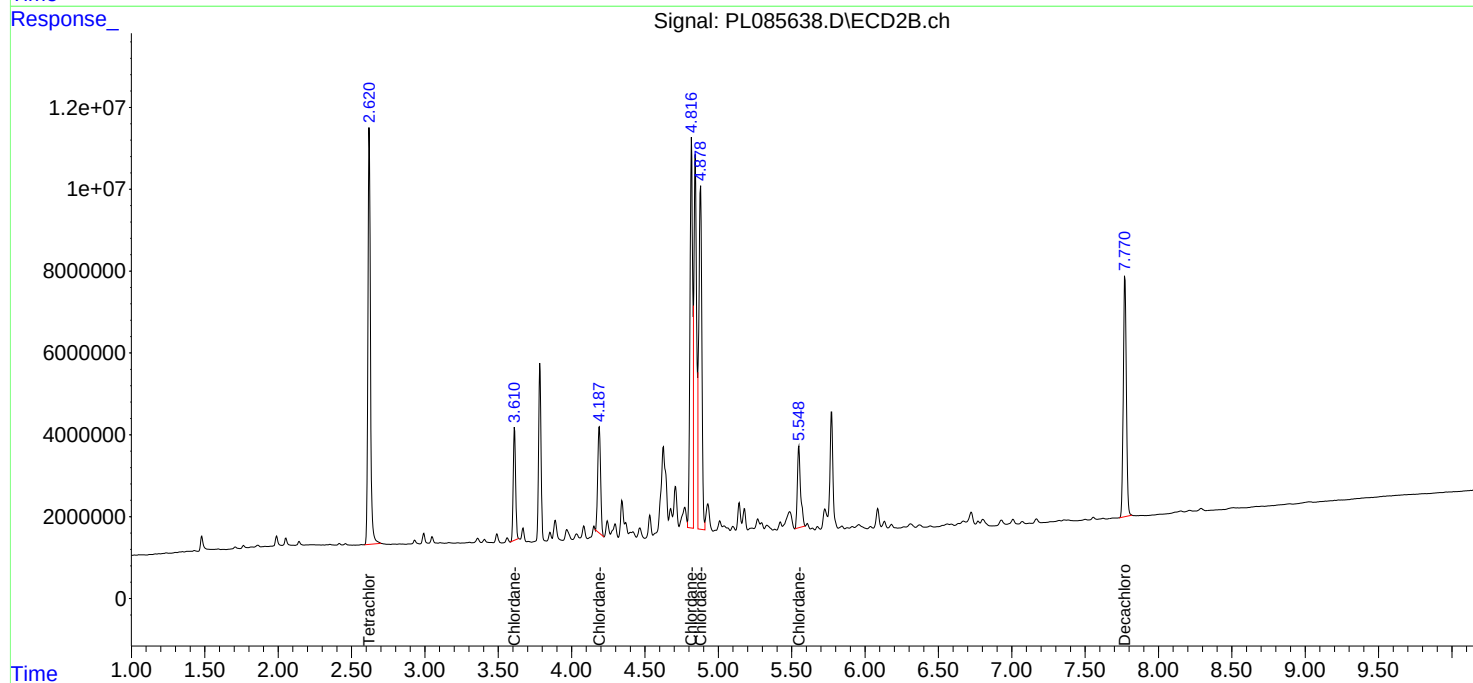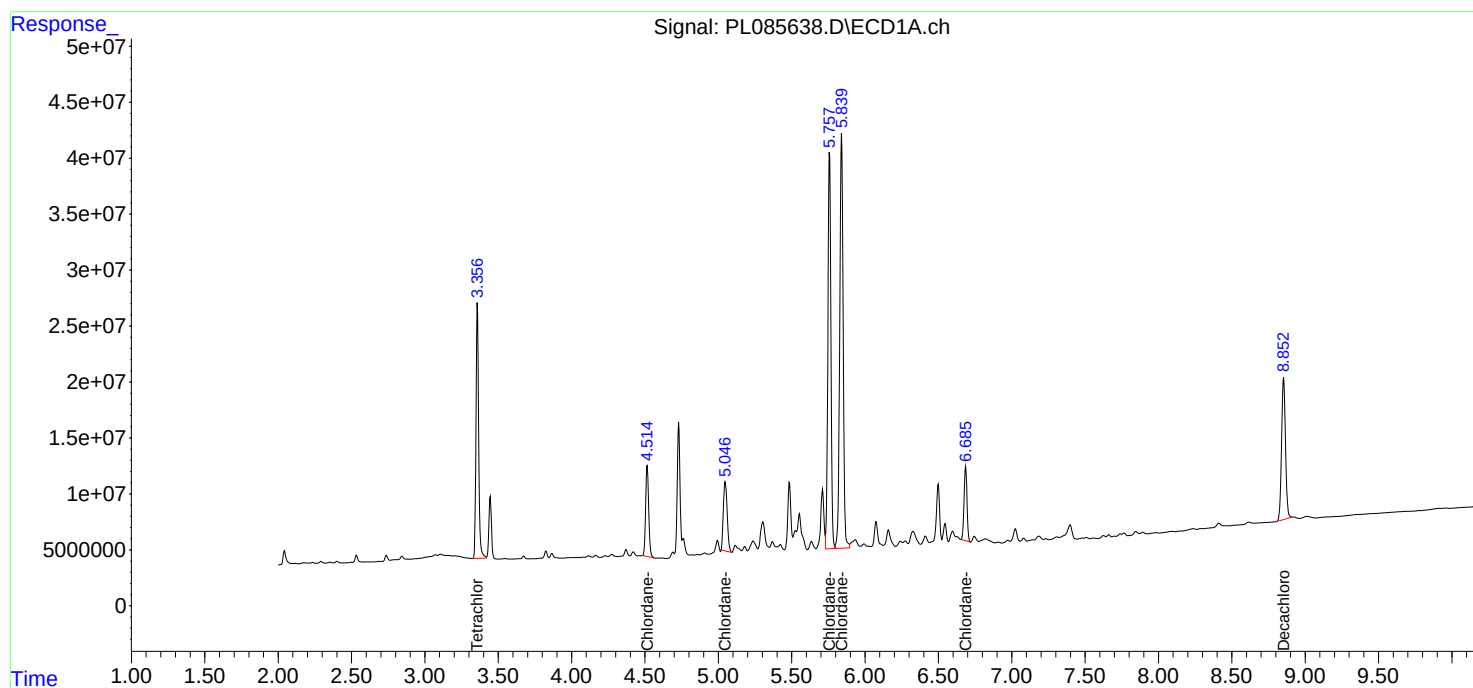


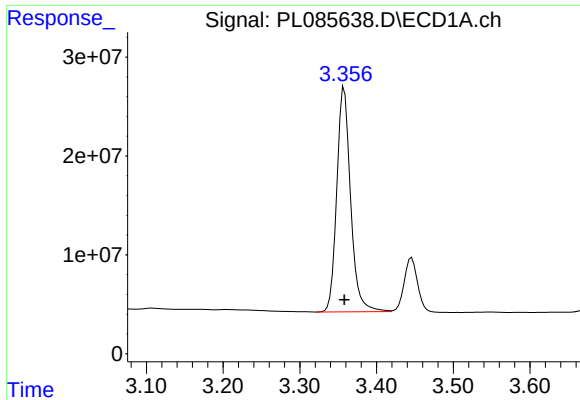

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: 0.000 min
Response: 284853166
Conc: 100.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

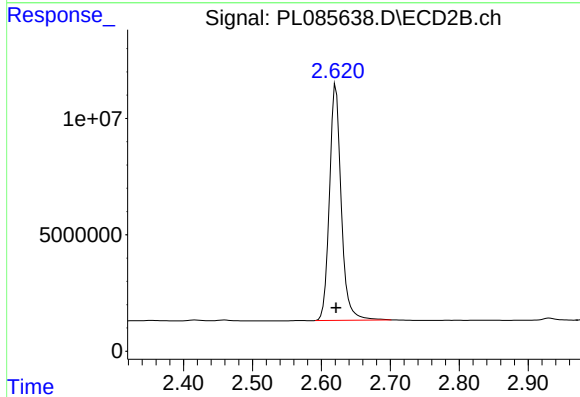


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 120017312
Conc: 101.46 ng/ml

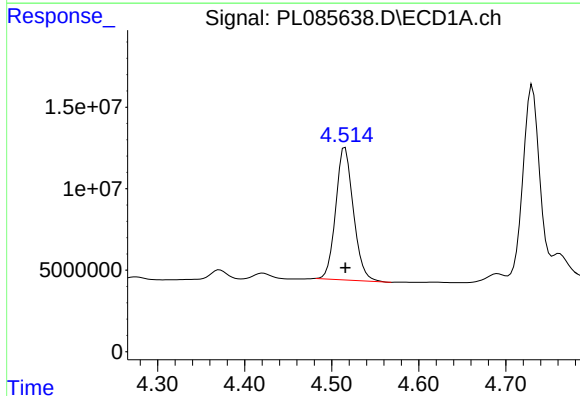


#23 Chlordane-1

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 114699955
Conc: 999.45 ng/ml

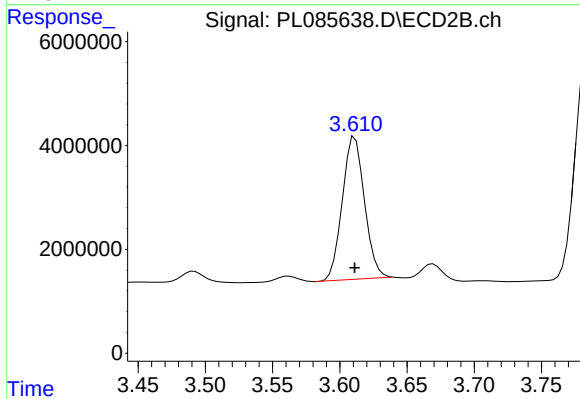

#23 Chlordane-1


R.T.: 3.611 min
Delta R.T.: 0.000 min
Response: 31497633
Conc: 997.06 ng/ml

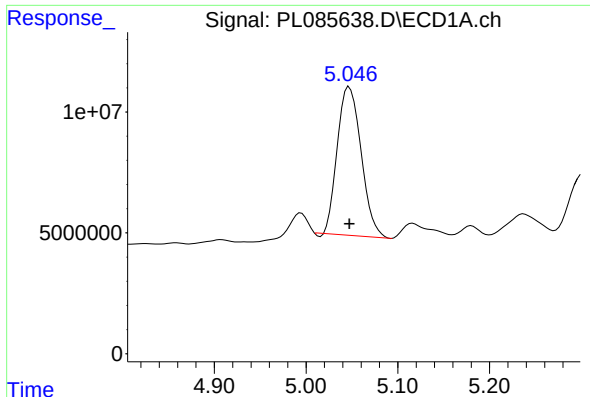

#24 Chlordane-2


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 110930218
Conc: 978.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

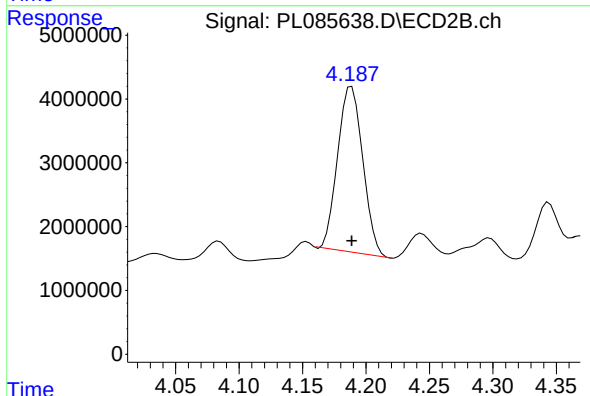


#24 Chlordane-2

R.T.: 4.189 min
Delta R.T.: 0.000 min
Response: 35549724
Conc: 966.00 ng/ml

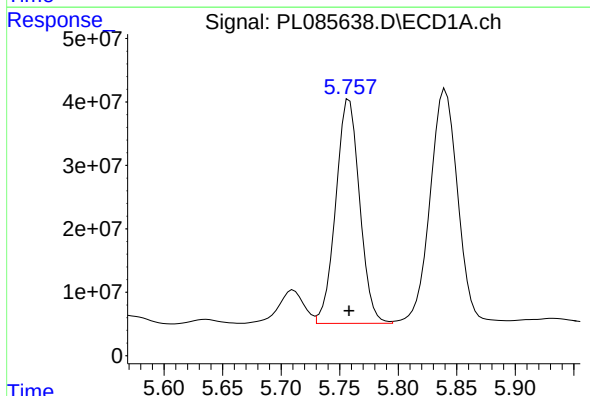


#25 Chlordane-3

R.T.: 5.758 min
Delta R.T.: 0.000 min
Response: 501681392
Conc: 1017.48 ng/ml

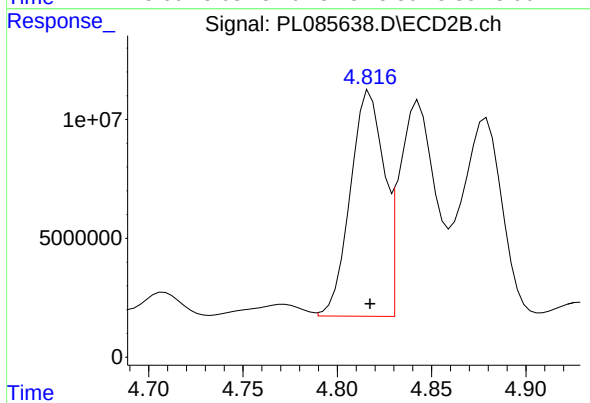

#25 Chlordane-3


R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 117468077
Conc: 1020.67 ng/ml

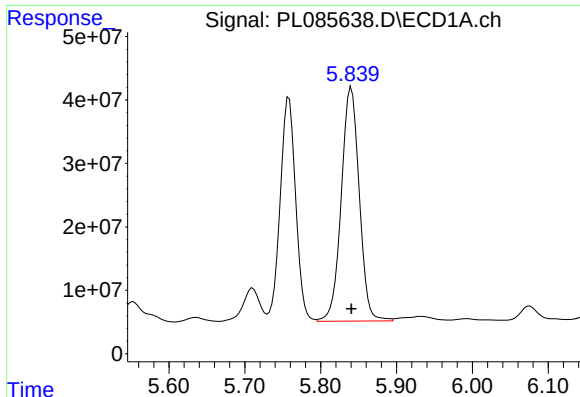

#26 Chlordane-4


R.T.: 5.840 min
Delta R.T.: 0.000 min
Response: 607870025
Conc: 1007.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

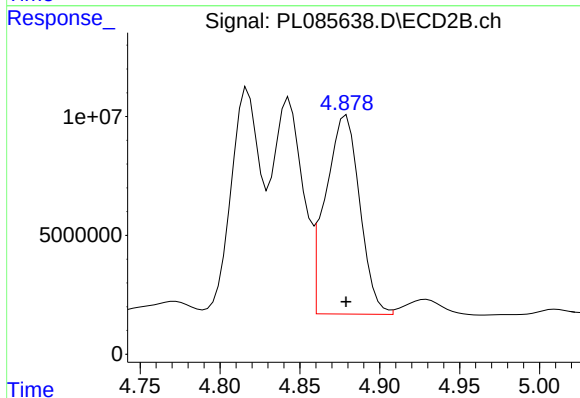


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.000 min
Response: 124284134
Conc: 1015.81 ng/ml

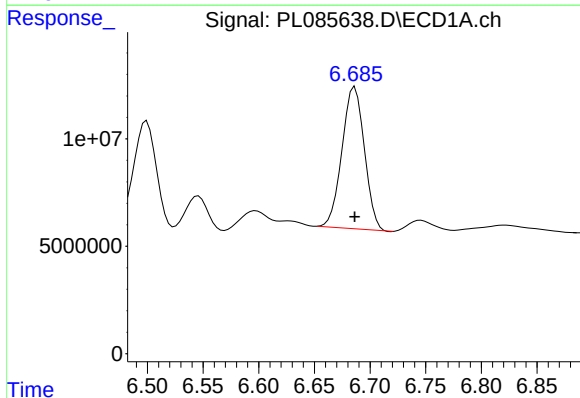


#27 Chlordane-5

R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 92113096
Conc: 1012.50 ng/ml

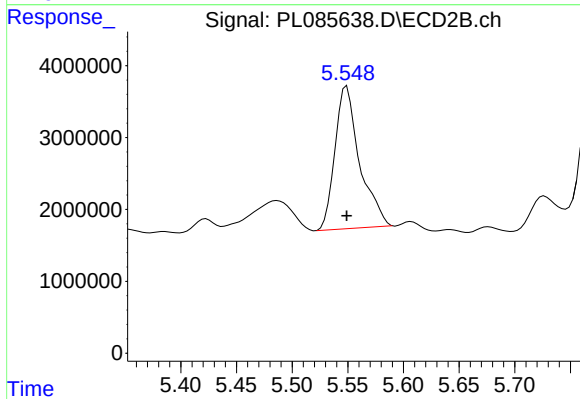

#27 Chlordane-5


R.T.: 5.549 min
Delta R.T.: 0.000 min
Response: 30665131
Conc: 997.71 ng/ml

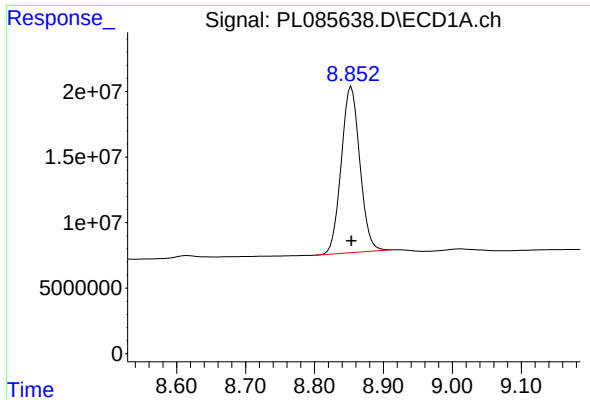

#28 Decachlorobiphenyl

R.T.: 8.853 min
Delta R.T.: 0.000 min
Response: 238038497
Conc: 99.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

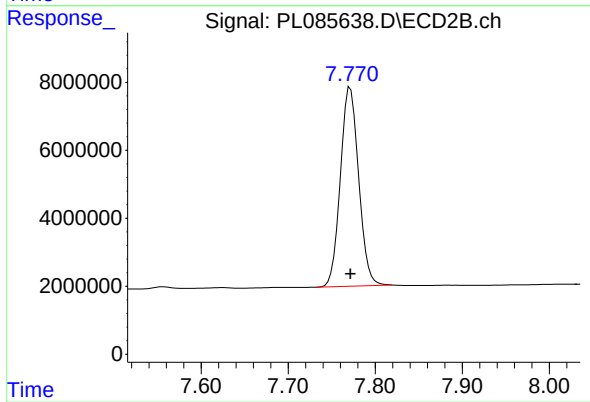

#28 Decachlorobiphenyl

R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 85636708
Conc: 98.17 ng/ml