

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
 Data File : PL085640.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 21:11
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:48:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 04:44:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	2.621	141.3E6	58276483	50.000	50.000
28)	SA Decachlor...	8.855	7.772	121.2E6	44410942	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.515	3.611	57413416	15841636	500.000	500.000
24)	Chlordane-2	5.047	4.189	57905232	19026013	500.000	500.000
25)	Chlordane-3	5.757	4.817	242.2E6	56355503	500.000	500.000
26)	Chlordane-4	5.839	4.880	299.2E6	60207454	500.000	500.000
27)	Chlordane-5	6.686	5.549	44919377	15403074	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
Data File : PL085640.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 21:11
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:48:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 04:44:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

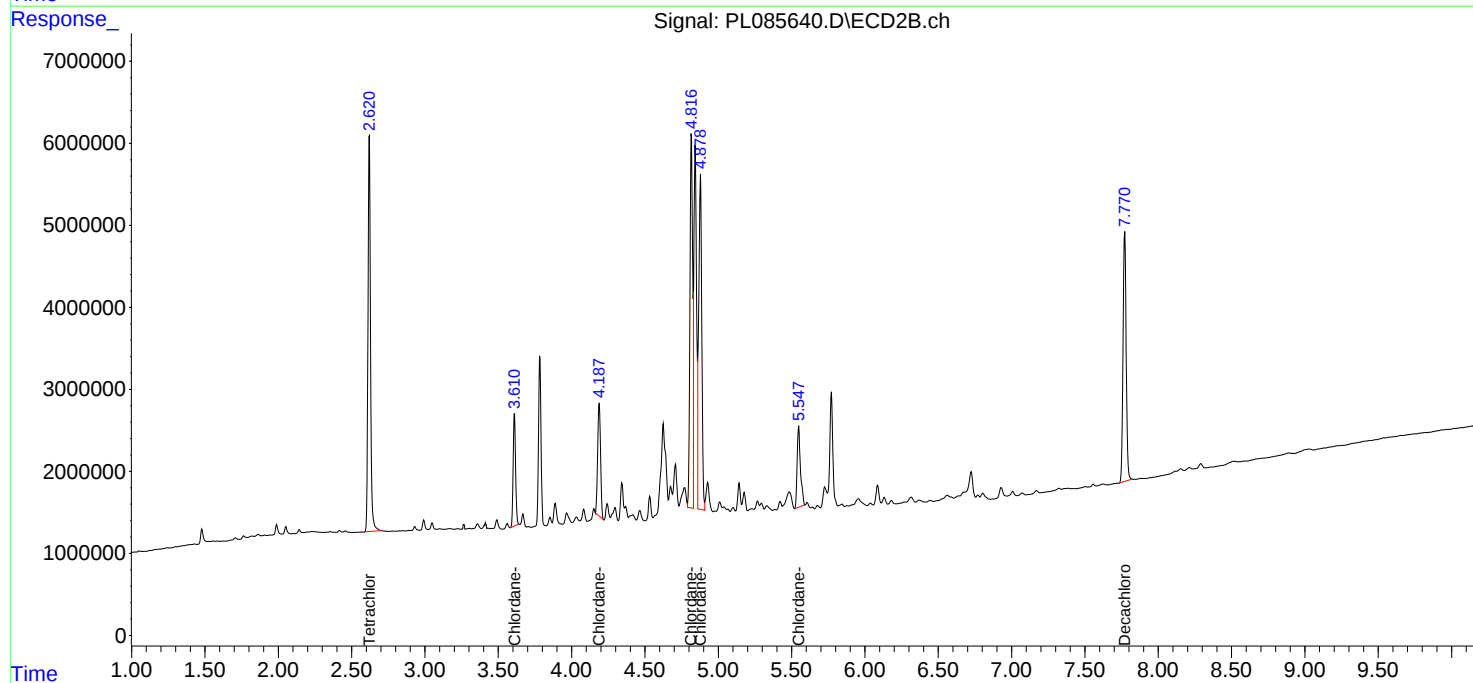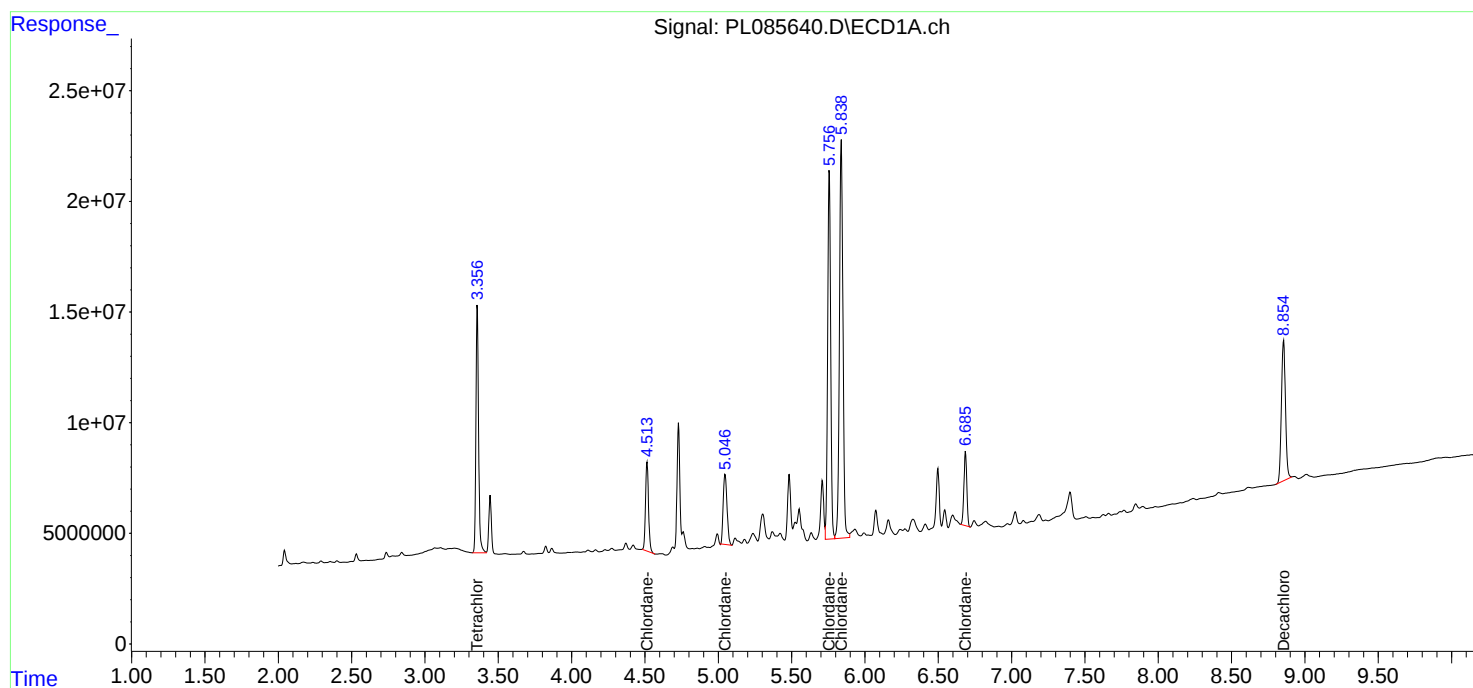


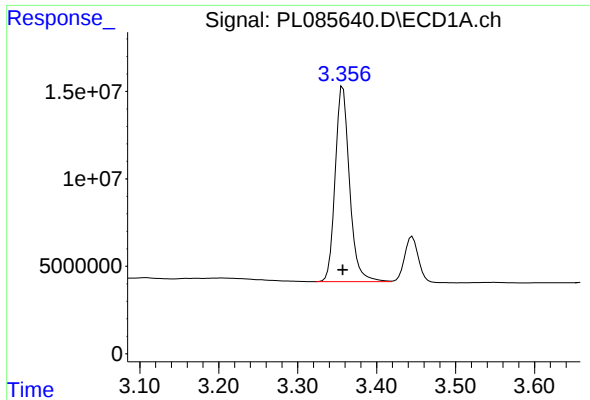

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: 0.000 min
Response: 141270514
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

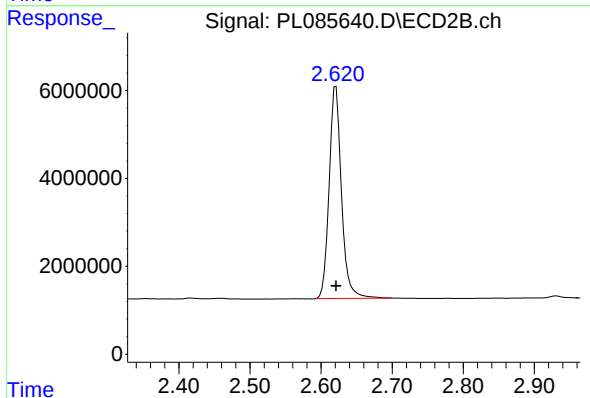


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 58276483
Conc: 50.00 ng/ml

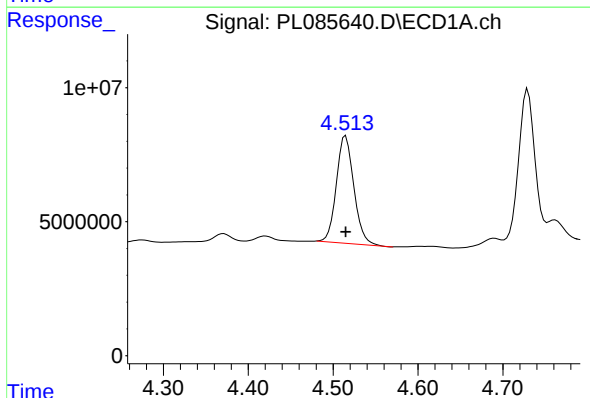


#23 Chlordane-1

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 57413416
Conc: 500.00 ng/ml

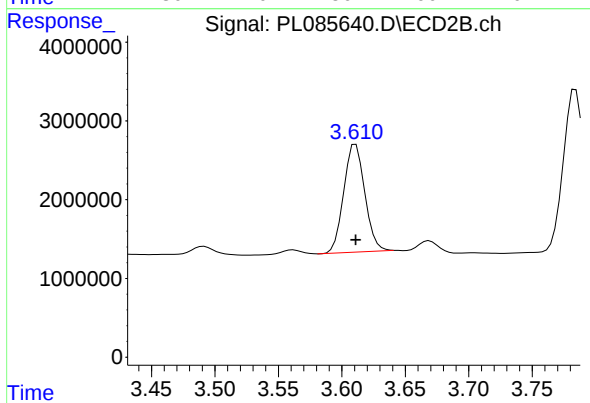

#23 Chlordane-1


R.T.: 3.611 min
Delta R.T.: 0.000 min
Response: 15841636
Conc: 500.00 ng/ml

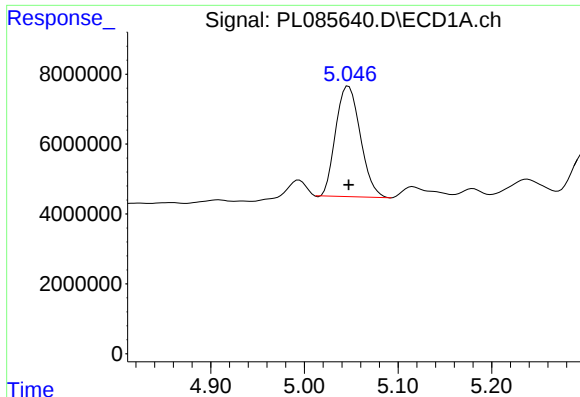

#24 Chlordane-2


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 57905232
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

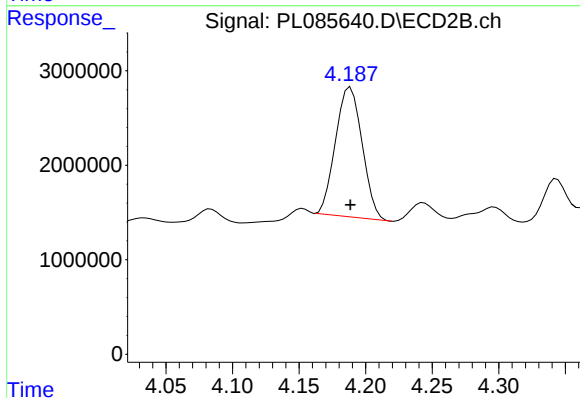


#24 Chlordane-2

R.T.: 4.189 min
Delta R.T.: 0.000 min
Response: 19026013
Conc: 500.00 ng/ml

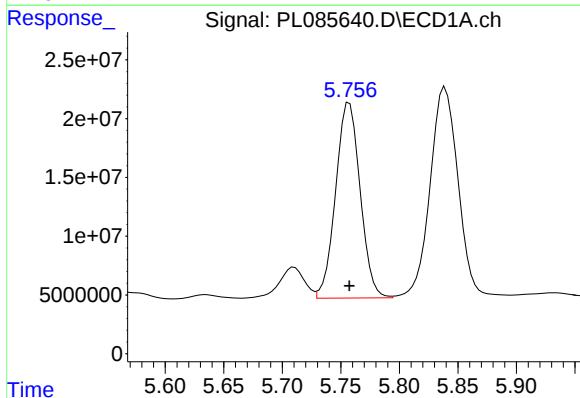


#25 Chlordane-3

R.T.: 5.757 min
Delta R.T.: 0.000 min
Response: 242224311
Conc: 500.00 ng/ml

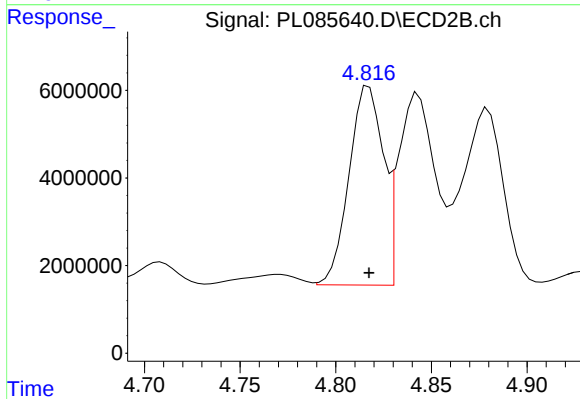

#25 Chlordane-3


R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 56355503
Conc: 500.00 ng/ml

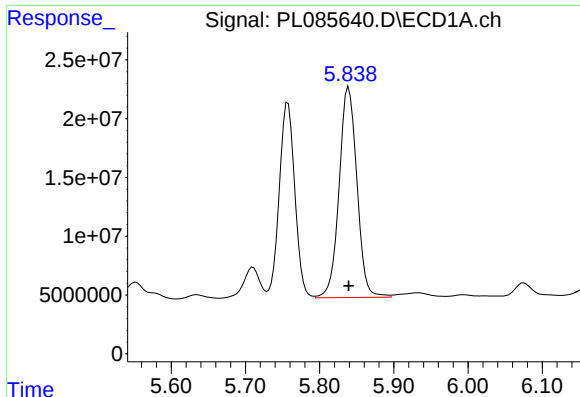

#26 Chlordane-4


R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 299236332
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

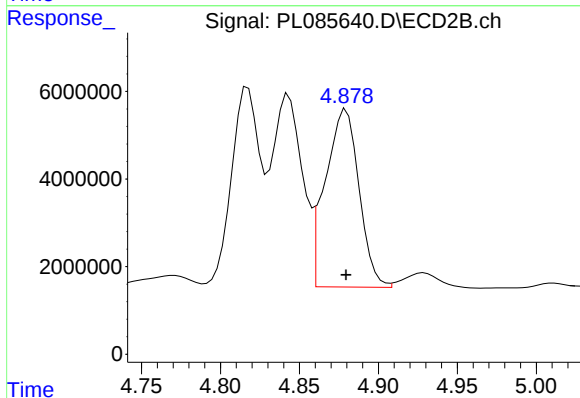


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 60207454
Conc: 500.00 ng/ml

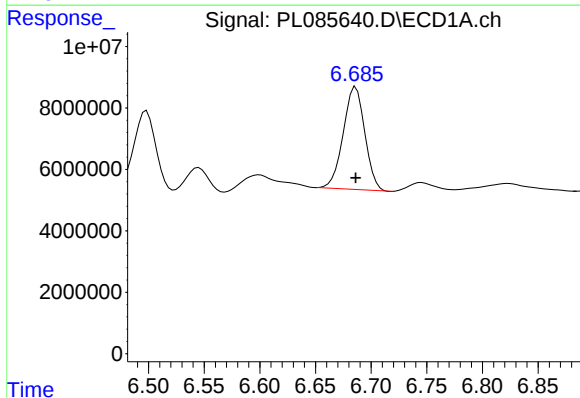


#27 Chlordane-5

R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 44919377
Conc: 500.00 ng/ml

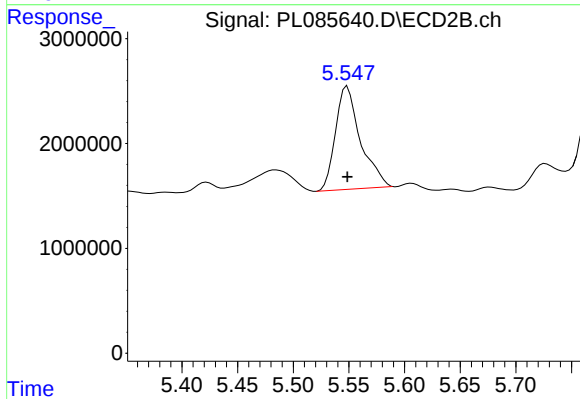

#27 Chlordane-5


R.T.: 5.549 min
Delta R.T.: 0.000 min
Response: 15403074
Conc: 500.00 ng/ml

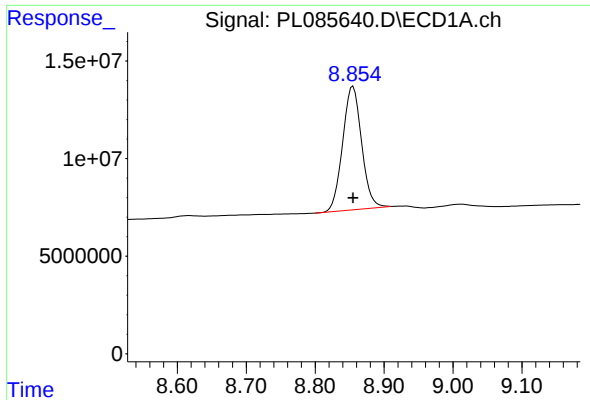

#28 Decachlorobiphenyl

R.T.: 8.855 min
Delta R.T.: 0.000 min
Response: 121238586
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

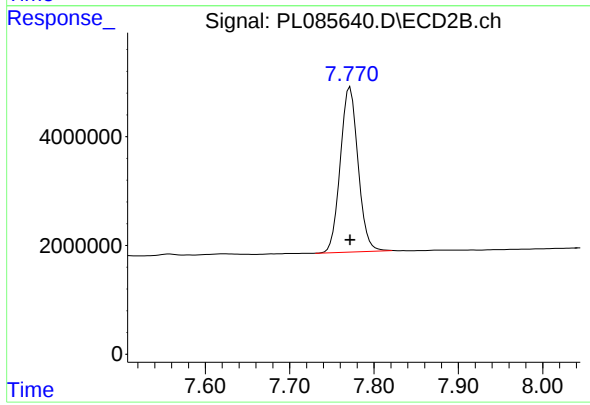

#28 Decachlorobiphenyl

R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 44410942
Conc: 50.00 ng/ml