

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
 Data File : PL085641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 21:25
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:52:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 04:52:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	2.621	66938792	27951182	23.955	23.998
28)	SA Decachlor...	8.855	7.772	60093331	21780335	25.086	25.049
Target Compounds							
23)	Chlordane-1	4.515	3.611	27996919	7633177	246.756	244.229
24)	Chlordane-2	5.047	4.189	27496039	9401658	245.419	254.372
25)	Chlordane-3	5.757	4.818	113.0E6	25561154	234.469	228.781
26)	Chlordane-4	5.841	4.879	142.4E6	28104539	239.827	234.896
27)	Chlordane-5	6.686	5.549	21266921	7466327	238.025	245.553



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
Data File : PL085641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 21:25
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:52:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 04:52:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

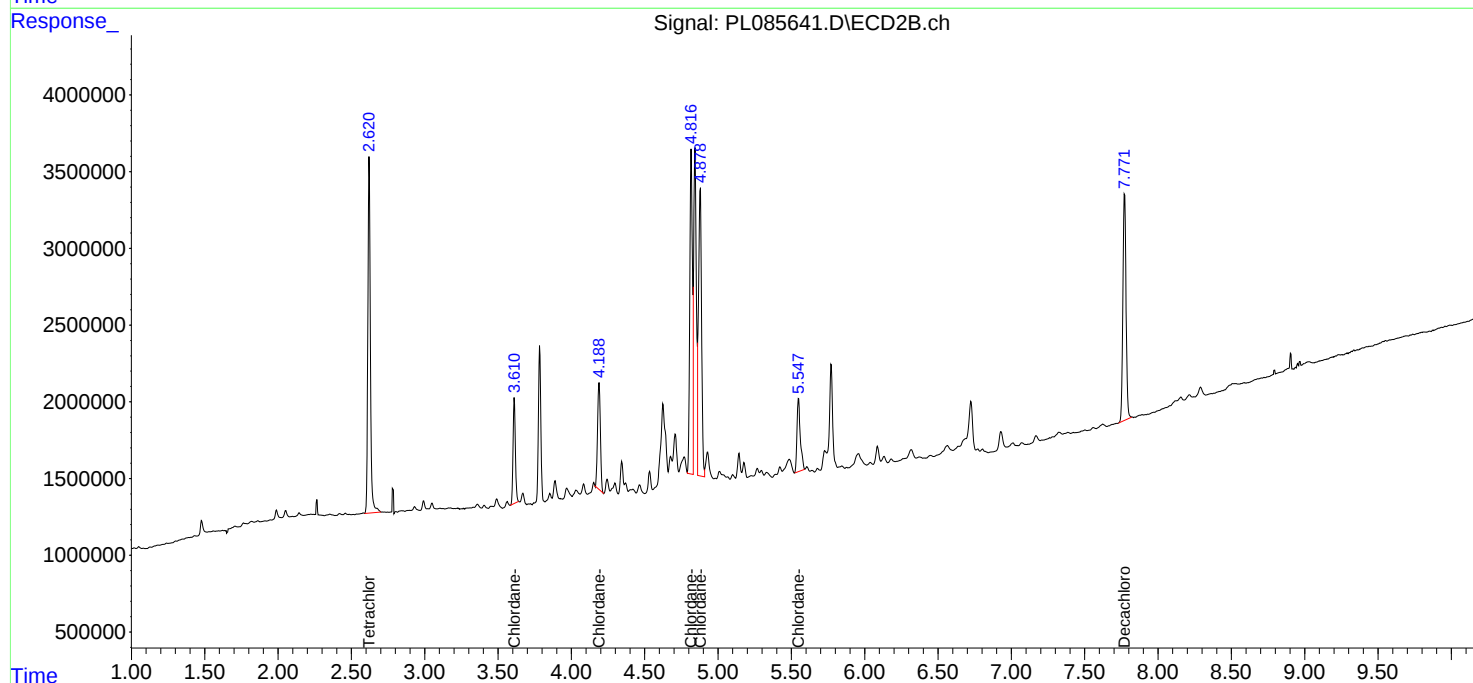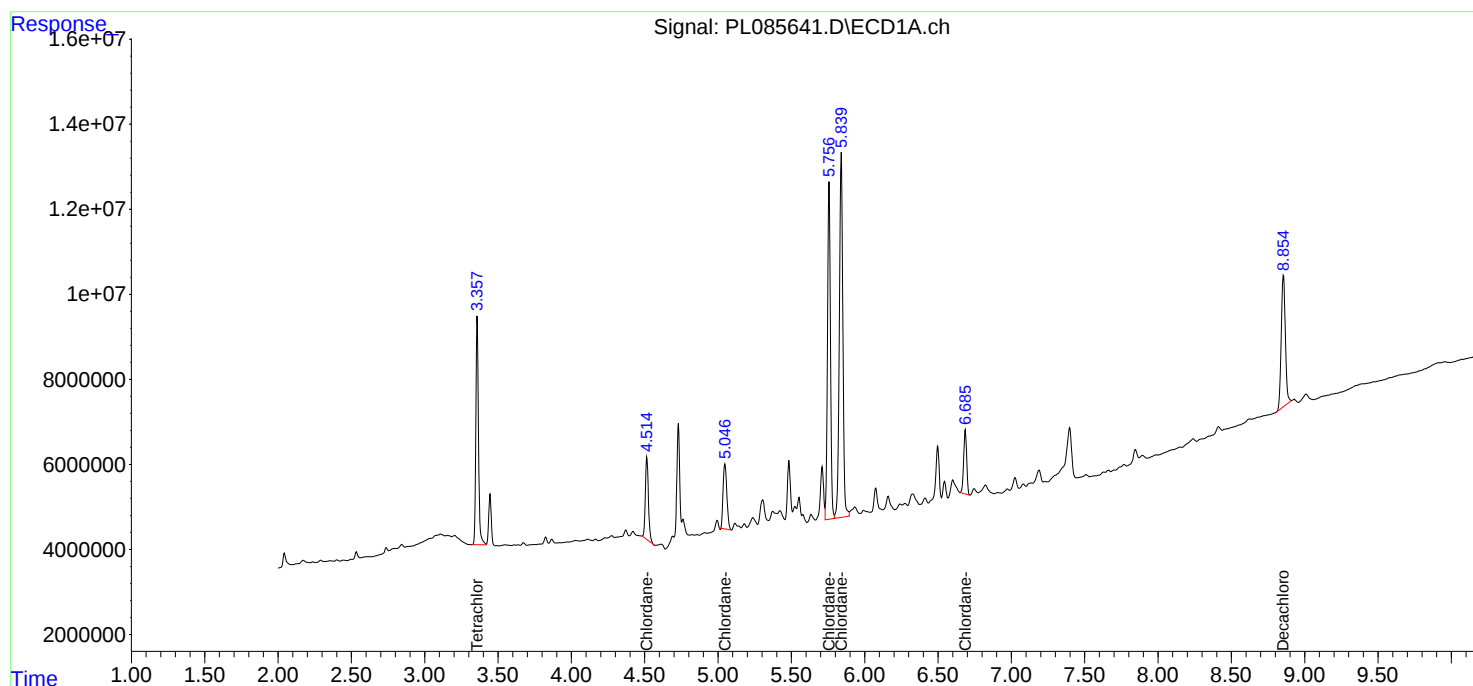


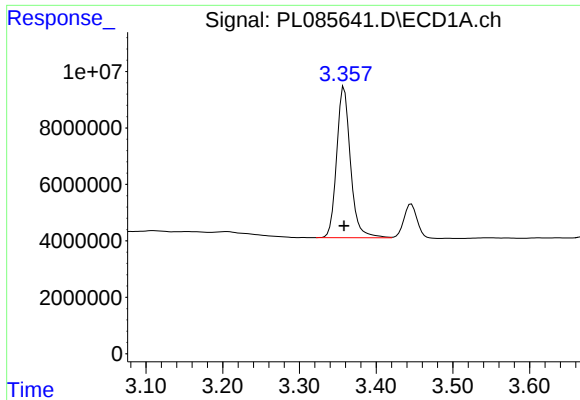

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: 0.000 min
Response: 66938792
Conc: 23.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

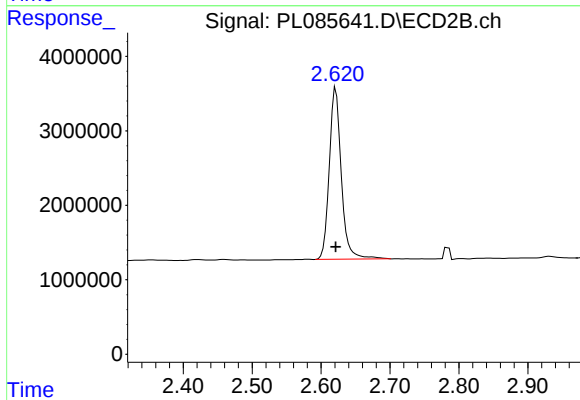


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 27951182
Conc: 24.00 ng/ml

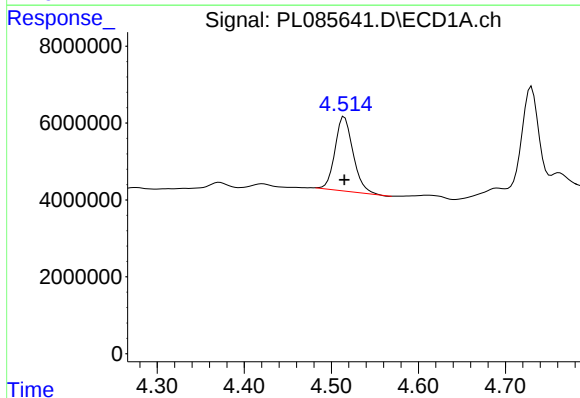


#23 Chlordane-1

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 27996919
Conc: 246.76 ng/ml

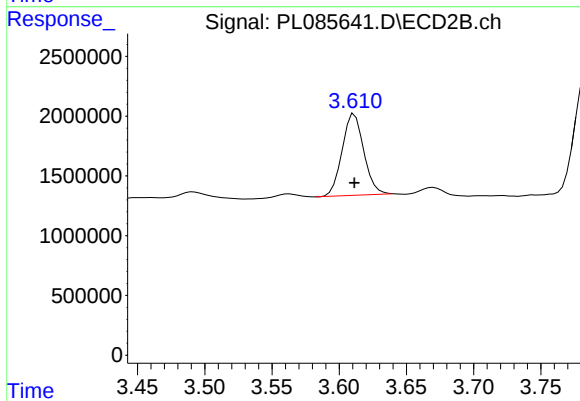

#23 Chlordane-1


R.T.: 3.611 min
Delta R.T.: 0.000 min
Response: 7633177
Conc: 244.23 ng/ml

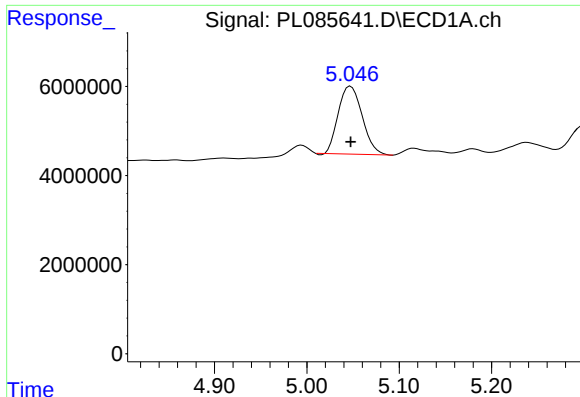

#24 Chlordane-2


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 27496039
Conc: 245.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

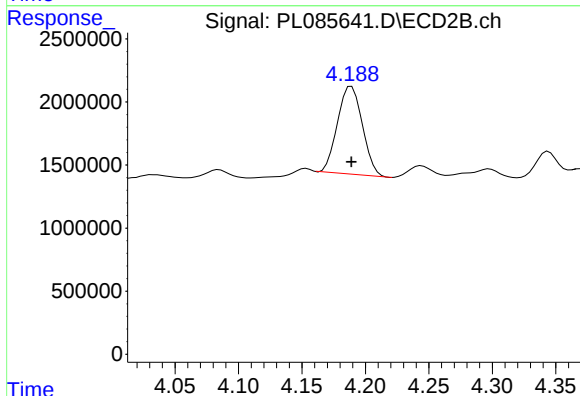


#24 Chlordane-2

R.T.: 4.189 min
Delta R.T.: 0.000 min
Response: 9401658
Conc: 254.37 ng/ml

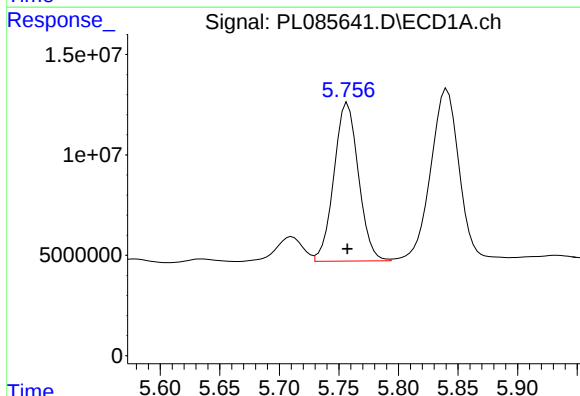


#25 Chlordane-3

R.T.: 5.757 min
Delta R.T.: 0.000 min
Response: 113003227
Conc: 234.47 ng/ml

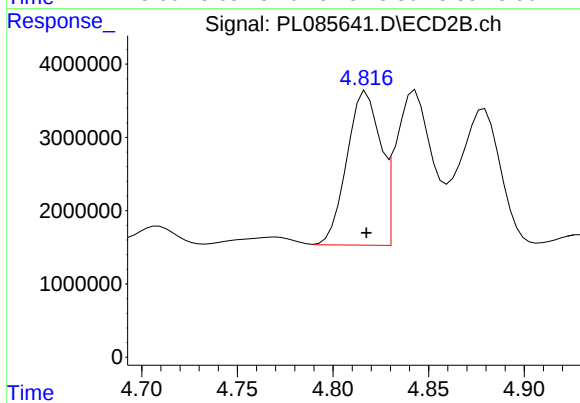

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: 0.000 min
Response: 25561154
Conc: 228.78 ng/ml

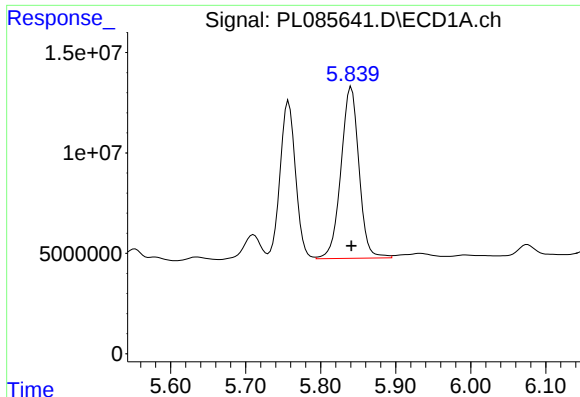

#26 Chlordane-4


R.T.: 5.841 min
Delta R.T.: 0.000 min
Response: 142370168
Conc: 239.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

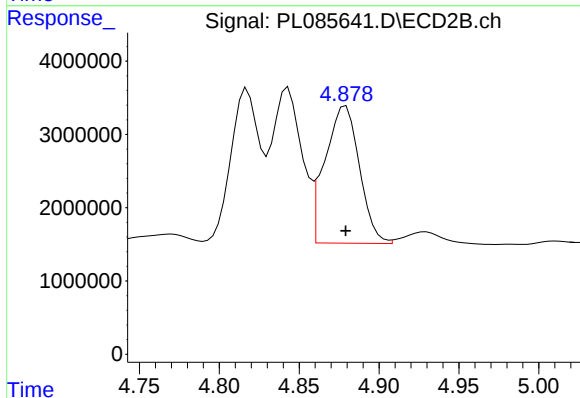


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.000 min
Response: 28104539
Conc: 234.90 ng/ml

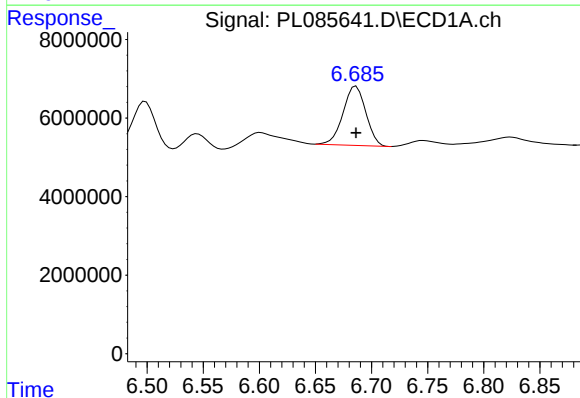


#27 Chlordane-5

R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 21266921
Conc: 238.02 ng/ml

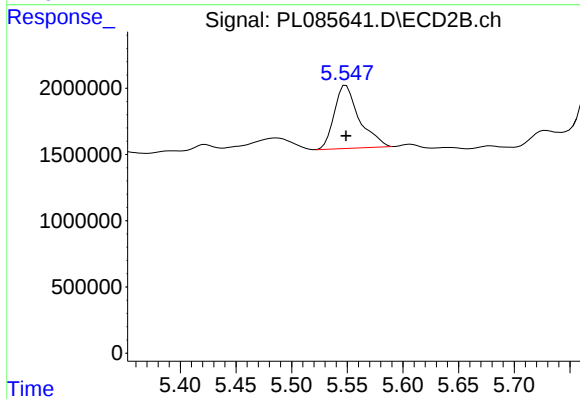

#27 Chlordane-5


R.T.: 5.549 min
Delta R.T.: 0.000 min
Response: 7466327
Conc: 245.55 ng/ml

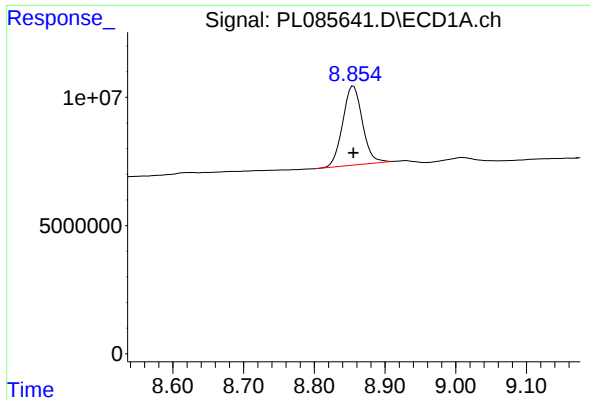

#28 Decachlorobiphenyl

R.T.: 8.855 min
Delta R.T.: 0.000 min
Response: 60093331
Conc: 25.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

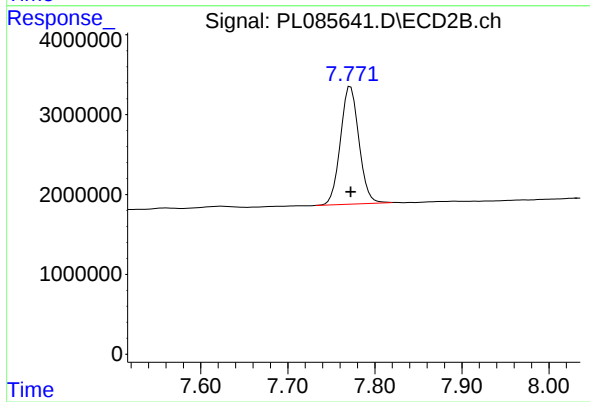

#28 Decachlorobiphenyl

R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 21780335
Conc: 25.05 ng/ml