

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
 Data File : PL085649.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 23:31
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL100223CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:47:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 04:44:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	2.621	144.4E6	58877020	51.096	50.515
28)	SA Decachlor...	8.856	7.772	123.5E6	47976620	50.935	54.014
Target Compounds							
23)	Chlordane-1	4.515	3.611	58143119	16143889	497.095	500.077
24)	Chlordane-2	5.047	4.189	59080442	19385678	472.852	496.144
25)	Chlordane-3	5.758	4.817	248.6E6	56905642	520.972	503.200
26)	Chlordane-4	5.840	4.879	306.3E6	60669686	522.048	515.655
27)	Chlordane-5	6.686	5.549	45523704	15514023	490.445	496.242



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100223\
Data File : PL085649.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 23:31
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL100223CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:47:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100223.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 04:44:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

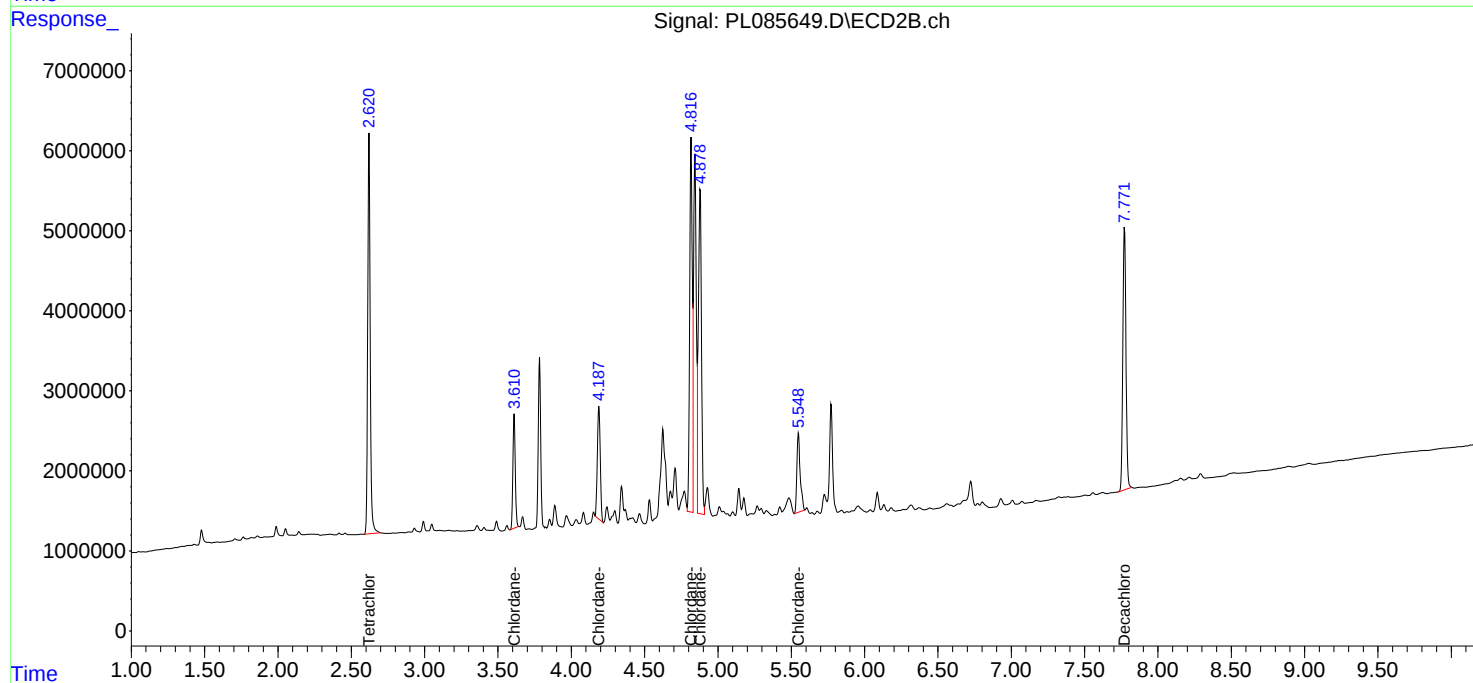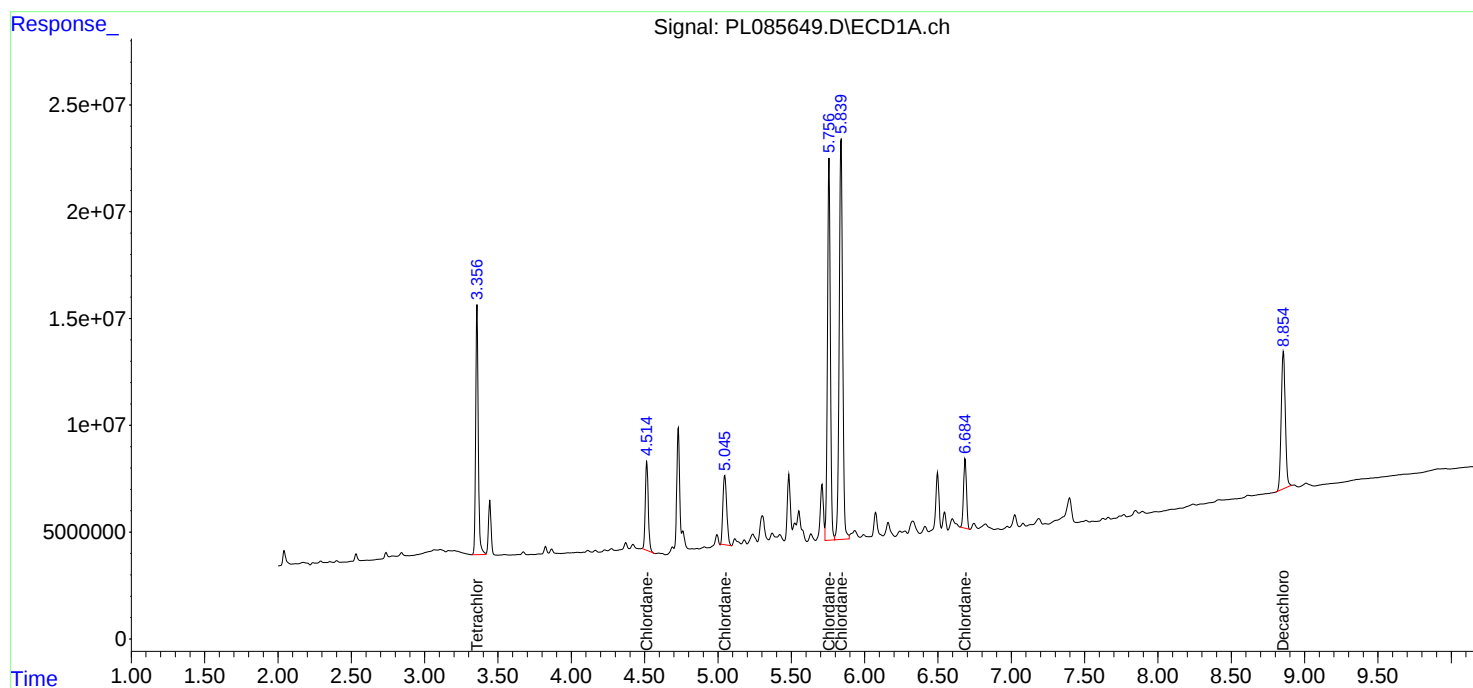


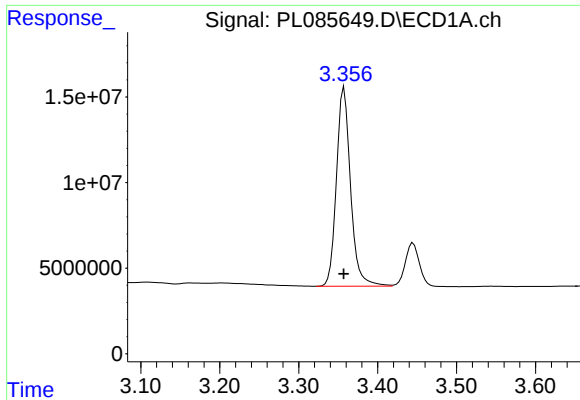

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: 0.000 min
Response: 144367976
Conc: 51.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100223CHLOR

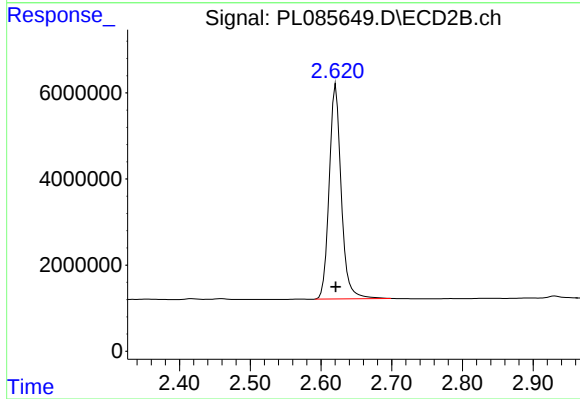


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 58877020
Conc: 50.52 ng/ml

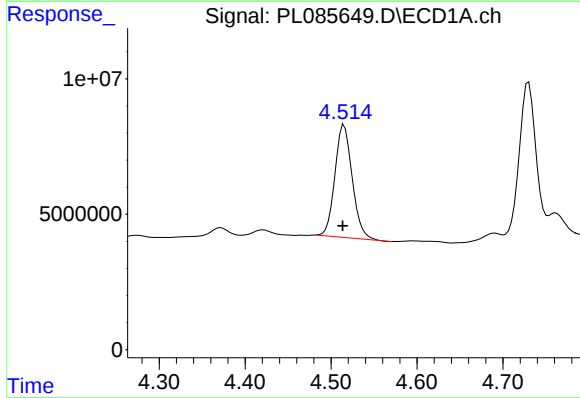


#23 Chlordane-1

R.T.: 4.515 min
Delta R.T.: 0.002 min
Response: 58143119
Conc: 497.09 ng/ml

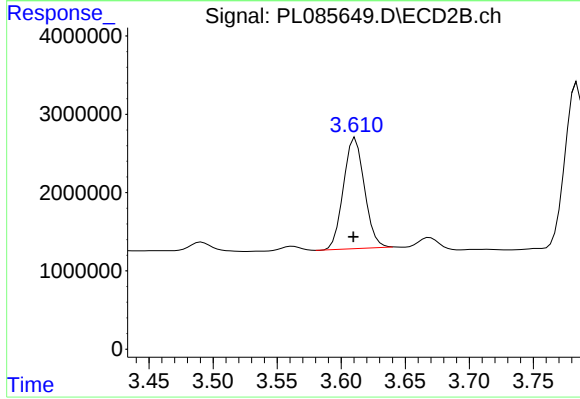

#23 Chlordane-1


R.T.: 3.611 min
Delta R.T.: 0.002 min
Response: 16143889
Conc: 500.08 ng/ml

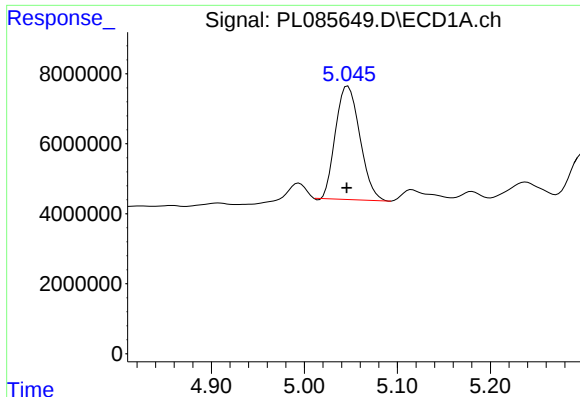

#24 Chlordane-2


R.T.: 5.047 min
Delta R.T.: 0.001 min
Response: 59080442
Conc: 472.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100223CHLOR

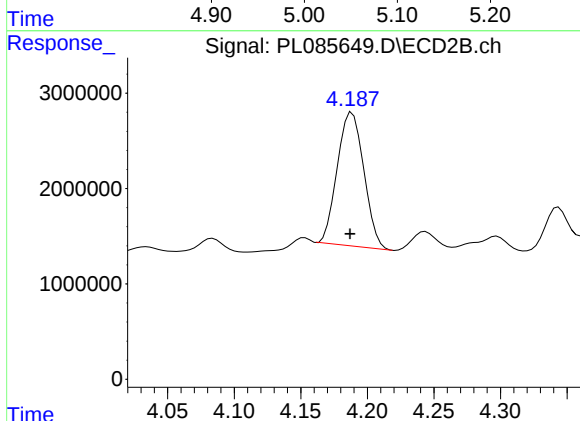


#24 Chlordane-2

R.T.: 4.189 min
Delta R.T.: 0.001 min
Response: 19385678
Conc: 496.14 ng/ml

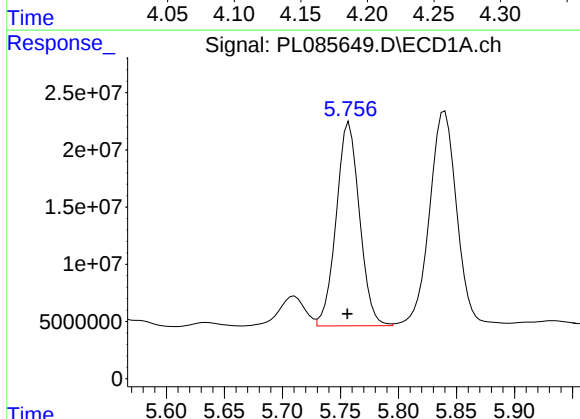


#25 Chlordane-3

R.T.: 5.758 min
Delta R.T.: 0.002 min
Response: 248613836
Conc: 520.97 ng/ml

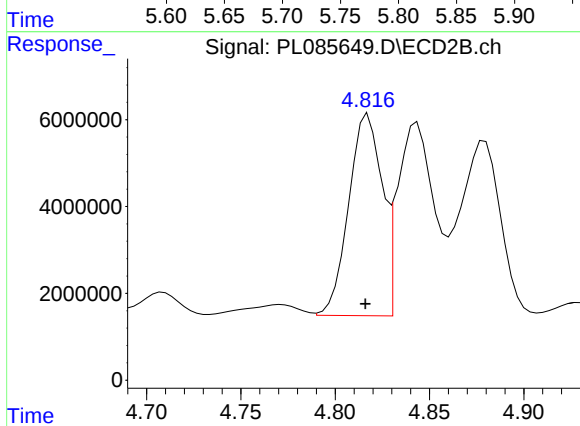

#25 Chlordane-3


R.T.: 4.817 min
Delta R.T.: 0.002 min
Response: 56905642
Conc: 503.20 ng/ml

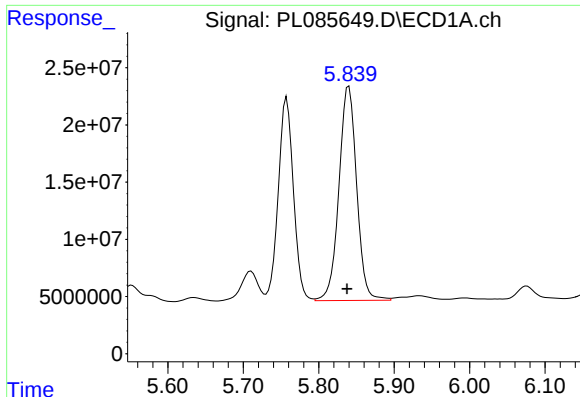

#26 Chlordane-4


R.T.: 5.840 min
Delta R.T.: 0.002 min
Response: 306292445
Conc: 522.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100223CHLOR

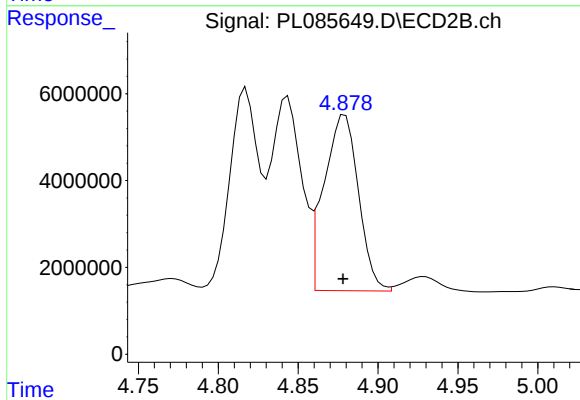


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.001 min
Response: 60669686
Conc: 515.66 ng/ml

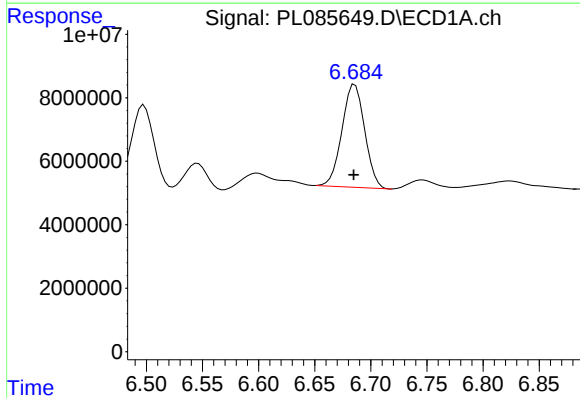


#27 Chlordane-5

R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 45523704
Conc: 490.44 ng/ml

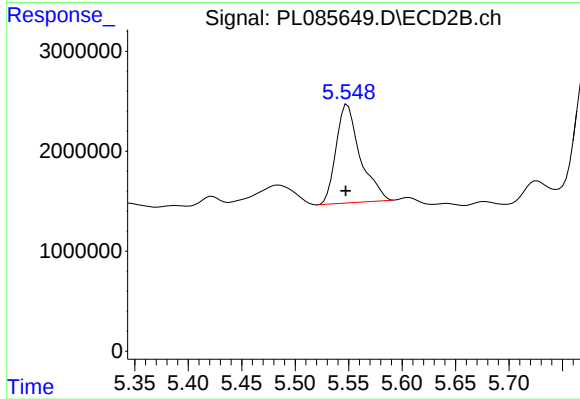

#27 Chlordane-5


R.T.: 5.549 min
Delta R.T.: 0.002 min
Response: 15514023
Conc: 496.24 ng/ml

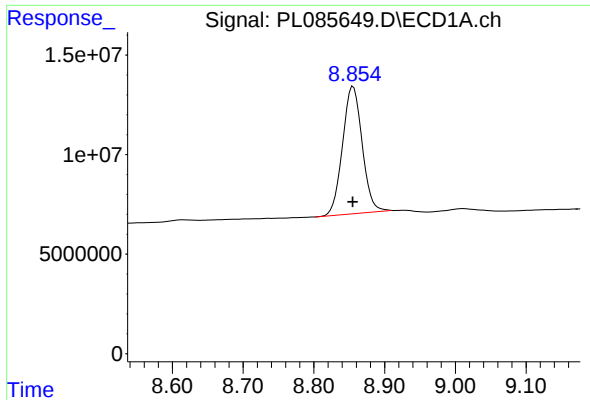

#28 Decachlorobiphenyl

R.T.: 8.856 min
Delta R.T.: 0.000 min
Response: 123506499
Conc: 50.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100223CHLOR

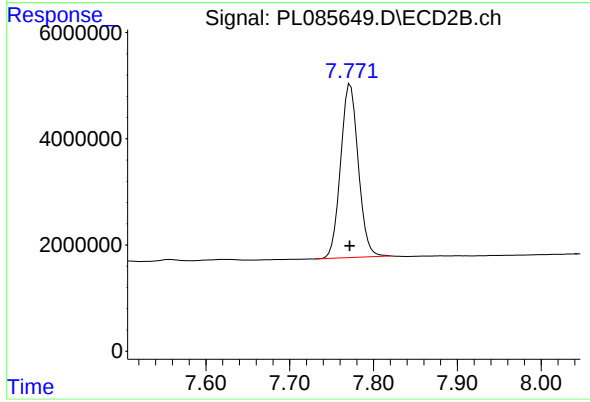

#28 Decachlorobiphenyl

R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 47976620
Conc: 54.01 ng/ml