

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100225\
 Data File : PL097492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2025 09:13
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:58:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.643	0.000	87518348	0	15.229	N.D. #
10) B	gamma-Chl...	5.880f	0.000	57136849	0	10.106	N.D. #
13) MA	Dieldrin	0.000	5.437	0	42496390	N.D.	5.197 #
14) MA	Endrin	0.000	5.706	0	126.7E6	N.D.	16.868 #
15) B	Endosulfa...	0.000	5.995	0	3042109	N.D.	0.428 #
25)	Chlordane-3	5.880f	0.000	57136849	0	70.052	N.D. #
27)	Chlordane-5	0.000	5.995	0	3042109	N.D.	10.204 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100225\
Data File : PL097492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2025 09:13
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:58:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

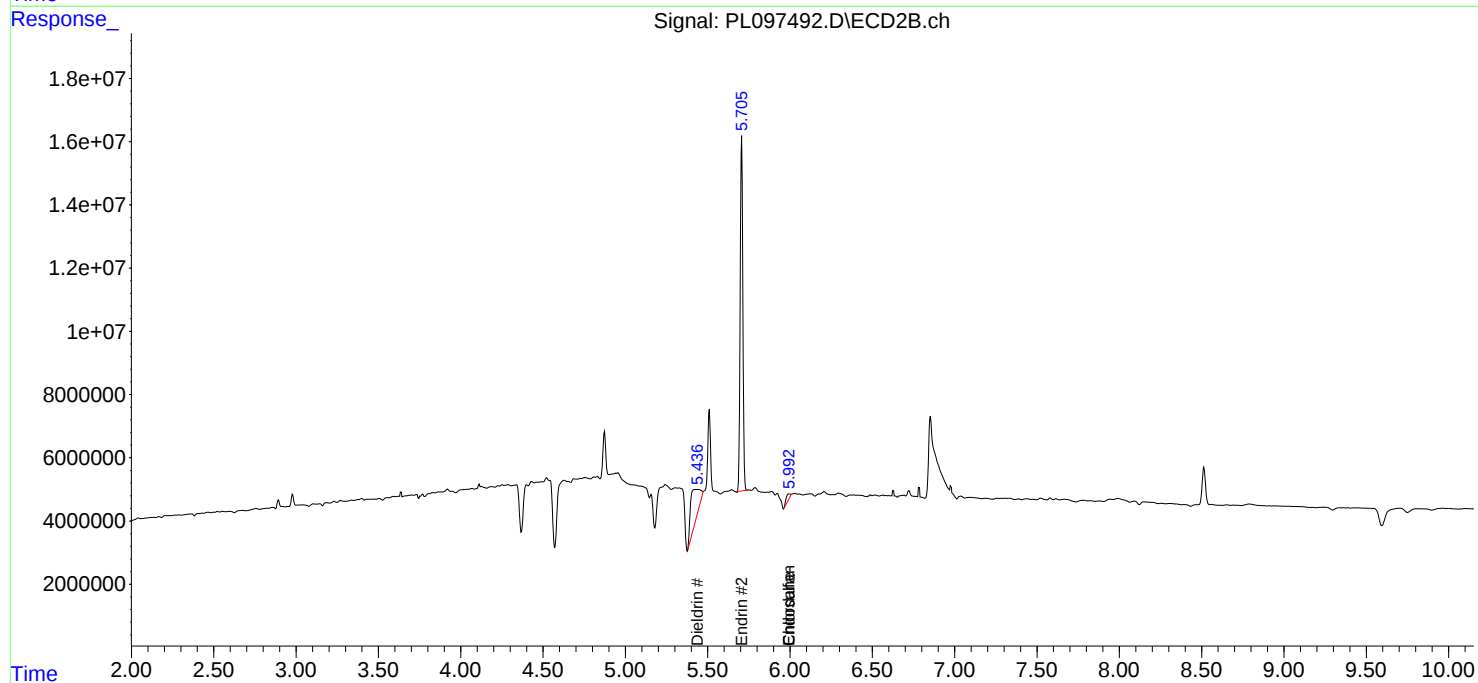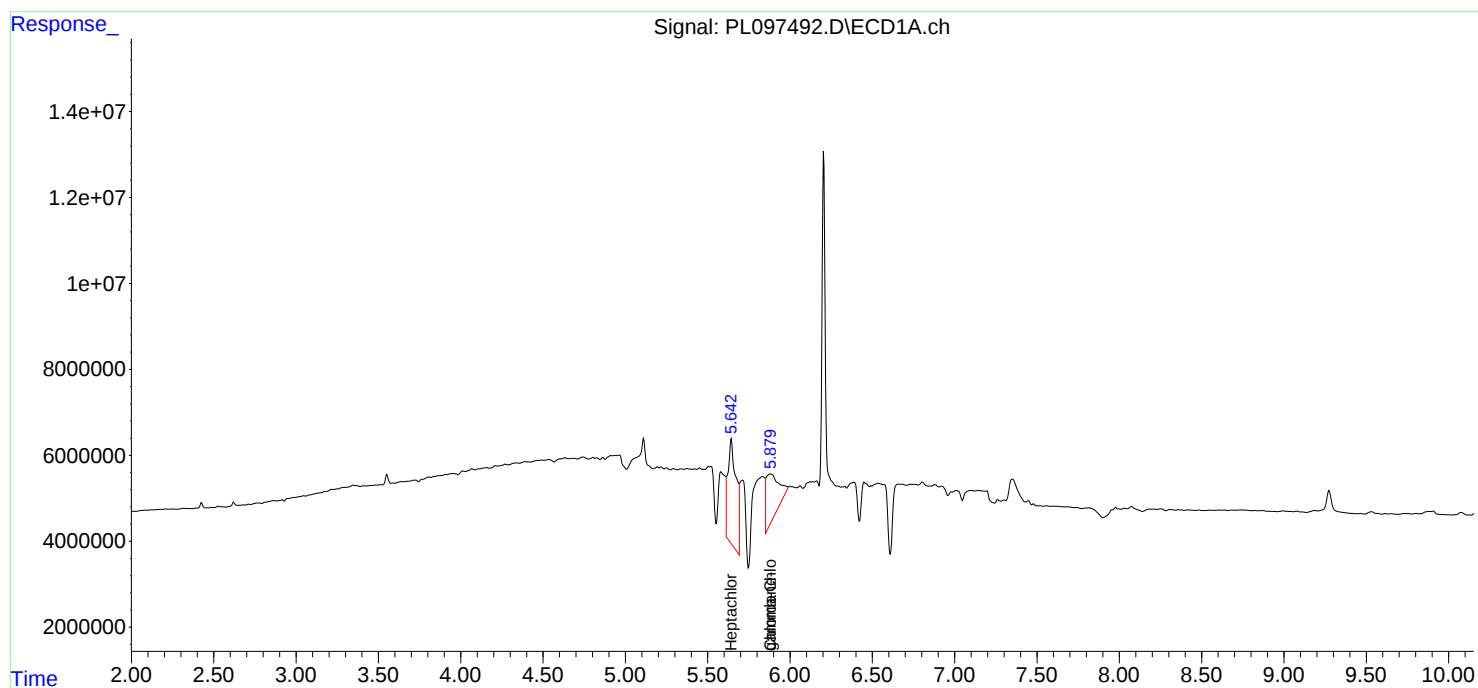


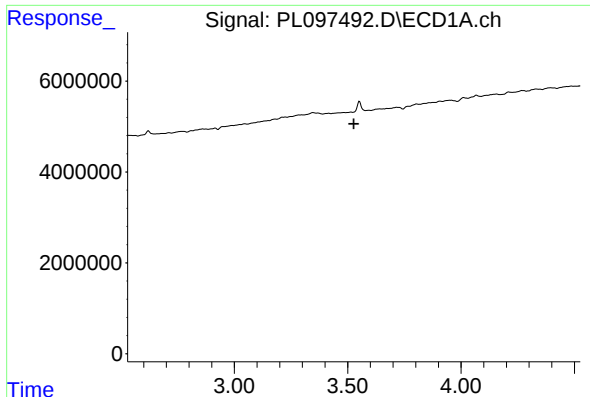

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

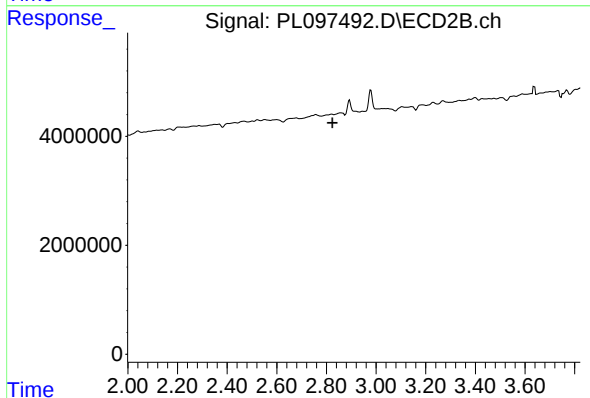

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 2.823 min
Response: 0
Conc: N.D.

#8 Heptachlor epoxide

R.T.: 5.643 min
Delta R.T.: -0.009 min
Response: 87518348
Conc: 15.23 ng/ml

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.793 min
Response: 0
Conc: N.D.

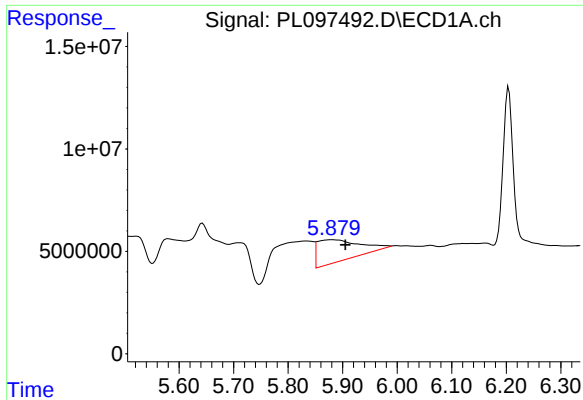

#10 gamma-Chlordane


R.T.: 5.880 min
Delta R.T.: -0.025 min
Response: 57136849
Conc: 10.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

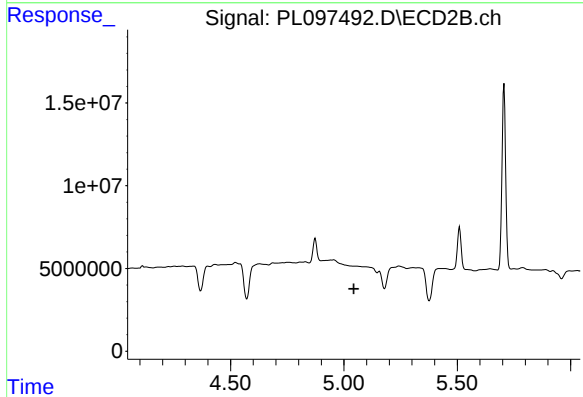


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.044 min
Response: 0
Conc: N.D.

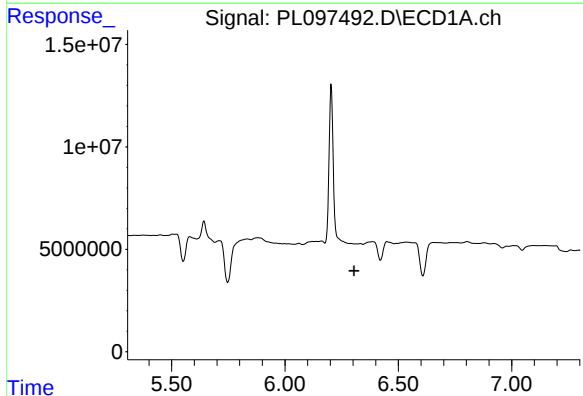


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.306 min
Response: 0
Conc: N.D.

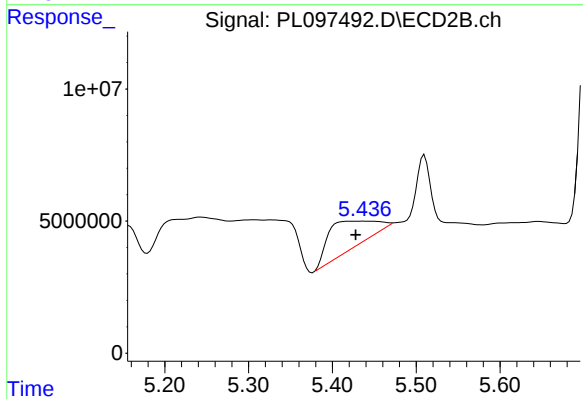

#13 Dieldrin


R.T.: 5.437 min
Delta R.T.: 0.009 min
Response: 42496390
Conc: 5.20 ng/ml

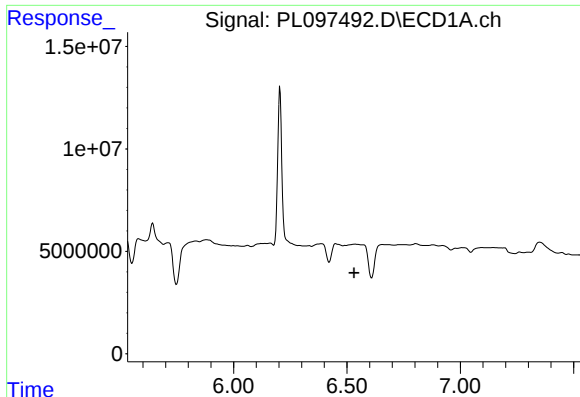

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

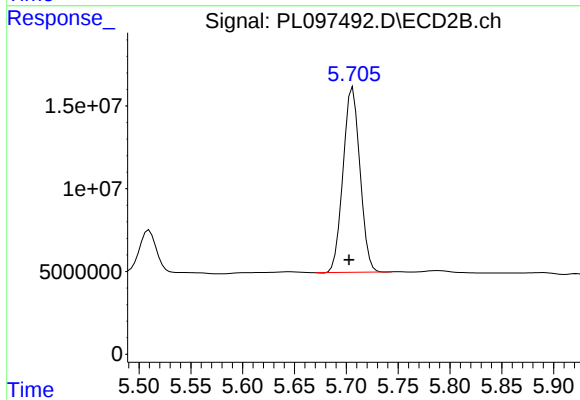


#14 Endrin

R.T.: 5.706 min
Delta R.T.: 0.004 min
Response: 126690598
Conc: 16.87 ng/ml

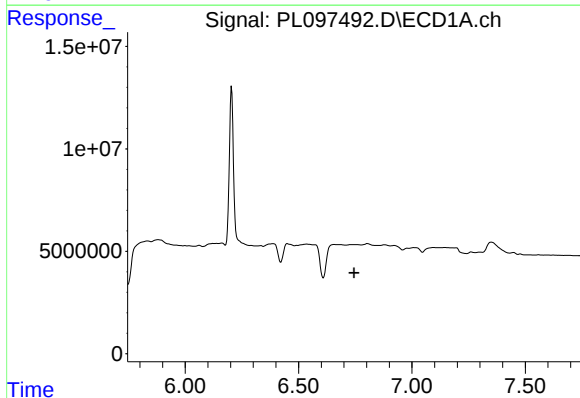


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.745 min
Response: 0
Conc: N.D.

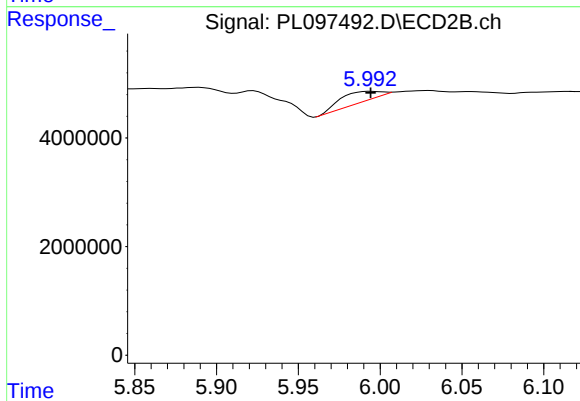

#15 Endosulfan II


R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 3042109
Conc: 0.43 ng/ml

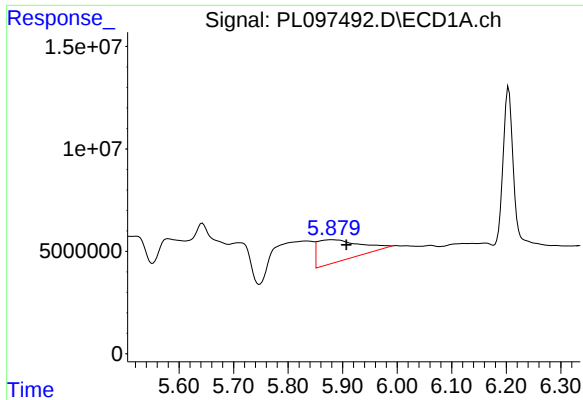

#25 Chlordane-3


R.T.: 5.880 min
Delta R.T.: -0.026 min
Response: 57136849
Conc: 70.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

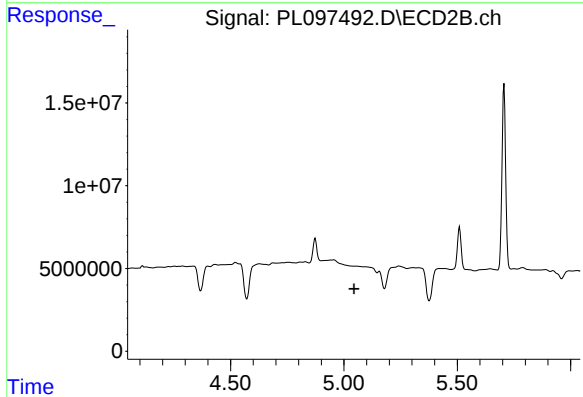


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.045 min
Response: 0
Conc: N.D.

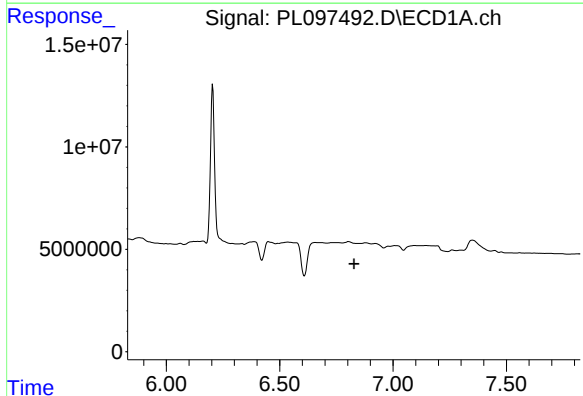


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.828 min
Response: 0
Conc: N.D.

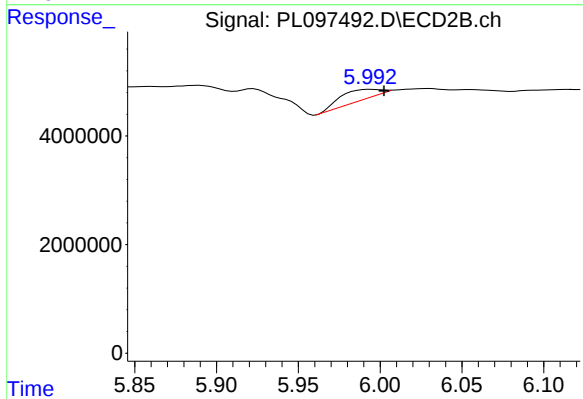

#27 Chlordane-5


R.T.: 5.995 min
Delta R.T.: -0.008 min
Response: 3042109
Conc: 10.20 ng/ml

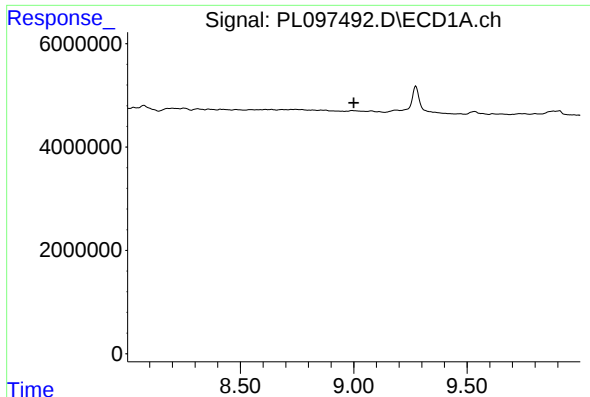

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.001 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

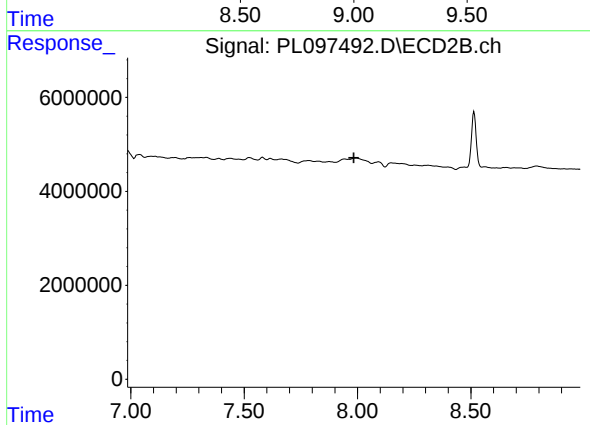

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.984 min
Response: 0
Conc: N.D.