

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100225\
 Data File : PL097498.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2025 14:29
 Operator : AR\AJ
 Sample : Q3262-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MOO-25-0280

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:59:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.819	70408909	69140049	15.553	10.515 #
28)	SA Decachlor...	8.999	7.979	40740136	57955471	12.450	10.183
Target Compounds							
3)	MA gamma-BHC...	0.000	3.659	0	8392275	N.D.	0.901 #
8)	B Heptachlo...	5.667f	0.000	10949684	0	1.905	N.D. #
9)	A Endosulfan I	6.058f	5.179f	11185143	44376124	2.159	5.775 #
11)	B alpha-Chl...	0.000	5.095	0	17114702	N.D.	2.062 #
13)	MA Dieldrin	0.000	5.425	0	16007782	N.D.	1.958 #
16)	A 4,4'-DDD	0.000	5.840	0	19804745	N.D.	3.071 #
17)	MA 4,4'-DDT	0.000	6.112	0	9812948	N.D.	1.418 #
20)	A Methoxychlor	0.000	6.696f	0	14607390	N.D.	3.875 #
21)	B Endrin ke...	7.566f	0.000	17430631	0	4.107	N.D. #
24)	Chlordane-2	5.177f	0.000	22759153	0	102.531	N.D. #
26)	Chlordane-4	0.000	5.095	0	17114702	N.D.	22.474 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100225\
Data File : PL097498.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2025 14:29
Operator : AR\AJ
Sample : Q3262-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MOO-25-0280

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:59:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

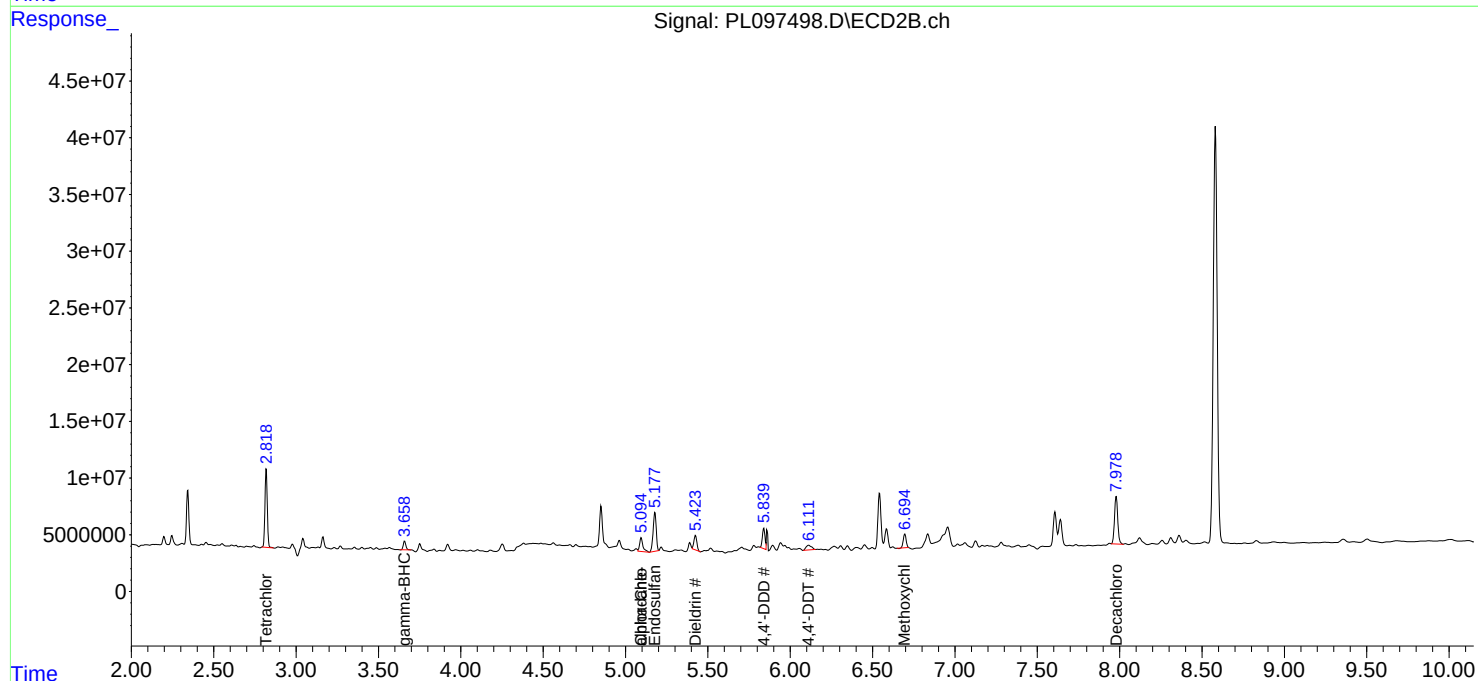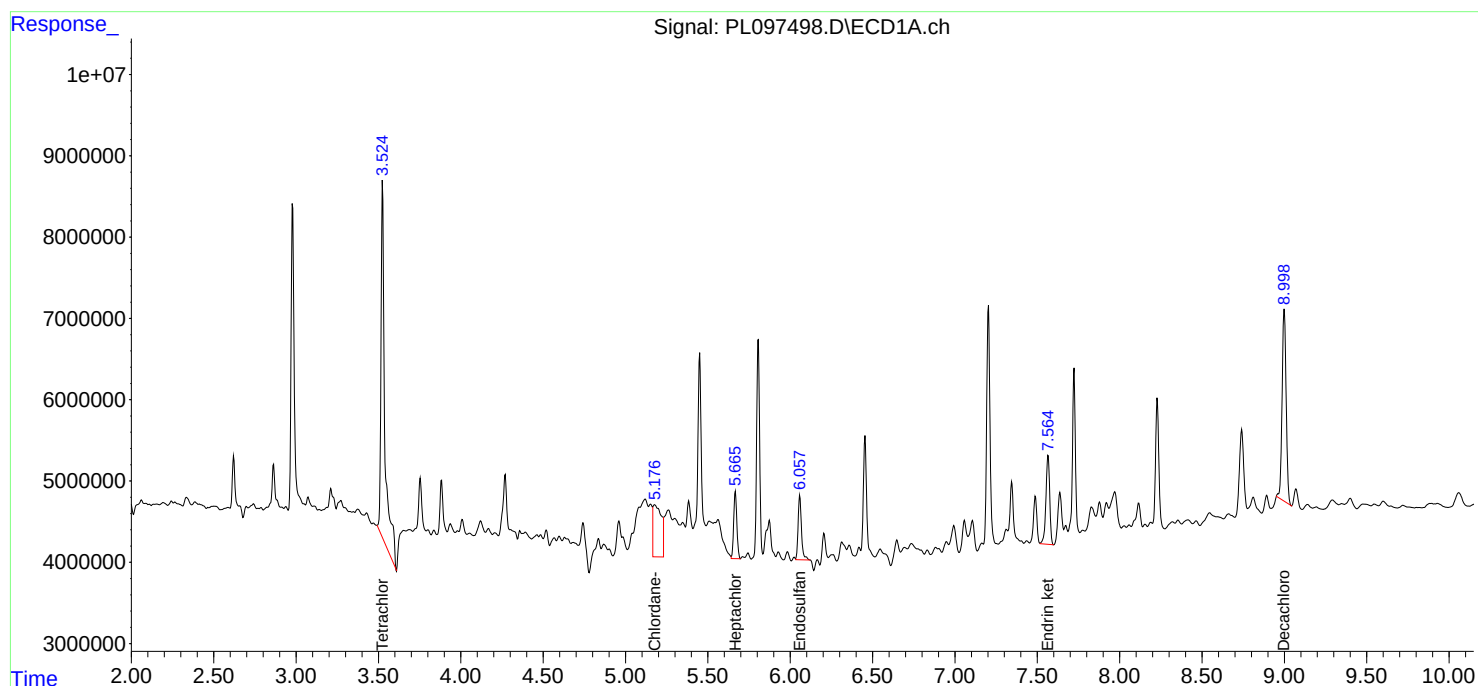


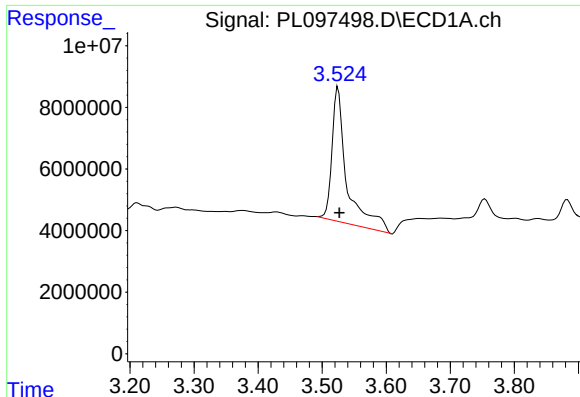

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: -0.002 min
Response: 70408909
Conc: 15.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-25-0280

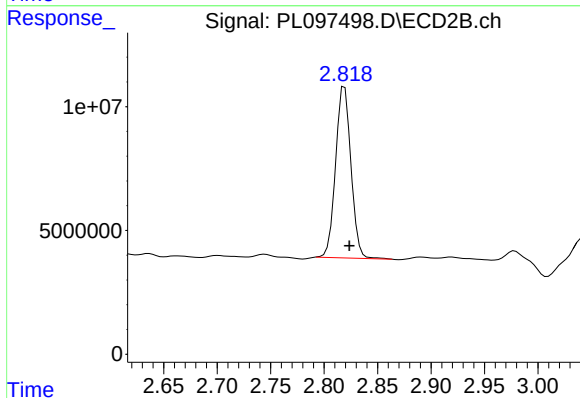


#1 Tetrachloro-m-xylene

R.T.: 2.819 min
Delta R.T.: -0.004 min
Response: 69140049
Conc: 10.51 ng/ml

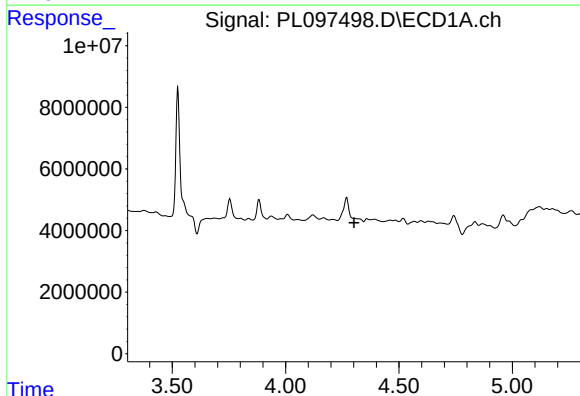


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.302 min
Response: 0
Conc: N.D.

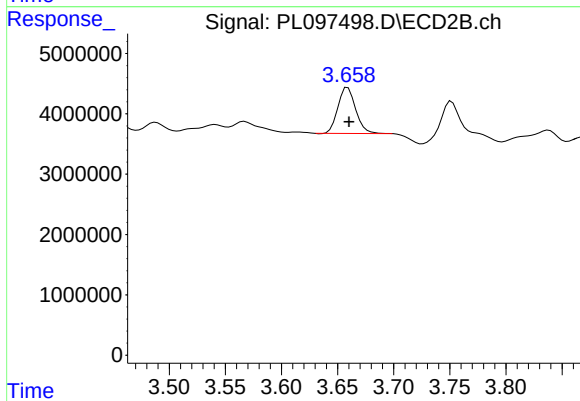

#3 gamma-BHC (Lindane)


R.T.: 3.659 min
Delta R.T.: -0.001 min
Response: 8392275
Conc: 0.90 ng/ml

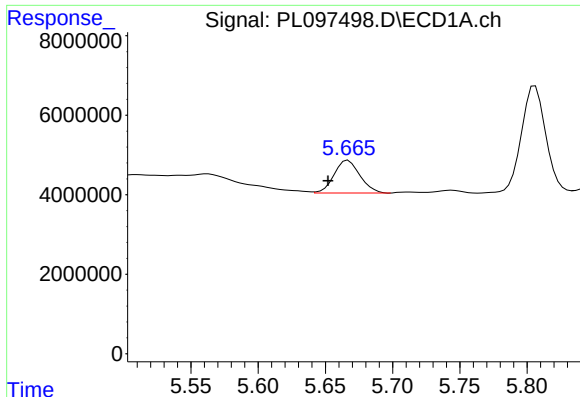

#8 Heptachlor epoxide


R.T.: 5.667 min
Delta R.T.: 0.015 min
Response: 10949684
Conc: 1.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-25-0280

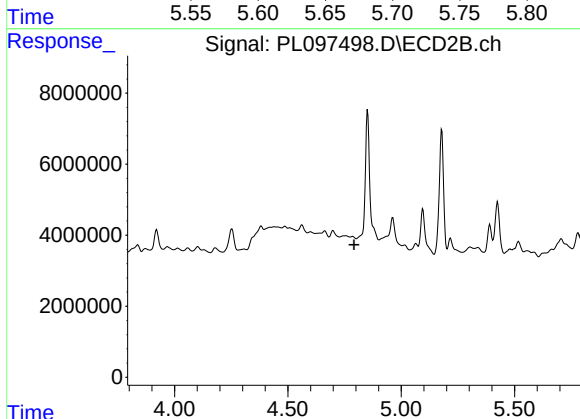


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.793 min
Response: 0
Conc: N.D.

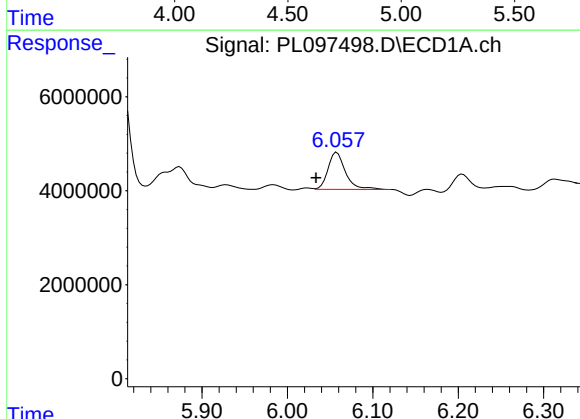


#9 Endosulfan I

R.T.: 6.058 min
Delta R.T.: 0.025 min
Response: 11185143
Conc: 2.16 ng/ml

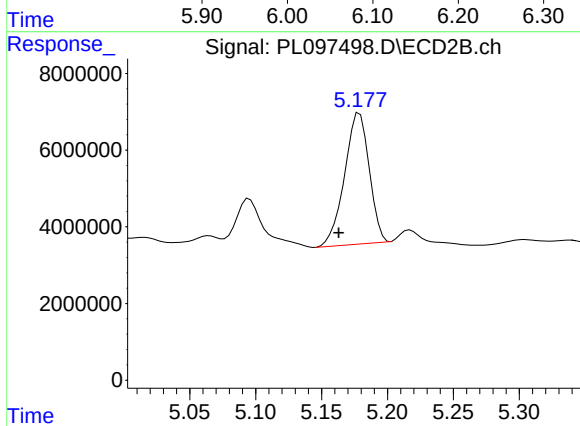

#9 Endosulfan I


R.T.: 5.179 min
Delta R.T.: 0.016 min
Response: 44376124
Conc: 5.78 ng/ml

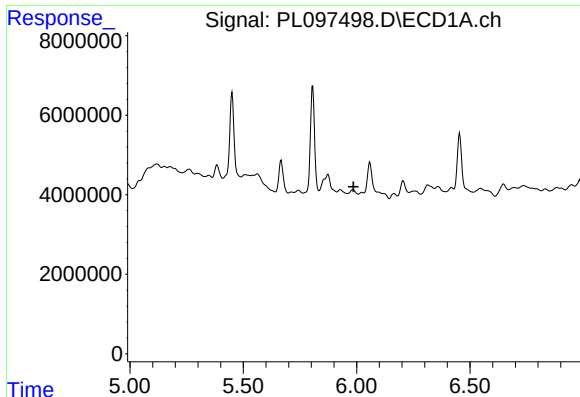

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.986 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MOO-25-0280

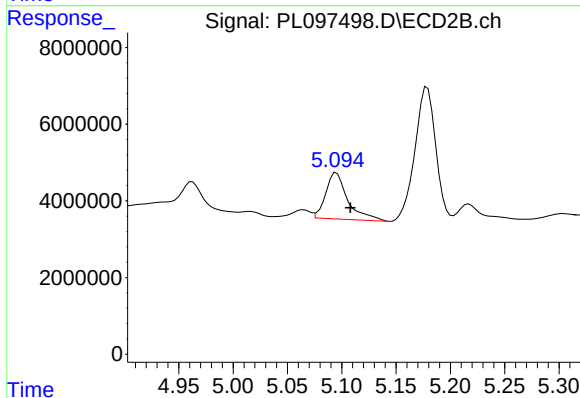


#11 alpha-Chlordane

R.T.: 5.095 min
Delta R.T.: -0.013 min
Response: 17114702
Conc: 2.06 ng/ml

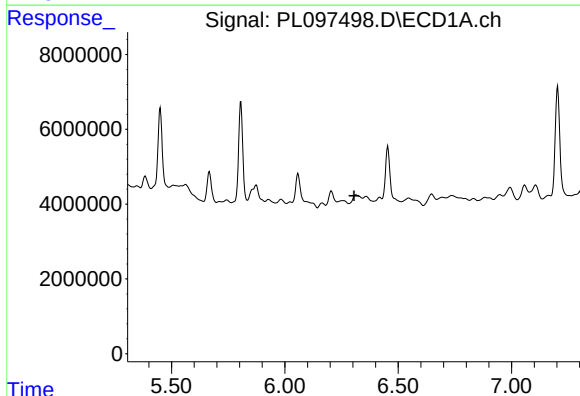


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.306 min
Response: 0
Conc: N.D.

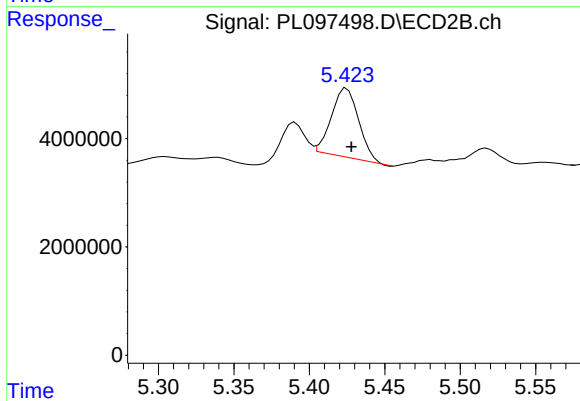

#13 Dieldrin


R.T.: 5.425 min
Delta R.T.: -0.003 min
Response: 16007782
Conc: 1.96 ng/ml

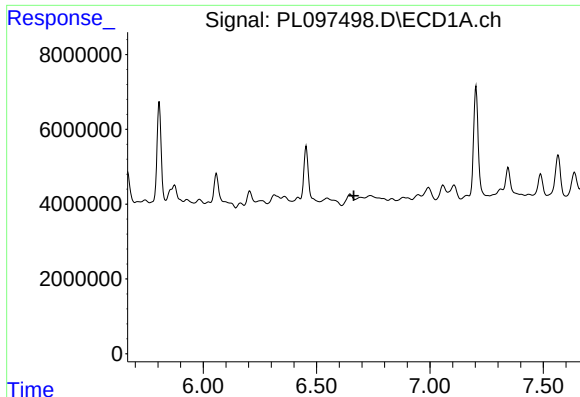

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.665 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MOO-25-0280

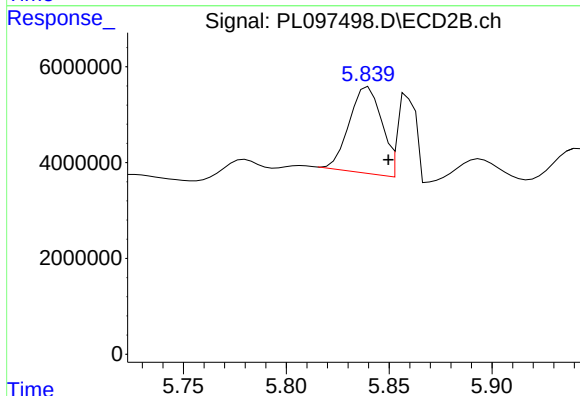


#16 4,4'-DDD

R.T.: 5.840 min
Delta R.T.: -0.010 min
Response: 19804745
Conc: 3.07 ng/ml

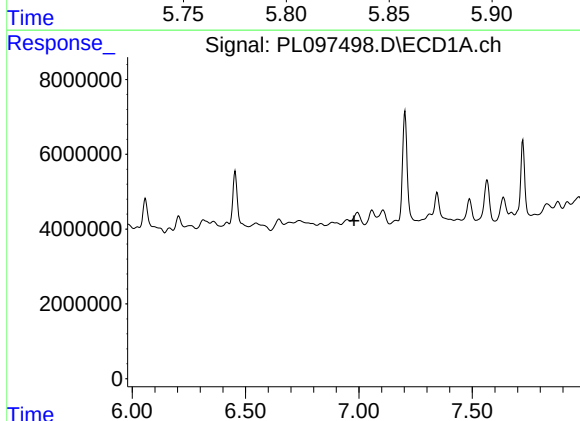


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.979 min
Response: 0
Conc: N.D.

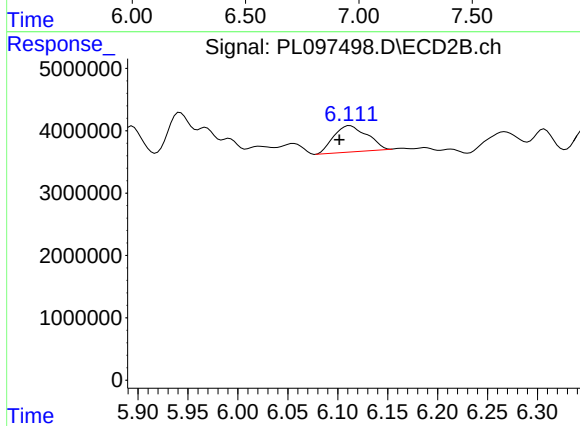

#17 4,4'-DDT


R.T.: 6.112 min
Delta R.T.: 0.011 min
Response: 9812948
Conc: 1.42 ng/ml

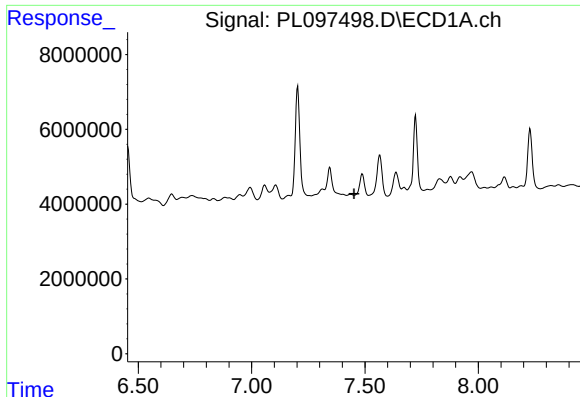

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MOO-25-0280

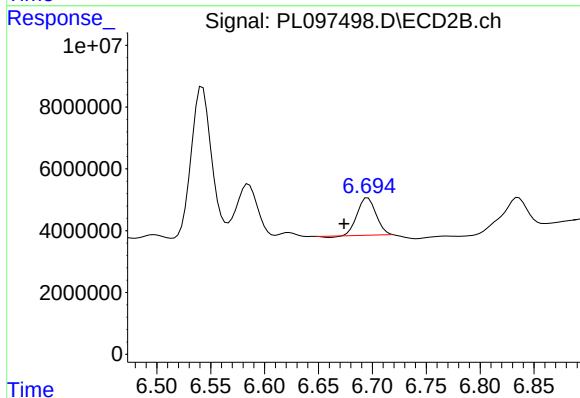


#20 Methoxychlor

R.T.: 6.696 min
Delta R.T.: 0.022 min
Response: 14607390
Conc: 3.88 ng/ml

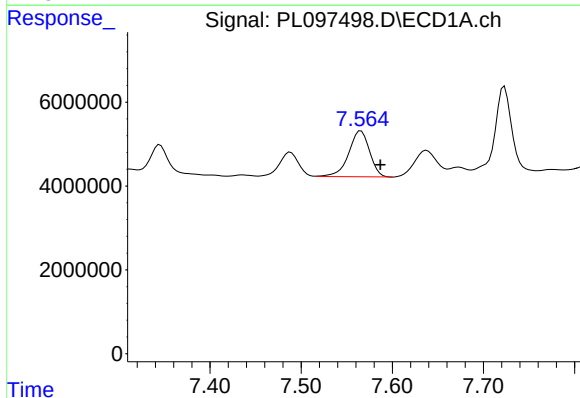


#21 Endrin ketone

R.T.: 7.566 min
Delta R.T.: -0.021 min
Response: 17430631
Conc: 4.11 ng/ml

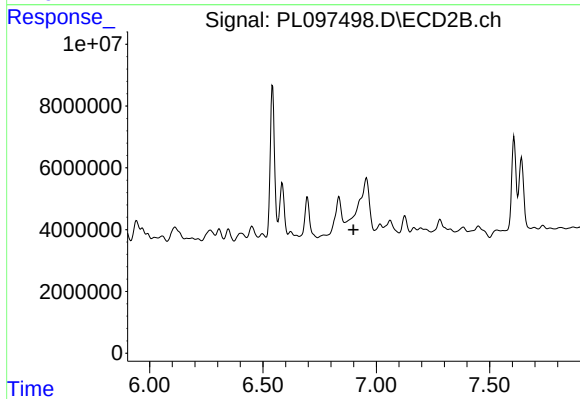

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.900 min
Response: 0
Conc: N.D.

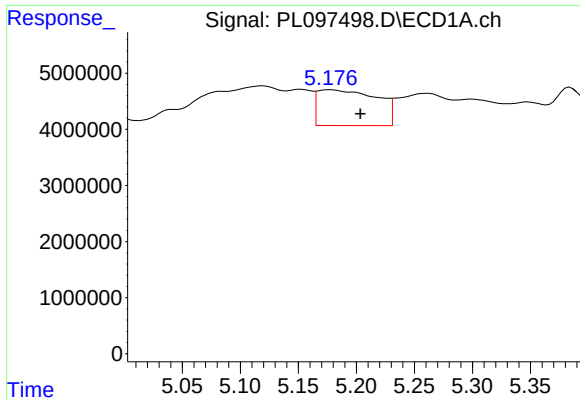

#24 Chlordane-2


R.T.: 5.177 min
Delta R.T.: -0.026 min
Response: 22759153
Conc: 102.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-25-0280

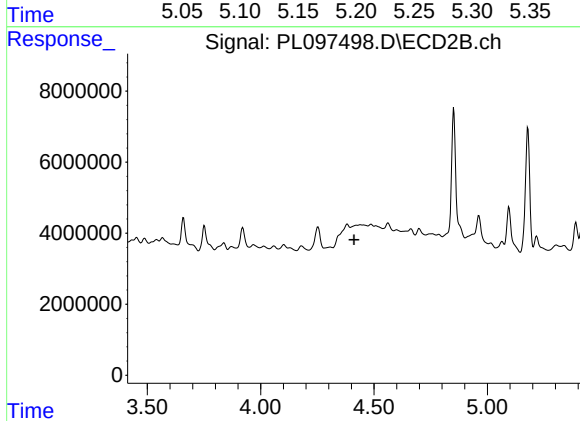


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.412 min
Response: 0
Conc: N.D.

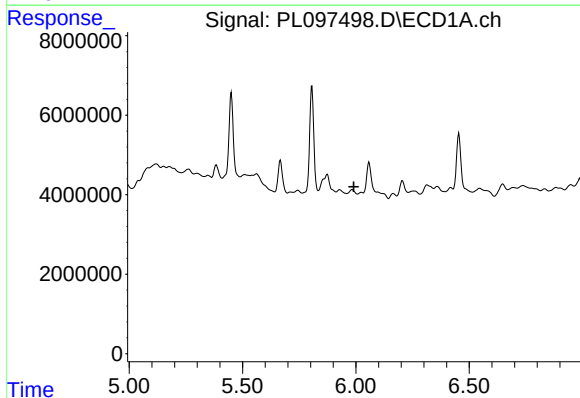


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.991 min
Response: 0
Conc: N.D.

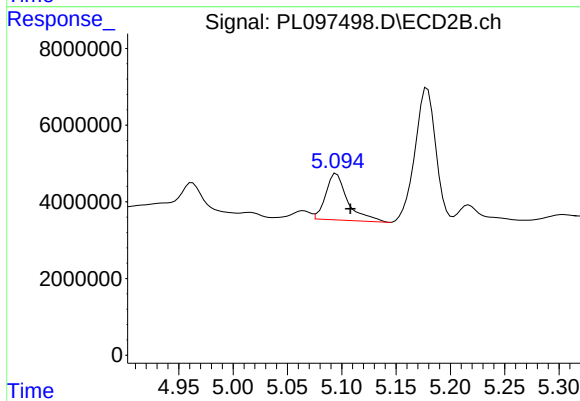

#26 Chlordane-4


R.T.: 5.095 min
Delta R.T.: -0.013 min
Response: 17114702
Conc: 22.47 ng/ml

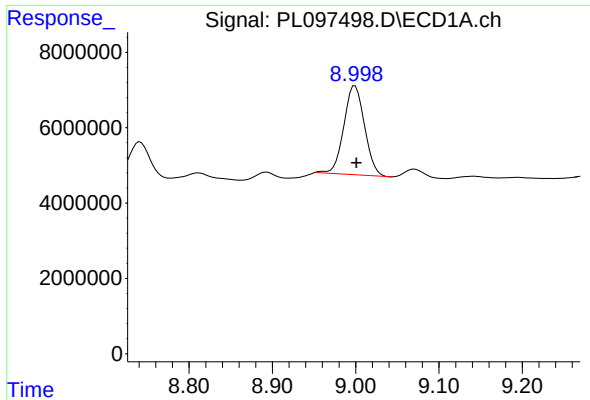

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.002 min
Response: 40740136
Conc: 12.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-25-0280

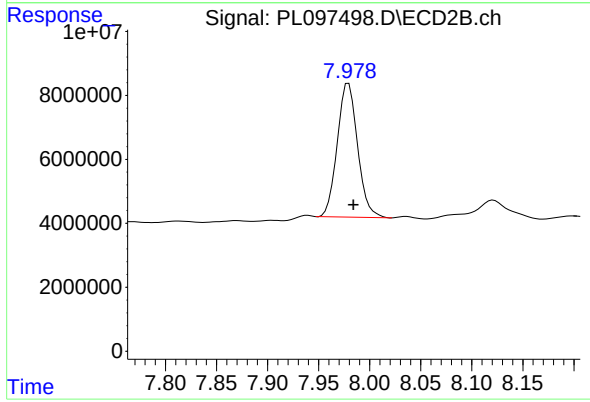

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.005 min
Response: 57955471
Conc: 10.18 ng/ml