

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100318\
 Data File : PL040597.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2018 14:30
 Operator : AJ\SJ
 Sample : J5198-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 02:17:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.805	119.8E6	39041884	16.372	12.364
28)	SA Decachlor...	7.810	8.730	134.6E6	44911365	14.162	14.182
Target Compounds							
4)	MA Heptachlor	4.107f	0.000	44318026	0	3.766	N.D. #
6)	B beta-BHC	4.107f	4.633	44318026	-2664940	10.500	N.D. #
10)	B gamma-Chl...	5.063	5.830	30871052	9885382	2.843	2.502
11)	B alpha-Chl...	5.063f	0.000	30871052	0	2.947	N.D. #
12)	B 4,4'-DDE	5.278	6.084	110.1E6	24925878	9.957	6.191 #
16)	A 4,4'-DDD	5.784	6.561	32942825	14133688	3.568	4.449
17)	MA 4,4'-DDT	6.013	0.000	21923871	0	2.711	N.D. #
23)	Chlordane-1	0.000	4.770	0	4324958	N.D.	28.025 #
25)	Chlordane-3	5.063	5.830	30871052	9885382	24.033	17.725 #
26)	Chlordane-4	5.063	0.000	30871052	0	26.054	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100318\
Data File : PL040597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2018 14:30
Operator : AJ\SJ
Sample : J5198-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 02:17:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

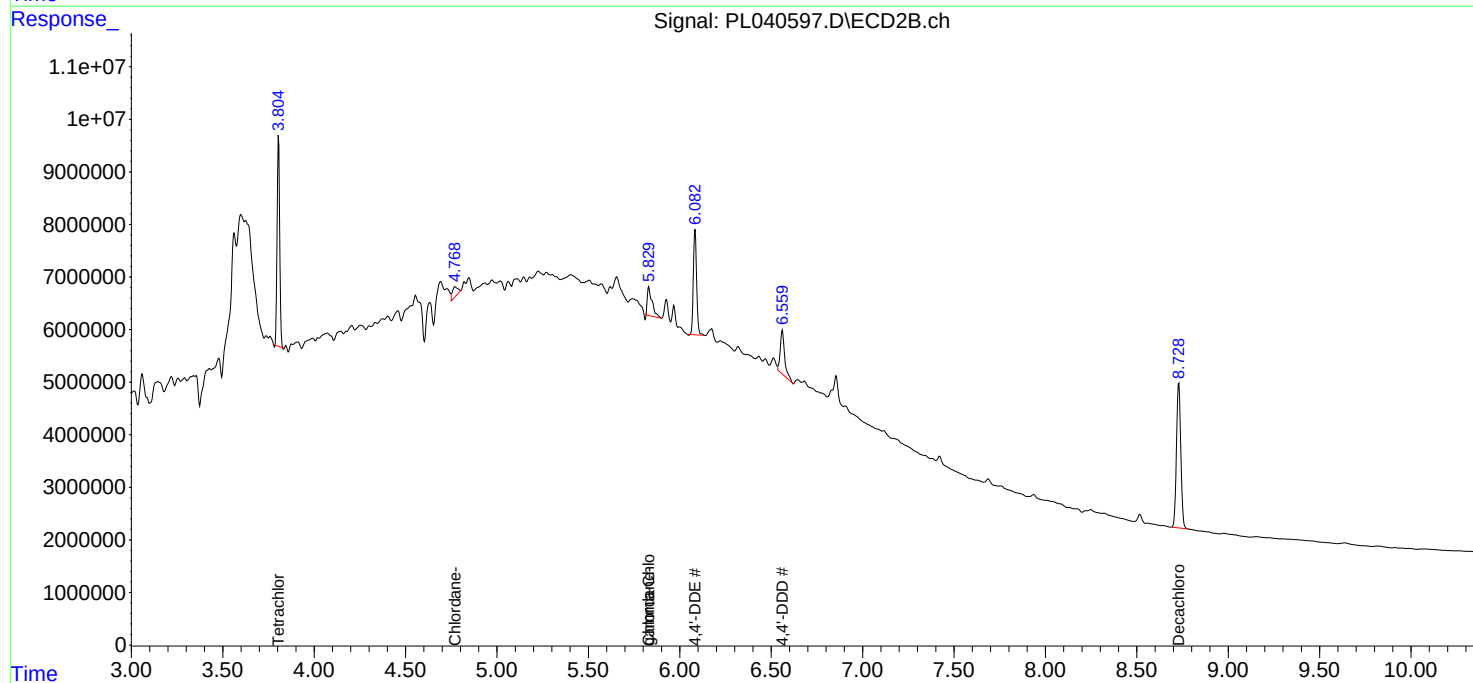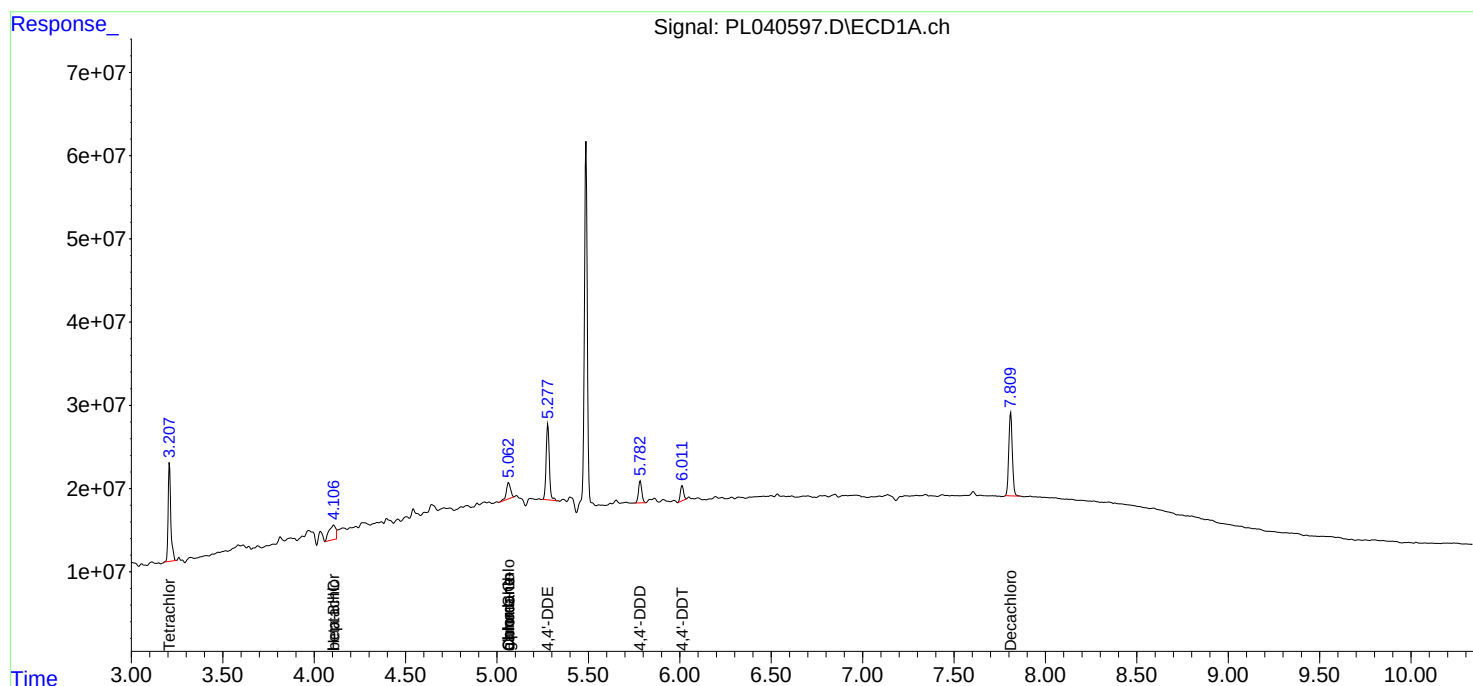


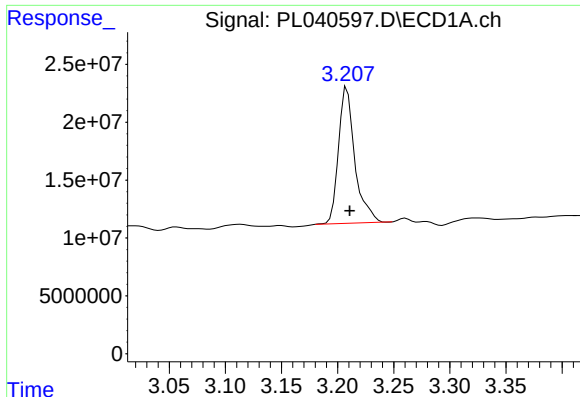

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 119846774
Conc: 16.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

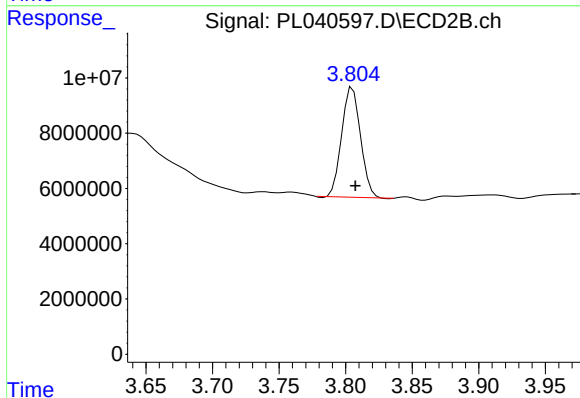


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: -0.002 min
Response: 39041884
Conc: 12.36 ng/ml

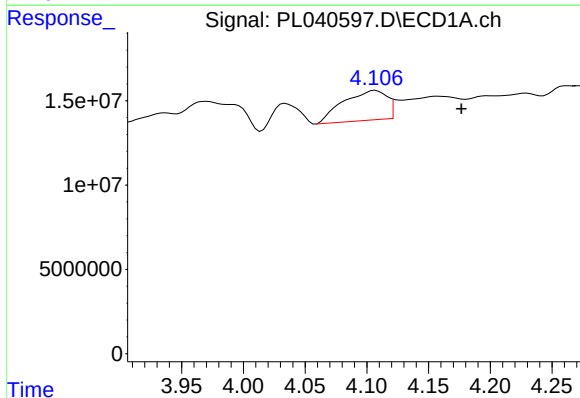


#4 Heptachlor

R.T.: 4.107 min
Delta R.T.: -0.070 min
Response: 44318026
Conc: 3.77 ng/ml

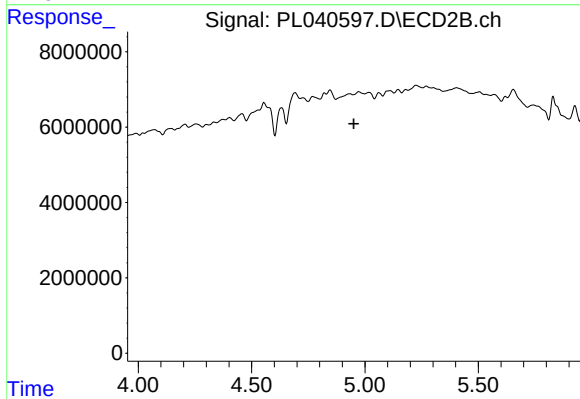

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.951 min
Response: 0
Conc: N.D.

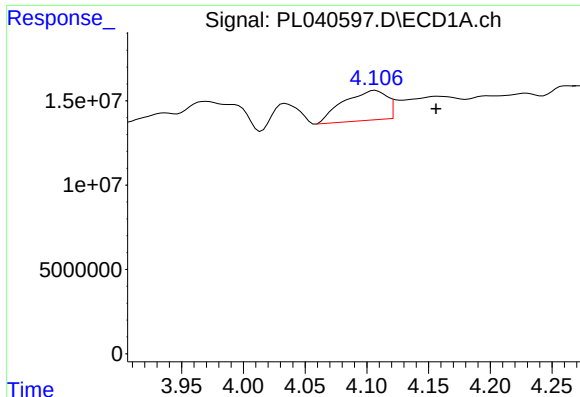

#6 beta-BHC


R.T.: 4.107 min
Delta R.T.: -0.049 min
Response: 44318026
Conc: 10.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

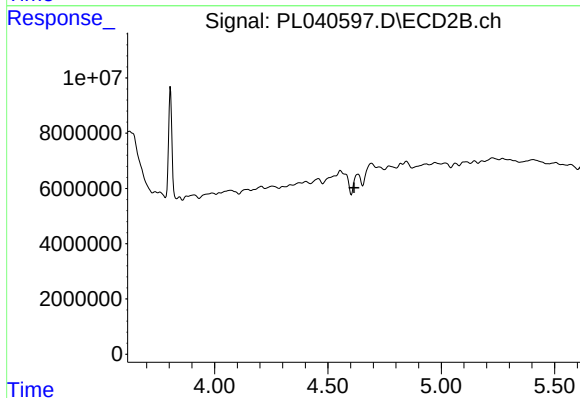


#6 beta-BHC

R.T.: 4.633 min
Delta R.T.: 0.018 min
Response: -2664940
Conc: N.D.

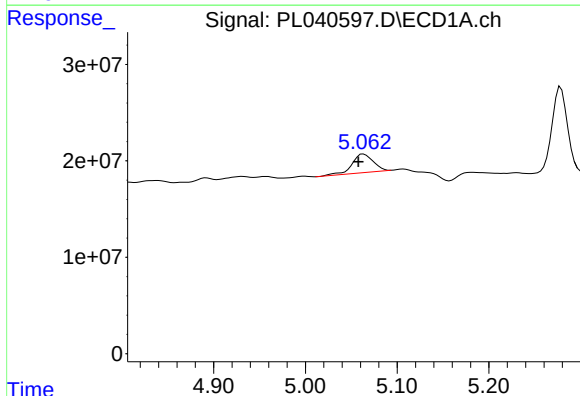


#10 gamma-Chlordane

R.T.: 5.063 min
Delta R.T.: 0.005 min
Response: 30871052
Conc: 2.84 ng/ml

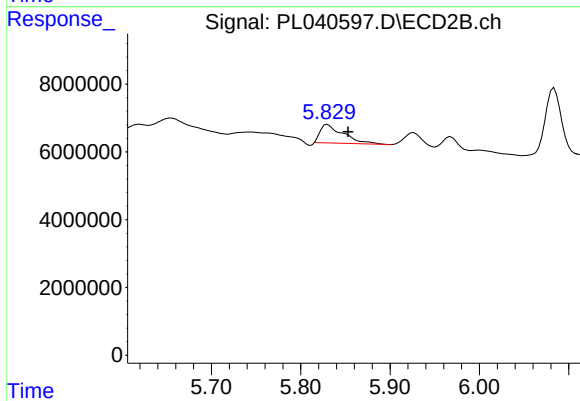

#10 gamma-Chlordane


R.T.: 5.830 min
Delta R.T.: -0.023 min
Response: 9885382
Conc: 2.50 ng/ml

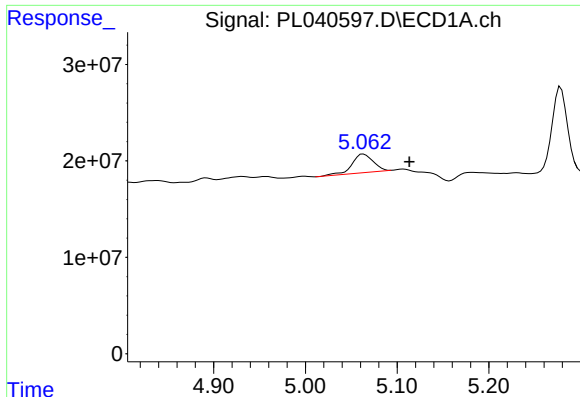

#11 alpha-Chlordane


R.T.: 5.063 min
Delta R.T.: -0.050 min
Response: 30871052
Conc: 2.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

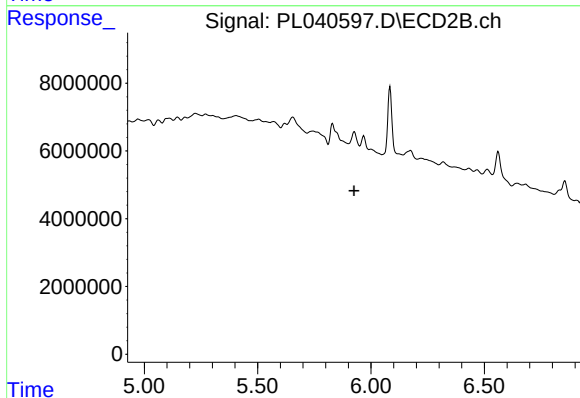


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

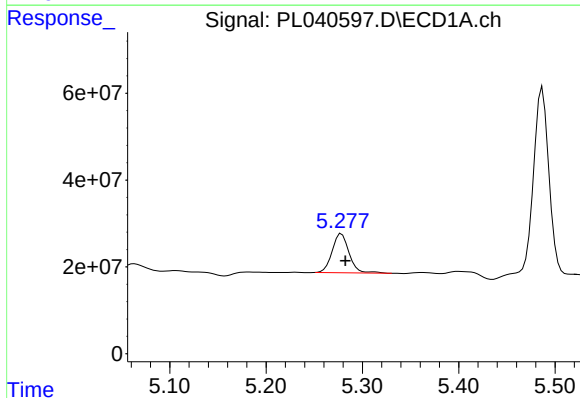


#12 4,4'-DDE

R.T.: 5.278 min
Delta R.T.: -0.004 min
Response: 110059447
Conc: 9.96 ng/ml

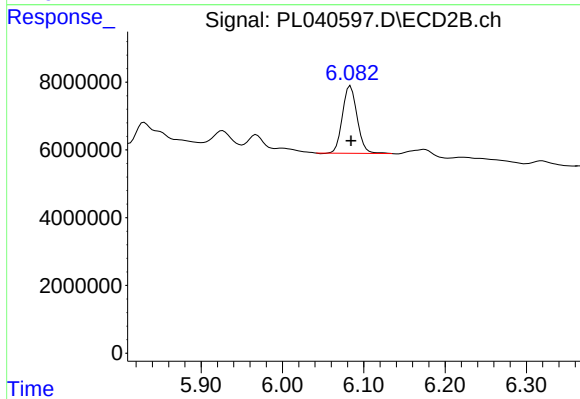

#12 4,4'-DDE


R.T.: 6.084 min
Delta R.T.: 0.000 min
Response: 24925878
Conc: 6.19 ng/ml

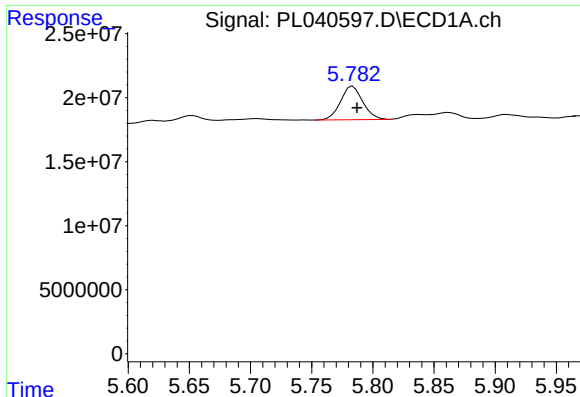

#16 4,4'-DDD


R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 32942825
Conc: 3.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

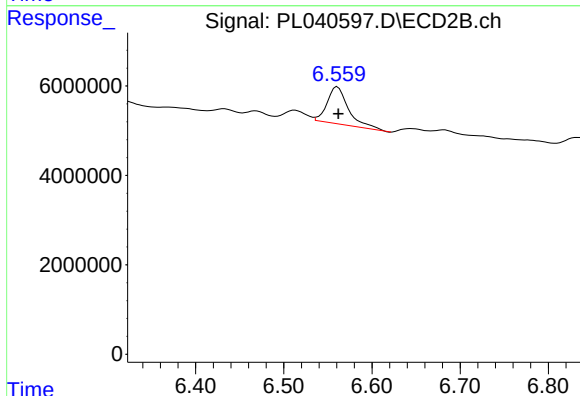


#16 4,4'-DDD

R.T.: 6.561 min
Delta R.T.: -0.001 min
Response: 14133688
Conc: 4.45 ng/ml

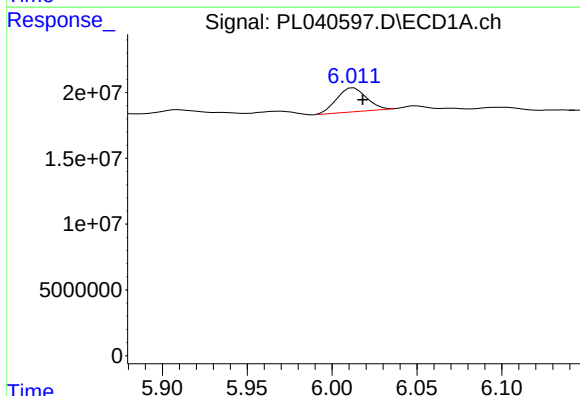


#17 4,4'-DDT

R.T.: 6.013 min
Delta R.T.: -0.005 min
Response: 21923871
Conc: 2.71 ng/ml

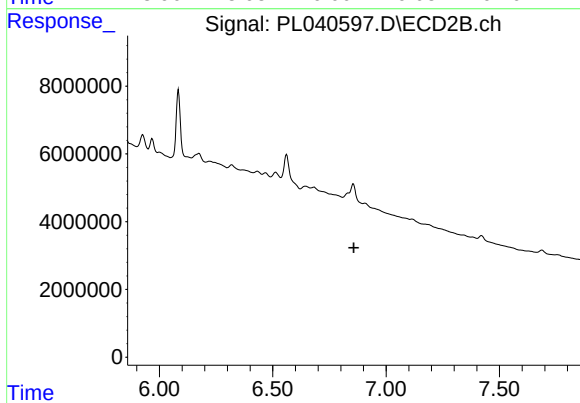

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.858 min
Response: 0
Conc: N.D.

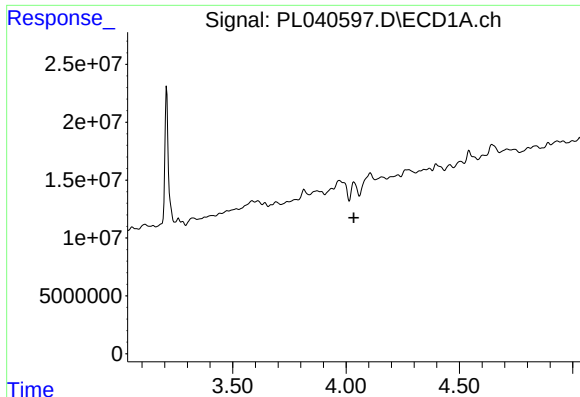

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

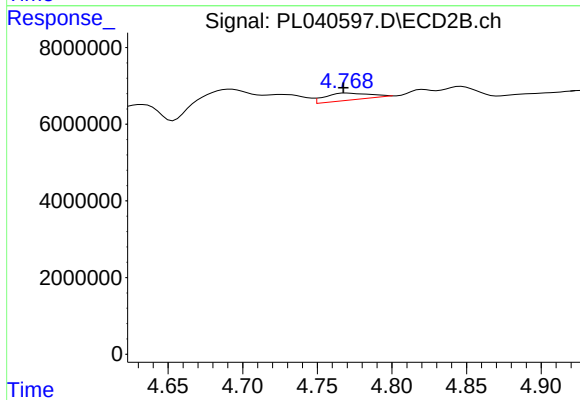


#23 Chlordane-1

R.T.: 4.770 min
Delta R.T.: 0.002 min
Response: 4324958
Conc: 28.02 ng/ml

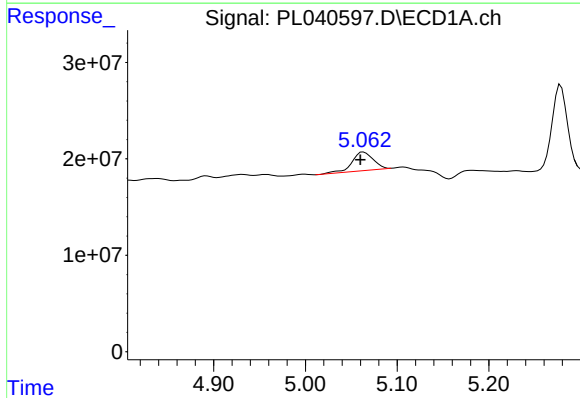


#25 Chlordane-3

R.T.: 5.063 min
Delta R.T.: 0.003 min
Response: 30871052
Conc: 24.03 ng/ml

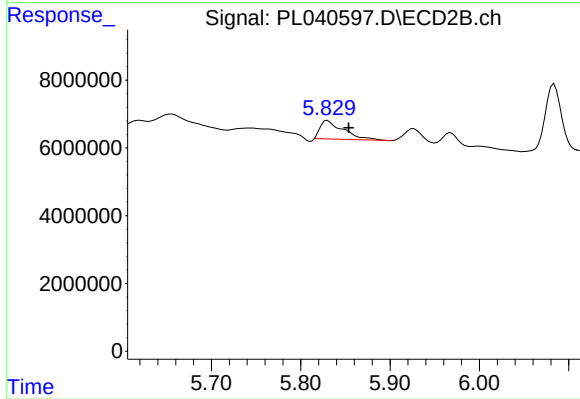

#25 Chlordane-3


R.T.: 5.830 min
Delta R.T.: -0.024 min
Response: 9885382
Conc: 17.72 ng/ml

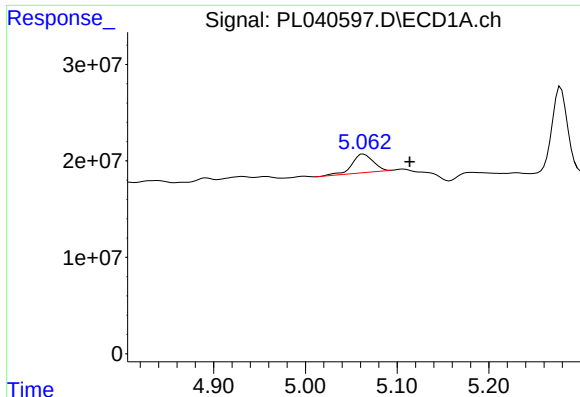

#26 Chlordane-4


R.T.: 5.063 min
Delta R.T.: -0.051 min
Response: 30871052
Conc: 26.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

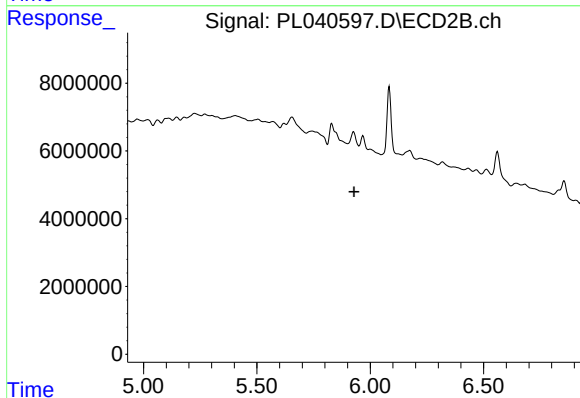


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.928 min
Response: 0
Conc: N.D.

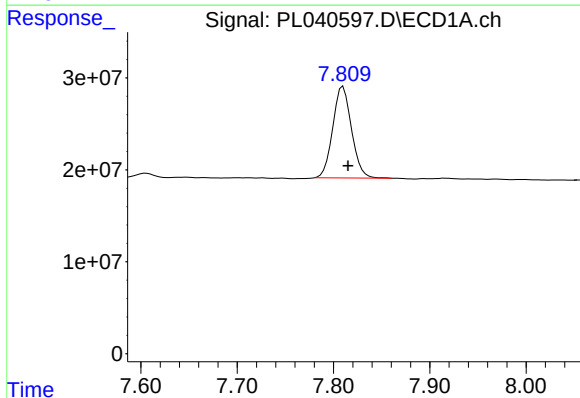

#28 Decachlorobiphenyl

R.T.: 7.810 min
Delta R.T.: -0.005 min
Response: 134619564
Conc: 14.16 ng/ml

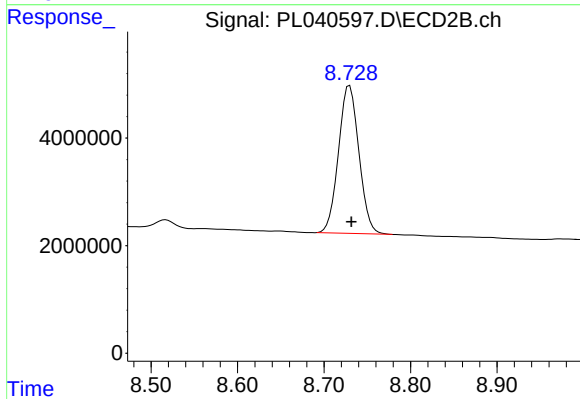

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.002 min
Response: 44911365
Conc: 14.18 ng/ml