

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100318\
 Data File : PL040598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2018 14:45
 Operator : AJ\SJ
 Sample : J5194-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 02:18:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.805	97399853	30209992	13.306	9.567 #
28)	SA Decachlor...	7.810	8.730	93218186	32402133	9.806	10.232
Target Compounds							
9)	A Endosulfan I	0.000	5.926f	0	11771164	N.D.	3.164 #
10)	B gamma-Chl...	5.056	5.850	3089578	11149651	0.284	2.821 #
11)	B alpha-Chl...	5.056f	5.926	3089578	11771164	0.295	2.999 #
12)	B 4,4'-DDE	5.279	6.083	47175745	16180687	4.268	4.019
16)	A 4,4'-DDD	5.783	6.562	40221822	13679257	4.357	4.306
17)	MA 4,4'-DDT	6.012	0.000	31850165	0	3.939	N.D. #
25)	Chlordane-3	5.056	5.850	3089578	11149651	2.405	19.992 #
26)	Chlordane-4	5.056	5.926	3089578	11771164	2.607	17.836 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100318\
Data File : PL040598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2018 14:45
Operator : AJ\SJ
Sample : J5194-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 02:18:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

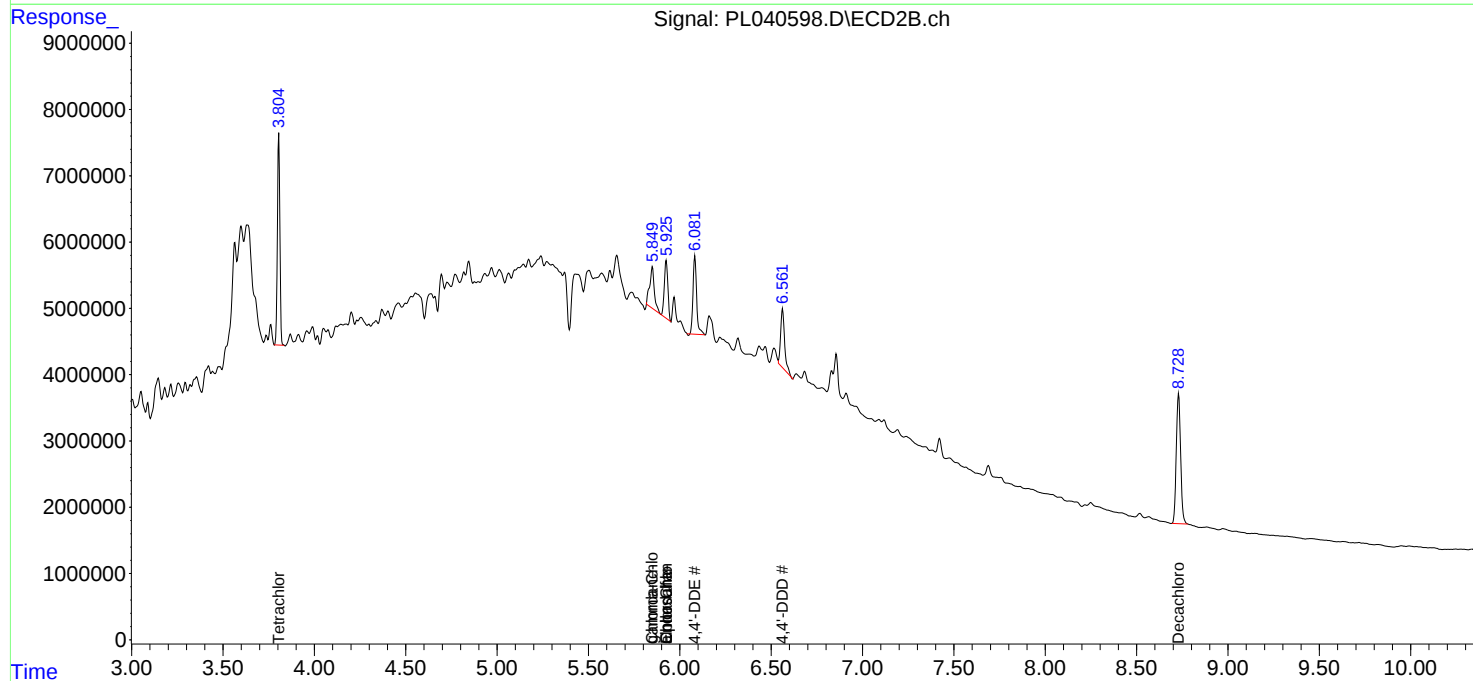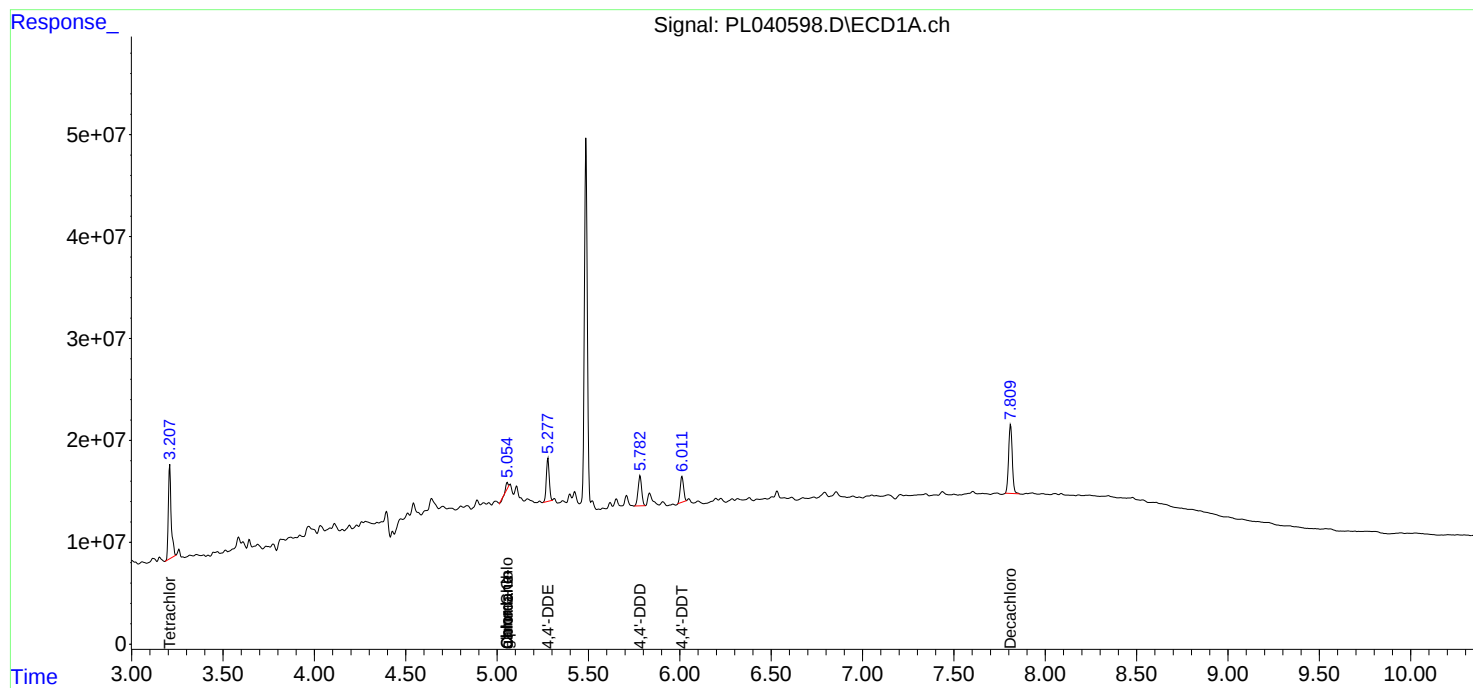


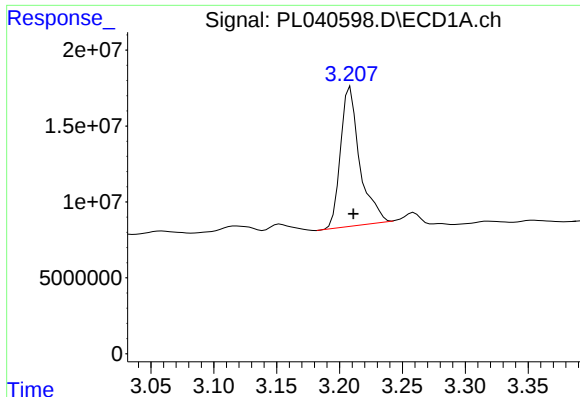

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 97399853
Conc: 13.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

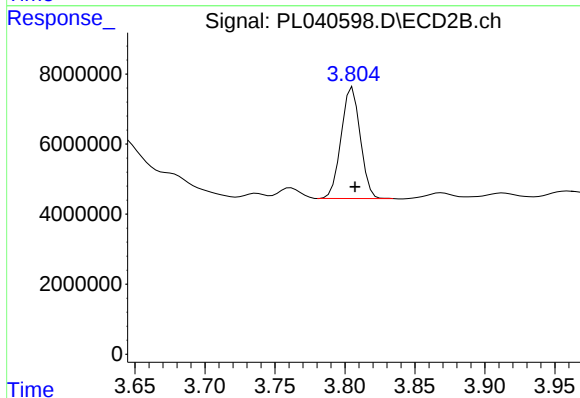


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: -0.002 min
Response: 30209992
Conc: 9.57 ng/ml

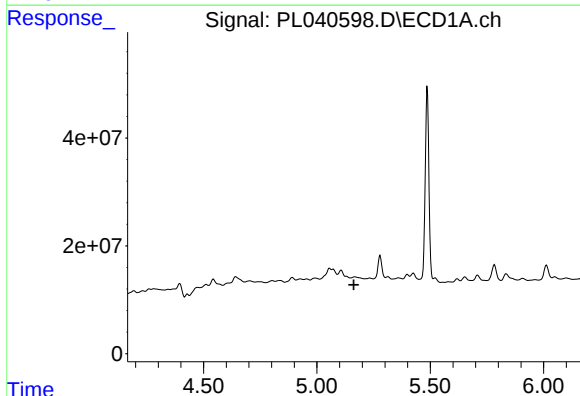


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.163 min
Response: 0
Conc: N.D.

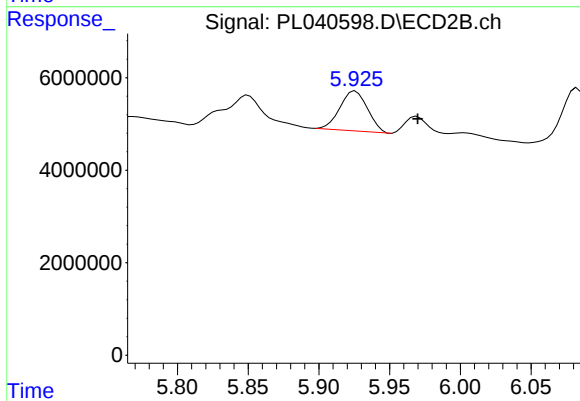

#9 Endosulfan I


R.T.: 5.926 min
Delta R.T.: -0.044 min
Response: 11771164
Conc: 3.16 ng/ml

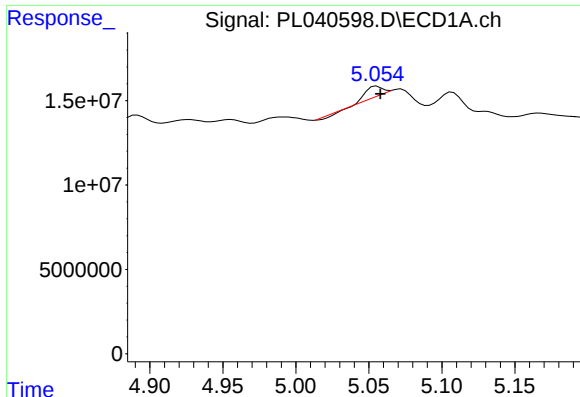

#10 gamma-Chlordane


R.T.: 5.056 min
Delta R.T.: -0.002 min
Response: 3089578
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

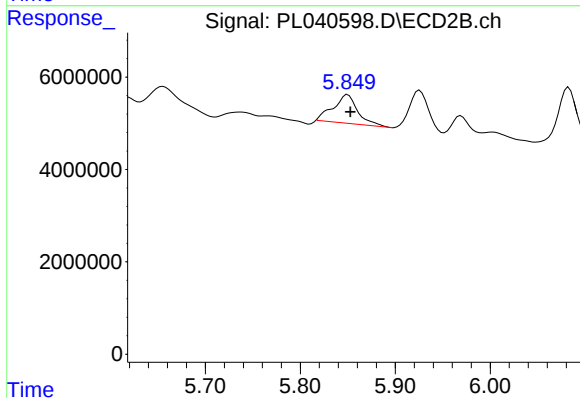


#10 gamma-Chlordane

R.T.: 5.850 min
Delta R.T.: -0.003 min
Response: 11149651
Conc: 2.82 ng/ml

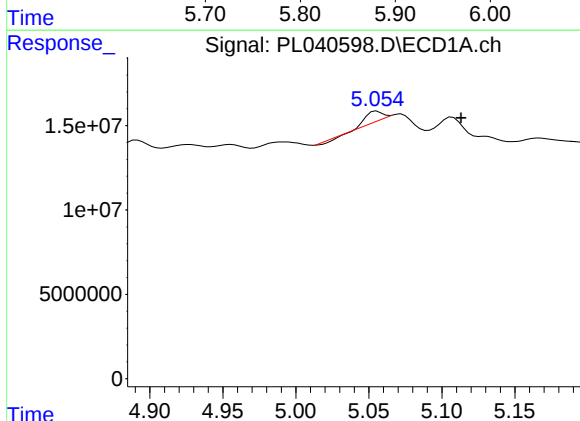


#11 alpha-Chlordane

R.T.: 5.056 min
Delta R.T.: -0.058 min
Response: 3089578
Conc: 0.29 ng/ml

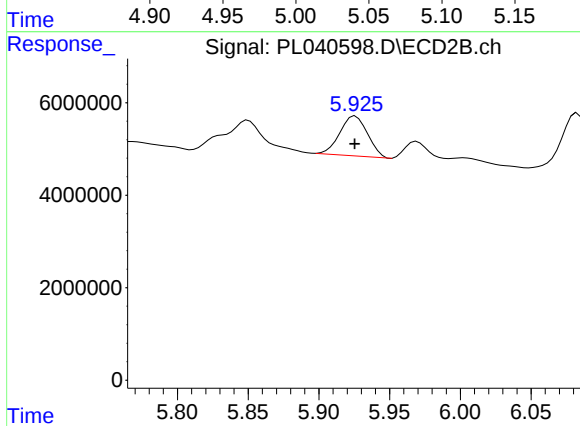

#11 alpha-Chlordane


R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 11771164
Conc: 3.00 ng/ml

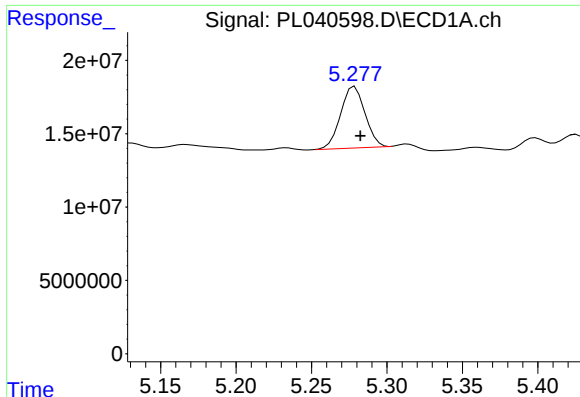

#12 4,4'-DDE


R.T.: 5.279 min
Delta R.T.: -0.004 min
Response: 47175745
Conc: 4.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

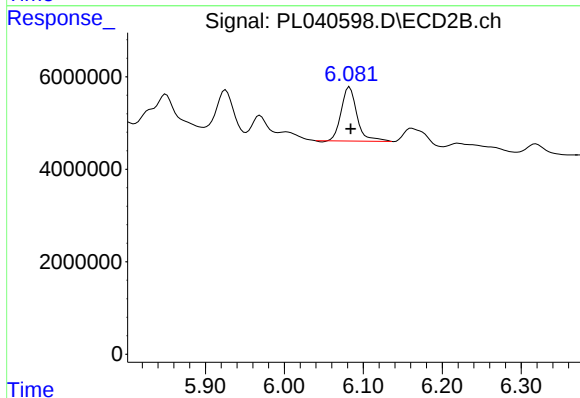


#12 4,4'-DDE

R.T.: 6.083 min
Delta R.T.: -0.002 min
Response: 16180687
Conc: 4.02 ng/ml

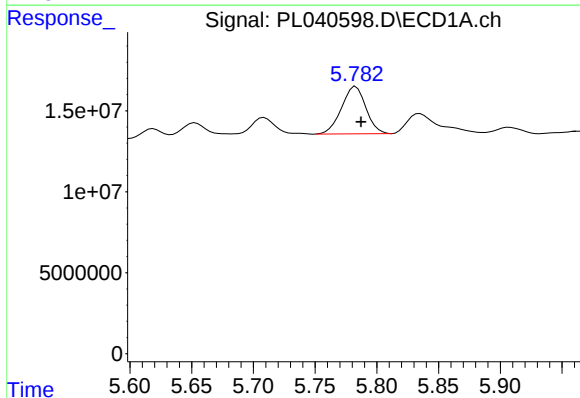


#16 4,4'-DDD

R.T.: 5.783 min
Delta R.T.: -0.004 min
Response: 40221822
Conc: 4.36 ng/ml

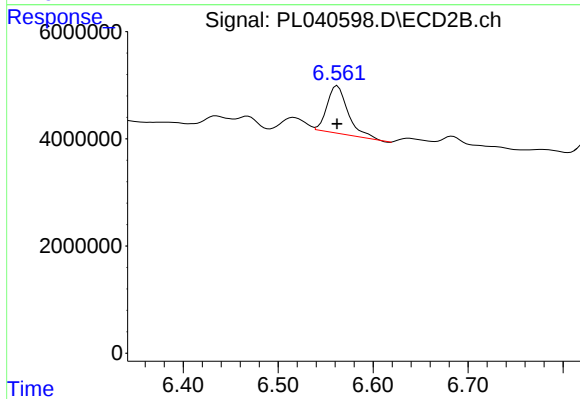

#16 4,4'-DDD


R.T.: 6.562 min
Delta R.T.: 0.000 min
Response: 13679257
Conc: 4.31 ng/ml

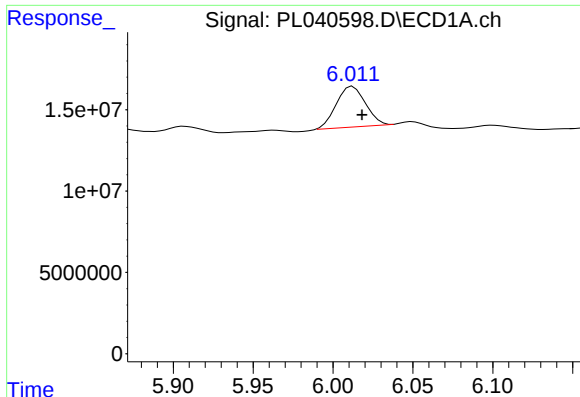

#17 4,4'-DDT


R.T.: 6.012 min
Delta R.T.: -0.006 min
Response: 31850165
Conc: 3.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

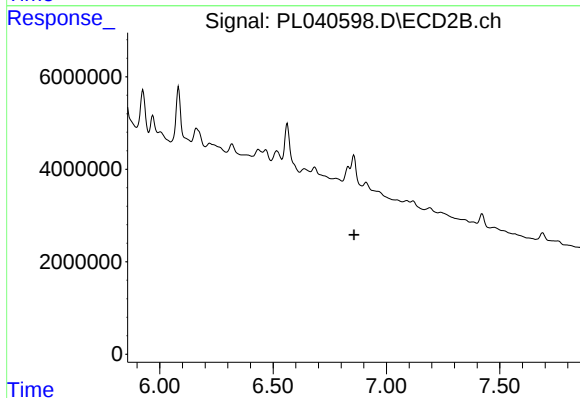


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.858 min
Response: 0
Conc: N.D.

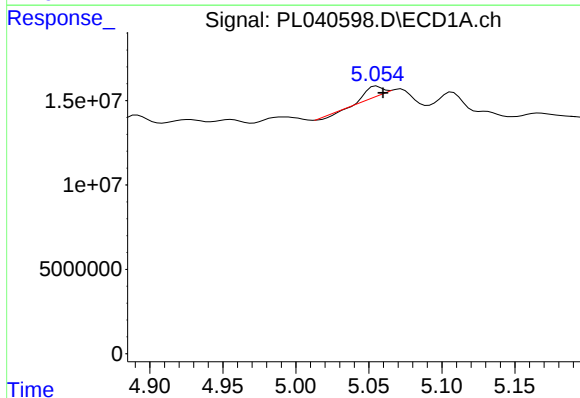


#25 Chlordane-3

R.T.: 5.056 min
Delta R.T.: -0.004 min
Response: 3089578
Conc: 2.41 ng/ml

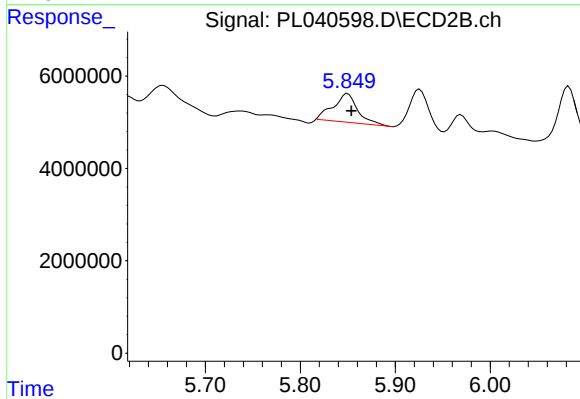

#25 Chlordane-3


R.T.: 5.850 min
Delta R.T.: -0.004 min
Response: 11149651
Conc: 19.99 ng/ml

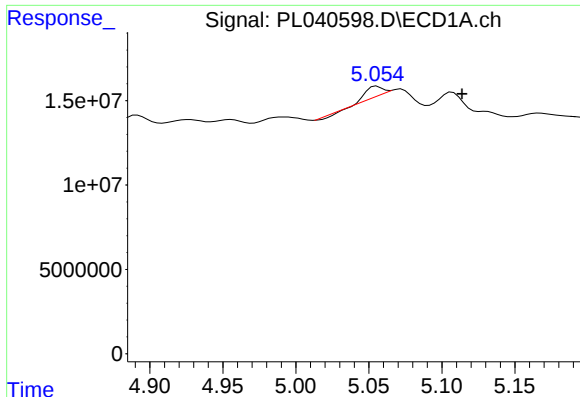

#26 Chlordane-4


R.T.: 5.056 min
Delta R.T.: -0.058 min
Response: 3089578
Conc: 2.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

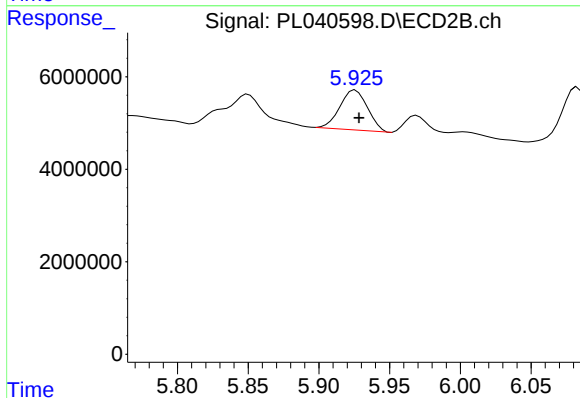


#26 Chlordane-4

R.T.: 5.926 min
Delta R.T.: -0.003 min
Response: 11771164
Conc: 17.84 ng/ml

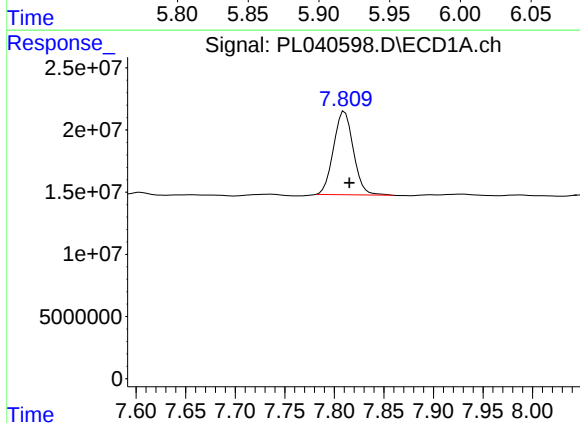

#28 Decachlorobiphenyl

R.T.: 7.810 min
Delta R.T.: -0.005 min
Response: 93218186
Conc: 9.81 ng/ml

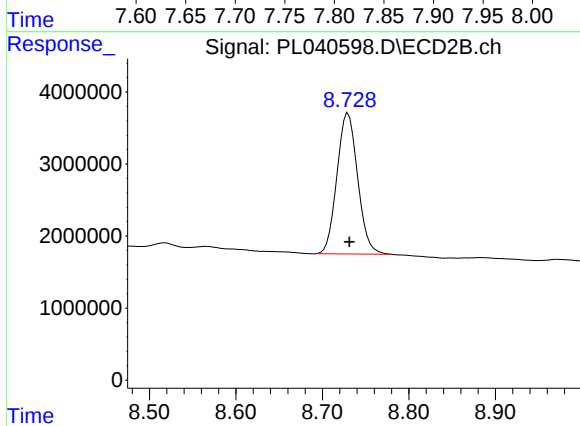

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.002 min
Response: 32402133
Conc: 10.23 ng/ml