

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100318\
 Data File : PL040600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2018 15:13
 Operator : AJ\SJ
 Sample : J5198-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 02:18:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.805	131.9E6	37792132	18.021	11.968 #
28)	SA Decachlor...	7.811	8.730	85360860	28316657	8.980	8.942
Target Compounds							
7)	B delta-BHC	0.000	4.846	0	7093720	N.D.	1.537 #
9)	A Endosulfan I	0.000	5.927f	0	6650891	N.D.	1.788 #
11)	B alpha-Chl...	0.000	5.927	0	6650891	N.D.	1.695 #
12)	B 4,4'-DDE	5.280	6.083	361.7E6	117.6E6	32.725	29.202
14)	MA Endrin	5.654	0.000	20223735	0	2.036	N.D. #
16)	A 4,4'-DDD	5.784	6.563	35890475	11091628	3.888	3.491
17)	MA 4,4'-DDT	6.015	6.857	190.3E6	63223336	23.535	20.748
24)	Chlordane-2	4.543	0.000	24005680	0	63.999	N.D. #
26)	Chlordane-4	0.000	5.927	0	6650891	N.D.	10.078 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100318\
Data File : PL040600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2018 15:13
Operator : AJ\SJ
Sample : J5198-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 02:18:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

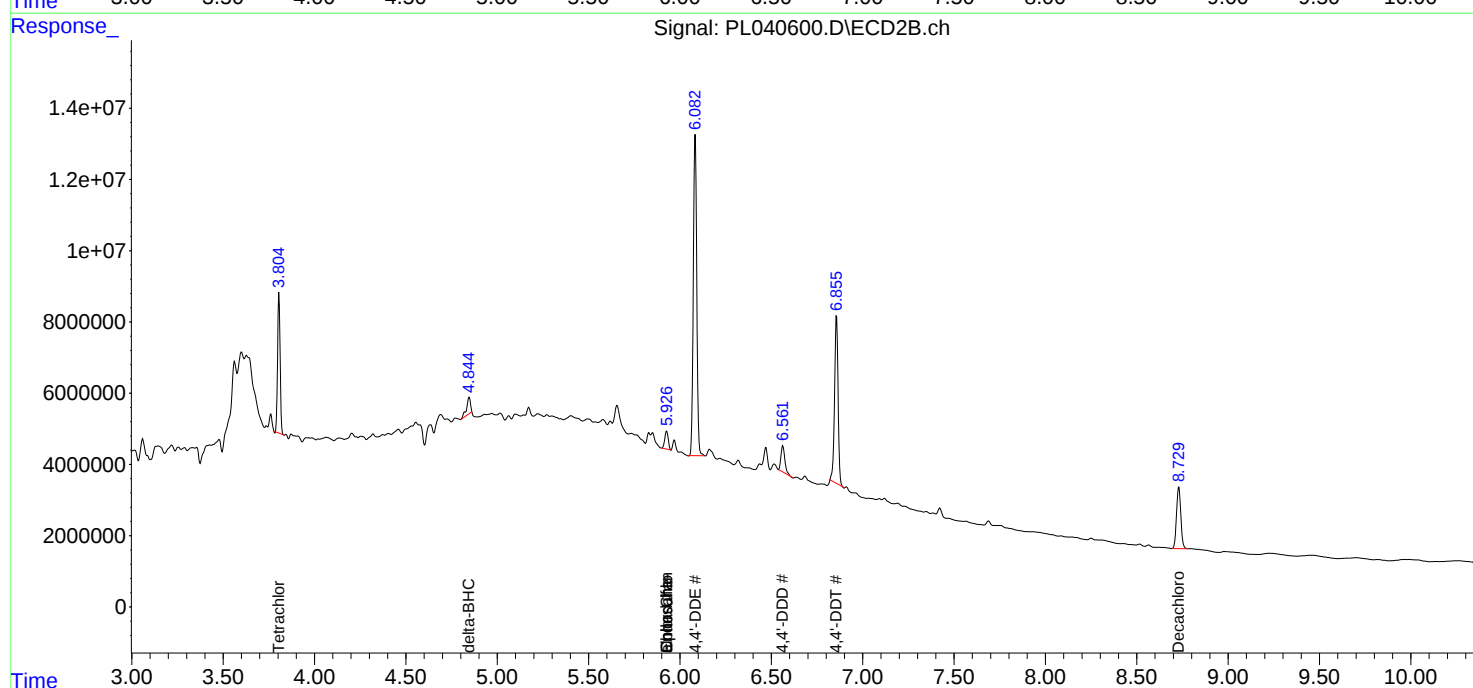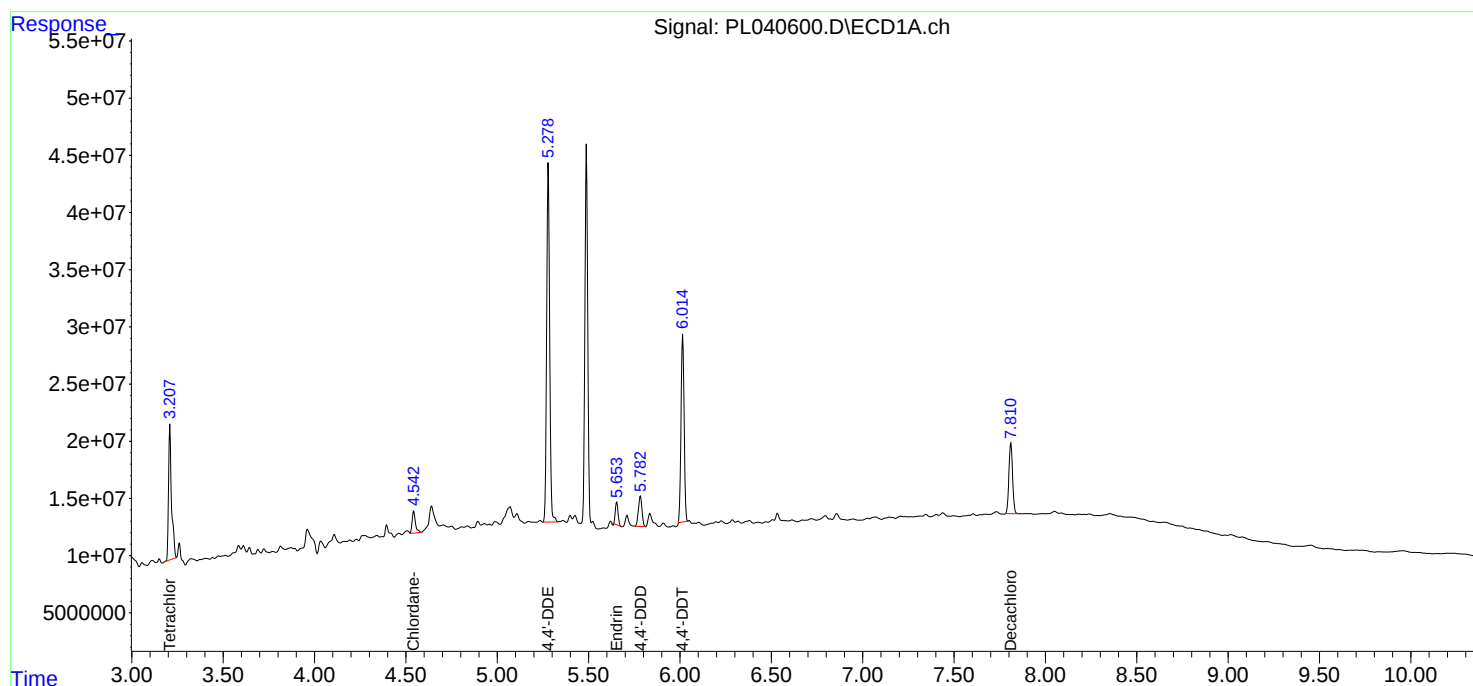


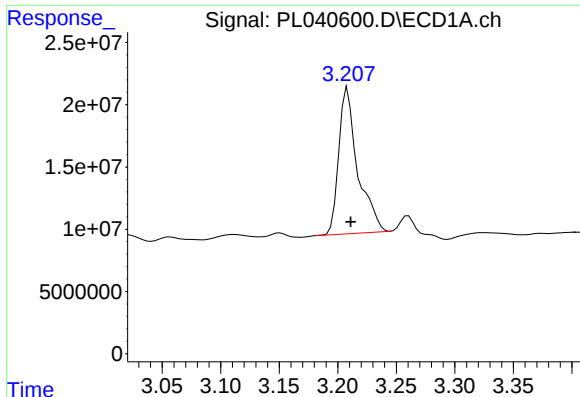

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 131917759
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

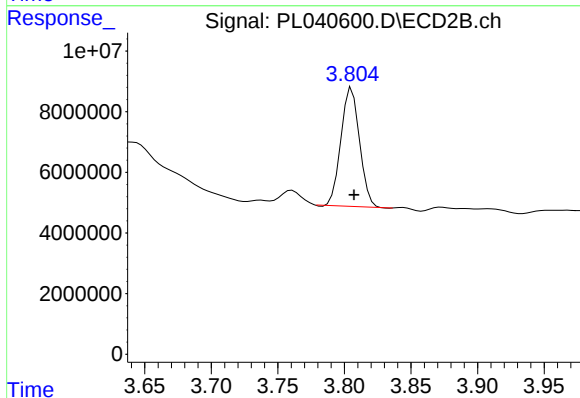


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: -0.002 min
Response: 37792132
Conc: 11.97 ng/ml

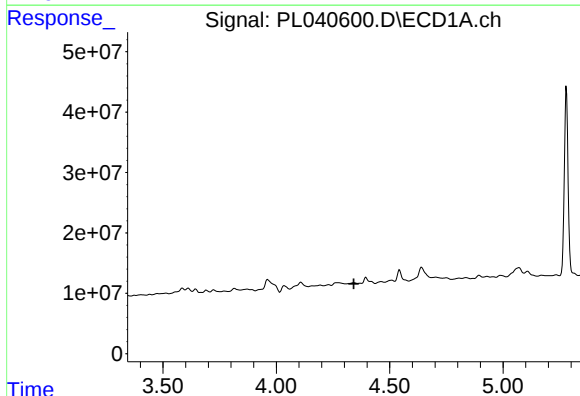


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

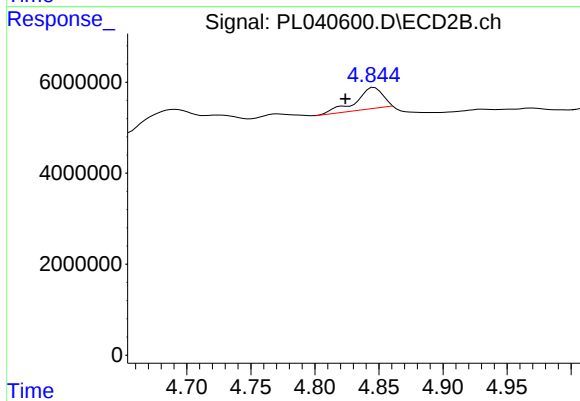

#7 delta-BHC


R.T.: 4.846 min
Delta R.T.: 0.023 min
Response: 7093720
Conc: 1.54 ng/ml

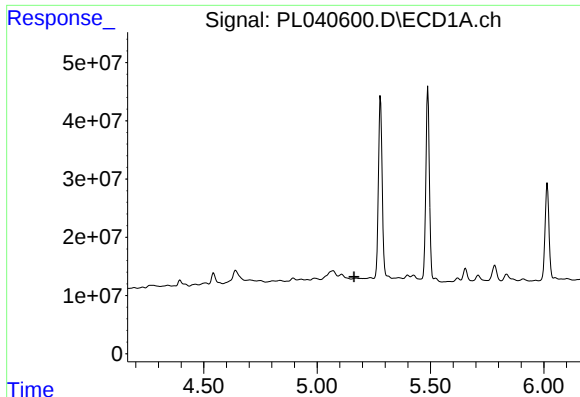

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

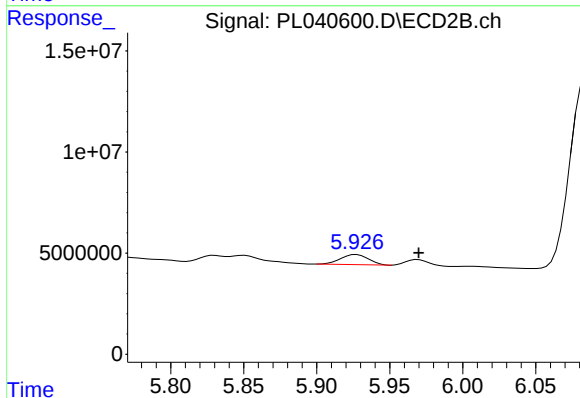


#9 Endosulfan I

R.T.: 5.927 min
Delta R.T.: -0.043 min
Response: 6650891
Conc: 1.79 ng/ml

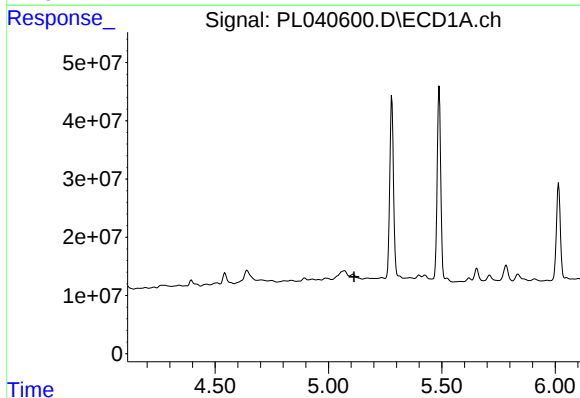


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.113 min
Response: 0
Conc: N.D.

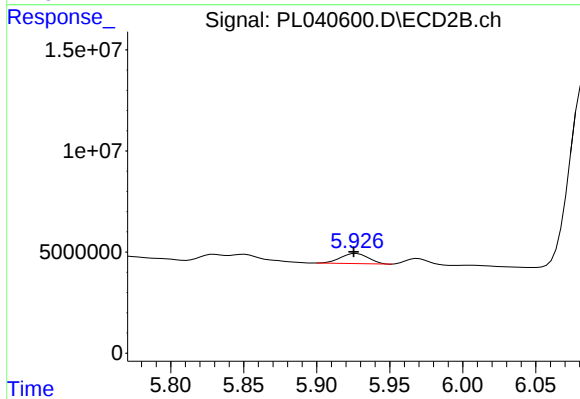

#11 alpha-Chlordane


R.T.: 5.927 min
Delta R.T.: 0.002 min
Response: 6650891
Conc: 1.69 ng/ml

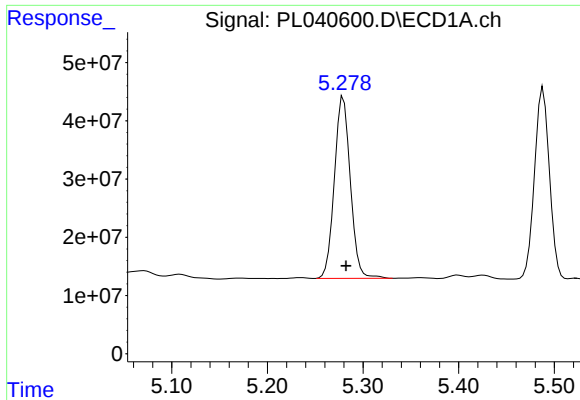

#12 4,4'-DDE


R.T.: 5.280 min
Delta R.T.: -0.003 min
Response: 361710693
Conc: 32.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

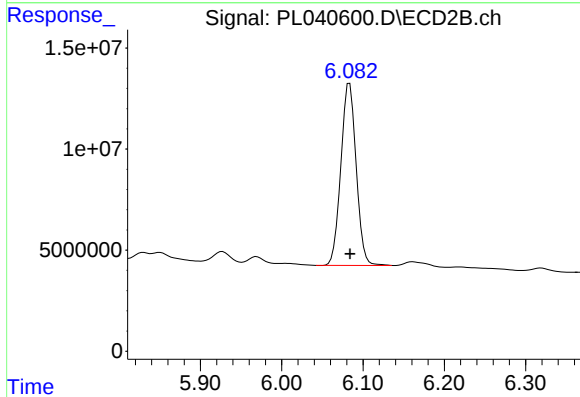


#12 4,4'-DDE

R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 117576690
Conc: 29.20 ng/ml

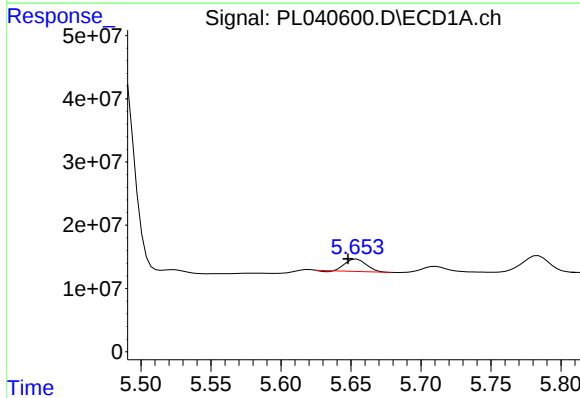


#14 Endrin

R.T.: 5.654 min
Delta R.T.: 0.006 min
Response: 20223735
Conc: 2.04 ng/ml

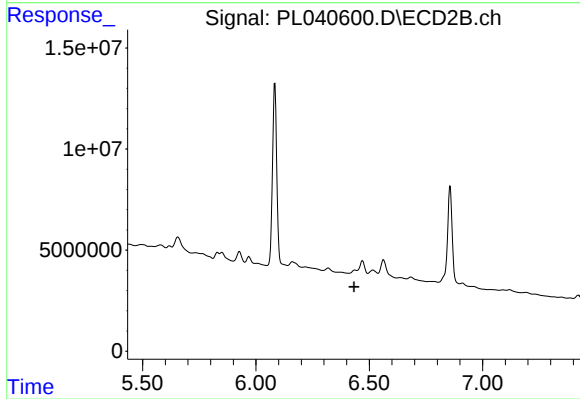

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

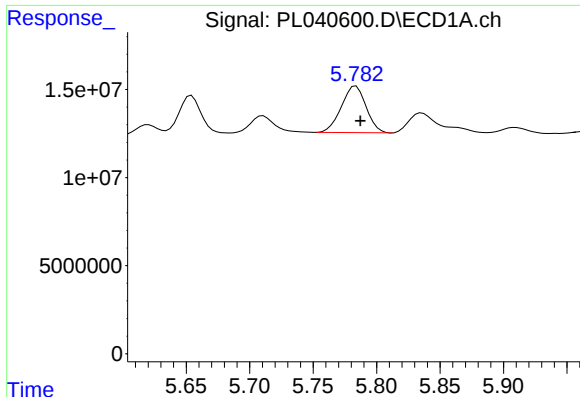

#16 4,4'-DDD


R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 35890475
Conc: 3.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

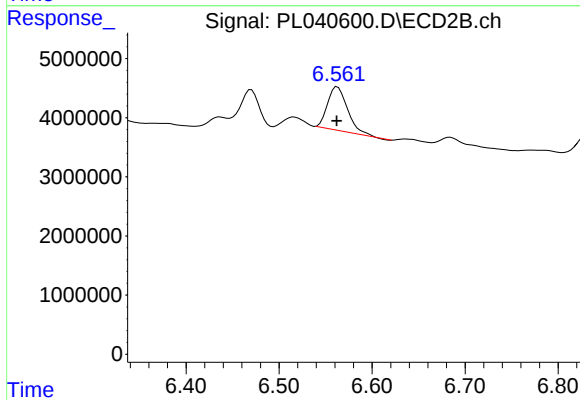


#16 4,4'-DDD

R.T.: 6.563 min
Delta R.T.: 0.000 min
Response: 11091628
Conc: 3.49 ng/ml

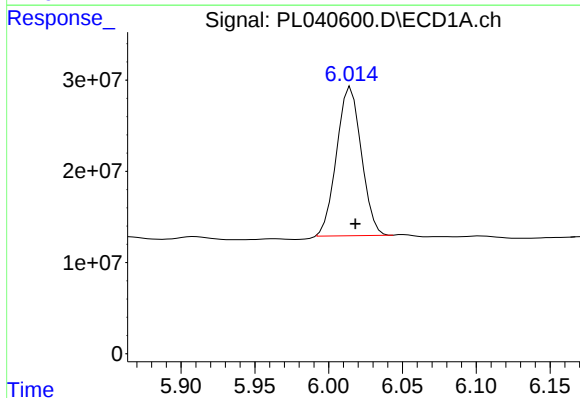


#17 4,4'-DDT

R.T.: 6.015 min
Delta R.T.: -0.003 min
Response: 190322569
Conc: 23.53 ng/ml

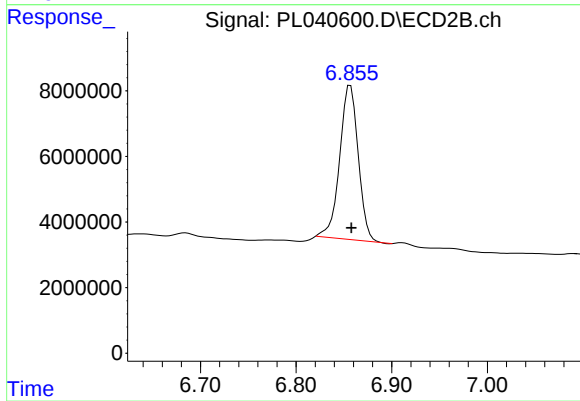

#17 4,4'-DDT


R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 63223336
Conc: 20.75 ng/ml

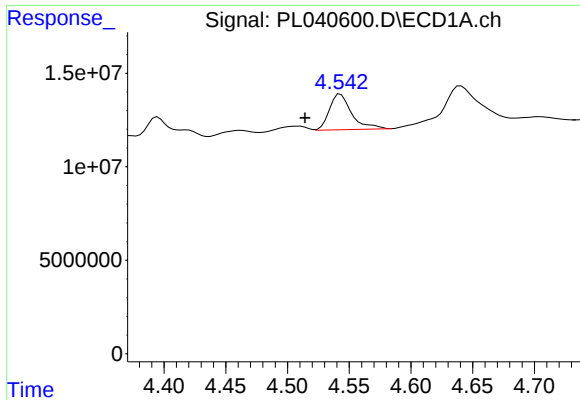

#24 Chlordane-2


R.T.: 4.543 min
Delta R.T.: 0.029 min
Response: 24005680
Conc: 64.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

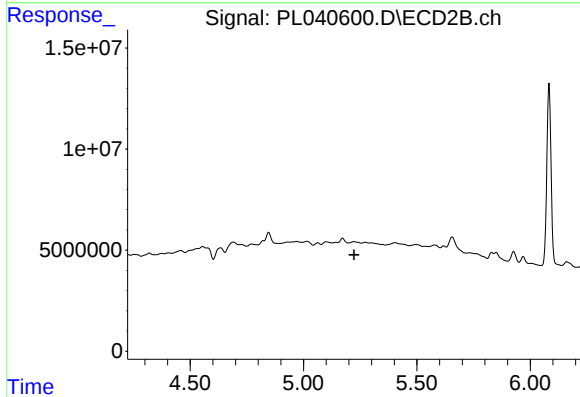


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.223 min
Response: 0
Conc: N.D.

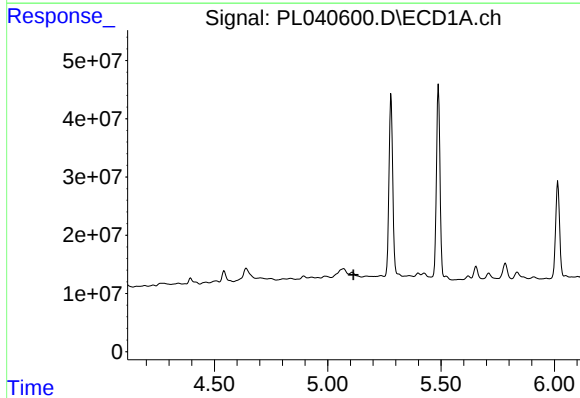


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

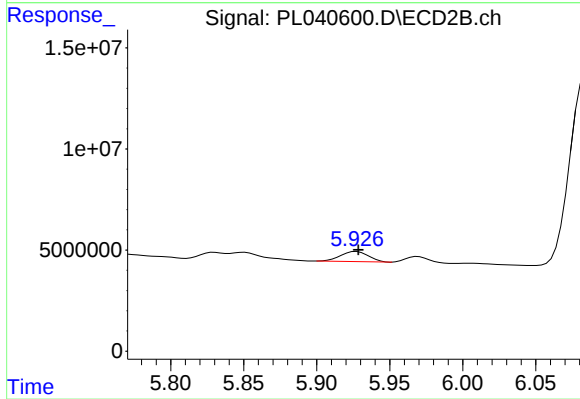

#26 Chlordane-4


R.T.: 5.927 min
Delta R.T.: -0.001 min
Response: 6650891
Conc: 10.08 ng/ml

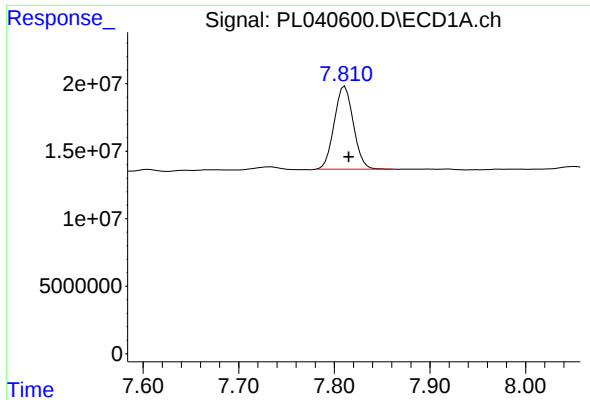

#28 Decachlorobiphenyl

R.T.: 7.811 min
Delta R.T.: -0.004 min
Response: 85360860
Conc: 8.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

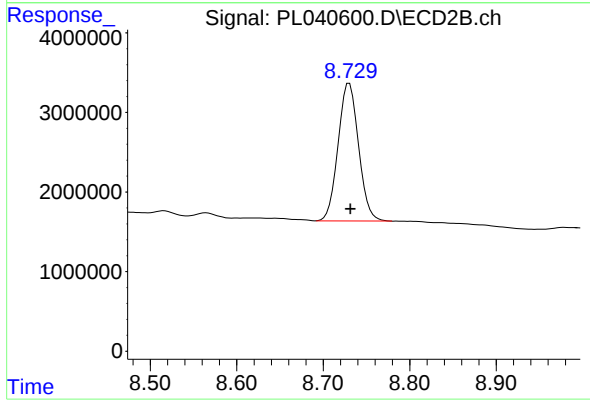

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.001 min
Response: 28316657
Conc: 8.94 ng/ml