

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100318\
 Data File : PL040601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2018 15:27
 Operator : AJ\SJ
 Sample : J5198-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 02:19:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.805	108.7E6	29820618	14.846	9.443 #
28)	SA Decachlor...	7.811	8.730	76918205	27601103	8.092	8.716
Target Compounds							
4)	MA Heptachlor	4.109f	0.000	29767264	0	2.530	N.D. #
6)	B beta-BHC	4.109f	4.634	29767264	-79937	7.052	N.D. #
10)	B gamma-Chl...	5.064	0.000	21986892	0	2.025	N.D. #
11)	B alpha-Chl...	5.064f	0.000	21986892	0	2.099	N.D. #
12)	B 4,4'-DDE	5.279	6.083	60859293	15386627	5.506	3.821 #
24)	Chlordane-2	4.543	0.000	19445878	0	51.843	N.D. #
25)	Chlordane-3	5.064	0.000	21986892	0	17.117	N.D. #
26)	Chlordane-4	5.064	0.000	21986892	0	18.556	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100318\
Data File : PL040601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2018 15:27
Operator : AJ\SJ
Sample : J5198-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 02:19:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

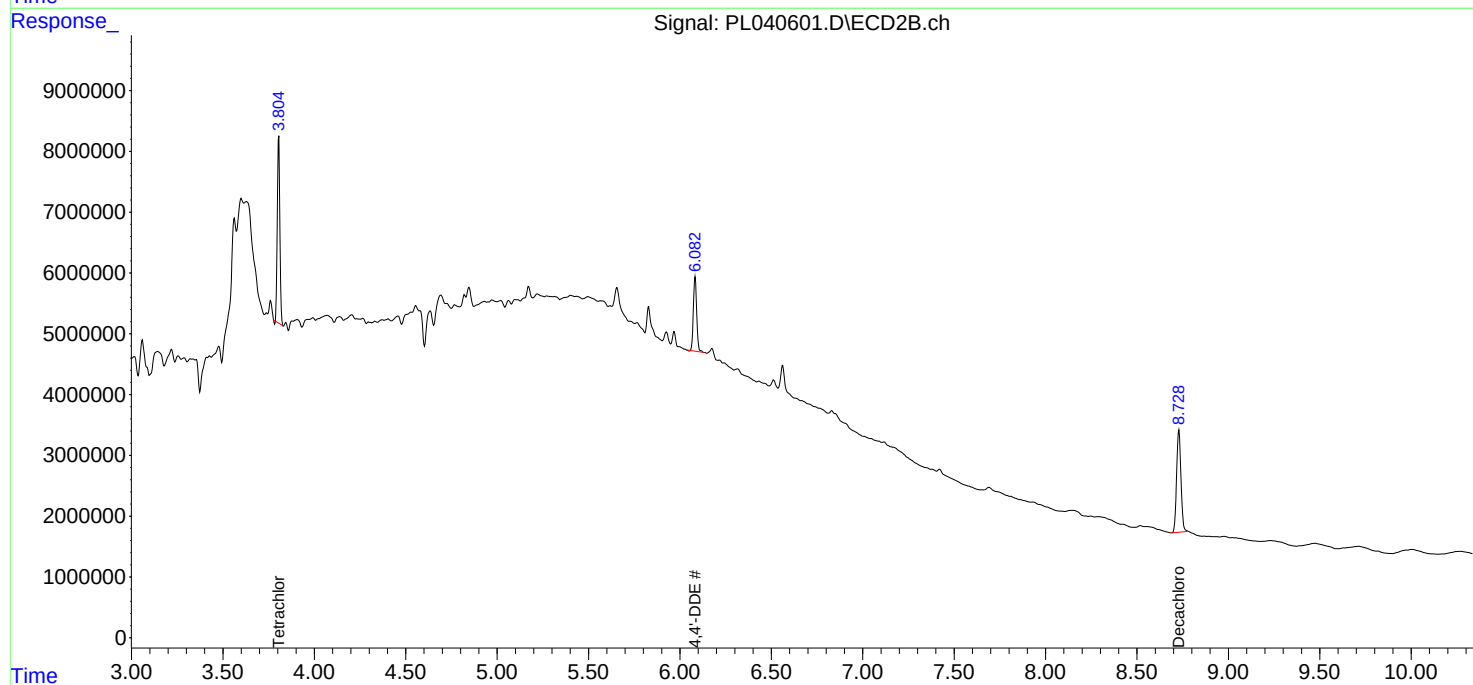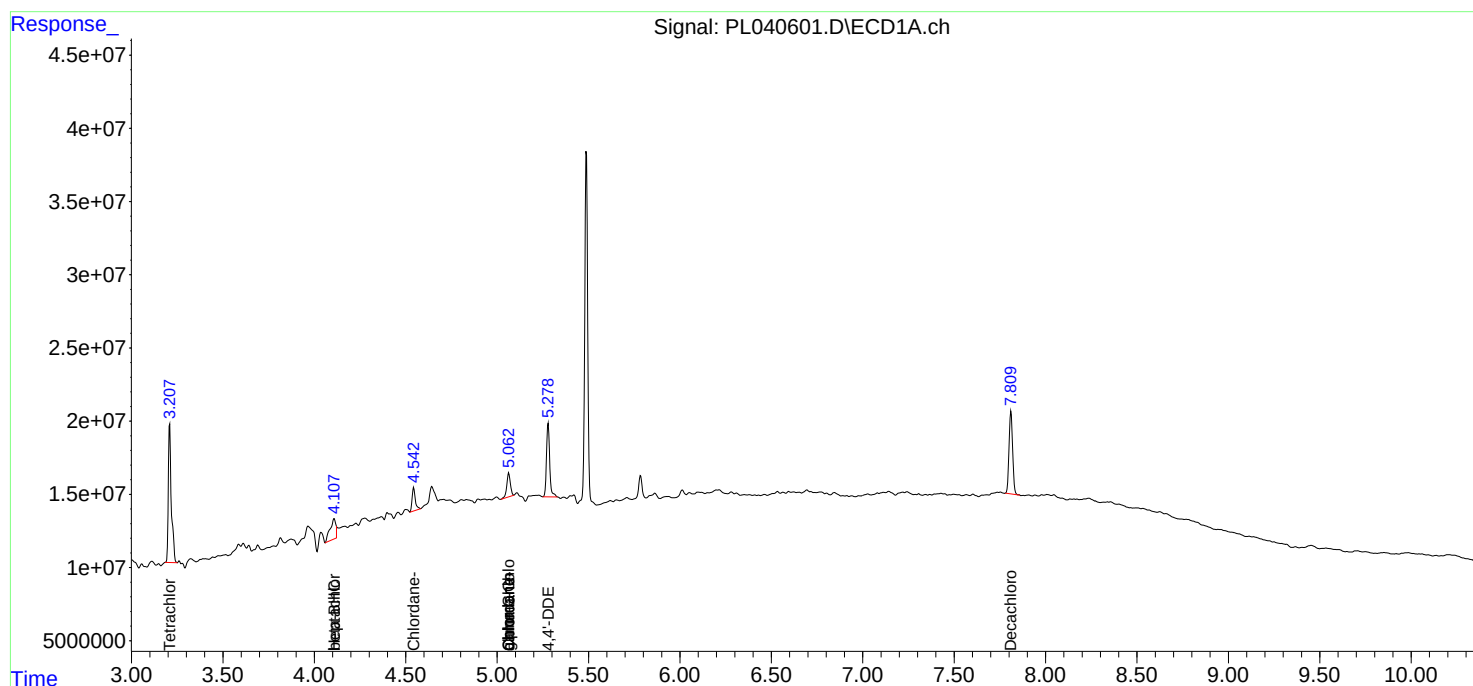


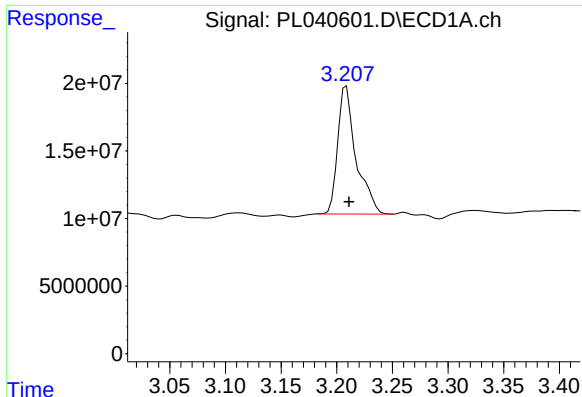

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 108671647
Conc: 14.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

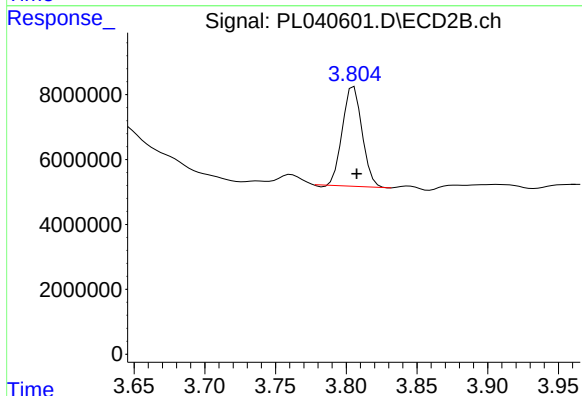


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: -0.002 min
Response: 29820618
Conc: 9.44 ng/ml

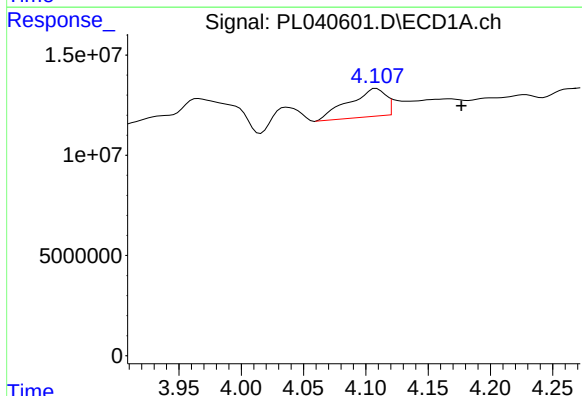


#4 Heptachlor

R.T.: 4.109 min
Delta R.T.: -0.068 min
Response: 29767264
Conc: 2.53 ng/ml

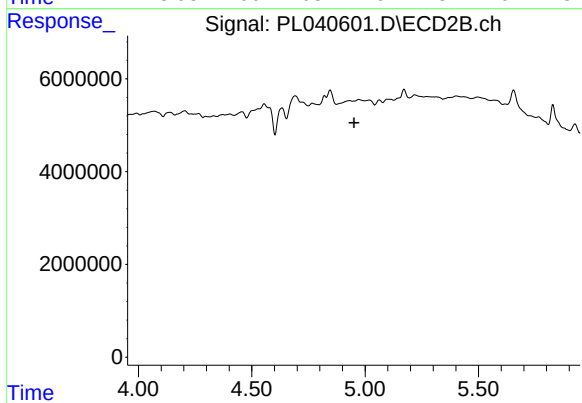

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.951 min
Response: 0
Conc: N.D.

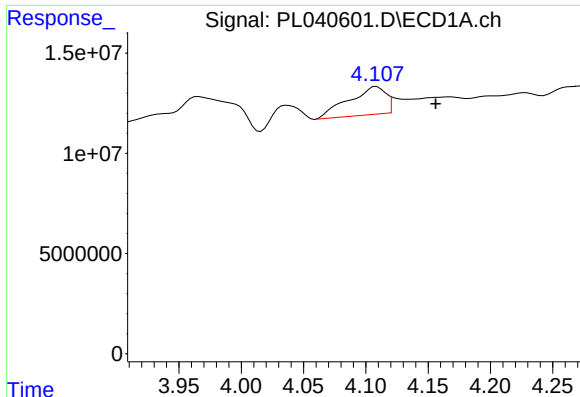

#6 beta-BHC


R.T.: 4.109 min
Delta R.T.: -0.048 min
Response: 29767264
Conc: 7.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

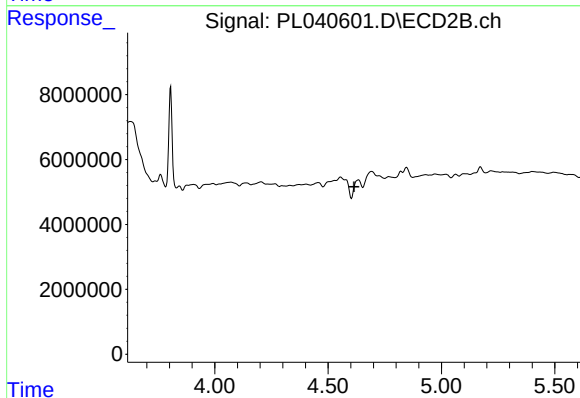


#6 beta-BHC

R.T.: 4.634 min
Delta R.T.: 0.019 min
Response: -79937
Conc: N.D.

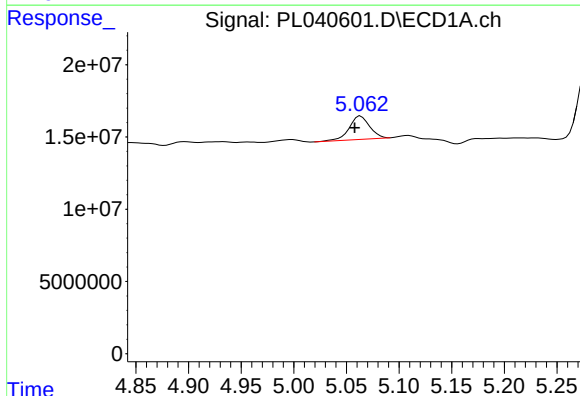


#10 gamma-Chlordane

R.T.: 5.064 min
Delta R.T.: 0.006 min
Response: 21986892
Conc: 2.02 ng/ml

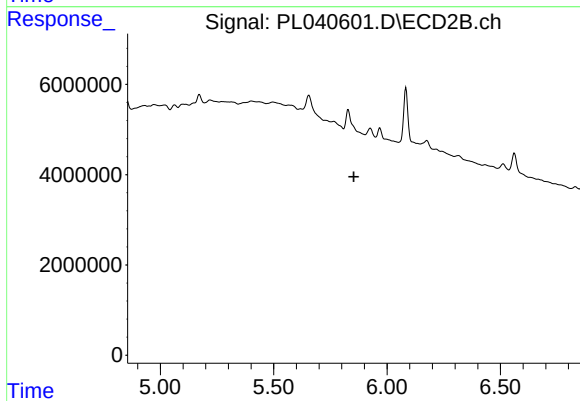

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.853 min
Response: 0
Conc: N.D.

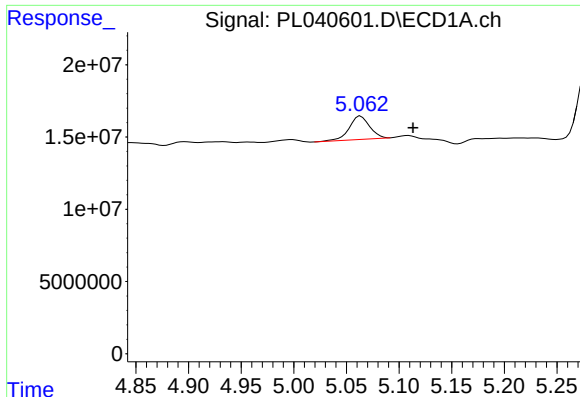

#11 alpha-Chlordane


R.T.: 5.064 min
Delta R.T.: -0.050 min
Response: 21986892
Conc: 2.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

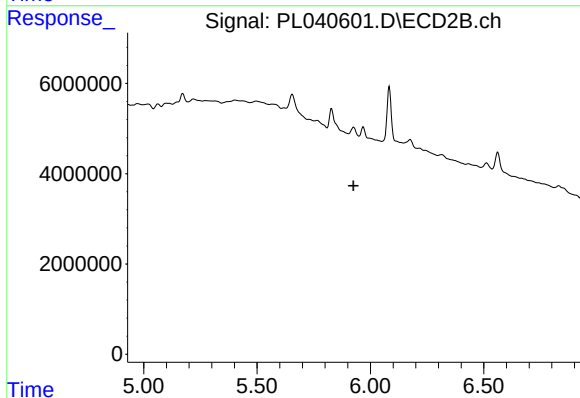


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

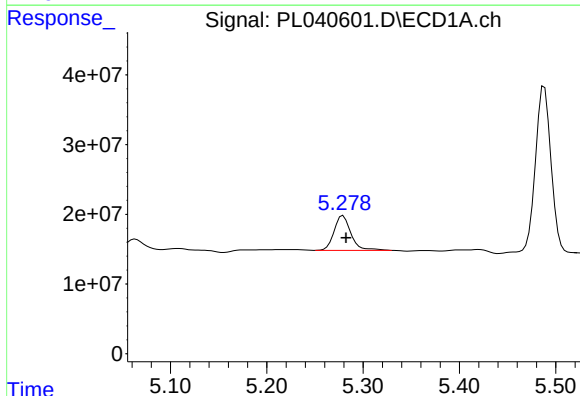


#12 4,4'-DDE

R.T.: 5.279 min
Delta R.T.: -0.003 min
Response: 60859293
Conc: 5.51 ng/ml

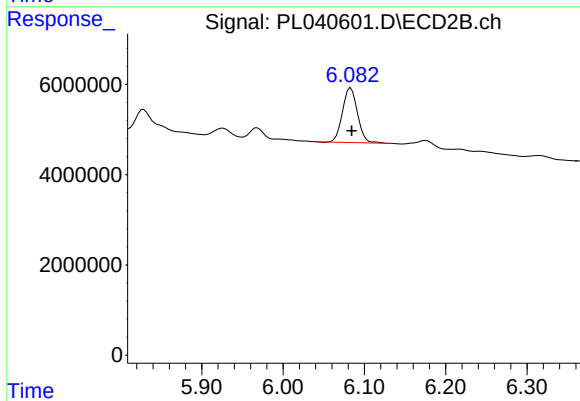

#12 4,4'-DDE


R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 15386627
Conc: 3.82 ng/ml

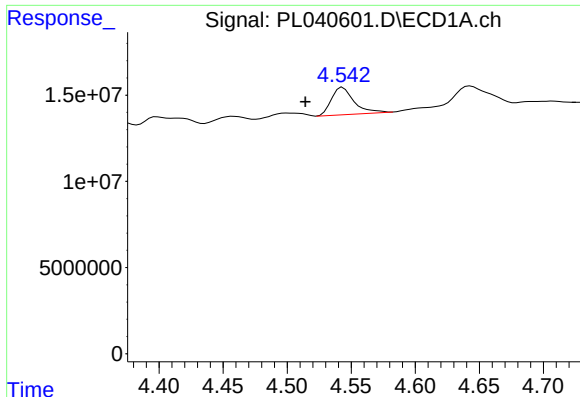

#24 Chlordane-2


R.T.: 4.543 min
Delta R.T.: 0.029 min
Response: 19445878
Conc: 51.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

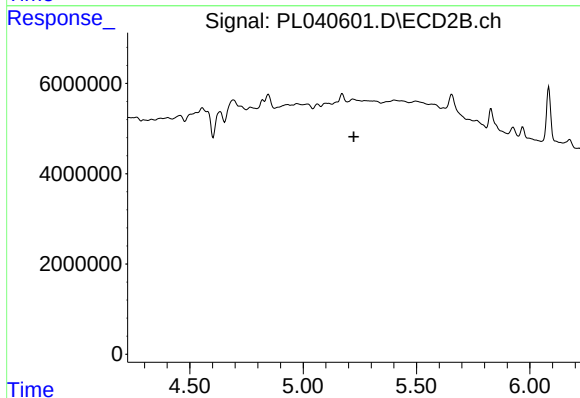


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.223 min
Response: 0
Conc: N.D.

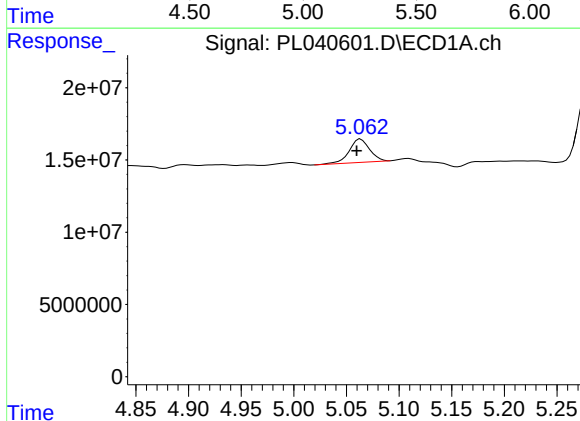


#25 Chlordane-3

R.T.: 5.064 min
Delta R.T.: 0.004 min
Response: 21986892
Conc: 17.12 ng/ml

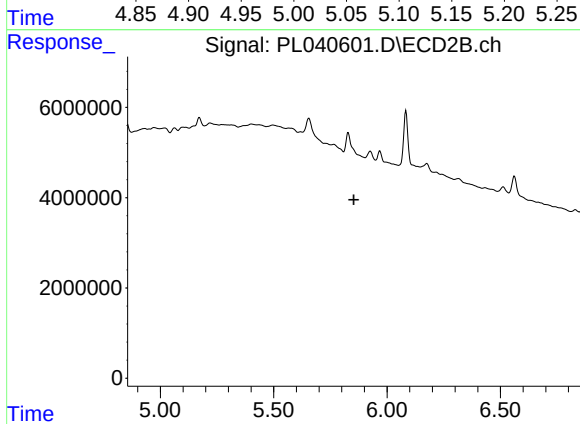

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.854 min
Response: 0
Conc: N.D.

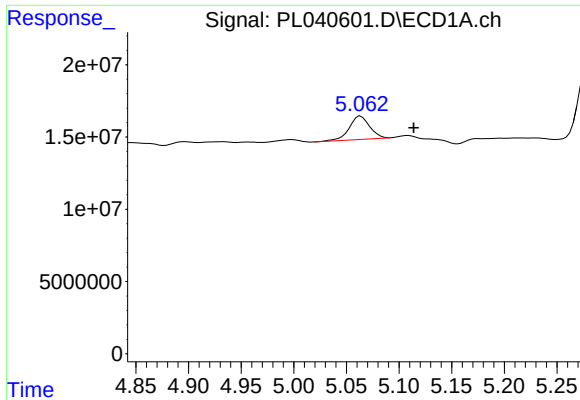

#26 Chlordane-4


R.T.: 5.064 min
Delta R.T.: -0.050 min
Response: 21986892
Conc: 18.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

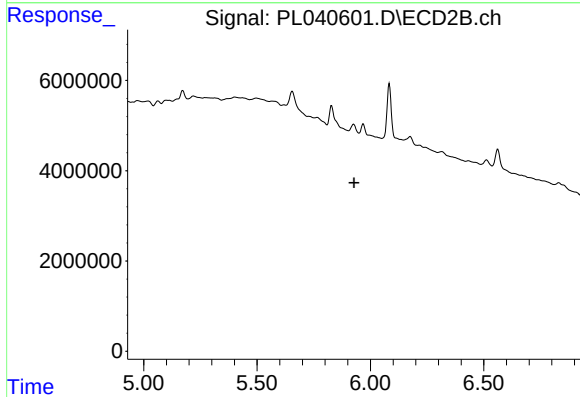


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

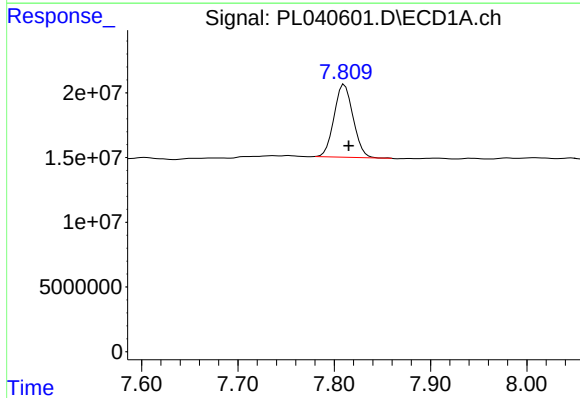

#28 Decachlorobiphenyl

R.T.: 7.811 min
Delta R.T.: -0.004 min
Response: 76918205
Conc: 8.09 ng/ml

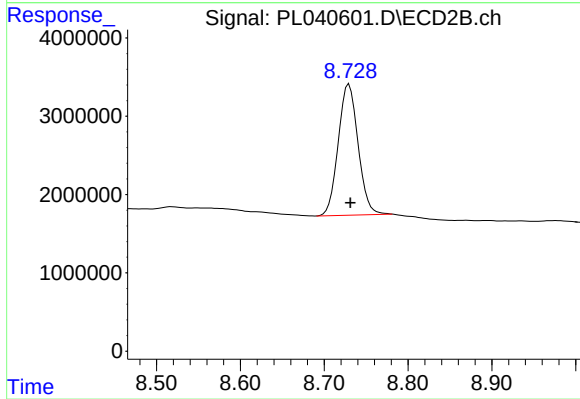

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.002 min
Response: 27601103
Conc: 8.72 ng/ml