

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100318\
 Data File : PL040645.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2018 02:45
 Operator : AJ\SJ
 Sample : J5198-02
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 09:59:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.806	179.1E6	70247596	24.465	22.246
28)	SA Decachlor...	7.811	8.730	199.6E6	56314434	21.000	17.783
Target Compounds							
4)	MA Heptachlor	4.108f	0.000	22142608	0	1.882	N.D. #
6)	B beta-BHC	4.108f	0.000	22142608	0	5.246	N.D. #
7)	B delta-BHC	0.000	4.820	0	10829644	N.D.	2.346 #
23)	Chlordane-1	0.000	4.820	0	10829644	N.D.	70.173 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100318\
Data File : PL040645.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2018 02:45
Operator : AJ\SJ
Sample : J5198-02
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 09:59:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

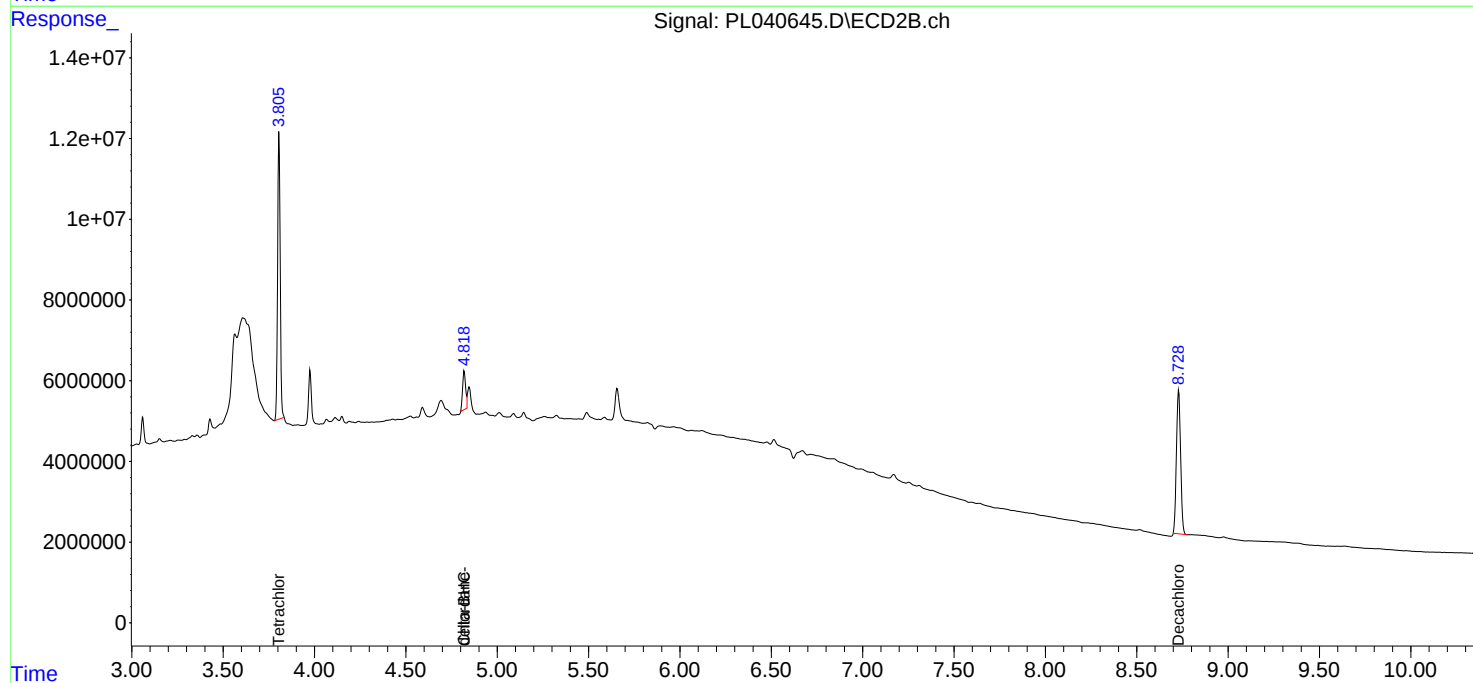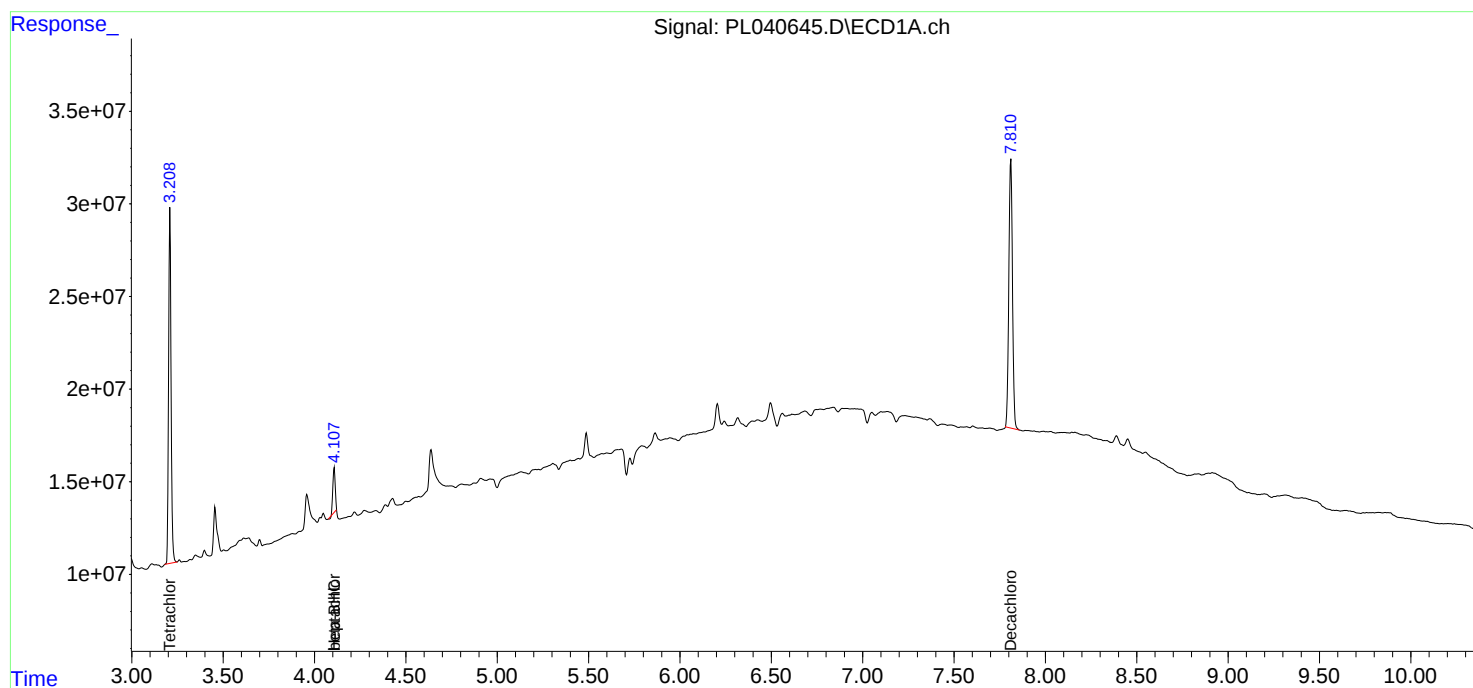


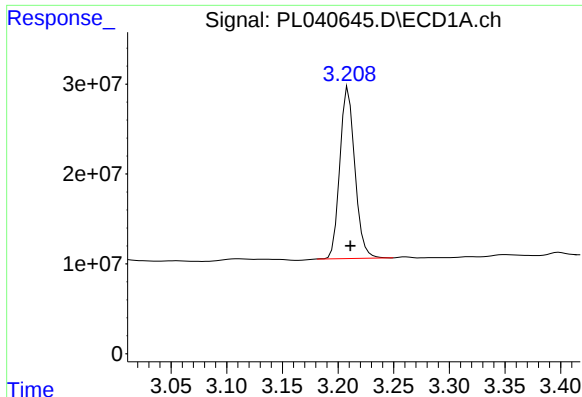

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 179083086
Conc: 24.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

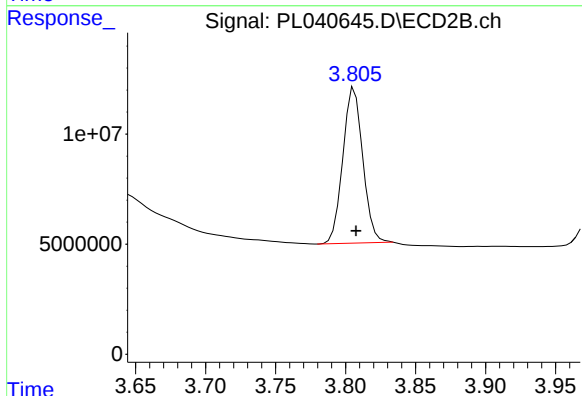


#1 Tetrachloro-m-xylene

R.T.: 3.806 min
Delta R.T.: -0.001 min
Response: 70247596
Conc: 22.25 ng/ml

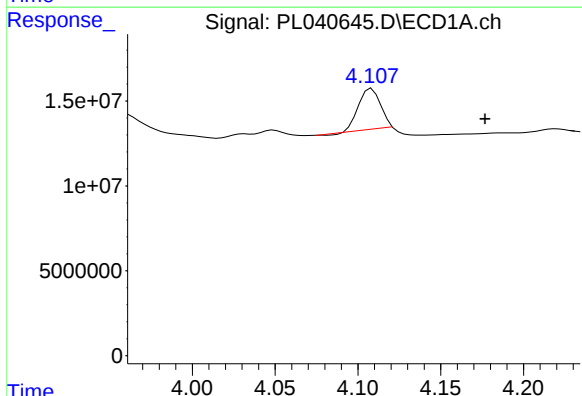


#4 Heptachlor

R.T.: 4.108 min
Delta R.T.: -0.068 min
Response: 22142608
Conc: 1.88 ng/ml

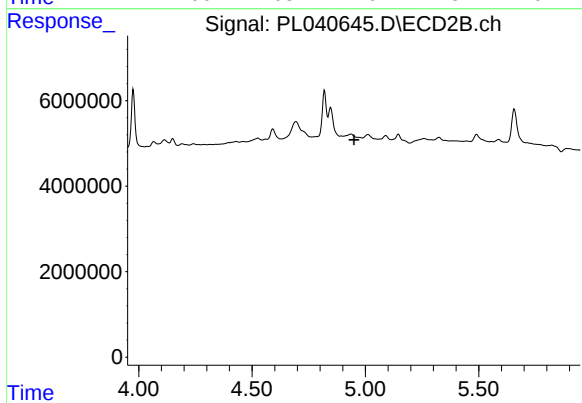

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.951 min
Response: 0
Conc: N.D.

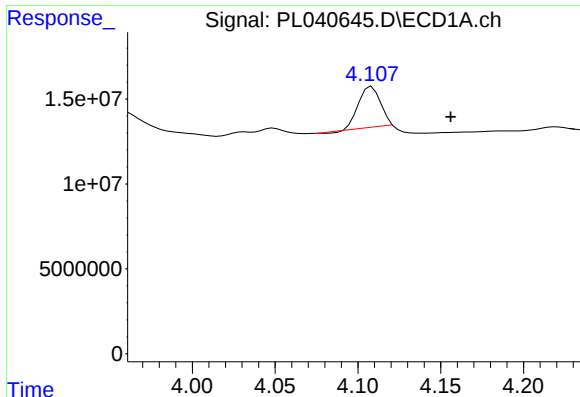

#6 beta-BHC


R.T.: 4.108 min
Delta R.T.: -0.048 min
Response: 22142608
Conc: 5.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

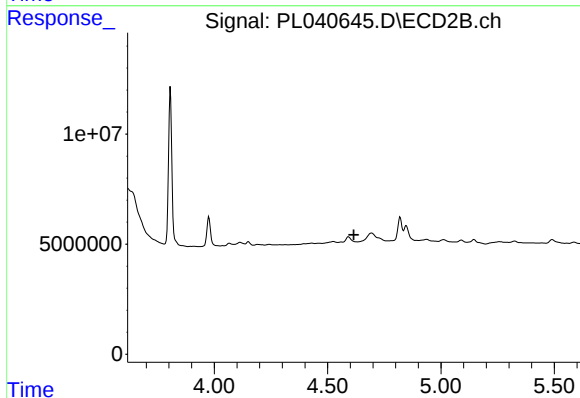


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.615 min
Response: 0
Conc: N.D.

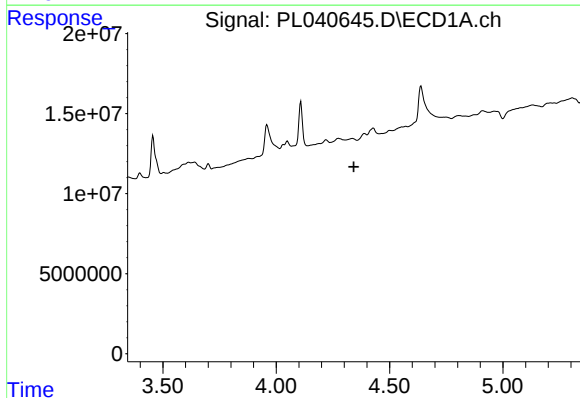


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

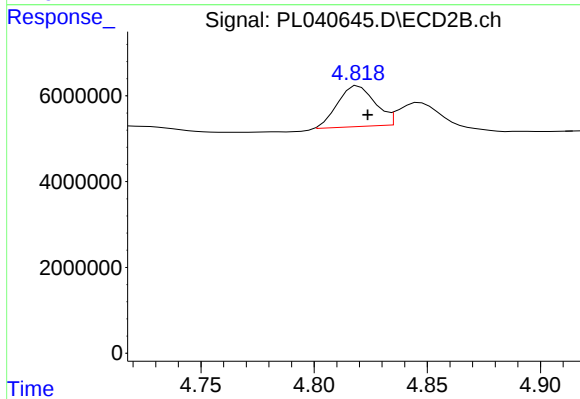

#7 delta-BHC


R.T.: 4.820 min
Delta R.T.: -0.004 min
Response: 10829644
Conc: 2.35 ng/ml

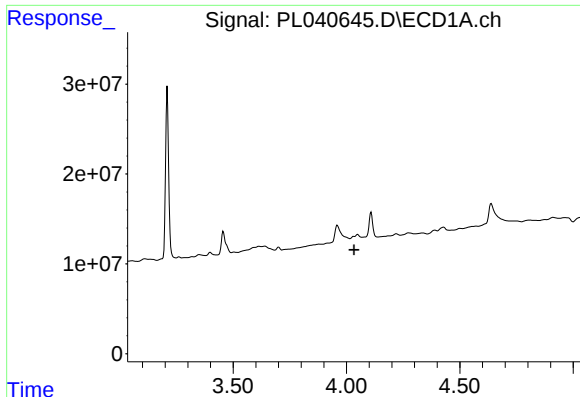

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

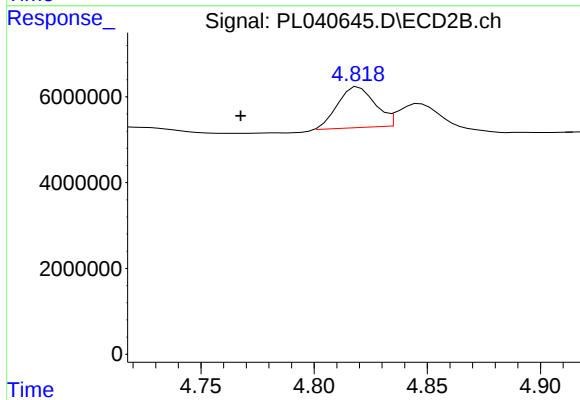


#23 Chlordane-1

R.T.: 4.820 min
Delta R.T.: 0.052 min
Response: 10829644
Conc: 70.17 ng/ml

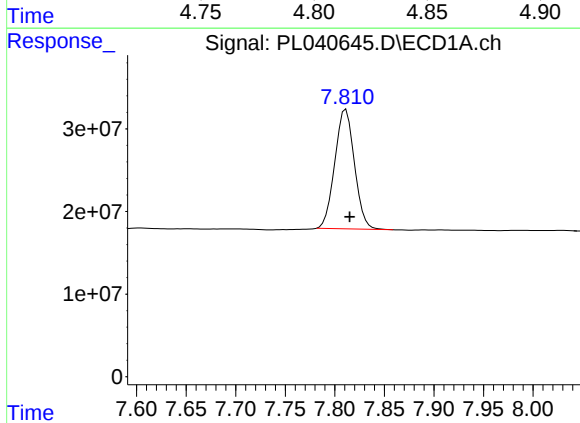

#28 Decachlorobiphenyl

R.T.: 7.811 min
Delta R.T.: -0.004 min
Response: 199618607
Conc: 21.00 ng/ml

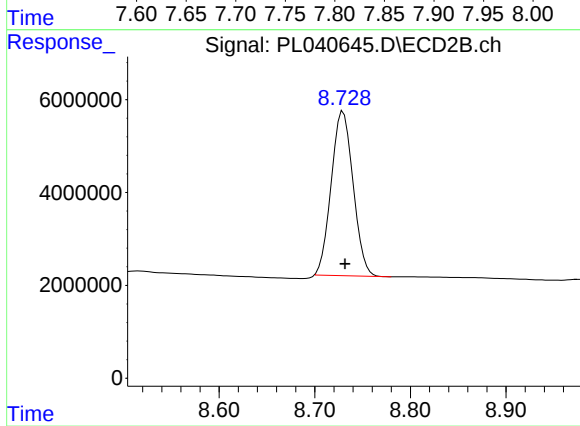

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.002 min
Response: 56314434
Conc: 17.78 ng/ml