

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100319\
 Data File : PL053060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2019 20:59
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 00:59:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	4.049	239.2E6	62887832	24.050	23.420
28)	SA Decachlor...	8.341	9.128	240.6E6	62560412	24.022	21.325
Target Compounds							
5)	MB Aldrin	0.000	5.541	0	5142187	N.D.	1.484 #
7)	B delta-BHC	0.000	5.089f	0	1700797	N.D.	0.470 #
8)	B Heptachlo...	0.000	5.923	0	15063428	N.D.	4.495 #
10)	B gamma-Chl...	0.000	6.132f	0	9274360	N.D.	2.741 #
15)	B Endosulfa...	0.000	6.971	0	720367	N.D.	0.243 #
16)	A 4,4'-DDD	0.000	6.872	0	1181571	N.D.	0.482 #
21)	B Endrin ke...	0.000	7.780	0	2157248	N.D.	0.756 #
24)	Chlordane-2	0.000	5.541f	0	5142187	N.D.	45.944 #
25)	Chlordane-3	0.000	6.132f	0	9274360	N.D.	21.295 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100319\
Data File : PL053060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2019 20:59
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 00:59:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

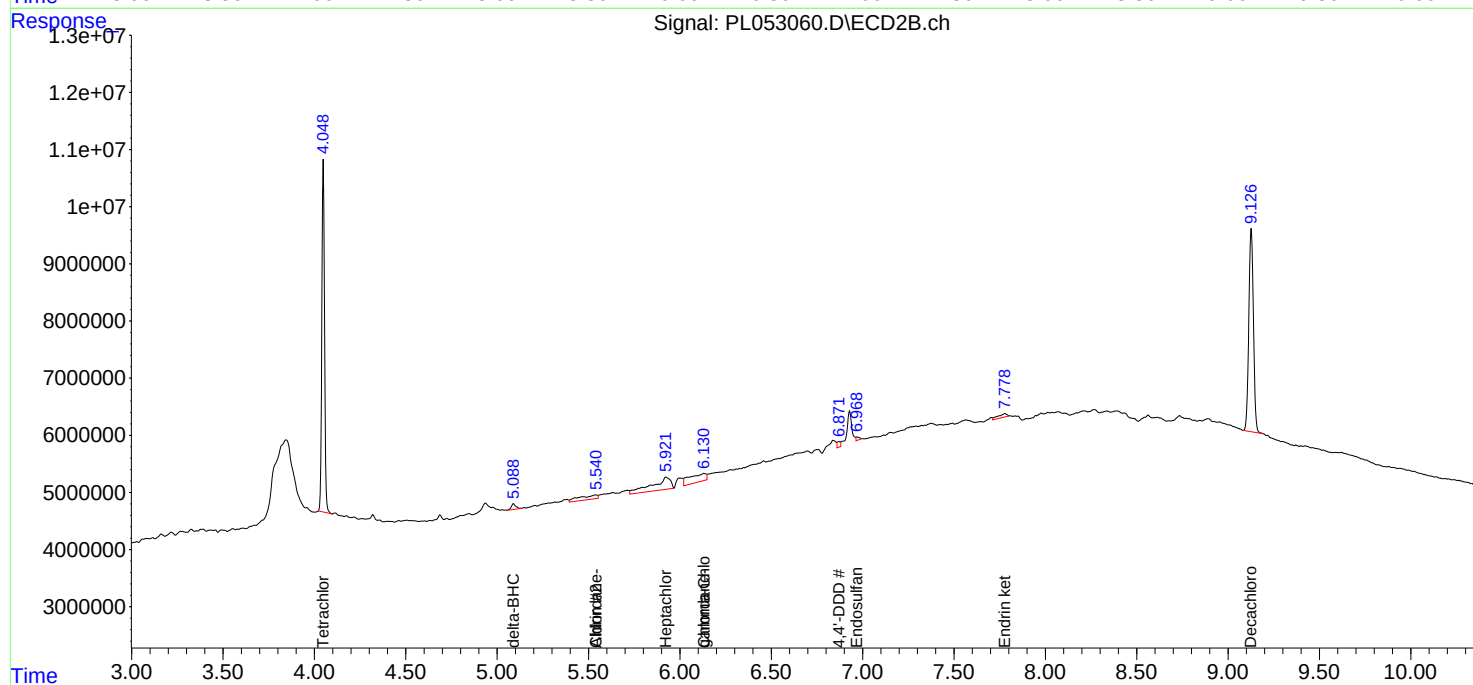


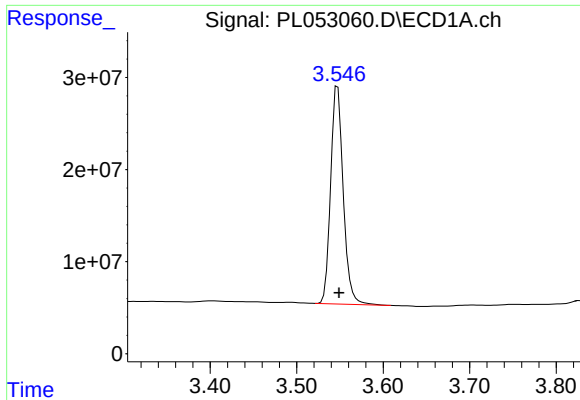

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: -0.002 min
Response: 239218197
Conc: 24.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

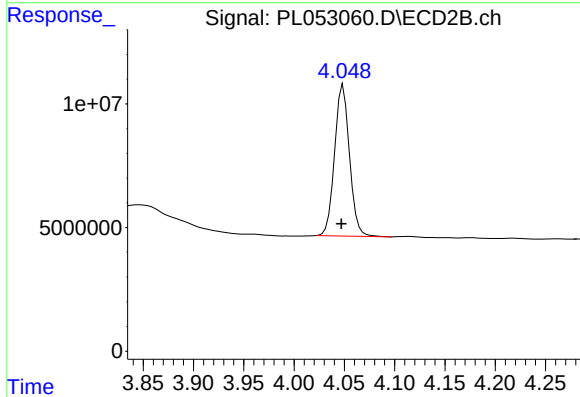


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.002 min
Response: 62887832
Conc: 23.42 ng/ml

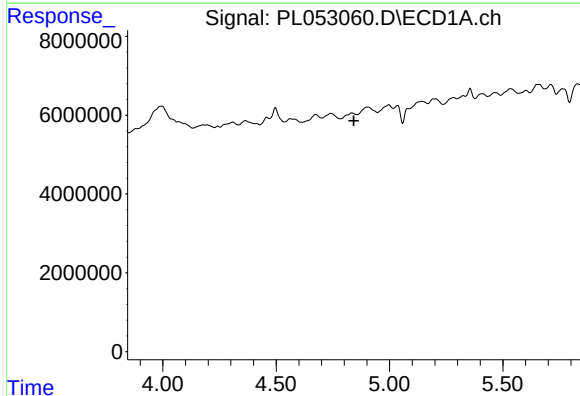


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.843 min
Response: 0
Conc: N.D.

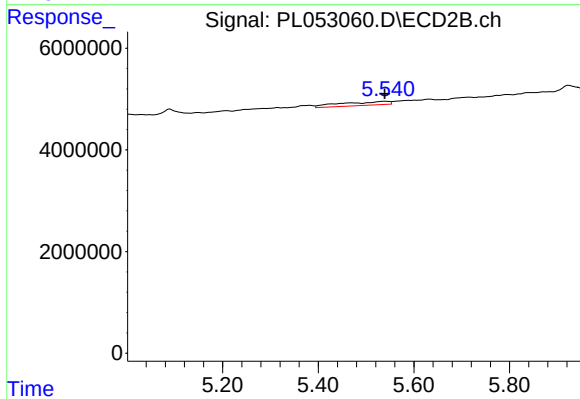

#5 Aldrin


R.T.: 5.541 min
Delta R.T.: 0.003 min
Response: 5142187
Conc: 1.48 ng/ml

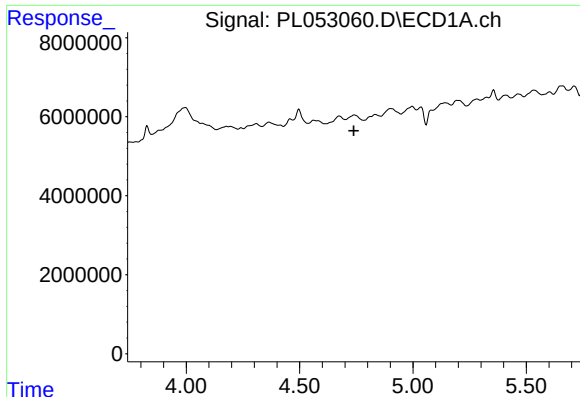

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

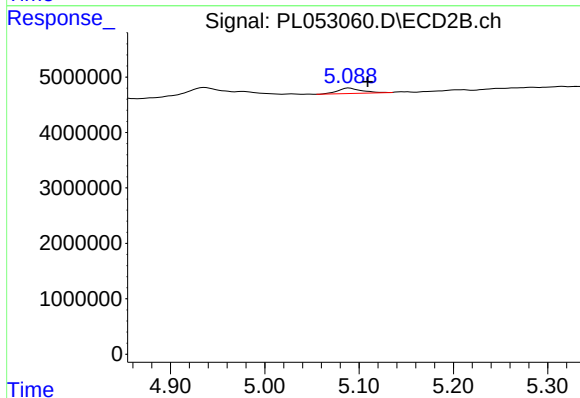


#7 delta-BHC

R.T.: 5.089 min
Delta R.T.: -0.020 min
Response: 1700797
Conc: 0.47 ng/ml

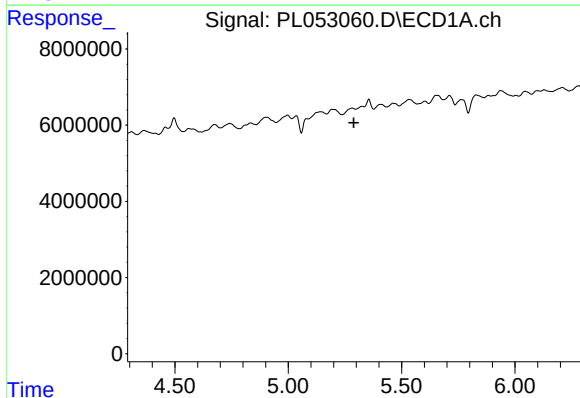


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

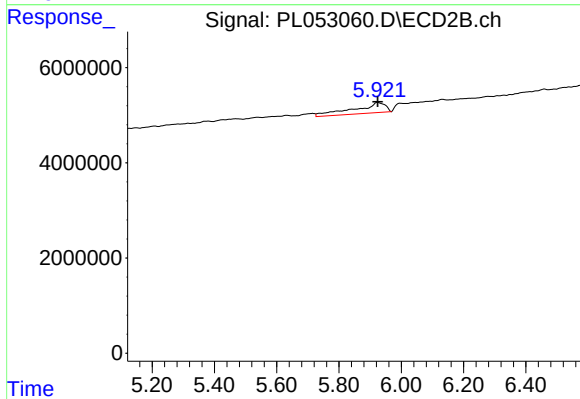

#8 Heptachlor epoxide


R.T.: 5.923 min
Delta R.T.: -0.002 min
Response: 15063428
Conc: 4.49 ng/ml

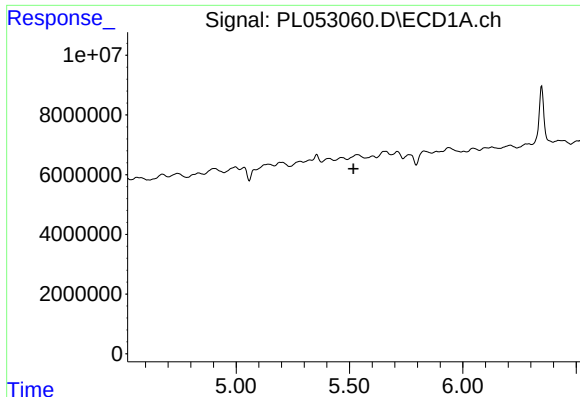

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

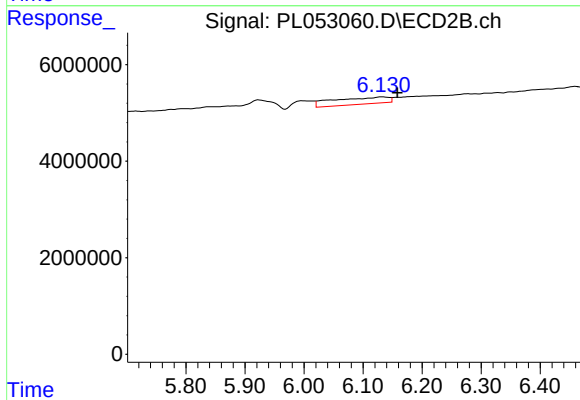


#10 gamma-Chlordane

R.T.: 6.132 min
Delta R.T.: -0.026 min
Response: 9274360
Conc: 2.74 ng/ml

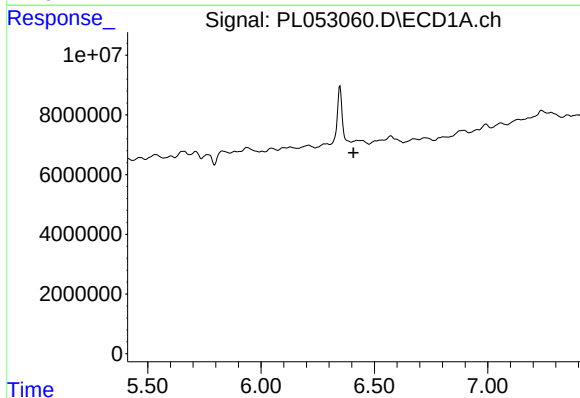


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

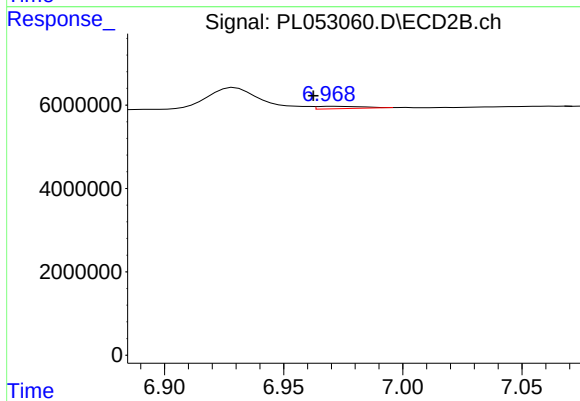

#15 Endosulfan II


R.T.: 6.971 min
Delta R.T.: 0.008 min
Response: 720367
Conc: 0.24 ng/ml

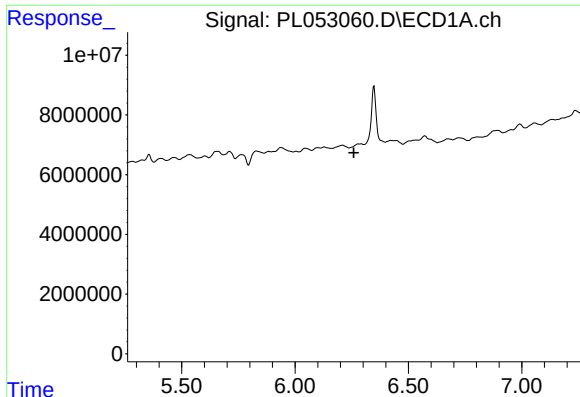

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

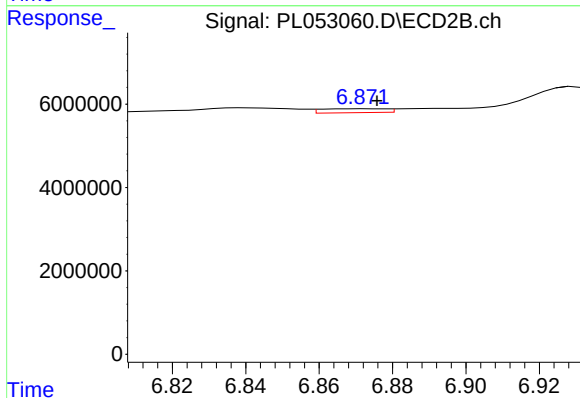


#16 4,4'-DDD

R.T.: 6.872 min
Delta R.T.: -0.003 min
Response: 1181571
Conc: 0.48 ng/ml

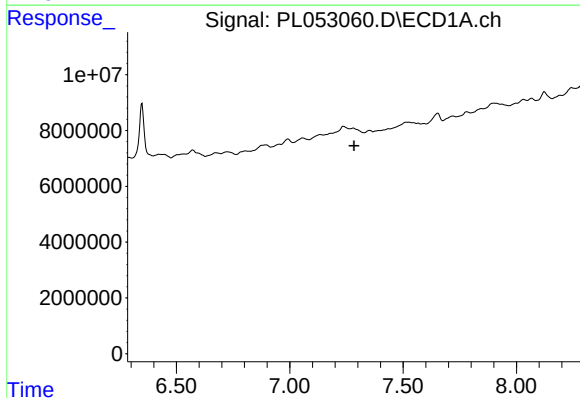


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

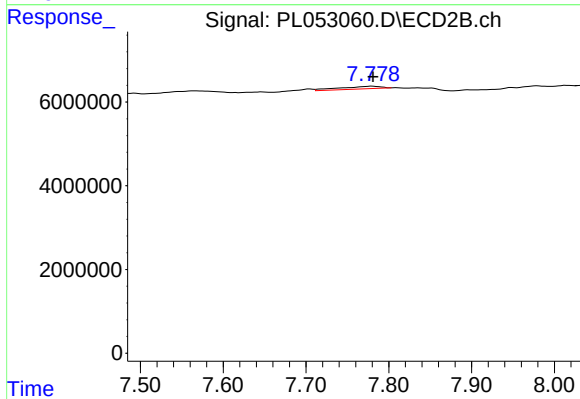

#21 Endrin ketone


R.T.: 7.780 min
Delta R.T.: -0.001 min
Response: 2157248
Conc: 0.76 ng/ml

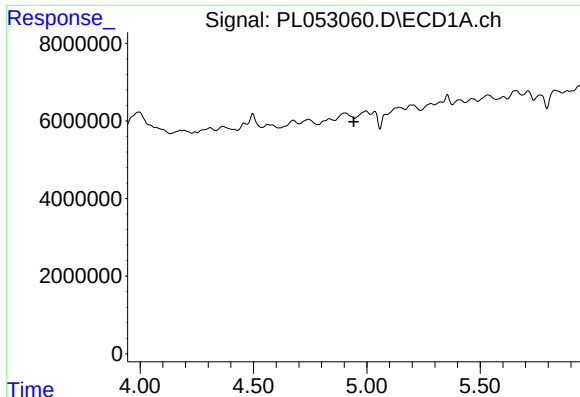

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

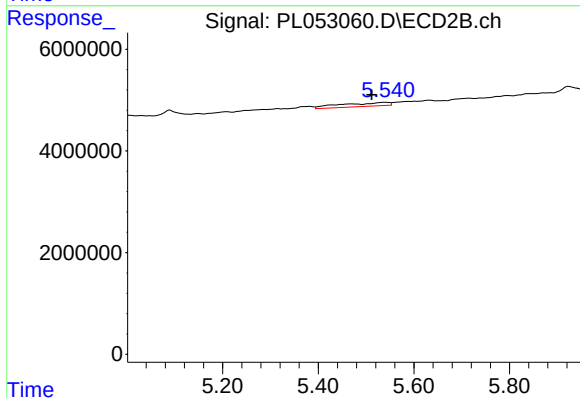


#24 Chlordane-2

R.T.: 5.541 min
Delta R.T.: 0.029 min
Response: 5142187
Conc: 45.94 ng/ml

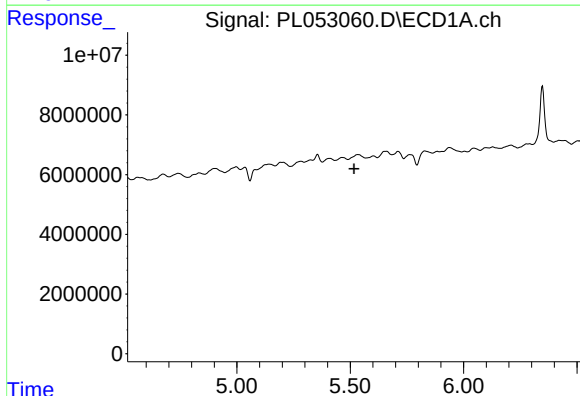


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

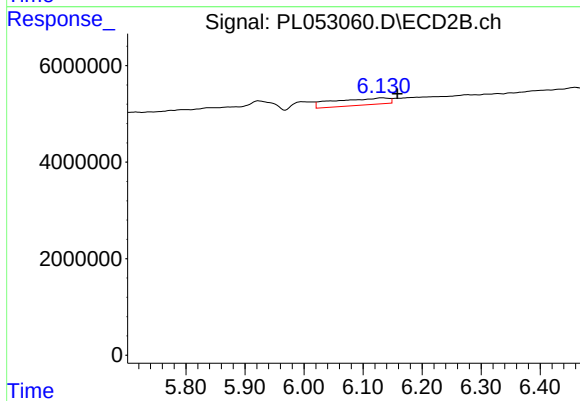

#25 Chlordane-3

R.T.: 6.132 min
Delta R.T.: -0.026 min
Response: 9274360
Conc: 21.30 ng/ml

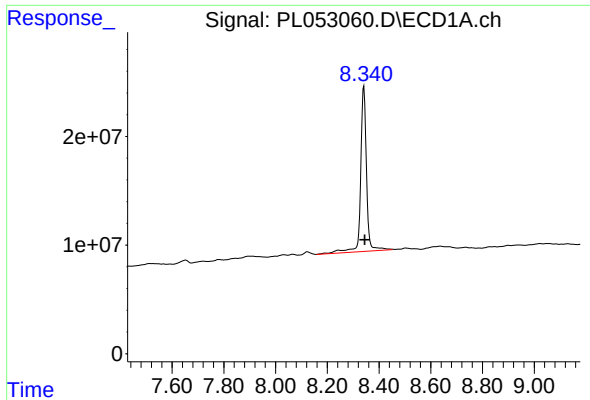

#28 Decachlorobiphenyl


R.T.: 8.341 min

Delta R.T.: -0.004 min

Response: 240610767

Conc: 24.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

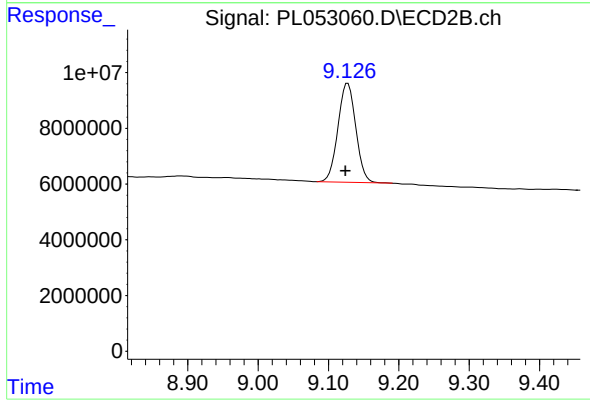

#28 Decachlorobiphenyl

R.T.: 9.128 min

Delta R.T.: 0.003 min

Response: 62560412

Conc: 21.32 ng/ml