

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100319\
 Data File : PL053057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2019 20:17
 Operator : SG\AJ
 Sample : K5095-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMPOSITE-3

Manual Integrations
 APPROVED

Ankita
 10/4/2019 2:16:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 00:58:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.046	867.6E6	47293269	87.223	17.613m#
28)	SA Decachlor...	8.338	9.124	223.9E6	74365527	22.349m	25.349m
Target Compounds							
16)	A 4,4'-DDD	6.256	6.880	747.7E6	381.3E6	83.185	155.465m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100319\
Data File : PL053057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2019 20:17
Operator : SG\AJ
Sample : K5095-03
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMPOSITE-3


Manual Integrations
APPROVED

Ankita
10/4/2019 2:16:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 00:58:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

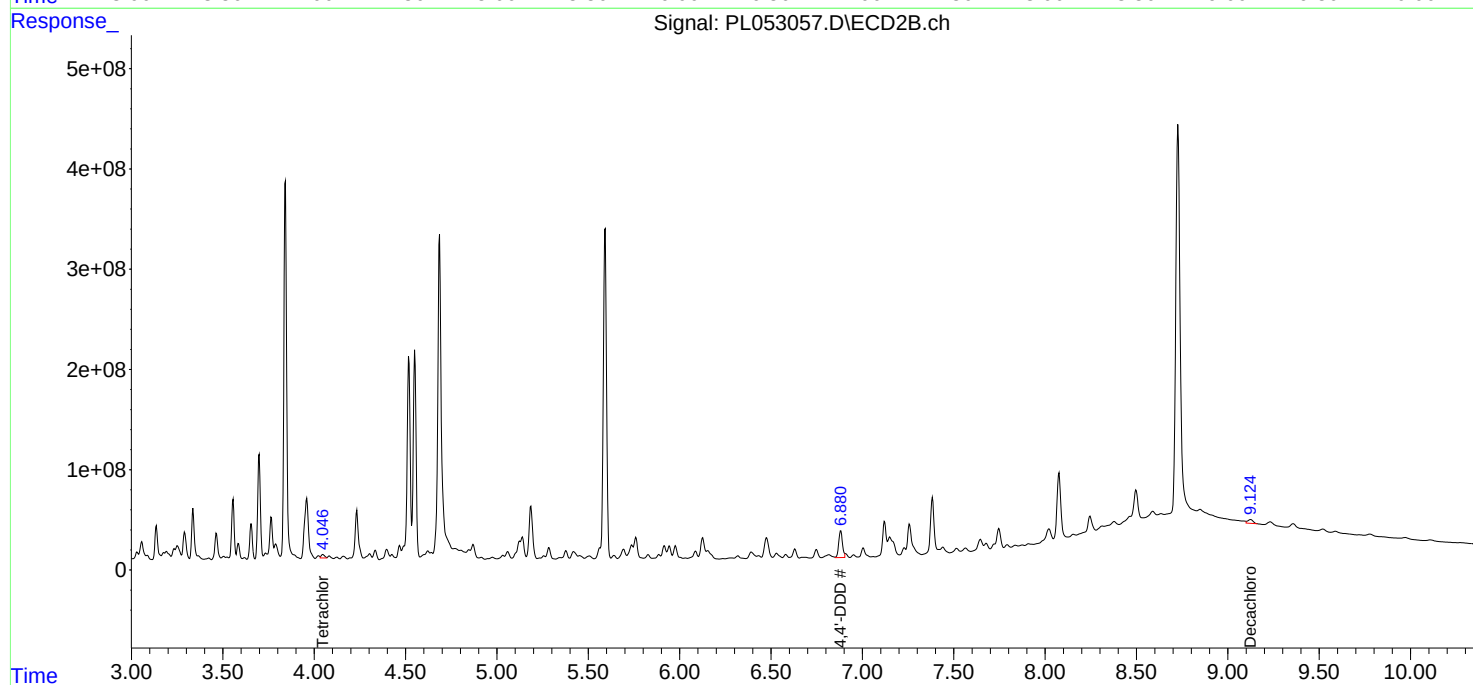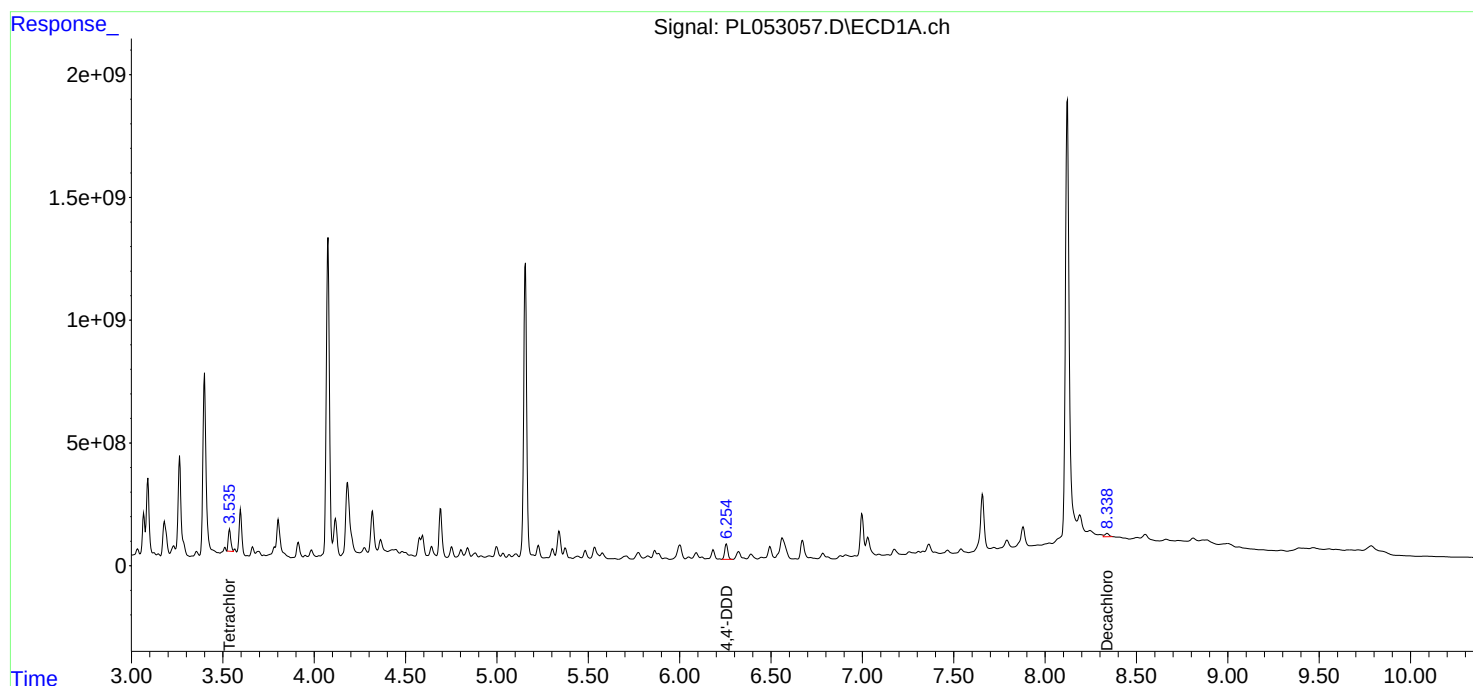

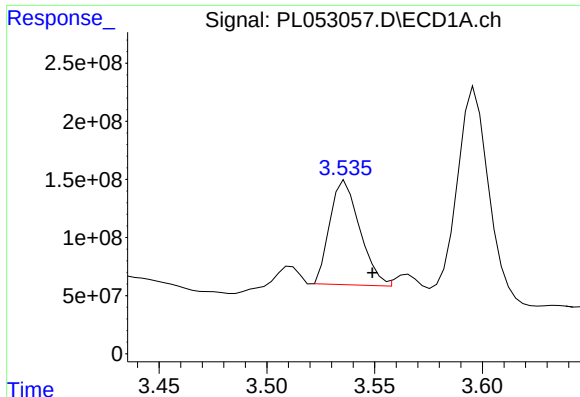


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: -0.012 min
Response: 867579633
Conc: 87.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-3


Manual Integrations
APPROVED

Ankita
10/4/2019 2:16:38 PM

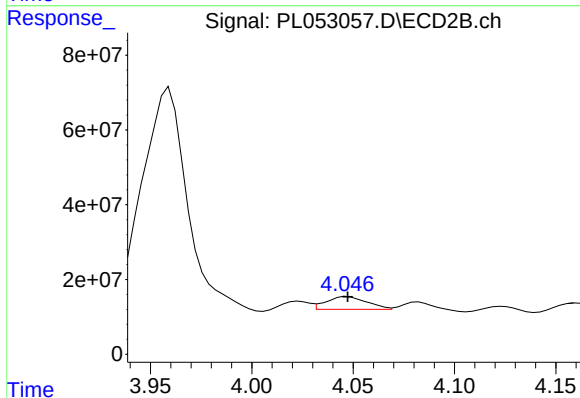


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: -0.001 min
Response: 47293269
Conc: 17.61 ng/ml m

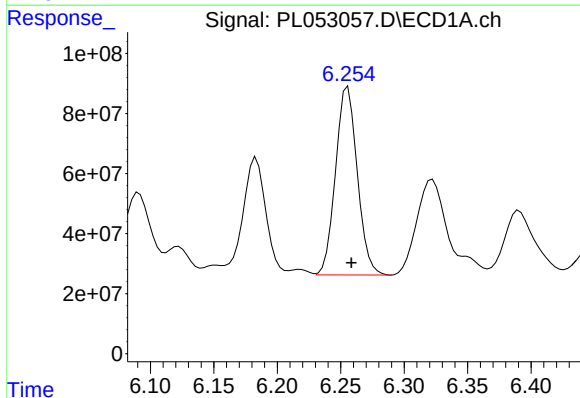


#16 4,4'-DDD

R.T.: 6.256 min
Delta R.T.: -0.003 min
Response: 747692974
Conc: 83.18 ng/ml

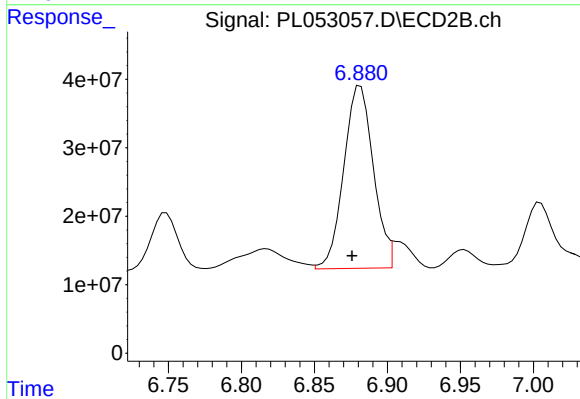

#16 4,4'-DDD

R.T.: 6.880 min
Delta R.T.: 0.004 min
Response: 381288329
Conc: 155.47 ng/ml m

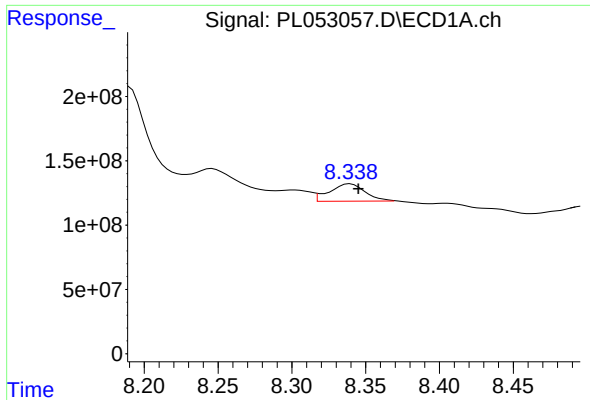


#28 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: -0.007 min
Response: 223851379
Conc: 22.35 ng/ml m

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-3

Manual Integrations
APPROVED

Ankita
10/4/2019 2:16:38 PM

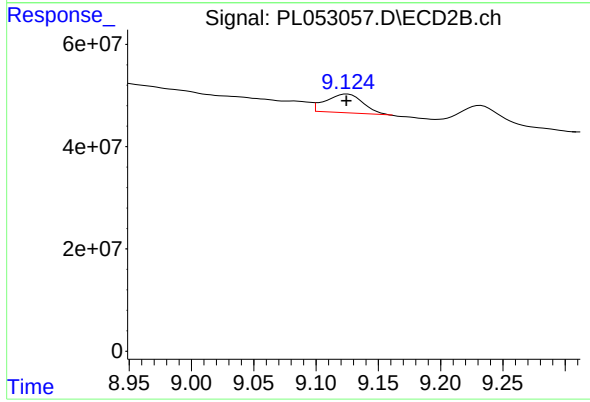

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: 0.000 min
Response: 74365527
Conc: 25.35 ng/ml m