

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100319\
 Data File : PL053058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2019 20:31
 Operator : SG\AJ
 Sample : K5095-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMPOSITE-4

Manual Integrations
 APPROVED

Ankita
 10/4/2019 2:16:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 00:58:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.048	750.4E6	55641114	75.439m	20.721m#
28)	SA Decachlor...	8.339	9.125	233.4E6	58491368	23.298m	19.938m
Target Compounds							
16)	A 4,4'-DDD	6.255	6.885	45072094	19123186	5.015m	7.797m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100319\
Data File : PL053058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2019 20:31
Operator : SG\AJ
Sample : K5095-04
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMPOSITE-4


Manual Integrations
APPROVED

Ankita
10/4/2019 2:16:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 00:58:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

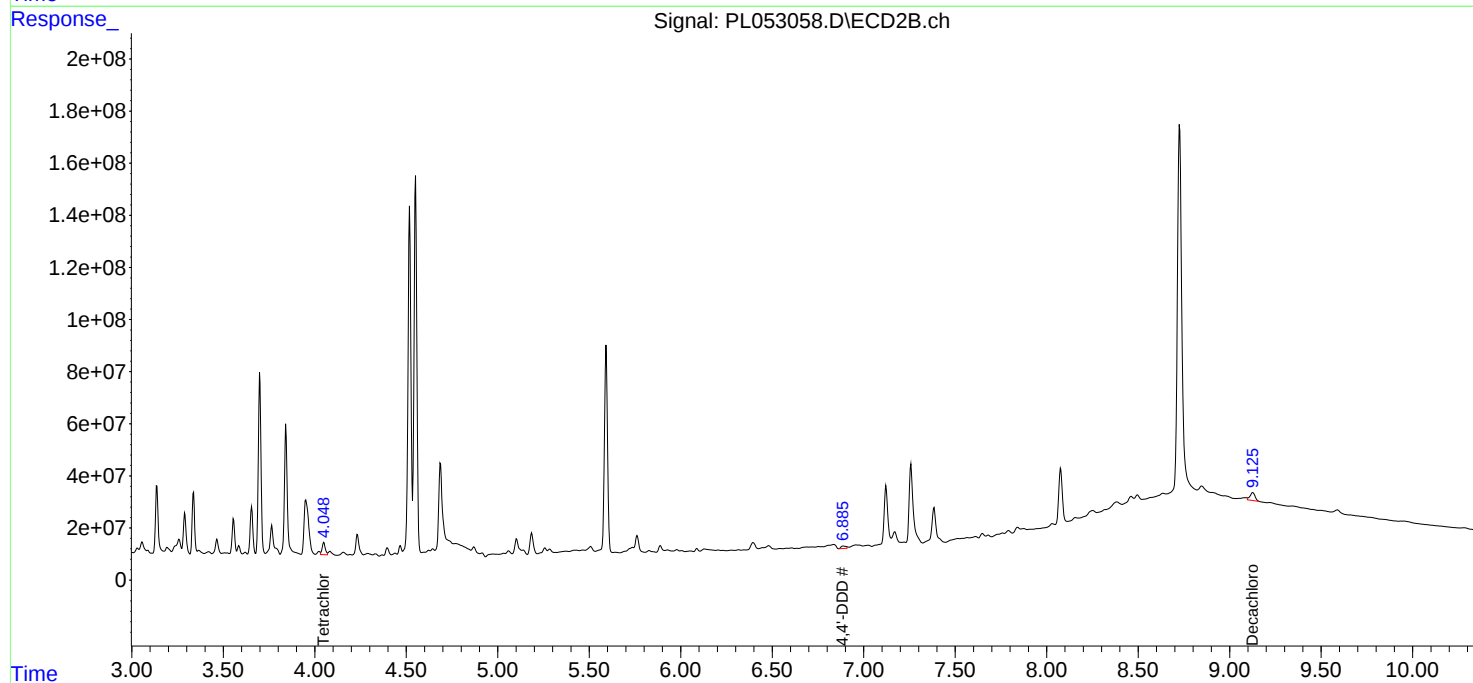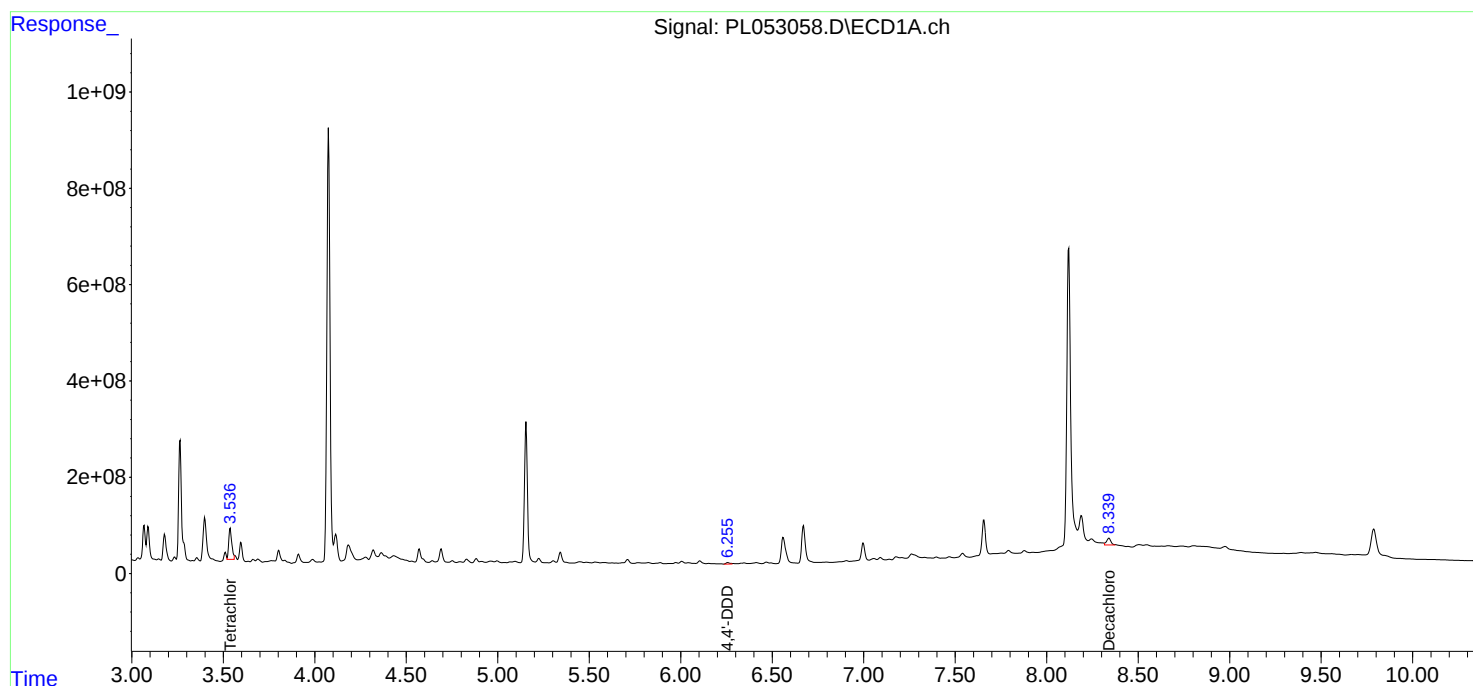

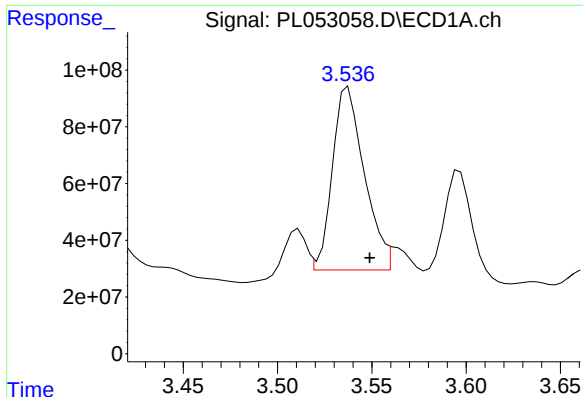


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.013 min
Response: 750364584
Conc: 75.44 ng/ml m

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-4


Manual Integrations
APPROVED

Ankita
10/4/2019 2:16:40 PM

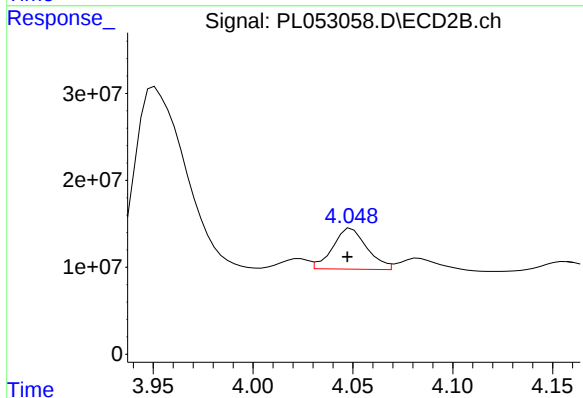


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 55641114
Conc: 20.72 ng/ml m

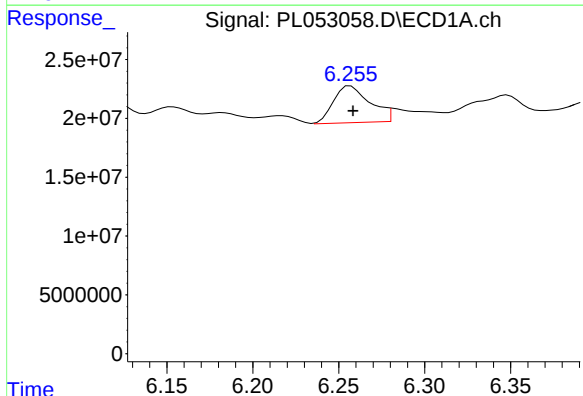


#16 4,4'-DDD

R.T.: 6.255 min
Delta R.T.: -0.003 min
Response: 45072094
Conc: 5.01 ng/ml m

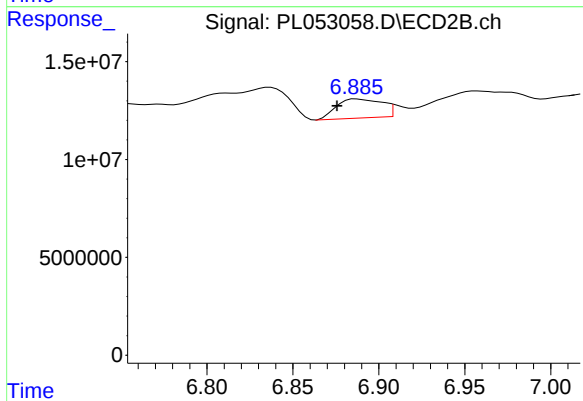

#16 4,4'-DDD

R.T.: 6.885 min
Delta R.T.: 0.010 min
Response: 19123186
Conc: 7.80 ng/ml m

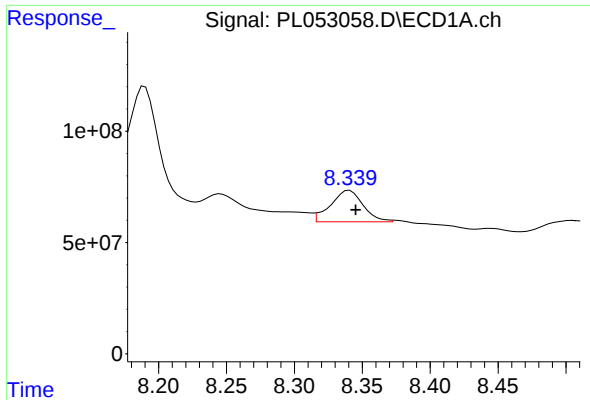


#28 Decachlorobiphenyl

R.T.: 8.339 min
Delta R.T.: -0.006 min
Response: 233355343
Conc: 23.30 ng/ml m

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-4

Manual Integrations
APPROVED

Ankita
10/4/2019 2:16:40 PM

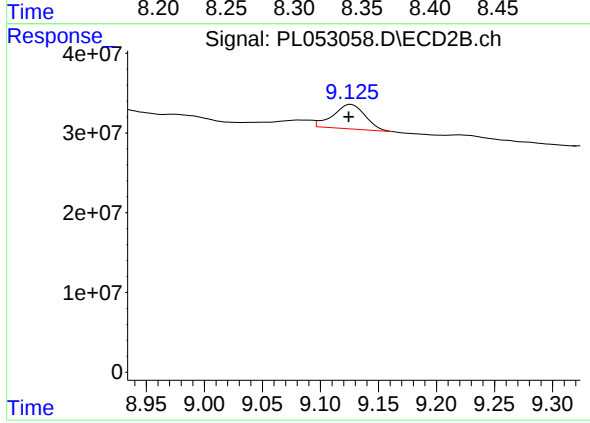

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 58491368
Conc: 19.94 ng/ml m