

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
 Data File : PL078032.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 14:46
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 15:51:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 15:50:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	182.5E6	327.1E6	99.842	98.618
28)	SA Decachlor...	8.902	7.720	143.6E6	203.6E6	92.733	96.065
Target Compounds							
23)	Chlordane-1	4.574	3.600	73965832	98388046	998.622	973.105
24)	Chlordane-2	5.107	4.169	76050239	102.9E6	965.219	954.381
25)	Chlordane-3	5.819	4.792	303.5E6	304.8E6	1020.750	987.115
26)	Chlordane-4	5.897	4.853	359.1E6	316.8E6	1003.444	980.041
27)	Chlordane-5	6.756	5.518	59479148	78399752	1006.329	953.715



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
Data File : PL078032.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 14:46
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 15:51:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 15:50:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

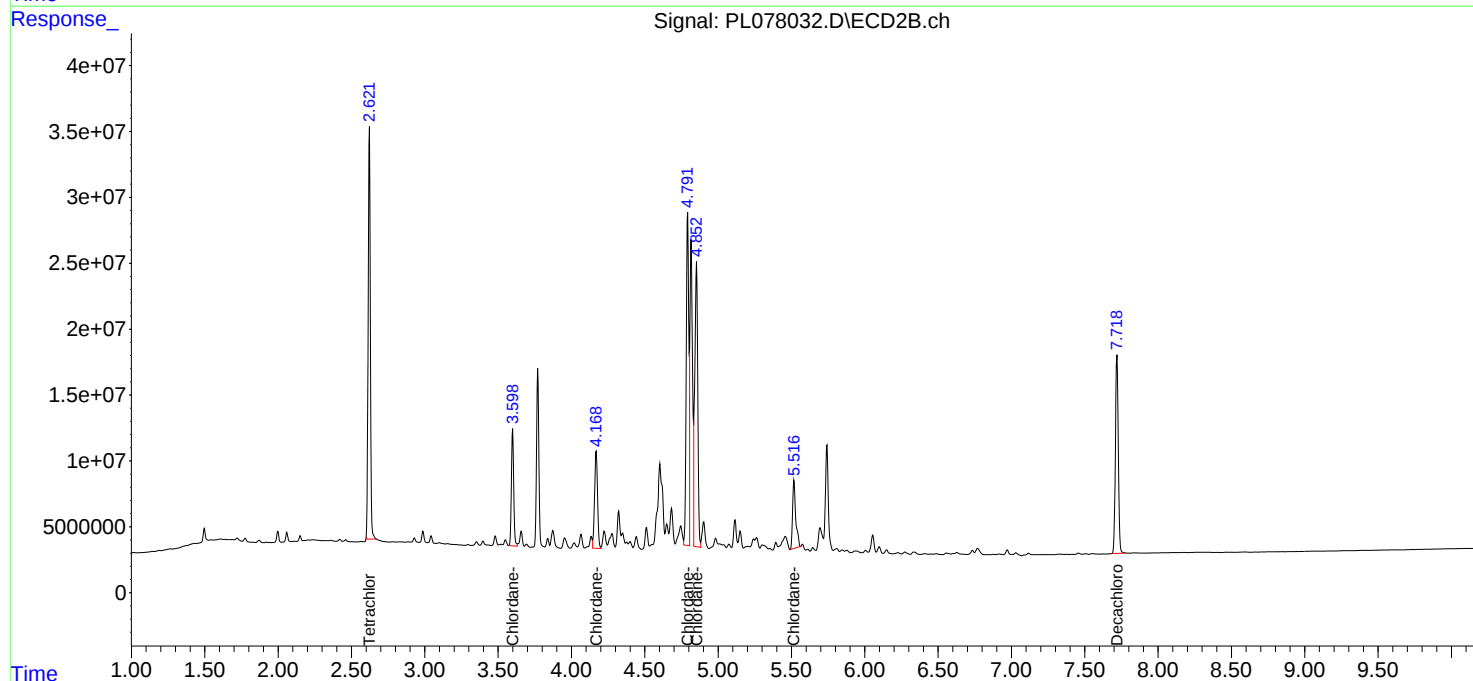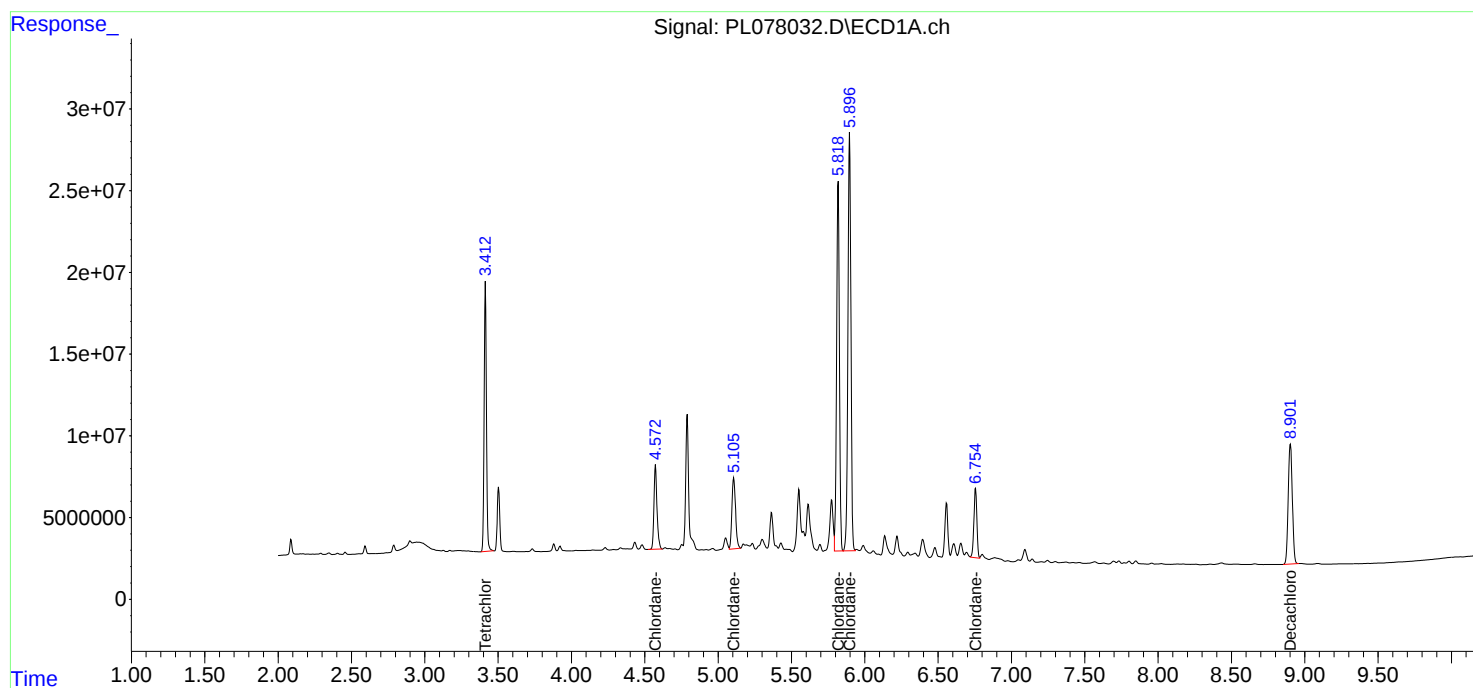


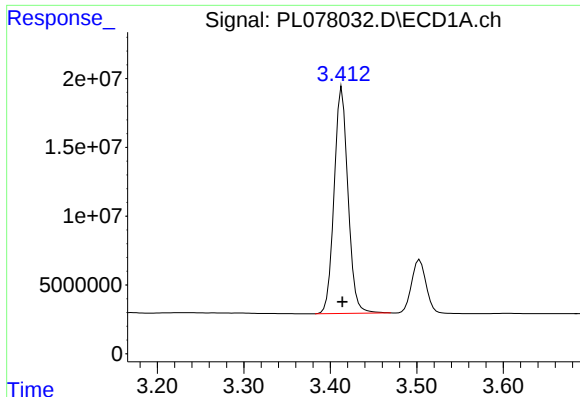

#1 Tetrachloro-m-xylene


R.T.: 3.414 min
Delta R.T.: 0.000 min
Response: 182510948
Conc: 99.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

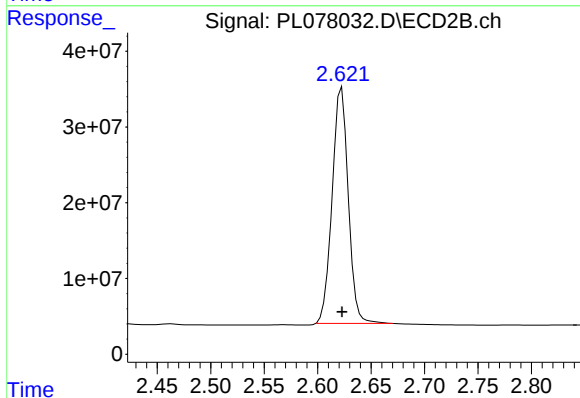


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 327097748
Conc: 98.62 ng/ml

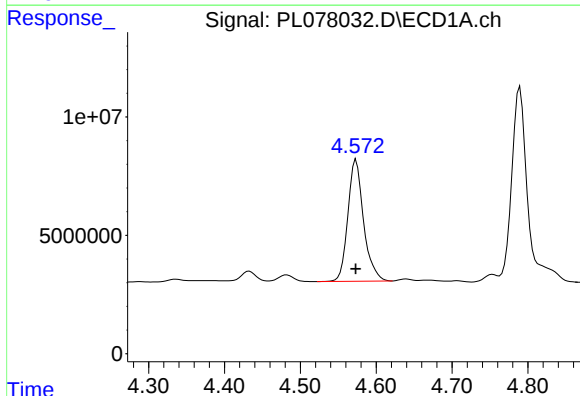


#23 Chlordane-1

R.T.: 4.574 min
Delta R.T.: 0.000 min
Response: 73965832
Conc: 998.62 ng/ml

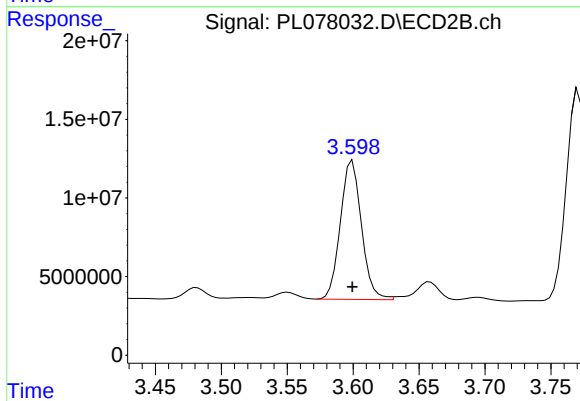

#23 Chlordane-1


R.T.: 3.600 min
Delta R.T.: 0.000 min
Response: 98388046
Conc: 973.11 ng/ml

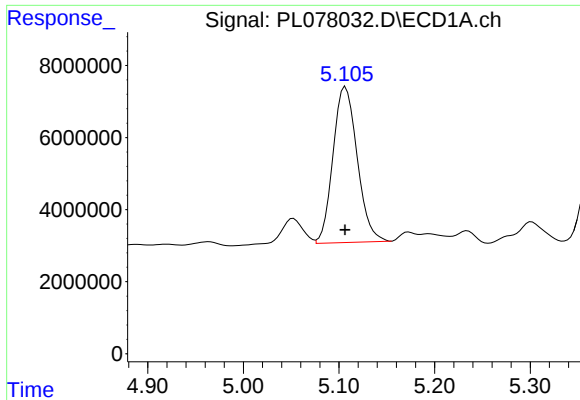

#24 Chlordane-2


R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 76050239
Conc: 965.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

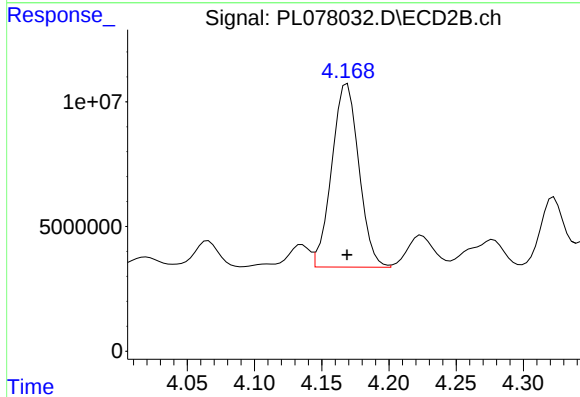


#24 Chlordane-2

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 102853043
Conc: 954.38 ng/ml

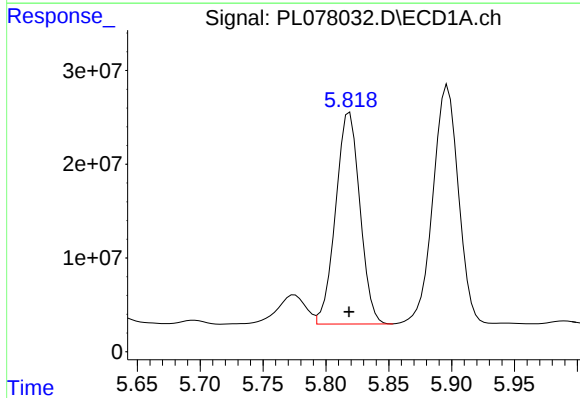


#25 Chlordane-3

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 303474013
Conc: 1020.75 ng/ml

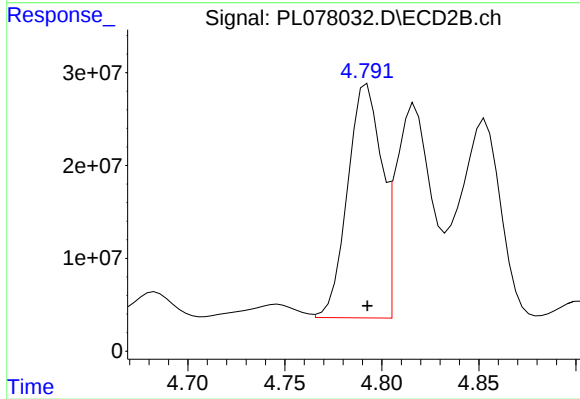

#25 Chlordane-3


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 304847125
Conc: 987.12 ng/ml

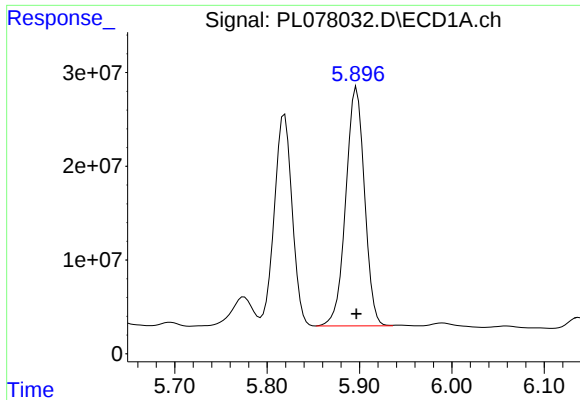

#26 Chlordane-4


R.T.: 5.897 min
Delta R.T.: 0.000 min
Response: 359069744
Conc: 1003.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

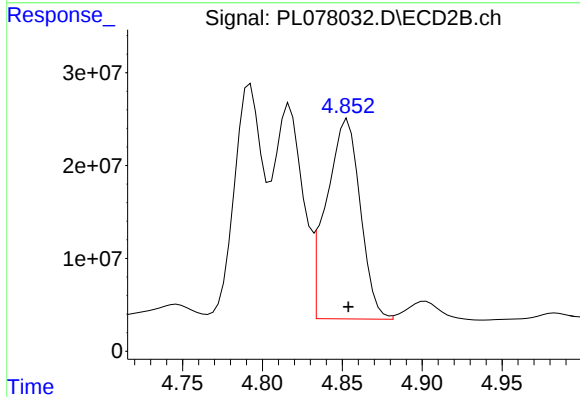


#26 Chlordane-4

R.T.: 4.853 min
Delta R.T.: 0.000 min
Response: 316837114
Conc: 980.04 ng/ml

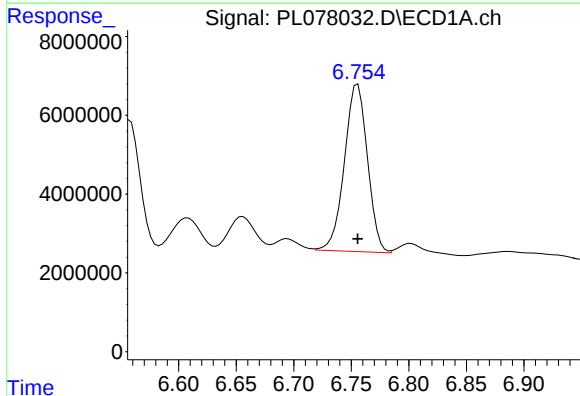


#27 Chlordane-5

R.T.: 6.756 min
Delta R.T.: 0.000 min
Response: 59479148
Conc: 1006.33 ng/ml

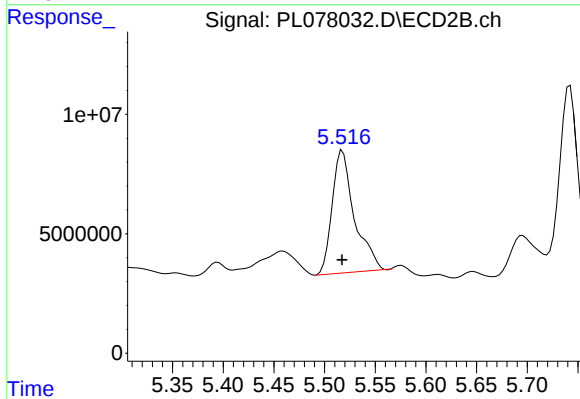

#27 Chlordane-5


R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 78399752
Conc: 953.72 ng/ml

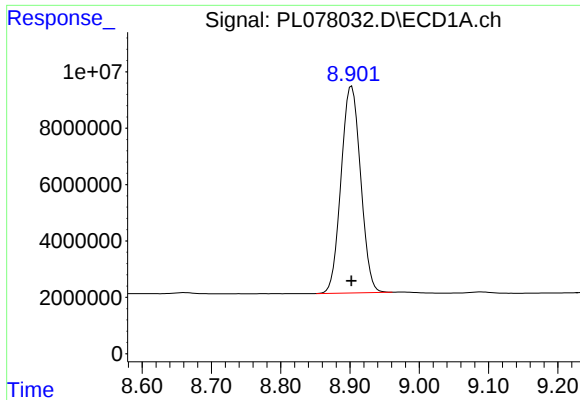

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 143571180
Conc: 92.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

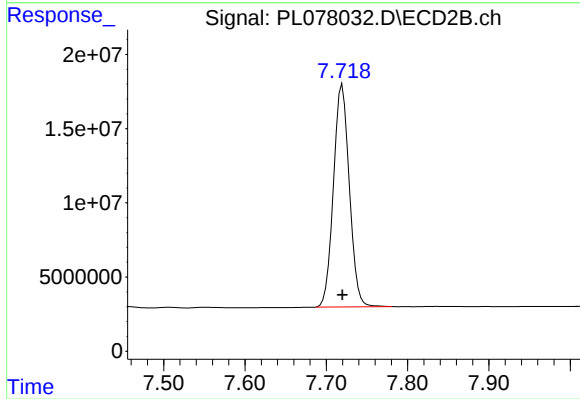

#28 Decachlorobiphenyl

R.T.: 7.720 min
Delta R.T.: 0.000 min
Response: 203616004
Conc: 96.07 ng/ml