

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
 Data File : PL078033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 15:00
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 15:51:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 15:50:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	137.6E6	247.0E6	75.294	74.478
28)	SA Decachlor...	8.901	7.720	110.5E6	156.3E6	71.389	73.739
Target Compounds							
23)	Chlordane-1	4.574	3.599	55521884	74493162	749.608	736.773
24)	Chlordane-2	5.107	4.170	57931679	79096435	735.261	733.942
25)	Chlordane-3	5.819	4.794	225.3E6	231.5E6	757.970	749.567
26)	Chlordane-4	5.897	4.854	268.8E6	240.3E6	751.071	743.232
27)	Chlordane-5	6.756	5.518	44389520	59599015	751.027	725.008



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
Data File : PL078033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 15:00
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 15:51:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 15:50:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

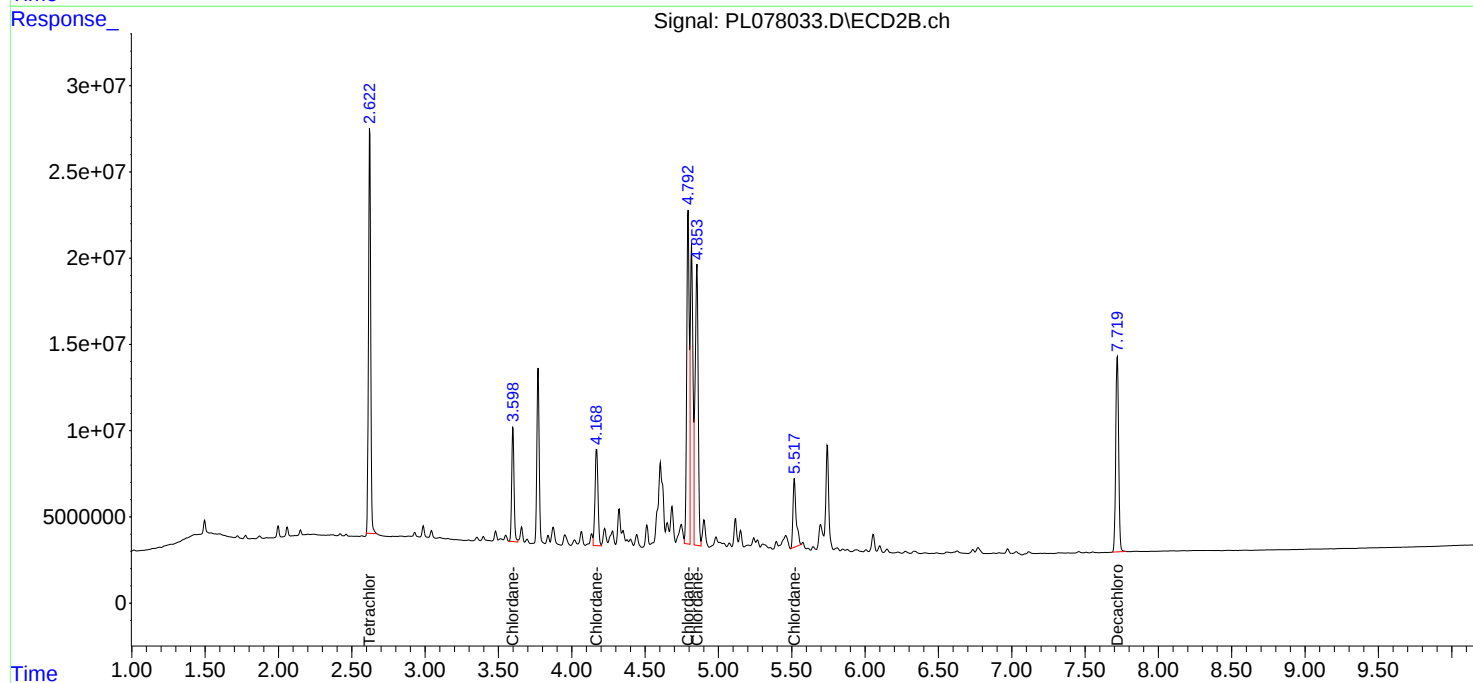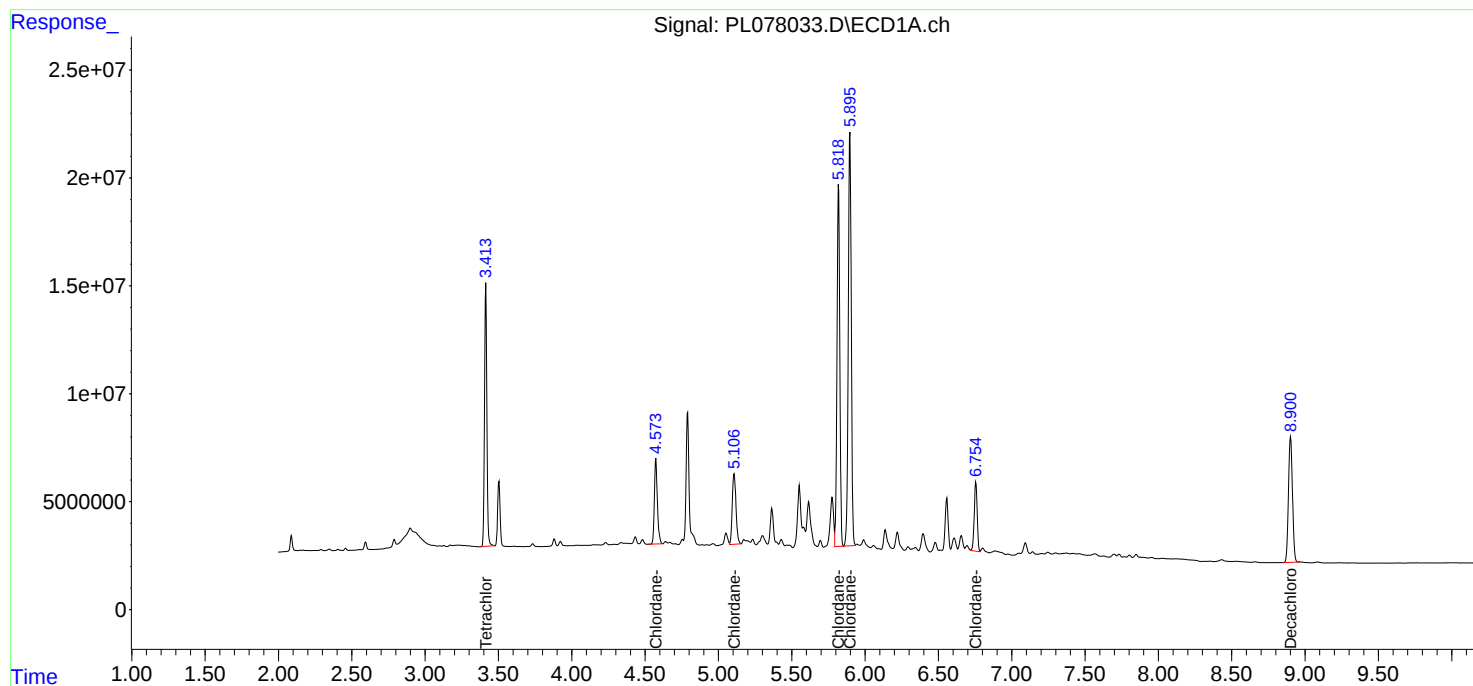


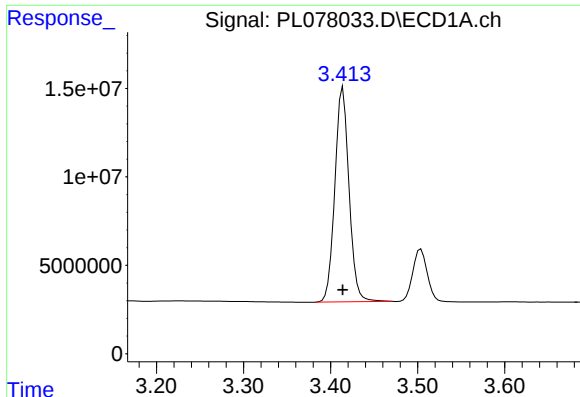

#1 Tetrachloro-m-xylene


R.T.: 3.414 min
Delta R.T.: 0.000 min
Response: 137638068
Conc: 75.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

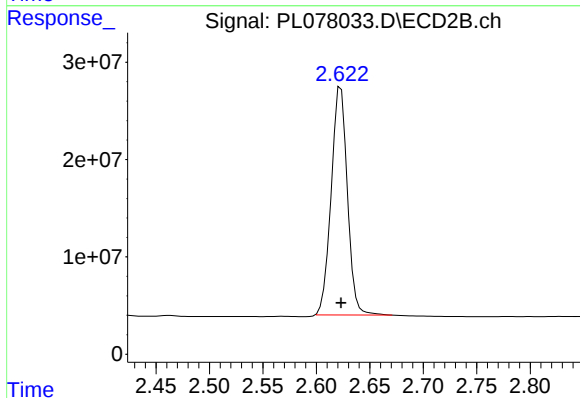


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 247031006
Conc: 74.48 ng/ml

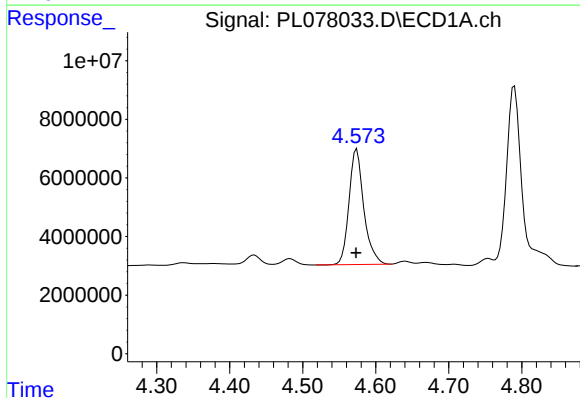


#23 Chlordane-1

R.T.: 4.574 min
Delta R.T.: 0.000 min
Response: 55521884
Conc: 749.61 ng/ml

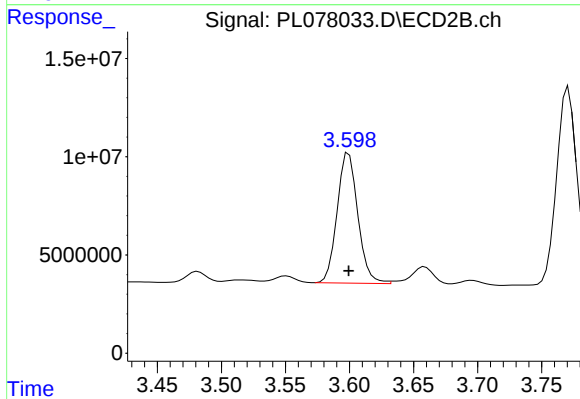

#23 Chlordane-1


R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 74493162
Conc: 736.77 ng/ml

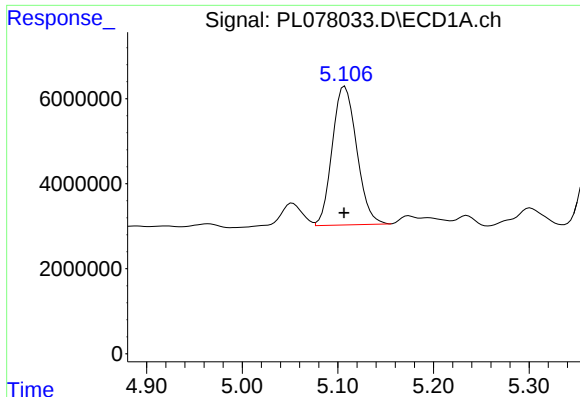

#24 Chlordane-2


R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 57931679
Conc: 735.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

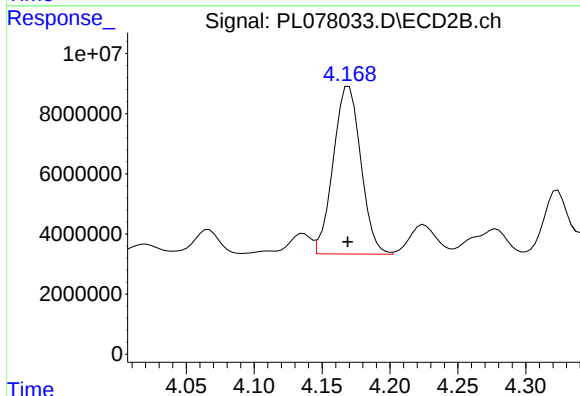


#24 Chlordane-2

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 79096435
Conc: 733.94 ng/ml

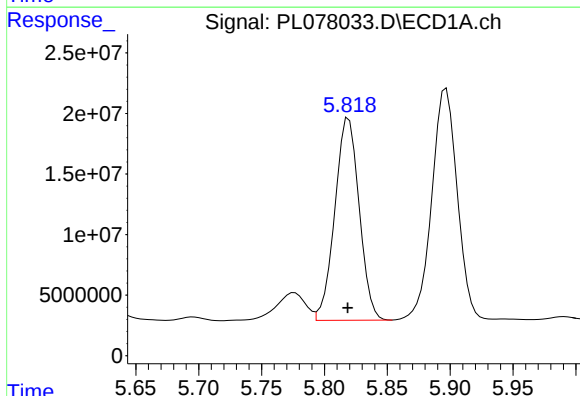


#25 Chlordane-3

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 225348148
Conc: 757.97 ng/ml

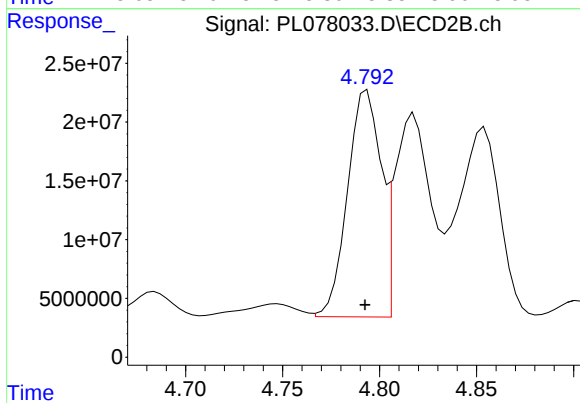

#25 Chlordane-3


R.T.: 4.794 min
Delta R.T.: 0.001 min
Response: 231485906
Conc: 749.57 ng/ml

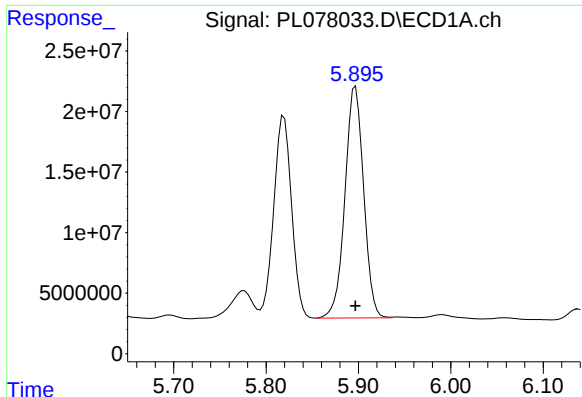

#26 Chlordane-4


R.T.: 5.897 min
Delta R.T.: 0.000 min
Response: 268761362
Conc: 751.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

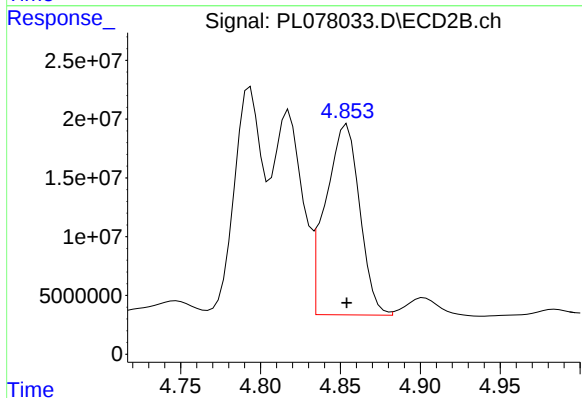


#26 Chlordane-4

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 240279060
Conc: 743.23 ng/ml

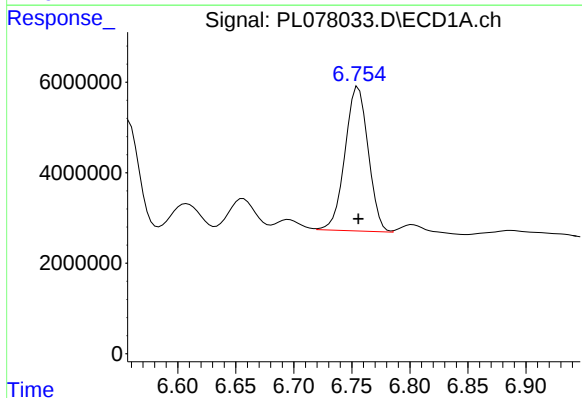


#27 Chlordane-5

R.T.: 6.756 min
Delta R.T.: 0.000 min
Response: 44389520
Conc: 751.03 ng/ml

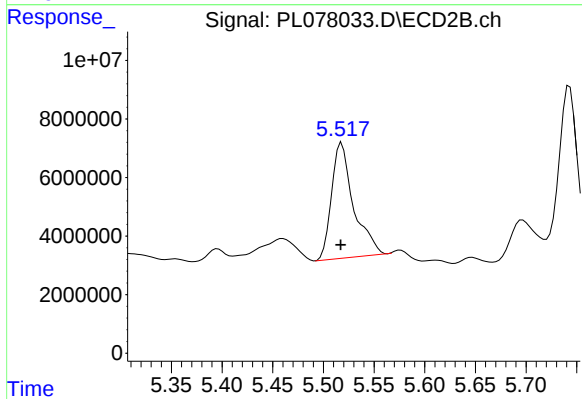

#27 Chlordane-5


R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 59599015
Conc: 725.01 ng/ml

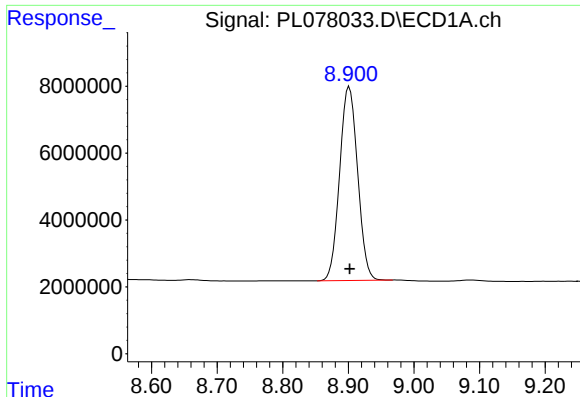

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.000 min
Response: 110526296
Conc: 71.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

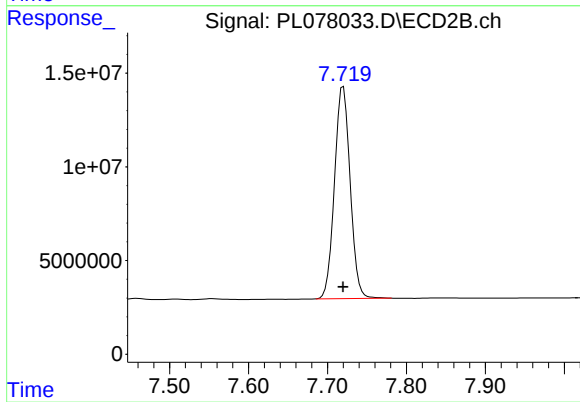

#28 Decachlorobiphenyl

R.T.: 7.720 min
Delta R.T.: 0.000 min
Response: 156295343
Conc: 73.74 ng/ml